

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091024\
 Data File : P0106373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2024 18:36
 Operator : YP/AJ
 Sample : P3906-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU-701-COMP-02

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/11/2024
 Supervised By :Ankita Jodhani 09/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 02:26:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.451	3.715	177.3E6	62780580	23.642m	23.503
2) SA Decachlor...	10.194	8.740	106.1E6	46201421	21.459	23.098

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091024\
Data File : PO106373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2024 18:36
Operator : YP/AJ
Sample : P3906-07
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU-701-COMP-02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2024
Supervised By :Ankita Jodhani 09/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:26:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

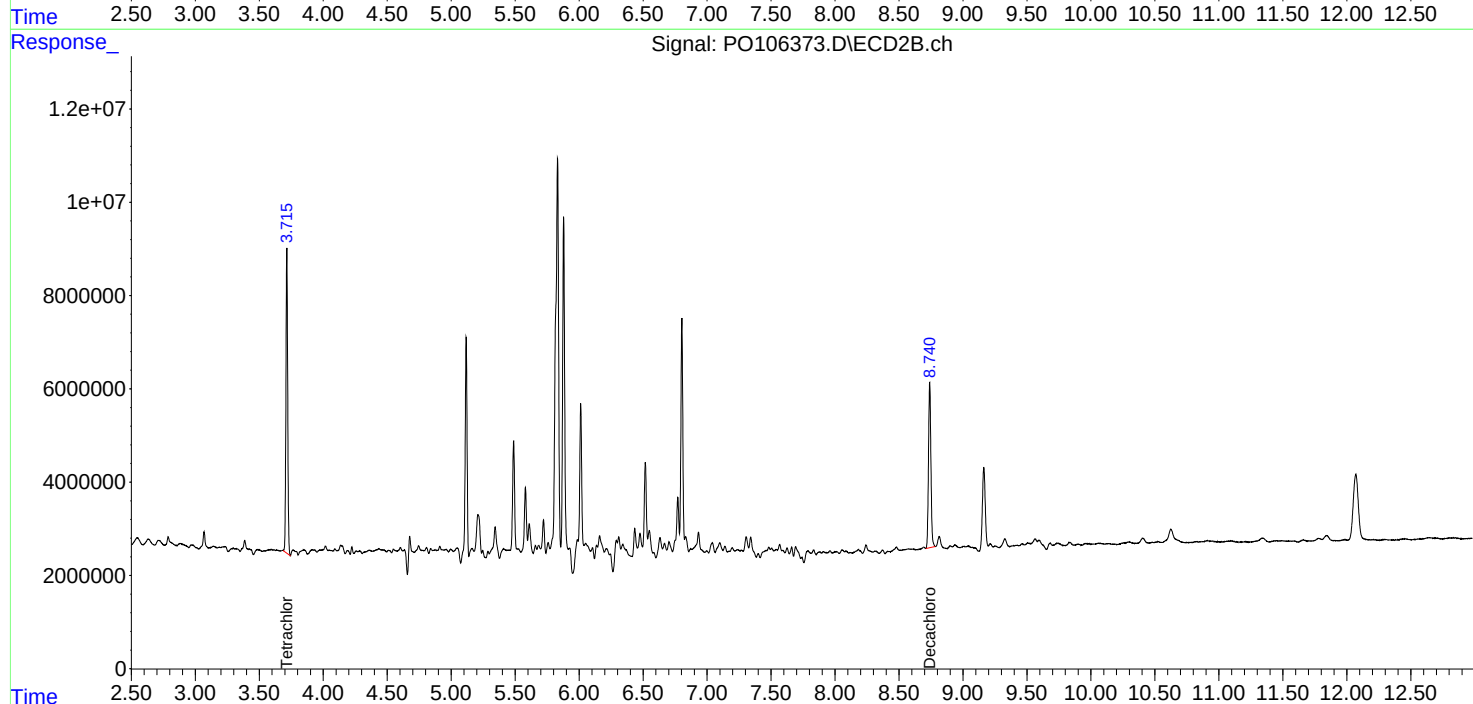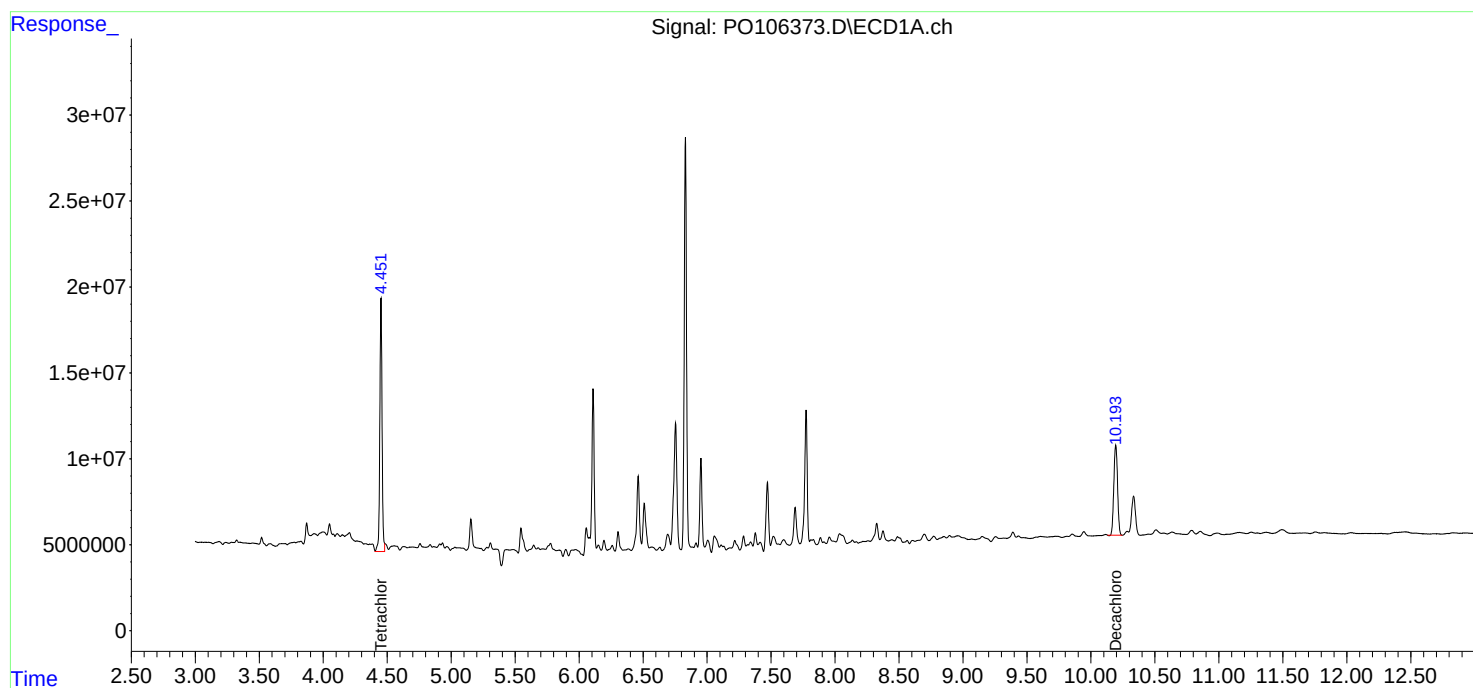

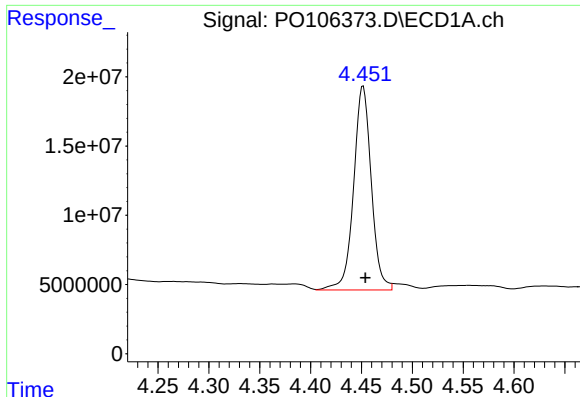


#1 Tetrachloro-m-xylene

R.T.: 4.451 min
Delta R.T.: -0.003 min
Response: 177345271
Conc: 23.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU-701-COMP-02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2024
Supervised By :Ankita Jodhani 09/12/2024

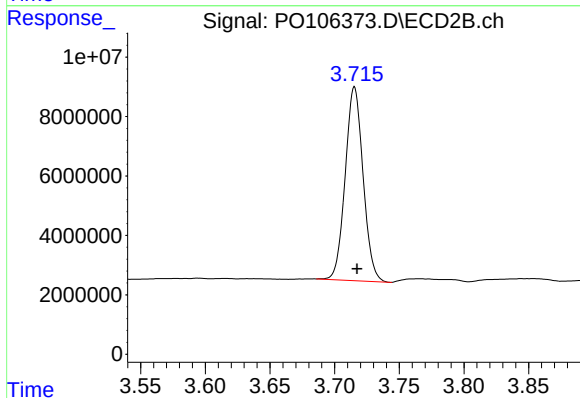


#1 Tetrachloro-m-xylene

R.T.: 3.715 min
Delta R.T.: -0.002 min
Response: 62780580
Conc: 23.50 ng/ml

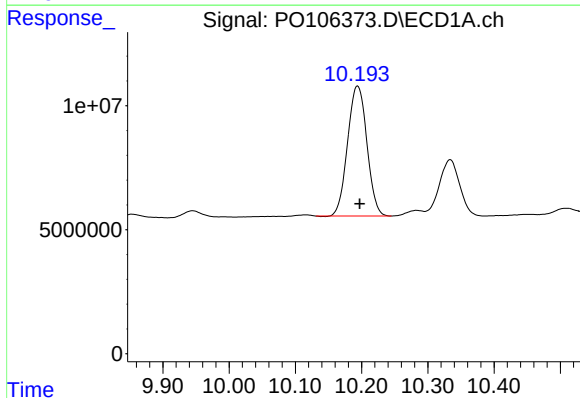

#2 Decachlorobiphenyl

R.T.: 10.194 min
Delta R.T.: -0.003 min
Response: 106069784
Conc: 21.46 ng/ml

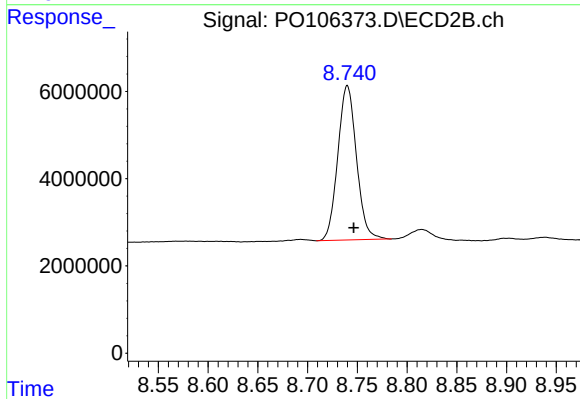

#2 Decachlorobiphenyl

R.T.: 8.740 min
Delta R.T.: -0.006 min
Response: 46201421
Conc: 23.10 ng/ml