

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091024\
 Data File : P0106375.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2024 19:11
 Operator : YP/AJ
 Sample : P3907-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PL-701-COMP-54

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/11/2024
 Supervised By :Ankita Jodhani 09/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 02:27:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.452	3.716	154.2E6	54404005	20.557m	20.367
2) SA Decachlor...	10.194	8.741	79198830	34470521	16.023	17.233

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091024\
Data File : PO106375.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2024 19:11
Operator : YP/AJ
Sample : P3907-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PL-701-COMP-54


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2024
Supervised By :Ankita Jodhani 09/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:27:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

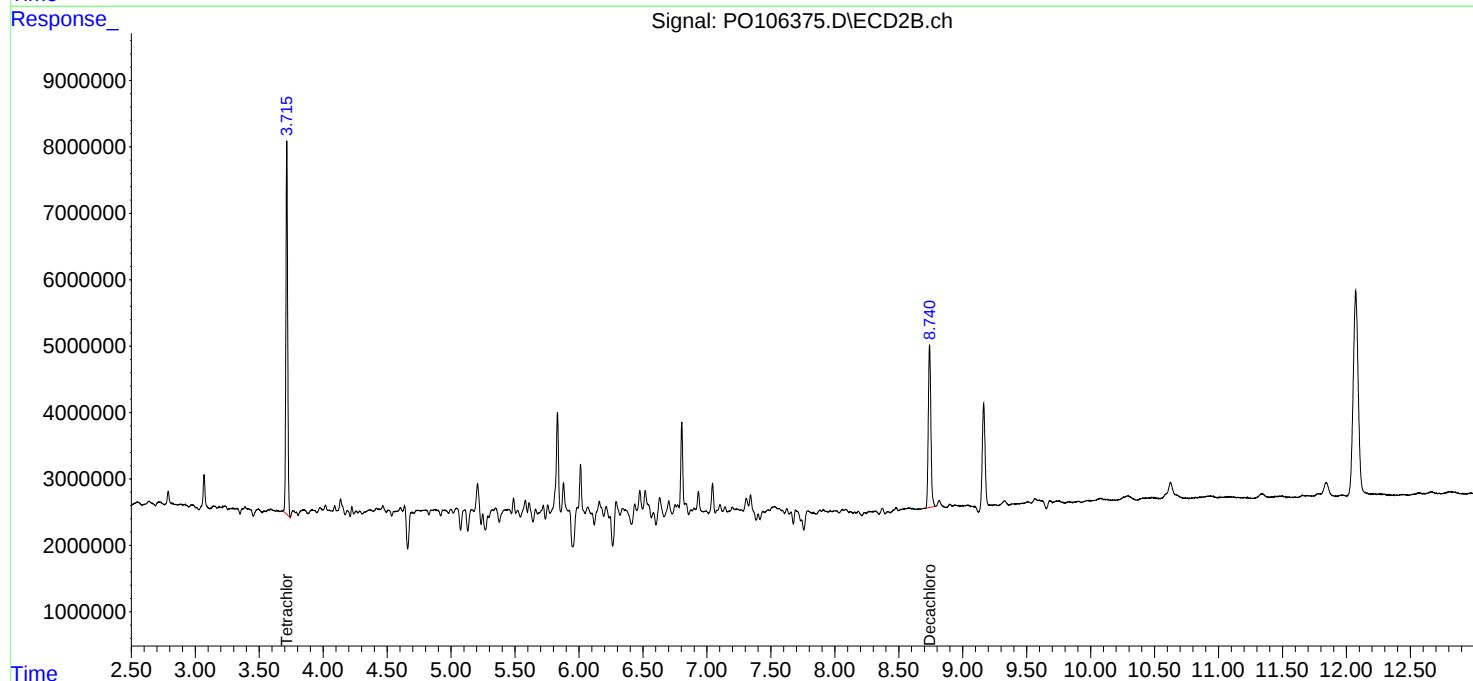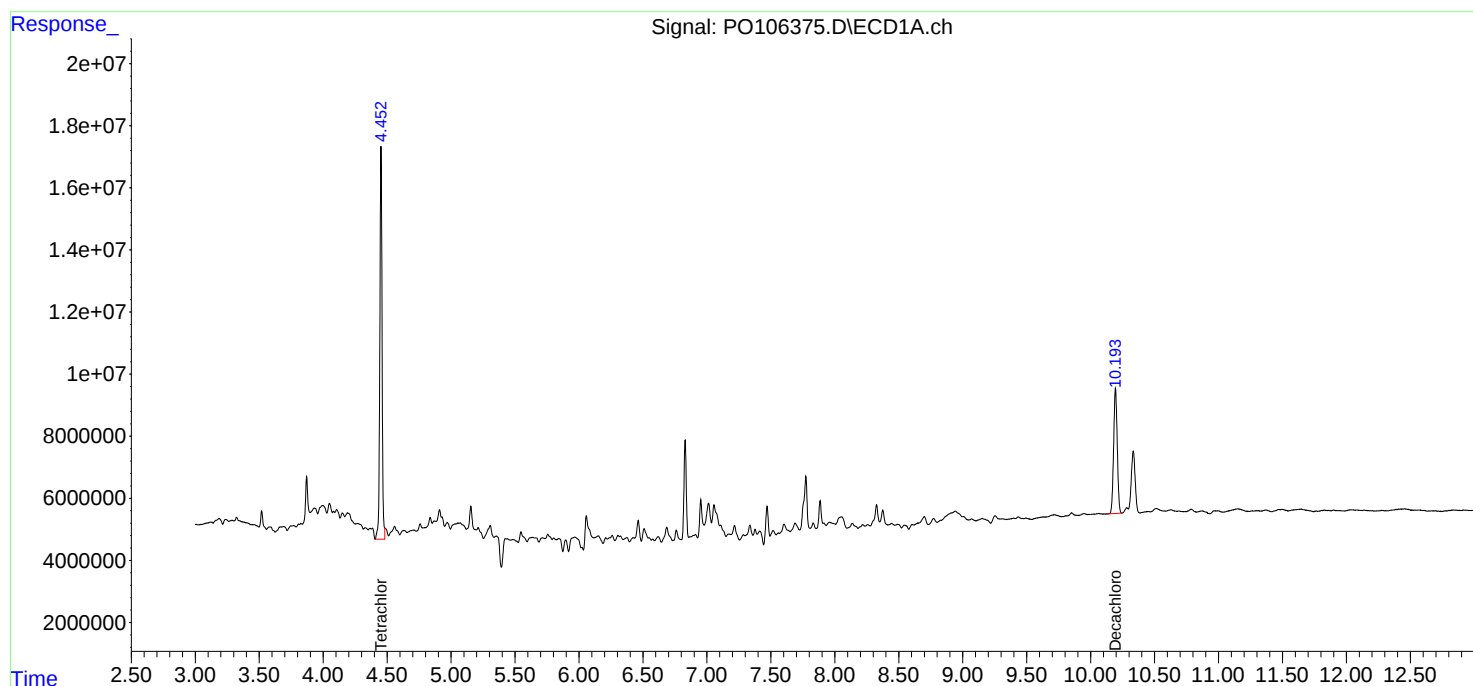

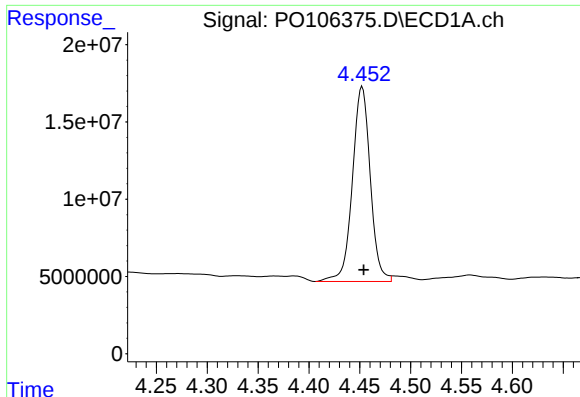


#1 Tetrachloro-m-xylene

R.T.: 4.452 min
Delta R.T.: -0.002 min
Response: 154206858
Conc: 20.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
PL-701-COMP-54


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2024
Supervised By :Ankita Jodhani 09/12/2024

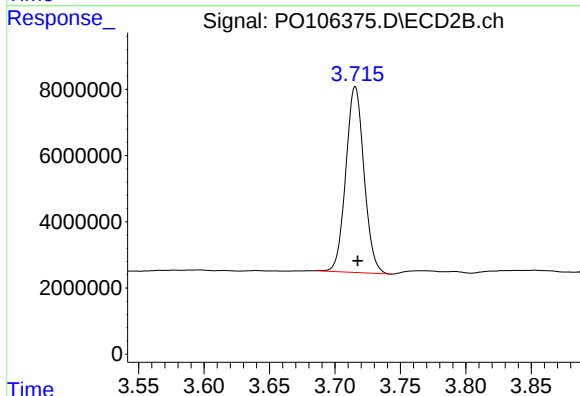


#1 Tetrachloro-m-xylene

R.T.: 3.716 min
Delta R.T.: -0.002 min
Response: 54404005
Conc: 20.37 ng/ml

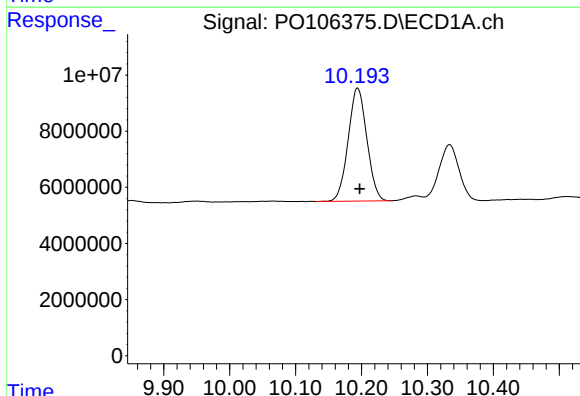

#2 Decachlorobiphenyl

R.T.: 10.194 min
Delta R.T.: -0.003 min
Response: 79198830
Conc: 16.02 ng/ml

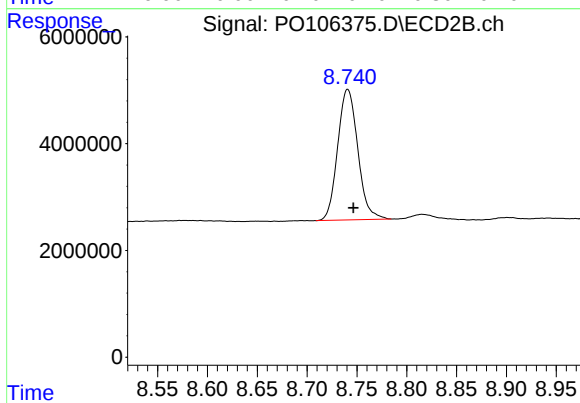

#2 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: -0.006 min
Response: 34470521
Conc: 17.23 ng/ml