

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
 Data File : P0113631.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 02:07
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1660 WATER LOD 40PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:29:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.657	3.648	189.4E6	110.4E6	23.140	21.811
2)	SA Decachlor...	8.669	8.613	155.3E6	44958109	22.410	23.726
Target Compounds							
3)	L1 AR-1016-1	4.741	4.720	12364178	7919702	46.310	46.430
4)	L1 AR-1016-2	4.760	4.738	19325906	12320175	48.142	47.816
5)	L1 AR-1016-3	4.817	4.913	11976891	7693597	46.964	55.106
6)	L1 AR-1016-4	4.936	4.956	9665077	6347002	44.321	54.388
7)	L1 AR-1016-5	5.192	5.167	13728442	9150723	61.944	64.202
8)	L2 AR-1221-1	3.869	3.855	631051	771015	6.744	12.215 #
9)	L2 AR-1221-2	3.956	3.943	2591398	3801588	38.362	81.451 #
10)	L2 AR-1221-3	4.030	4.016	5915218	4748392	26.723	31.981
11)	L3 AR-1232-1	4.030	4.016	5915218	4748392	32.949	39.265
12)	L3 AR-1232-2	4.520	4.738	9298485	12320175	86.163	100.944
13)	L3 AR-1232-3	4.760	4.913	19325906	7693597	97.905	116.295
14)	L3 AR-1232-4	4.936	4.997	9665077	7463424	98.329	124.539 #
15)	L3 AR-1232-5	4.980	5.167	7452768	9150723	113.295	135.333
16)	L4 AR-1242-1	4.741	4.738	12364178	12320175	53.773	85.258 #
17)	L4 AR-1242-2	4.760	4.738	19325906	12320175	56.241	56.798
18)	L4 AR-1242-3	4.817	4.913	11976891	7693597	53.978	65.777
19)	L4 AR-1242-4	4.936	4.997	9665077	7463424	55.718	63.444
20)	L4 AR-1242-5	5.588	5.516	12697165	9010560	63.434	60.420
21)	L5 AR-1248-1	4.741	4.738	12364178	12320175	70.869	110.483 #
22)	L5 AR-1248-2	4.980	4.956	7452768	6347002	30.814	39.496 #
23)	L5 AR-1248-3	5.192	4.997	13728442	7463424	43.054	43.990
24)	L5 AR-1248-4	5.544	5.167	18234457	9150723	36.498	45.933 #
25)	L5 AR-1248-5	5.588	5.557	12697165	5123307	37.181	24.133 #
26)	L6 AR-1254-1	5.544	5.516	18234457	9010560	33.769	28.573
27)	L6 AR-1254-2	5.694	5.664	20349528	7578033	41.239	27.032 #
28)	L6 AR-1254-3	6.113	6.079	20317806	10093424	27.498	24.209
29)	L6 AR-1254-4	6.326	6.291	4974533	1670559	8.931	6.078 #
30)	L6 AR-1254-5	6.743	6.705	28483314	13439973	40.634	37.595
31)	L7 AR-1260-1	6.227	6.193	26366333	12949361	59.120	50.768
32)	L7 AR-1260-2	6.417	6.382	37410715	19928826	54.477	57.646
33)	L7 AR-1260-3	6.782	6.533	28255679	11777710	45.760	39.598
34)	L7 AR-1260-4	7.040	7.001	19964153	7360608	44.575	35.516
35)	L7 AR-1260-5	7.283	7.243	59158464	19464108	48.864	41.552
36)	L8 AR-1262-1	6.782	6.745	28255679	12702906	30.855	30.638
37)	L8 AR-1262-2	7.283	7.243	59158464	19464108	39.122	37.599
38)	L8 AR-1262-3	7.567	7.524	15335704	3998616	27.676	22.265
39)	L8 AR-1262-4	7.629	7.587	39636198	10940655	40.529	37.739
40)	L8 AR-1262-5	8.125	8.081	13382945	3248604	32.103	29.988
41)	L9 AR-1268-1	7.567	7.524	15335704	3998616	8.912	7.849

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
Data File : P0113631.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 02:07
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1660 WATER LOD 40PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:29:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.629	7.587	39636198	10940655	27.370	26.337
43) L9	AR-1268-3	7.841	7.795	391419	368217	0.324	1.128 #
44) L9	AR-1268-4	8.125	8.081	13382945	3248604	29.051	26.974
45) L9	AR-1268-5	8.440	8.369	162204	775039	0.051	0.992 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091025\
Data File : PO113631.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 02:07
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1660 WATER LOD 40PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:29:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

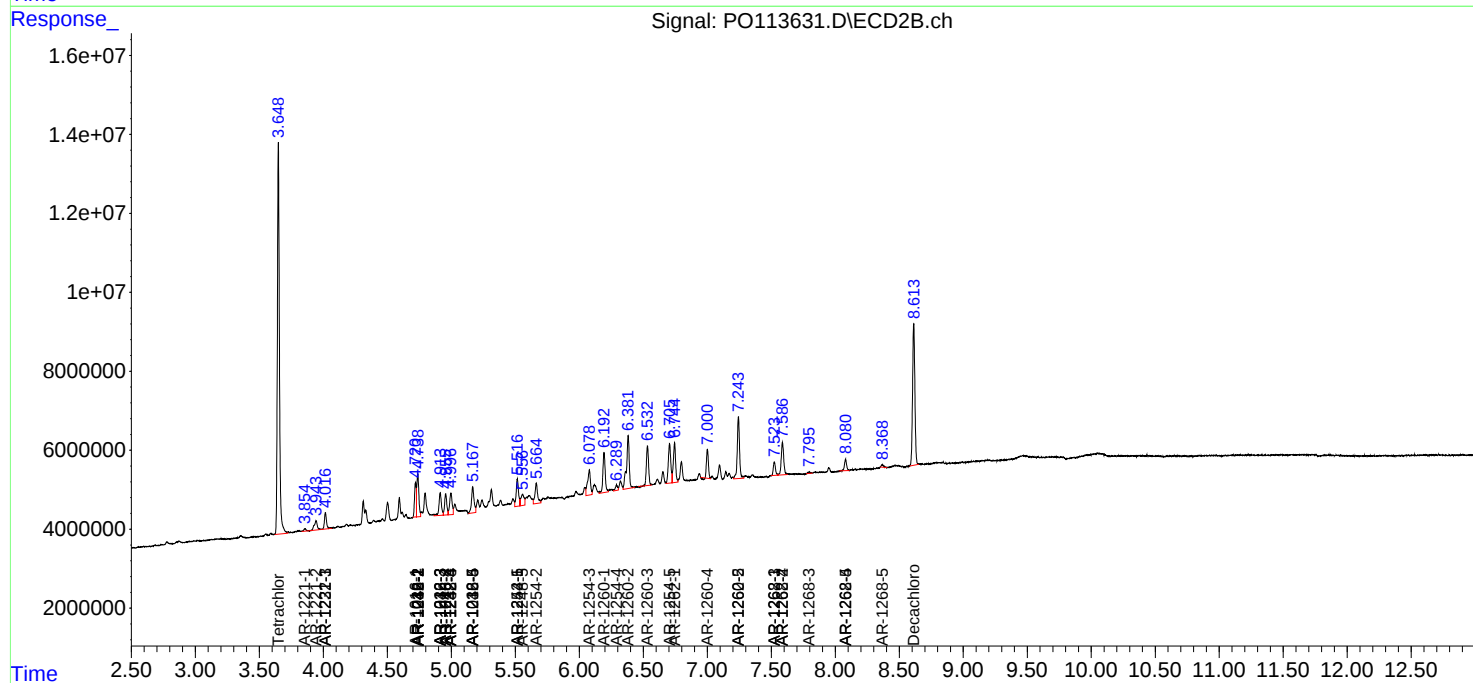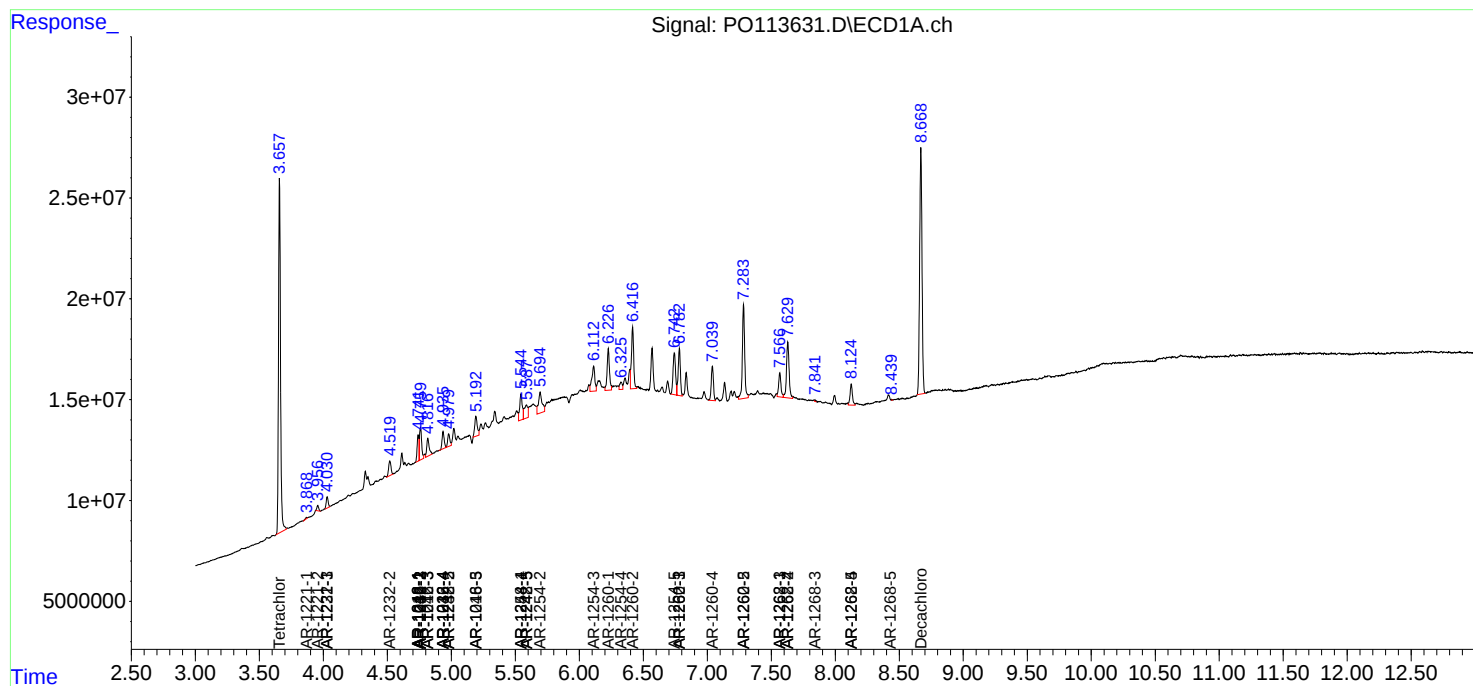


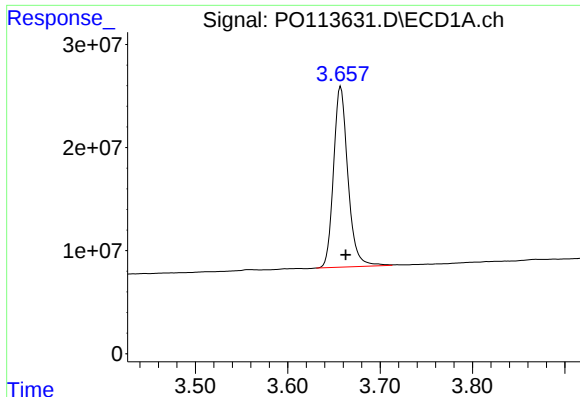

#1 Tetrachloro-m-xylene


R.T.: 3.657 min
Delta R.T.: -0.006 min
Response: 189437379
Conc: 23.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

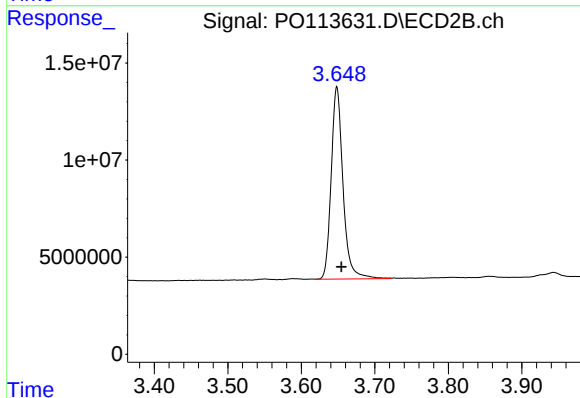


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: -0.006 min
Response: 110377218
Conc: 21.81 ng/ml

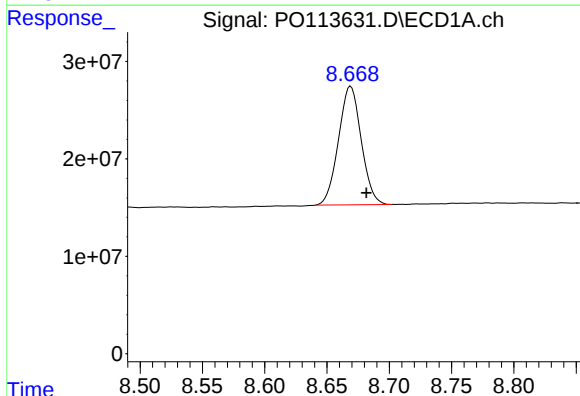


#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.013 min
Response: 155330910
Conc: 22.41 ng/ml

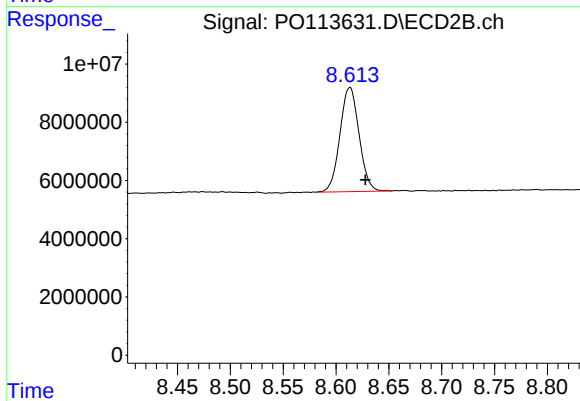

#2 Decachlorobiphenyl


R.T.: 8.613 min
Delta R.T.: -0.015 min
Response: 44958109
Conc: 23.73 ng/ml

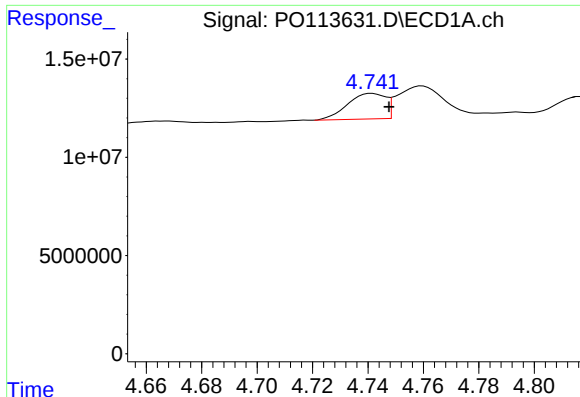

#3 AR-1016-1


R.T.: 4.741 min
Delta R.T.: -0.006 min
Response: 12364178
Conc: 46.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

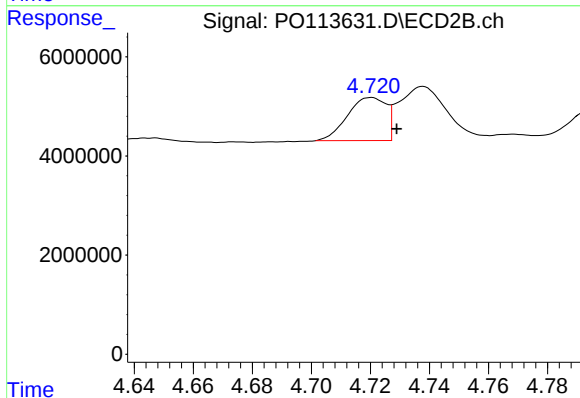


#3 AR-1016-1

R.T.: 4.720 min
Delta R.T.: -0.009 min
Response: 7919702
Conc: 46.43 ng/ml

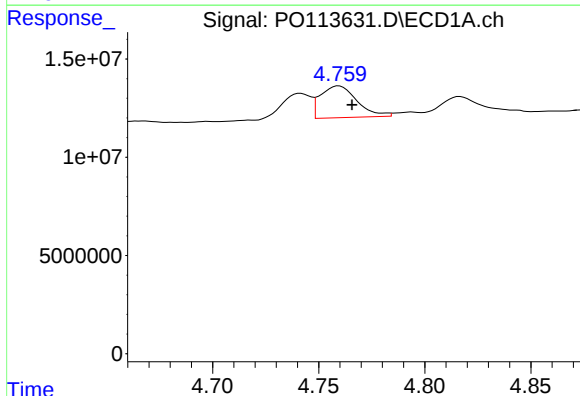


#4 AR-1016-2

R.T.: 4.760 min
Delta R.T.: -0.006 min
Response: 19325906
Conc: 48.14 ng/ml

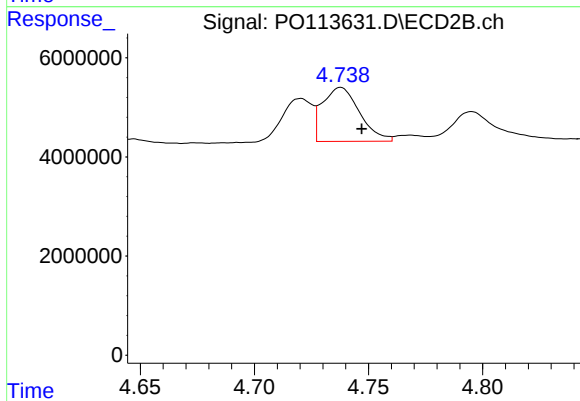

#4 AR-1016-2


R.T.: 4.738 min
Delta R.T.: -0.009 min
Response: 12320175
Conc: 47.82 ng/ml

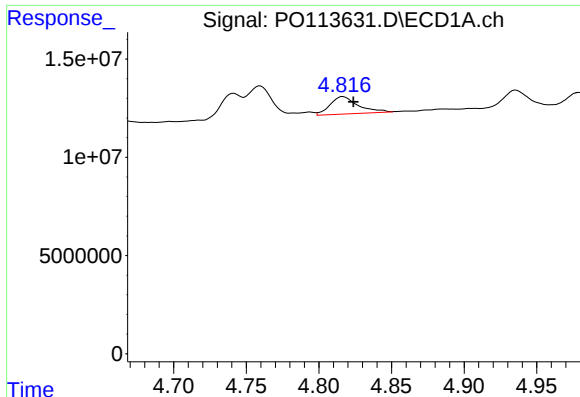

#5 AR-1016-3


R.T.: 4.817 min
Delta R.T.: -0.007 min
Response: 11976891
Conc: 46.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

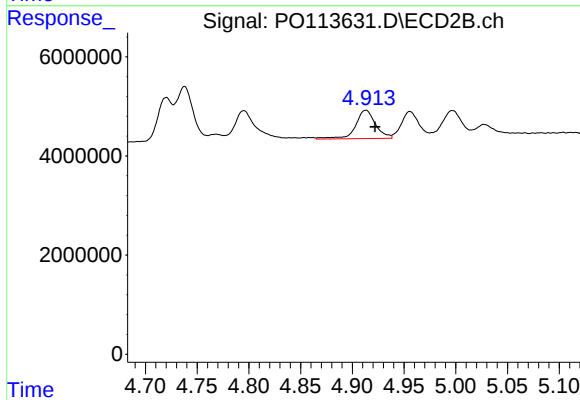


#5 AR-1016-3

R.T.: 4.913 min
Delta R.T.: -0.009 min
Response: 7693597
Conc: 55.11 ng/ml

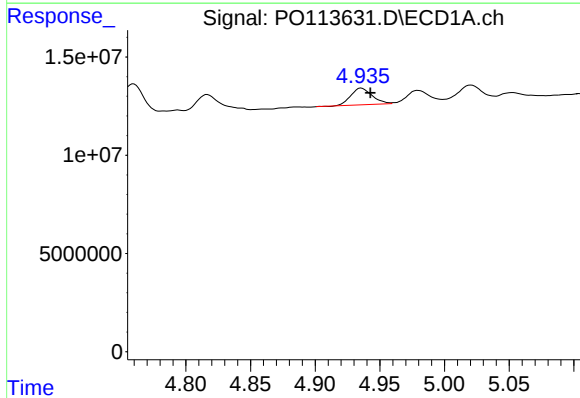


#6 AR-1016-4

R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 9665077
Conc: 44.32 ng/ml

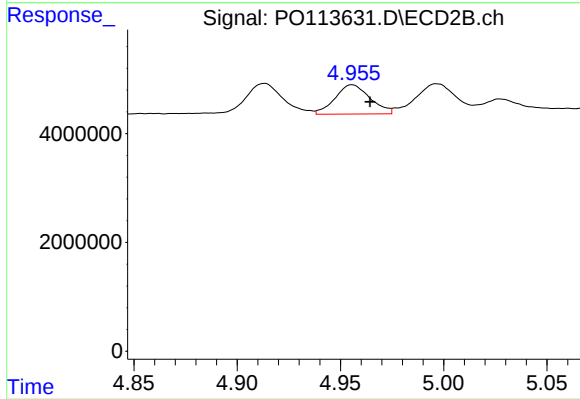

#6 AR-1016-4


R.T.: 4.956 min
Delta R.T.: -0.009 min
Response: 6347002
Conc: 54.39 ng/ml

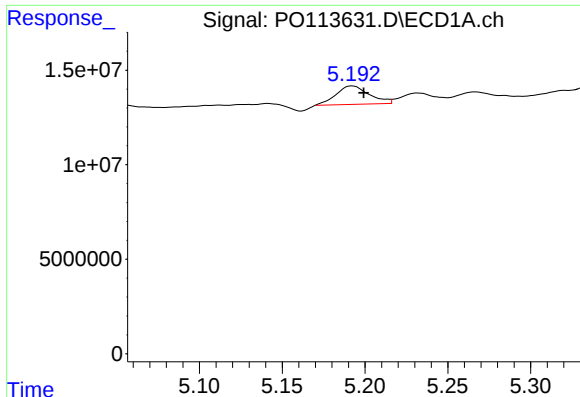

#7 AR-1016-5


R.T.: 5.192 min
Delta R.T.: -0.007 min
Response: 13728442
Conc: 61.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

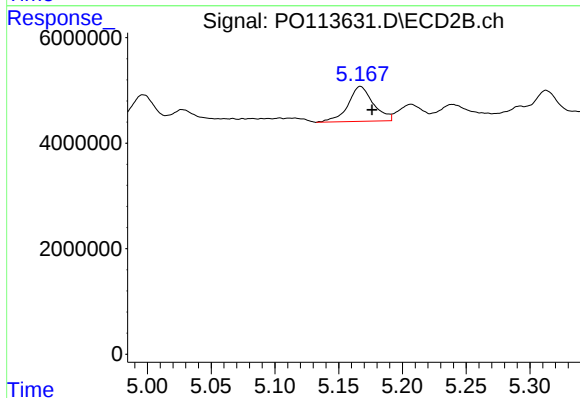


#7 AR-1016-5

R.T.: 5.167 min
Delta R.T.: -0.009 min
Response: 9150723
Conc: 64.20 ng/ml

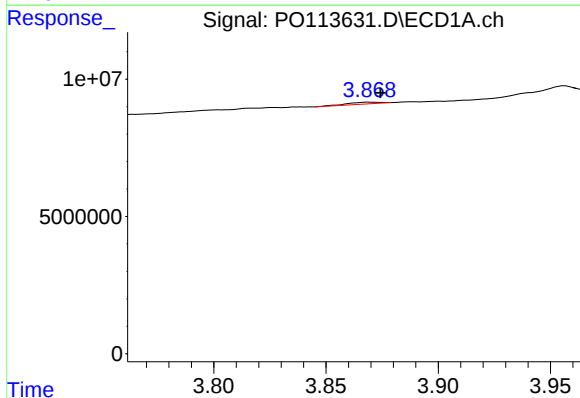


#8 AR-1221-1

R.T.: 3.869 min
Delta R.T.: -0.005 min
Response: 631051
Conc: 6.74 ng/ml

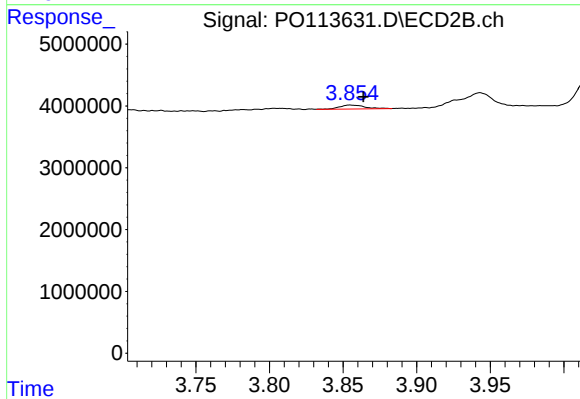

#8 AR-1221-1


R.T.: 3.855 min
Delta R.T.: -0.009 min
Response: 771015
Conc: 12.21 ng/ml

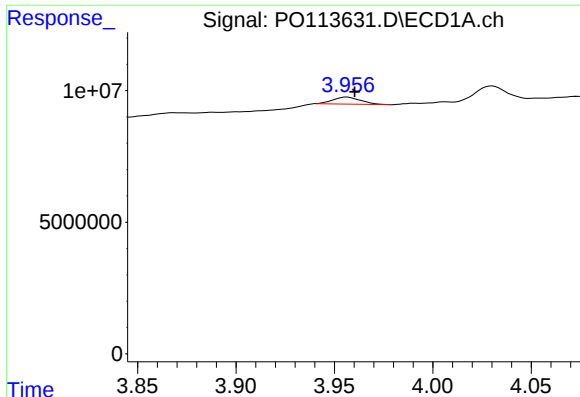

#9 AR-1221-2


R.T.: 3.956 min
Delta R.T.: -0.004 min
Response: 2591398
Conc: 38.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

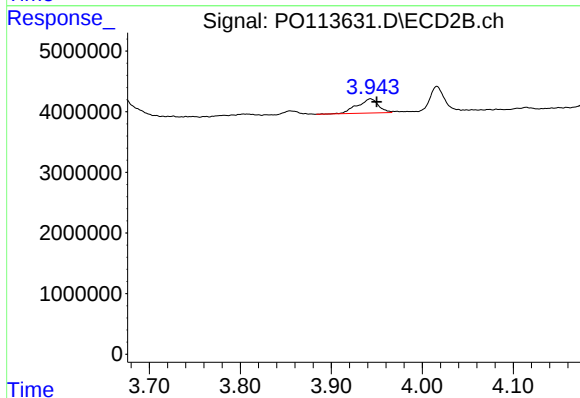


#9 AR-1221-2

R.T.: 3.943 min
Delta R.T.: -0.007 min
Response: 3801588
Conc: 81.45 ng/ml

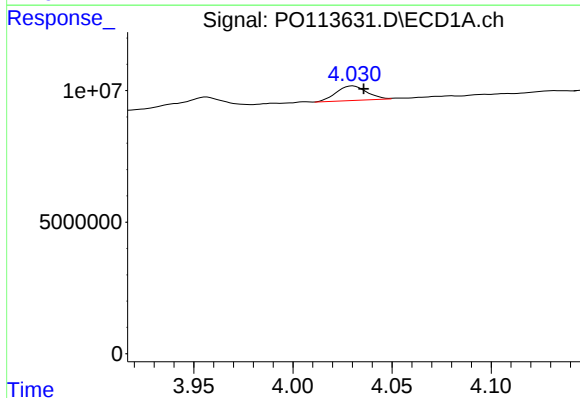


#10 AR-1221-3

R.T.: 4.030 min
Delta R.T.: -0.005 min
Response: 5915218
Conc: 26.72 ng/ml

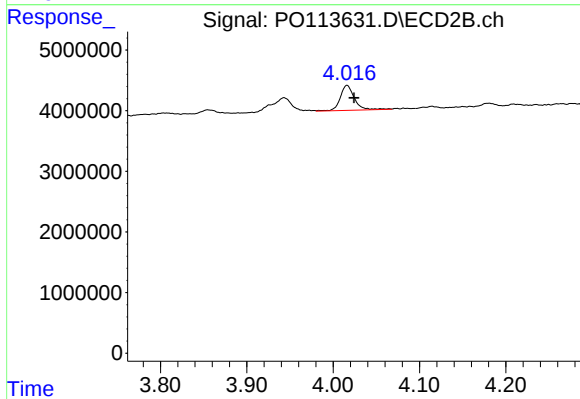

#10 AR-1221-3


R.T.: 4.016 min
Delta R.T.: -0.008 min
Response: 4748392
Conc: 31.98 ng/ml

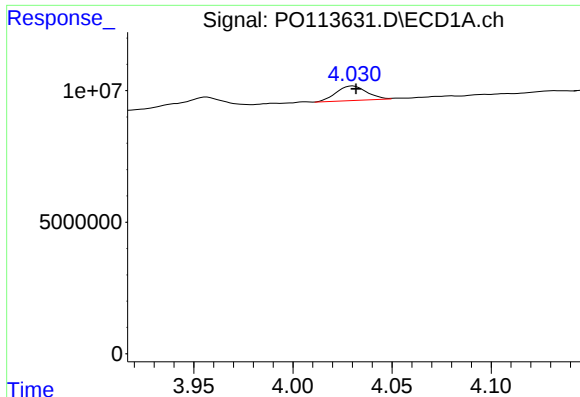

#11 AR-1232-1


R.T.: 4.030 min
Delta R.T.: -0.002 min
Response: 5915218
Conc: 32.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

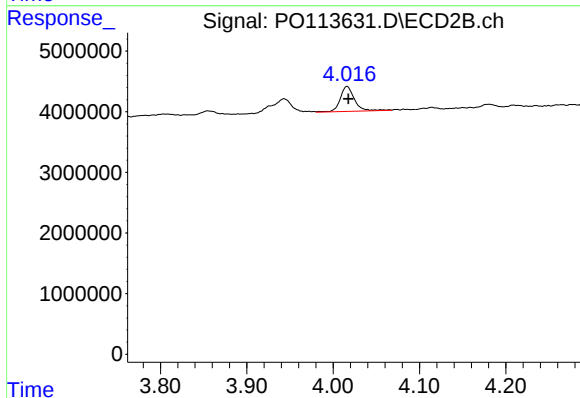


#11 AR-1232-1

R.T.: 4.016 min
Delta R.T.: -0.002 min
Response: 4748392
Conc: 39.26 ng/ml

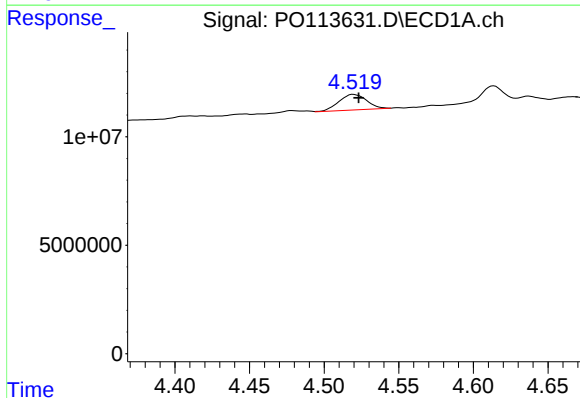


#12 AR-1232-2

R.T.: 4.520 min
Delta R.T.: -0.003 min
Response: 9298485
Conc: 86.16 ng/ml

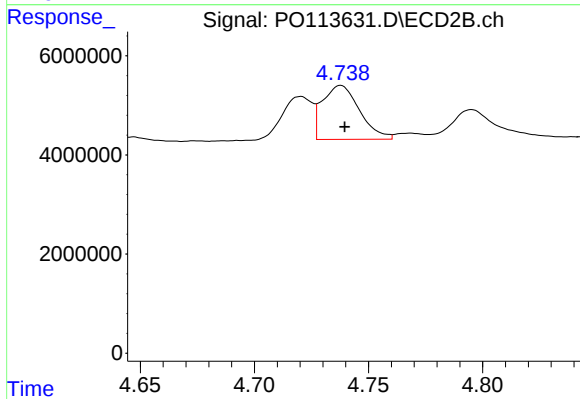

#12 AR-1232-2


R.T.: 4.738 min
Delta R.T.: -0.002 min
Response: 12320175
Conc: 100.94 ng/ml

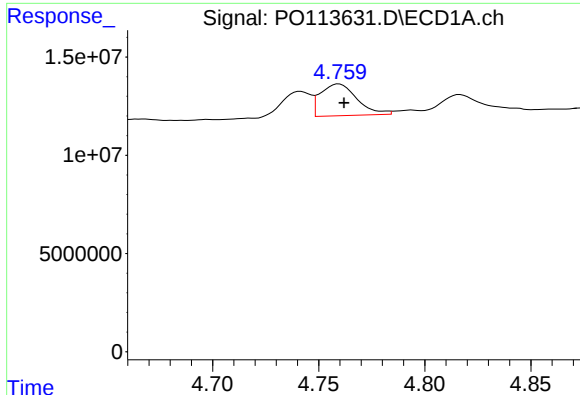

#13 AR-1232-3


R.T.: 4.760 min
Delta R.T.: -0.002 min
Response: 19325906
Conc: 97.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

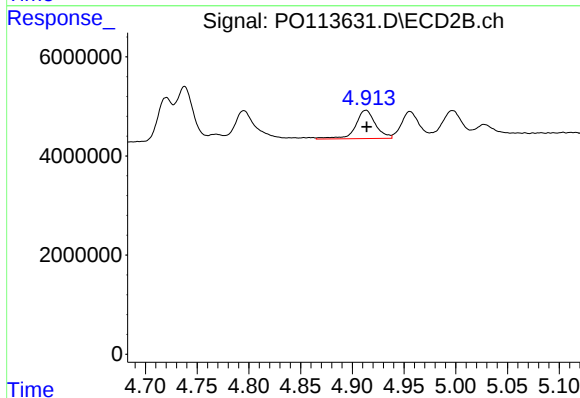


#13 AR-1232-3

R.T.: 4.913 min
Delta R.T.: 0.000 min
Response: 7693597
Conc: 116.29 ng/ml

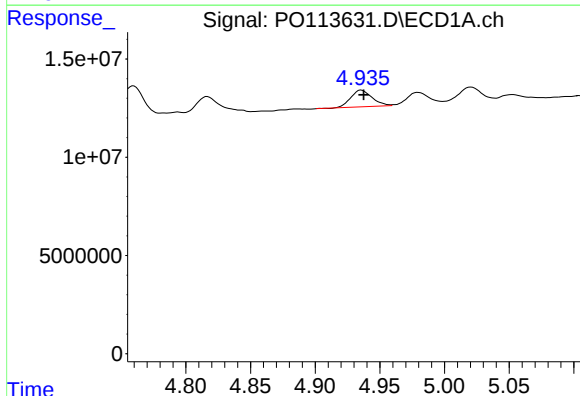


#14 AR-1232-4

R.T.: 4.936 min
Delta R.T.: -0.002 min
Response: 9665077
Conc: 98.33 ng/ml

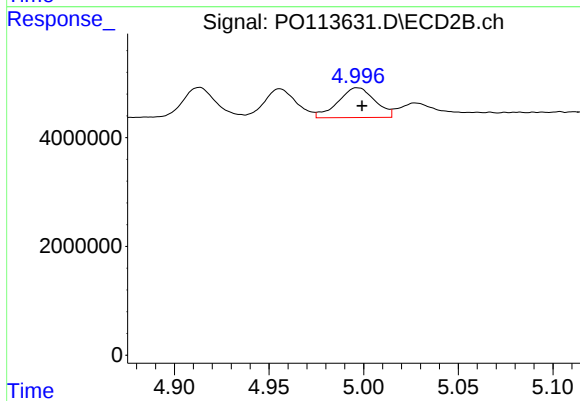

#14 AR-1232-4


R.T.: 4.997 min
Delta R.T.: -0.002 min
Response: 7463424
Conc: 124.54 ng/ml

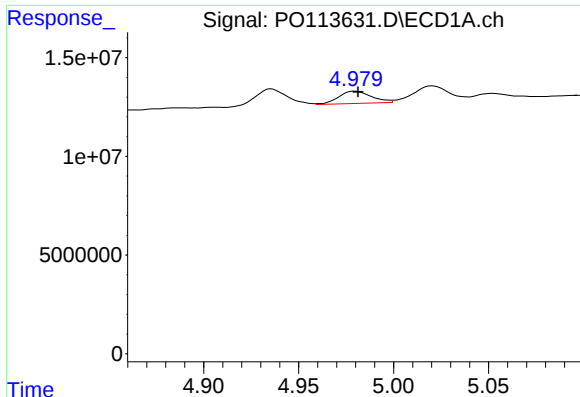

#15 AR-1232-5


R.T.: 4.980 min
Delta R.T.: -0.002 min
Response: 7452768
Conc: 113.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

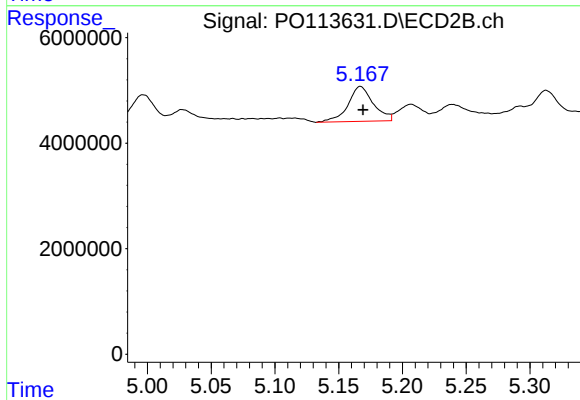


#15 AR-1232-5

R.T.: 5.167 min
Delta R.T.: -0.002 min
Response: 9150723
Conc: 135.33 ng/ml

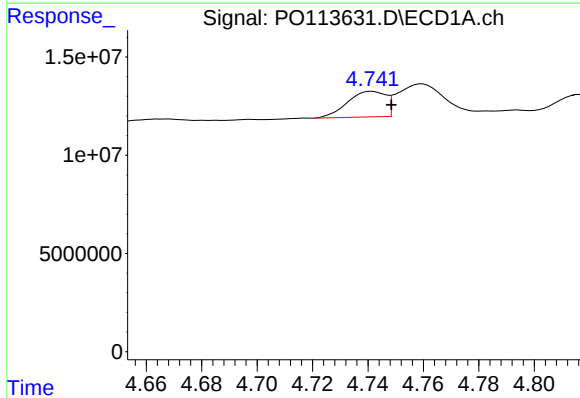


#16 AR-1242-1

R.T.: 4.741 min
Delta R.T.: -0.007 min
Response: 12364178
Conc: 53.77 ng/ml

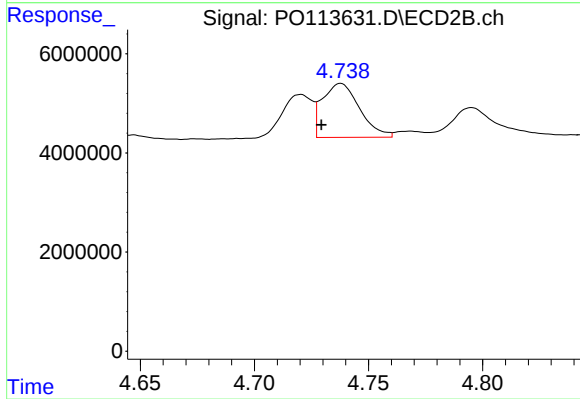

#16 AR-1242-1


R.T.: 4.738 min
Delta R.T.: 0.008 min
Response: 12320175
Conc: 85.26 ng/ml

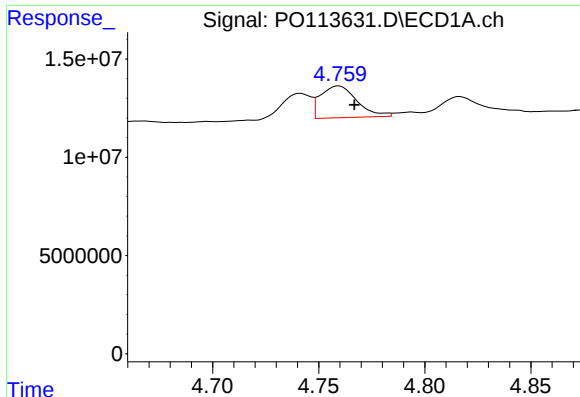

#17 AR-1242-2


R.T.: 4.760 min
Delta R.T.: -0.007 min
Response: 19325906
Conc: 56.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

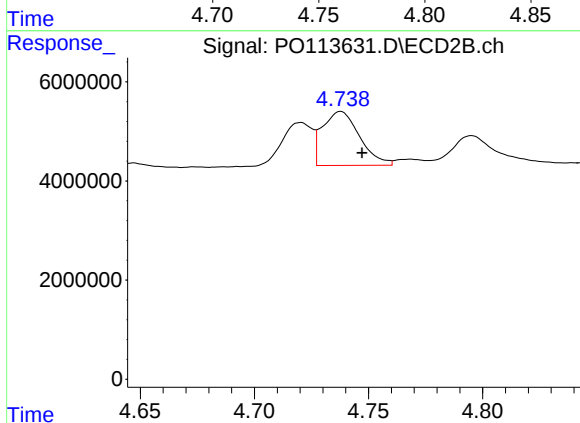


#17 AR-1242-2

R.T.: 4.738 min
Delta R.T.: -0.009 min
Response: 12320175
Conc: 56.80 ng/ml

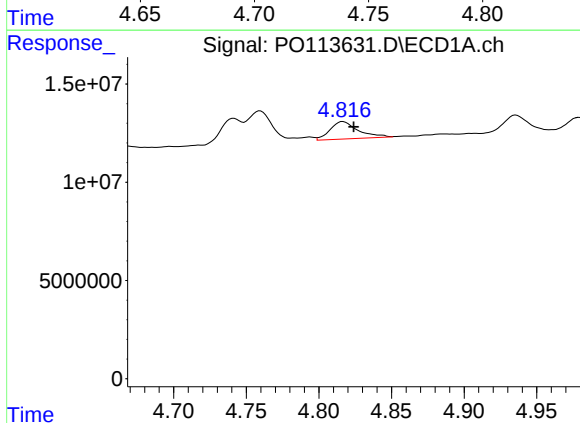


#18 AR-1242-3

R.T.: 4.817 min
Delta R.T.: -0.007 min
Response: 11976891
Conc: 53.98 ng/ml

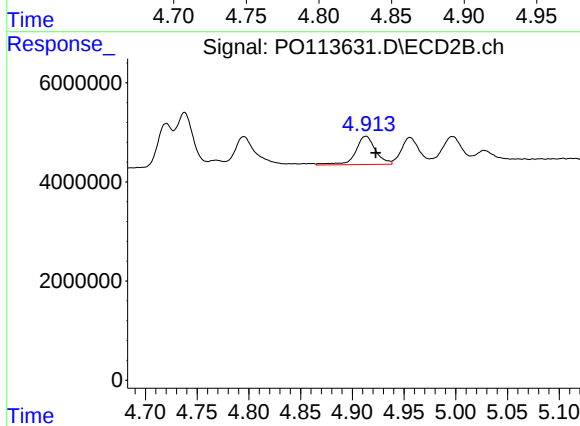

#18 AR-1242-3


R.T.: 4.913 min
Delta R.T.: -0.009 min
Response: 7693597
Conc: 65.78 ng/ml

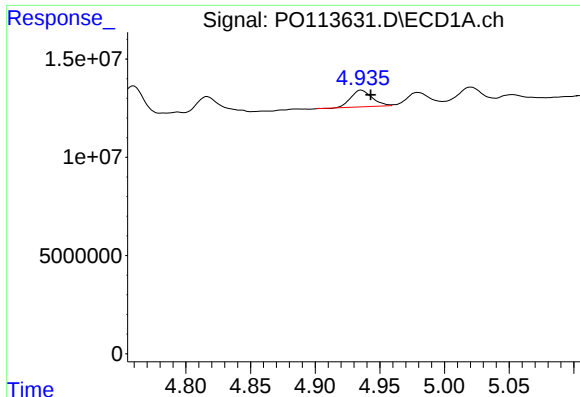

#19 AR-1242-4


R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 9665077
Conc: 55.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

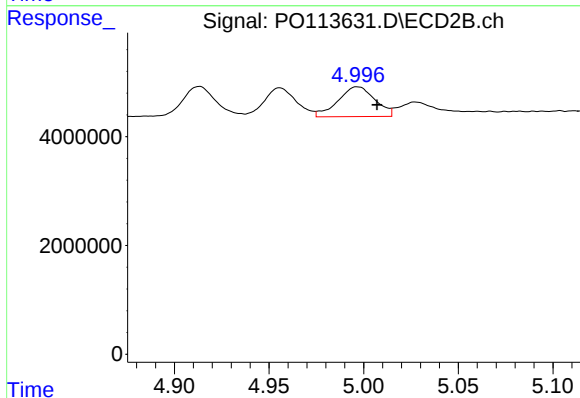


#19 AR-1242-4

R.T.: 4.997 min
Delta R.T.: -0.010 min
Response: 7463424
Conc: 63.44 ng/ml

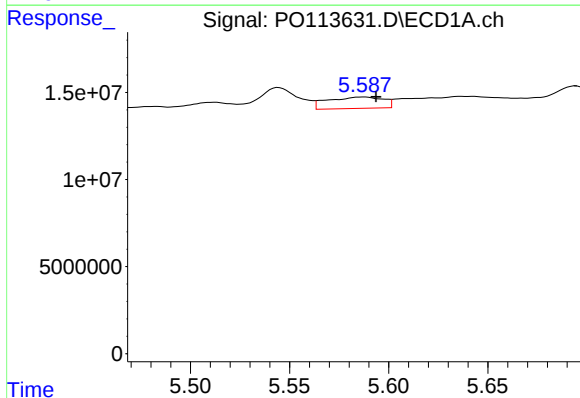


#20 AR-1242-5

R.T.: 5.588 min
Delta R.T.: -0.006 min
Response: 12697165
Conc: 63.43 ng/ml

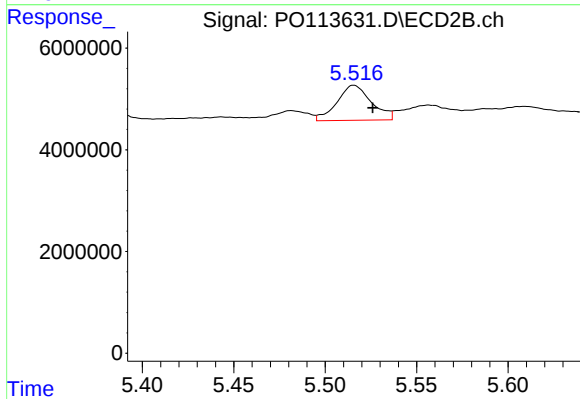

#20 AR-1242-5


R.T.: 5.516 min
Delta R.T.: -0.010 min
Response: 9010560
Conc: 60.42 ng/ml

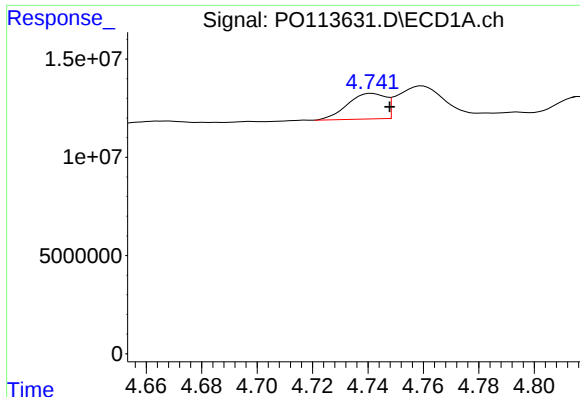

#21 AR-1248-1


R.T.: 4.741 min
Delta R.T.: -0.007 min
Response: 12364178
Conc: 70.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

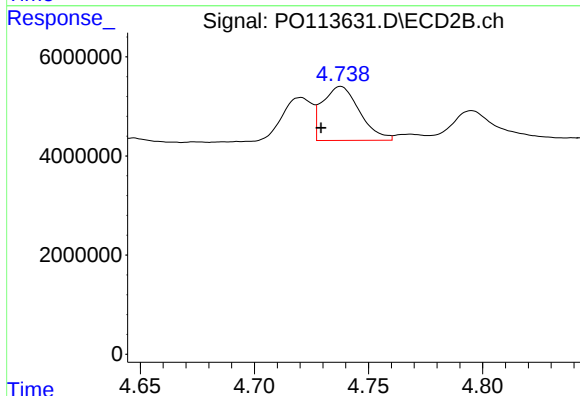


#21 AR-1248-1

R.T.: 4.738 min
Delta R.T.: 0.009 min
Response: 12320175
Conc: 110.48 ng/ml

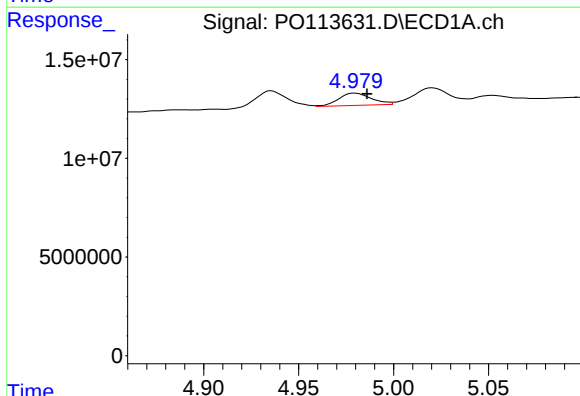


#22 AR-1248-2

R.T.: 4.980 min
Delta R.T.: -0.006 min
Response: 7452768
Conc: 30.81 ng/ml

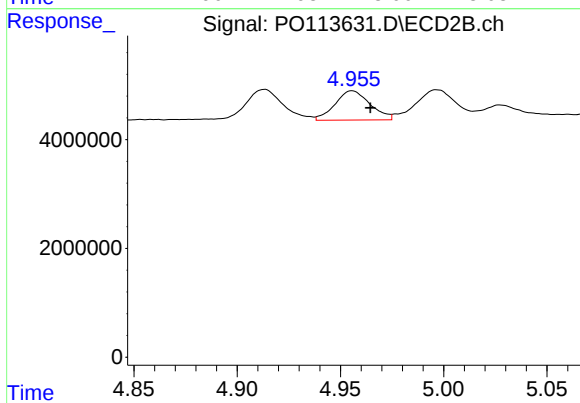

#22 AR-1248-2


R.T.: 4.956 min
Delta R.T.: -0.009 min
Response: 6347002
Conc: 39.50 ng/ml

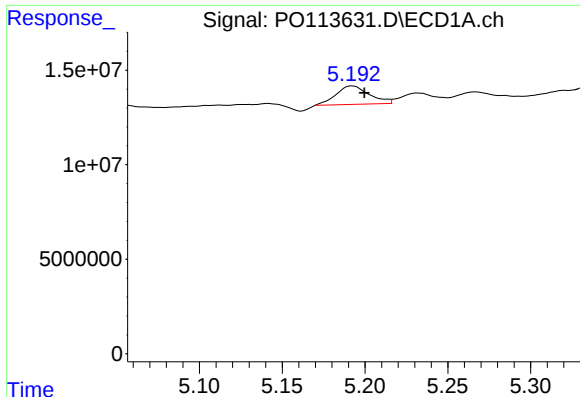

#23 AR-1248-3


R.T.: 5.192 min
Delta R.T.: -0.007 min
Response: 13728442
Conc: 43.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

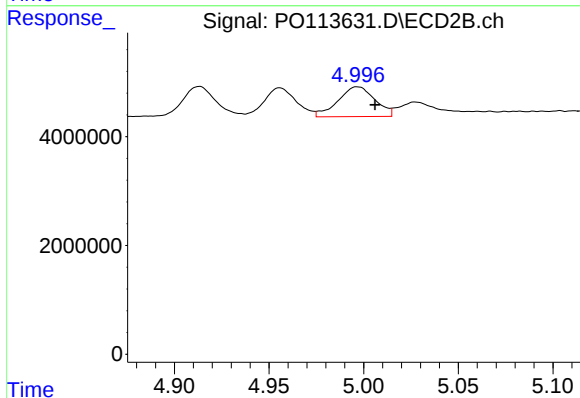


#23 AR-1248-3

R.T.: 4.997 min
Delta R.T.: -0.009 min
Response: 7463424
Conc: 43.99 ng/ml

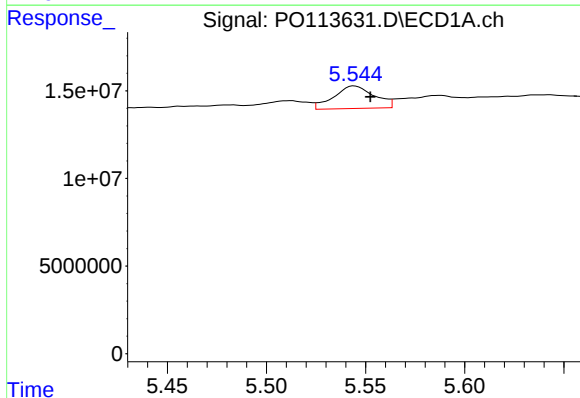


#24 AR-1248-4

R.T.: 5.544 min
Delta R.T.: -0.008 min
Response: 18234457
Conc: 36.50 ng/ml

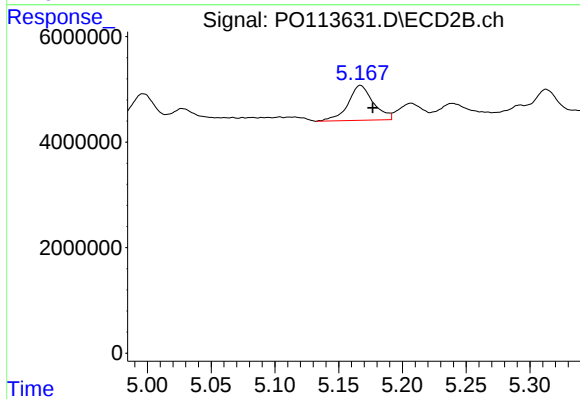

#24 AR-1248-4


R.T.: 5.167 min
Delta R.T.: -0.010 min
Response: 9150723
Conc: 45.93 ng/ml

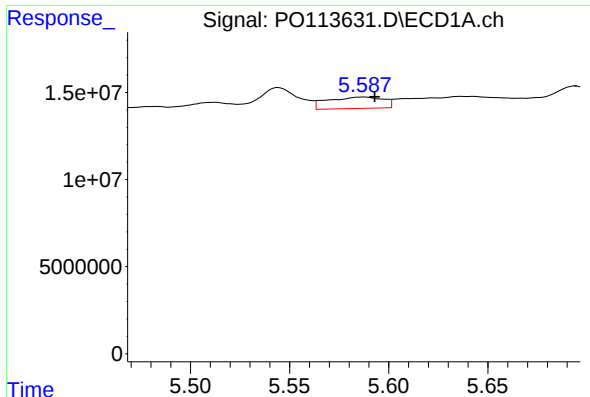

#25 AR-1248-5


R.T.: 5.588 min
Delta R.T.: -0.005 min
Response: 12697165
Conc: 37.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

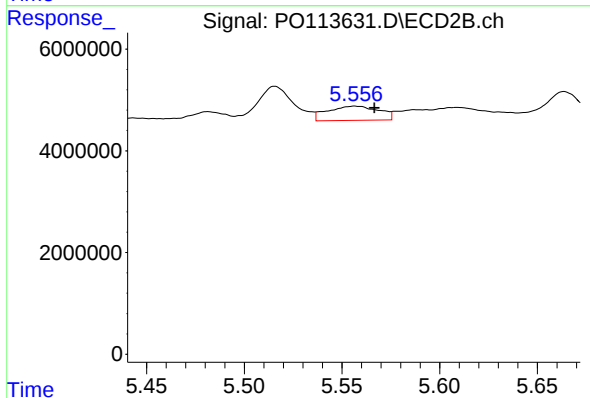


#25 AR-1248-5

R.T.: 5.557 min
Delta R.T.: -0.010 min
Response: 5123307
Conc: 24.13 ng/ml

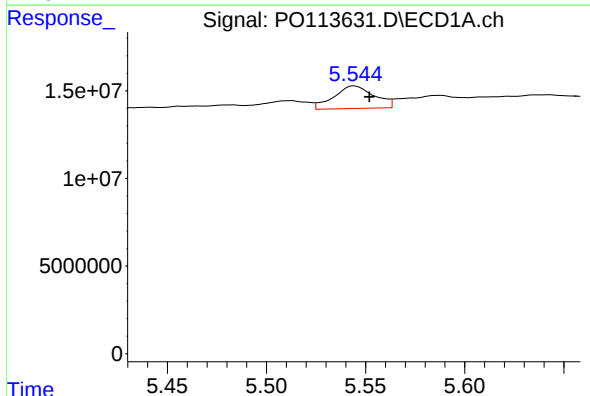


#26 AR-1254-1

R.T.: 5.544 min
Delta R.T.: -0.008 min
Response: 18234457
Conc: 33.77 ng/ml

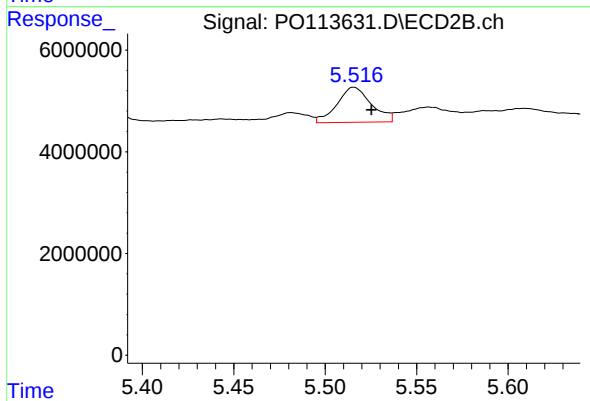

#26 AR-1254-1


R.T.: 5.516 min
Delta R.T.: -0.010 min
Response: 9010560
Conc: 28.57 ng/ml

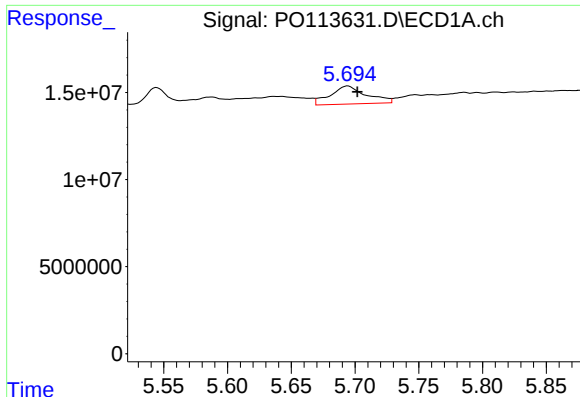

#27 AR-1254-2


R.T.: 5.694 min
Delta R.T.: -0.007 min
Response: 20349528
Conc: 41.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

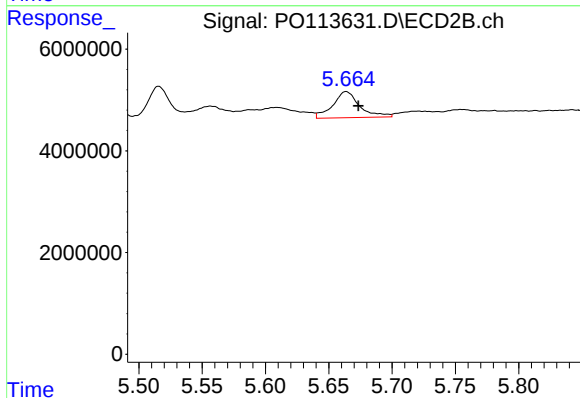


#27 AR-1254-2

R.T.: 5.664 min
Delta R.T.: -0.010 min
Response: 7578033
Conc: 27.03 ng/ml

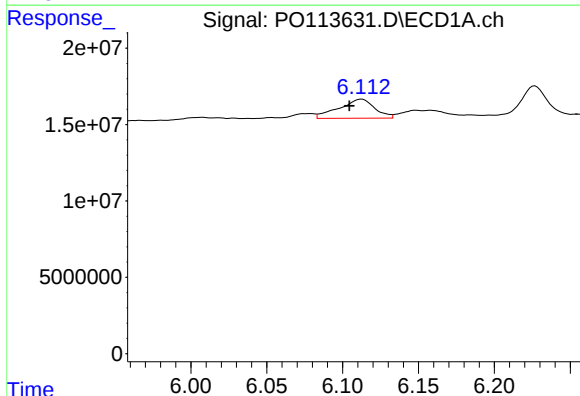


#28 AR-1254-3

R.T.: 6.113 min
Delta R.T.: 0.008 min
Response: 20317806
Conc: 27.50 ng/ml

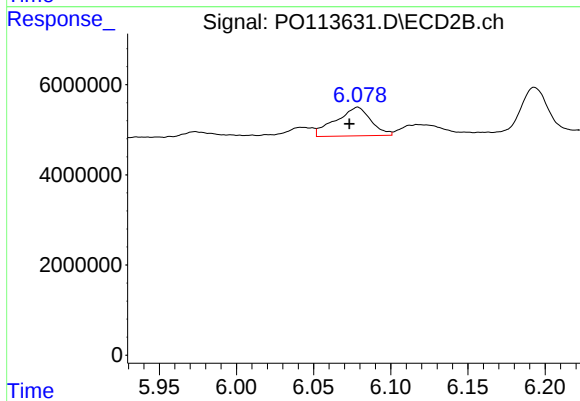

#28 AR-1254-3


R.T.: 6.079 min
Delta R.T.: 0.005 min
Response: 10093424
Conc: 24.21 ng/ml

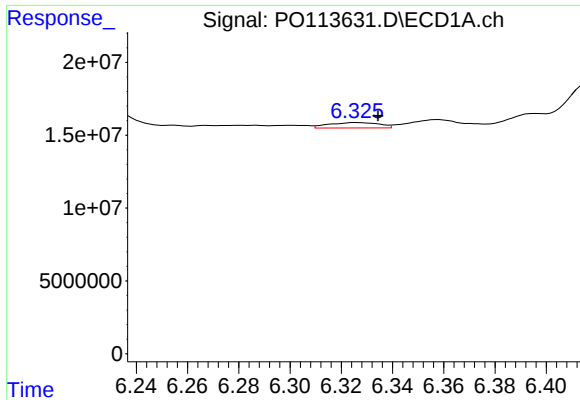

#29 AR-1254-4


R.T.: 6.326 min
Delta R.T.: -0.008 min
Response: 4974533
Conc: 8.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

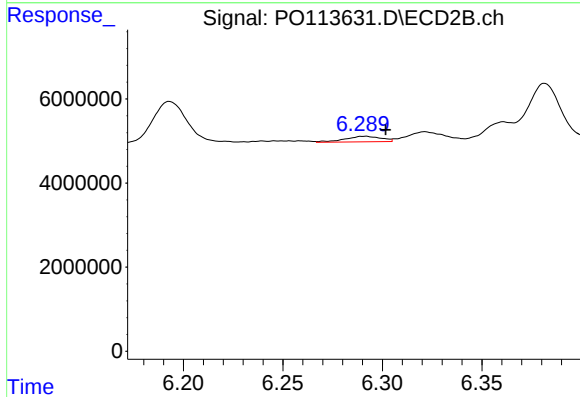


#29 AR-1254-4

R.T.: 6.291 min
Delta R.T.: -0.011 min
Response: 1670559
Conc: 6.08 ng/ml

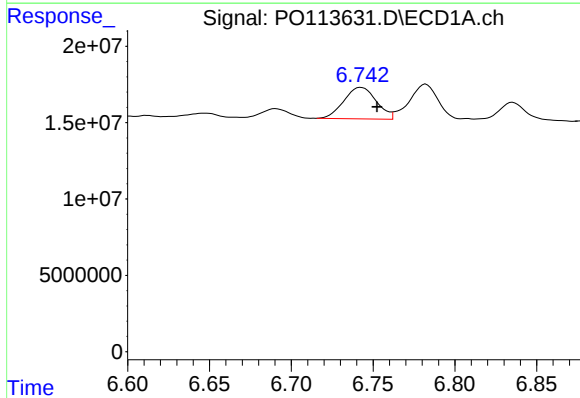


#30 AR-1254-5

R.T.: 6.743 min
Delta R.T.: -0.010 min
Response: 28483314
Conc: 40.63 ng/ml

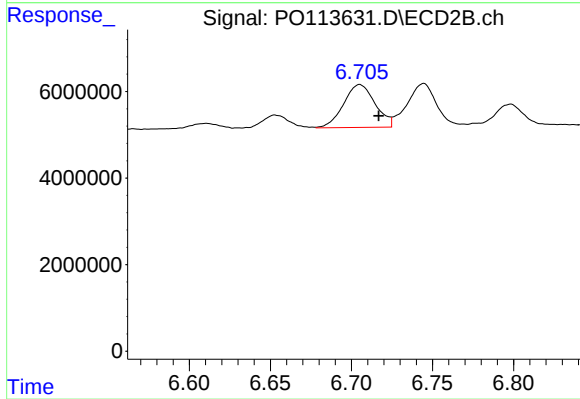

#30 AR-1254-5


R.T.: 6.705 min
Delta R.T.: -0.012 min
Response: 13439973
Conc: 37.60 ng/ml

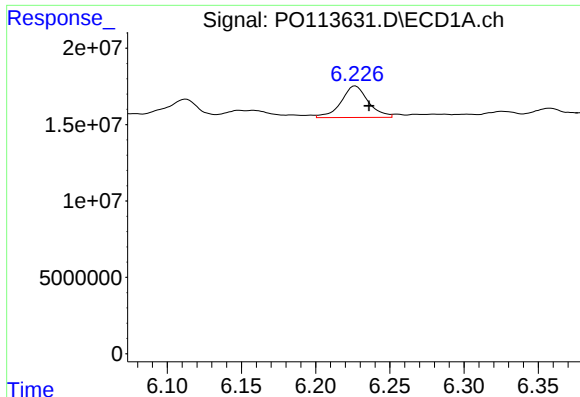

#31 AR-1260-1


R.T.: 6.227 min
Delta R.T.: -0.009 min
Response: 26366333
Conc: 59.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

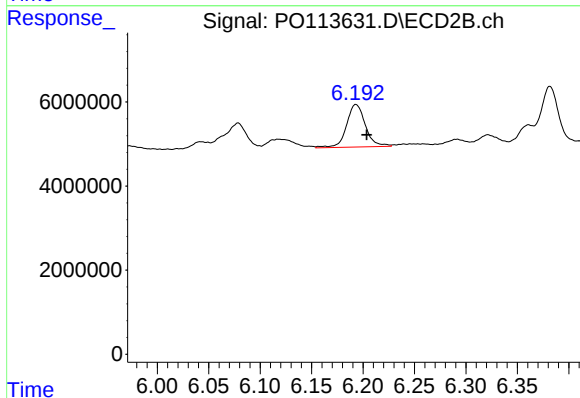


#31 AR-1260-1

R.T.: 6.193 min
Delta R.T.: -0.010 min
Response: 12949361
Conc: 50.77 ng/ml

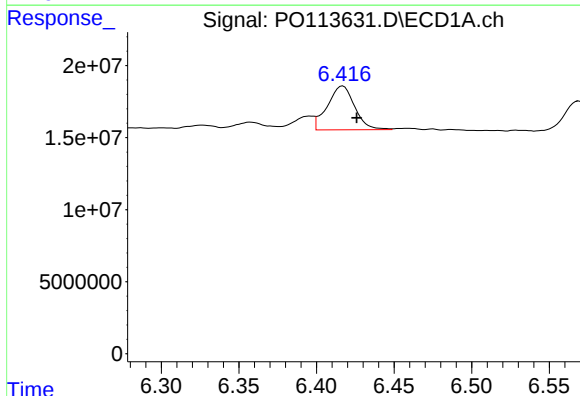


#32 AR-1260-2

R.T.: 6.417 min
Delta R.T.: -0.009 min
Response: 37410715
Conc: 54.48 ng/ml

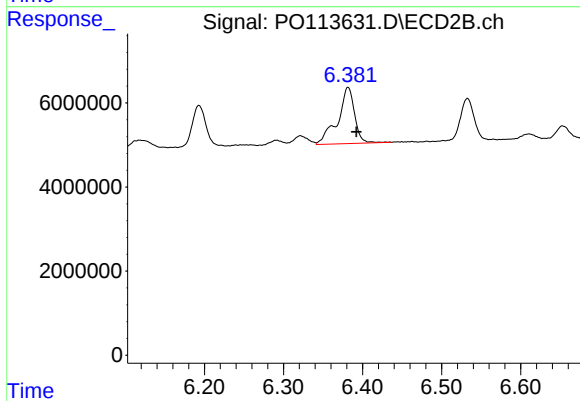

#32 AR-1260-2


R.T.: 6.382 min
Delta R.T.: -0.010 min
Response: 19928826
Conc: 57.65 ng/ml

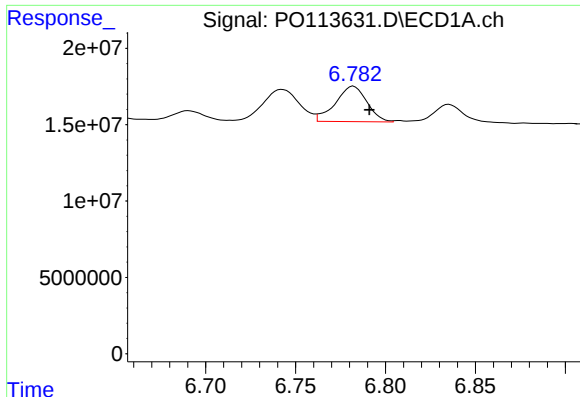

#33 AR-1260-3


R.T.: 6.782 min
Delta R.T.: -0.009 min
Response: 28255679
Conc: 45.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

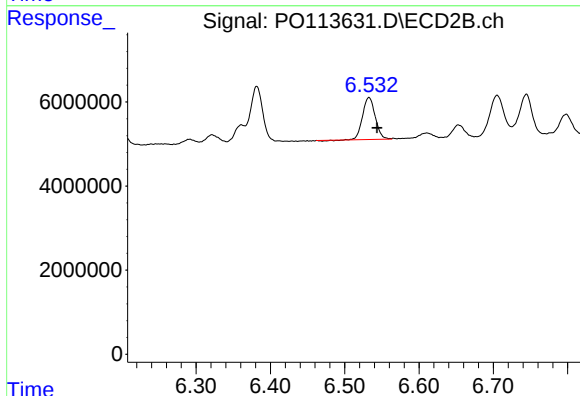


#33 AR-1260-3

R.T.: 6.533 min
Delta R.T.: -0.011 min
Response: 11777710
Conc: 39.60 ng/ml

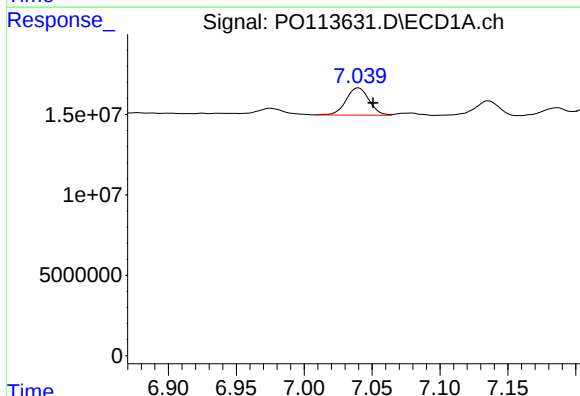


#34 AR-1260-4

R.T.: 7.040 min
Delta R.T.: -0.011 min
Response: 19964153
Conc: 44.58 ng/ml

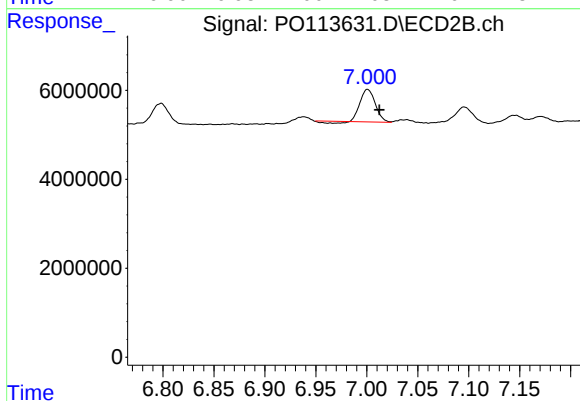

#34 AR-1260-4


R.T.: 7.001 min
Delta R.T.: -0.011 min
Response: 7360608
Conc: 35.52 ng/ml

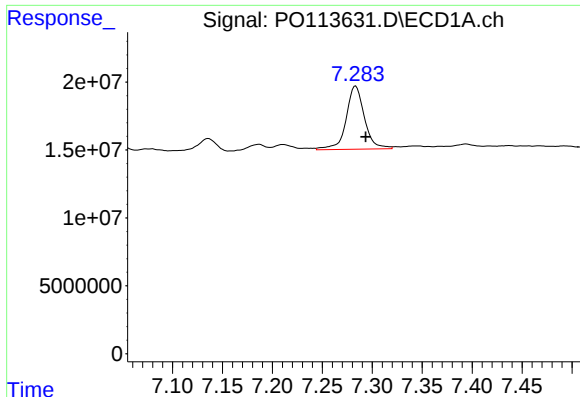

#35 AR-1260-5


R.T.: 7.283 min
Delta R.T.: -0.010 min
Response: 59158464
Conc: 48.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

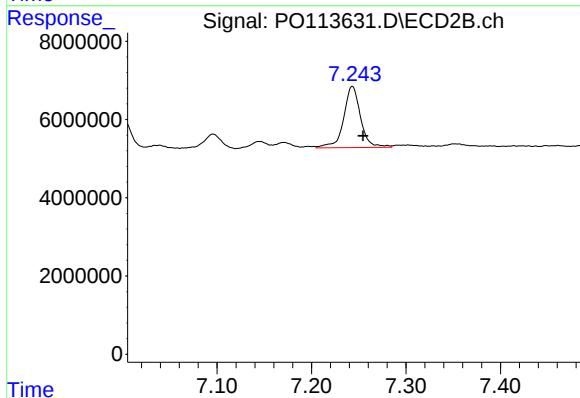


#35 AR-1260-5

R.T.: 7.243 min
Delta R.T.: -0.011 min
Response: 19464108
Conc: 41.55 ng/ml

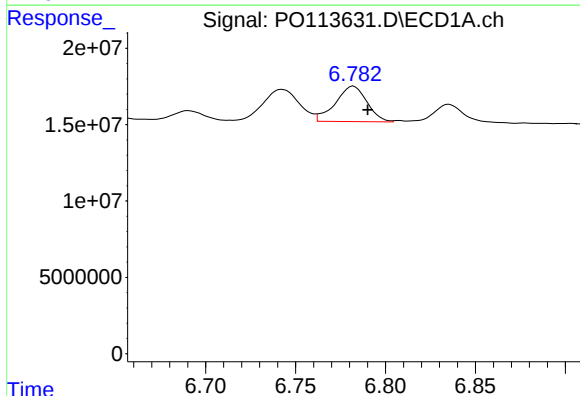


#36 AR-1262-1

R.T.: 6.782 min
Delta R.T.: -0.008 min
Response: 28255679
Conc: 30.85 ng/ml

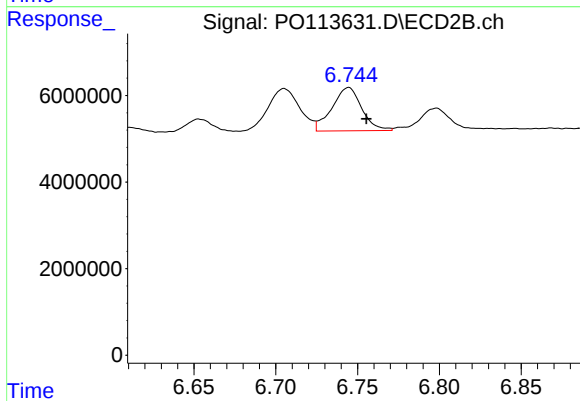

#36 AR-1262-1


R.T.: 6.745 min
Delta R.T.: -0.011 min
Response: 12702906
Conc: 30.64 ng/ml

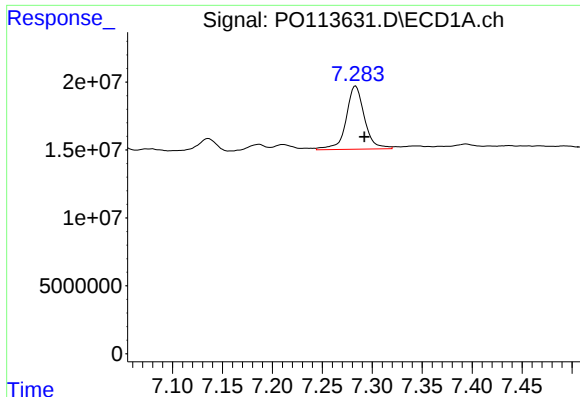

#37 AR-1262-2


R.T.: 7.283 min
Delta R.T.: -0.009 min
Response: 59158464
Conc: 39.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

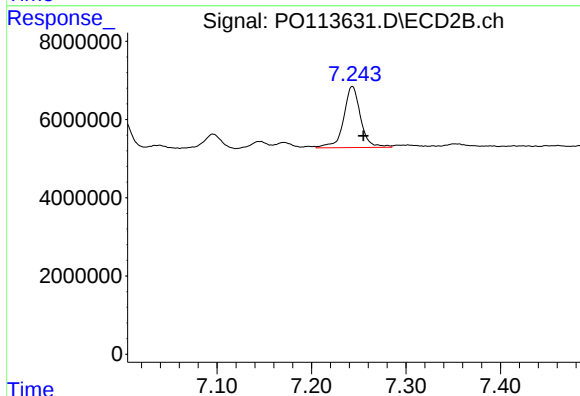


#37 AR-1262-2

R.T.: 7.243 min
Delta R.T.: -0.012 min
Response: 19464108
Conc: 37.60 ng/ml

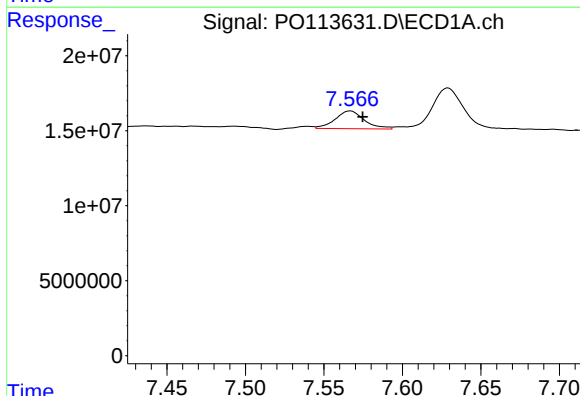


#38 AR-1262-3

R.T.: 7.567 min
Delta R.T.: -0.008 min
Response: 15335704
Conc: 27.68 ng/ml

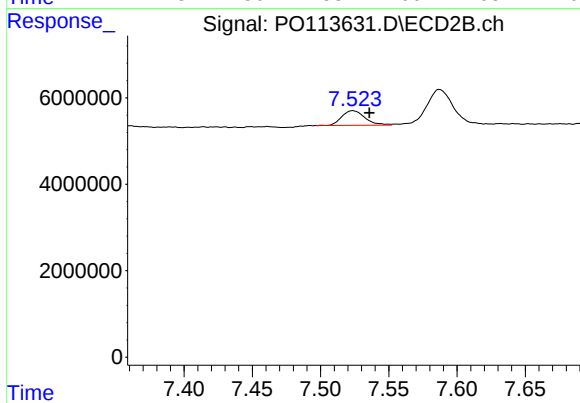

#38 AR-1262-3


R.T.: 7.524 min
Delta R.T.: -0.012 min
Response: 3998616
Conc: 22.27 ng/ml

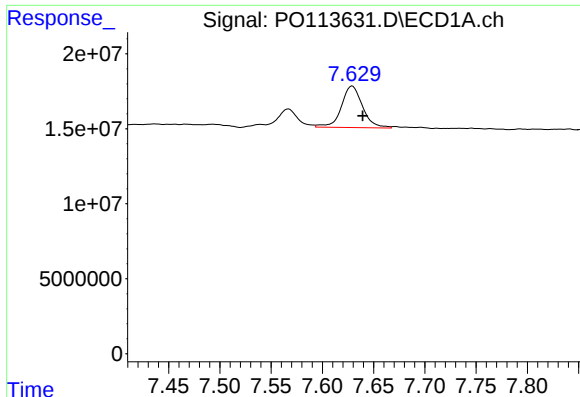

#39 AR-1262-4


R.T.: 7.629 min
Delta R.T.: -0.010 min
Response: 39636198
Conc: 40.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

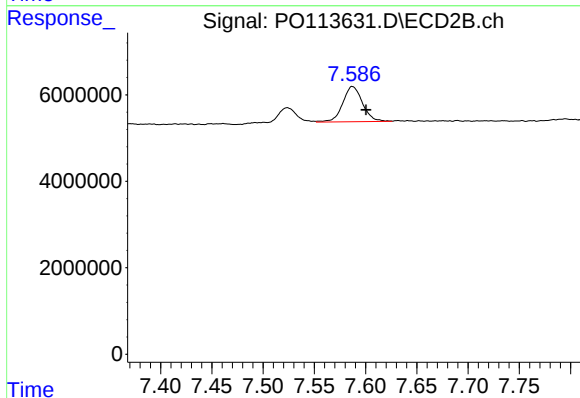


#39 AR-1262-4

R.T.: 7.587 min
Delta R.T.: -0.013 min
Response: 10940655
Conc: 37.74 ng/ml

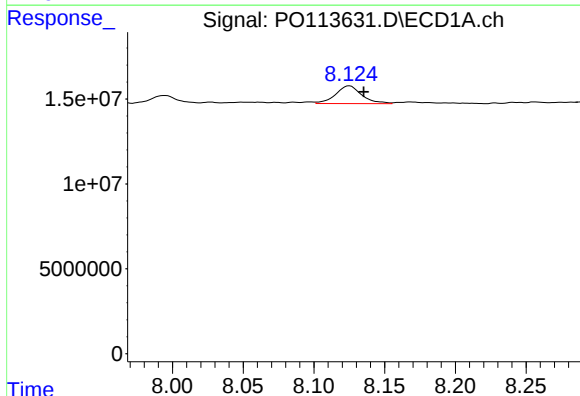


#40 AR-1262-5

R.T.: 8.125 min
Delta R.T.: -0.010 min
Response: 13382945
Conc: 32.10 ng/ml

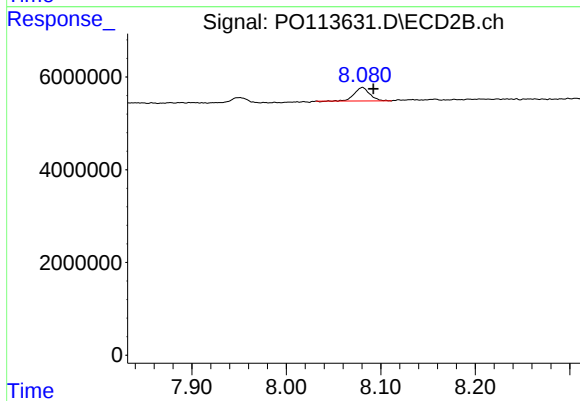

#40 AR-1262-5


R.T.: 8.081 min
Delta R.T.: -0.012 min
Response: 3248604
Conc: 29.99 ng/ml

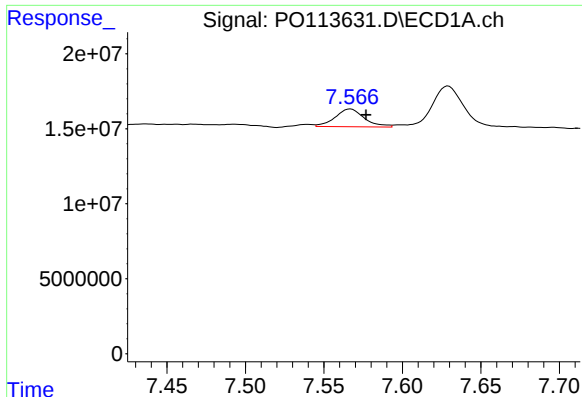

#41 AR-1268-1


R.T.: 7.567 min
Delta R.T.: -0.010 min
Response: 15335704
Conc: 8.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

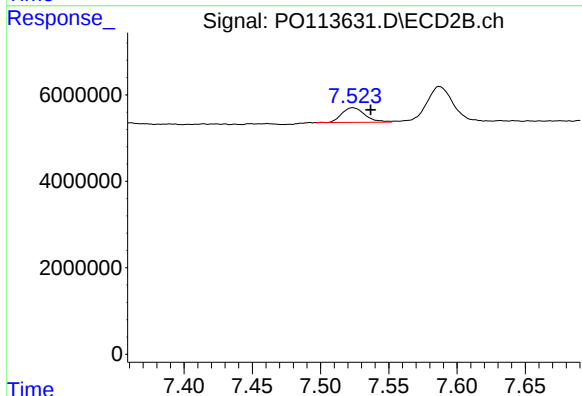


#41 AR-1268-1

R.T.: 7.524 min
Delta R.T.: -0.013 min
Response: 3998616
Conc: 7.85 ng/ml

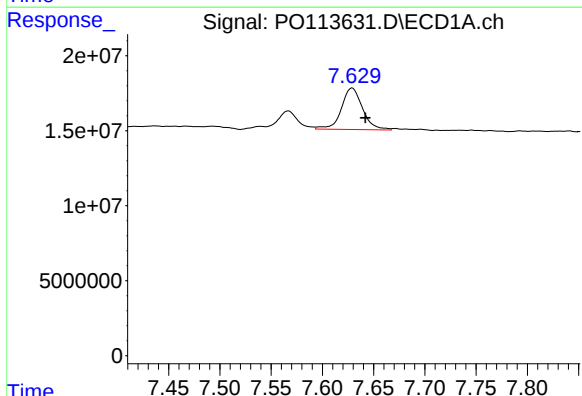


#42 AR-1268-2

R.T.: 7.629 min
Delta R.T.: -0.013 min
Response: 39636198
Conc: 27.37 ng/ml

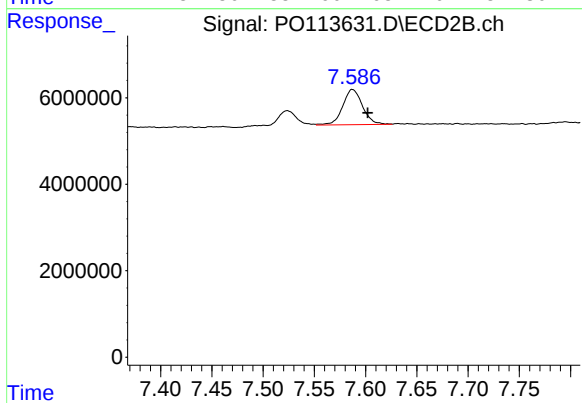

#42 AR-1268-2


R.T.: 7.587 min
Delta R.T.: -0.015 min
Response: 10940655
Conc: 26.34 ng/ml

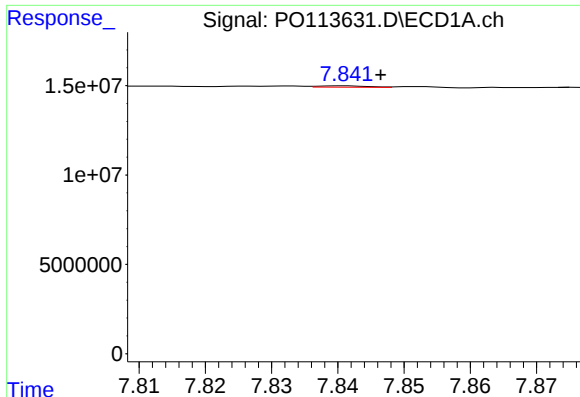

#43 AR-1268-3


R.T.: 7.841 min
Delta R.T.: -0.005 min
Response: 391419
Conc: 0.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

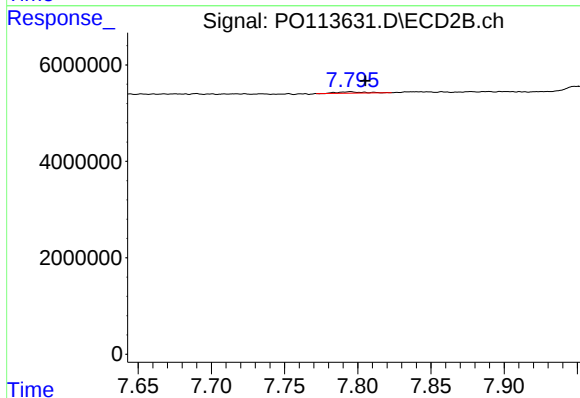


#43 AR-1268-3

R.T.: 7.795 min
Delta R.T.: -0.010 min
Response: 368217
Conc: 1.13 ng/ml

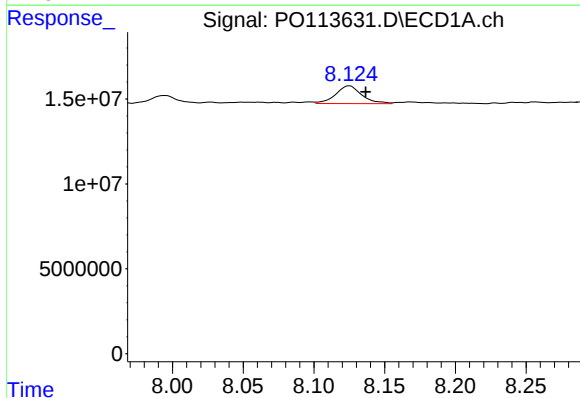


#44 AR-1268-4

R.T.: 8.125 min
Delta R.T.: -0.012 min
Response: 13382945
Conc: 29.05 ng/ml

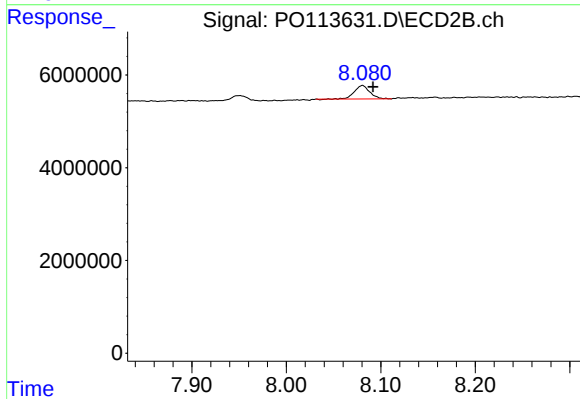

#44 AR-1268-4


R.T.: 8.081 min
Delta R.T.: -0.011 min
Response: 3248604
Conc: 26.97 ng/ml

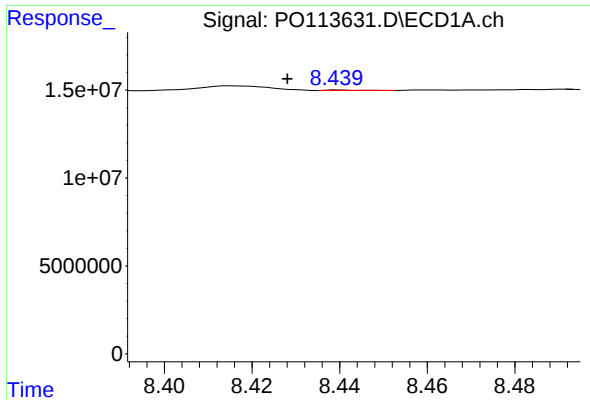

#45 AR-1268-5

R.T.: 8.440 min
Delta R.T.: 0.012 min
Response: 162204
Conc: 0.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

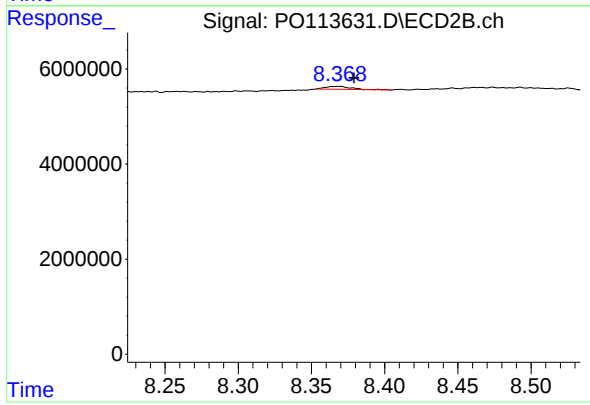

#45 AR-1268-5

R.T.: 8.369 min
Delta R.T.: -0.010 min
Response: 775039
Conc: 0.99 ng/ml