

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
 Data File : P0113632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 02:25
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1221 WATER LOD 40PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:29:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.658	3.649	183.3E6	107.7E6	22.392	21.275
2)	SA Decachlor...	8.669	8.613	151.7E6	44030058	21.882	23.237
Target Compounds							
3)	L1 AR-1016-1	4.742	4.723	675496	583985	2.530	3.424 #
4)	L1 AR-1016-2	4.765	4.741	1073303	455384	2.674	1.767 #
5)	L1 AR-1016-3	4.817	4.912	864835	1013607	3.391	7.260 #
6)	L1 AR-1016-4	4.941	4.967	1428774	357397	6.552	3.063 #
7)	L1 AR-1016-5	5.206	5.181	2684864	339479	12.114	2.382 #
8)	L2 AR-1221-1	3.870	3.857	3779465	2292885	40.390	36.325
9)	L2 AR-1221-2	3.956	3.944	3761380	3081733	55.682	66.028
10)	L2 AR-1221-3	4.030	4.016	7771932	5934380	35.111	39.969
11)	L3 AR-1232-1	4.030	4.016	7771932	5934380	43.291	49.072
12)	L3 AR-1232-2	4.526	4.741	702223	455384	6.507	3.731 #
13)	L3 AR-1232-3	4.765	4.912	1073303	1013607	5.437	15.321 #
14)	L3 AR-1232-4	4.941	4.995	1428774	347202	14.536	5.794 #
15)	L3 AR-1232-5	4.959	5.169	451503	347640	6.864	5.141 #
16)	L4 AR-1242-1	4.742	4.723	675496	583985	2.938	4.041 #
17)	L4 AR-1242-2	4.765	4.741	1073303	455384	3.123	2.099 #
18)	L4 AR-1242-3	4.817	4.912	864835	1013607	3.898	8.666 #
19)	L4 AR-1242-4	4.941	5.010	1428774	146227	8.237	1.243 #
20)	L4 AR-1242-5	5.601	5.522	16706776	199516	83.466	1.338 #
21)	L5 AR-1248-1	4.742	4.723	675496	583985	3.872	5.237 #
22)	L5 AR-1248-2	5.004	4.967	1708726	357397	7.065	2.224 #
23)	L5 AR-1248-3	5.206	5.003	2684864	218352	8.420	1.287 #
24)	L5 AR-1248-4	5.522	5.181	6230087	339479	12.470	1.704 #
25)	L5 AR-1248-5	5.601	5.565	16706776	802549	48.923	3.780 #
26)	L6 AR-1254-1	5.522	5.522	6230087	199516	11.538	0.633 #
27)	L6 AR-1254-2	5.706	5.676	2010174	221974	4.074	0.792 #
28)	L6 AR-1254-3	6.097	6.073	1060052	151308	1.435	0.363 #
29)	L6 AR-1254-4	6.346	6.301	1733222	134262	3.112	0.489 #
30)	L6 AR-1254-5	6.755	6.709	568942	216644	0.812	0.606 #
31)	L7 AR-1260-1	6.234	6.204	1356466	80456	3.042	0.315 #
32)	L7 AR-1260-2	6.395	6.392	13804735	56650	20.102	0.164 #
33)	L7 AR-1260-3	6.779	6.547	530800	39971	0.860	0.134 #
34)	L7 AR-1260-4	7.052	7.015	398242	193021	0.889	0.931
35)	L7 AR-1260-5	7.303	7.250	1187919	109278	0.981	0.233 #
36)	L8 AR-1262-1	6.779	6.756	530800	71604	0.580	0.173 #
37)	L8 AR-1262-2	7.303	7.250	1187919	109278	0.786	0.211 #
38)	L8 AR-1262-3	7.579	7.534	359415	134263	0.649	0.748
39)	L8 AR-1262-4	7.632	7.602	522942	31338	0.535	0.108 #
40)	L8 AR-1262-5	8.135	8.094	547566	32578	1.313	0.301 #
41)	L9 AR-1268-1	7.579	7.534	359415	134263	0.209	0.264 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
Data File : P0113632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 02:25
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1221 WATER LOD 40PPB
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:29:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.650	7.602	324625	31338	0.224	0.075 #
43)	L9 AR-1268-3	7.832	7.808	957017	53551	0.793	0.164 #
44)	L9 AR-1268-4	8.135	8.094	547566	32578	1.189	0.271 #
45)	L9 AR-1268-5	8.423	8.377	700201	75851	0.220	0.097 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091025\
Data File : PO113632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 02:25
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1221 WATER LOD 40PPB
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:29:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

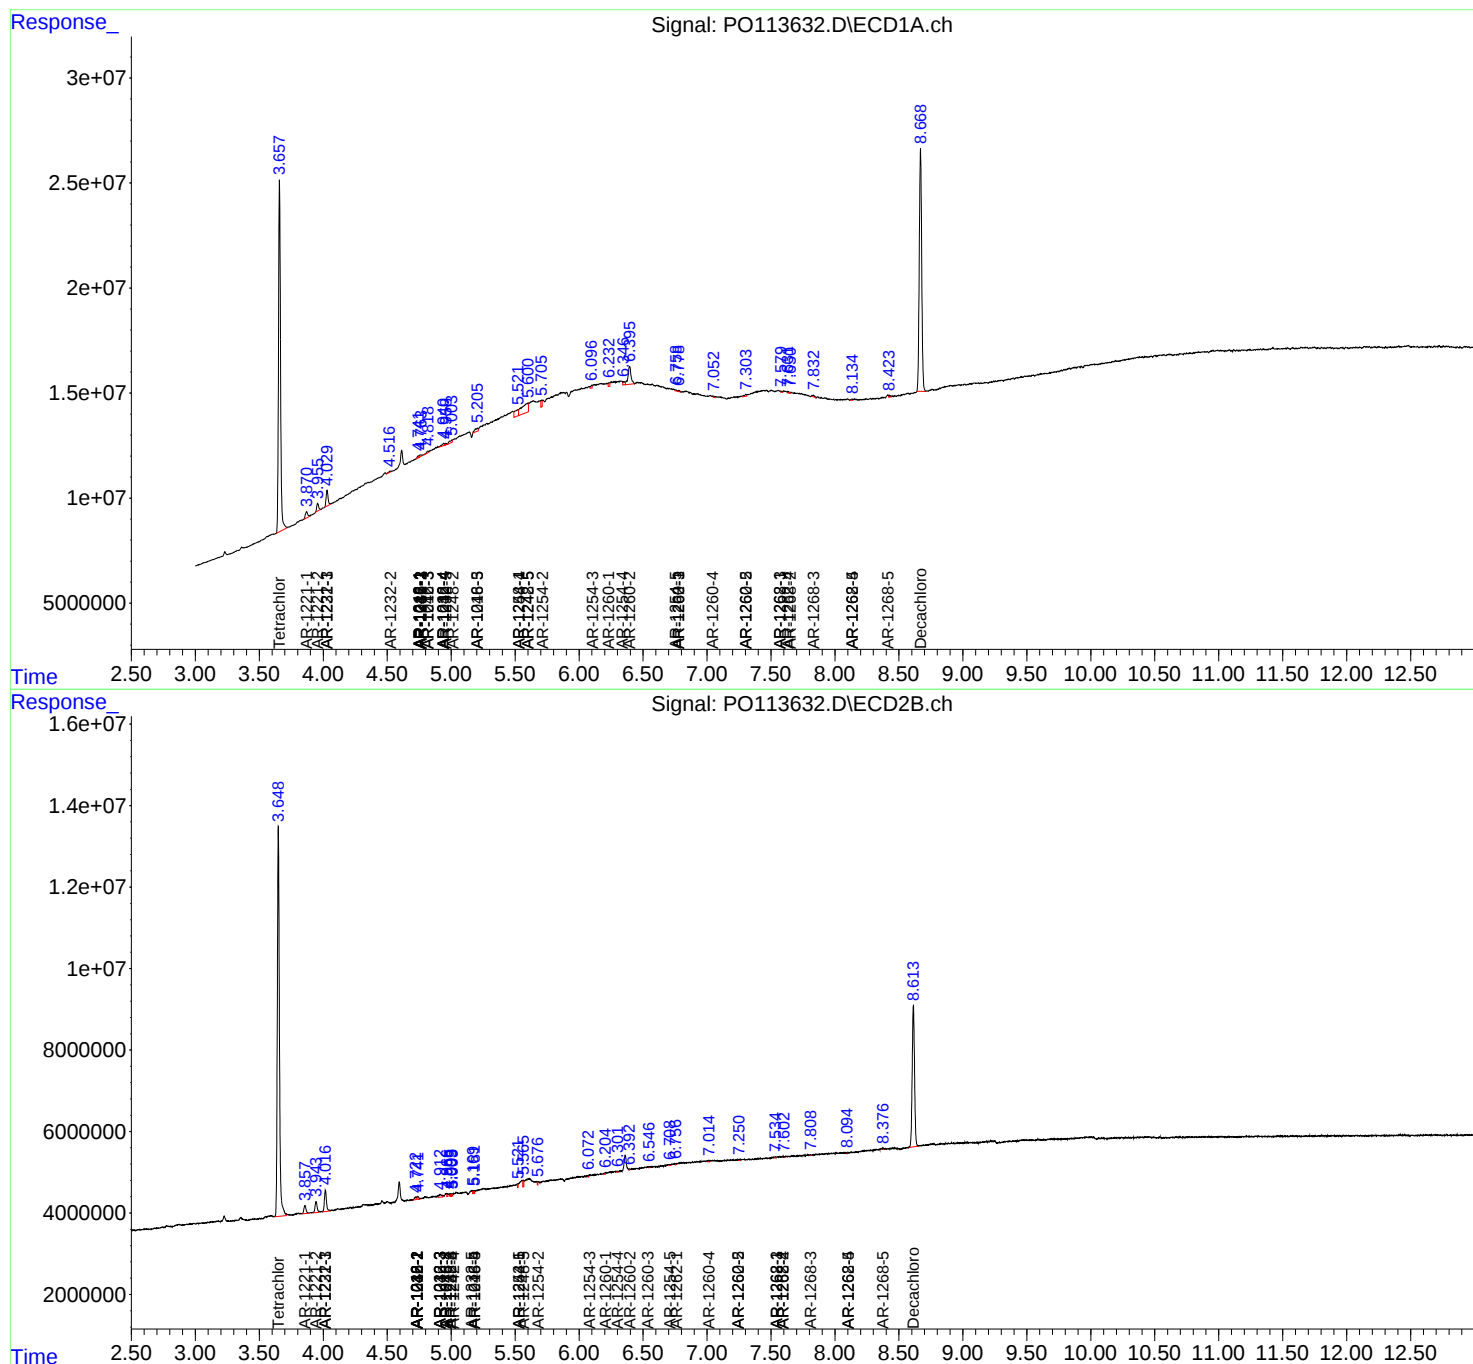


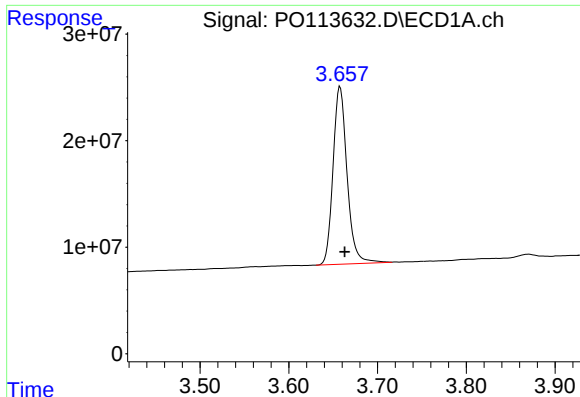

#1 Tetrachloro-m-xylene


R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 183315446
Conc: 22.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

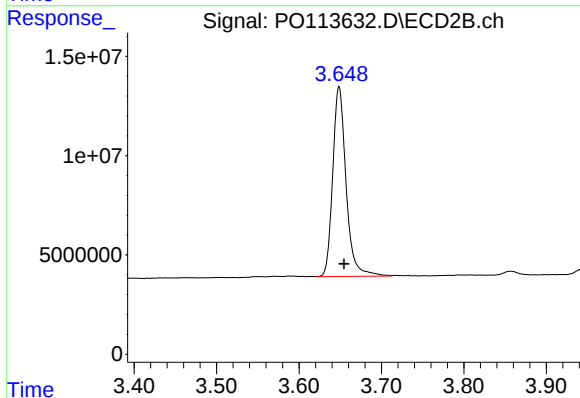


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.006 min
Response: 107662976
Conc: 21.27 ng/ml

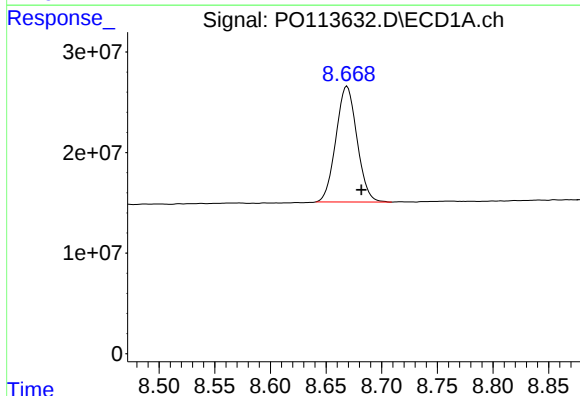


#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.013 min
Response: 151674761
Conc: 21.88 ng/ml

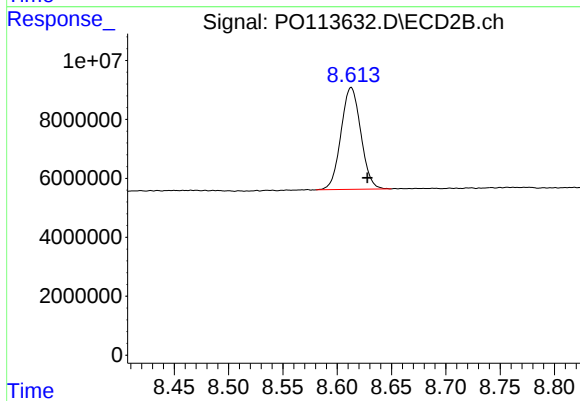

#2 Decachlorobiphenyl


R.T.: 8.613 min
Delta R.T.: -0.015 min
Response: 44030058
Conc: 23.24 ng/ml

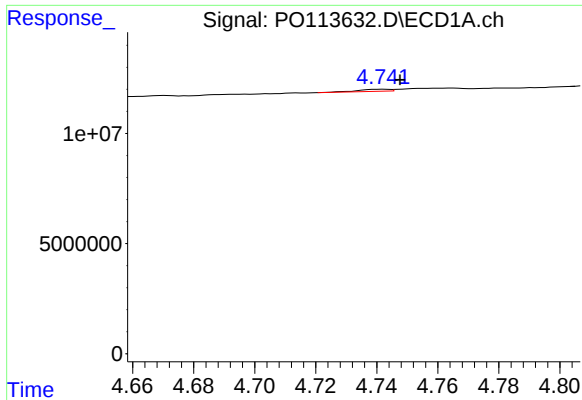

#3 AR-1016-1


R.T.: 4.742 min
Delta R.T.: -0.006 min
Response: 675496
Conc: 2.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

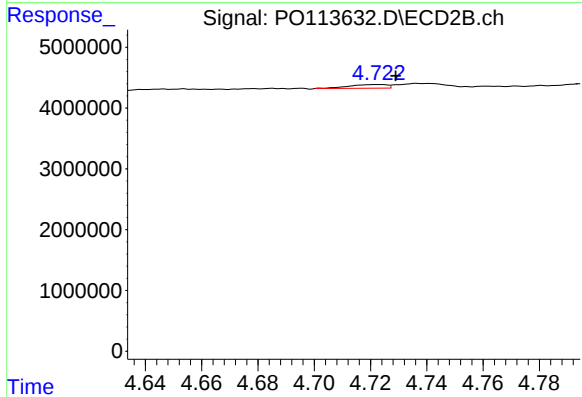


#3 AR-1016-1

R.T.: 4.723 min
Delta R.T.: -0.006 min
Response: 583985
Conc: 3.42 ng/ml

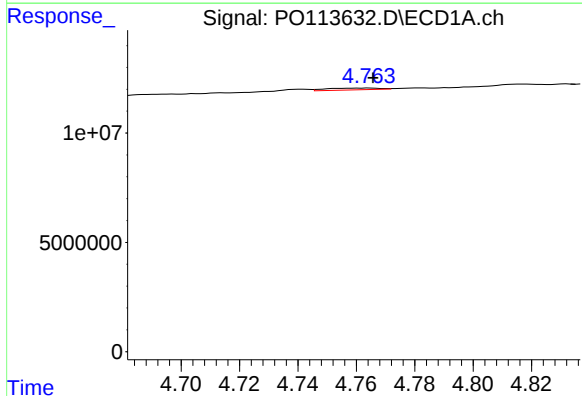


#4 AR-1016-2

R.T.: 4.765 min
Delta R.T.: -0.001 min
Response: 1073303
Conc: 2.67 ng/ml

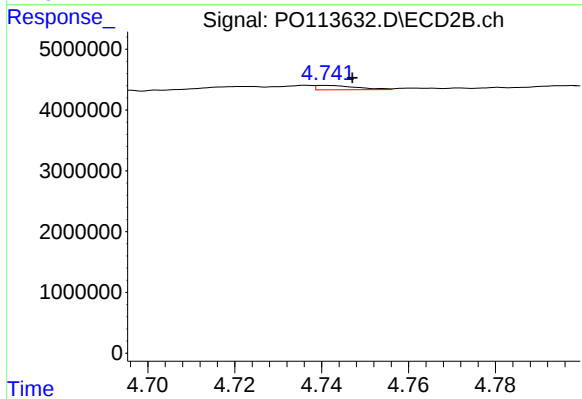

#4 AR-1016-2


R.T.: 4.741 min
Delta R.T.: -0.006 min
Response: 455384
Conc: 1.77 ng/ml

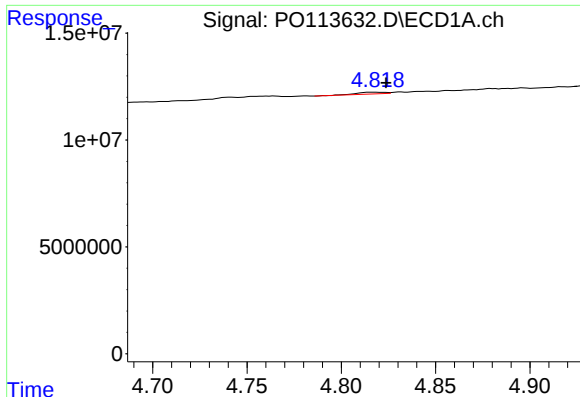

#5 AR-1016-3


R.T.: 4.817 min
Delta R.T.: -0.007 min
Response: 864835
Conc: 3.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

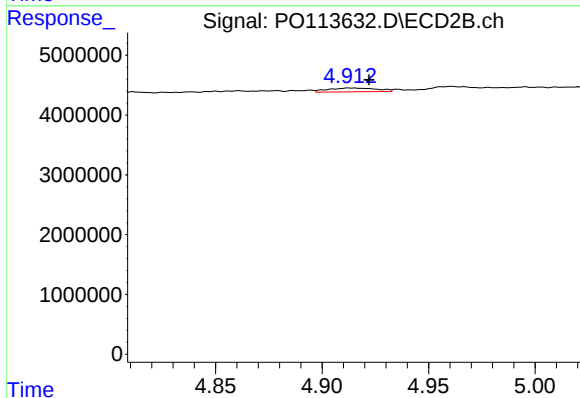


#5 AR-1016-3

R.T.: 4.912 min
Delta R.T.: -0.010 min
Response: 1013607
Conc: 7.26 ng/ml

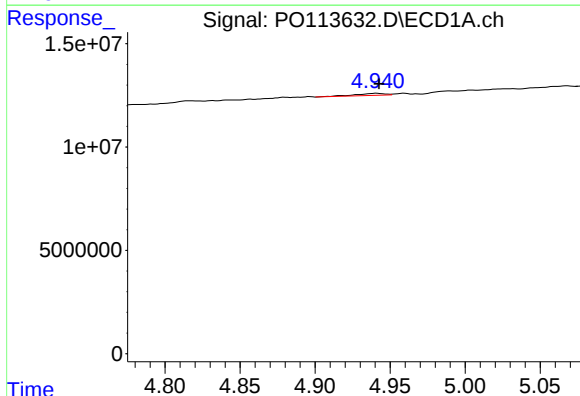


#6 AR-1016-4

R.T.: 4.941 min
Delta R.T.: -0.002 min
Response: 1428774
Conc: 6.55 ng/ml

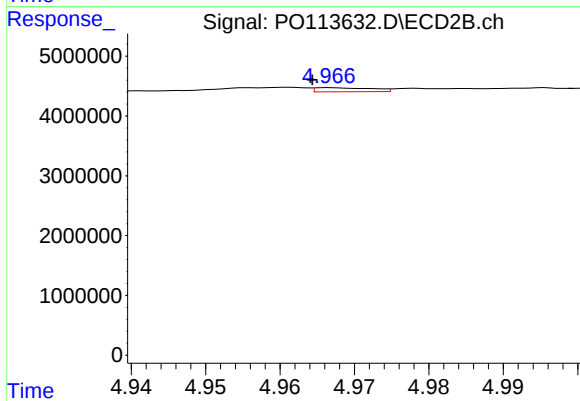

#6 AR-1016-4


R.T.: 4.967 min
Delta R.T.: 0.002 min
Response: 357397
Conc: 3.06 ng/ml

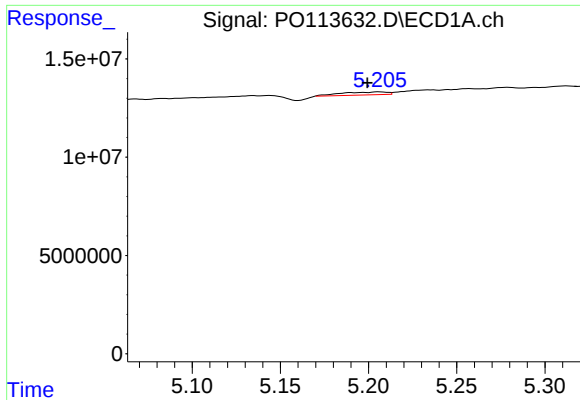

#7 AR-1016-5


R.T.: 5.206 min
Delta R.T.: 0.006 min
Response: 2684864
Conc: 12.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

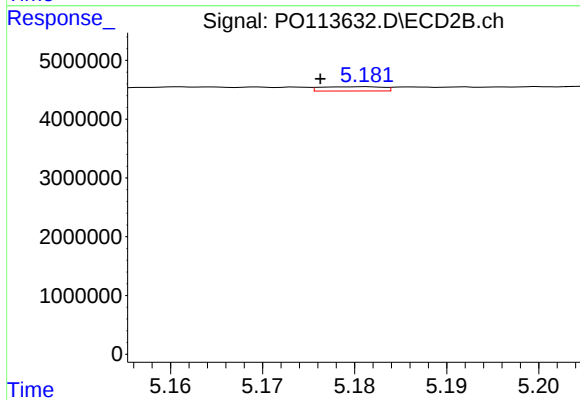


#7 AR-1016-5

R.T.: 5.181 min
Delta R.T.: 0.005 min
Response: 339479
Conc: 2.38 ng/ml

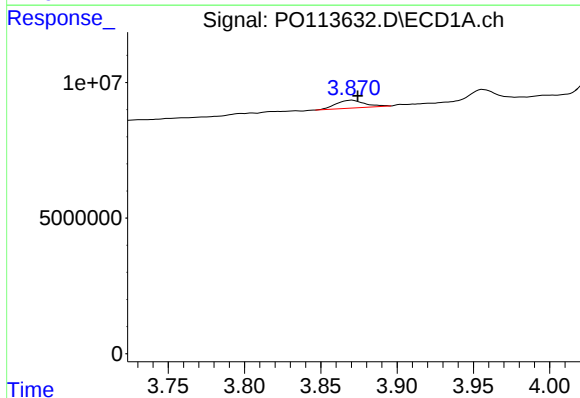


#8 AR-1221-1

R.T.: 3.870 min
Delta R.T.: -0.004 min
Response: 3779465
Conc: 40.39 ng/ml

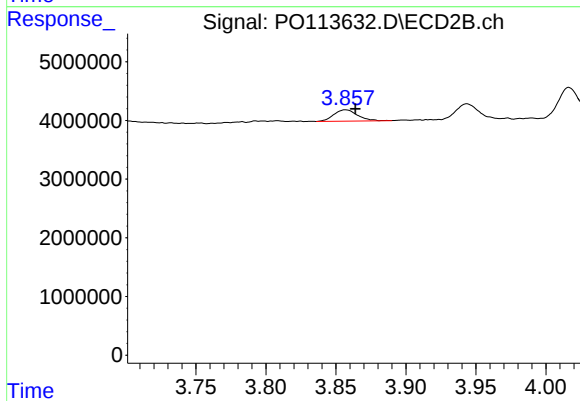

#8 AR-1221-1


R.T.: 3.857 min
Delta R.T.: -0.007 min
Response: 2292885
Conc: 36.33 ng/ml

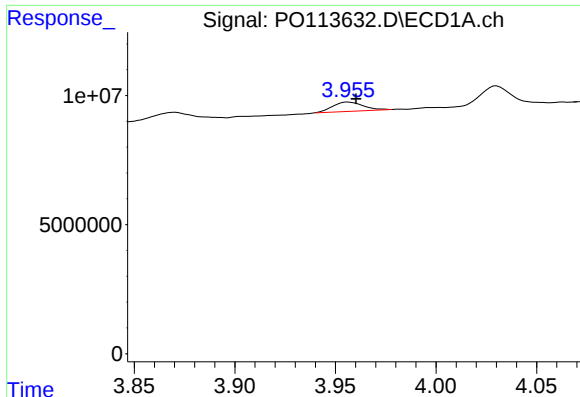

#9 AR-1221-2


R.T.: 3.956 min
Delta R.T.: -0.004 min
Response: 3761380
Conc: 55.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

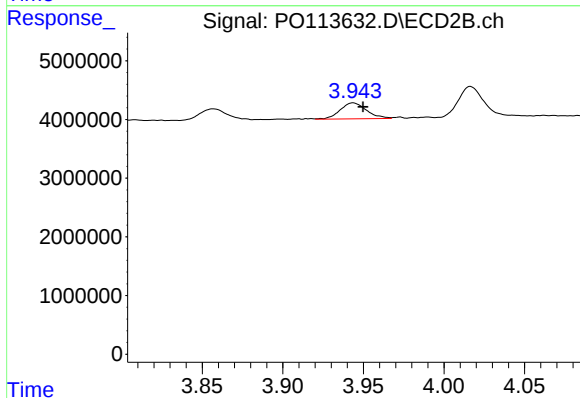


#9 AR-1221-2

R.T.: 3.944 min
Delta R.T.: -0.006 min
Response: 3081733
Conc: 66.03 ng/ml

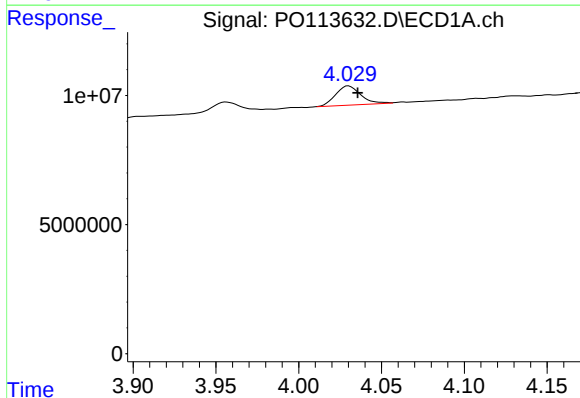


#10 AR-1221-3

R.T.: 4.030 min
Delta R.T.: -0.005 min
Response: 7771932
Conc: 35.11 ng/ml

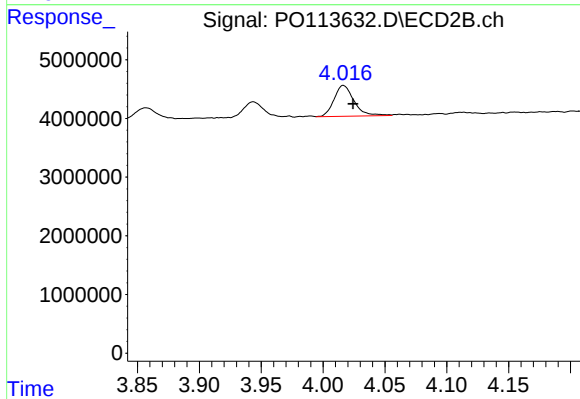

#10 AR-1221-3


R.T.: 4.016 min
Delta R.T.: -0.008 min
Response: 5934380
Conc: 39.97 ng/ml

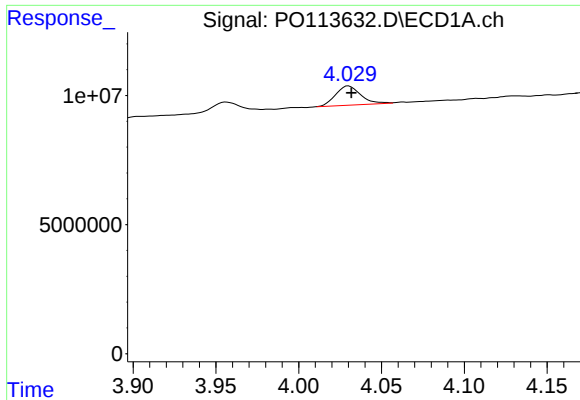

#11 AR-1232-1


R.T.: 4.030 min
Delta R.T.: -0.002 min
Response: 7771932
Conc: 43.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

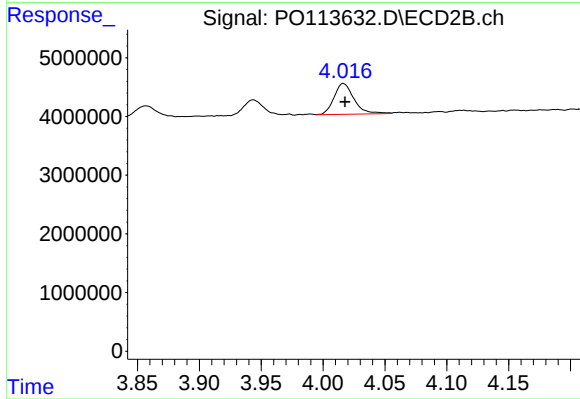


#11 AR-1232-1

R.T.: 4.016 min
Delta R.T.: -0.001 min
Response: 5934380
Conc: 49.07 ng/ml

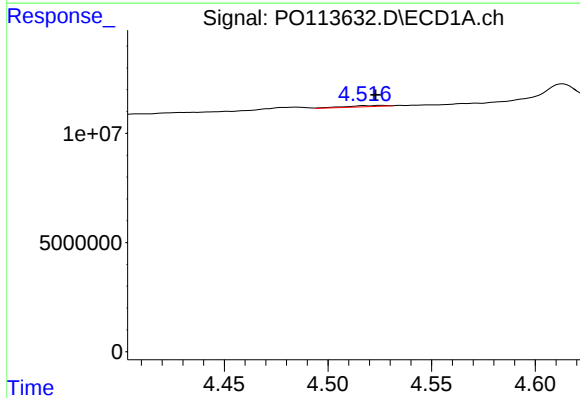


#12 AR-1232-2

R.T.: 4.526 min
Delta R.T.: 0.003 min
Response: 702223
Conc: 6.51 ng/ml

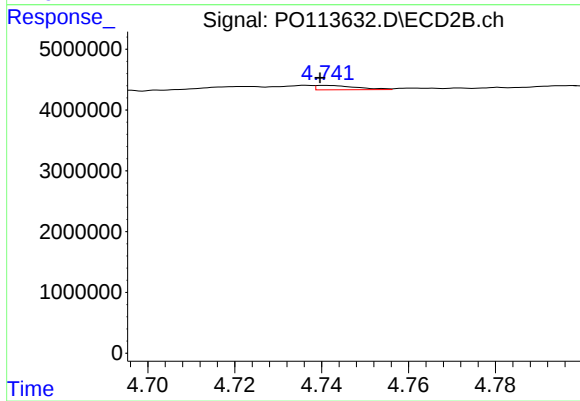

#12 AR-1232-2


R.T.: 4.741 min
Delta R.T.: 0.001 min
Response: 455384
Conc: 3.73 ng/ml

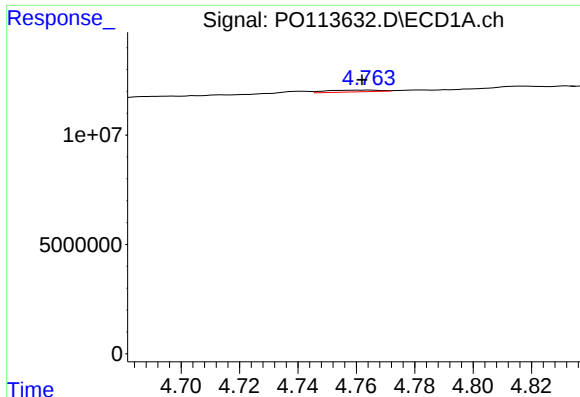

#13 AR-1232-3


R.T.: 4.765 min
Delta R.T.: 0.003 min
Response: 1073303
Conc: 5.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

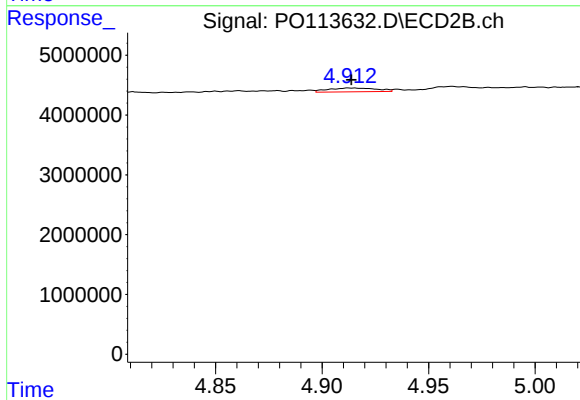


#13 AR-1232-3

R.T.: 4.912 min
Delta R.T.: -0.001 min
Response: 1013607
Conc: 15.32 ng/ml

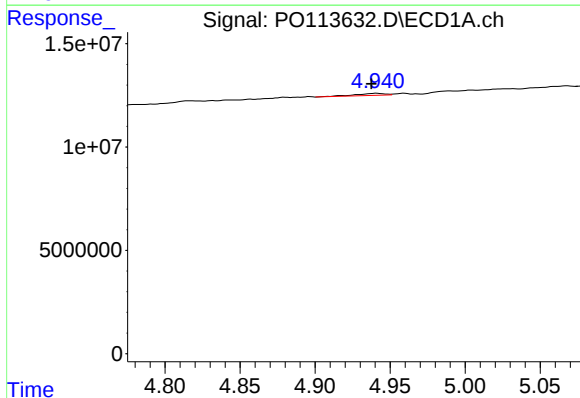


#14 AR-1232-4

R.T.: 4.941 min
Delta R.T.: 0.003 min
Response: 1428774
Conc: 14.54 ng/ml

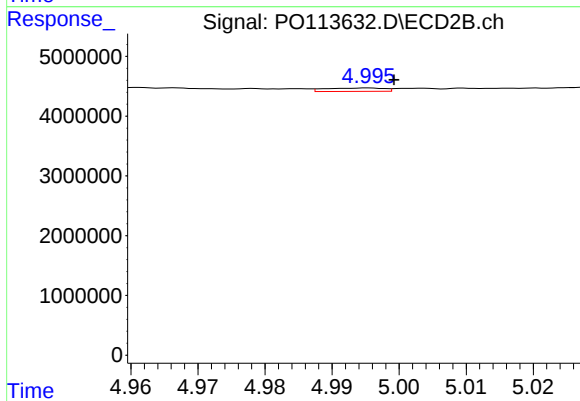

#14 AR-1232-4


R.T.: 4.995 min
Delta R.T.: -0.004 min
Response: 347202
Conc: 5.79 ng/ml

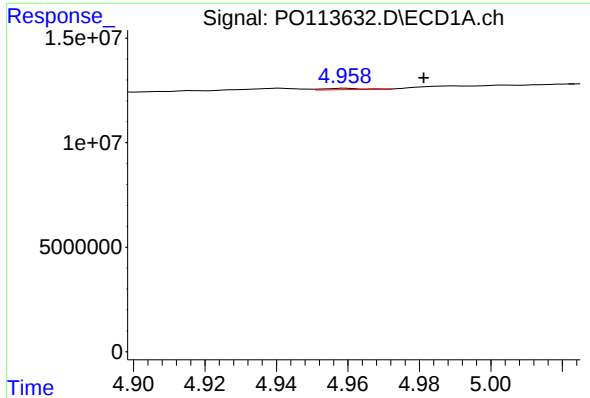

#15 AR-1232-5


R.T.: 4.959 min
Delta R.T.: -0.022 min
Response: 451503
Conc: 6.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

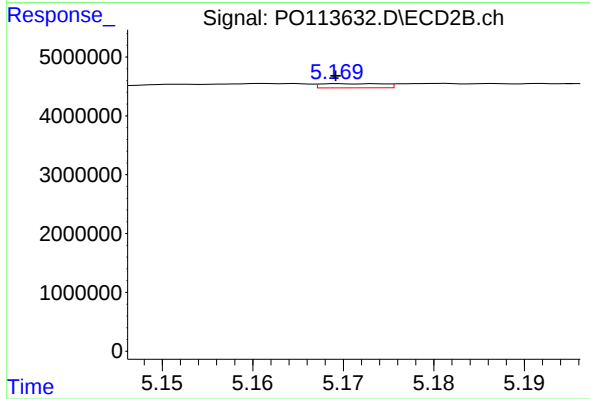


#15 AR-1232-5

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 347640
Conc: 5.14 ng/ml

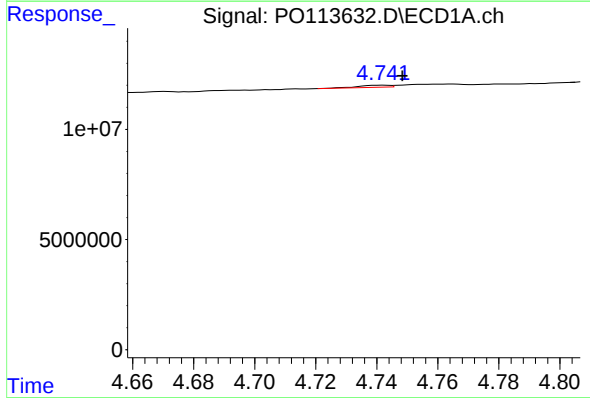


#16 AR-1242-1

R.T.: 4.742 min
Delta R.T.: -0.007 min
Response: 675496
Conc: 2.94 ng/ml

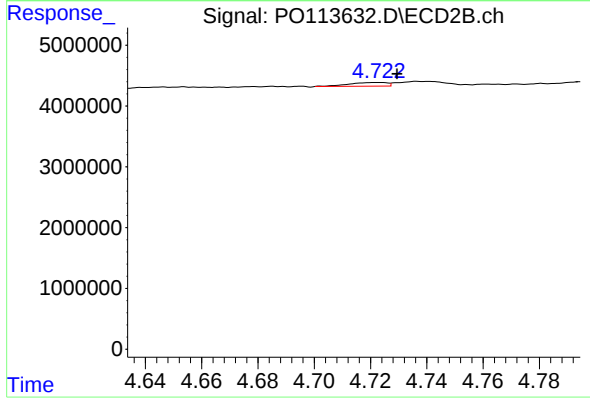

#16 AR-1242-1


R.T.: 4.723 min
Delta R.T.: -0.006 min
Response: 583985
Conc: 4.04 ng/ml

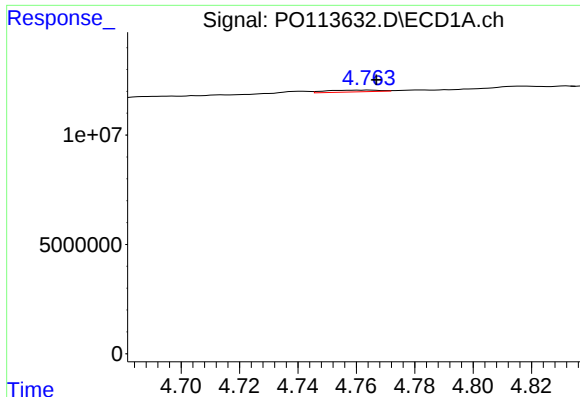

#17 AR-1242-2


R.T.: 4.765 min
Delta R.T.: -0.002 min
Response: 1073303
Conc: 3.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

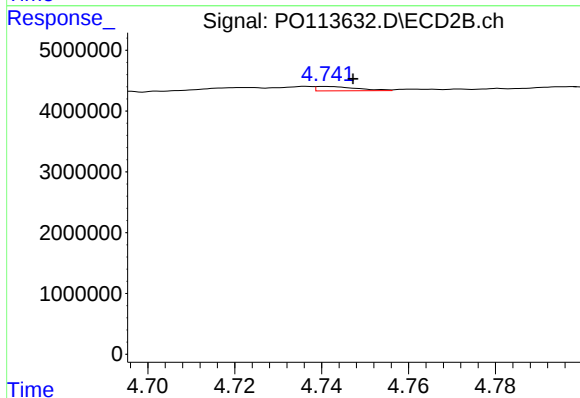


#17 AR-1242-2

R.T.: 4.741 min
Delta R.T.: -0.006 min
Response: 455384
Conc: 2.10 ng/ml

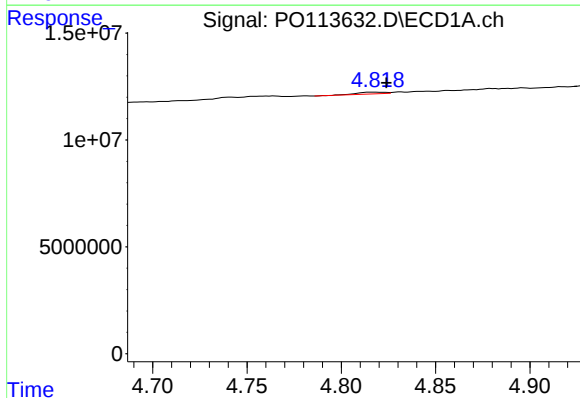


#18 AR-1242-3

R.T.: 4.817 min
Delta R.T.: -0.007 min
Response: 864835
Conc: 3.90 ng/ml

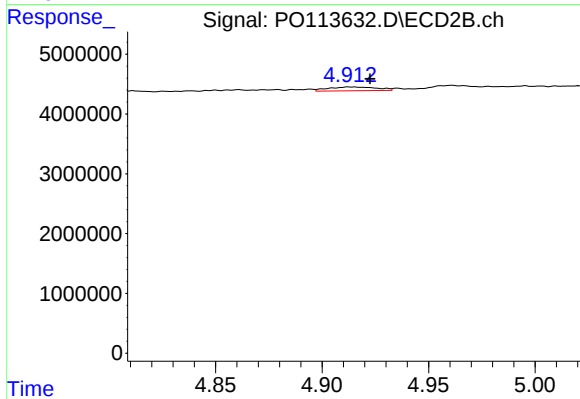

#18 AR-1242-3


R.T.: 4.912 min
Delta R.T.: -0.010 min
Response: 1013607
Conc: 8.67 ng/ml

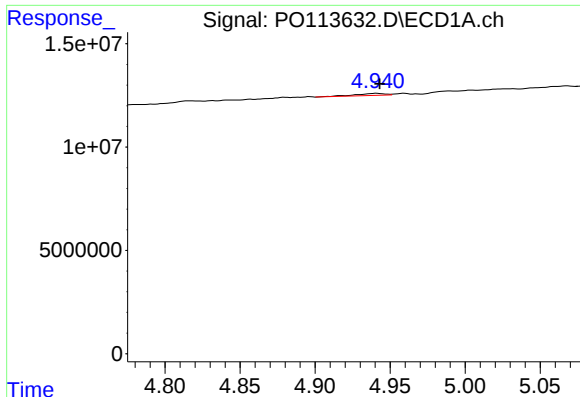

#19 AR-1242-4


R.T.: 4.941 min
Delta R.T.: -0.002 min
Response: 1428774
Conc: 8.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

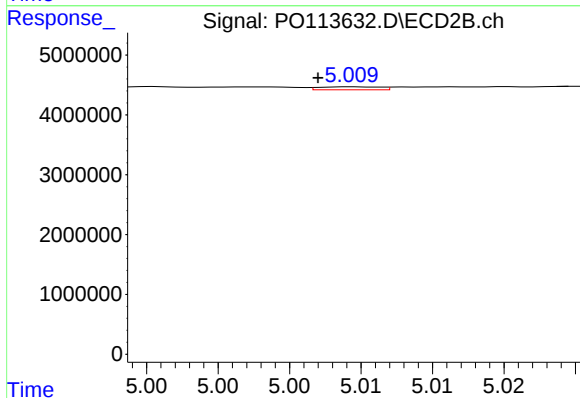


#19 AR-1242-4

R.T.: 5.010 min
Delta R.T.: 0.003 min
Response: 146227
Conc: 1.24 ng/ml

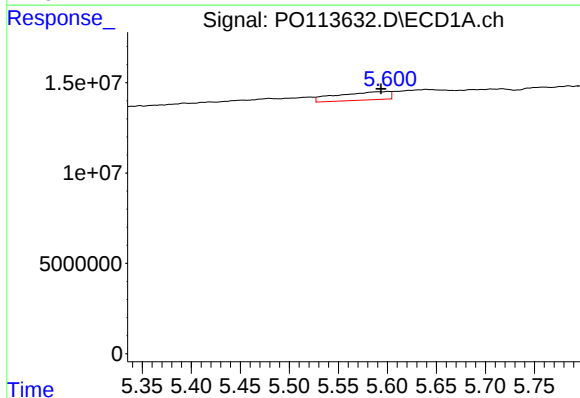


#20 AR-1242-5

R.T.: 5.601 min
Delta R.T.: 0.007 min
Response: 16706776
Conc: 83.47 ng/ml

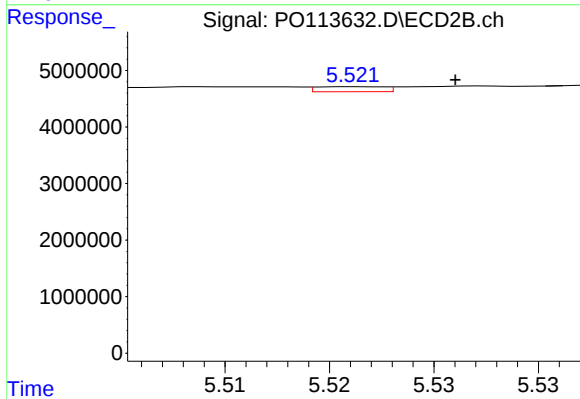

#20 AR-1242-5


R.T.: 5.522 min
Delta R.T.: -0.005 min
Response: 199516
Conc: 1.34 ng/ml

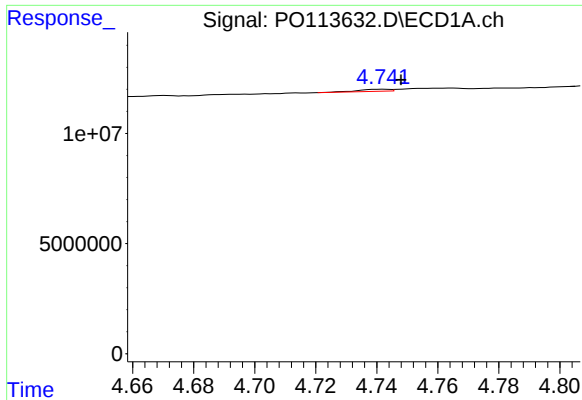

#21 AR-1248-1


R.T.: 4.742 min
Delta R.T.: -0.006 min
Response: 675496
Conc: 3.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

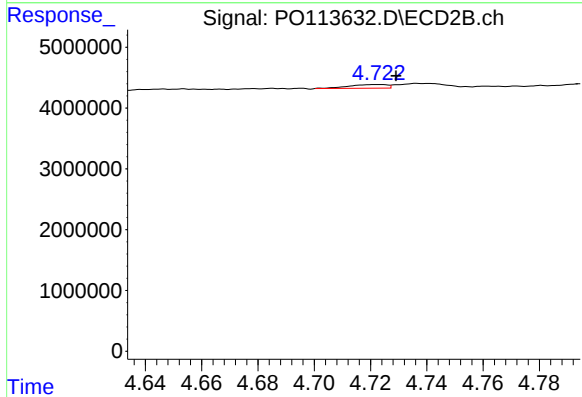


#21 AR-1248-1

R.T.: 4.723 min
Delta R.T.: -0.006 min
Response: 583985
Conc: 5.24 ng/ml

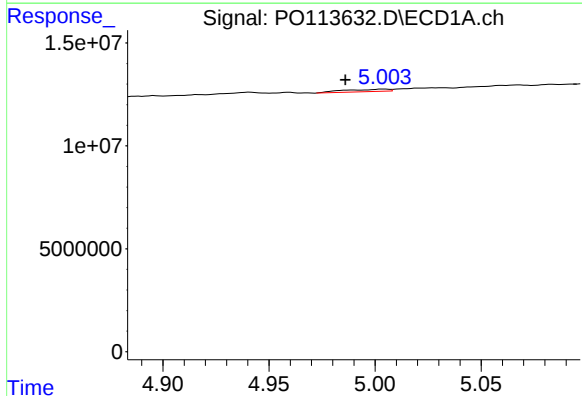


#22 AR-1248-2

R.T.: 5.004 min
Delta R.T.: 0.018 min
Response: 1708726
Conc: 7.06 ng/ml

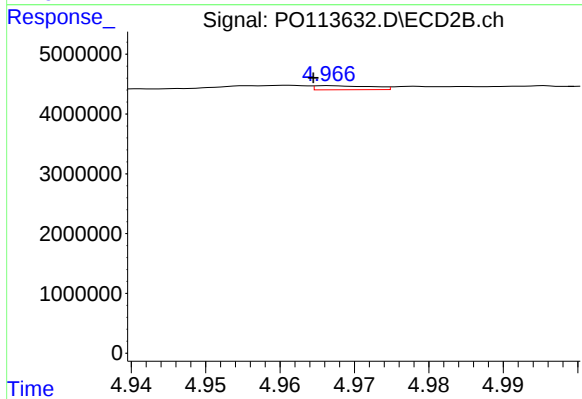

#22 AR-1248-2


R.T.: 4.967 min
Delta R.T.: 0.002 min
Response: 357397
Conc: 2.22 ng/ml

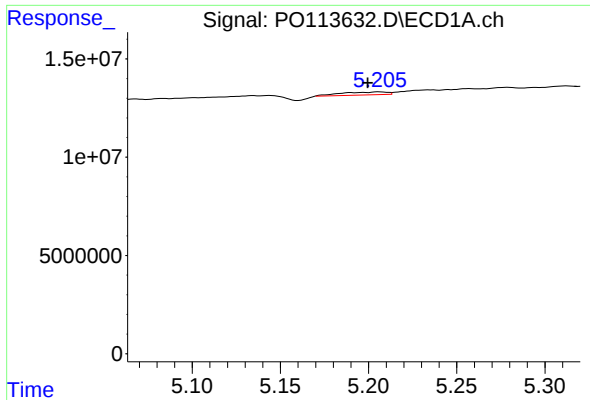

#23 AR-1248-3


R.T.: 5.206 min
Delta R.T.: 0.006 min
Response: 2684864
Conc: 8.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

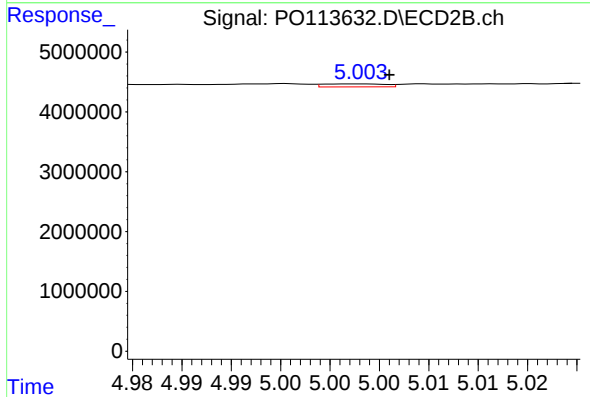


#23 AR-1248-3

R.T.: 5.003 min
Delta R.T.: -0.003 min
Response: 218352
Conc: 1.29 ng/ml

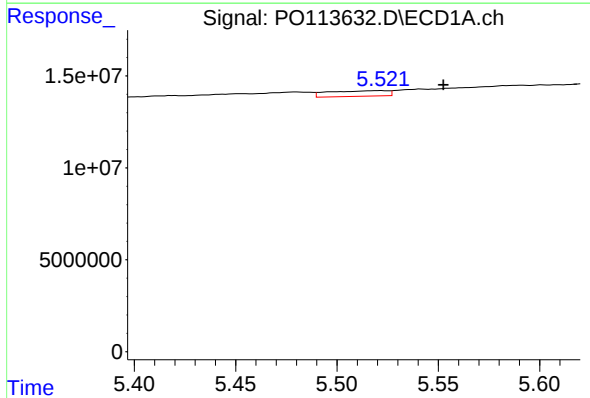


#24 AR-1248-4

R.T.: 5.522 min
Delta R.T.: -0.031 min
Response: 6230087
Conc: 12.47 ng/ml

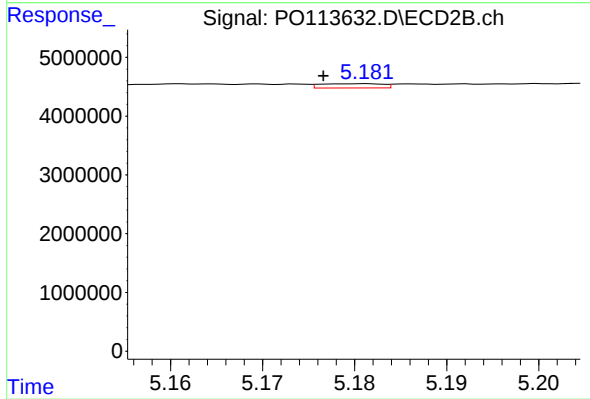

#24 AR-1248-4


R.T.: 5.181 min
Delta R.T.: 0.005 min
Response: 339479
Conc: 1.70 ng/ml

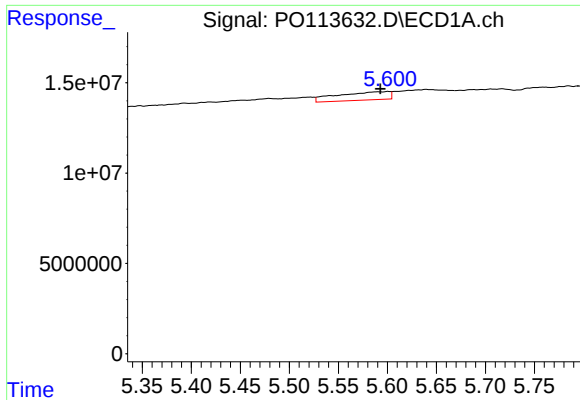

#25 AR-1248-5


R.T.: 5.601 min
Delta R.T.: 0.008 min
Response: 16706776
Conc: 48.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

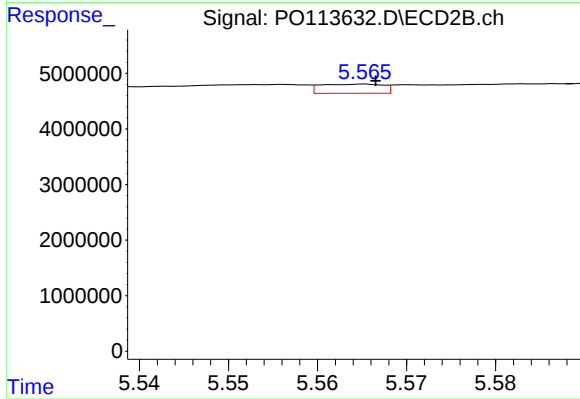


#25 AR-1248-5

R.T.: 5.565 min
Delta R.T.: -0.001 min
Response: 802549
Conc: 3.78 ng/ml

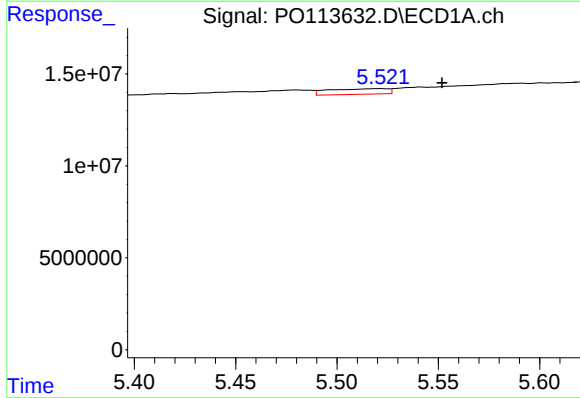


#26 AR-1254-1

R.T.: 5.522 min
Delta R.T.: -0.030 min
Response: 6230087
Conc: 11.54 ng/ml

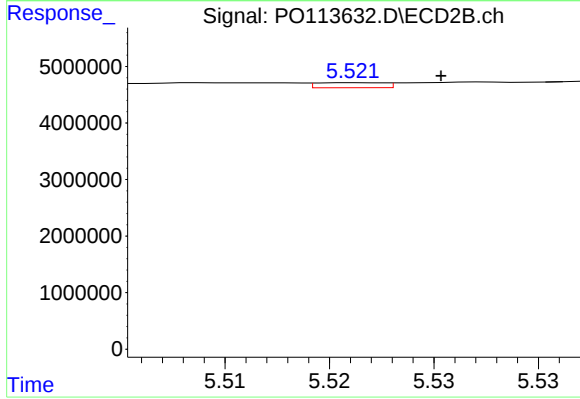

#26 AR-1254-1


R.T.: 5.522 min
Delta R.T.: -0.004 min
Response: 199516
Conc: 0.63 ng/ml

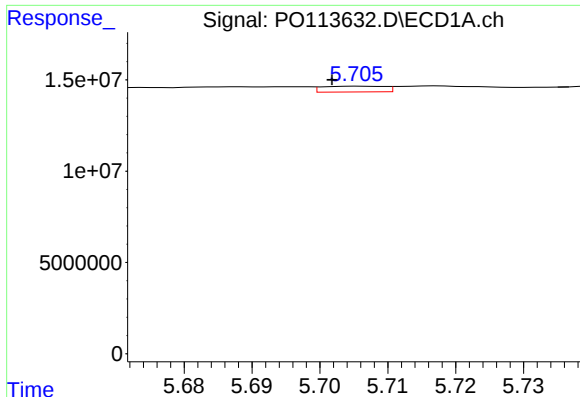

#27 AR-1254-2


R.T.: 5.706 min
Delta R.T.: 0.004 min
Response: 2010174
Conc: 4.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

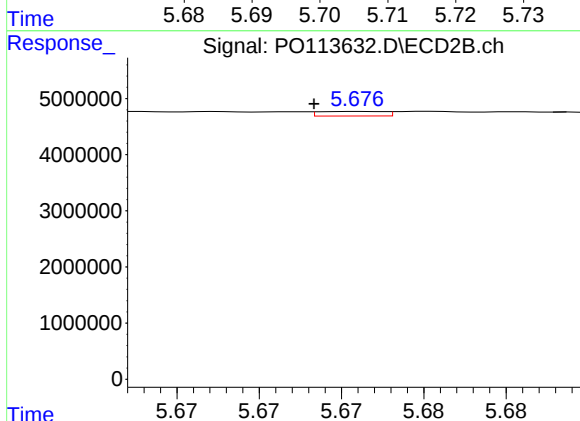


#27 AR-1254-2

R.T.: 5.676 min
Delta R.T.: 0.003 min
Response: 221974
Conc: 0.79 ng/ml

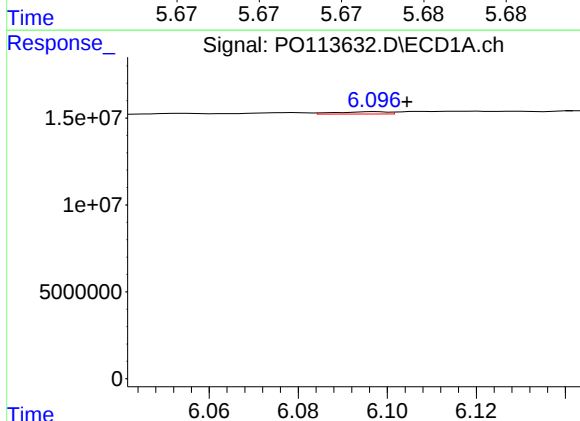


#28 AR-1254-3

R.T.: 6.097 min
Delta R.T.: -0.007 min
Response: 1060052
Conc: 1.43 ng/ml

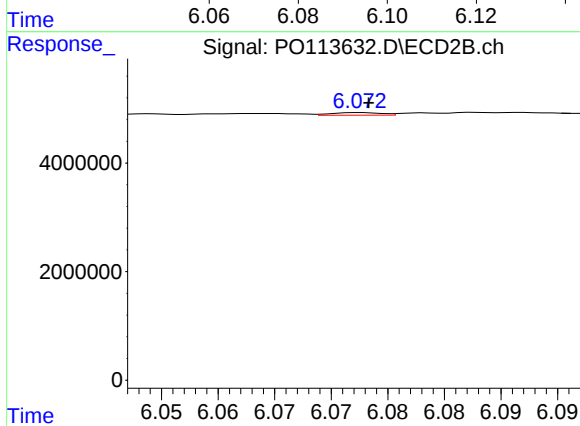

#28 AR-1254-3


R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 151308
Conc: 0.36 ng/ml

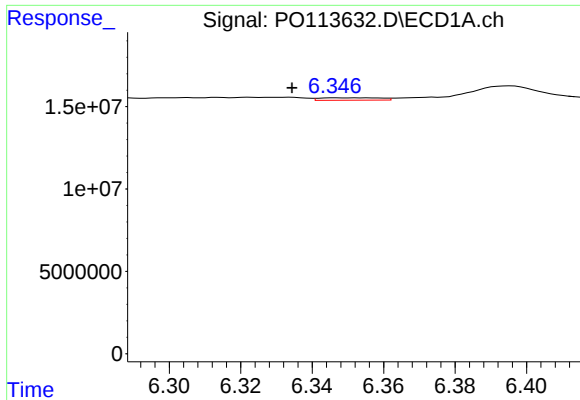

#29 AR-1254-4


R.T.: 6.346 min
Delta R.T.: 0.012 min
Response: 1733222
Conc: 3.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

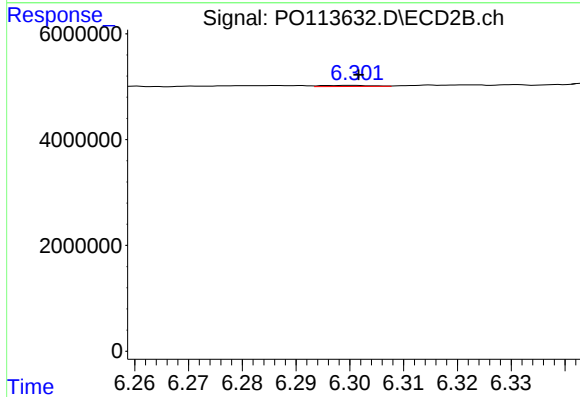


#29 AR-1254-4

R.T.: 6.301 min
Delta R.T.: 0.000 min
Response: 134262
Conc: 0.49 ng/ml

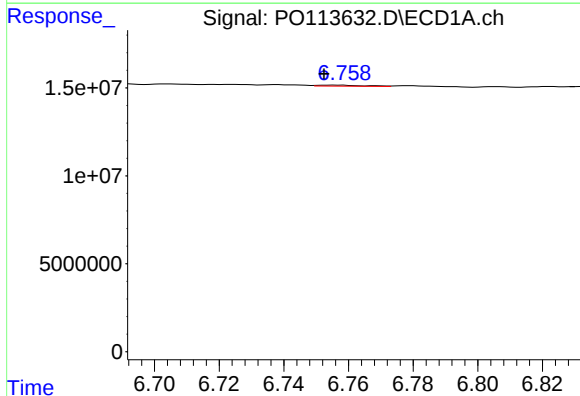


#30 AR-1254-5

R.T.: 6.755 min
Delta R.T.: 0.003 min
Response: 568942
Conc: 0.81 ng/ml

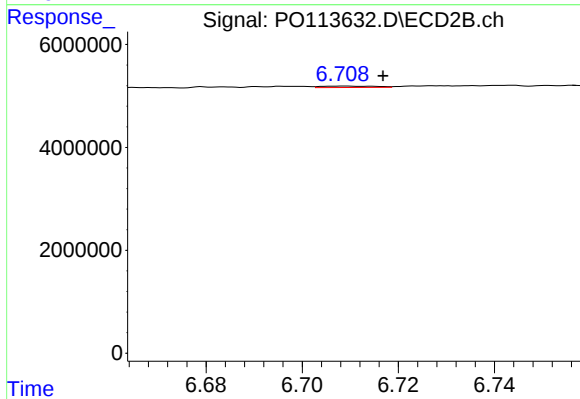

#30 AR-1254-5


R.T.: 6.709 min
Delta R.T.: -0.008 min
Response: 216644
Conc: 0.61 ng/ml

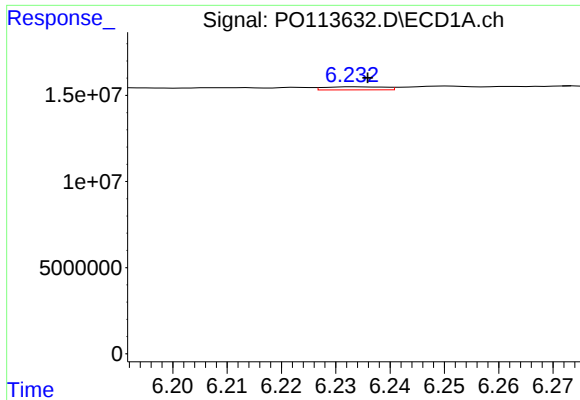

#31 AR-1260-1


R.T.: 6.234 min
Delta R.T.: -0.002 min
Response: 1356466
Conc: 3.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

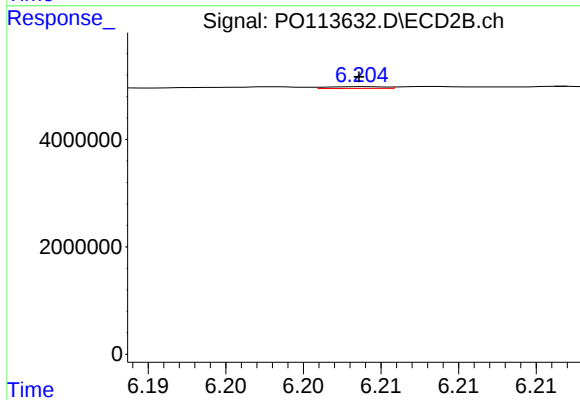


#31 AR-1260-1

R.T.: 6.204 min
Delta R.T.: 0.000 min
Response: 80456
Conc: 0.32 ng/ml

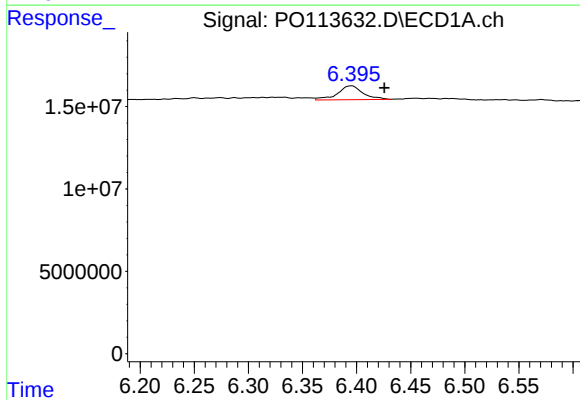


#32 AR-1260-2

R.T.: 6.395 min
Delta R.T.: -0.030 min
Response: 13804735
Conc: 20.10 ng/ml

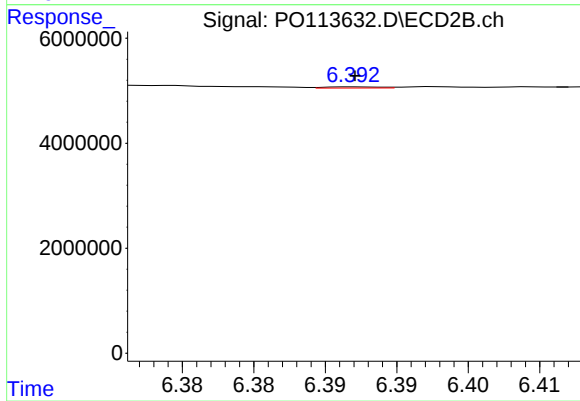

#32 AR-1260-2


R.T.: 6.392 min
Delta R.T.: 0.000 min
Response: 56650
Conc: 0.16 ng/ml

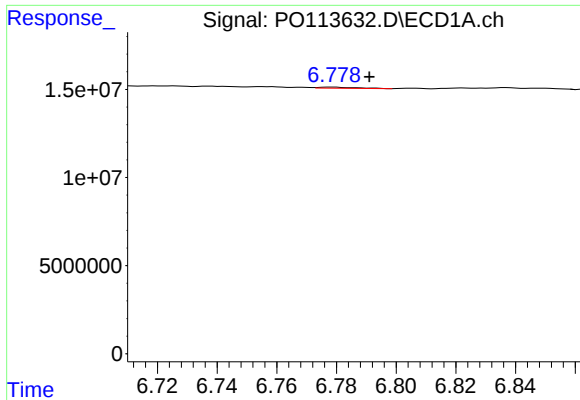

#33 AR-1260-3


R.T.: 6.779 min
Delta R.T.: -0.012 min
Response: 530800
Conc: 0.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

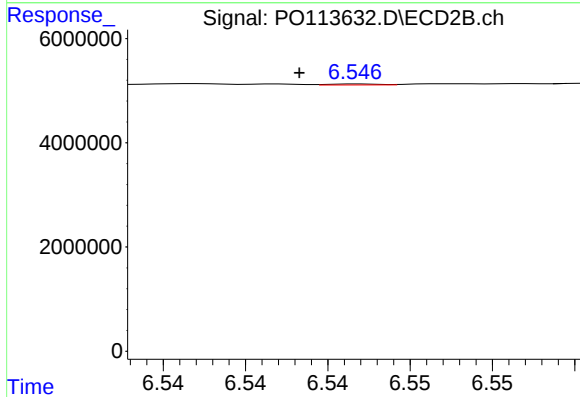


#33 AR-1260-3

R.T.: 6.547 min
Delta R.T.: 0.004 min
Response: 39971
Conc: 0.13 ng/ml

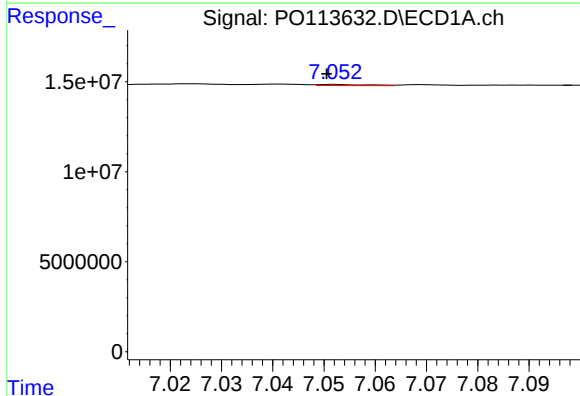


#34 AR-1260-4

R.T.: 7.052 min
Delta R.T.: 0.002 min
Response: 398242
Conc: 0.89 ng/ml

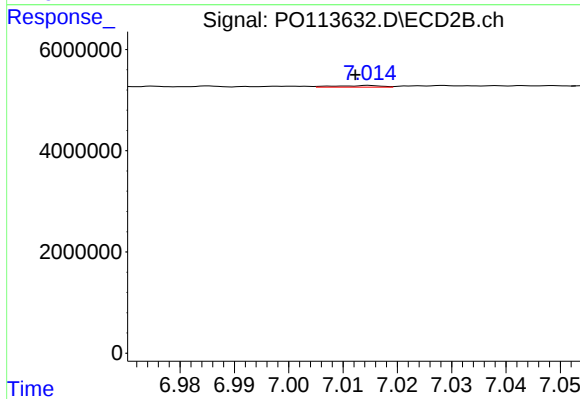

#34 AR-1260-4


R.T.: 7.015 min
Delta R.T.: 0.003 min
Response: 193021
Conc: 0.93 ng/ml

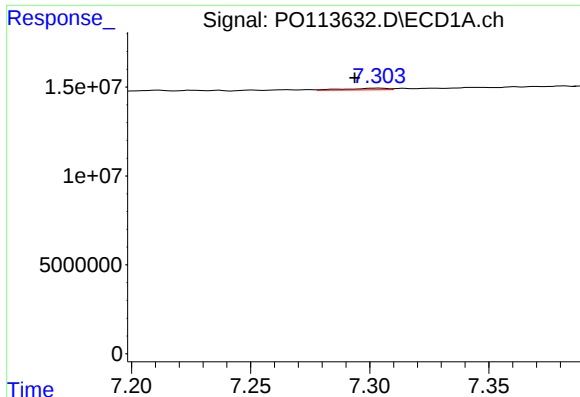

#35 AR-1260-5


R.T.: 7.303 min
Delta R.T.: 0.009 min
Response: 1187919
Conc: 0.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

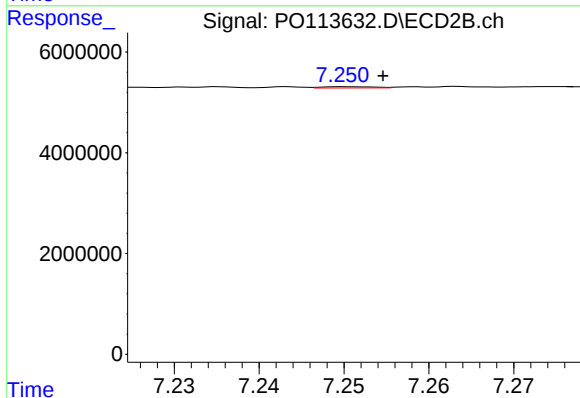


#35 AR-1260-5

R.T.: 7.250 min
Delta R.T.: -0.004 min
Response: 109278
Conc: 0.23 ng/ml

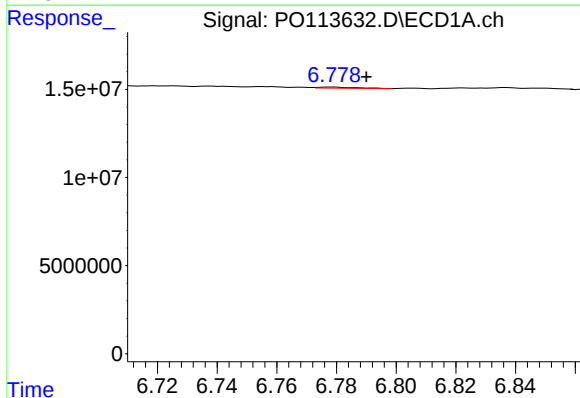


#36 AR-1262-1

R.T.: 6.779 min
Delta R.T.: -0.011 min
Response: 530800
Conc: 0.58 ng/ml

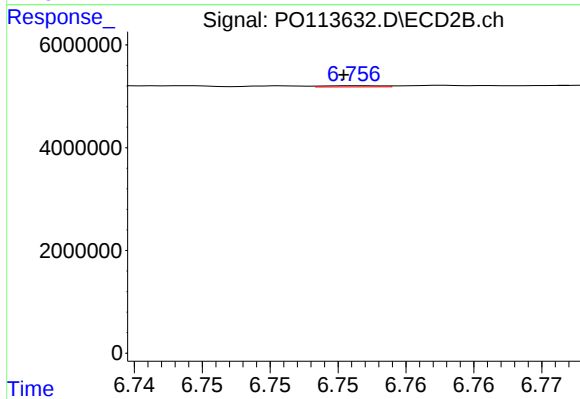

#36 AR-1262-1


R.T.: 6.756 min
Delta R.T.: 0.001 min
Response: 71604
Conc: 0.17 ng/ml

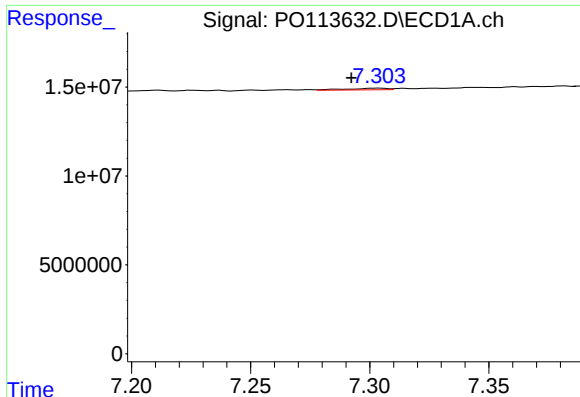

#37 AR-1262-2


R.T.: 7.303 min
Delta R.T.: 0.011 min
Response: 1187919
Conc: 0.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

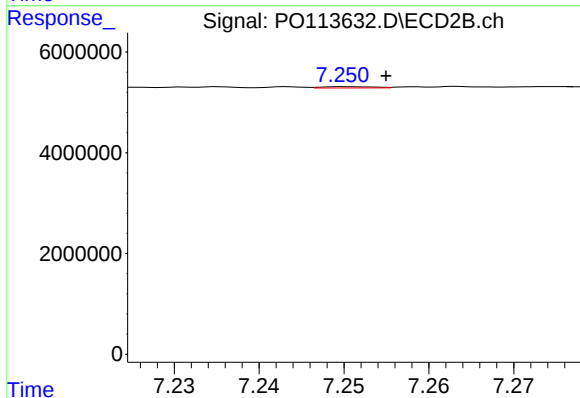


#37 AR-1262-2

R.T.: 7.250 min
Delta R.T.: -0.005 min
Response: 109278
Conc: 0.21 ng/ml

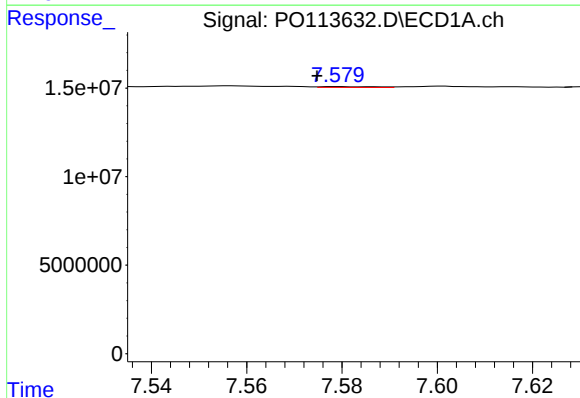


#38 AR-1262-3

R.T.: 7.579 min
Delta R.T.: 0.004 min
Response: 359415
Conc: 0.65 ng/ml

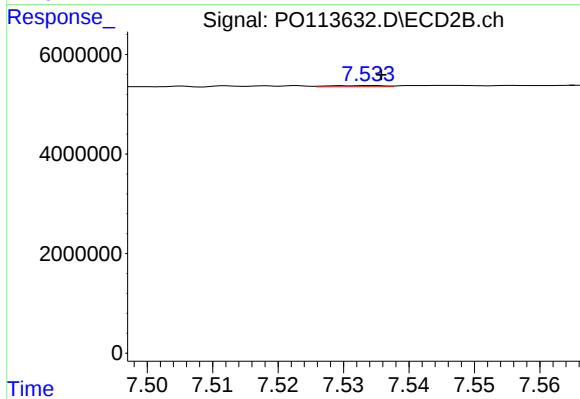

#38 AR-1262-3


R.T.: 7.534 min
Delta R.T.: -0.002 min
Response: 134263
Conc: 0.75 ng/ml

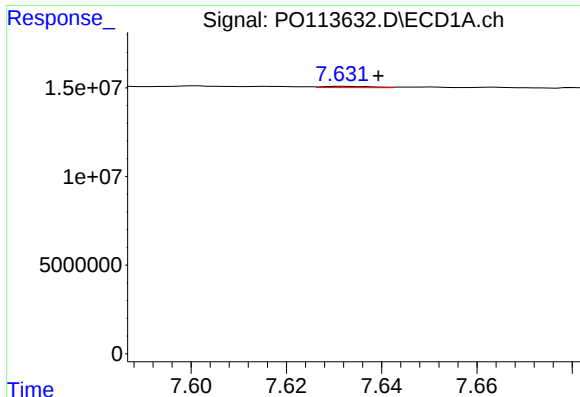

#39 AR-1262-4


R.T.: 7.632 min
Delta R.T.: -0.007 min
Response: 522942
Conc: 0.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

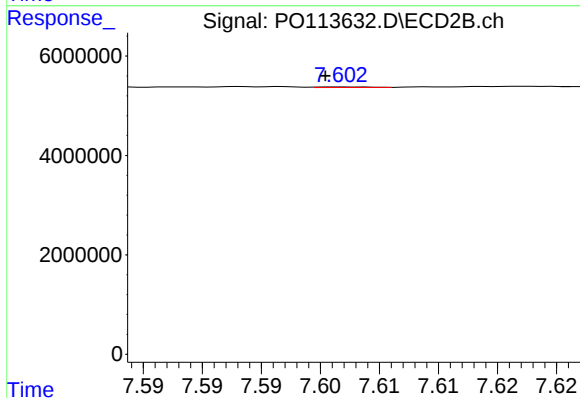


#39 AR-1262-4

R.T.: 7.602 min
Delta R.T.: 0.002 min
Response: 31338
Conc: 0.11 ng/ml

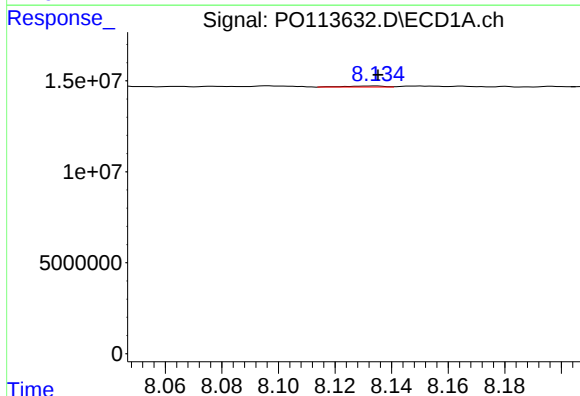


#40 AR-1262-5

R.T.: 8.135 min
Delta R.T.: 0.000 min
Response: 547566
Conc: 1.31 ng/ml

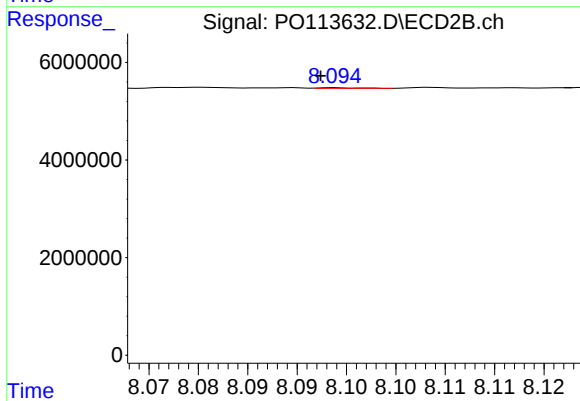

#40 AR-1262-5


R.T.: 8.094 min
Delta R.T.: 0.002 min
Response: 32578
Conc: 0.30 ng/ml

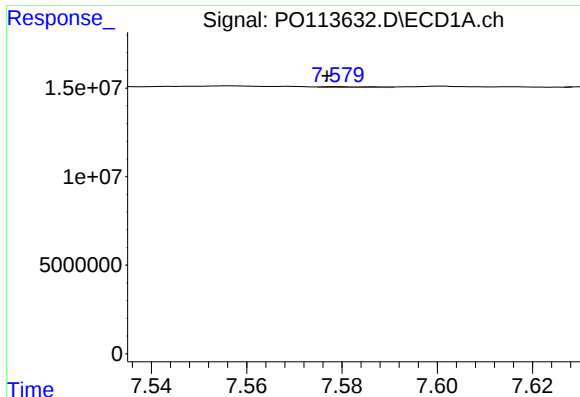

#41 AR-1268-1


R.T.: 7.579 min
Delta R.T.: 0.002 min
Response: 359415
Conc: 0.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

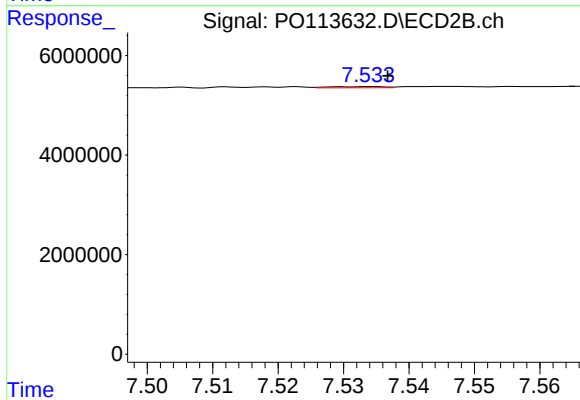


#41 AR-1268-1

R.T.: 7.534 min
Delta R.T.: -0.003 min
Response: 134263
Conc: 0.26 ng/ml

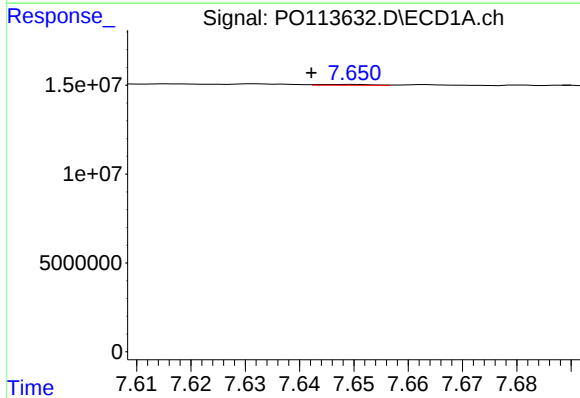


#42 AR-1268-2

R.T.: 7.650 min
Delta R.T.: 0.008 min
Response: 324625
Conc: 0.22 ng/ml

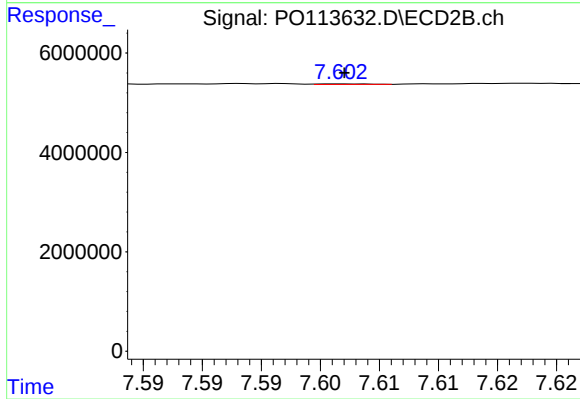

#42 AR-1268-2


R.T.: 7.602 min
Delta R.T.: 0.000 min
Response: 31338
Conc: 0.08 ng/ml

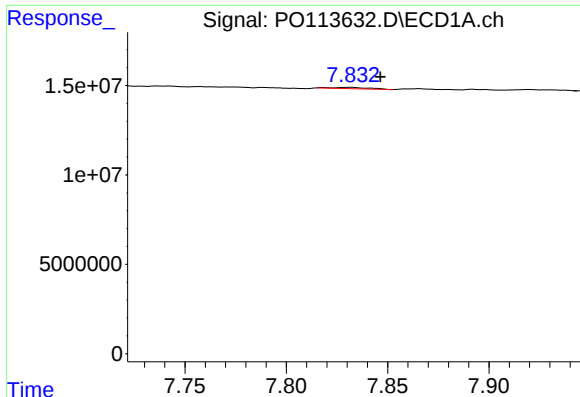

#43 AR-1268-3


R.T.: 7.832 min
Delta R.T.: -0.015 min
Response: 957017
Conc: 0.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

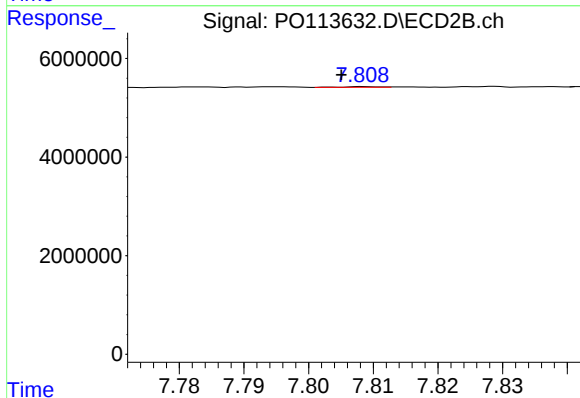


#43 AR-1268-3

R.T.: 7.808 min
Delta R.T.: 0.003 min
Response: 53551
Conc: 0.16 ng/ml

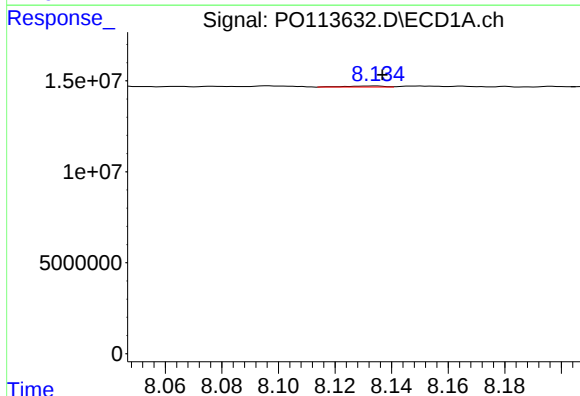


#44 AR-1268-4

R.T.: 8.135 min
Delta R.T.: -0.002 min
Response: 547566
Conc: 1.19 ng/ml

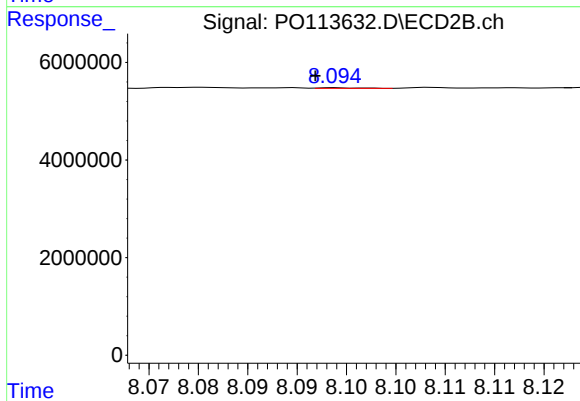

#44 AR-1268-4


R.T.: 8.094 min
Delta R.T.: 0.002 min
Response: 32578
Conc: 0.27 ng/ml

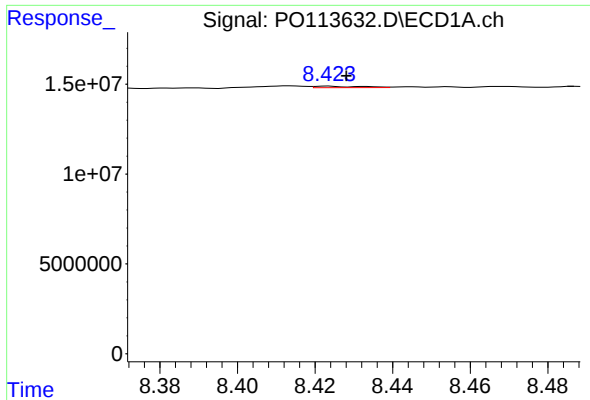

#45 AR-1268-5

R.T.: 8.423 min
Delta R.T.: -0.005 min
Response: 700201
Conc: 0.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

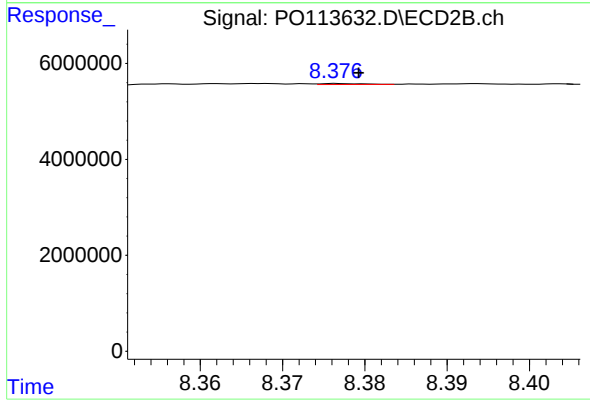

#45 AR-1268-5

R.T.: 8.377 min
Delta R.T.: -0.003 min
Response: 75851
Conc: 0.10 ng/ml