

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
 Data File : P0113633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 02:44
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1232 WATER LOD 40PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:30:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.658	3.649	184.9E6	108.6E6	22.592	21.465
2)	SA Decachlor...	8.667	8.613	153.3E6	44048737	22.124	23.247
Target Compounds							
3)	L1 AR-1016-1	4.742	4.721	4720105	3253444	17.679	19.074
4)	L1 AR-1016-2	4.760	4.739	8101258	5154985	20.181	20.007
5)	L1 AR-1016-3	4.818	4.914	5476415	3611573	21.474	25.868
6)	L1 AR-1016-4	4.936	4.957	4174520	3052709	19.143	26.159 #
7)	L1 AR-1016-5	5.193	5.168	6343563	4882805	28.623	34.258
8)	L2 AR-1221-1	3.870	3.856	2205347	1718226	23.568	27.221
9)	L2 AR-1221-2	3.957	3.944	3440369	3167318	50.930	67.862 #
10)	L2 AR-1221-3	4.030	4.017	6615187	4962547	29.885	33.423
11)	L3 AR-1232-1	4.030	4.017	6615187	4962547	36.848	41.036
12)	L3 AR-1232-2	4.520	4.739	3979030	5154985	36.871	42.237
13)	L3 AR-1232-3	4.760	4.914	8101258	3611573	41.041	54.592 #
14)	L3 AR-1232-4	4.936	4.998	4174520	3689797	42.470	61.570 #
15)	L3 AR-1232-5	4.985	5.168	2177582	4882805	33.103	72.214 #
16)	L4 AR-1242-1	4.742	4.721	4720105	3253444	20.528	22.514
17)	L4 AR-1242-2	4.760	4.739	8101258	5154985	23.576	23.765
18)	L4 AR-1242-3	4.818	4.914	5476415	3611573	24.681	30.878 #
19)	L4 AR-1242-4	4.936	4.998	4174520	3689797	24.066	31.366 #
20)	L4 AR-1242-5	5.586	5.518	15808996	4719288	78.981	31.645 #
21)	L5 AR-1248-1	4.742	4.721	4720105	3253444	27.055	29.176
22)	L5 AR-1248-2	4.985	4.957	2177582	3052709	9.003	18.996 #
23)	L5 AR-1248-3	5.193	4.998	6343563	3689797	19.894	21.748
24)	L5 AR-1248-4	5.545	5.168	12364618	4882805	24.749	24.510
25)	L5 AR-1248-5	5.586	5.557	15808996	7234530	46.294	34.077 #
26)	L6 AR-1254-1	5.545	5.518	12364618	4719288	22.898	14.965 #
27)	L6 AR-1254-2	5.693	5.663	6976238	2832022	14.138	10.102 #
28)	L6 AR-1254-3	6.111	6.063	396651	1825089	0.537	4.378 #
29)	L6 AR-1254-4	6.327	6.291	3702545	641807	6.647	2.335 #
30)	L6 AR-1254-5	6.763	6.713	204022	651439	0.291	1.822 #
31)	L7 AR-1260-1	6.238	6.208	549032	935188	1.231	3.666 #
32)	L7 AR-1260-2	6.441	6.416	298611	95332	0.435	0.276 #
33)	L7 AR-1260-3	6.808	6.552	207211	158909	0.336	0.534 #
34)	L7 AR-1260-4	7.049	7.016	1190296	700580	2.658	3.380 #
35)	L7 AR-1260-5	7.296	7.244	146637	201988	0.121	0.431 #
36)	L8 AR-1262-1	6.808	6.789	207211	718582	0.226	1.733 #
37)	L8 AR-1262-2	7.296	7.266	146637	230058	0.097	0.444 #
38)	L8 AR-1262-3	7.577	7.536	1392403	450700	2.513	2.510
39)	L8 AR-1262-4	7.632	7.599	1006119	100716	1.029	0.347 #
40)	L8 AR-1262-5	8.140	8.101	633682	107336	1.520	0.991 #
41)	L9 AR-1268-1	7.577	7.536	1392403	450700	0.809	0.885

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
Data File : P0113633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 02:44
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1232 WATER LOD 40PPB
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:30:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.649	7.599	697595	100716	0.482	0.242 #
43)	L9 AR-1268-3	7.860	7.795	368050	139948	0.305	0.429 #
44)	L9 AR-1268-4	8.140	8.101	633682	107336	1.376	0.891 #
45)	L9 AR-1268-5	8.440	8.366	110205	93064	0.035	0.119 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091025\
Data File : PO113633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 02:44
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1232 WATER LOD 40PPB
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:30:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

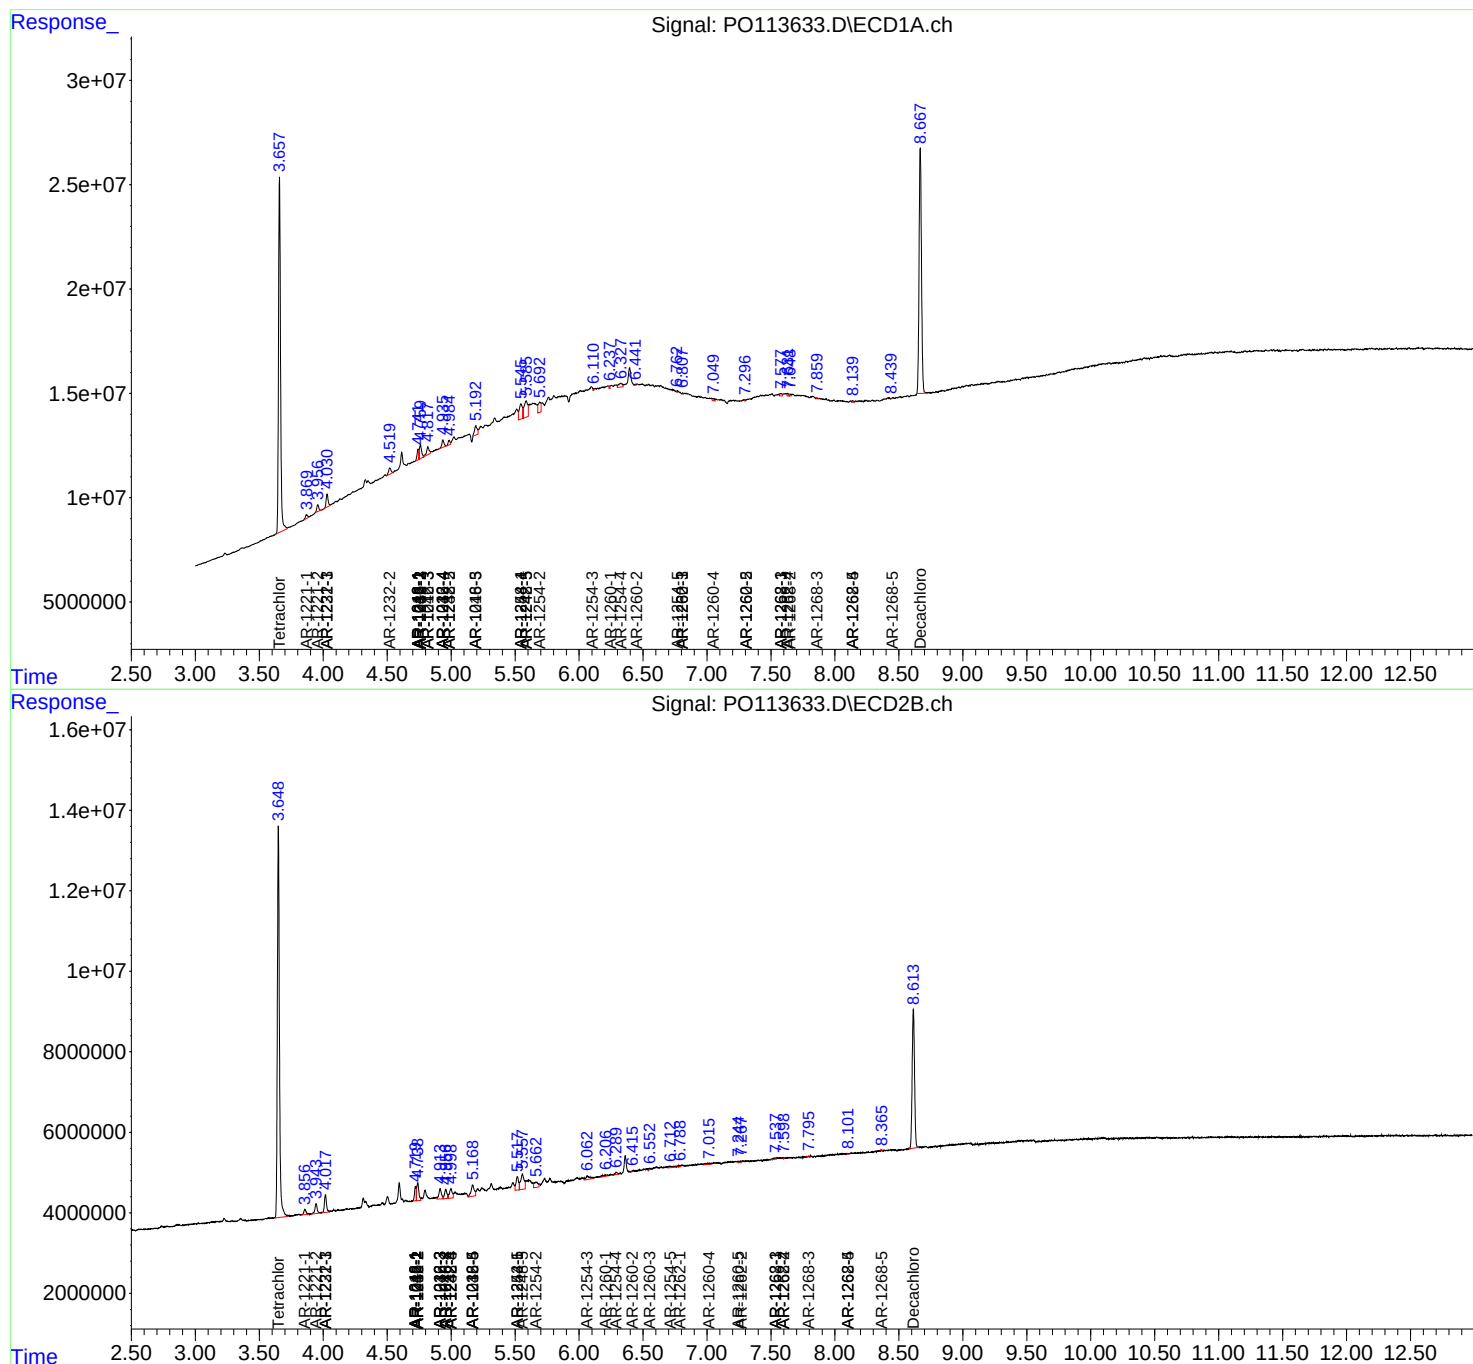


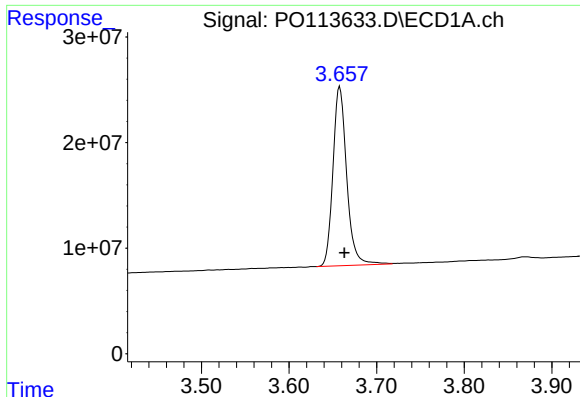

#1 Tetrachloro-m-xylene


R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 184948507
Conc: 22.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

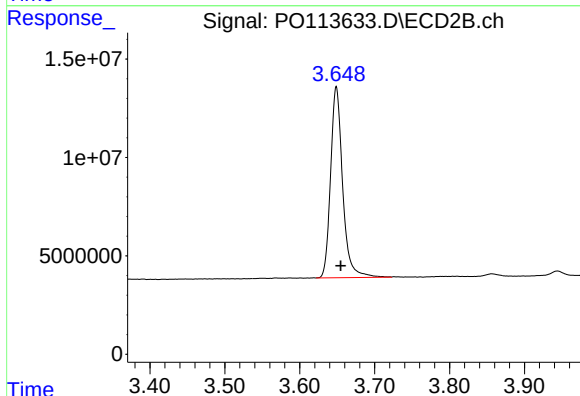


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.006 min
Response: 108629014
Conc: 21.47 ng/ml

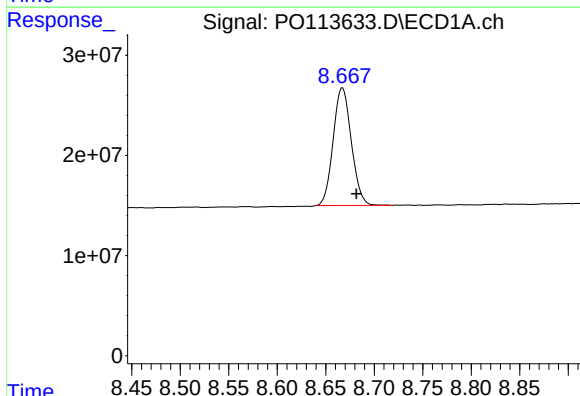


#2 Decachlorobiphenyl

R.T.: 8.667 min
Delta R.T.: -0.014 min
Response: 153348294
Conc: 22.12 ng/ml

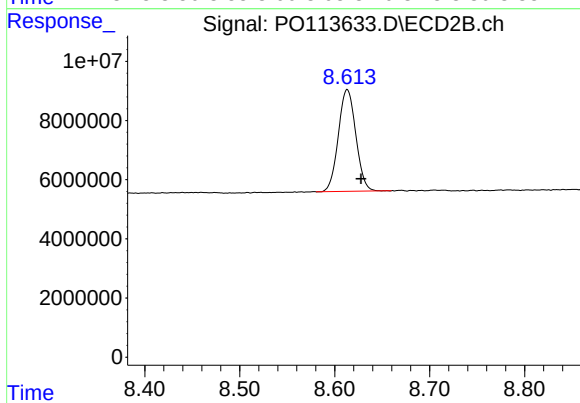

#2 Decachlorobiphenyl


R.T.: 8.613 min
Delta R.T.: -0.014 min
Response: 44048737
Conc: 23.25 ng/ml

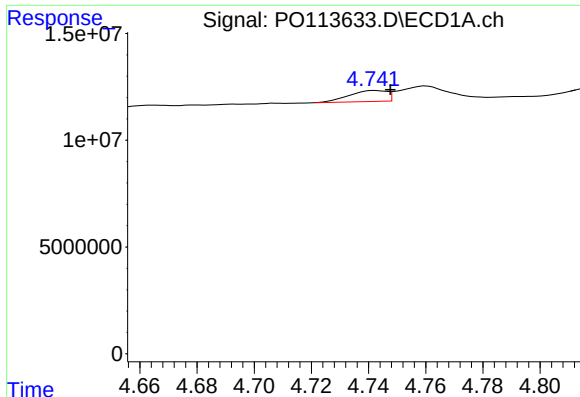

#3 AR-1016-1


R.T.: 4.742 min
Delta R.T.: -0.005 min
Response: 4720105
Conc: 17.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

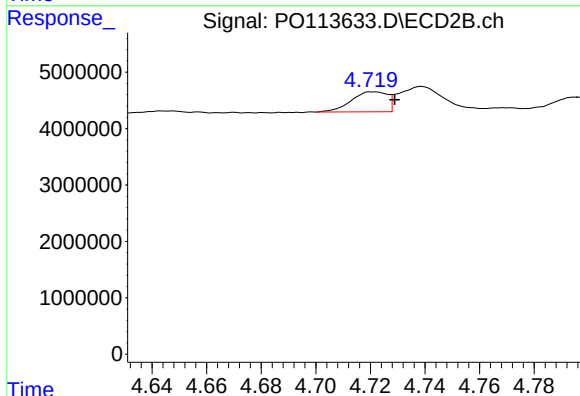


#3 AR-1016-1

R.T.: 4.721 min
Delta R.T.: -0.008 min
Response: 3253444
Conc: 19.07 ng/ml

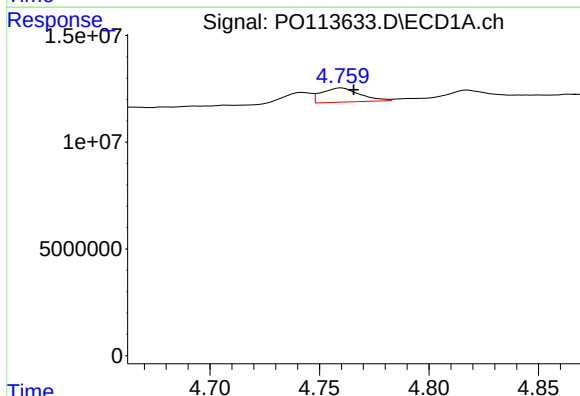


#4 AR-1016-2

R.T.: 4.760 min
Delta R.T.: -0.006 min
Response: 8101258
Conc: 20.18 ng/ml

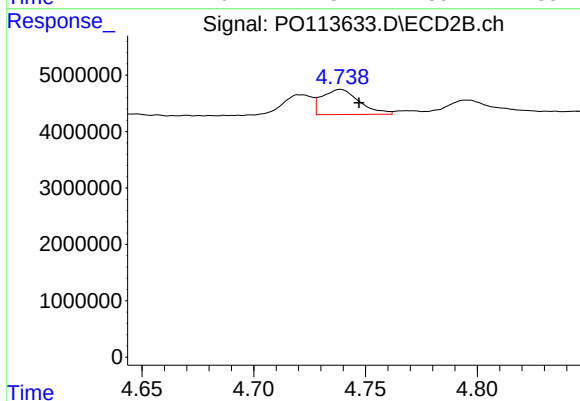

#4 AR-1016-2


R.T.: 4.739 min
Delta R.T.: -0.008 min
Response: 5154985
Conc: 20.01 ng/ml

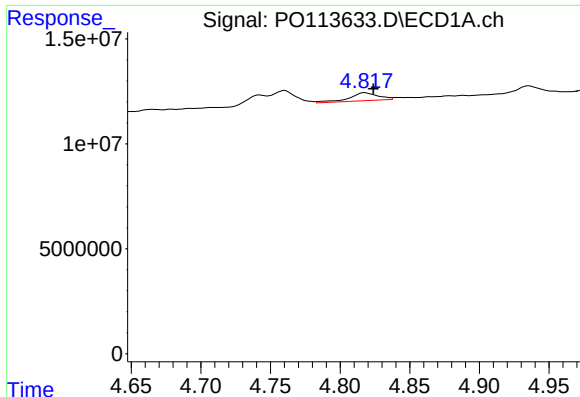

#5 AR-1016-3


R.T.: 4.818 min
Delta R.T.: -0.006 min
Response: 5476415
Conc: 21.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

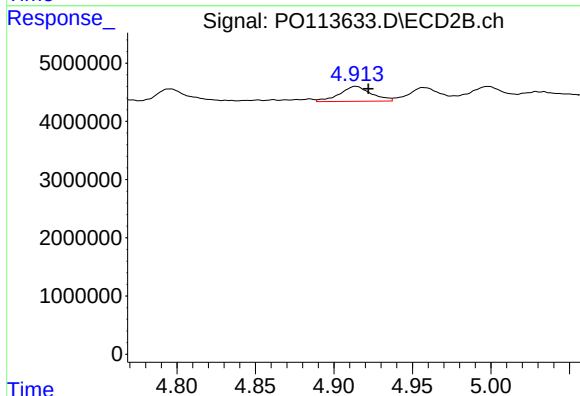


#5 AR-1016-3

R.T.: 4.914 min
Delta R.T.: -0.008 min
Response: 3611573
Conc: 25.87 ng/ml

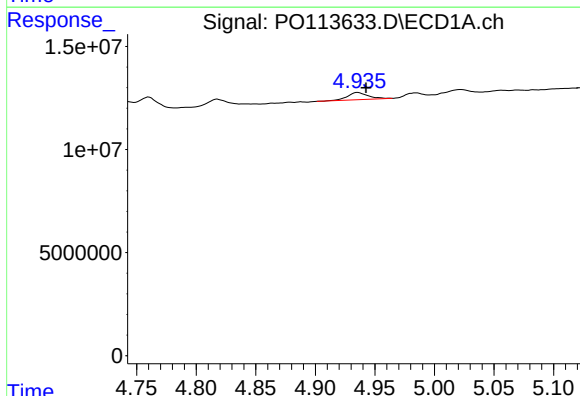


#6 AR-1016-4

R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 4174520
Conc: 19.14 ng/ml

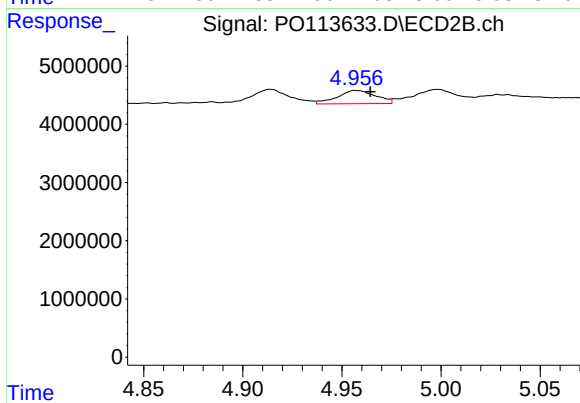

#6 AR-1016-4


R.T.: 4.957 min
Delta R.T.: -0.007 min
Response: 3052709
Conc: 26.16 ng/ml

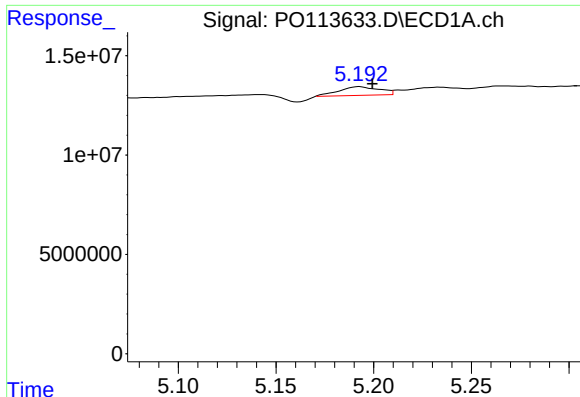

#7 AR-1016-5


R.T.: 5.193 min
Delta R.T.: -0.007 min
Response: 6343563
Conc: 28.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

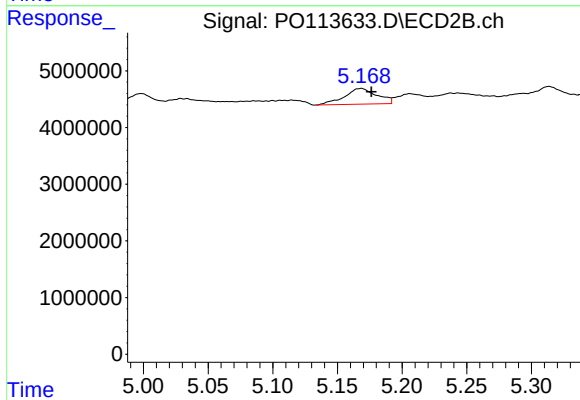


#7 AR-1016-5

R.T.: 5.168 min
Delta R.T.: -0.008 min
Response: 4882805
Conc: 34.26 ng/ml

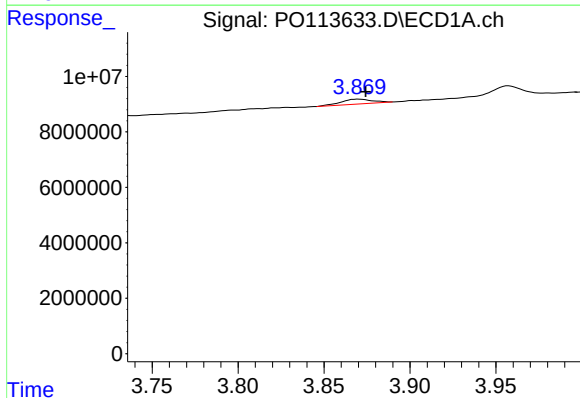


#8 AR-1221-1

R.T.: 3.870 min
Delta R.T.: -0.004 min
Response: 2205347
Conc: 23.57 ng/ml

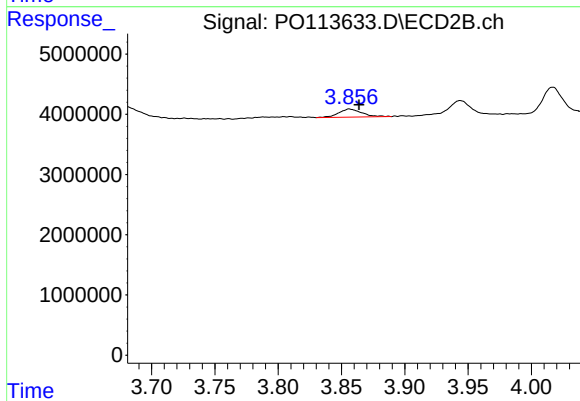

#8 AR-1221-1


R.T.: 3.856 min
Delta R.T.: -0.008 min
Response: 1718226
Conc: 27.22 ng/ml

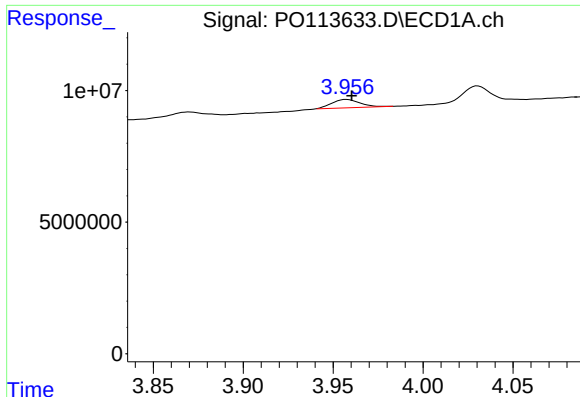

#9 AR-1221-2


R.T.: 3.957 min
Delta R.T.: -0.003 min
Response: 3440369
Conc: 50.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

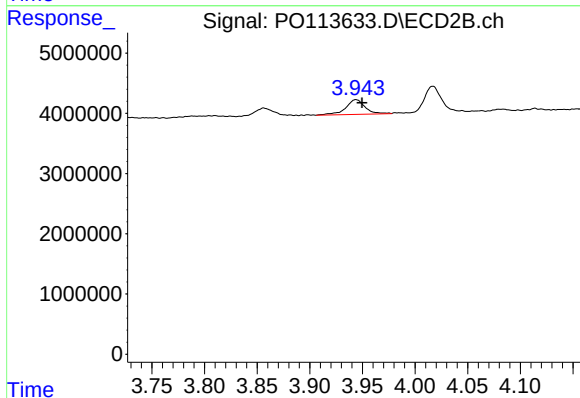


#9 AR-1221-2

R.T.: 3.944 min
Delta R.T.: -0.006 min
Response: 3167318
Conc: 67.86 ng/ml

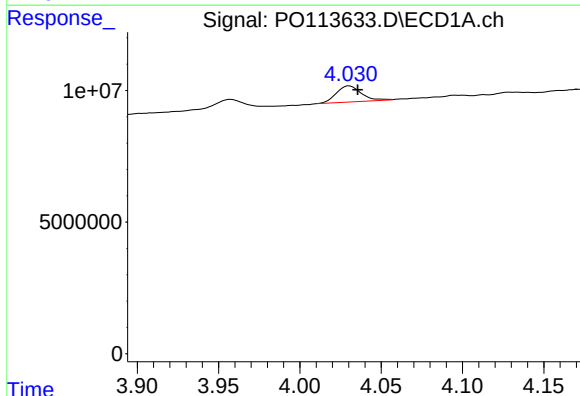


#10 AR-1221-3

R.T.: 4.030 min
Delta R.T.: -0.005 min
Response: 6615187
Conc: 29.89 ng/ml

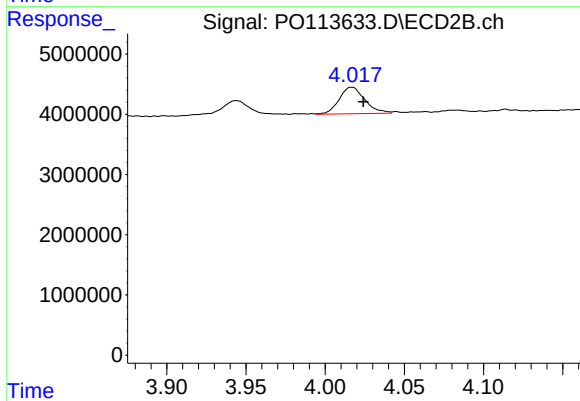

#10 AR-1221-3


R.T.: 4.017 min
Delta R.T.: -0.007 min
Response: 4962547
Conc: 33.42 ng/ml

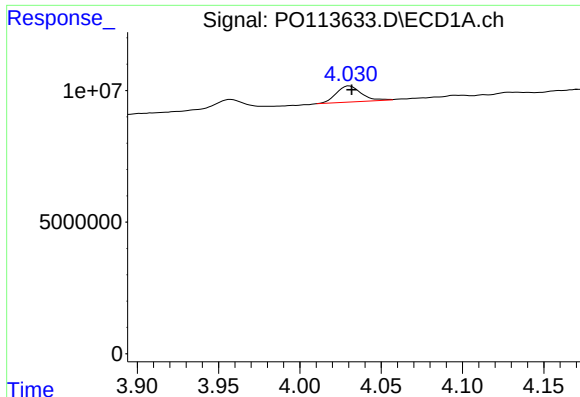

#11 AR-1232-1


R.T.: 4.030 min
Delta R.T.: -0.001 min
Response: 6615187
Conc: 36.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

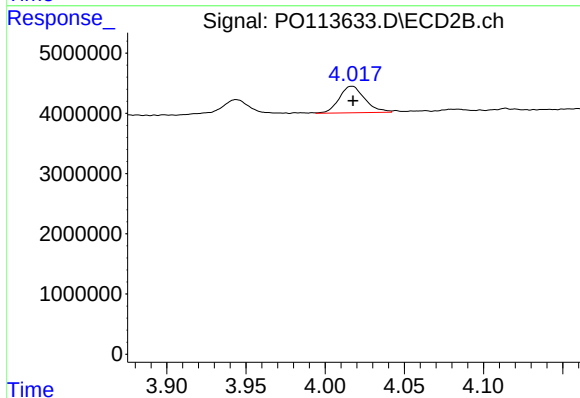


#11 AR-1232-1

R.T.: 4.017 min
Delta R.T.: 0.000 min
Response: 4962547
Conc: 41.04 ng/ml

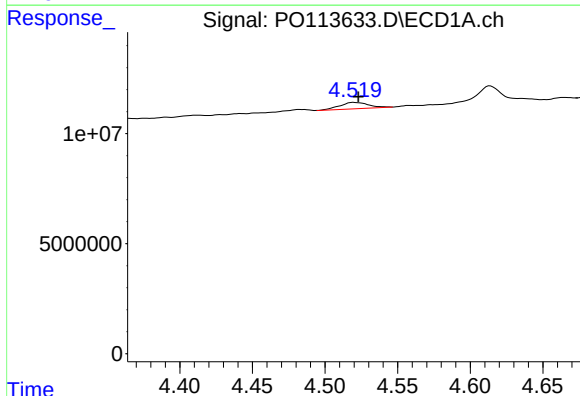


#12 AR-1232-2

R.T.: 4.520 min
Delta R.T.: -0.003 min
Response: 3979030
Conc: 36.87 ng/ml

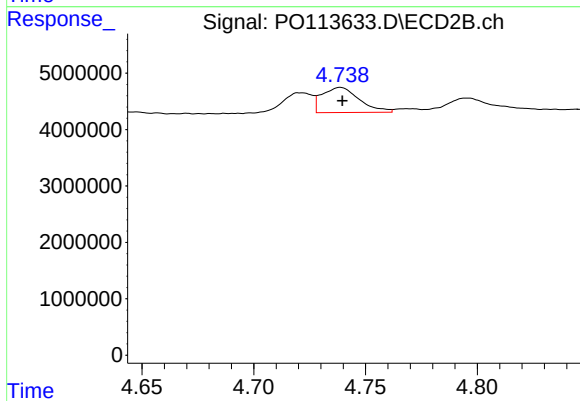

#12 AR-1232-2


R.T.: 4.739 min
Delta R.T.: 0.000 min
Response: 5154985
Conc: 42.24 ng/ml

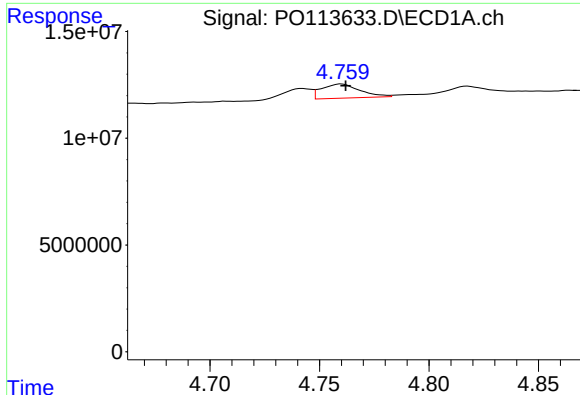

#13 AR-1232-3


R.T.: 4.760 min
Delta R.T.: -0.002 min
Response: 8101258
Conc: 41.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

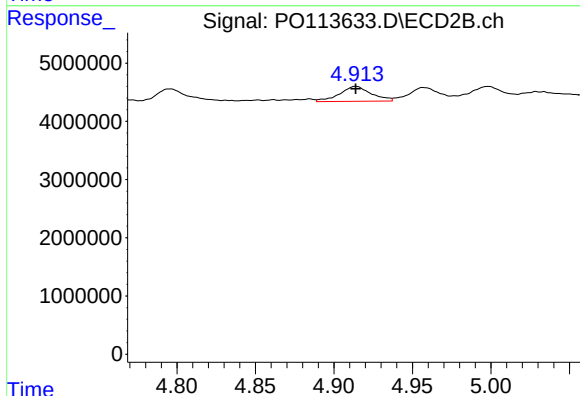


#13 AR-1232-3

R.T.: 4.914 min
Delta R.T.: 0.000 min
Response: 3611573
Conc: 54.59 ng/ml

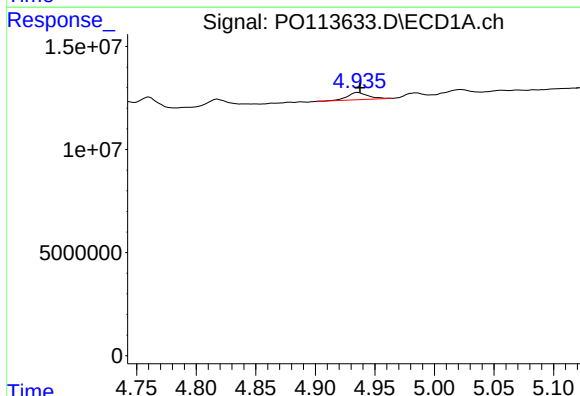


#14 AR-1232-4

R.T.: 4.936 min
Delta R.T.: -0.002 min
Response: 4174520
Conc: 42.47 ng/ml

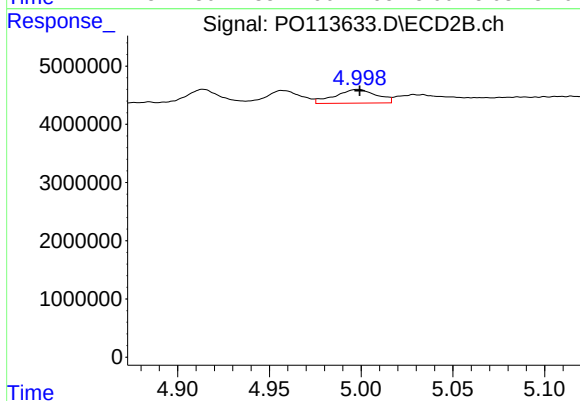

#14 AR-1232-4


R.T.: 4.998 min
Delta R.T.: 0.000 min
Response: 3689797
Conc: 61.57 ng/ml

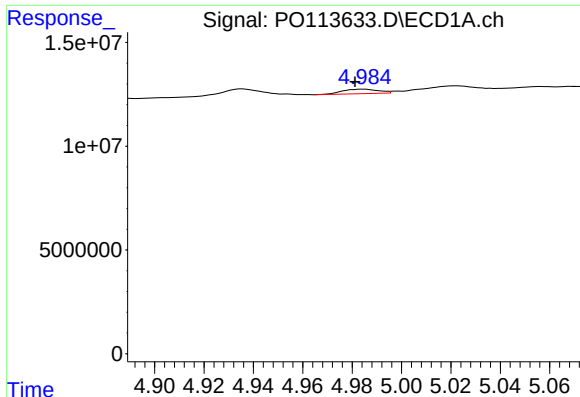

#15 AR-1232-5


R.T.: 4.985 min
Delta R.T.: 0.004 min
Response: 2177582
Conc: 33.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

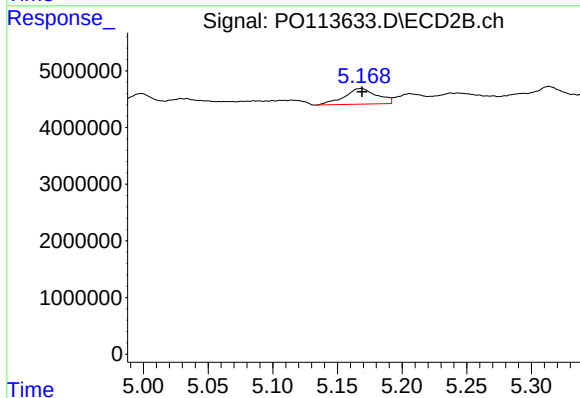


#15 AR-1232-5

R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 4882805
Conc: 72.21 ng/ml

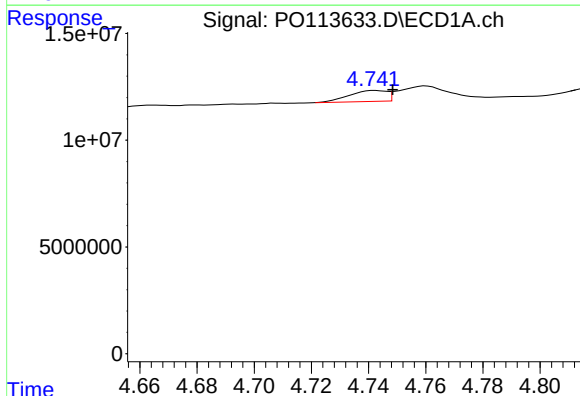


#16 AR-1242-1

R.T.: 4.742 min
Delta R.T.: -0.006 min
Response: 4720105
Conc: 20.53 ng/ml

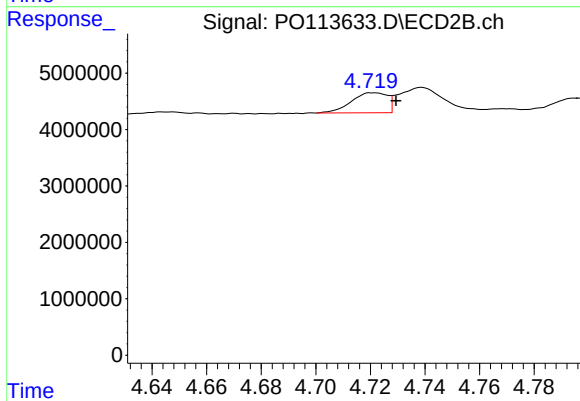

#16 AR-1242-1


R.T.: 4.721 min
Delta R.T.: -0.008 min
Response: 3253444
Conc: 22.51 ng/ml

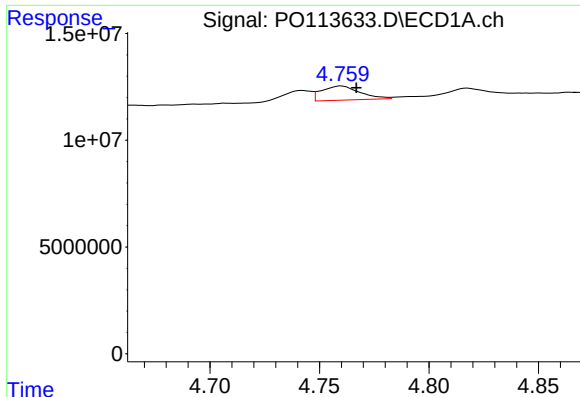

#17 AR-1242-2


R.T.: 4.760 min
Delta R.T.: -0.007 min
Response: 8101258
Conc: 23.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

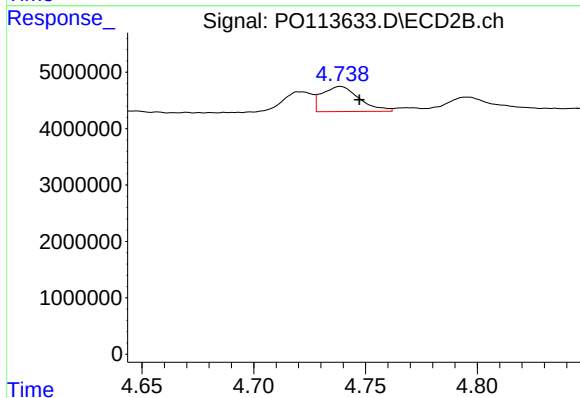


#17 AR-1242-2

R.T.: 4.739 min
Delta R.T.: -0.008 min
Response: 5154985
Conc: 23.77 ng/ml

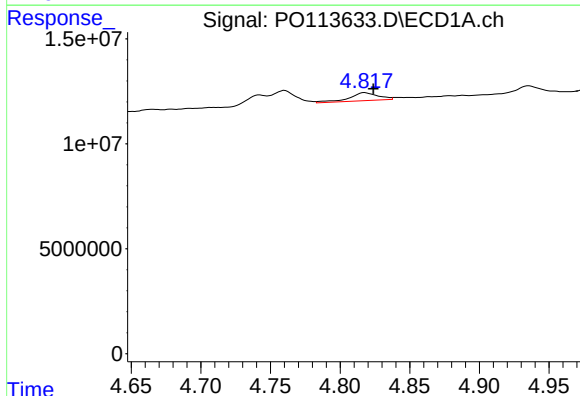


#18 AR-1242-3

R.T.: 4.818 min
Delta R.T.: -0.006 min
Response: 5476415
Conc: 24.68 ng/ml

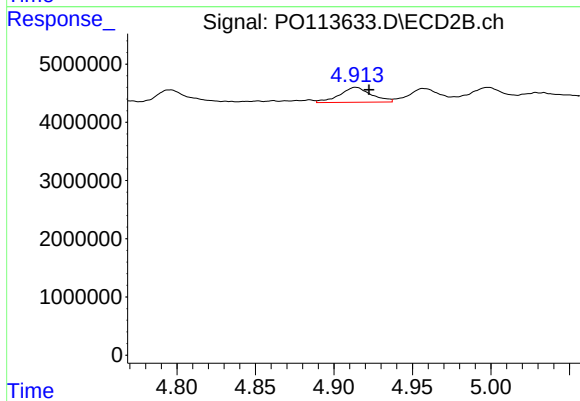

#18 AR-1242-3


R.T.: 4.914 min
Delta R.T.: -0.009 min
Response: 3611573
Conc: 30.88 ng/ml

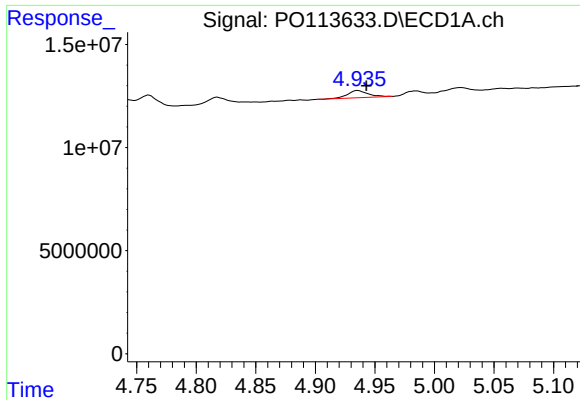

#19 AR-1242-4


R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 4174520
Conc: 24.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

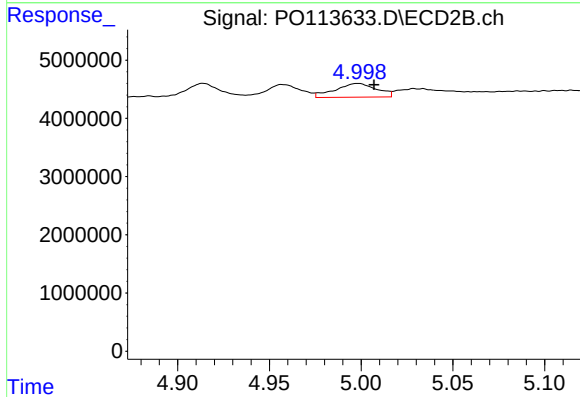


#19 AR-1242-4

R.T.: 4.998 min
Delta R.T.: -0.009 min
Response: 3689797
Conc: 31.37 ng/ml

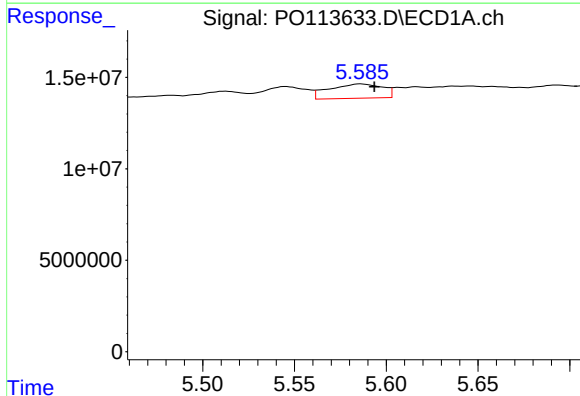


#20 AR-1242-5

R.T.: 5.586 min
Delta R.T.: -0.008 min
Response: 15808996
Conc: 78.98 ng/ml

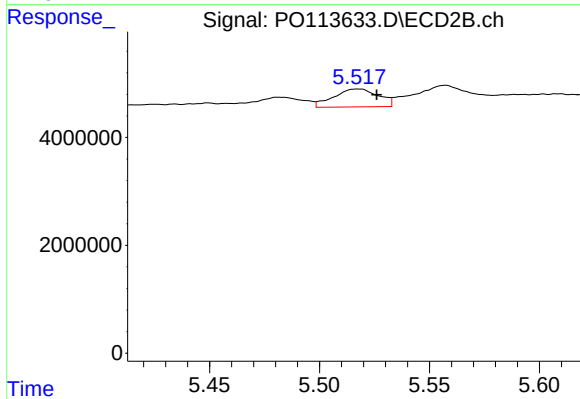

#20 AR-1242-5


R.T.: 5.518 min
Delta R.T.: -0.008 min
Response: 4719288
Conc: 31.64 ng/ml

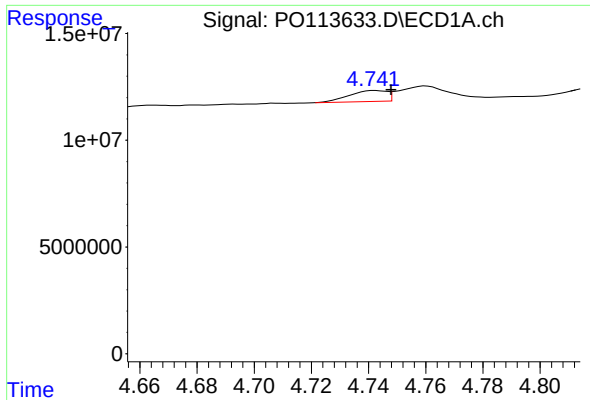

#21 AR-1248-1


R.T.: 4.742 min
Delta R.T.: -0.006 min
Response: 4720105
Conc: 27.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

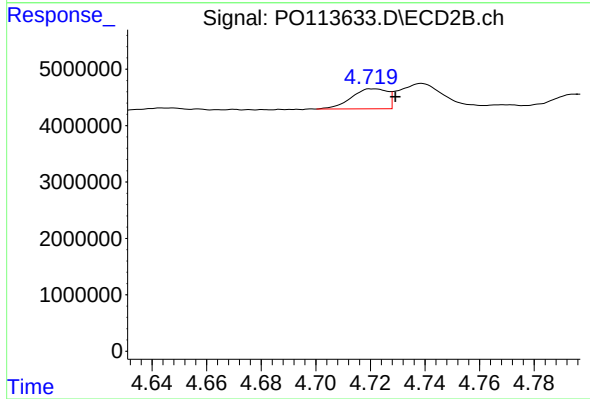


#21 AR-1248-1

R.T.: 4.721 min
Delta R.T.: -0.008 min
Response: 3253444
Conc: 29.18 ng/ml

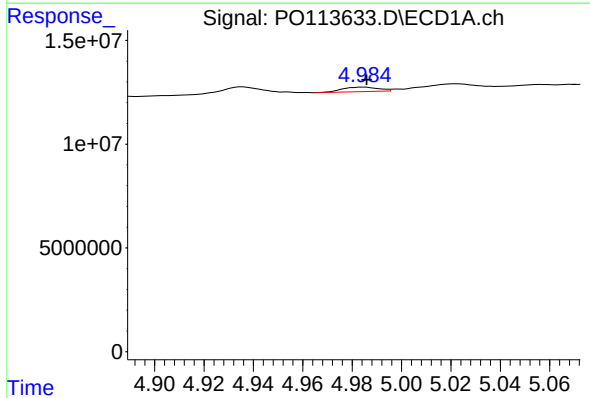


#22 AR-1248-2

R.T.: 4.985 min
Delta R.T.: -0.001 min
Response: 2177582
Conc: 9.00 ng/ml

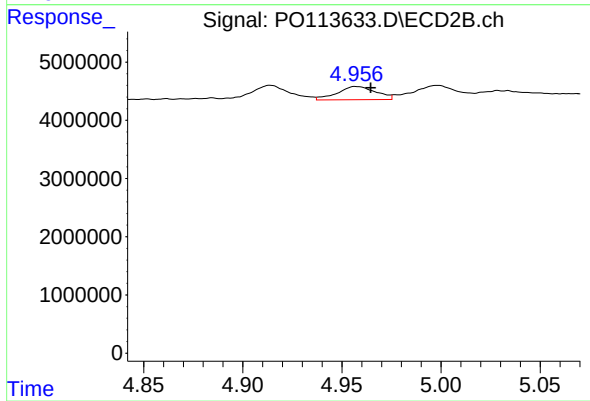

#22 AR-1248-2


R.T.: 4.957 min
Delta R.T.: -0.007 min
Response: 3052709
Conc: 19.00 ng/ml

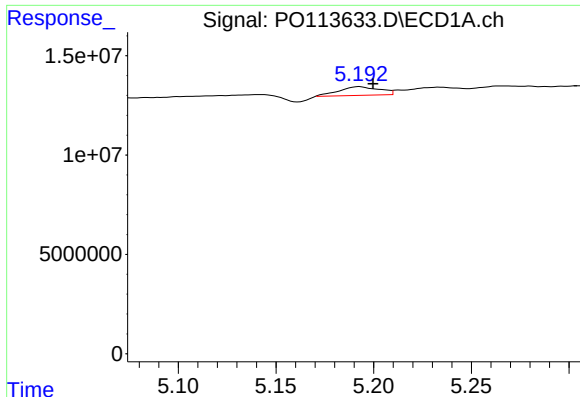

#23 AR-1248-3


R.T.: 5.193 min
Delta R.T.: -0.007 min
Response: 6343563
Conc: 19.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

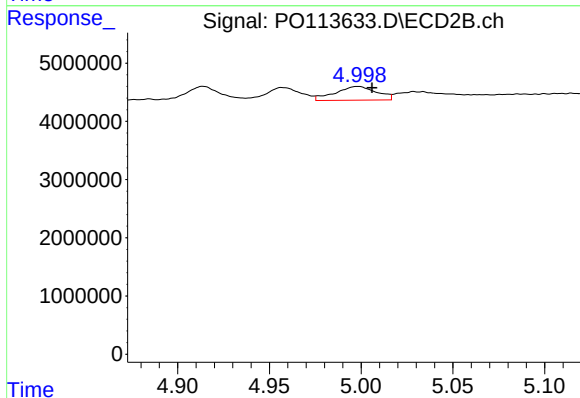


#23 AR-1248-3

R.T.: 4.998 min
Delta R.T.: -0.008 min
Response: 3689797
Conc: 21.75 ng/ml

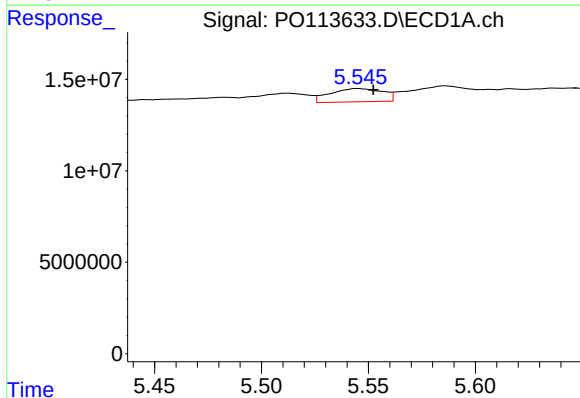


#24 AR-1248-4

R.T.: 5.545 min
Delta R.T.: -0.007 min
Response: 12364618
Conc: 24.75 ng/ml

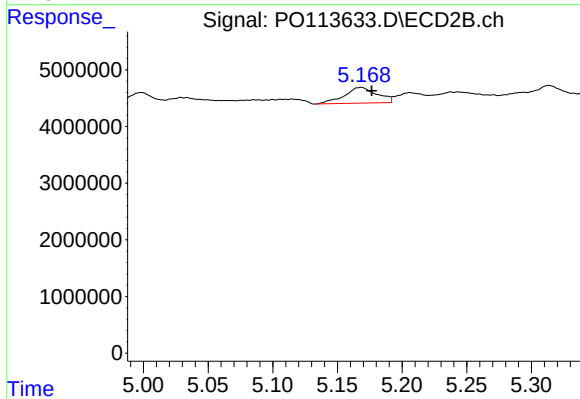

#24 AR-1248-4


R.T.: 5.168 min
Delta R.T.: -0.008 min
Response: 4882805
Conc: 24.51 ng/ml

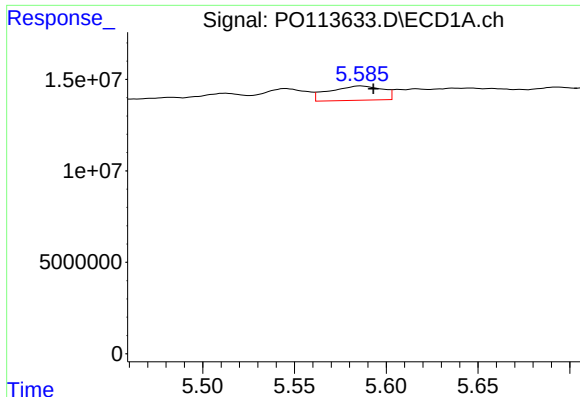

#25 AR-1248-5


R.T.: 5.586 min
Delta R.T.: -0.007 min
Response: 15808996
Conc: 46.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

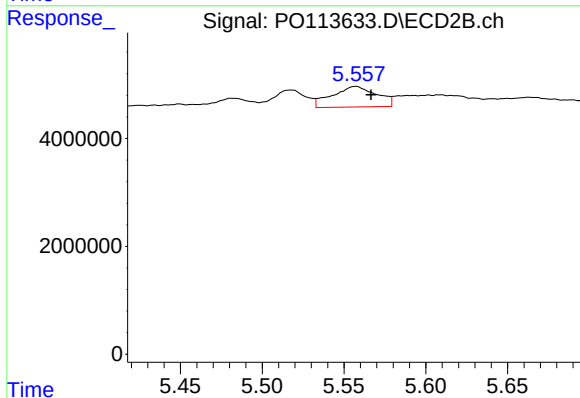


#25 AR-1248-5

R.T.: 5.557 min
Delta R.T.: -0.009 min
Response: 7234530
Conc: 34.08 ng/ml

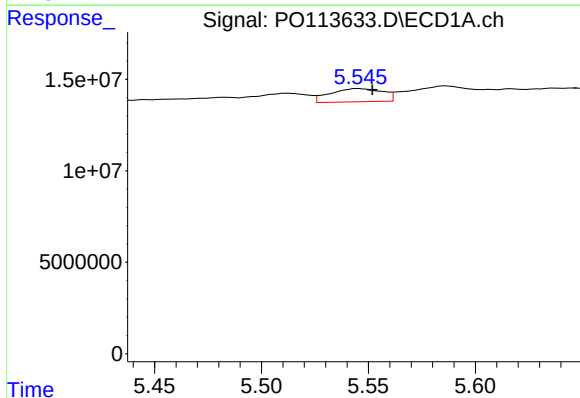


#26 AR-1254-1

R.T.: 5.545 min
Delta R.T.: -0.007 min
Response: 12364618
Conc: 22.90 ng/ml

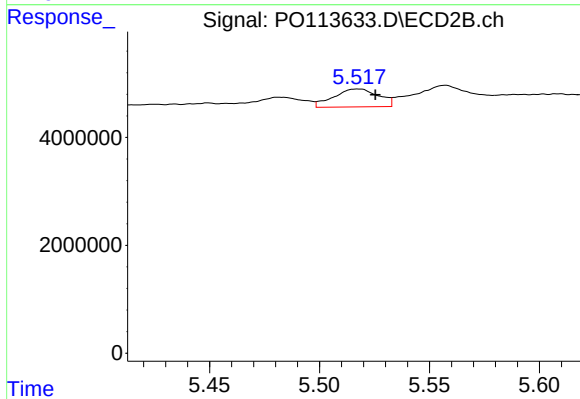

#26 AR-1254-1


R.T.: 5.518 min
Delta R.T.: -0.008 min
Response: 4719288
Conc: 14.97 ng/ml

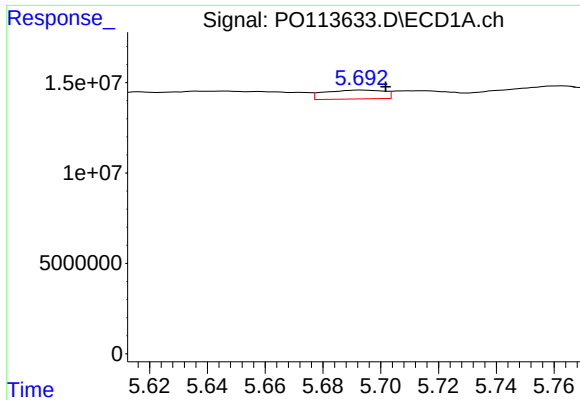

#27 AR-1254-2


R.T.: 5.693 min
Delta R.T.: -0.008 min
Response: 6976238
Conc: 14.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

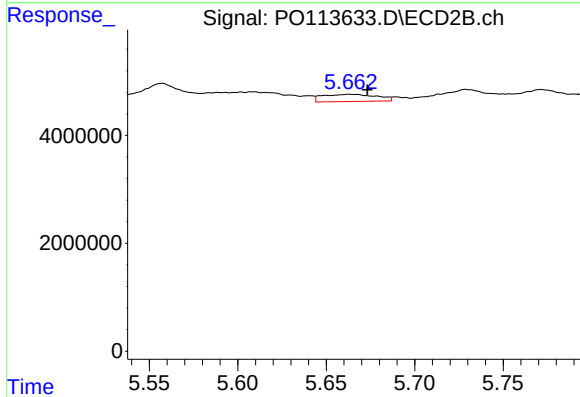


#27 AR-1254-2

R.T.: 5.663 min
Delta R.T.: -0.010 min
Response: 2832022
Conc: 10.10 ng/ml

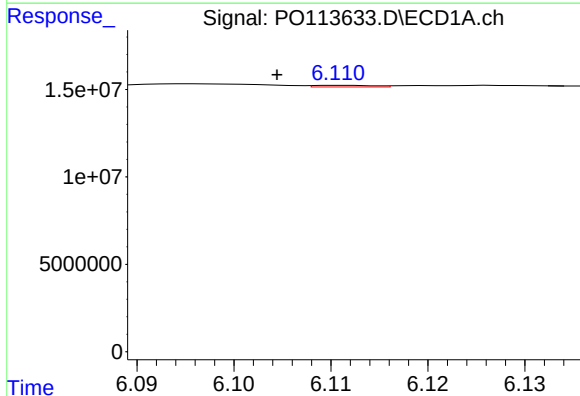


#28 AR-1254-3

R.T.: 6.111 min
Delta R.T.: 0.007 min
Response: 396651
Conc: 0.54 ng/ml

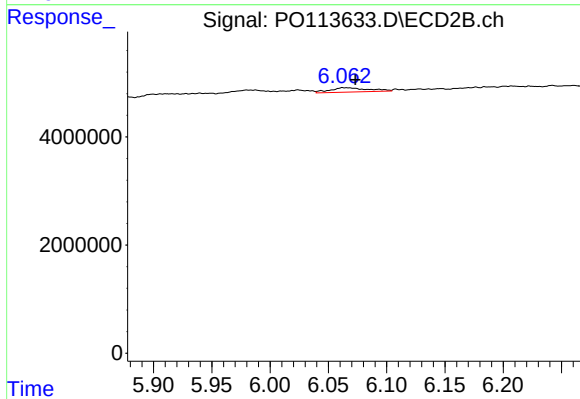

#28 AR-1254-3


R.T.: 6.063 min
Delta R.T.: -0.010 min
Response: 1825089
Conc: 4.38 ng/ml

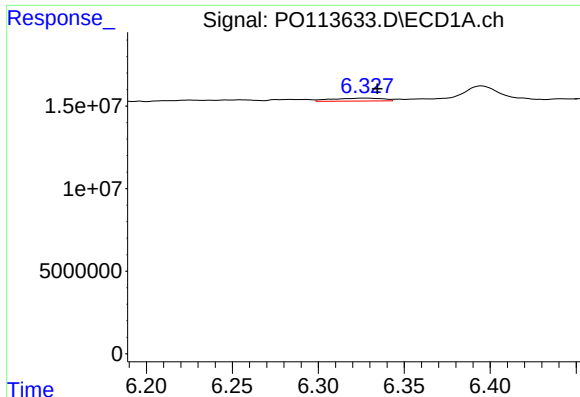

#29 AR-1254-4


R.T.: 6.327 min
Delta R.T.: -0.008 min
Response: 3702545
Conc: 6.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

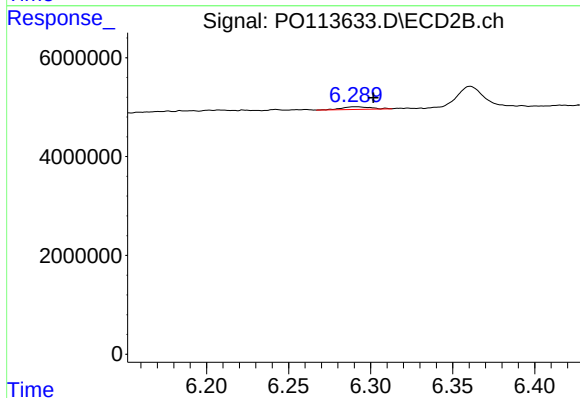


#29 AR-1254-4

R.T.: 6.291 min
Delta R.T.: -0.011 min
Response: 641807
Conc: 2.34 ng/ml

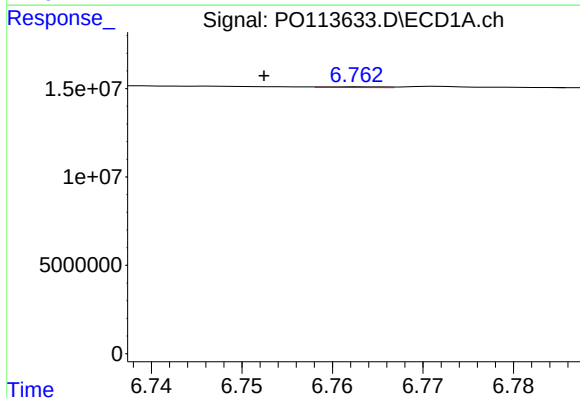


#30 AR-1254-5

R.T.: 6.763 min
Delta R.T.: 0.010 min
Response: 204022
Conc: 0.29 ng/ml

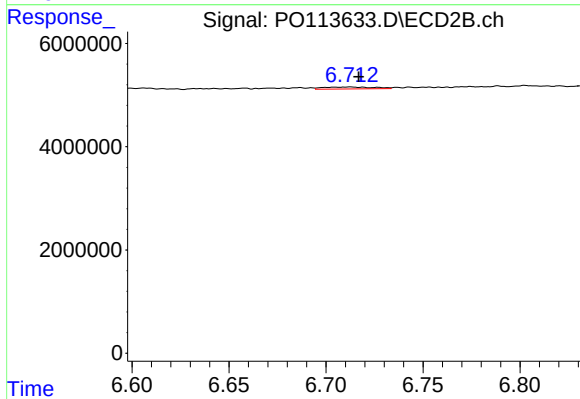

#30 AR-1254-5


R.T.: 6.713 min
Delta R.T.: -0.004 min
Response: 651439
Conc: 1.82 ng/ml

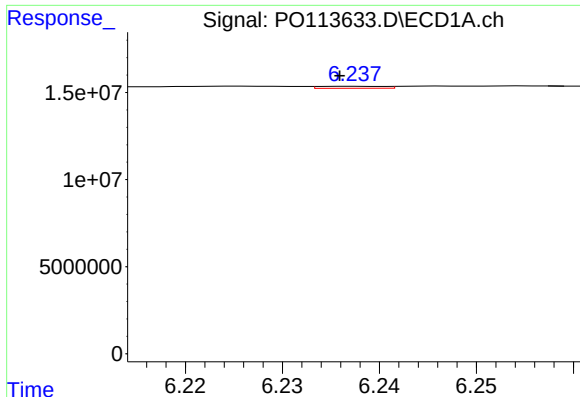

#31 AR-1260-1


R.T.: 6.238 min
Delta R.T.: 0.002 min
Response: 549032
Conc: 1.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

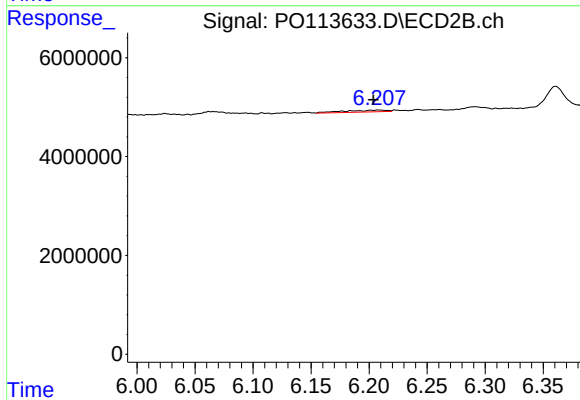


#31 AR-1260-1

R.T.: 6.208 min
Delta R.T.: 0.004 min
Response: 935188
Conc: 3.67 ng/ml

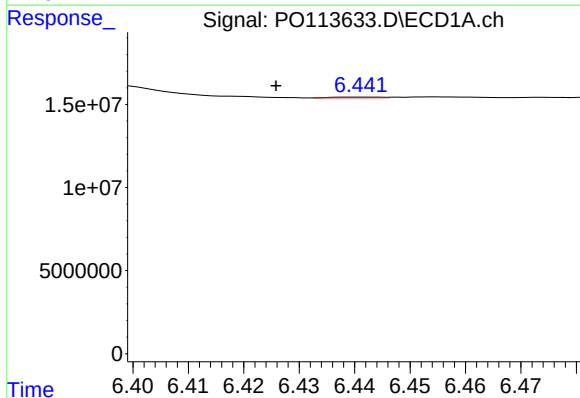


#32 AR-1260-2

R.T.: 6.441 min
Delta R.T.: 0.015 min
Response: 298611
Conc: 0.43 ng/ml

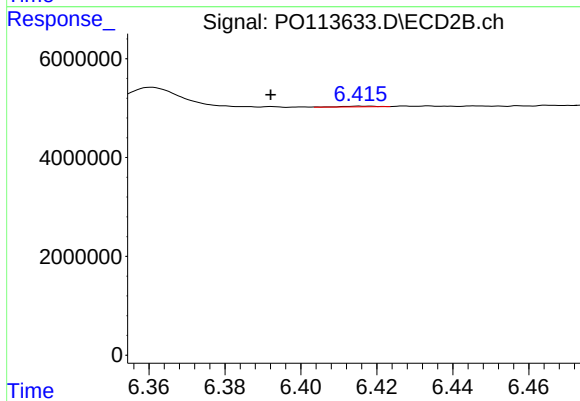

#32 AR-1260-2


R.T.: 6.416 min
Delta R.T.: 0.024 min
Response: 95332
Conc: 0.28 ng/ml

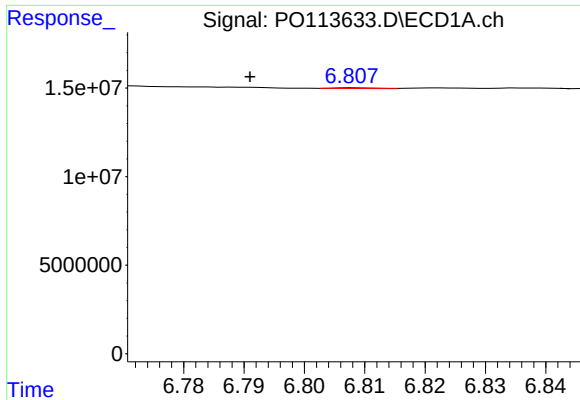

#33 AR-1260-3


R.T.: 6.808 min
Delta R.T.: 0.017 min
Response: 207211
Conc: 0.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

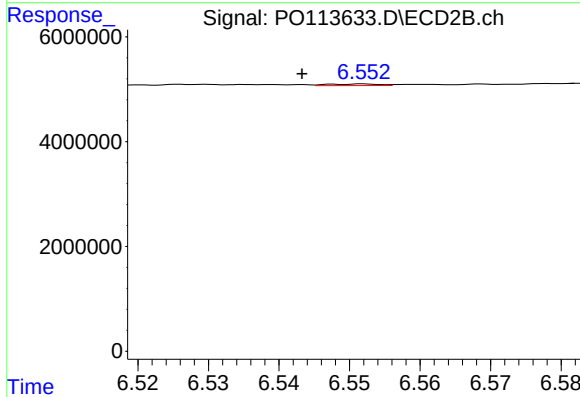


#33 AR-1260-3

R.T.: 6.552 min
Delta R.T.: 0.009 min
Response: 158909
Conc: 0.53 ng/ml

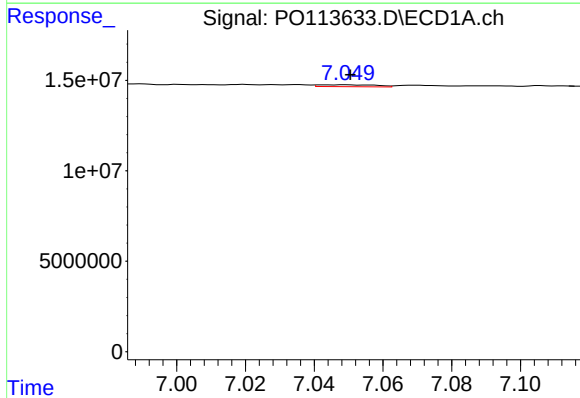


#34 AR-1260-4

R.T.: 7.049 min
Delta R.T.: -0.001 min
Response: 1190296
Conc: 2.66 ng/ml

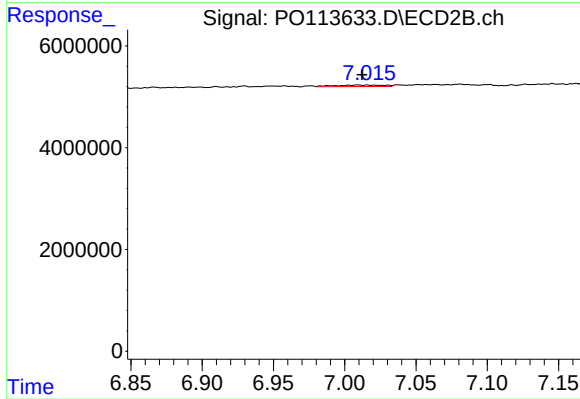

#34 AR-1260-4


R.T.: 7.016 min
Delta R.T.: 0.003 min
Response: 700580
Conc: 3.38 ng/ml

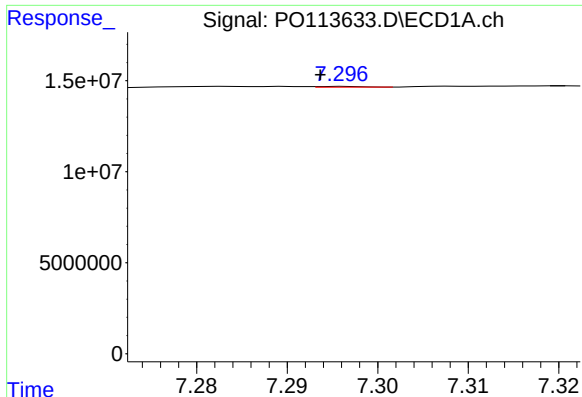

#35 AR-1260-5


R.T.: 7.296 min
Delta R.T.: 0.002 min
Response: 146637
Conc: 0.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

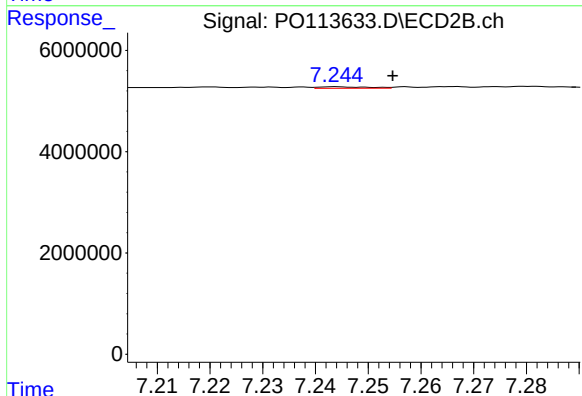


#35 AR-1260-5

R.T.: 7.244 min
Delta R.T.: -0.011 min
Response: 201988
Conc: 0.43 ng/ml

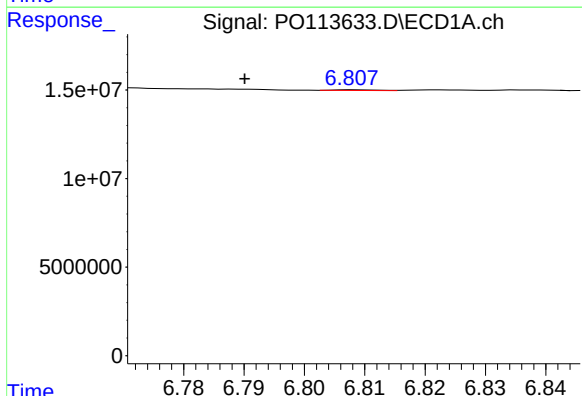


#36 AR-1262-1

R.T.: 6.808 min
Delta R.T.: 0.018 min
Response: 207211
Conc: 0.23 ng/ml

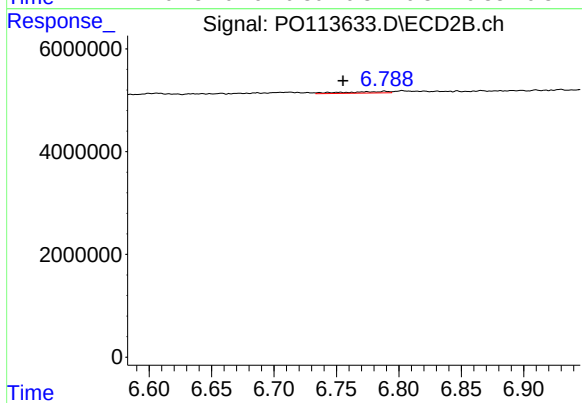

#36 AR-1262-1


R.T.: 6.789 min
Delta R.T.: 0.033 min
Response: 718582
Conc: 1.73 ng/ml

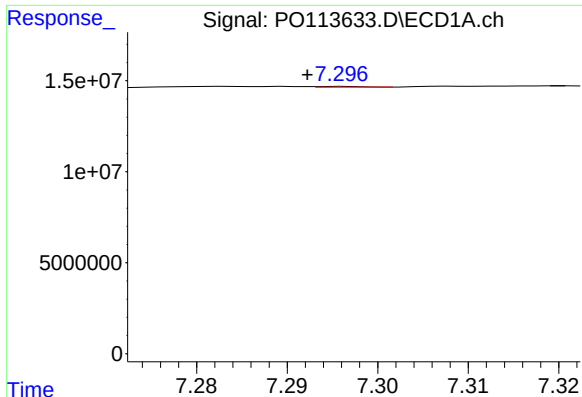

#37 AR-1262-2


R.T.: 7.296 min
Delta R.T.: 0.004 min
Response: 146637
Conc: 0.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

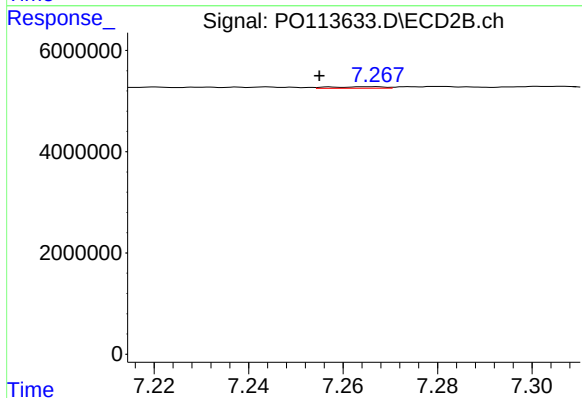


#37 AR-1262-2

R.T.: 7.266 min
Delta R.T.: 0.011 min
Response: 230058
Conc: 0.44 ng/ml

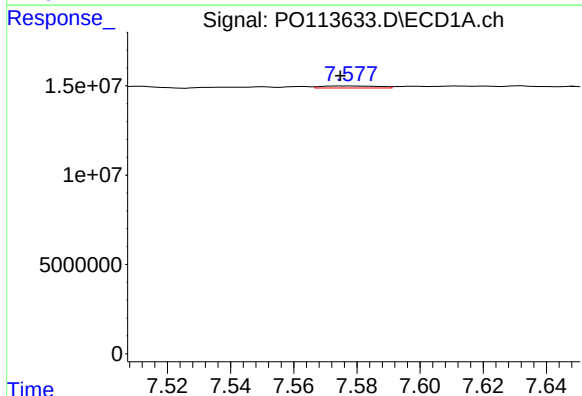


#38 AR-1262-3

R.T.: 7.577 min
Delta R.T.: 0.003 min
Response: 1392403
Conc: 2.51 ng/ml

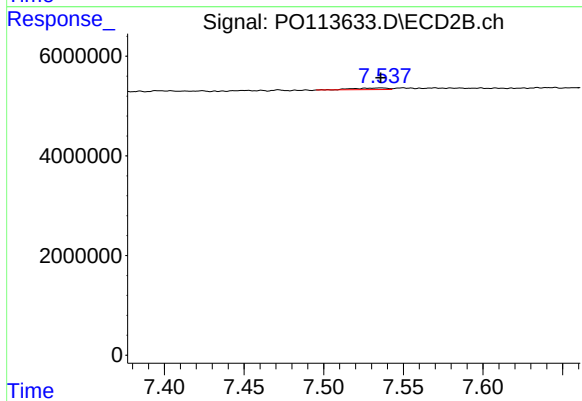

#38 AR-1262-3


R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 450700
Conc: 2.51 ng/ml

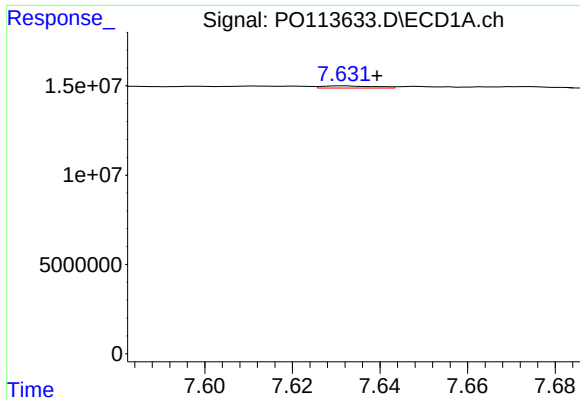

#39 AR-1262-4


R.T.: 7.632 min
Delta R.T.: -0.007 min
Response: 1006119
Conc: 1.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

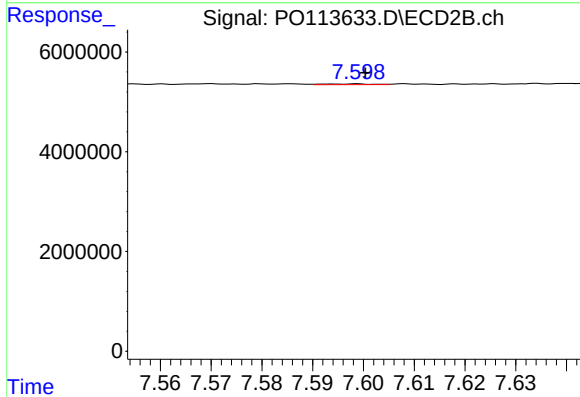


#39 AR-1262-4

R.T.: 7.599 min
Delta R.T.: -0.002 min
Response: 100716
Conc: 0.35 ng/ml

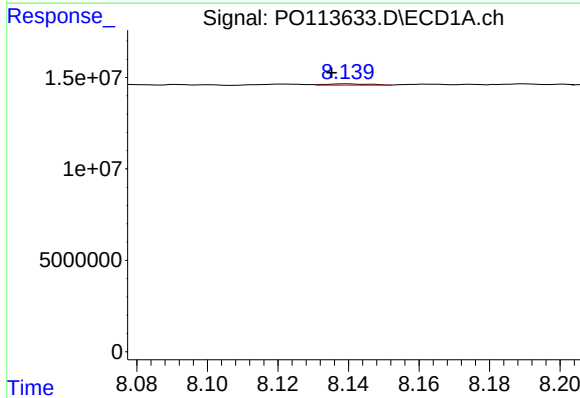


#40 AR-1262-5

R.T.: 8.140 min
Delta R.T.: 0.004 min
Response: 633682
Conc: 1.52 ng/ml

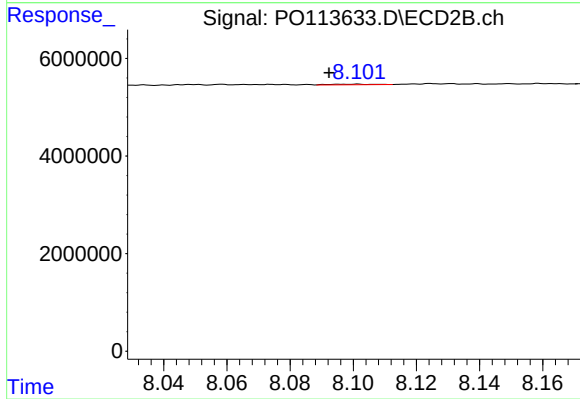

#40 AR-1262-5


R.T.: 8.101 min
Delta R.T.: 0.009 min
Response: 107336
Conc: 0.99 ng/ml

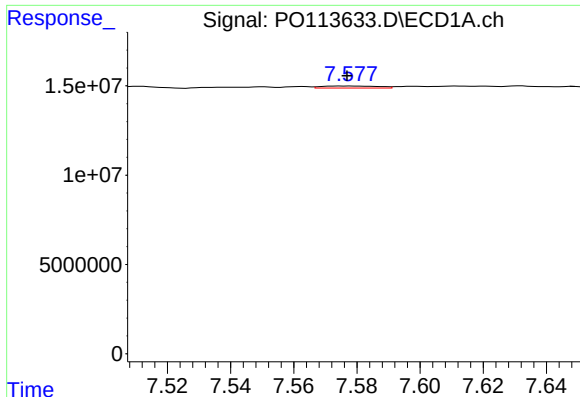

#41 AR-1268-1


R.T.: 7.577 min
Delta R.T.: 0.000 min
Response: 1392403
Conc: 0.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

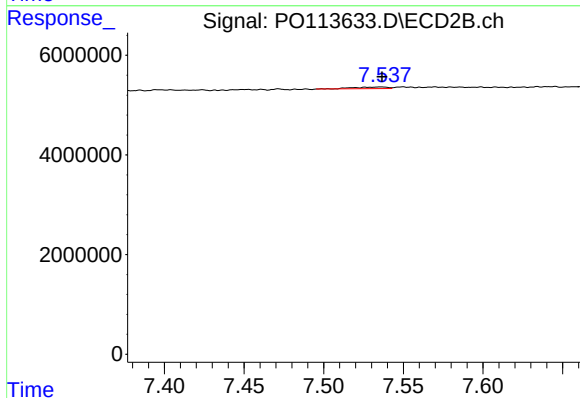


#41 AR-1268-1

R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 450700
Conc: 0.88 ng/ml

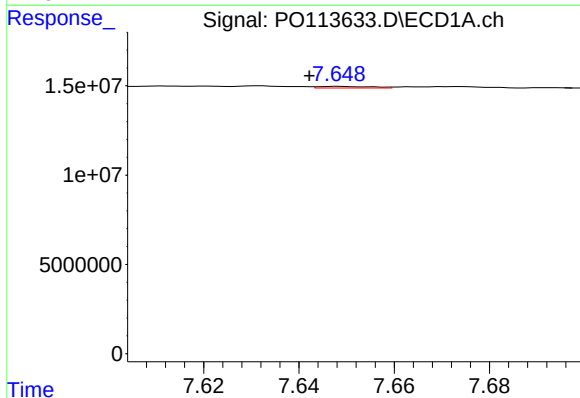


#42 AR-1268-2

R.T.: 7.649 min
Delta R.T.: 0.006 min
Response: 697595
Conc: 0.48 ng/ml

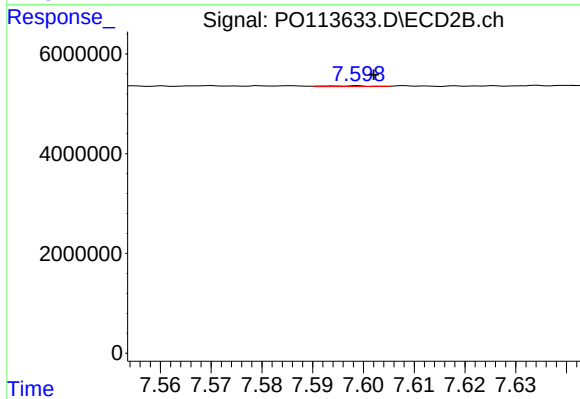

#42 AR-1268-2


R.T.: 7.599 min
Delta R.T.: -0.003 min
Response: 100716
Conc: 0.24 ng/ml

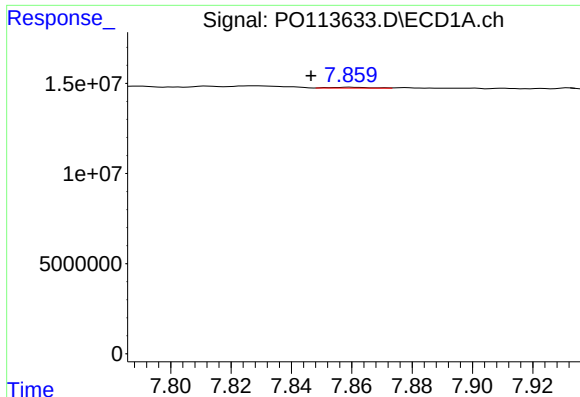

#43 AR-1268-3


R.T.: 7.860 min
Delta R.T.: 0.013 min
Response: 368050
Conc: 0.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

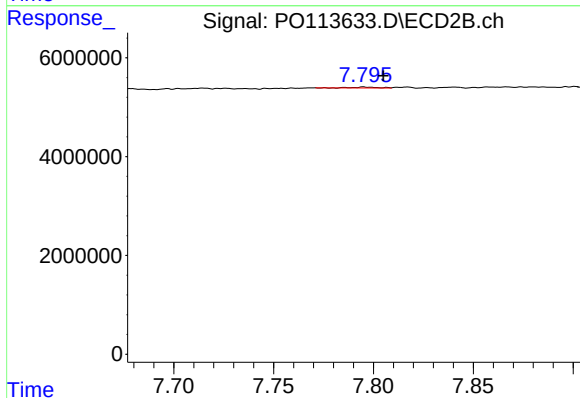


#43 AR-1268-3

R.T.: 7.795 min
Delta R.T.: -0.010 min
Response: 139948
Conc: 0.43 ng/ml

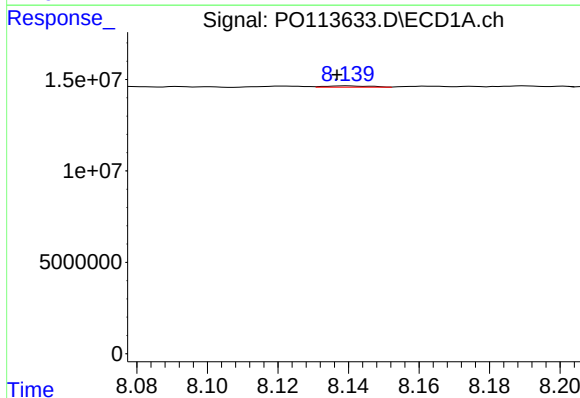


#44 AR-1268-4

R.T.: 8.140 min
Delta R.T.: 0.003 min
Response: 633682
Conc: 1.38 ng/ml

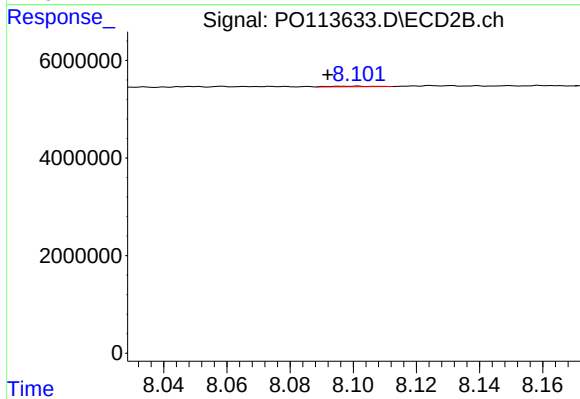

#44 AR-1268-4


R.T.: 8.101 min
Delta R.T.: 0.010 min
Response: 107336
Conc: 0.89 ng/ml

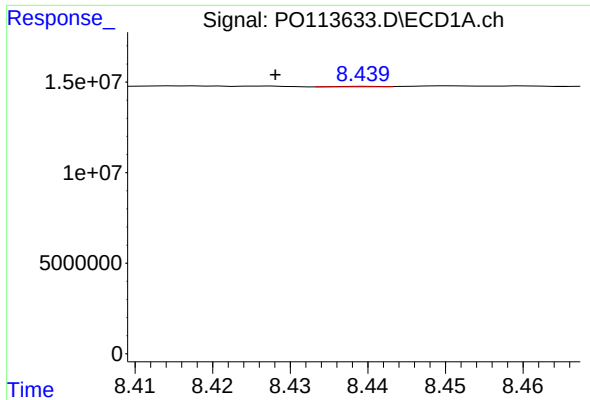

#45 AR-1268-5

R.T.: 8.440 min
Delta R.T.: 0.012 min
Response: 110205
Conc: 0.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

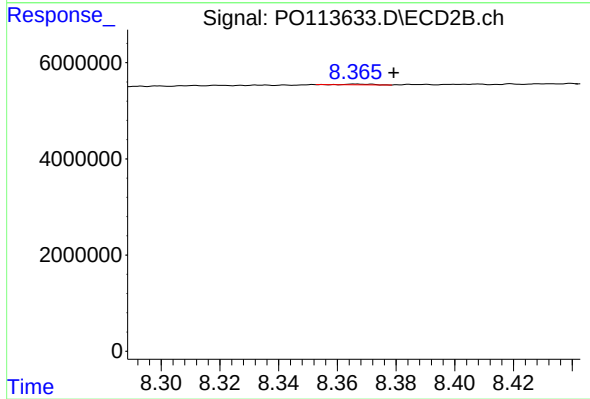

#45 AR-1268-5

R.T.: 8.366 min
Delta R.T.: -0.013 min
Response: 93064
Conc: 0.12 ng/ml