

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
 Data File : P0113634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 03:02
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1242 WATER LOD 40PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:30:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.658	3.649	176.9E6	104.4E6	21.610	20.631
2)	SA Decachlor...	8.669	8.614	150.0E6	43200392	21.648	22.799
Target Compounds							
3)	L1 AR-1016-1	4.741	4.721	9219200	6179911	34.531	36.230
4)	L1 AR-1016-2	4.760	4.739	14305357	9406278	35.636	36.507
5)	L1 AR-1016-3	4.816	4.914	10173251	5860061	39.892	41.973
6)	L1 AR-1016-4	4.936	4.957	7744252	5679794	35.513	48.670 #
7)	L1 AR-1016-5	5.192	5.167	11197672	7669972	50.525	53.813
8)	L2 AR-1221-1	3.870	3.861	294069	592530	3.143	9.387 #
9)	L2 AR-1221-2	3.957	3.944	1974300	3209411	29.227	68.763 #
10)	L2 AR-1221-3	4.030	4.017	4542321	3518186	20.521	23.695
11)	L3 AR-1232-1	4.030	4.017	4542321	3518186	25.302	29.092
12)	L3 AR-1232-2	4.520	4.739	7252579	9406278	67.205	77.069
13)	L3 AR-1232-3	4.760	4.914	14305357	5860061	72.471	88.579
14)	L3 AR-1232-4	4.936	4.997	7744252	6391763	78.787	106.657 #
15)	L3 AR-1232-5	4.981	5.167	5675034	7669972	86.270	113.434 #
16)	L4 AR-1242-1	4.741	4.721	9219200	6179911	40.095	42.766
17)	L4 AR-1242-2	4.760	4.739	14305357	9406278	41.631	43.365
18)	L4 AR-1242-3	4.816	4.914	10173251	5860061	45.849	50.101
19)	L4 AR-1242-4	4.936	4.997	7744252	6391763	44.645	54.334
20)	L4 AR-1242-5	5.585	5.516	17870203	8105786	89.279	54.353 #
21)	L5 AR-1248-1	4.741	4.721	9219200	6179911	52.842	55.419
22)	L5 AR-1248-2	4.981	4.957	5675034	5679794	23.464	35.344 #
23)	L5 AR-1248-3	5.192	4.997	11197672	6391763	35.117	37.674
24)	L5 AR-1248-4	5.544	5.167	18288935	7669972	36.607	38.500
25)	L5 AR-1248-5	5.585	5.557	17870203	9443870	52.330	44.484
26)	L6 AR-1254-1	5.544	5.516	18288935	8105786	33.870	25.704
27)	L6 AR-1254-2	5.695	5.662	12830814	3336780	26.002	11.903 #
28)	L6 AR-1254-3	6.095	6.082	4686587	325759	6.343	0.781 #
29)	L6 AR-1254-4	6.324	6.292	5908674	1539996	10.608	5.603 #
30)	L6 AR-1254-5	6.758	6.722	1113307	210690	1.588	0.589 #
31)	L7 AR-1260-1	6.242	6.206	4611089	487708	10.339	1.912 #
32)	L7 AR-1260-2	6.394	6.390	14153808	92900	20.611	0.269 #
33)	L7 AR-1260-3	6.768	6.548	3430783	68655	5.556	0.231 #
34)	L7 AR-1260-4	7.051	7.018	7254042	210566	16.197	1.016 #
35)	L7 AR-1260-5	7.287	7.250	1748969	621843	1.445	1.328
36)	L8 AR-1262-1	6.768	6.752	3430783	185087	3.746	0.446 #
37)	L8 AR-1262-2	7.287	7.250	1748969	621843	1.157	1.201
38)	L8 AR-1262-3	7.578	7.526	1732707	465509	3.127	2.592
39)	L8 AR-1262-4	7.636	7.585	634223	285028	0.649	0.983 #
40)	L8 AR-1262-5	8.128	8.093	212776	111385	0.510	1.028 #
41)	L9 AR-1268-1	7.578	7.526	1732707	465509	1.007	0.914

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
Data File : P0113634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 03:02
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1242 WATER LOD 40PPB
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:30:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.636	7.585	634223	285028	0.438	0.686 #
43) L9	AR-1268-3	7.827	7.804	724598	94645	0.601	0.290 #
44) L9	AR-1268-4	8.143	8.093	392091	111385	0.851	0.925
45) L9	AR-1268-5	8.433	8.370	298312	281812	0.094	0.361 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091025\
Data File : PO113634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 03:02
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1242 WATER LOD 40PPB
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:30:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

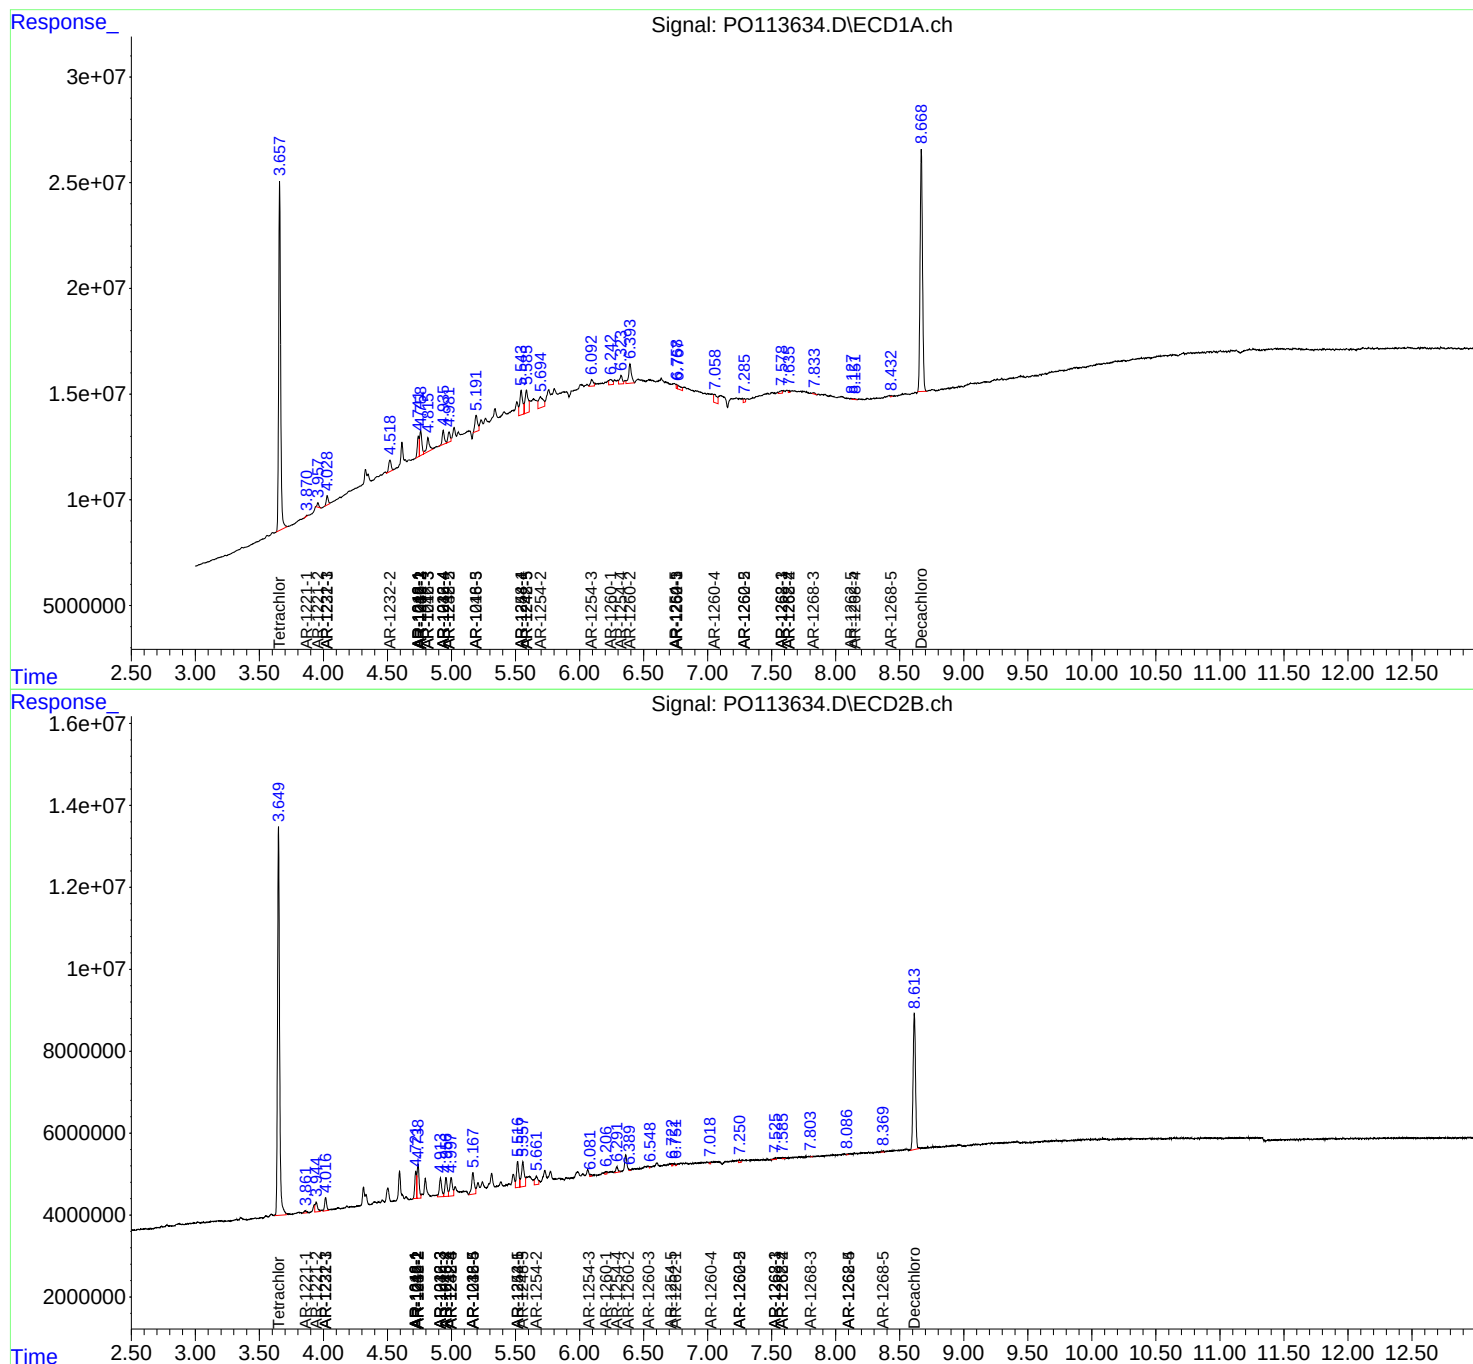


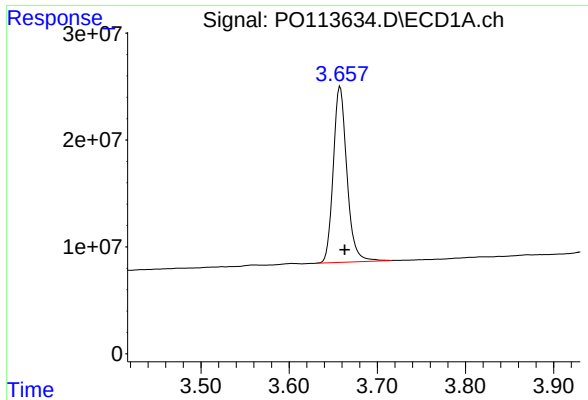

#1 Tetrachloro-m-xylene


R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 176909846
Conc: 21.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

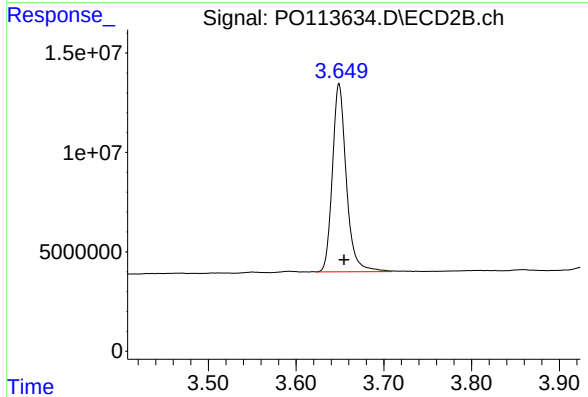


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.006 min
Response: 104405968
Conc: 20.63 ng/ml

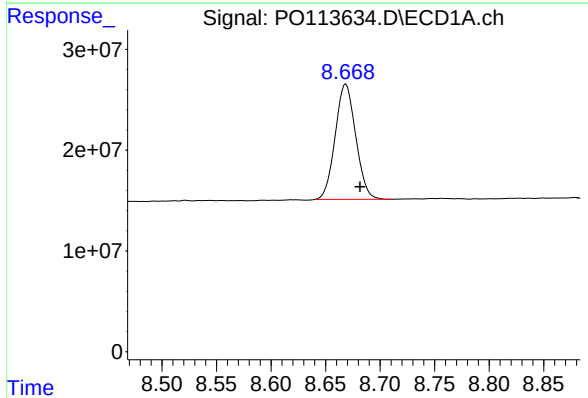


#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.013 min
Response: 150049218
Conc: 21.65 ng/ml

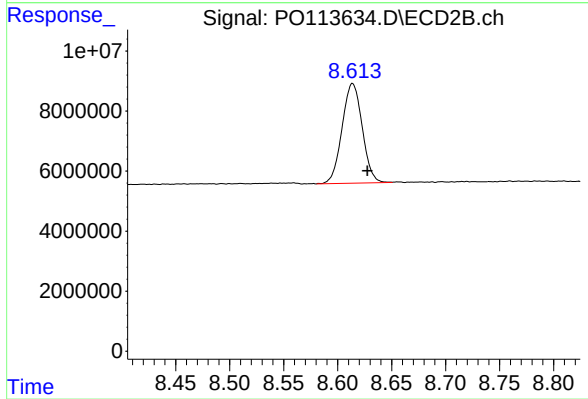

#2 Decachlorobiphenyl


R.T.: 8.614 min
Delta R.T.: -0.014 min
Response: 43200392
Conc: 22.80 ng/ml

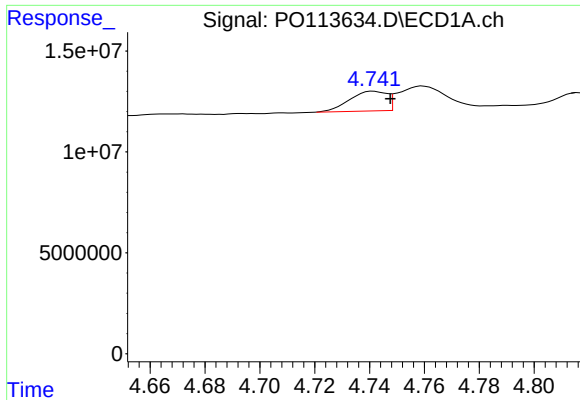

#3 AR-1016-1


R.T.: 4.741 min
Delta R.T.: -0.006 min
Response: 9219200
Conc: 34.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

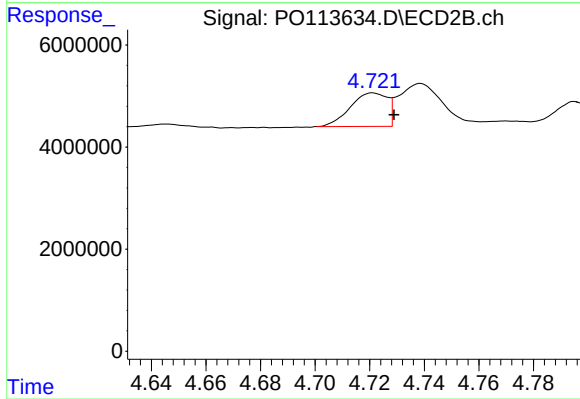


#3 AR-1016-1

R.T.: 4.721 min
Delta R.T.: -0.008 min
Response: 6179911
Conc: 36.23 ng/ml

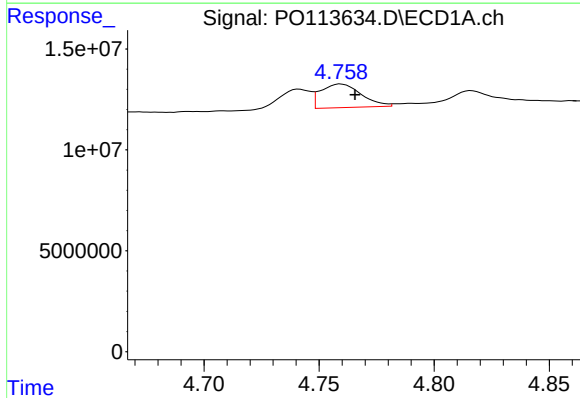


#4 AR-1016-2

R.T.: 4.760 min
Delta R.T.: -0.006 min
Response: 14305357
Conc: 35.64 ng/ml

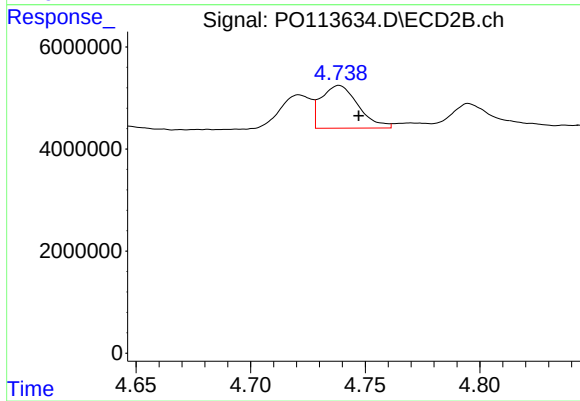

#4 AR-1016-2


R.T.: 4.739 min
Delta R.T.: -0.008 min
Response: 9406278
Conc: 36.51 ng/ml

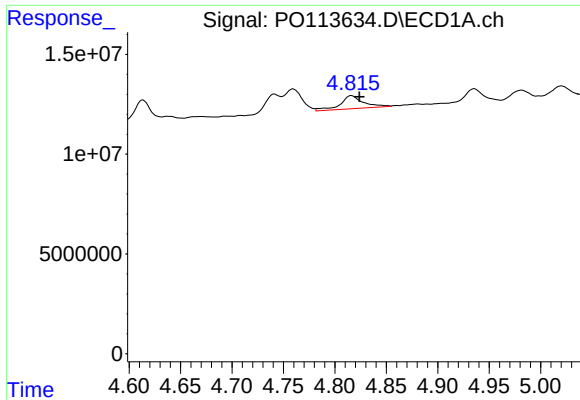

#5 AR-1016-3


R.T.: 4.816 min
Delta R.T.: -0.008 min
Response: 10173251
Conc: 39.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

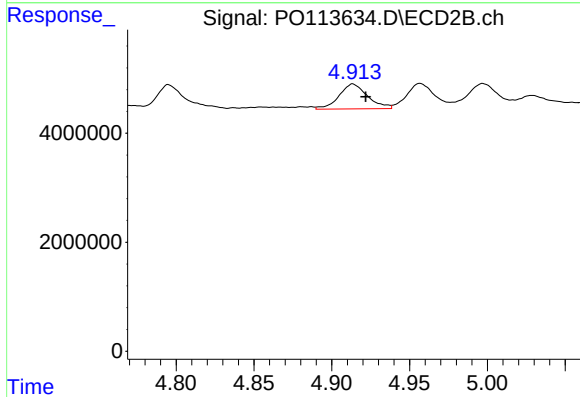


#5 AR-1016-3

R.T.: 4.914 min
Delta R.T.: -0.008 min
Response: 5860061
Conc: 41.97 ng/ml

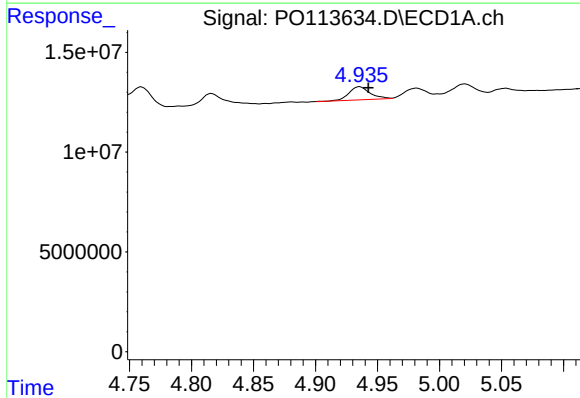


#6 AR-1016-4

R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 7744252
Conc: 35.51 ng/ml

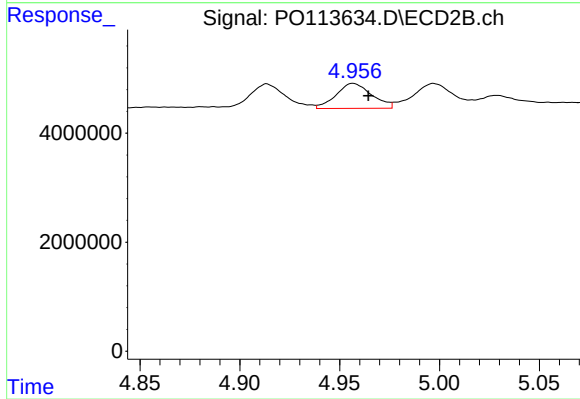

#6 AR-1016-4


R.T.: 4.957 min
Delta R.T.: -0.008 min
Response: 5679794
Conc: 48.67 ng/ml

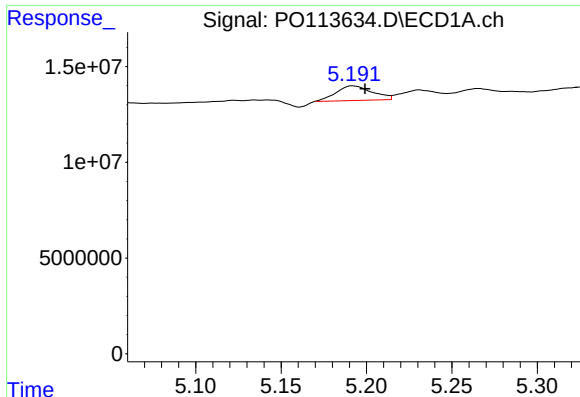

#7 AR-1016-5


R.T.: 5.192 min
Delta R.T.: -0.007 min
Response: 11197672
Conc: 50.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

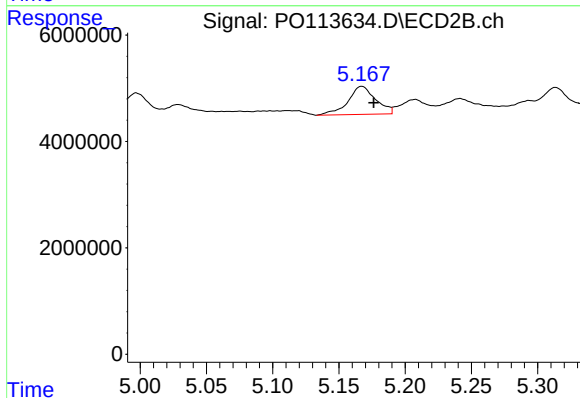


#7 AR-1016-5

R.T.: 5.167 min
Delta R.T.: -0.009 min
Response: 7669972
Conc: 53.81 ng/ml

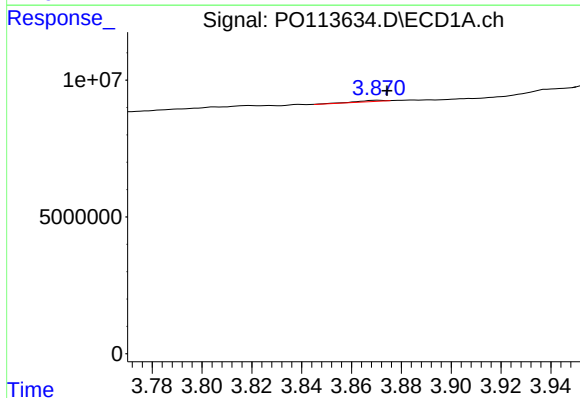


#8 AR-1221-1

R.T.: 3.870 min
Delta R.T.: -0.004 min
Response: 294069
Conc: 3.14 ng/ml

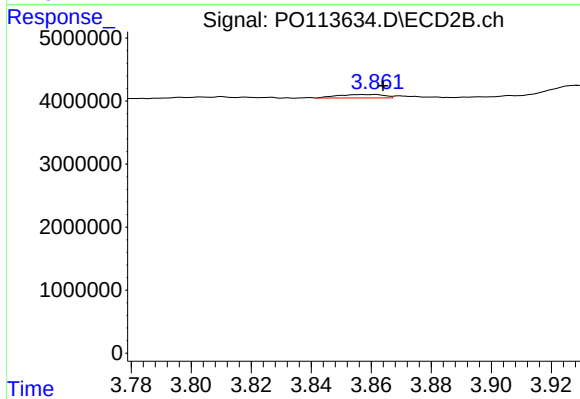

#8 AR-1221-1


R.T.: 3.861 min
Delta R.T.: -0.003 min
Response: 592530
Conc: 9.39 ng/ml

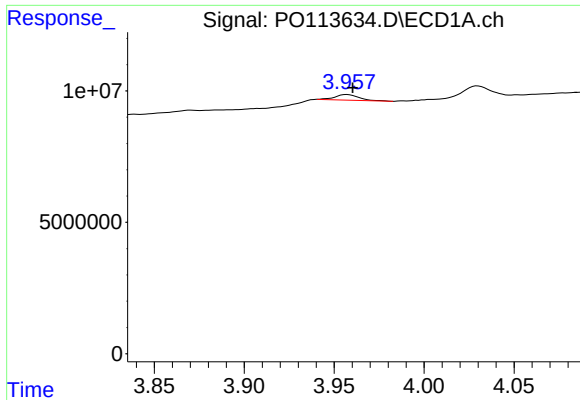

#9 AR-1221-2


R.T.: 3.957 min
Delta R.T.: -0.003 min
Response: 1974300
Conc: 29.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

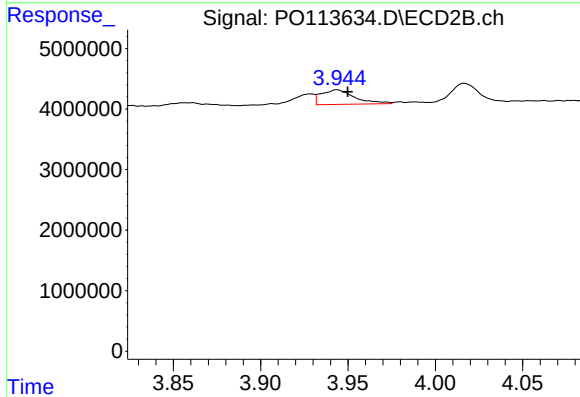


#9 AR-1221-2

R.T.: 3.944 min
Delta R.T.: -0.006 min
Response: 3209411
Conc: 68.76 ng/ml

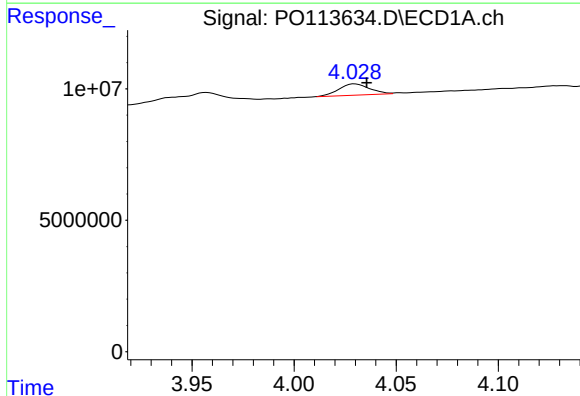


#10 AR-1221-3

R.T.: 4.030 min
Delta R.T.: -0.006 min
Response: 4542321
Conc: 20.52 ng/ml

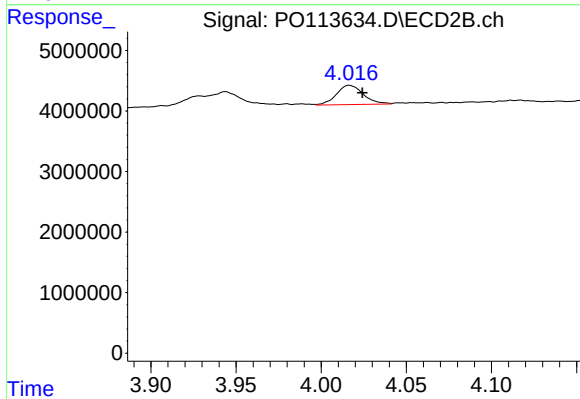

#10 AR-1221-3


R.T.: 4.017 min
Delta R.T.: -0.008 min
Response: 3518186
Conc: 23.70 ng/ml

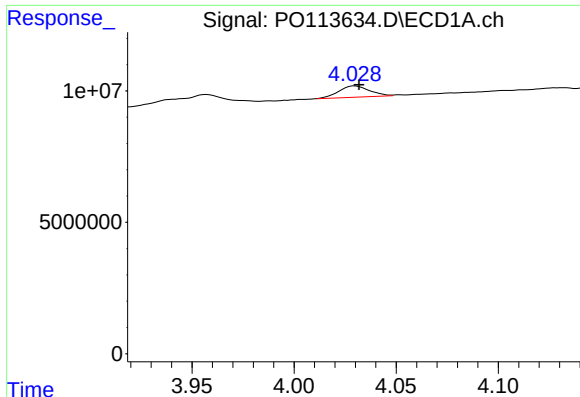

#11 AR-1232-1


R.T.: 4.030 min
Delta R.T.: -0.002 min
Response: 4542321
Conc: 25.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

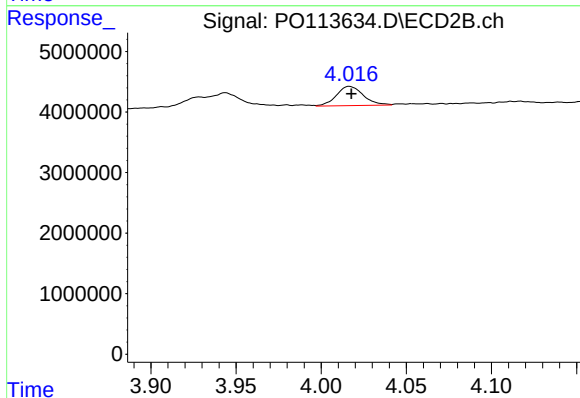


#11 AR-1232-1

R.T.: 4.017 min
Delta R.T.: -0.001 min
Response: 3518186
Conc: 29.09 ng/ml

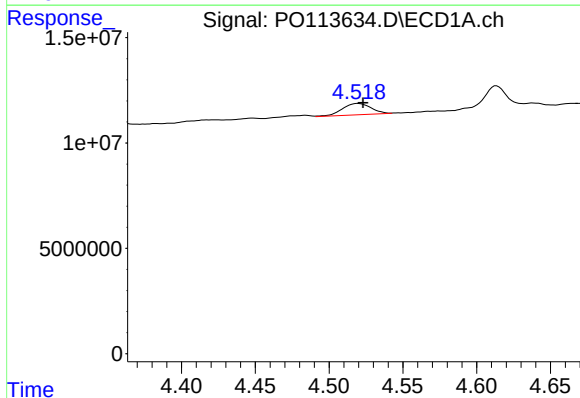


#12 AR-1232-2

R.T.: 4.520 min
Delta R.T.: -0.003 min
Response: 7252579
Conc: 67.21 ng/ml

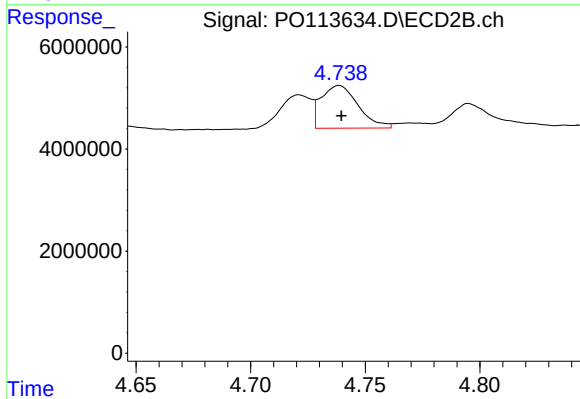

#12 AR-1232-2


R.T.: 4.739 min
Delta R.T.: 0.000 min
Response: 9406278
Conc: 77.07 ng/ml

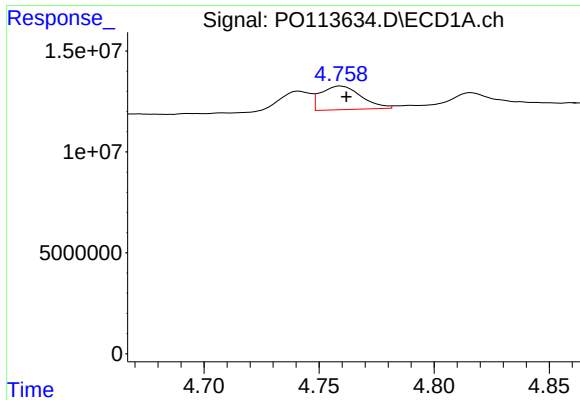

#13 AR-1232-3


R.T.: 4.760 min
Delta R.T.: -0.002 min
Response: 14305357
Conc: 72.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

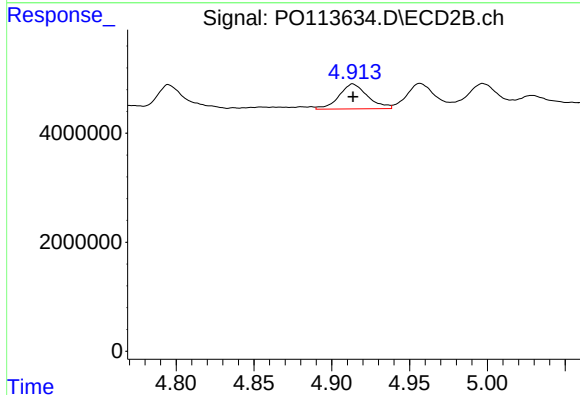


#13 AR-1232-3

R.T.: 4.914 min
Delta R.T.: 0.000 min
Response: 5860061
Conc: 88.58 ng/ml

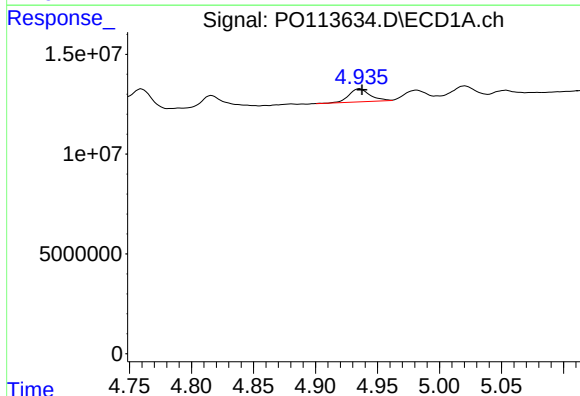


#14 AR-1232-4

R.T.: 4.936 min
Delta R.T.: -0.002 min
Response: 7744252
Conc: 78.79 ng/ml

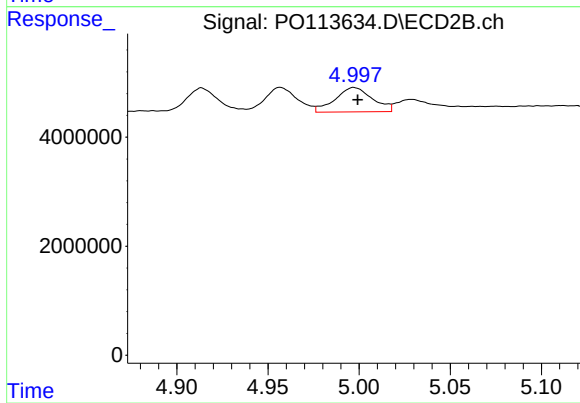

#14 AR-1232-4


R.T.: 4.997 min
Delta R.T.: -0.002 min
Response: 6391763
Conc: 106.66 ng/ml

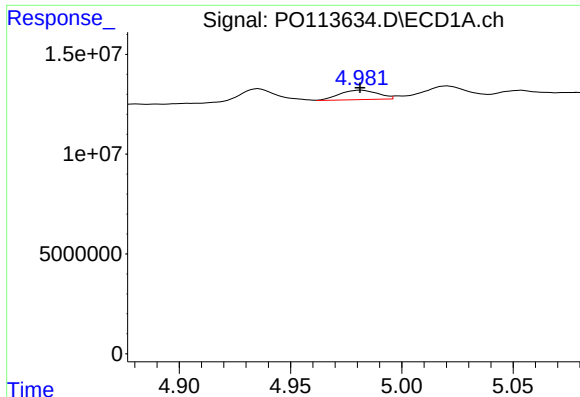

#15 AR-1232-5


R.T.: 4.981 min
Delta R.T.: 0.000 min
Response: 5675034
Conc: 86.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

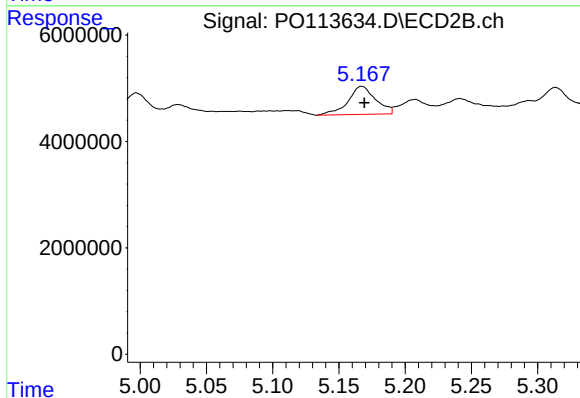


#15 AR-1232-5

R.T.: 5.167 min
Delta R.T.: -0.002 min
Response: 7669972
Conc: 113.43 ng/ml

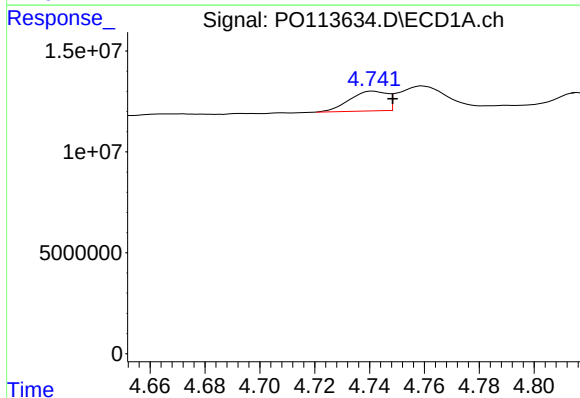


#16 AR-1242-1

R.T.: 4.741 min
Delta R.T.: -0.007 min
Response: 9219200
Conc: 40.10 ng/ml

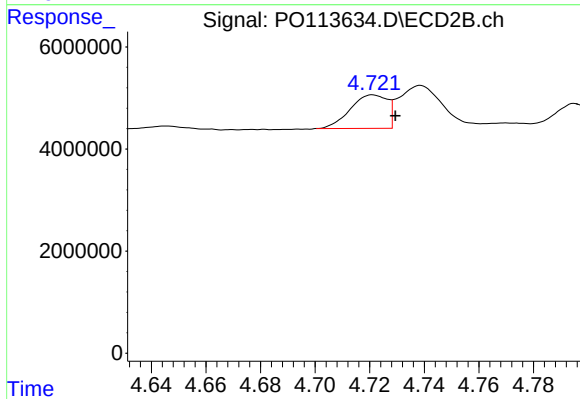

#16 AR-1242-1


R.T.: 4.721 min
Delta R.T.: -0.008 min
Response: 6179911
Conc: 42.77 ng/ml

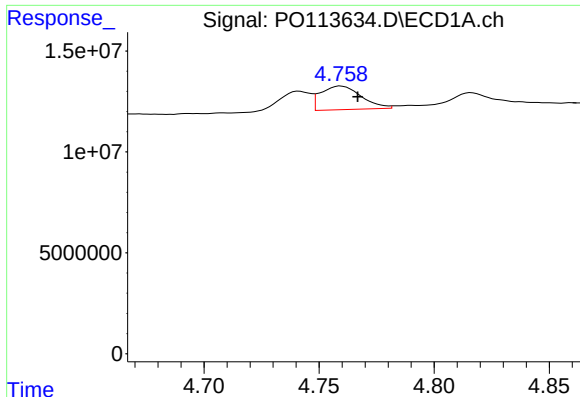

#17 AR-1242-2


R.T.: 4.760 min
Delta R.T.: -0.007 min
Response: 14305357
Conc: 41.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

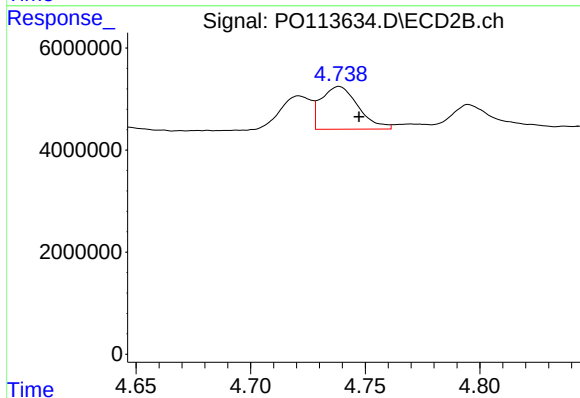


#17 AR-1242-2

R.T.: 4.739 min
Delta R.T.: -0.009 min
Response: 9406278
Conc: 43.36 ng/ml

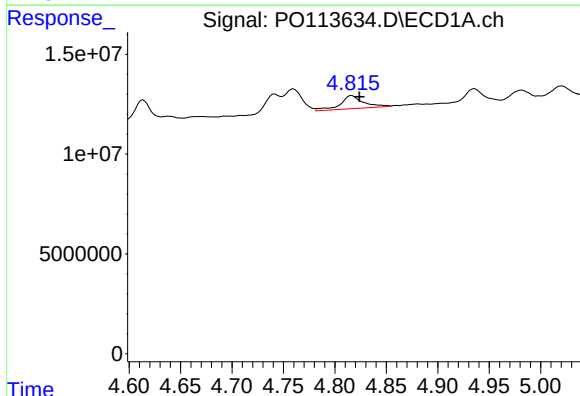


#18 AR-1242-3

R.T.: 4.816 min
Delta R.T.: -0.008 min
Response: 10173251
Conc: 45.85 ng/ml

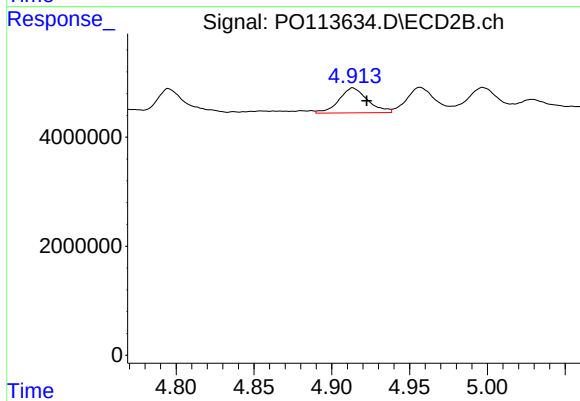

#18 AR-1242-3


R.T.: 4.914 min
Delta R.T.: -0.009 min
Response: 5860061
Conc: 50.10 ng/ml

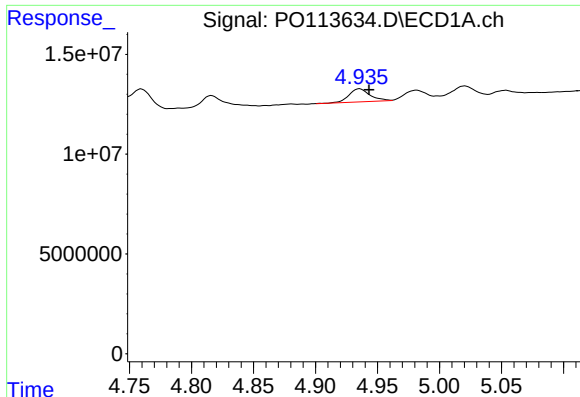

#19 AR-1242-4


R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 7744252
Conc: 44.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

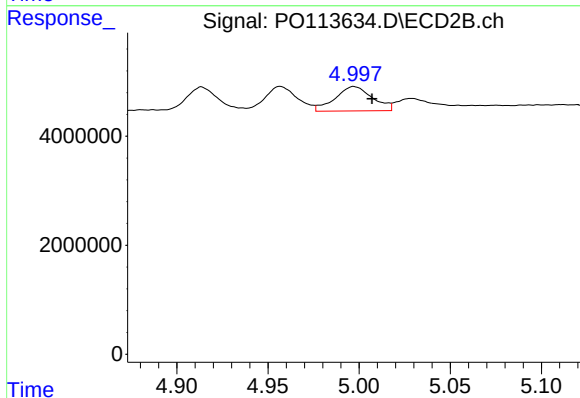


#19 AR-1242-4

R.T.: 4.997 min
Delta R.T.: -0.010 min
Response: 6391763
Conc: 54.33 ng/ml

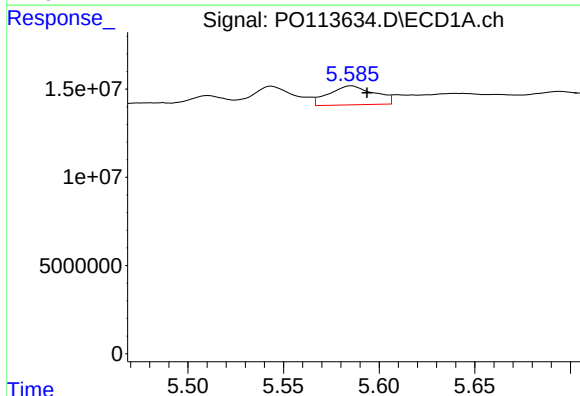


#20 AR-1242-5

R.T.: 5.585 min
Delta R.T.: -0.008 min
Response: 17870203
Conc: 89.28 ng/ml

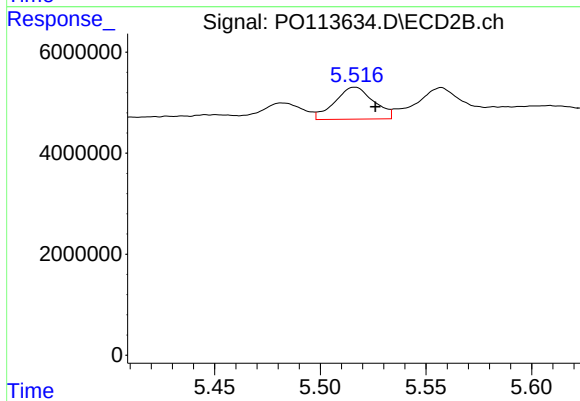

#20 AR-1242-5


R.T.: 5.516 min
Delta R.T.: -0.010 min
Response: 8105786
Conc: 54.35 ng/ml

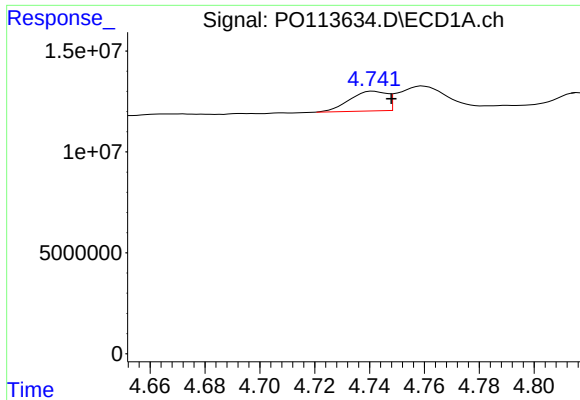

#21 AR-1248-1


R.T.: 4.741 min
Delta R.T.: -0.007 min
Response: 9219200
Conc: 52.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

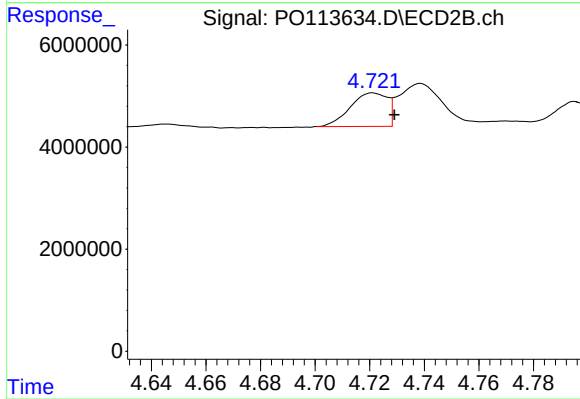


#21 AR-1248-1

R.T.: 4.721 min
Delta R.T.: -0.008 min
Response: 6179911
Conc: 55.42 ng/ml

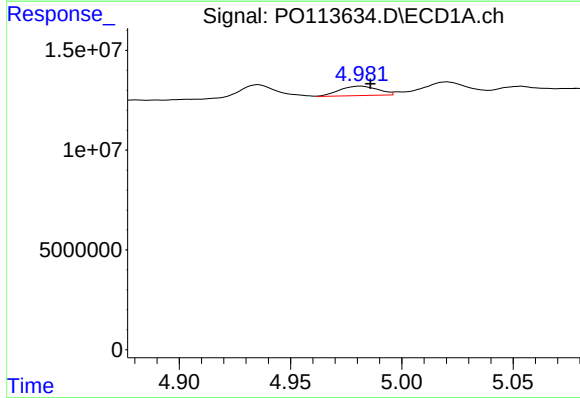


#22 AR-1248-2

R.T.: 4.981 min
Delta R.T.: -0.004 min
Response: 5675034
Conc: 23.46 ng/ml

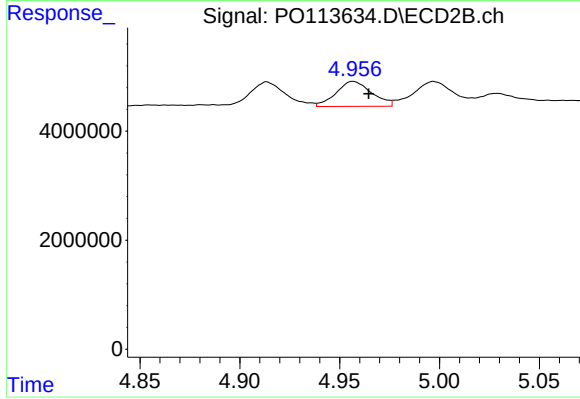

#22 AR-1248-2


R.T.: 4.957 min
Delta R.T.: -0.008 min
Response: 5679794
Conc: 35.34 ng/ml

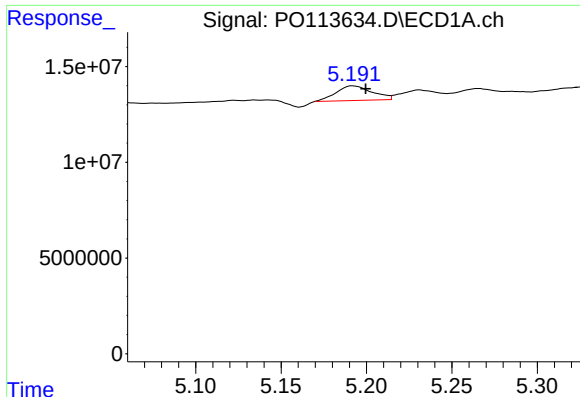

#23 AR-1248-3


R.T.: 5.192 min
Delta R.T.: -0.007 min
Response: 11197672
Conc: 35.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

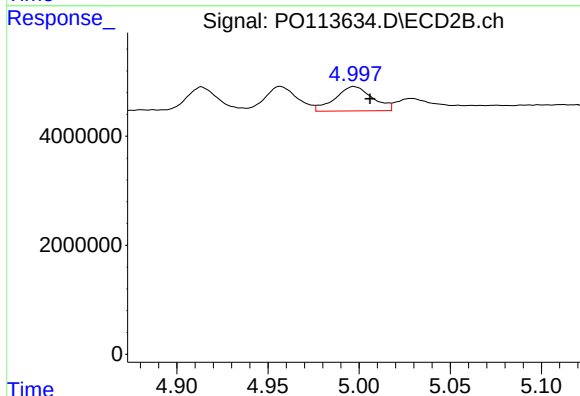


#23 AR-1248-3

R.T.: 4.997 min
Delta R.T.: -0.009 min
Response: 6391763
Conc: 37.67 ng/ml

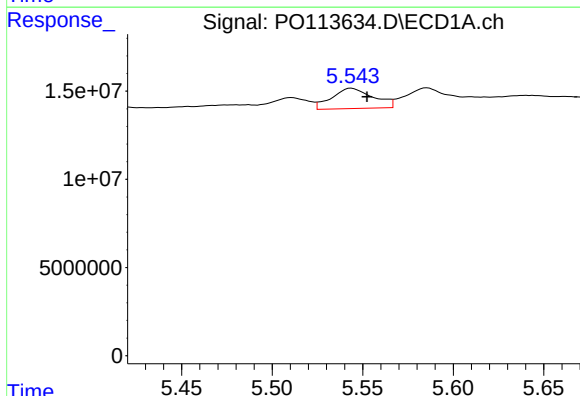


#24 AR-1248-4

R.T.: 5.544 min
Delta R.T.: -0.009 min
Response: 18288935
Conc: 36.61 ng/ml

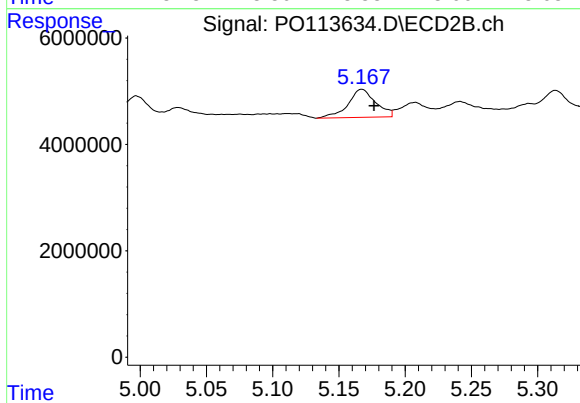

#24 AR-1248-4


R.T.: 5.167 min
Delta R.T.: -0.009 min
Response: 7669972
Conc: 38.50 ng/ml

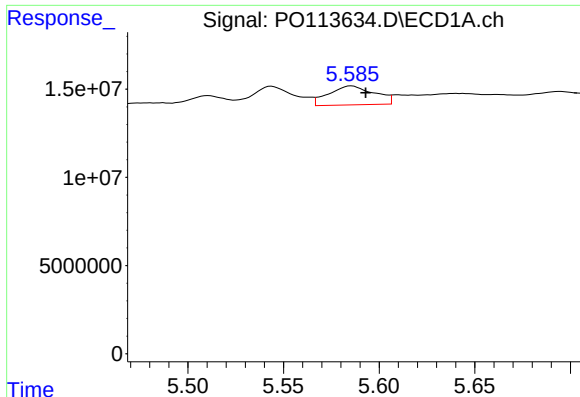

#25 AR-1248-5


R.T.: 5.585 min
Delta R.T.: -0.008 min
Response: 17870203
Conc: 52.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

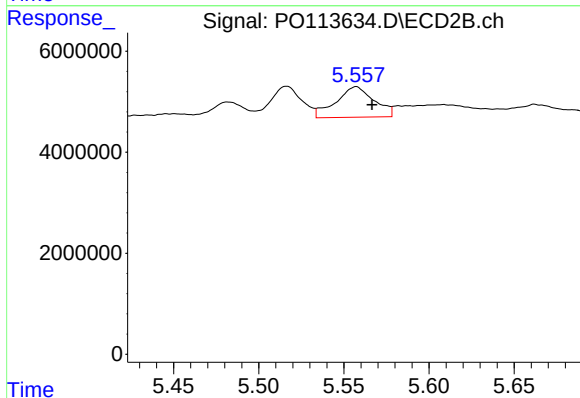


#25 AR-1248-5

R.T.: 5.557 min
Delta R.T.: -0.009 min
Response: 9443870
Conc: 44.48 ng/ml

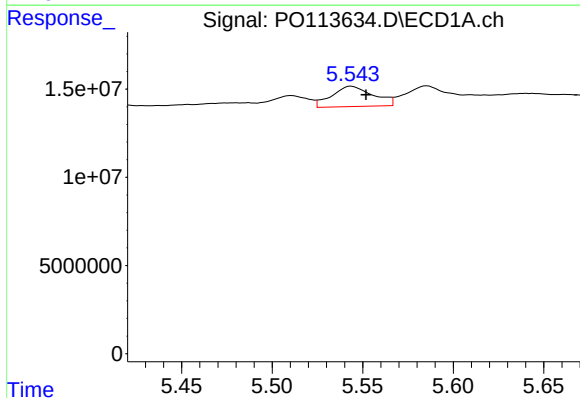


#26 AR-1254-1

R.T.: 5.544 min
Delta R.T.: -0.008 min
Response: 18288935
Conc: 33.87 ng/ml

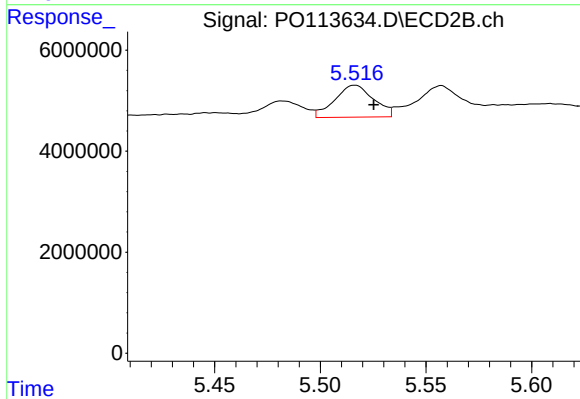

#26 AR-1254-1


R.T.: 5.516 min
Delta R.T.: -0.009 min
Response: 8105786
Conc: 25.70 ng/ml

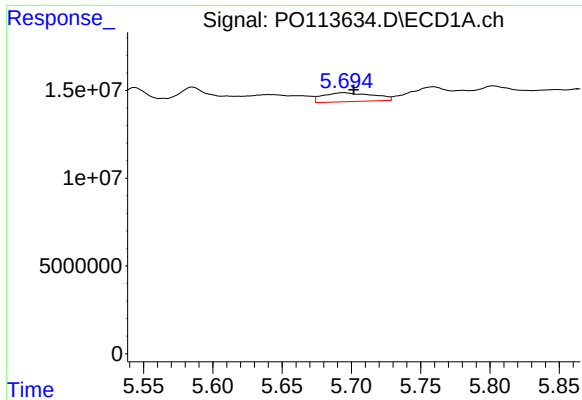

#27 AR-1254-2


R.T.: 5.695 min
Delta R.T.: -0.007 min
Response: 12830814
Conc: 26.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

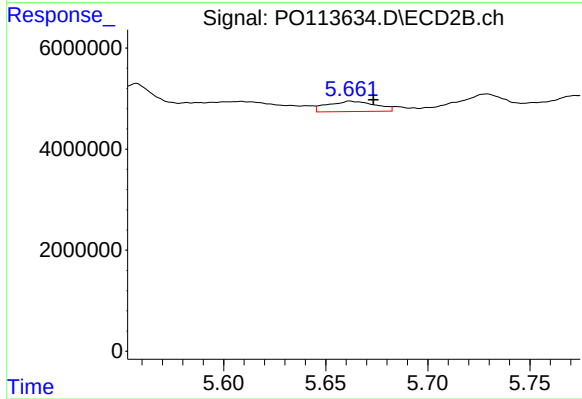


#27 AR-1254-2

R.T.: 5.662 min
Delta R.T.: -0.011 min
Response: 3336780
Conc: 11.90 ng/ml

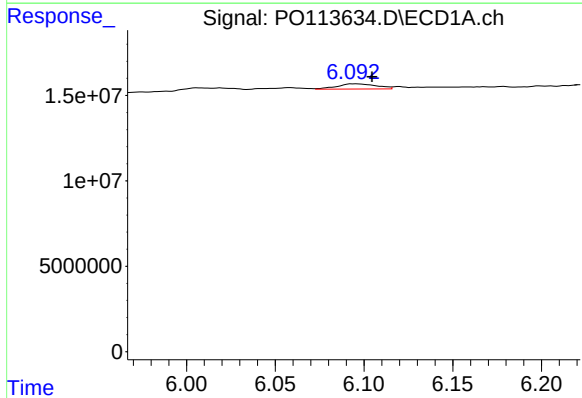


#28 AR-1254-3

R.T.: 6.095 min
Delta R.T.: -0.009 min
Response: 4686587
Conc: 6.34 ng/ml

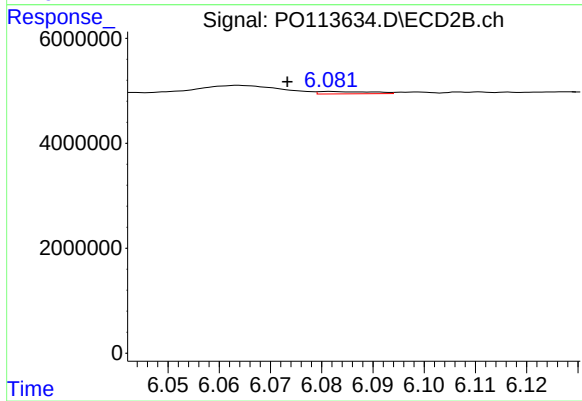

#28 AR-1254-3


R.T.: 6.082 min
Delta R.T.: 0.008 min
Response: 325759
Conc: 0.78 ng/ml

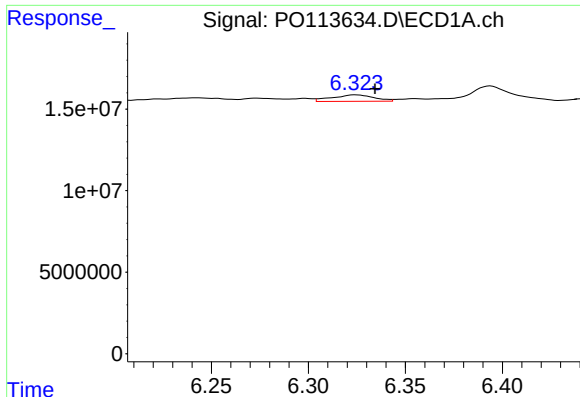

#29 AR-1254-4


R.T.: 6.324 min
Delta R.T.: -0.010 min
Response: 5908674
Conc: 10.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

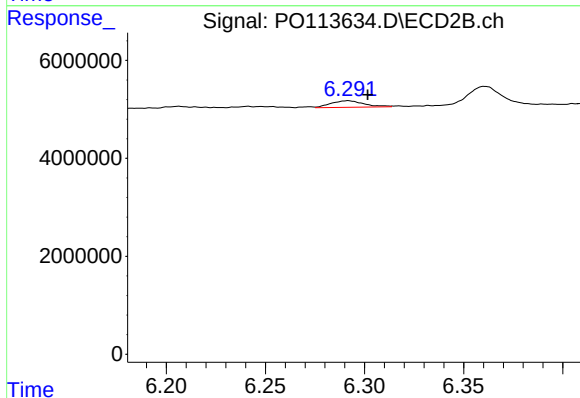


#29 AR-1254-4

R.T.: 6.292 min
Delta R.T.: -0.010 min
Response: 1539996
Conc: 5.60 ng/ml

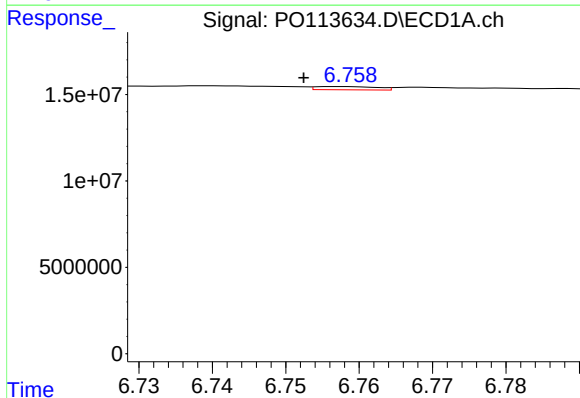


#30 AR-1254-5

R.T.: 6.758 min
Delta R.T.: 0.005 min
Response: 1113307
Conc: 1.59 ng/ml

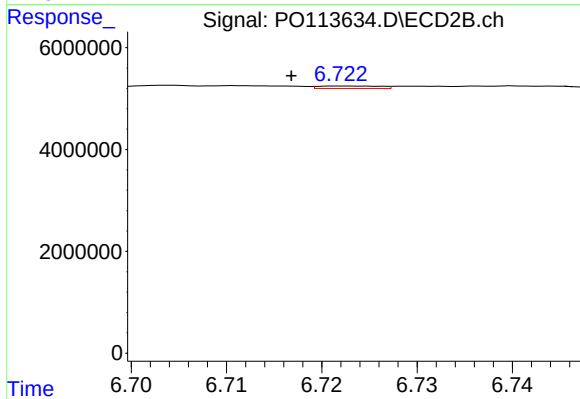

#30 AR-1254-5


R.T.: 6.722 min
Delta R.T.: 0.005 min
Response: 210690
Conc: 0.59 ng/ml

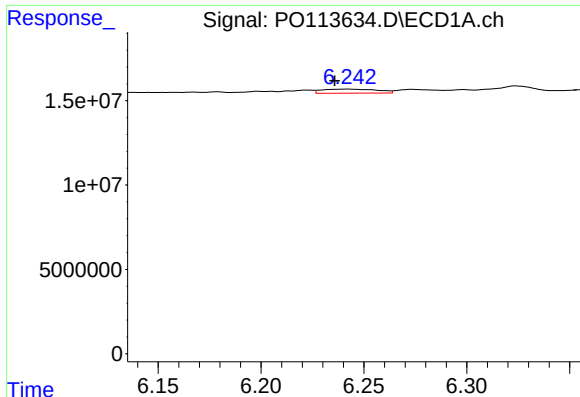

#31 AR-1260-1


R.T.: 6.242 min
Delta R.T.: 0.006 min
Response: 4611089
Conc: 10.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

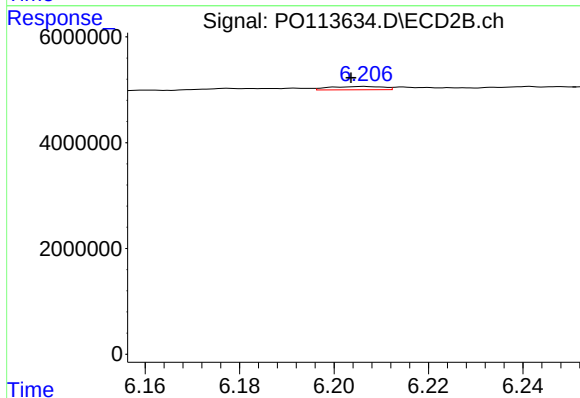


#31 AR-1260-1

R.T.: 6.206 min
Delta R.T.: 0.003 min
Response: 487708
Conc: 1.91 ng/ml

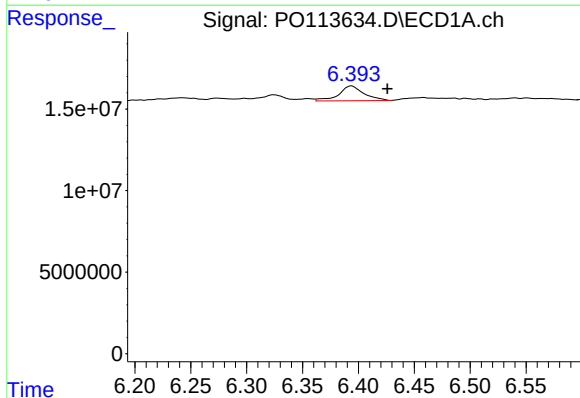


#32 AR-1260-2

R.T.: 6.394 min
Delta R.T.: -0.032 min
Response: 14153808
Conc: 20.61 ng/ml

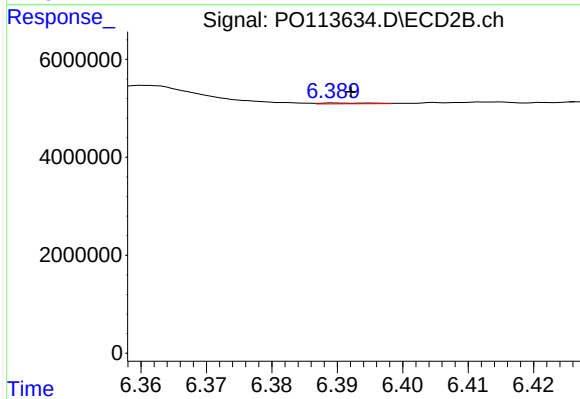

#32 AR-1260-2


R.T.: 6.390 min
Delta R.T.: -0.002 min
Response: 92900
Conc: 0.27 ng/ml

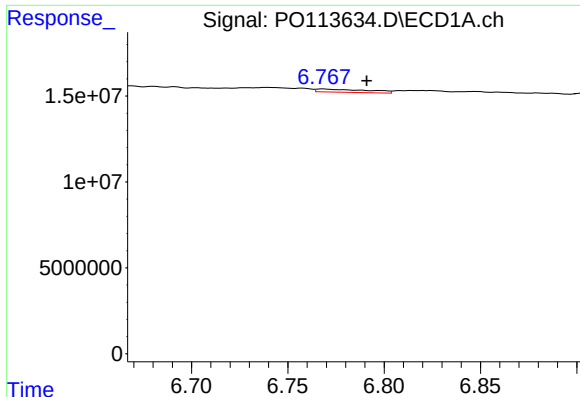

#33 AR-1260-3


R.T.: 6.768 min
Delta R.T.: -0.023 min
Response: 3430783
Conc: 5.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

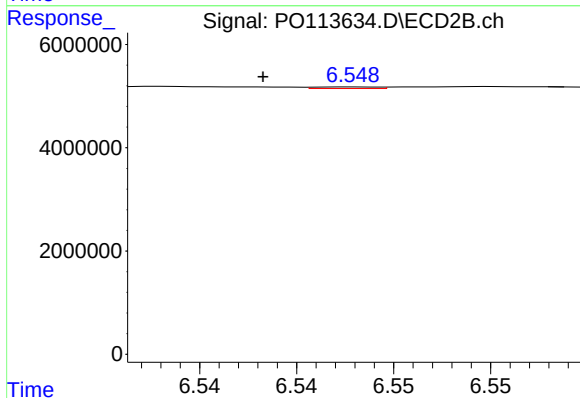


#33 AR-1260-3

R.T.: 6.548 min
Delta R.T.: 0.005 min
Response: 68655
Conc: 0.23 ng/ml

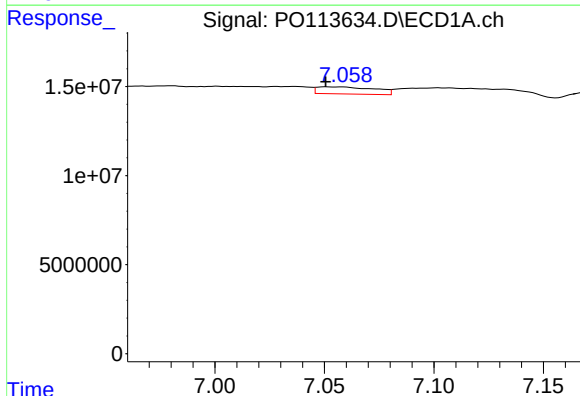


#34 AR-1260-4

R.T.: 7.051 min
Delta R.T.: 0.000 min
Response: 7254042
Conc: 16.20 ng/ml

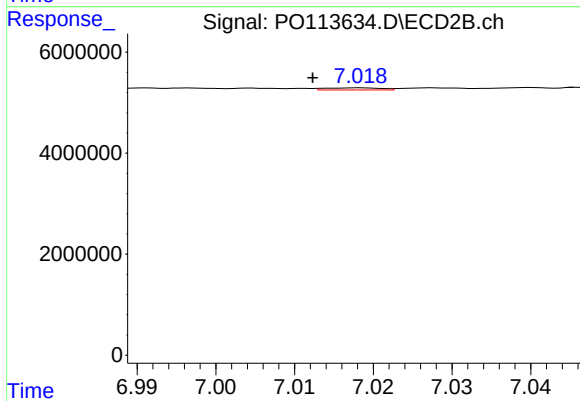

#34 AR-1260-4


R.T.: 7.018 min
Delta R.T.: 0.006 min
Response: 210566
Conc: 1.02 ng/ml

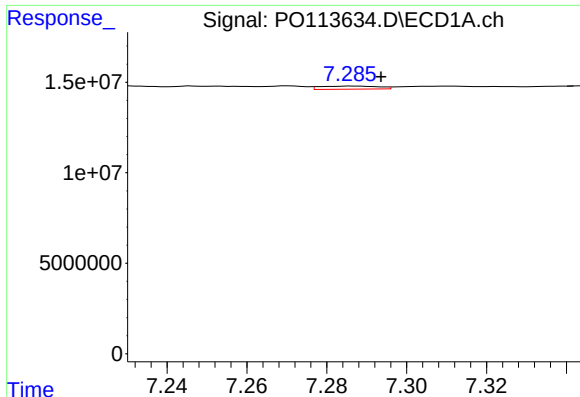

#35 AR-1260-5


R.T.: 7.287 min
Delta R.T.: -0.007 min
Response: 1748969
Conc: 1.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

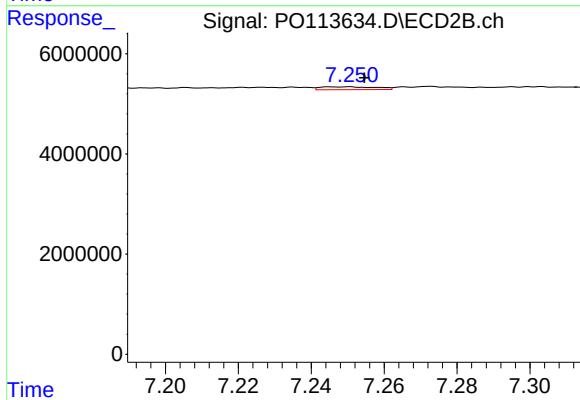


#35 AR-1260-5

R.T.: 7.250 min
Delta R.T.: -0.004 min
Response: 621843
Conc: 1.33 ng/ml

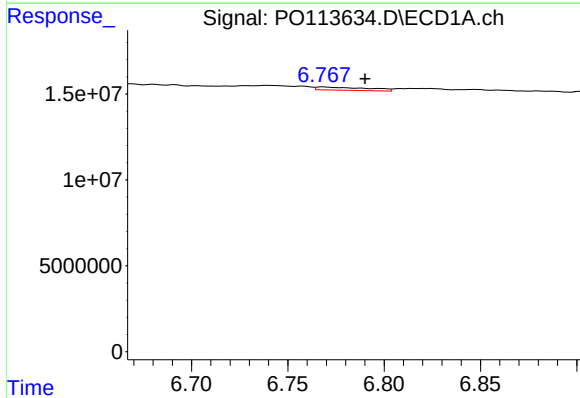


#36 AR-1262-1

R.T.: 6.768 min
Delta R.T.: -0.022 min
Response: 3430783
Conc: 3.75 ng/ml

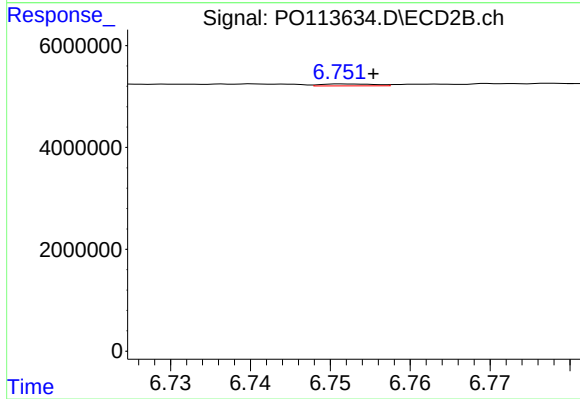

#36 AR-1262-1


R.T.: 6.752 min
Delta R.T.: -0.004 min
Response: 185087
Conc: 0.45 ng/ml

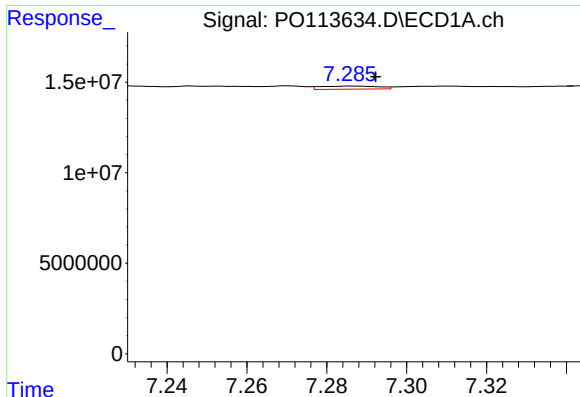

#37 AR-1262-2


R.T.: 7.287 min
Delta R.T.: -0.005 min
Response: 1748969
Conc: 1.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

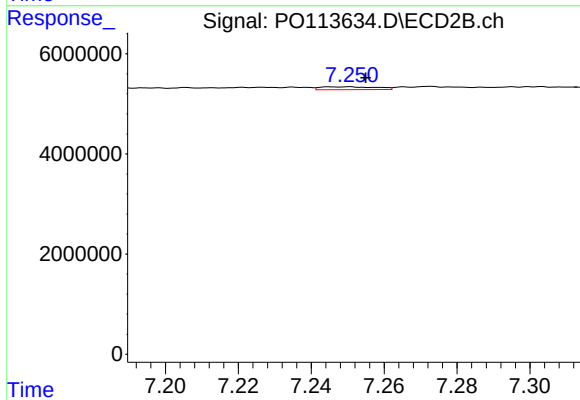


#37 AR-1262-2

R.T.: 7.250 min
Delta R.T.: -0.005 min
Response: 621843
Conc: 1.20 ng/ml

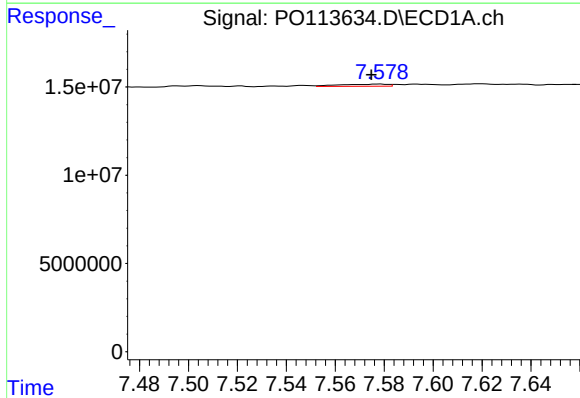


#38 AR-1262-3

R.T.: 7.578 min
Delta R.T.: 0.003 min
Response: 1732707
Conc: 3.13 ng/ml

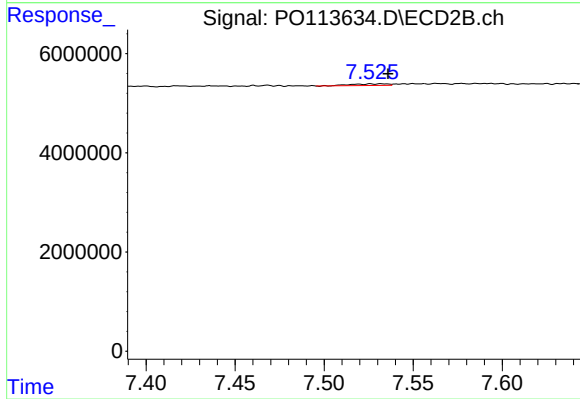

#38 AR-1262-3


R.T.: 7.526 min
Delta R.T.: -0.010 min
Response: 465509
Conc: 2.59 ng/ml

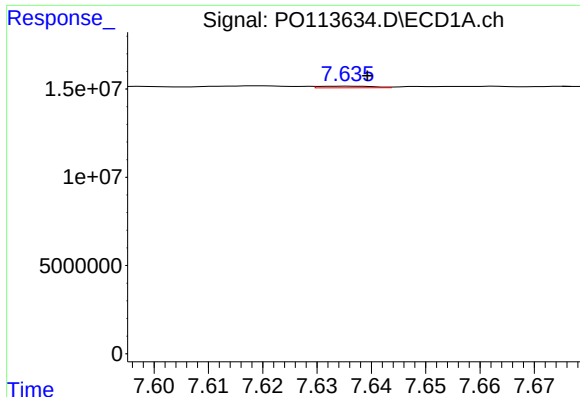

#39 AR-1262-4


R.T.: 7.636 min
Delta R.T.: -0.004 min
Response: 634223
Conc: 0.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

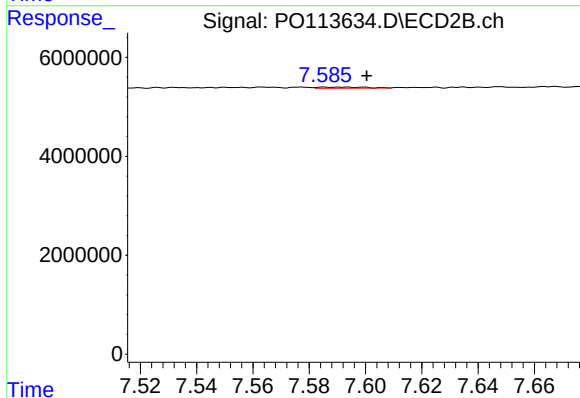


#39 AR-1262-4

R.T.: 7.585 min
Delta R.T.: -0.015 min
Response: 285028
Conc: 0.98 ng/ml

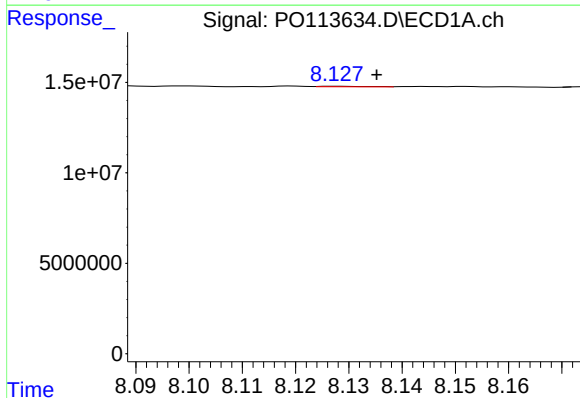


#40 AR-1262-5

R.T.: 8.128 min
Delta R.T.: -0.007 min
Response: 212776
Conc: 0.51 ng/ml

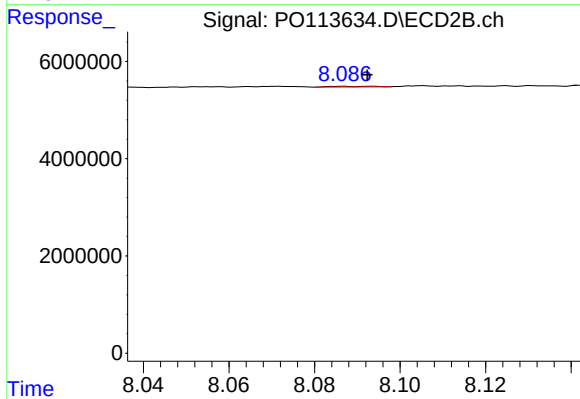

#40 AR-1262-5


R.T.: 8.093 min
Delta R.T.: 0.000 min
Response: 111385
Conc: 1.03 ng/ml

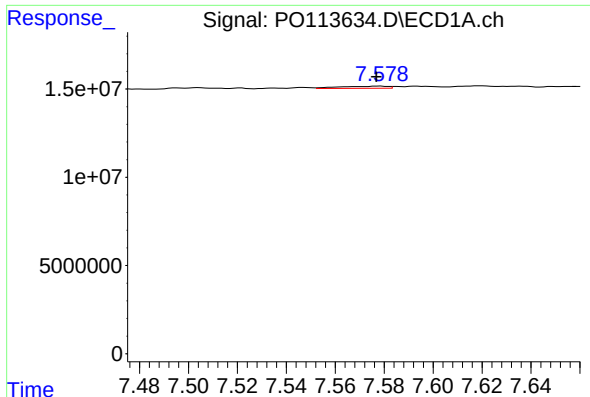

#41 AR-1268-1


R.T.: 7.578 min
Delta R.T.: 0.001 min
Response: 1732707
Conc: 1.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

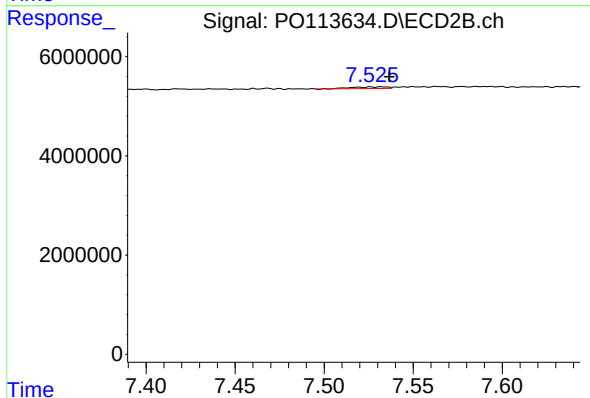


#41 AR-1268-1

R.T.: 7.526 min
Delta R.T.: -0.011 min
Response: 465509
Conc: 0.91 ng/ml

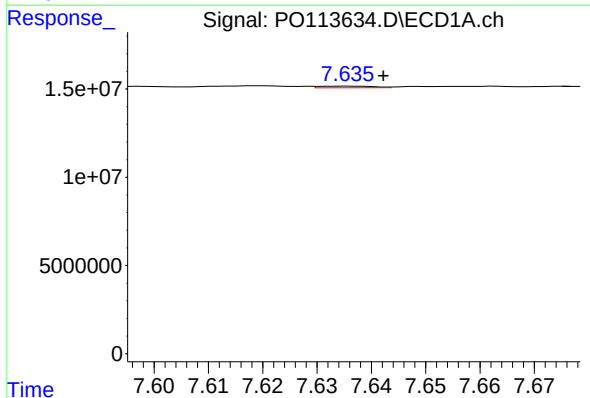


#42 AR-1268-2

R.T.: 7.636 min
Delta R.T.: -0.007 min
Response: 634223
Conc: 0.44 ng/ml

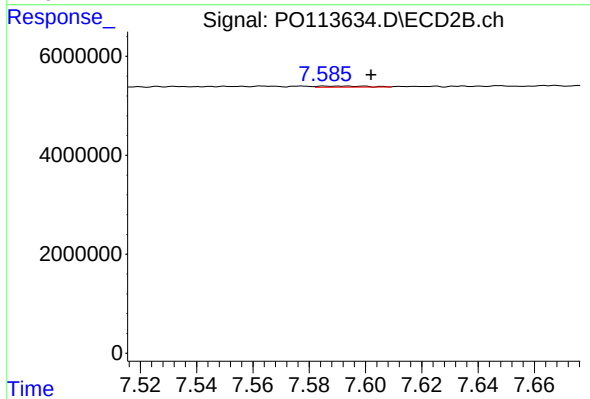

#42 AR-1268-2


R.T.: 7.585 min
Delta R.T.: -0.017 min
Response: 285028
Conc: 0.69 ng/ml

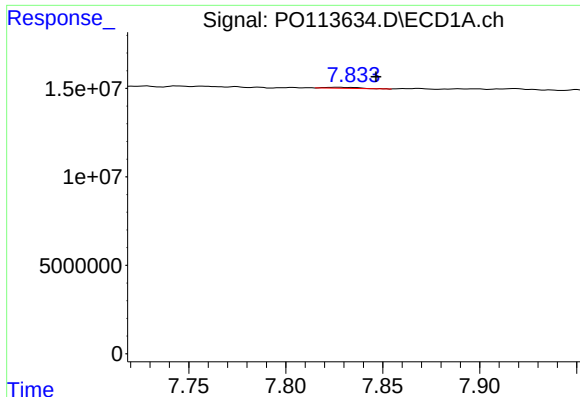

#43 AR-1268-3


R.T.: 7.827 min
Delta R.T.: -0.019 min
Response: 724598
Conc: 0.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

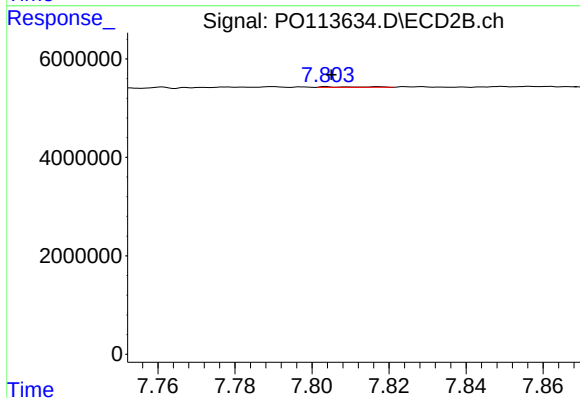


#43 AR-1268-3

R.T.: 7.804 min
Delta R.T.: -0.001 min
Response: 94645
Conc: 0.29 ng/ml

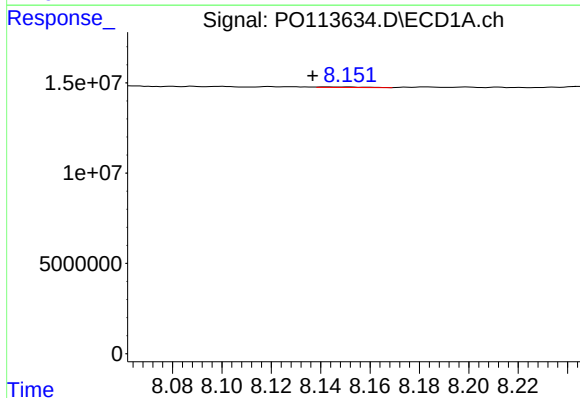


#44 AR-1268-4

R.T.: 8.143 min
Delta R.T.: 0.006 min
Response: 392091
Conc: 0.85 ng/ml

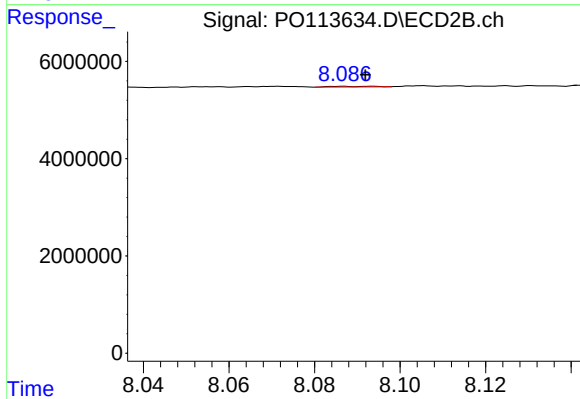

#44 AR-1268-4


R.T.: 8.093 min
Delta R.T.: 0.001 min
Response: 111385
Conc: 0.92 ng/ml

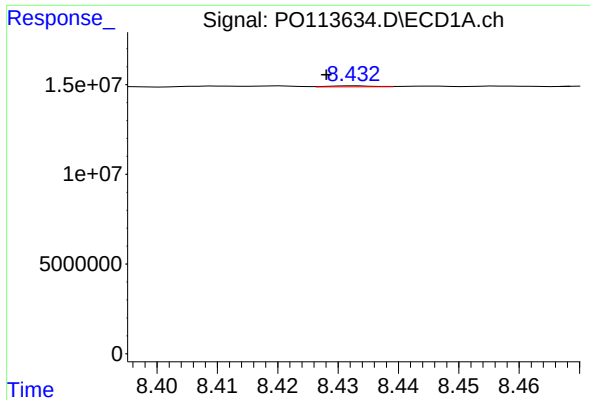

#45 AR-1268-5

R.T.: 8.433 min
Delta R.T.: 0.005 min
Response: 298312
Conc: 0.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

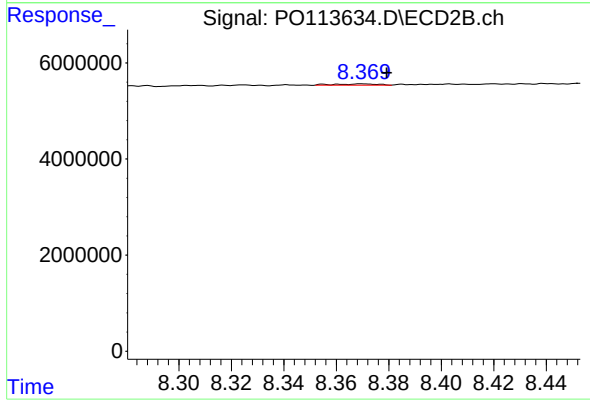

#45 AR-1268-5

R.T.: 8.370 min
Delta R.T.: -0.009 min
Response: 281812
Conc: 0.36 ng/ml