

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
 Data File : P0113635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 03:20
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1248 WATER LOD 40PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:30:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.658	3.649	180.5E6	105.9E6	22.050	20.924
2)	SA Decachlor...	8.669	8.614	151.5E6	43570276	21.862	22.994
Target Compounds							
3)	L1 AR-1016-1	4.741	4.721	7036614	4808403	26.356	28.190
4)	L1 AR-1016-2	4.760	4.739	7596185	4796623	18.923	18.616
5)	L1 AR-1016-3	4.818	4.915	3756385	4325690	14.730	30.983 #
6)	L1 AR-1016-4	4.937	4.956	5358702	8296940	24.574	71.097 #
7)	L1 AR-1016-5	5.192	5.167	17780788	10983633	80.228	77.062
8)	L2 AR-1221-1	3.885	3.867	211005	118785	2.255	1.882
9)	L2 AR-1221-2	3.958	3.944	1981840	2421280	29.339	51.877 #
10)	L2 AR-1221-3	4.036	4.014	509601	360933	2.302	2.431
11)	L3 AR-1232-1	4.036	4.014	509601	360933	2.839	2.985
12)	L3 AR-1232-2	4.519	4.739	4469927	4796623	41.420	39.301
13)	L3 AR-1232-3	4.760	4.915	7596185	4325690	38.482	65.386 #
14)	L3 AR-1232-4	4.937	4.996	5358702	8456969	54.517	141.118 #
15)	L3 AR-1232-5	4.979	5.167	10208937	10983633	155.193	162.441
16)	L4 AR-1242-1	4.741	4.721	7036614	4808403	30.603	33.275
17)	L4 AR-1242-2	4.760	4.739	7596185	4796623	22.106	22.113
18)	L4 AR-1242-3	4.818	4.915	3756385	4325690	16.929	36.983 #
19)	L4 AR-1242-4	4.937	4.996	5358702	8456969	30.893	71.890 #
20)	L4 AR-1242-5	5.586	5.517	25757341	14361961	128.682	96.303 #
21)	L5 AR-1248-1	4.741	4.721	7036614	4808403	40.332	43.120
22)	L5 AR-1248-2	4.979	4.956	10208937	8296940	42.209	51.630
23)	L5 AR-1248-3	5.192	4.996	17780788	8456969	55.763	49.846
24)	L5 AR-1248-4	5.544	5.167	28422700	10983633	56.890	55.133
25)	L5 AR-1248-5	5.586	5.557	25757341	12436310	75.426	58.580
26)	L6 AR-1254-1	5.544	5.517	28422700	14361961	52.637	45.542
27)	L6 AR-1254-2	5.694	5.665	16289437	6275905	33.011	22.387 #
28)	L6 AR-1254-3	6.097	6.064	9860923	5413577	13.346	12.985
29)	L6 AR-1254-4	6.325	6.292	7654188	3552286	13.742	12.925
30)	L6 AR-1254-5	6.744	6.710	3498108	1537137	4.990	4.300
31)	L7 AR-1260-1	6.240	6.205	6592308	2850778	14.782	11.177
32)	L7 AR-1260-2	6.435	6.361	150653	4904384	0.219	14.186 #
33)	L7 AR-1260-3	6.783	6.550	2475551	188424	4.009	0.633 #
34)	L7 AR-1260-4	7.061	7.015	3189332	211060	7.121	1.018 #
35)	L7 AR-1260-5	7.282	7.257	3183565	354910	2.630	0.758 #
36)	L8 AR-1262-1	6.783	6.737	2475551	565844	2.703	1.365 #
37)	L8 AR-1262-2	7.282	7.257	3183565	354910	2.105	0.686 #
38)	L8 AR-1262-3	7.574	7.537	398193	258093	0.719	1.437 #
39)	L8 AR-1262-4	7.632	7.612	1775562	58335	1.816	0.201 #
40)	L8 AR-1262-5	8.134	8.089	488499	81339	1.172	0.751 #
41)	L9 AR-1268-1	7.574	7.537	398193	258093	0.231	0.507 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
Data File : P0113635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 03:20
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1248 WATER LOD 40PPB
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:30:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.651	7.612	730571	58335	0.504	0.140 #
43)	L9 AR-1268-3	7.861	7.809	79599	72944	0.066	0.223 #
44)	L9 AR-1268-4	8.134	8.089	488499	81339	1.060	0.675 #
45)	L9 AR-1268-5	8.438	8.382	96706	17600	0.030	0.023 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091025\
Data File : PO113635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 03:20
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1248 WATER LOD 40PPB
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:30:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

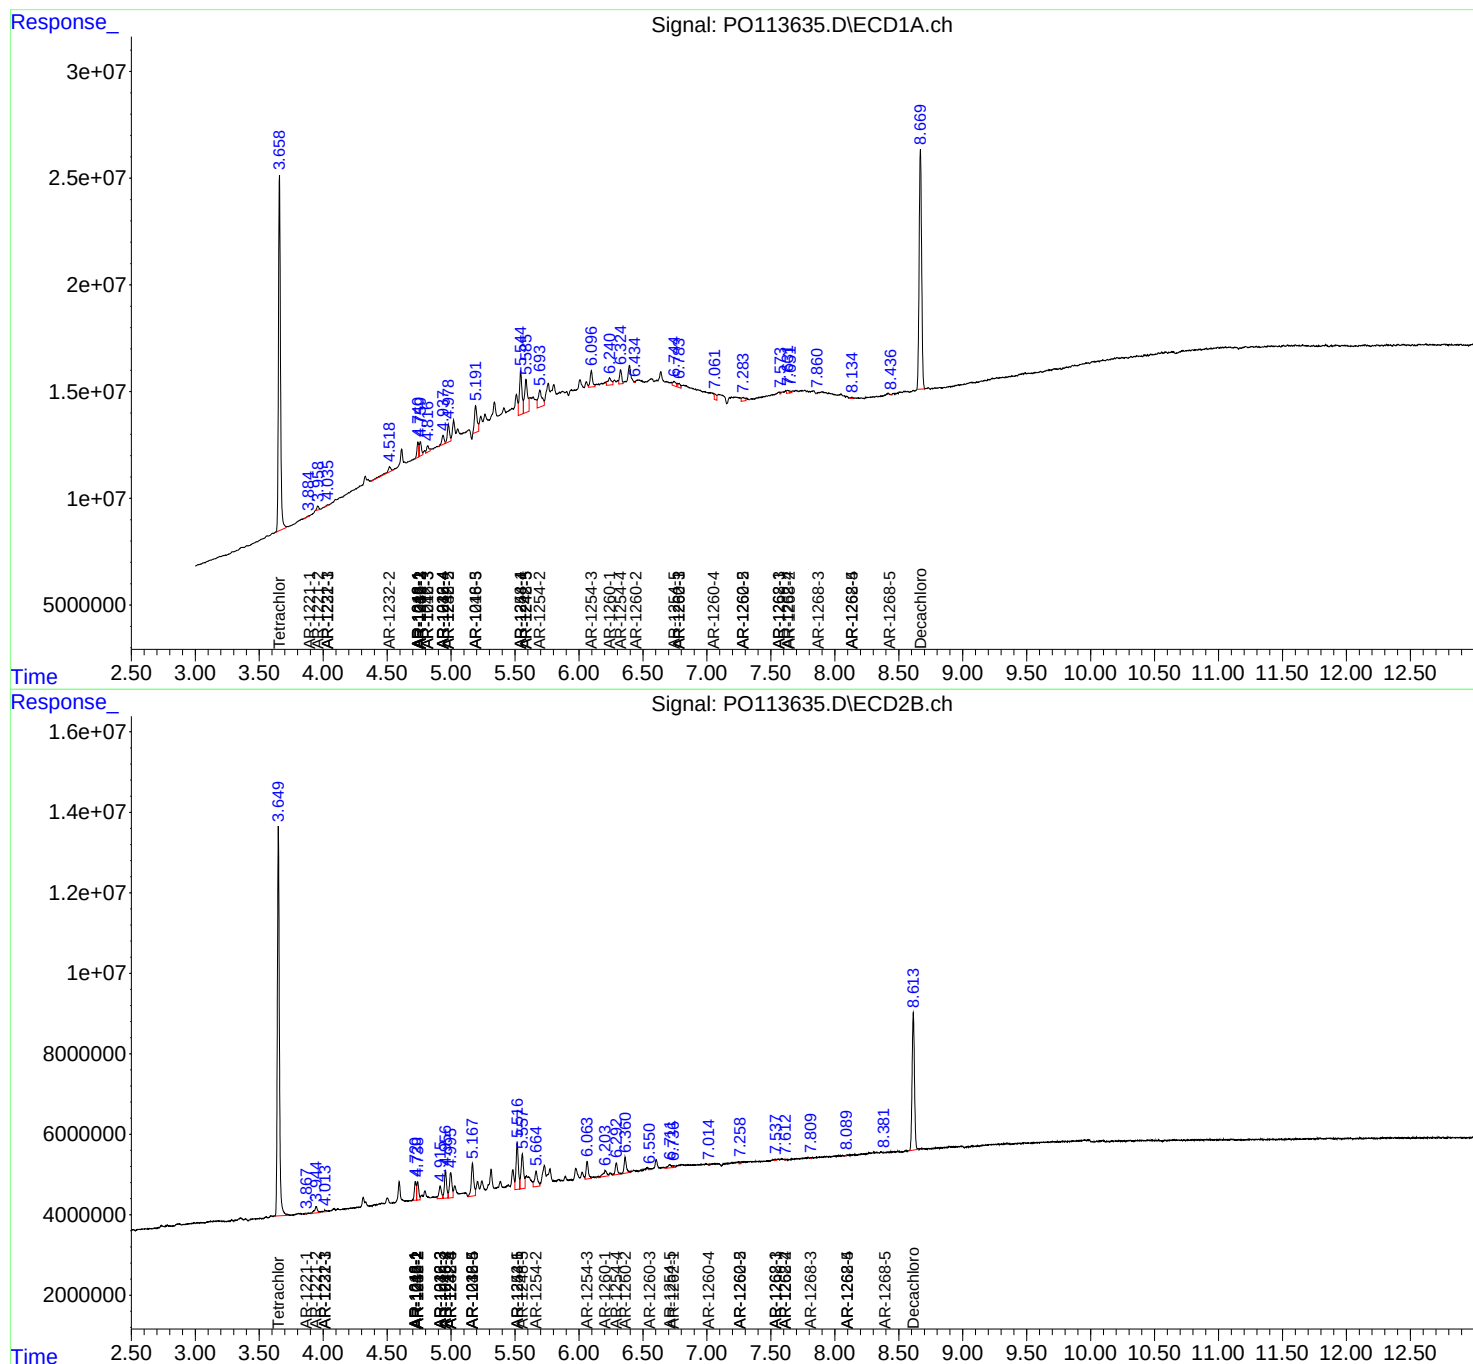


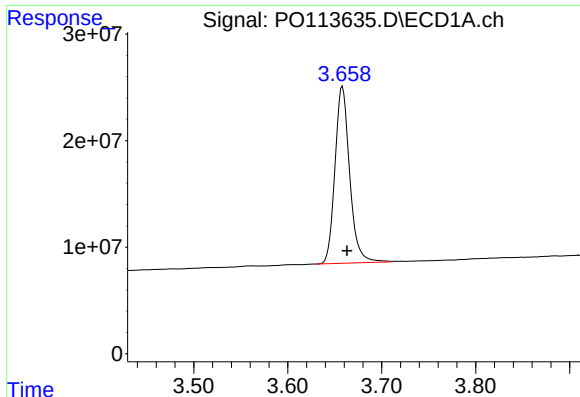

#1 Tetrachloro-m-xylene


R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 180514122
Conc: 22.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

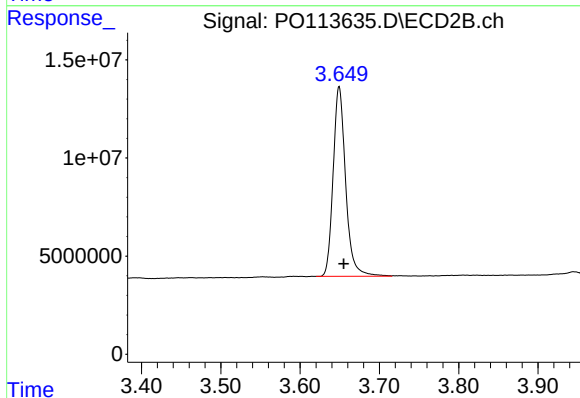


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.006 min
Response: 105890974
Conc: 20.92 ng/ml

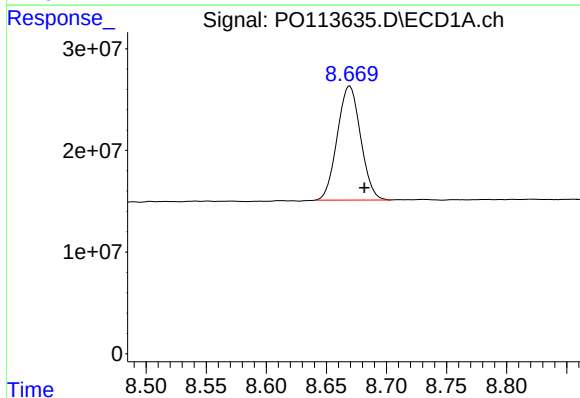


#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.012 min
Response: 151533459
Conc: 21.86 ng/ml

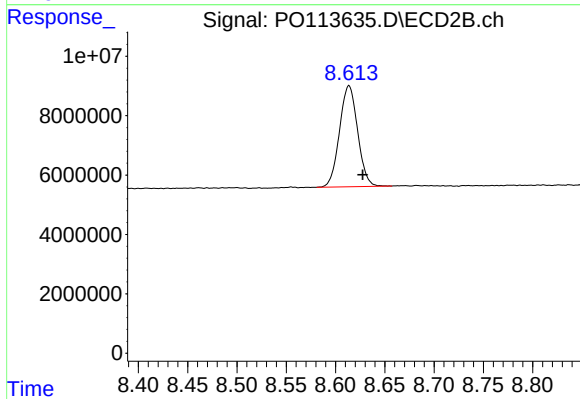

#2 Decachlorobiphenyl


R.T.: 8.614 min
Delta R.T.: -0.014 min
Response: 43570276
Conc: 22.99 ng/ml

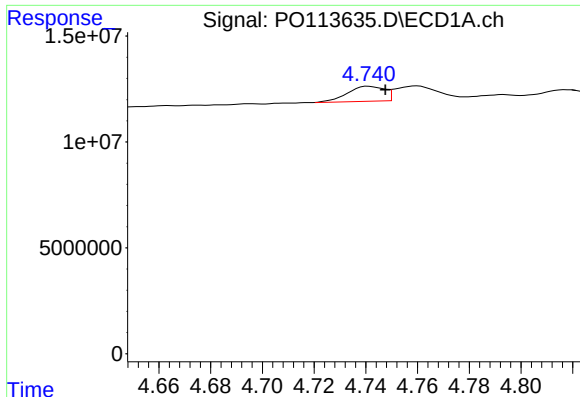

#3 AR-1016-1


R.T.: 4.741 min
Delta R.T.: -0.007 min
Response: 7036614
Conc: 26.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

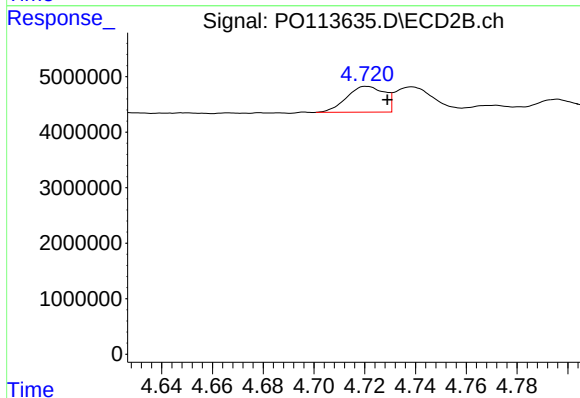


#3 AR-1016-1

R.T.: 4.721 min
Delta R.T.: -0.008 min
Response: 4808403
Conc: 28.19 ng/ml

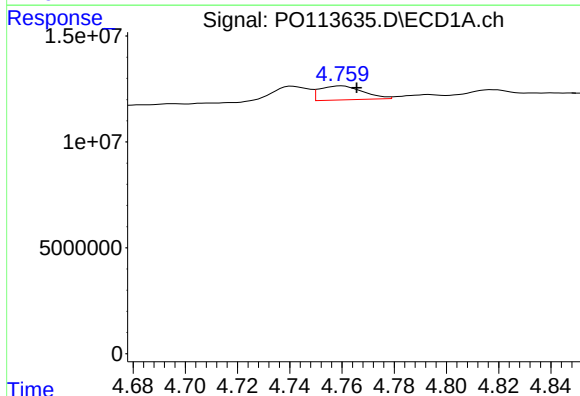


#4 AR-1016-2

R.T.: 4.760 min
Delta R.T.: -0.006 min
Response: 7596185
Conc: 18.92 ng/ml

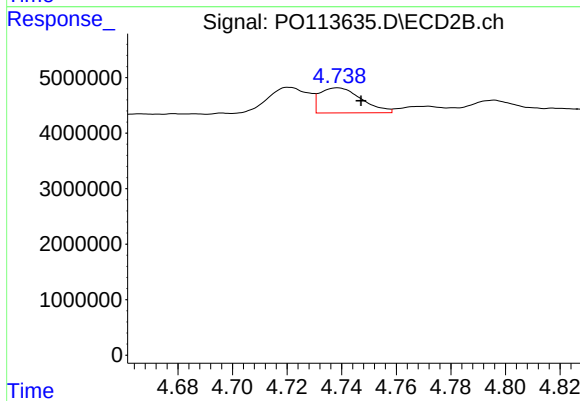

#4 AR-1016-2


R.T.: 4.739 min
Delta R.T.: -0.008 min
Response: 4796623
Conc: 18.62 ng/ml

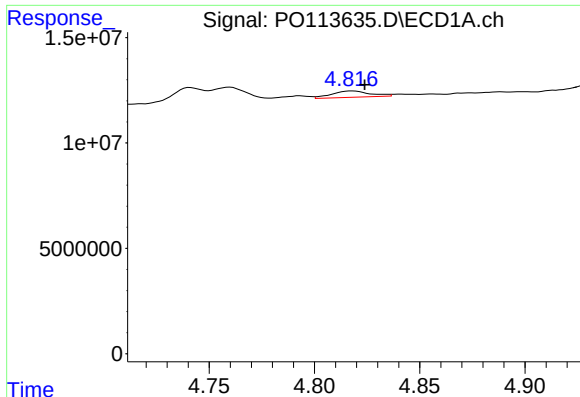

#5 AR-1016-3


R.T.: 4.818 min
Delta R.T.: -0.006 min
Response: 3756385
Conc: 14.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

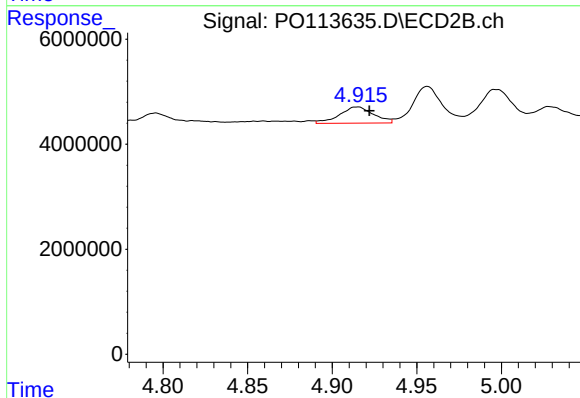


#5 AR-1016-3

R.T.: 4.915 min
Delta R.T.: -0.006 min
Response: 4325690
Conc: 30.98 ng/ml

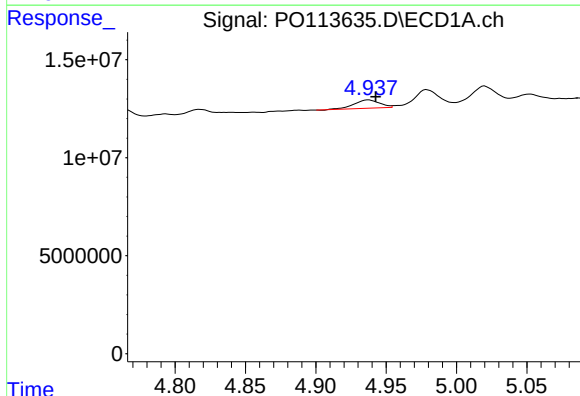


#6 AR-1016-4

R.T.: 4.937 min
Delta R.T.: -0.005 min
Response: 5358702
Conc: 24.57 ng/ml

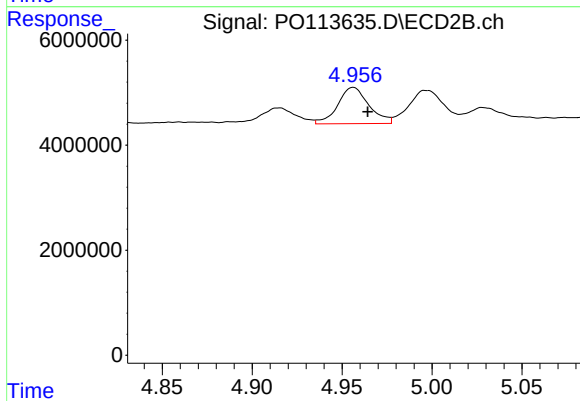

#6 AR-1016-4


R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 8296940
Conc: 71.10 ng/ml

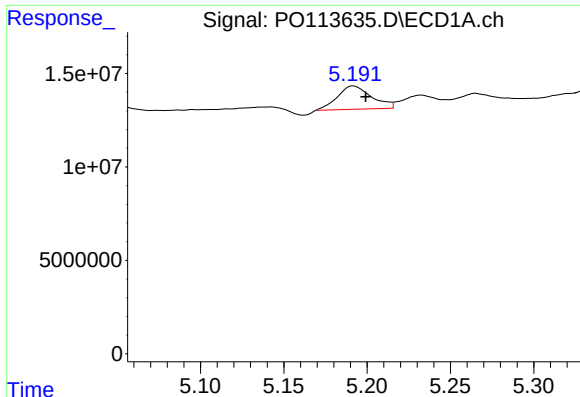

#7 AR-1016-5


R.T.: 5.192 min
Delta R.T.: -0.007 min
Response: 17780788
Conc: 80.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

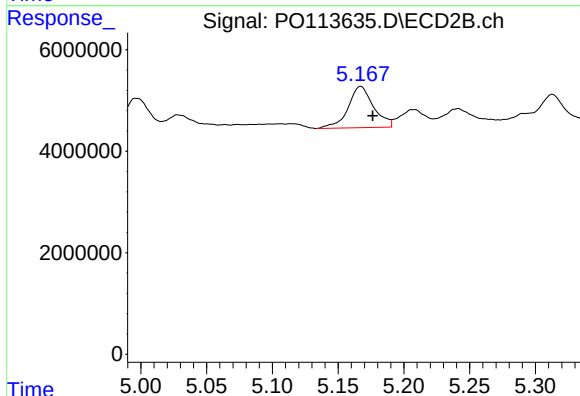


#7 AR-1016-5

R.T.: 5.167 min
Delta R.T.: -0.009 min
Response: 10983633
Conc: 77.06 ng/ml

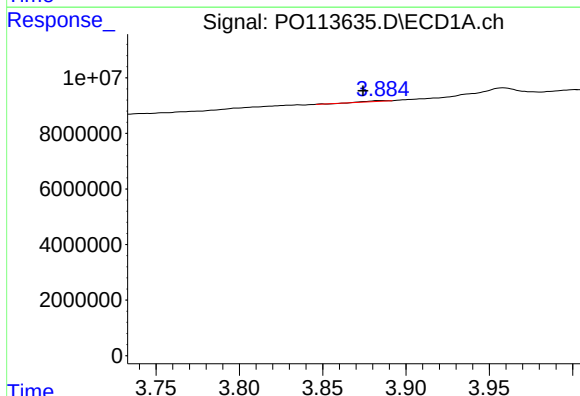


#8 AR-1221-1

R.T.: 3.885 min
Delta R.T.: 0.011 min
Response: 211005
Conc: 2.25 ng/ml

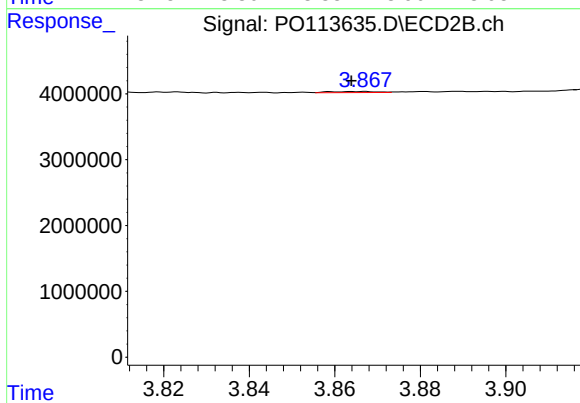

#8 AR-1221-1


R.T.: 3.867 min
Delta R.T.: 0.003 min
Response: 118785
Conc: 1.88 ng/ml

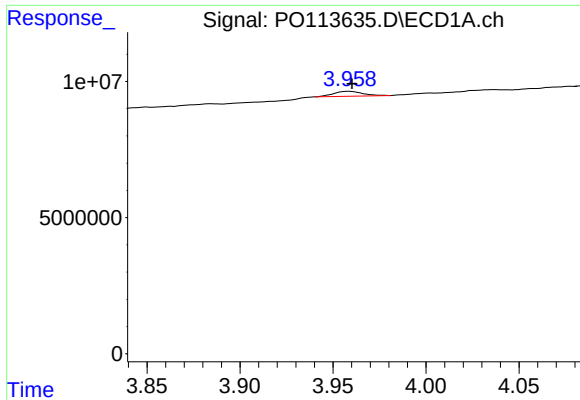

#9 AR-1221-2


R.T.: 3.958 min
Delta R.T.: -0.002 min
Response: 1981840
Conc: 29.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

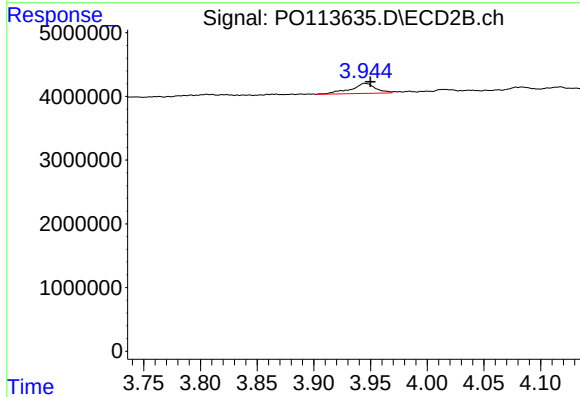


#9 AR-1221-2

R.T.: 3.944 min
Delta R.T.: -0.005 min
Response: 2421280
Conc: 51.88 ng/ml

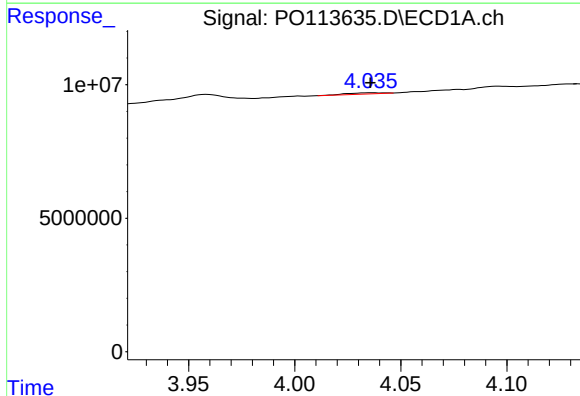


#10 AR-1221-3

R.T.: 4.036 min
Delta R.T.: 0.000 min
Response: 509601
Conc: 2.30 ng/ml

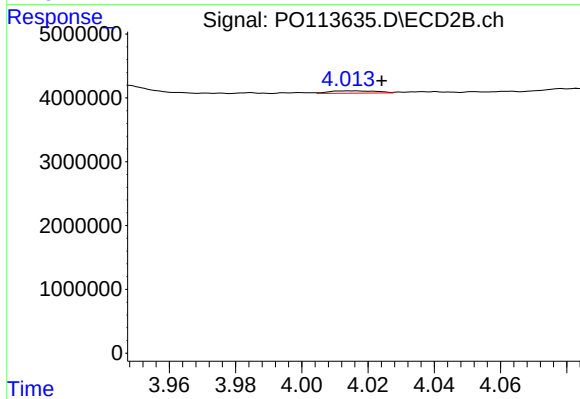

#10 AR-1221-3


R.T.: 4.014 min
Delta R.T.: -0.010 min
Response: 360933
Conc: 2.43 ng/ml

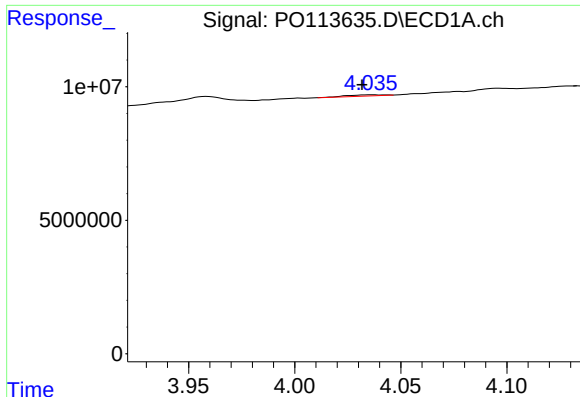

#11 AR-1232-1


R.T.: 4.036 min
Delta R.T.: 0.004 min
Response: 509601
Conc: 2.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

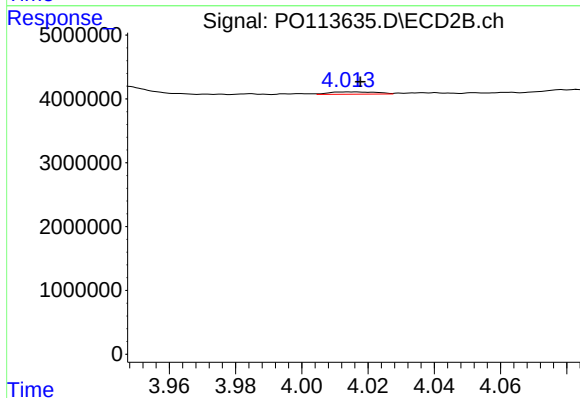


#11 AR-1232-1

R.T.: 4.014 min
Delta R.T.: -0.003 min
Response: 360933
Conc: 2.98 ng/ml

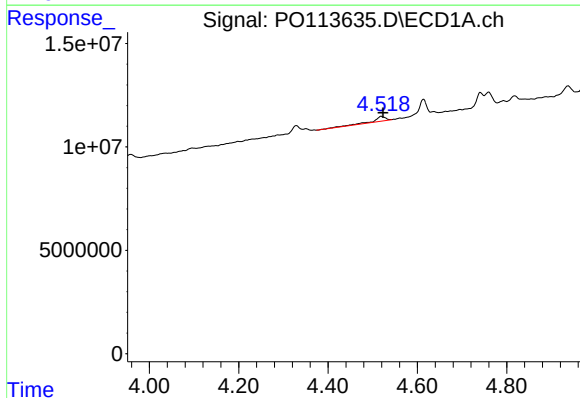


#12 AR-1232-2

R.T.: 4.519 min
Delta R.T.: -0.004 min
Response: 4469927
Conc: 41.42 ng/ml

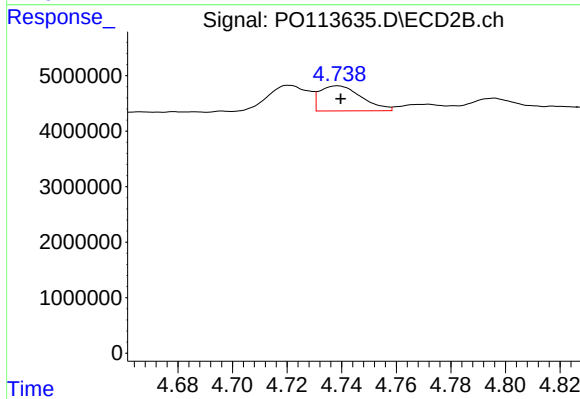

#12 AR-1232-2


R.T.: 4.739 min
Delta R.T.: 0.000 min
Response: 4796623
Conc: 39.30 ng/ml

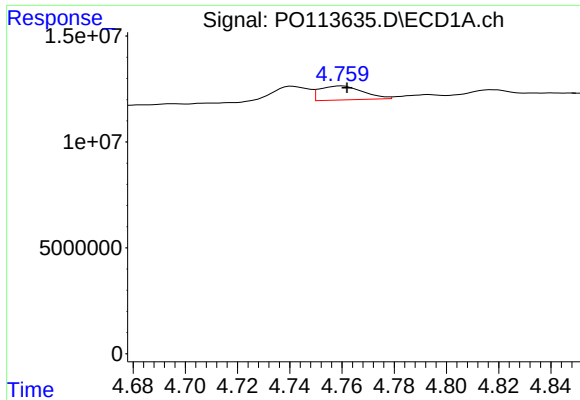

#13 AR-1232-3


R.T.: 4.760 min
Delta R.T.: -0.002 min
Response: 7596185
Conc: 38.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

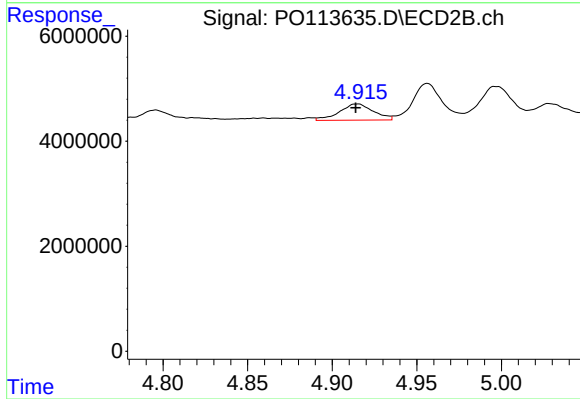


#13 AR-1232-3

R.T.: 4.915 min
Delta R.T.: 0.002 min
Response: 4325690
Conc: 65.39 ng/ml

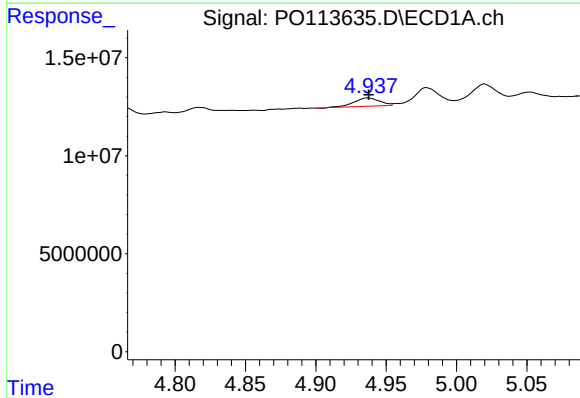


#14 AR-1232-4

R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 5358702
Conc: 54.52 ng/ml

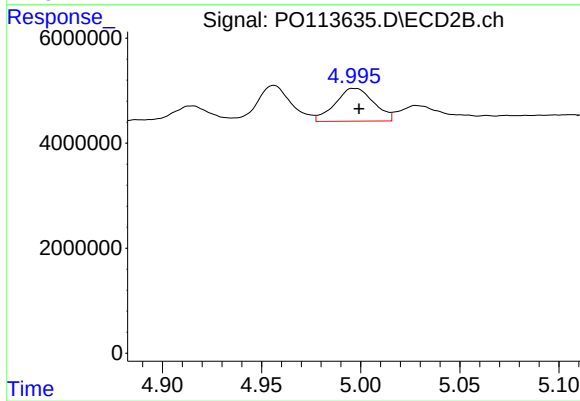

#14 AR-1232-4


R.T.: 4.996 min
Delta R.T.: -0.003 min
Response: 8456969
Conc: 141.12 ng/ml

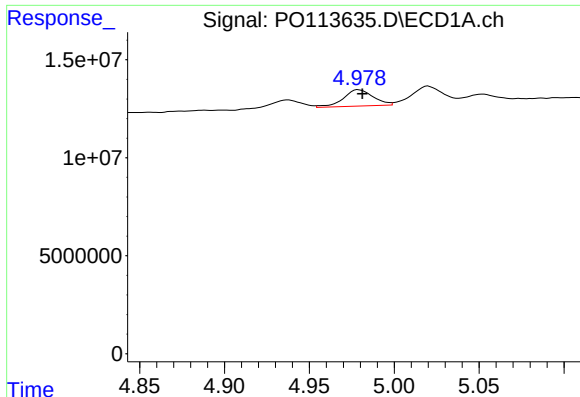

#15 AR-1232-5


R.T.: 4.979 min
Delta R.T.: -0.002 min
Response: 10208937
Conc: 155.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

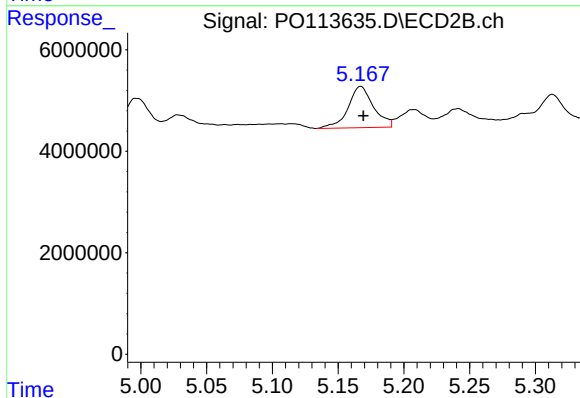


#15 AR-1232-5

R.T.: 5.167 min
Delta R.T.: -0.002 min
Response: 10983633
Conc: 162.44 ng/ml

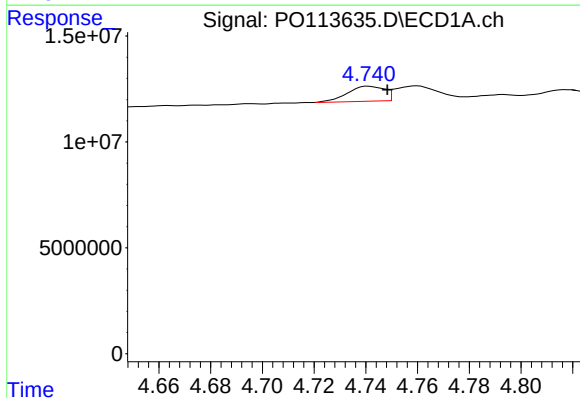


#16 AR-1242-1

R.T.: 4.741 min
Delta R.T.: -0.007 min
Response: 7036614
Conc: 30.60 ng/ml

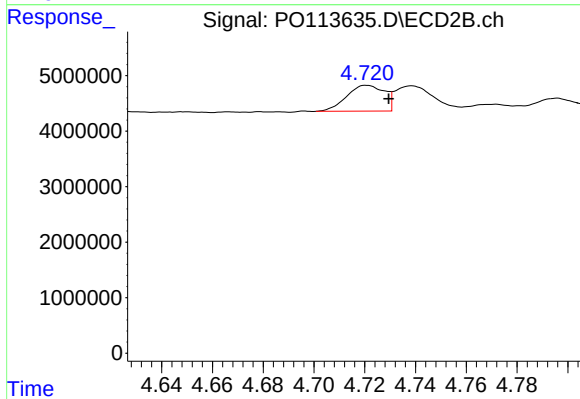

#16 AR-1242-1


R.T.: 4.721 min
Delta R.T.: -0.009 min
Response: 4808403
Conc: 33.28 ng/ml

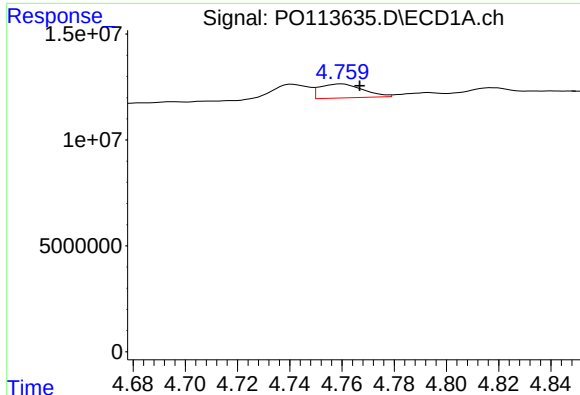

#17 AR-1242-2


R.T.: 4.760 min
Delta R.T.: -0.007 min
Response: 7596185
Conc: 22.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

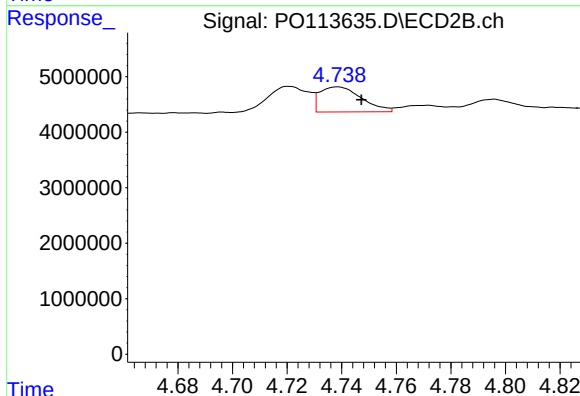


#17 AR-1242-2

R.T.: 4.739 min
Delta R.T.: -0.009 min
Response: 4796623
Conc: 22.11 ng/ml

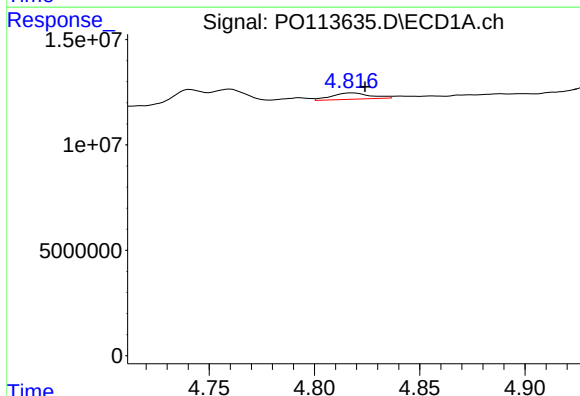


#18 AR-1242-3

R.T.: 4.818 min
Delta R.T.: -0.006 min
Response: 3756385
Conc: 16.93 ng/ml

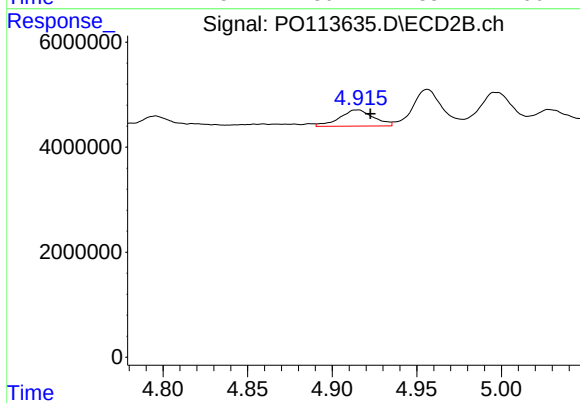

#18 AR-1242-3


R.T.: 4.915 min
Delta R.T.: -0.007 min
Response: 4325690
Conc: 36.98 ng/ml

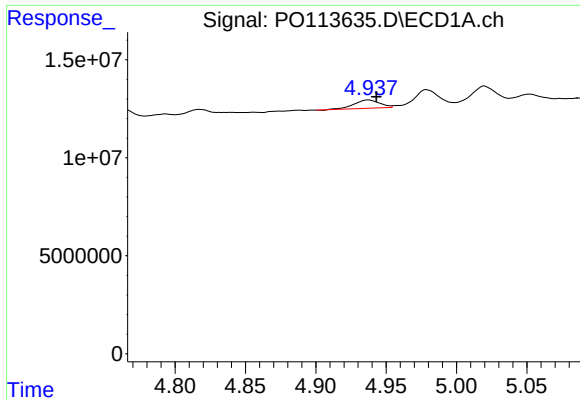

#19 AR-1242-4


R.T.: 4.937 min
Delta R.T.: -0.006 min
Response: 5358702
Conc: 30.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

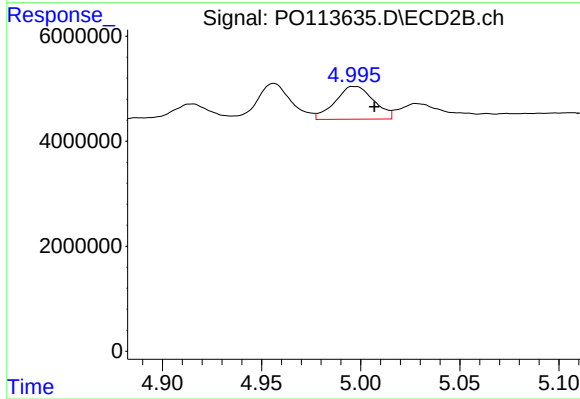


#19 AR-1242-4

R.T.: 4.996 min
Delta R.T.: -0.011 min
Response: 8456969
Conc: 71.89 ng/ml

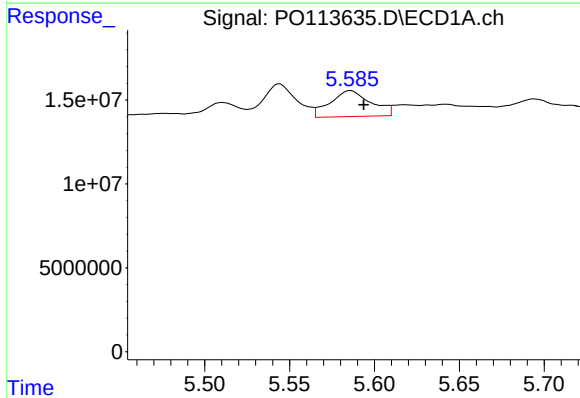


#20 AR-1242-5

R.T.: 5.586 min
Delta R.T.: -0.008 min
Response: 25757341
Conc: 128.68 ng/ml

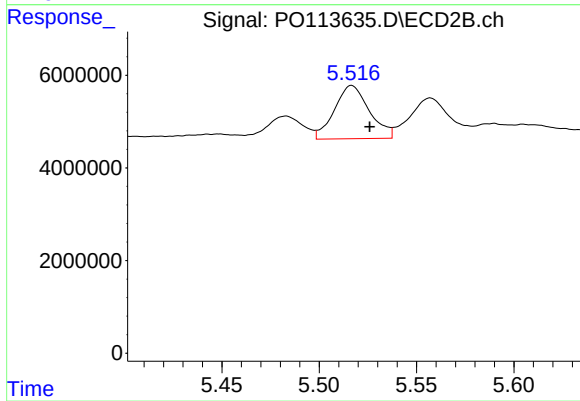

#20 AR-1242-5


R.T.: 5.517 min
Delta R.T.: -0.009 min
Response: 14361961
Conc: 96.30 ng/ml

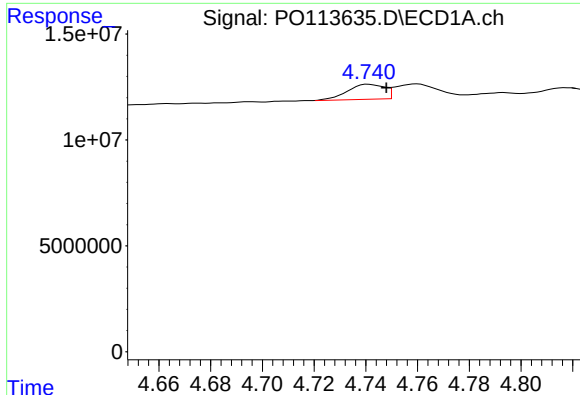

#21 AR-1248-1


R.T.: 4.741 min
Delta R.T.: -0.007 min
Response: 7036614
Conc: 40.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

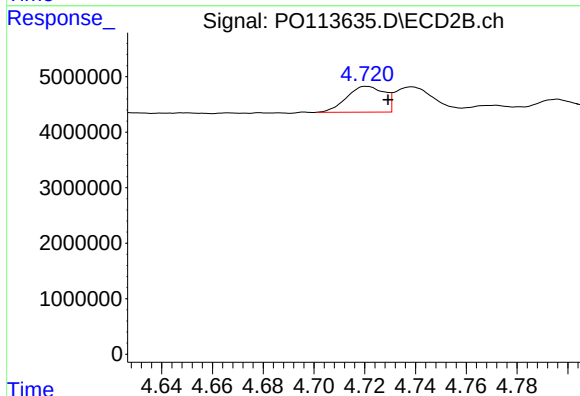


#21 AR-1248-1

R.T.: 4.721 min
Delta R.T.: -0.009 min
Response: 4808403
Conc: 43.12 ng/ml

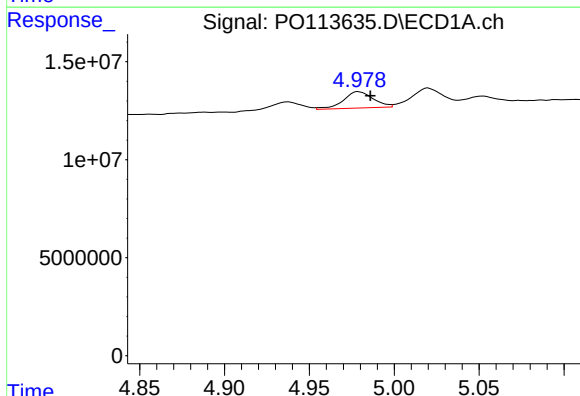


#22 AR-1248-2

R.T.: 4.979 min
Delta R.T.: -0.007 min
Response: 10208937
Conc: 42.21 ng/ml

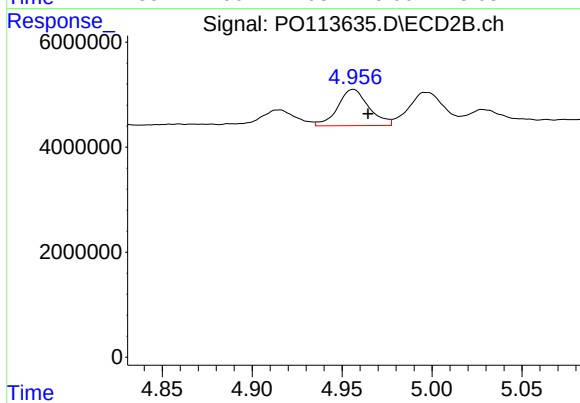

#22 AR-1248-2


R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 8296940
Conc: 51.63 ng/ml

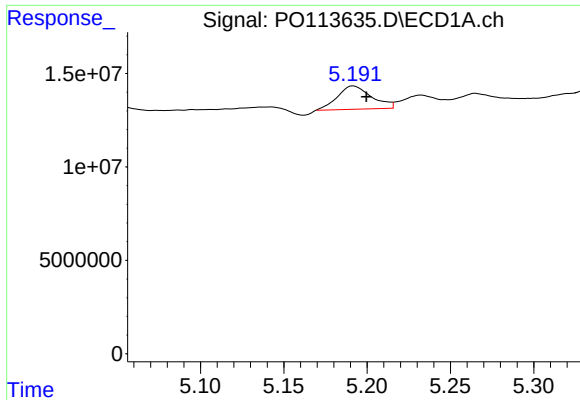

#23 AR-1248-3


R.T.: 5.192 min
Delta R.T.: -0.008 min
Response: 17780788
Conc: 55.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

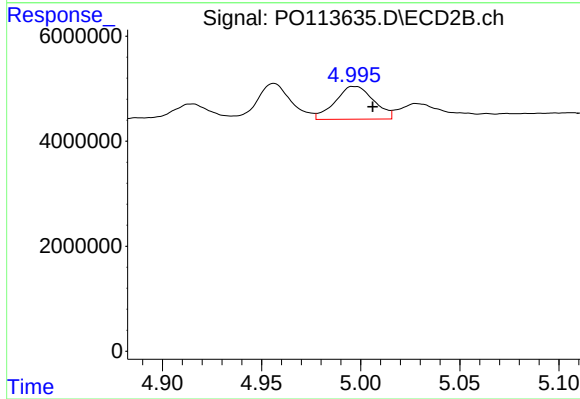


#23 AR-1248-3

R.T.: 4.996 min
Delta R.T.: -0.010 min
Response: 8456969
Conc: 49.85 ng/ml

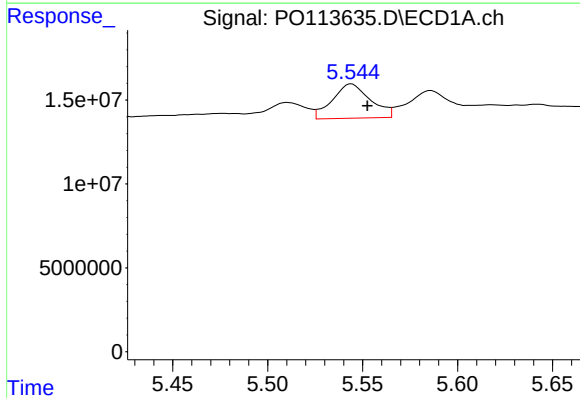


#24 AR-1248-4

R.T.: 5.544 min
Delta R.T.: -0.008 min
Response: 28422700
Conc: 56.89 ng/ml

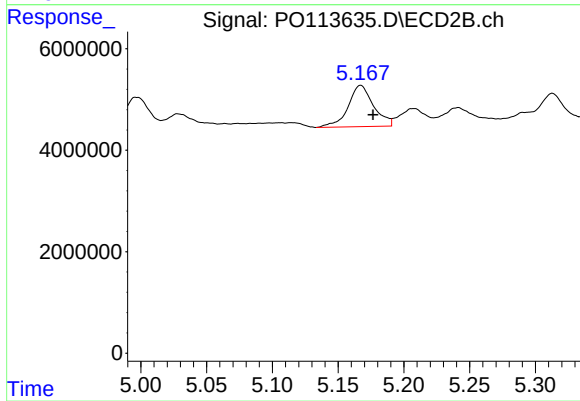

#24 AR-1248-4


R.T.: 5.167 min
Delta R.T.: -0.009 min
Response: 10983633
Conc: 55.13 ng/ml

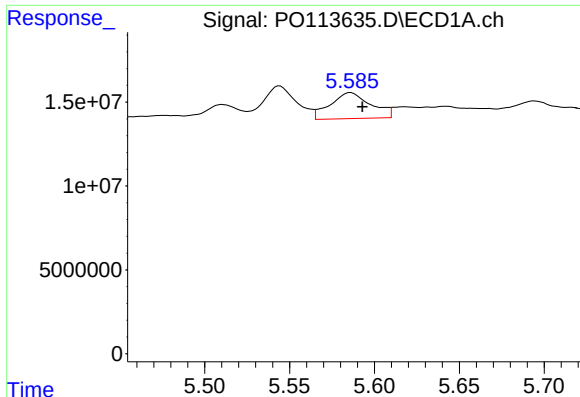

#25 AR-1248-5


R.T.: 5.586 min
Delta R.T.: -0.007 min
Response: 25757341
Conc: 75.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

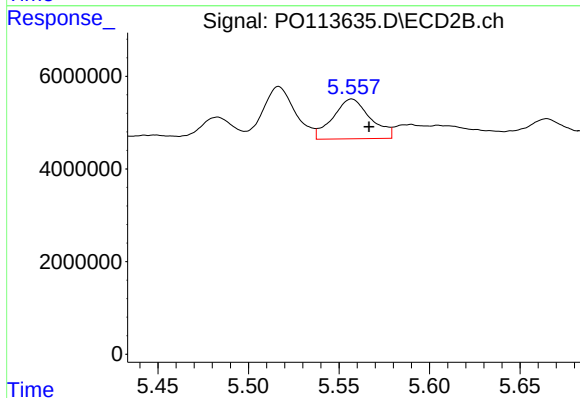


#25 AR-1248-5

R.T.: 5.557 min
Delta R.T.: -0.009 min
Response: 12436310
Conc: 58.58 ng/ml

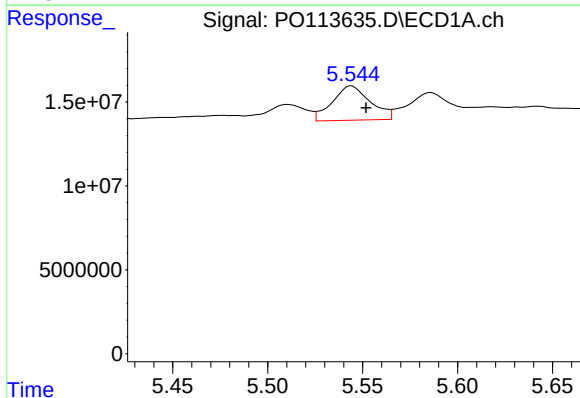


#26 AR-1254-1

R.T.: 5.544 min
Delta R.T.: -0.008 min
Response: 28422700
Conc: 52.64 ng/ml

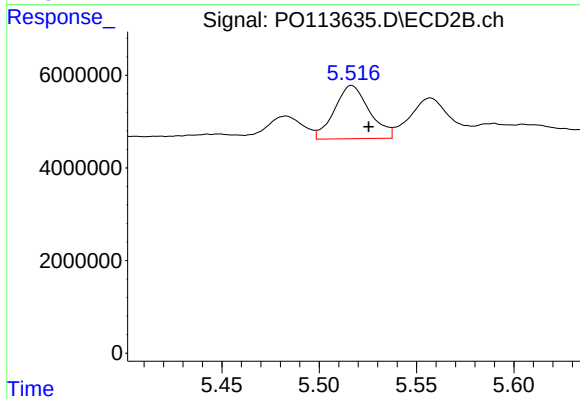

#26 AR-1254-1


R.T.: 5.517 min
Delta R.T.: -0.009 min
Response: 14361961
Conc: 45.54 ng/ml

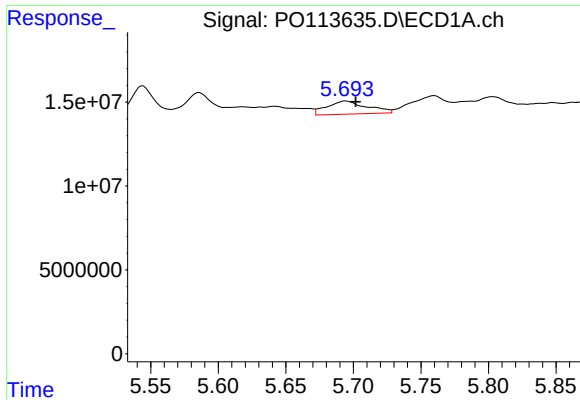

#27 AR-1254-2


R.T.: 5.694 min
Delta R.T.: -0.008 min
Response: 16289437
Conc: 33.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

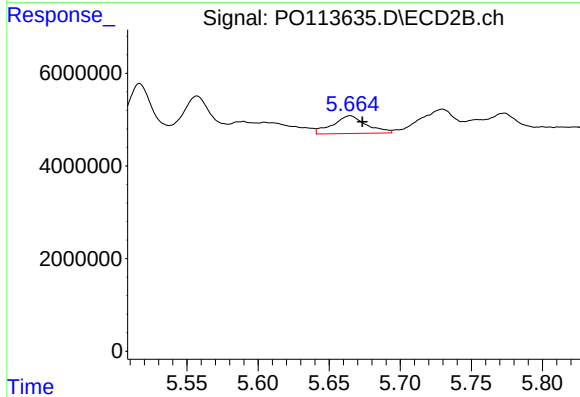


#27 AR-1254-2

R.T.: 5.665 min
Delta R.T.: -0.009 min
Response: 6275905
Conc: 22.39 ng/ml

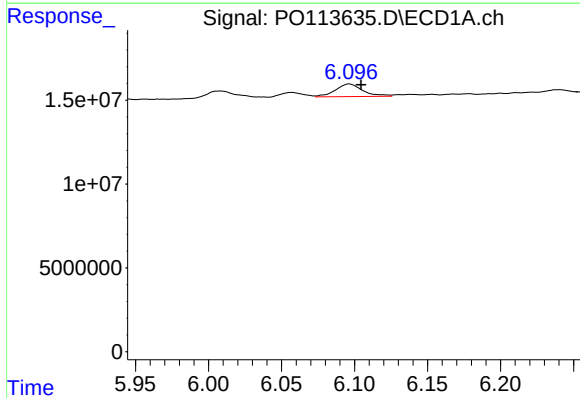


#28 AR-1254-3

R.T.: 6.097 min
Delta R.T.: -0.008 min
Response: 9860923
Conc: 13.35 ng/ml

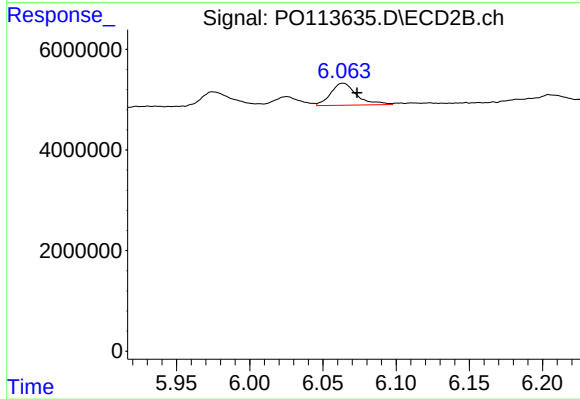

#28 AR-1254-3


R.T.: 6.064 min
Delta R.T.: -0.010 min
Response: 5413577
Conc: 12.98 ng/ml

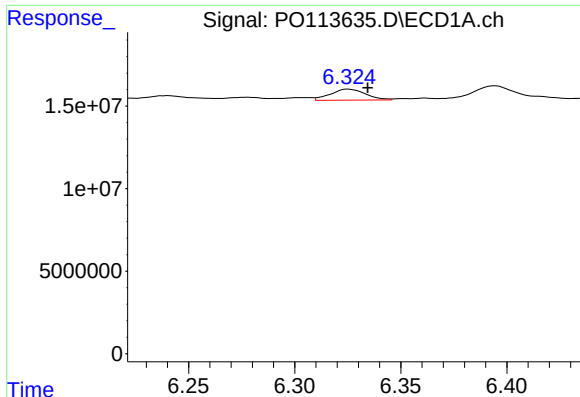

#29 AR-1254-4


R.T.: 6.325 min
Delta R.T.: -0.009 min
Response: 7654188
Conc: 13.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

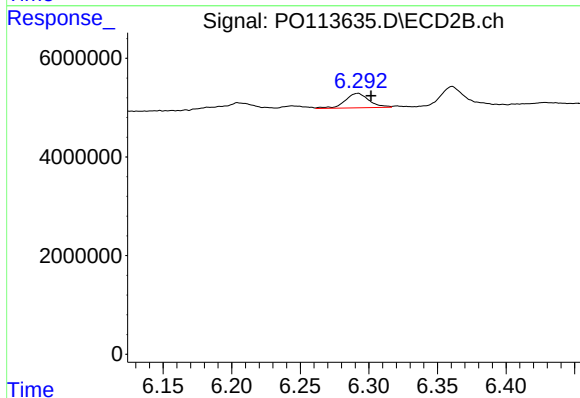


#29 AR-1254-4

R.T.: 6.292 min
Delta R.T.: -0.010 min
Response: 3552286
Conc: 12.93 ng/ml

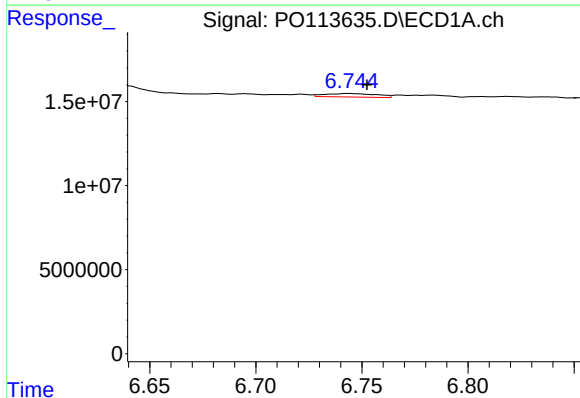


#30 AR-1254-5

R.T.: 6.744 min
Delta R.T.: -0.008 min
Response: 3498108
Conc: 4.99 ng/ml

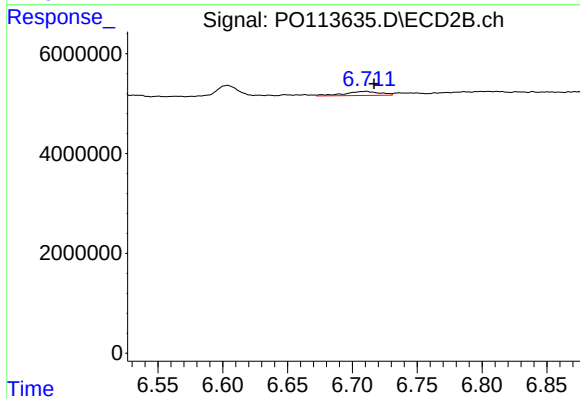

#30 AR-1254-5


R.T.: 6.710 min
Delta R.T.: -0.006 min
Response: 1537137
Conc: 4.30 ng/ml

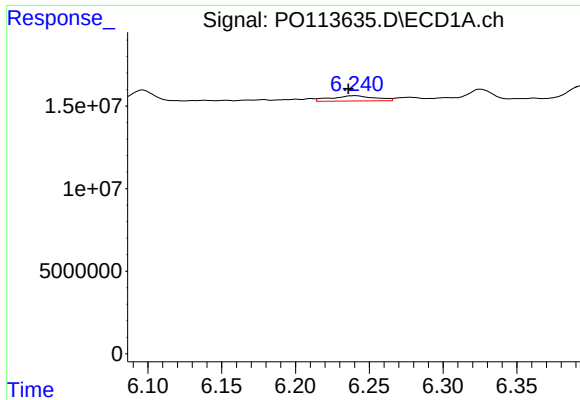

#31 AR-1260-1


R.T.: 6.240 min
Delta R.T.: 0.004 min
Response: 6592308
Conc: 14.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

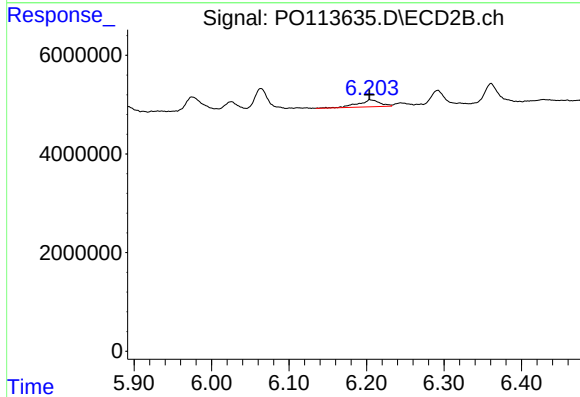


#31 AR-1260-1

R.T.: 6.205 min
Delta R.T.: 0.001 min
Response: 2850778
Conc: 11.18 ng/ml

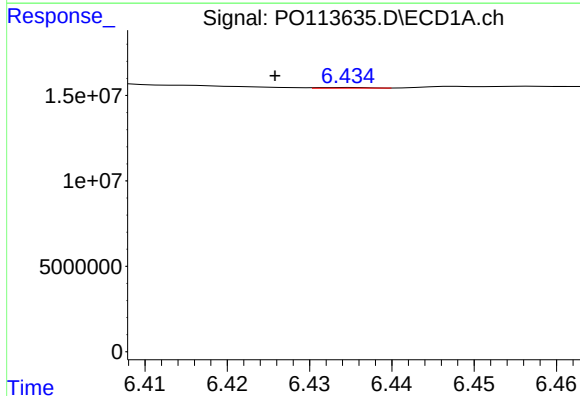


#32 AR-1260-2

R.T.: 6.435 min
Delta R.T.: 0.009 min
Response: 150653
Conc: 0.22 ng/ml

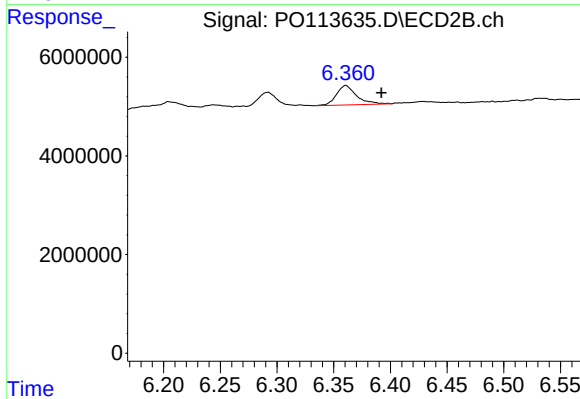

#32 AR-1260-2


R.T.: 6.361 min
Delta R.T.: -0.031 min
Response: 4904384
Conc: 14.19 ng/ml

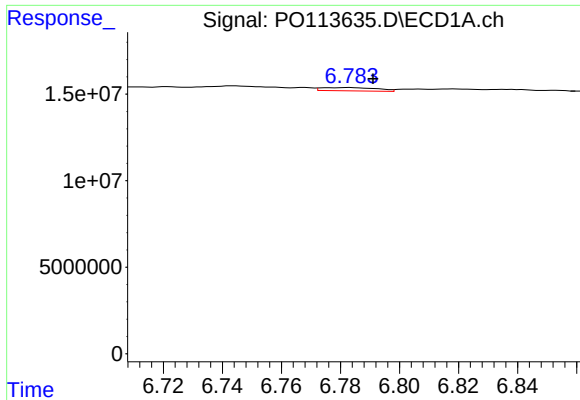

#33 AR-1260-3


R.T.: 6.783 min
Delta R.T.: -0.008 min
Response: 2475551
Conc: 4.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

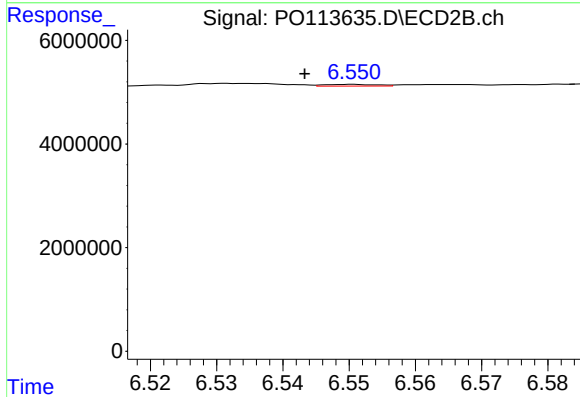


#33 AR-1260-3

R.T.: 6.550 min
Delta R.T.: 0.007 min
Response: 188424
Conc: 0.63 ng/ml

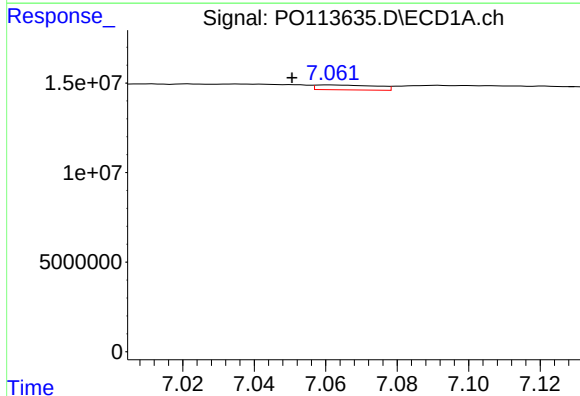


#34 AR-1260-4

R.T.: 7.061 min
Delta R.T.: 0.011 min
Response: 3189332
Conc: 7.12 ng/ml

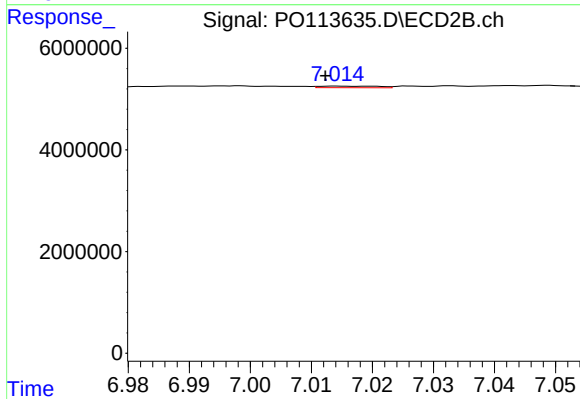

#34 AR-1260-4


R.T.: 7.015 min
Delta R.T.: 0.002 min
Response: 211060
Conc: 1.02 ng/ml

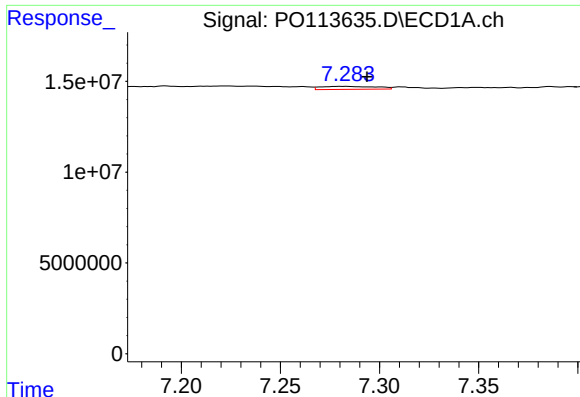

#35 AR-1260-5


R.T.: 7.282 min
Delta R.T.: -0.011 min
Response: 3183565
Conc: 2.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

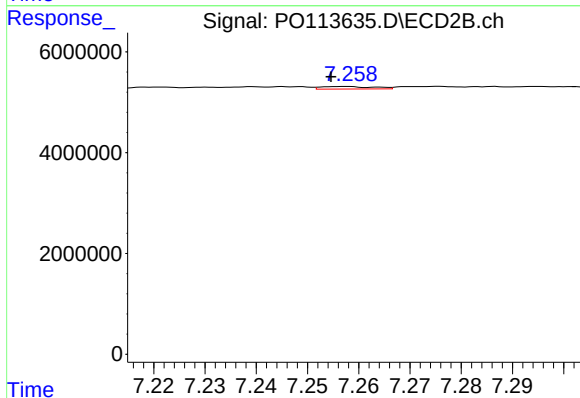


#35 AR-1260-5

R.T.: 7.257 min
Delta R.T.: 0.003 min
Response: 354910
Conc: 0.76 ng/ml

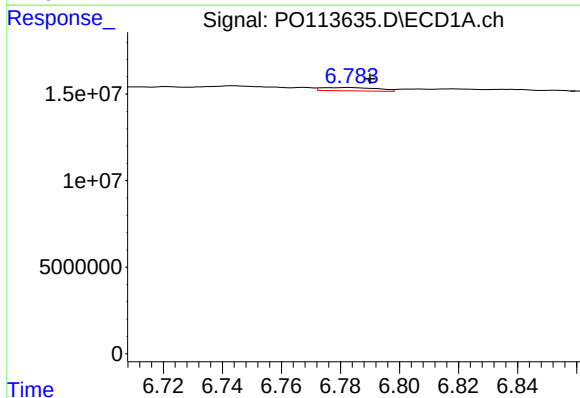


#36 AR-1262-1

R.T.: 6.783 min
Delta R.T.: -0.007 min
Response: 2475551
Conc: 2.70 ng/ml

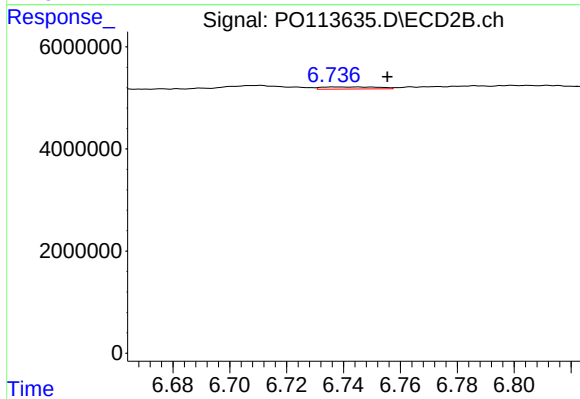

#36 AR-1262-1


R.T.: 6.737 min
Delta R.T.: -0.019 min
Response: 565844
Conc: 1.36 ng/ml

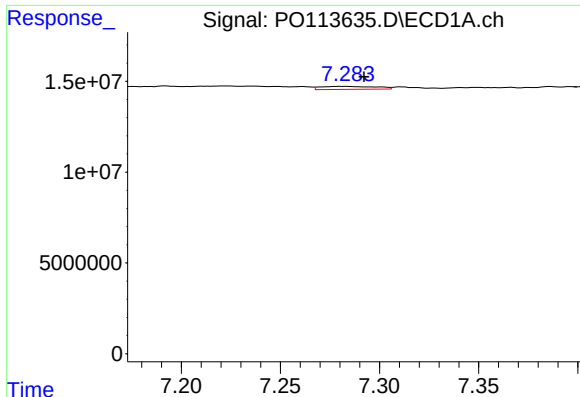

#37 AR-1262-2


R.T.: 7.282 min
Delta R.T.: -0.010 min
Response: 3183565
Conc: 2.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

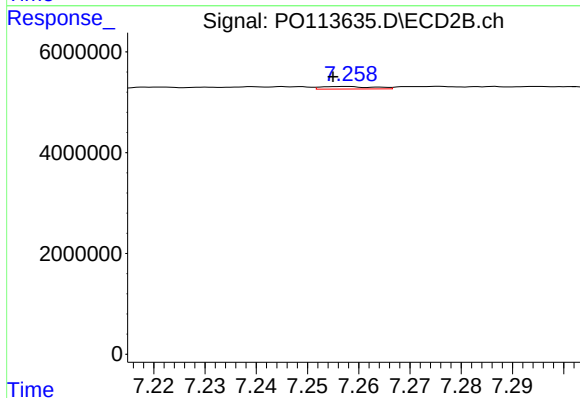


#37 AR-1262-2

R.T.: 7.257 min
Delta R.T.: 0.002 min
Response: 354910
Conc: 0.69 ng/ml

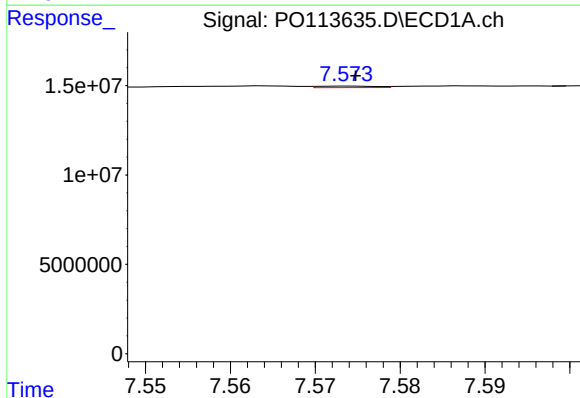


#38 AR-1262-3

R.T.: 7.574 min
Delta R.T.: 0.000 min
Response: 398193
Conc: 0.72 ng/ml

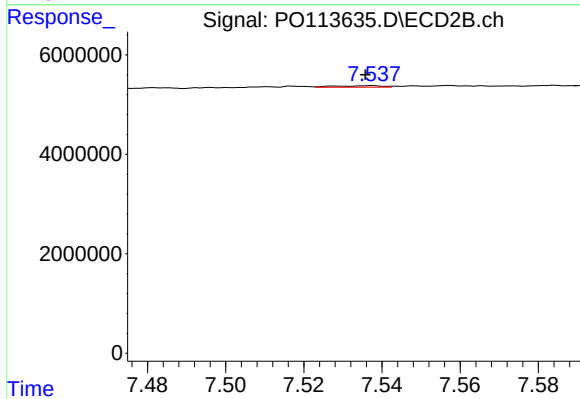

#38 AR-1262-3


R.T.: 7.537 min
Delta R.T.: 0.001 min
Response: 258093
Conc: 1.44 ng/ml

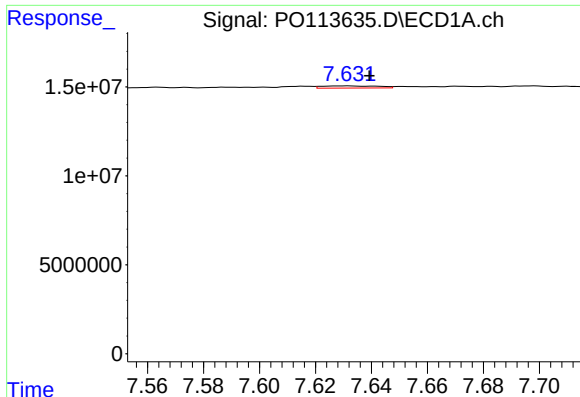

#39 AR-1262-4


R.T.: 7.632 min
Delta R.T.: -0.008 min
Response: 1775562
Conc: 1.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

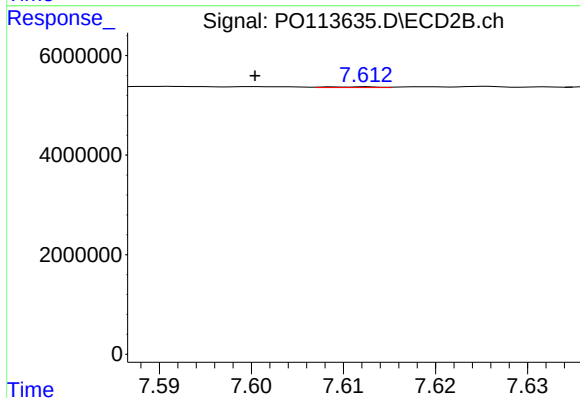


#39 AR-1262-4

R.T.: 7.612 min
Delta R.T.: 0.011 min
Response: 58335
Conc: 0.20 ng/ml

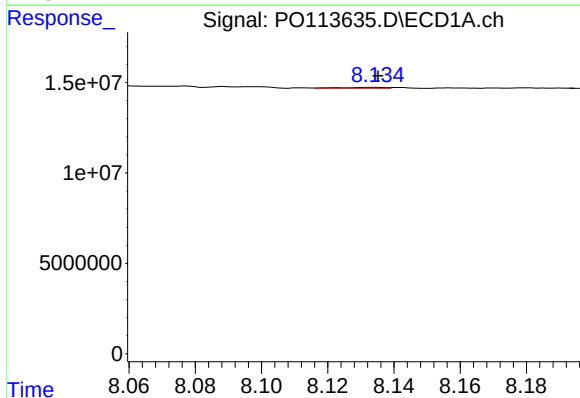


#40 AR-1262-5

R.T.: 8.134 min
Delta R.T.: -0.001 min
Response: 488499
Conc: 1.17 ng/ml

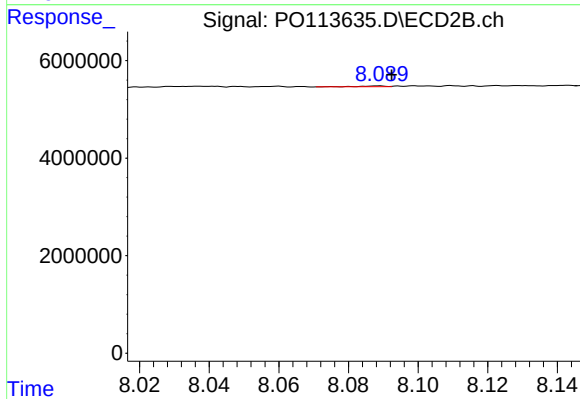

#40 AR-1262-5


R.T.: 8.089 min
Delta R.T.: -0.004 min
Response: 81339
Conc: 0.75 ng/ml

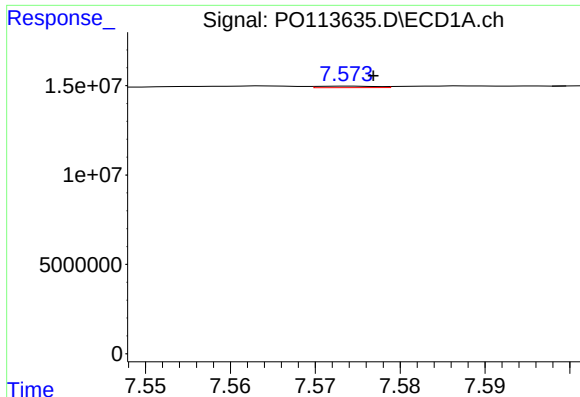

#41 AR-1268-1


R.T.: 7.574 min
Delta R.T.: -0.003 min
Response: 398193
Conc: 0.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

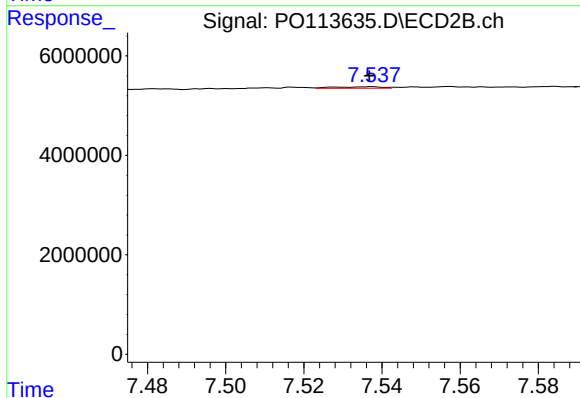


#41 AR-1268-1

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 258093
Conc: 0.51 ng/ml

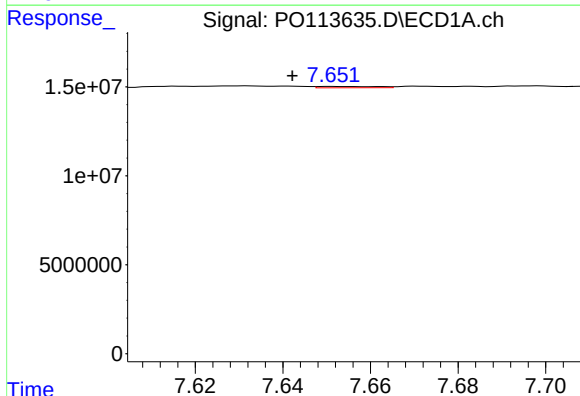


#42 AR-1268-2

R.T.: 7.651 min
Delta R.T.: 0.009 min
Response: 730571
Conc: 0.50 ng/ml

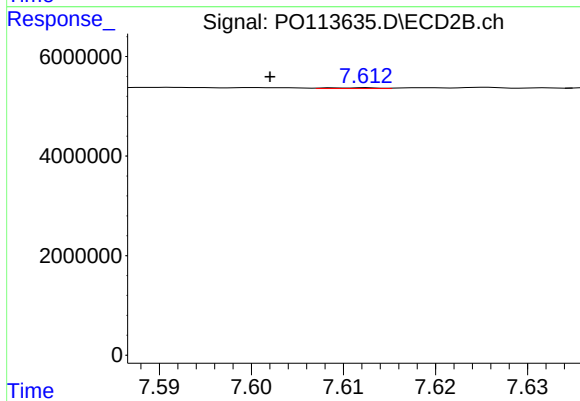

#42 AR-1268-2


R.T.: 7.612 min
Delta R.T.: 0.010 min
Response: 58335
Conc: 0.14 ng/ml

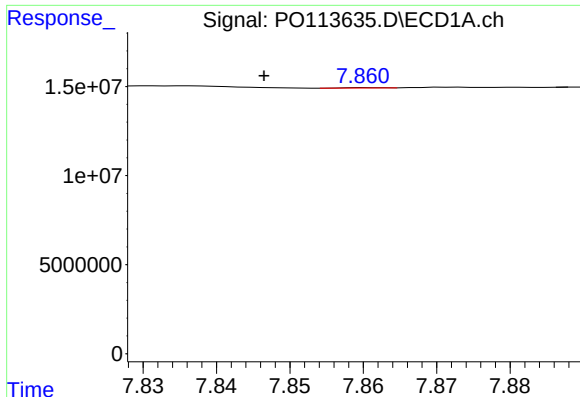

#43 AR-1268-3


R.T.: 7.861 min
Delta R.T.: 0.014 min
Response: 79599
Conc: 0.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

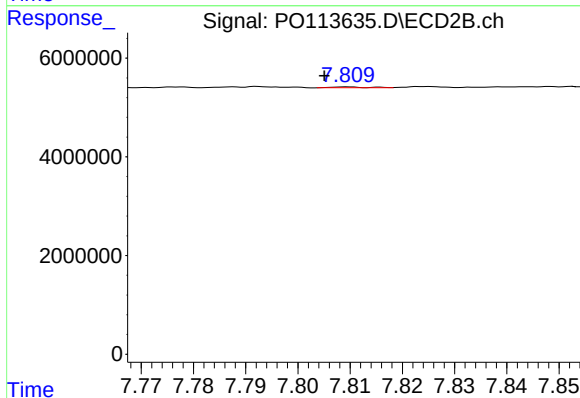


#43 AR-1268-3

R.T.: 7.809 min
Delta R.T.: 0.004 min
Response: 72944
Conc: 0.22 ng/ml

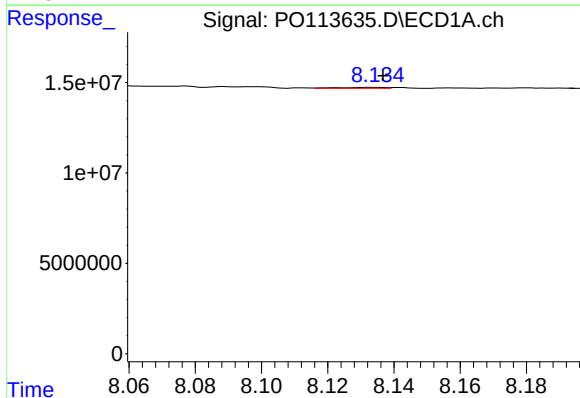


#44 AR-1268-4

R.T.: 8.134 min
Delta R.T.: -0.003 min
Response: 488499
Conc: 1.06 ng/ml

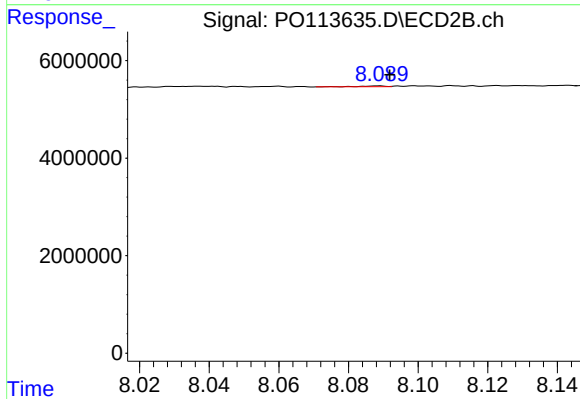

#44 AR-1268-4


R.T.: 8.089 min
Delta R.T.: -0.003 min
Response: 81339
Conc: 0.68 ng/ml

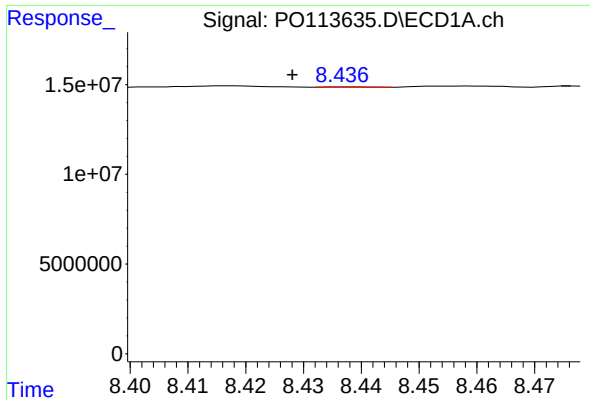

#45 AR-1268-5

R.T.: 8.438 min
Delta R.T.: 0.009 min
Response: 96706
Conc: 0.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

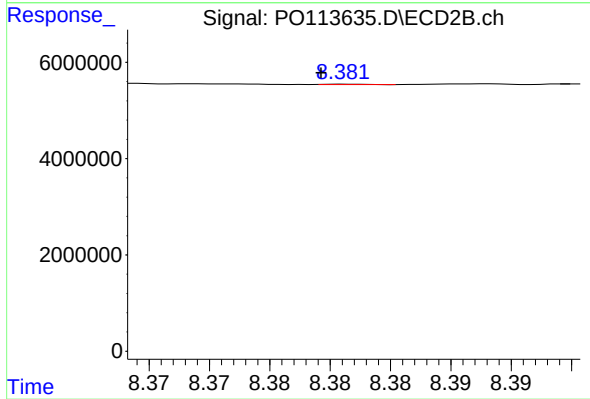

#45 AR-1268-5

R.T.: 8.382 min
Delta R.T.: 0.002 min
Response: 17600
Conc: 0.02 ng/ml