

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091025\
 Data File : P0113636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 03:39
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1254 WATER LOD 40PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:31:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.659	3.650	169.3E6	100.1E6	20.677	19.777
2)	SA Decachlor...	8.670	8.614	144.0E6	40800069	20.776	21.532
Target Compounds							
3)	L1 AR-1016-1	4.789f	4.722	728824	251025	2.730	1.472 #
4)	L1 AR-1016-2	4.789	4.750	728824	80606	1.816	0.313 #
5)	L1 AR-1016-3	4.816	4.920	475157	446529	1.863	3.198 #
6)	L1 AR-1016-4	4.932	4.957	718161	6307835	3.293	54.052 #
7)	L1 AR-1016-5	5.192	5.167	8693675	5755877	39.226	40.384
8)	L2 AR-1221-1	3.853	3.863	29327	52562	0.313	0.833 #
9)	L2 AR-1221-2	3.961	3.946	1999294	2112186	29.597	45.255 #
10)	L2 AR-1221-3	4.078f	4.017	302044	106645	1.365	0.718 #
11)	L3 AR-1232-1	4.078f	4.017	302044	106645	1.682	0.882 #
12)	L3 AR-1232-2	4.536	4.739	1524889	165965	14.130	1.360 #
13)	L3 AR-1232-3	4.789	4.920	728824	446529	3.692	6.750 #
14)	L3 AR-1232-4	4.932	4.996	718161	2995110	7.306	49.978 #
15)	L3 AR-1232-5	4.981	5.167	7191440	5755877	109.322	85.126
16)	L4 AR-1242-1	4.789f	4.722	728824	251025	3.170	1.737 #
17)	L4 AR-1242-2	4.789	4.750	728824	80606	2.121	0.372 #
18)	L4 AR-1242-3	4.816	4.925	475157	384601	2.141	3.288 #
19)	L4 AR-1242-4	4.932	4.996	718161	2995110	4.140	25.461 #
20)	L4 AR-1242-5	5.588	5.517	11265550	14665516	56.282	98.339 #
21)	L5 AR-1248-1	4.789f	4.722	728824	251025	4.177	2.251 #
22)	L5 AR-1248-2	4.981	4.957	7191440	6307835	29.733	39.252 #
23)	L5 AR-1248-3	5.192	4.996	8693675	2995110	27.265	17.654 #
24)	L5 AR-1248-4	5.546	5.167	27679753	5755877	55.403	28.892 #
25)	L5 AR-1248-5	5.588	5.557	11265550	4630617	32.989	21.812 #
26)	L6 AR-1254-1	5.546	5.517	27679753	14665516	51.261	46.505
27)	L6 AR-1254-2	5.694	5.664	25363887	13002015	51.401	46.380
28)	L6 AR-1254-3	6.097	6.064	27079649	15620976	36.650	37.467
29)	L6 AR-1254-4	6.327	6.293	19959928	9574712	35.835	34.838
30)	L6 AR-1254-5	6.744	6.707	31983567	12201656	45.627	34.131 #
31)	L7 AR-1260-1	6.229	6.194	14201665	7171809	31.844	28.117
32)	L7 AR-1260-2	6.417	6.381	13722191	6824967	19.982	19.742
33)	L7 AR-1260-3	6.813	6.532	4314948	5904278	6.988	19.851 #
34)	L7 AR-1260-4	7.040	7.004	2762490	761088	6.168	3.672 #
35)	L7 AR-1260-5	7.284	7.244	3743210	1389106	3.092	2.965
36)	L8 AR-1262-1	6.813	6.777	4314948	1574623	4.712	3.798
37)	L8 AR-1262-2	7.284	7.244	3743210	1389106	2.475	2.683
38)	L8 AR-1262-3	7.582	7.527	1564417	667649	2.823	3.718 #
39)	L8 AR-1262-4	7.628	7.584	5040430	1463938	5.154	5.050
40)	L8 AR-1262-5	8.140	8.099	320002	133894	0.768	1.236 #
41)	L9 AR-1268-1	7.582	7.527	1564417	667649	0.909	1.310 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
 Data File : P0113636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 03:39
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1254 WATER LOD 40PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:31:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.628	7.584	5040430	1463938	3.481	3.524
43) L9	AR-1268-3	7.860	7.821	150542	151611	0.125	0.464 #
44) L9	AR-1268-4	8.140	8.099	320002	133894	0.695	1.112 #
45) L9	AR-1268-5	8.434	8.369	94063	345709	0.030	0.443 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091025\
Data File : PO113636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 03:39
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1254 WATER LOD 40PPB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:31:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

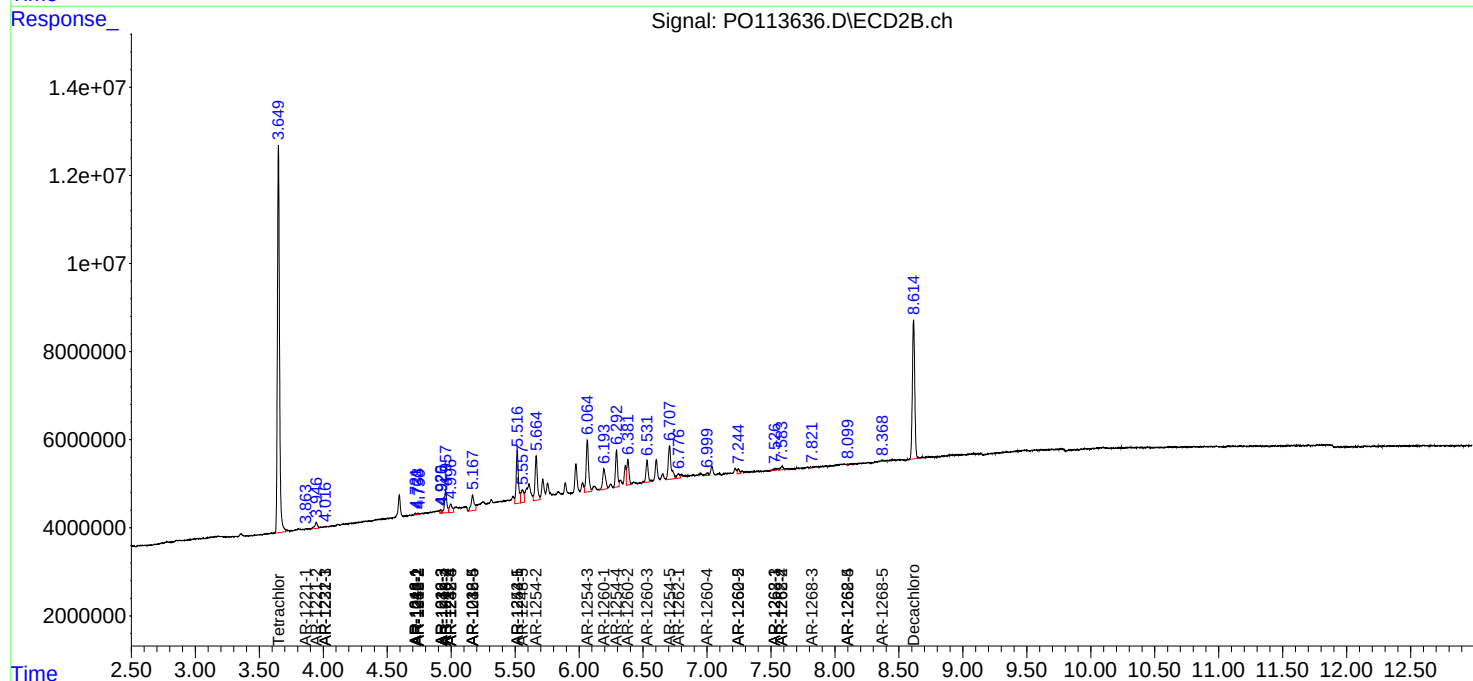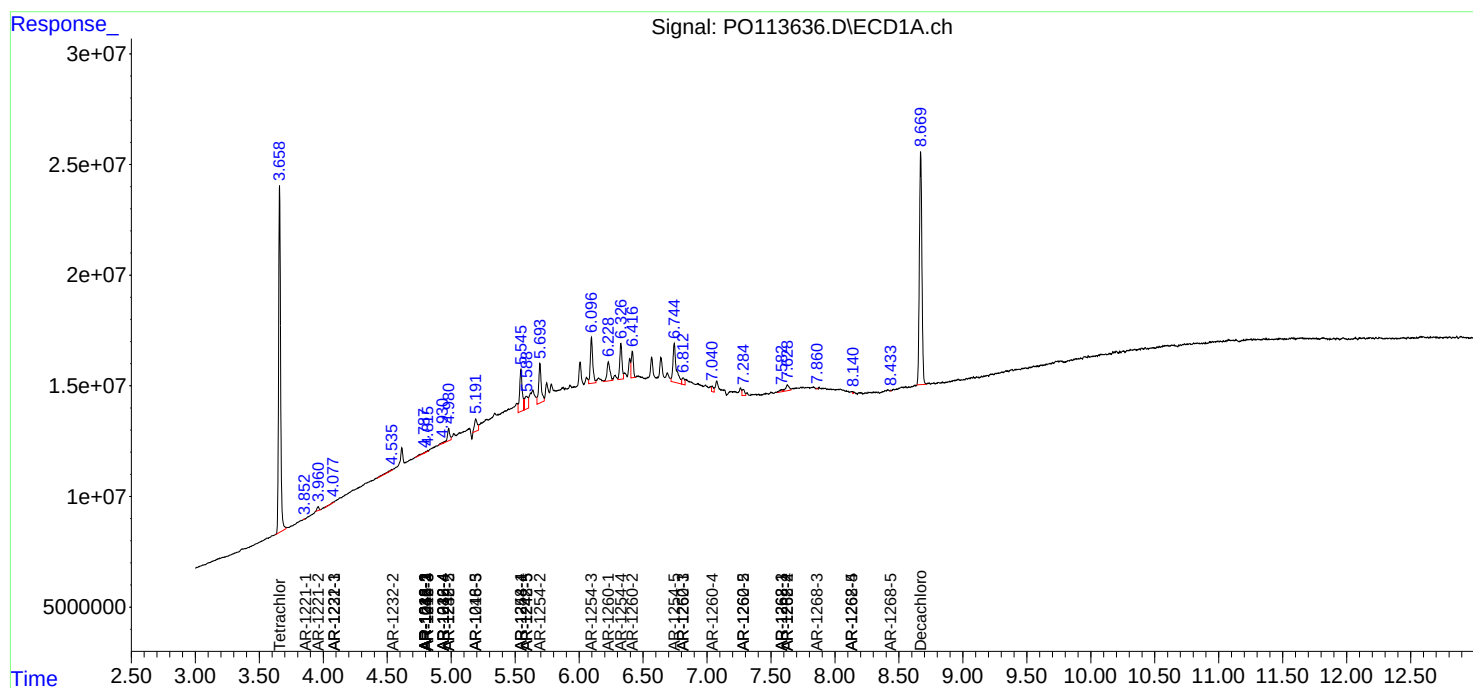


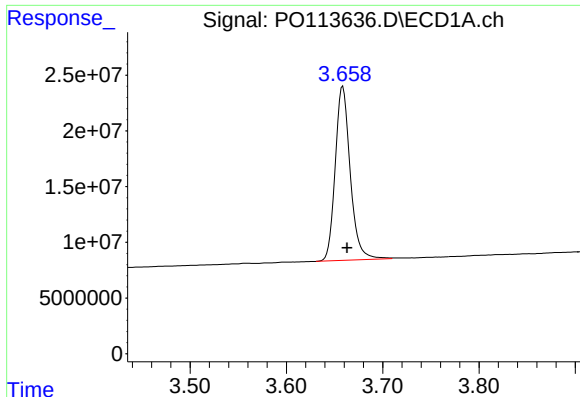

#1 Tetrachloro-m-xylene


R.T.: 3.659 min
Delta R.T.: -0.004 min
Response: 169278079
Conc: 20.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

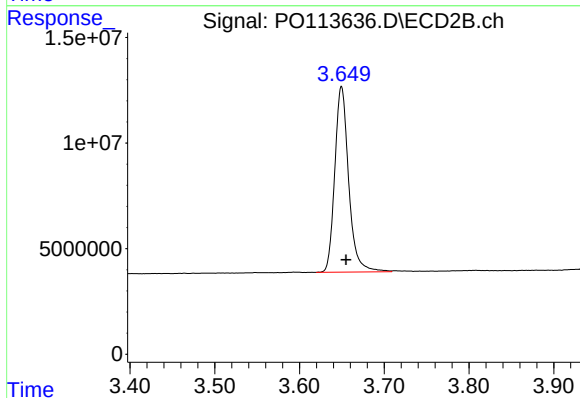


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: -0.005 min
Response: 100085317
Conc: 19.78 ng/ml

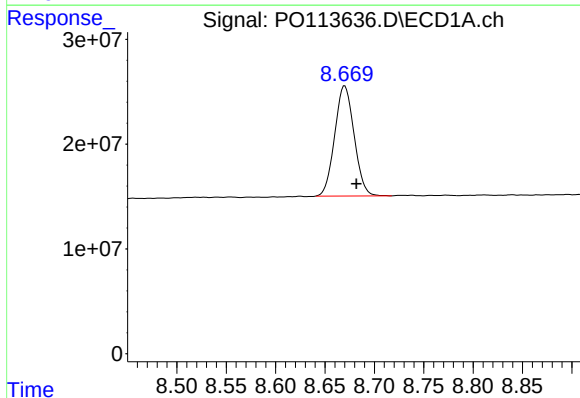


#2 Decachlorobiphenyl

R.T.: 8.670 min
Delta R.T.: -0.012 min
Response: 144004222
Conc: 20.78 ng/ml

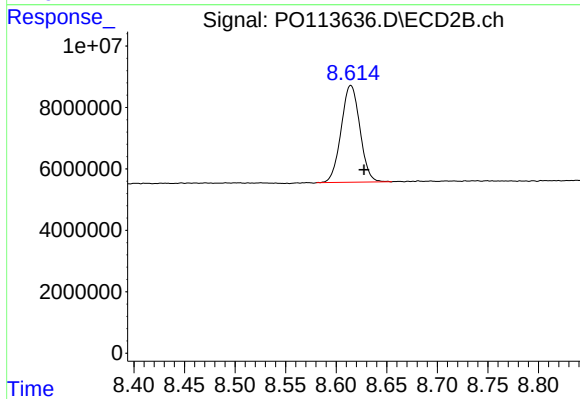

#2 Decachlorobiphenyl


R.T.: 8.614 min
Delta R.T.: -0.013 min
Response: 40800069
Conc: 21.53 ng/ml

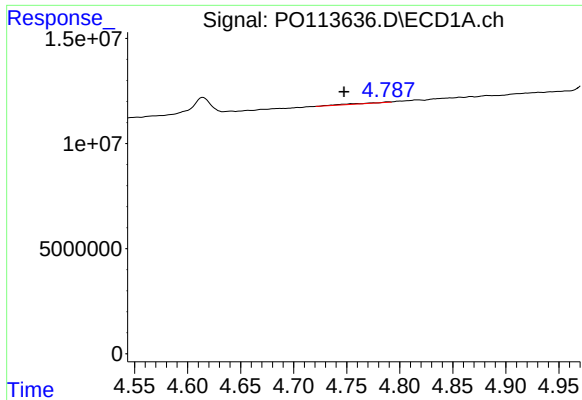

#3 AR-1016-1


R.T.: 4.789 min
Delta R.T.: 0.041 min
Response: 728824
Conc: 2.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

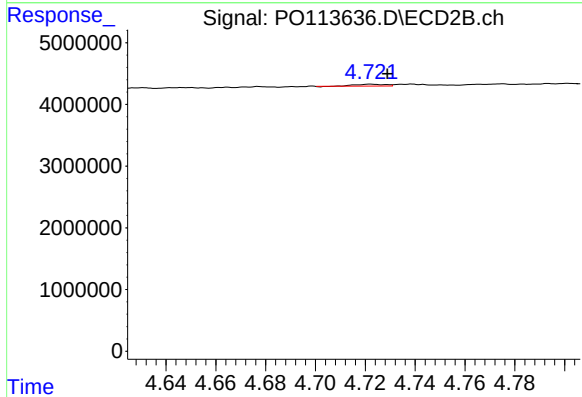


#3 AR-1016-1

R.T.: 4.722 min
Delta R.T.: -0.007 min
Response: 251025
Conc: 1.47 ng/ml

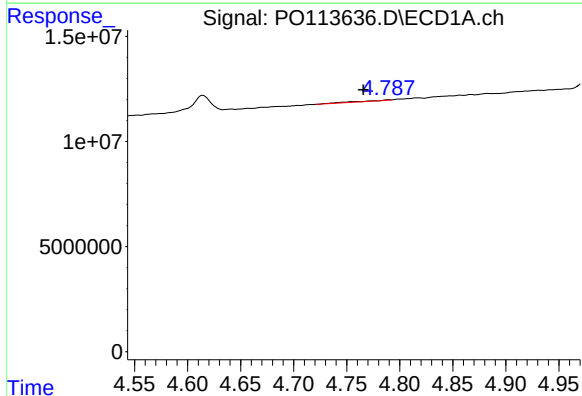


#4 AR-1016-2

R.T.: 4.789 min
Delta R.T.: 0.023 min
Response: 728824
Conc: 1.82 ng/ml

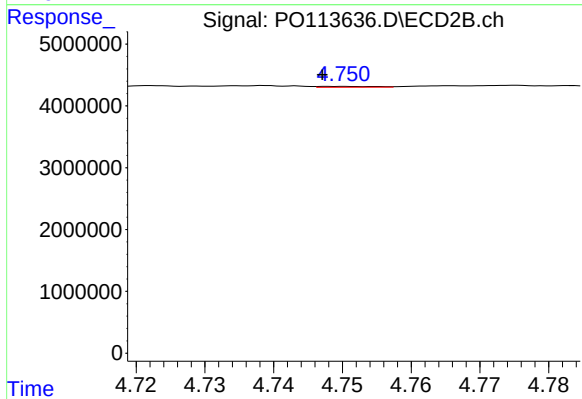

#4 AR-1016-2


R.T.: 4.750 min
Delta R.T.: 0.003 min
Response: 80606
Conc: 0.31 ng/ml

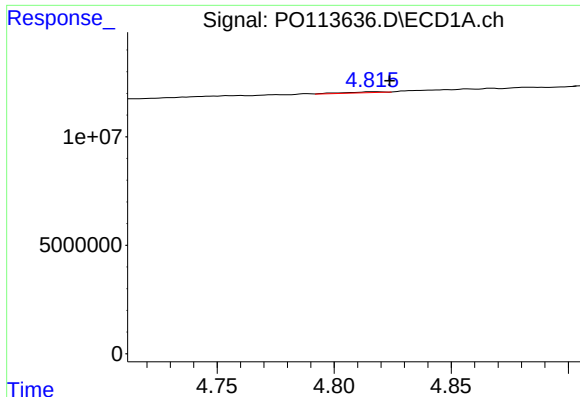

#5 AR-1016-3


R.T.: 4.816 min
Delta R.T.: -0.007 min
Response: 475157
Conc: 1.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

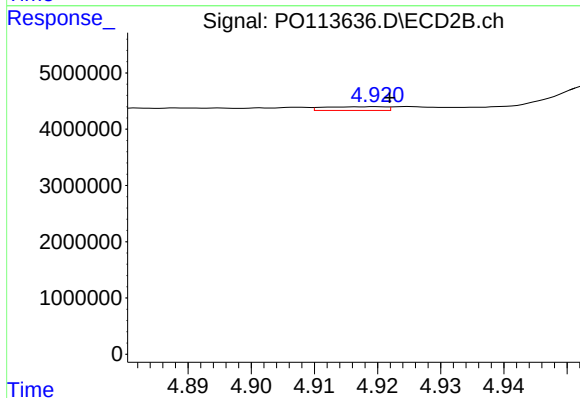


#5 AR-1016-3

R.T.: 4.920 min
Delta R.T.: -0.002 min
Response: 446529
Conc: 3.20 ng/ml

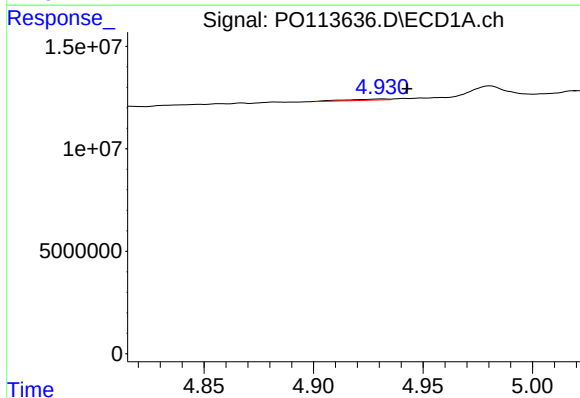


#6 AR-1016-4

R.T.: 4.932 min
Delta R.T.: -0.011 min
Response: 718161
Conc: 3.29 ng/ml

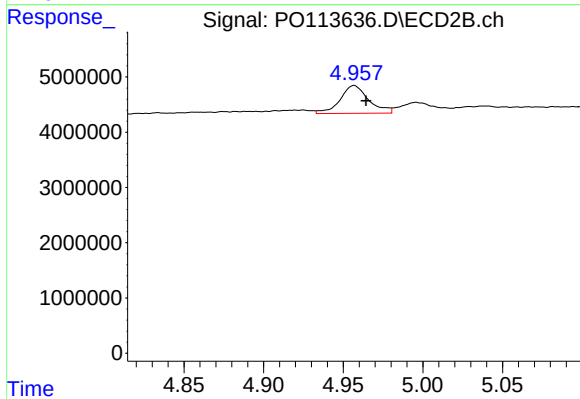

#6 AR-1016-4


R.T.: 4.957 min
Delta R.T.: -0.007 min
Response: 6307835
Conc: 54.05 ng/ml

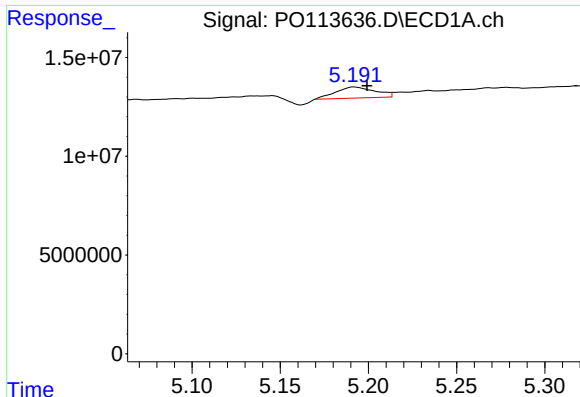

#7 AR-1016-5


R.T.: 5.192 min
Delta R.T.: -0.007 min
Response: 8693675
Conc: 39.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

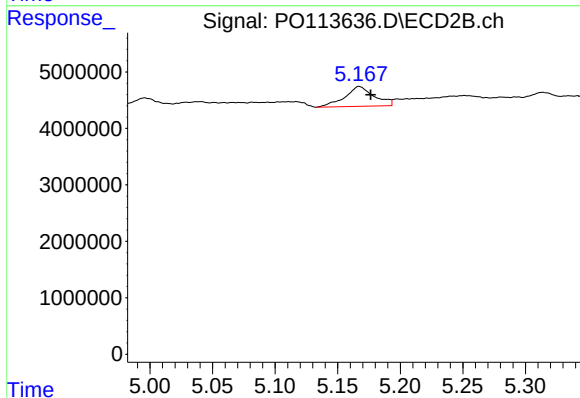


#7 AR-1016-5

R.T.: 5.167 min
Delta R.T.: -0.009 min
Response: 5755877
Conc: 40.38 ng/ml

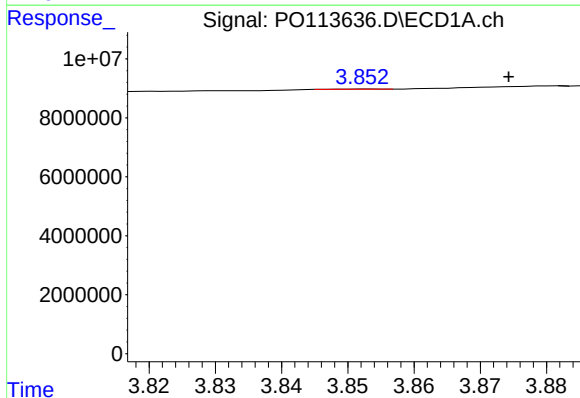


#8 AR-1221-1

R.T.: 3.853 min
Delta R.T.: -0.021 min
Response: 29327
Conc: 0.31 ng/ml

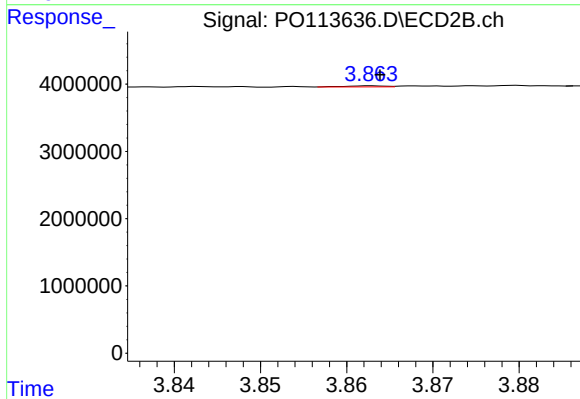

#8 AR-1221-1


R.T.: 3.863 min
Delta R.T.: 0.000 min
Response: 52562
Conc: 0.83 ng/ml

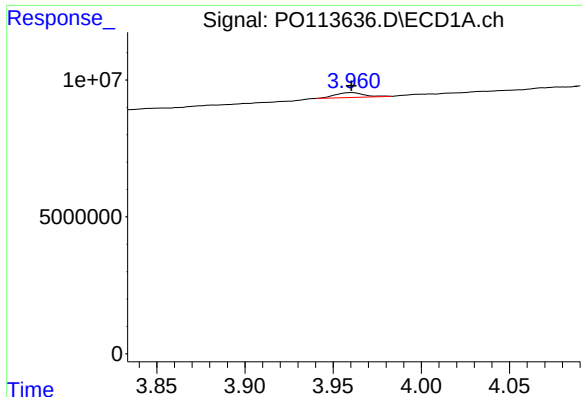

#9 AR-1221-2


R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 1999294
Conc: 29.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

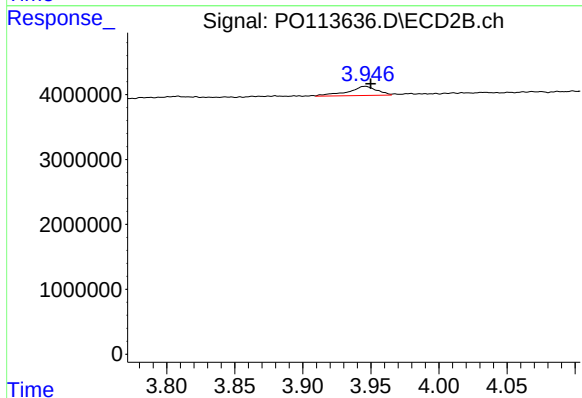


#9 AR-1221-2

R.T.: 3.946 min
Delta R.T.: -0.004 min
Response: 2112186
Conc: 45.25 ng/ml

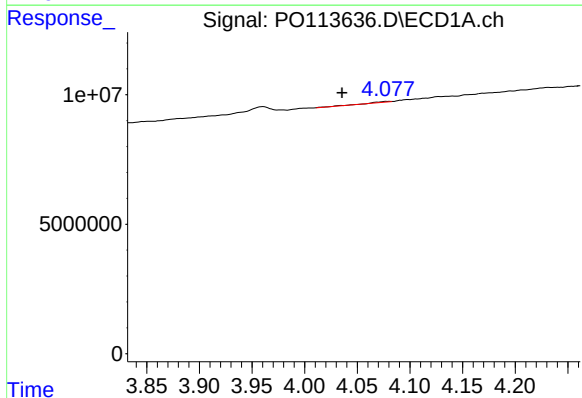


#10 AR-1221-3

R.T.: 4.078 min
Delta R.T.: 0.042 min
Response: 302044
Conc: 1.36 ng/ml

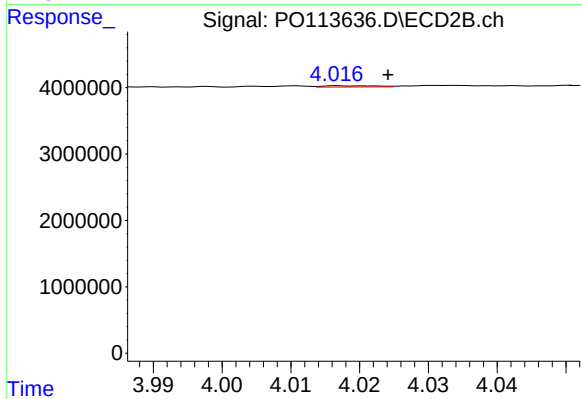

#10 AR-1221-3


R.T.: 4.017 min
Delta R.T.: -0.007 min
Response: 106645
Conc: 0.72 ng/ml

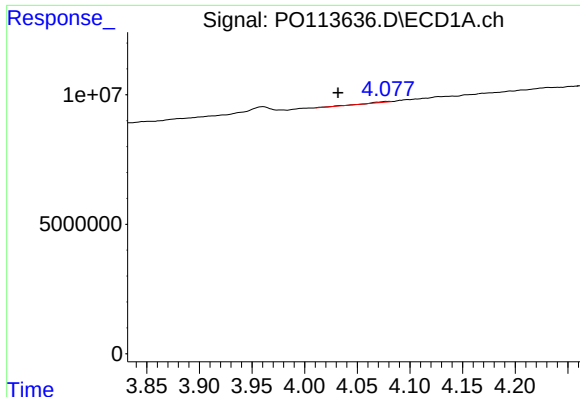

#11 AR-1232-1


R.T.: 4.078 min
Delta R.T.: 0.046 min
Response: 302044
Conc: 1.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

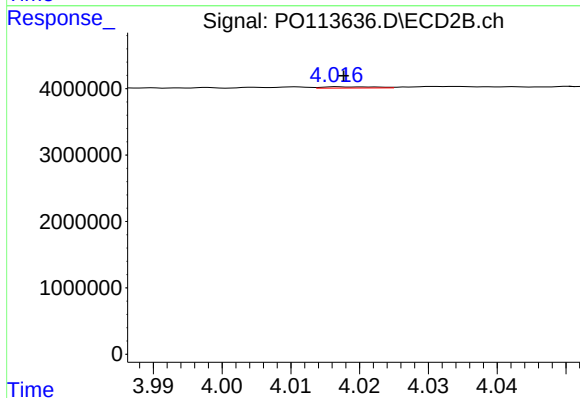


#11 AR-1232-1

R.T.: 4.017 min
Delta R.T.: 0.000 min
Response: 106645
Conc: 0.88 ng/ml

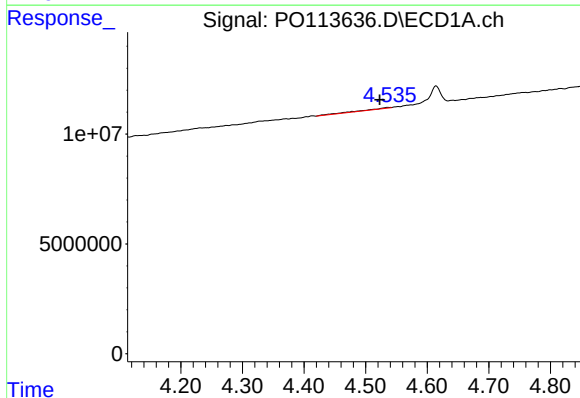


#12 AR-1232-2

R.T.: 4.536 min
Delta R.T.: 0.013 min
Response: 1524889
Conc: 14.13 ng/ml

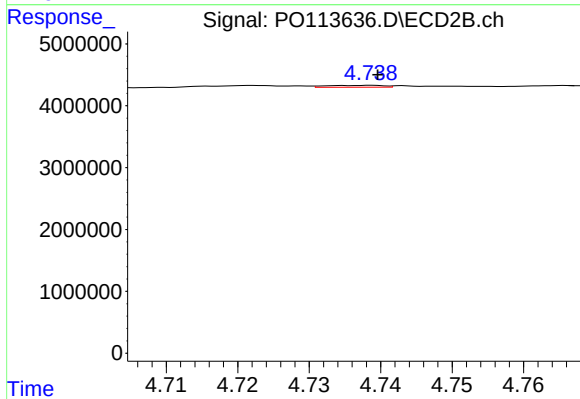

#12 AR-1232-2


R.T.: 4.739 min
Delta R.T.: 0.000 min
Response: 165965
Conc: 1.36 ng/ml

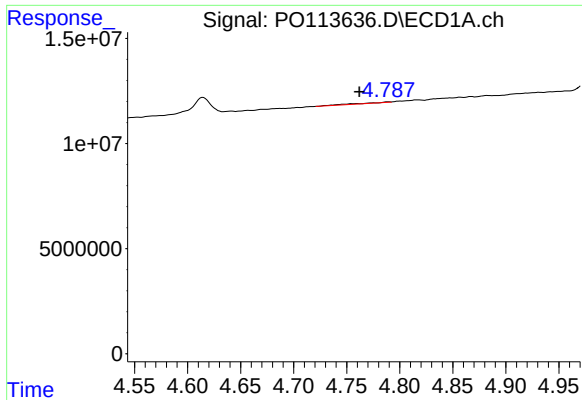

#13 AR-1232-3


R.T.: 4.789 min
Delta R.T.: 0.027 min
Response: 728824
Conc: 3.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

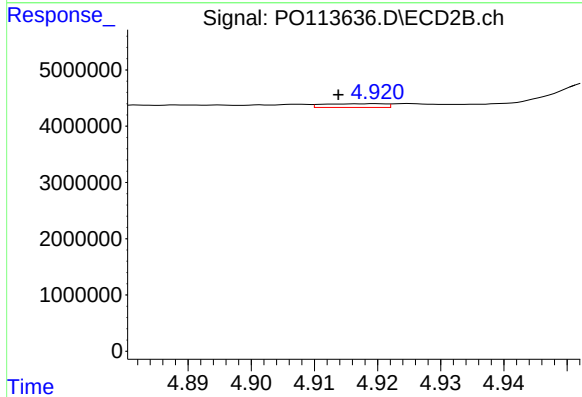


#13 AR-1232-3

R.T.: 4.920 min
Delta R.T.: 0.006 min
Response: 446529
Conc: 6.75 ng/ml

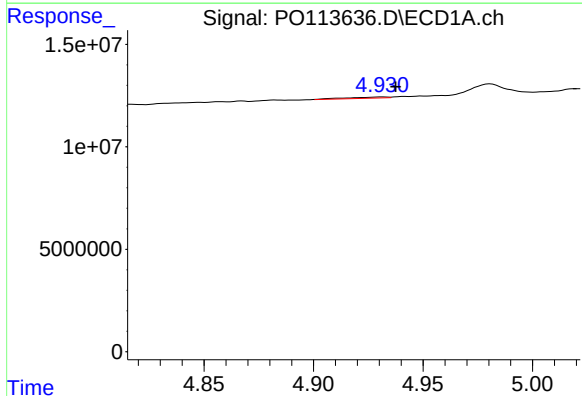


#14 AR-1232-4

R.T.: 4.932 min
Delta R.T.: -0.006 min
Response: 718161
Conc: 7.31 ng/ml

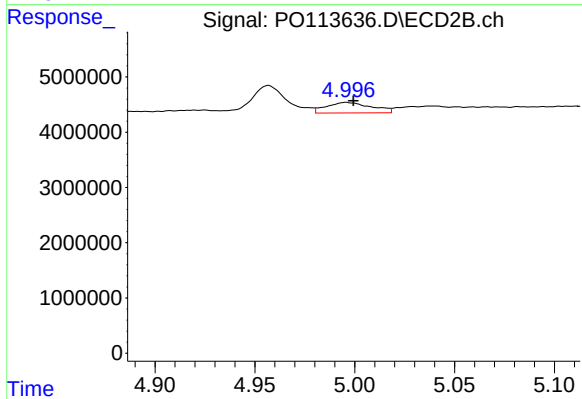

#14 AR-1232-4


R.T.: 4.996 min
Delta R.T.: -0.003 min
Response: 2995110
Conc: 49.98 ng/ml

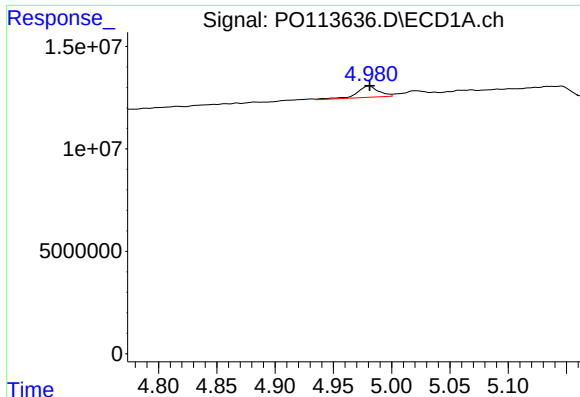

#15 AR-1232-5


R.T.: 4.981 min
Delta R.T.: 0.000 min
Response: 7191440
Conc: 109.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

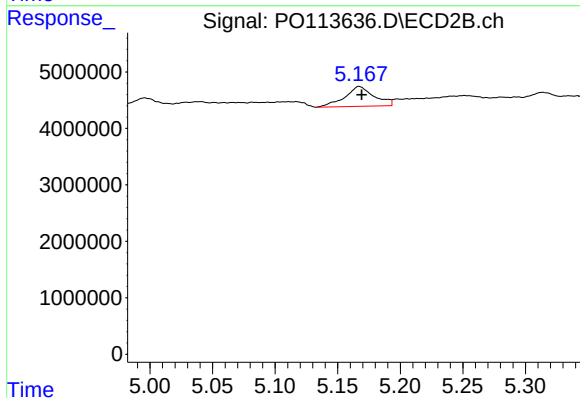


#15 AR-1232-5

R.T.: 5.167 min
Delta R.T.: -0.002 min
Response: 5755877
Conc: 85.13 ng/ml

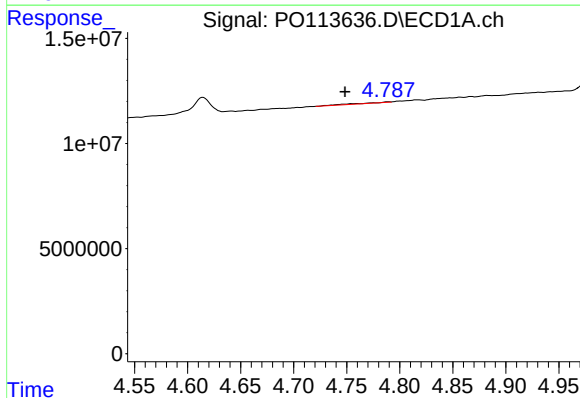


#16 AR-1242-1

R.T.: 4.789 min
Delta R.T.: 0.041 min
Response: 728824
Conc: 3.17 ng/ml

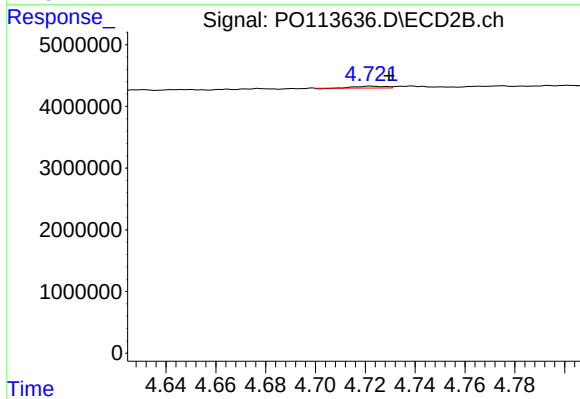

#16 AR-1242-1


R.T.: 4.722 min
Delta R.T.: -0.007 min
Response: 251025
Conc: 1.74 ng/ml

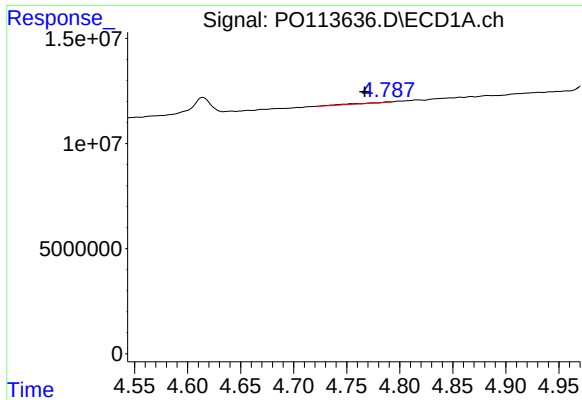

#17 AR-1242-2


R.T.: 4.789 min
Delta R.T.: 0.022 min
Response: 728824
Conc: 2.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

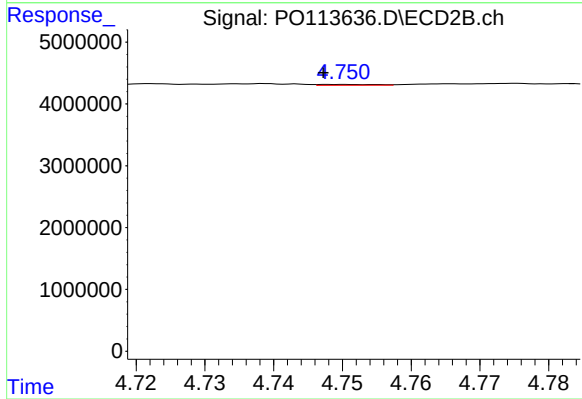


#17 AR-1242-2

R.T.: 4.750 min
Delta R.T.: 0.003 min
Response: 80606
Conc: 0.37 ng/ml

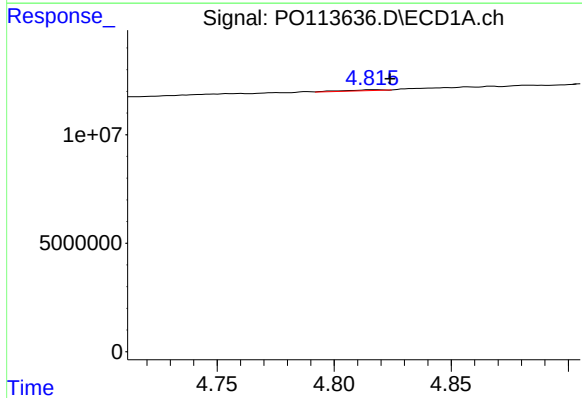


#18 AR-1242-3

R.T.: 4.816 min
Delta R.T.: -0.008 min
Response: 475157
Conc: 2.14 ng/ml

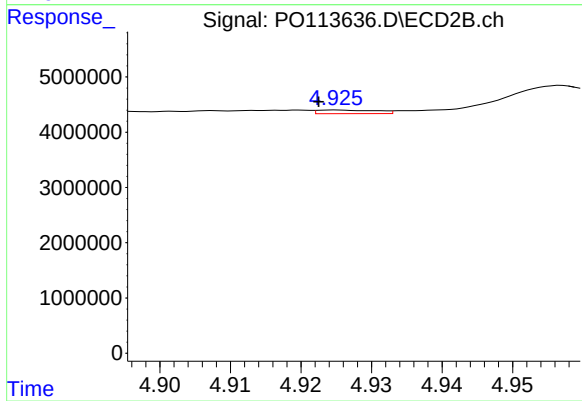

#18 AR-1242-3


R.T.: 4.925 min
Delta R.T.: 0.002 min
Response: 384601
Conc: 3.29 ng/ml

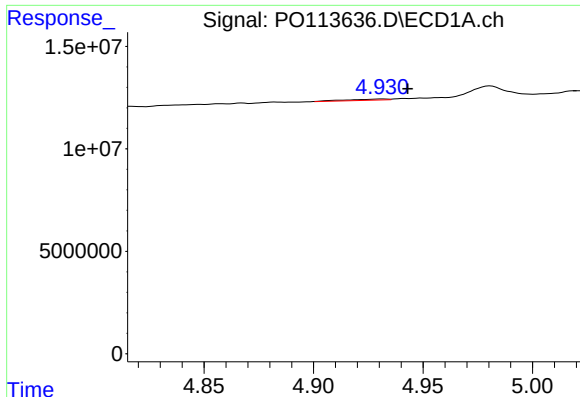

#19 AR-1242-4


R.T.: 4.932 min
Delta R.T.: -0.011 min
Response: 718161
Conc: 4.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

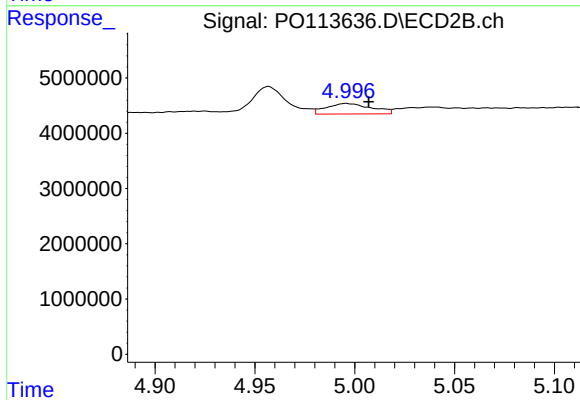


#19 AR-1242-4

R.T.: 4.996 min
Delta R.T.: -0.011 min
Response: 2995110
Conc: 25.46 ng/ml

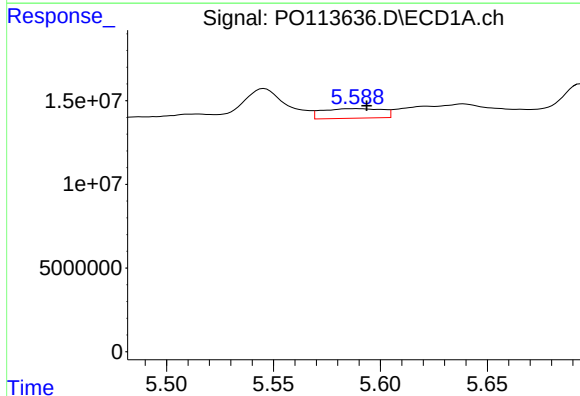


#20 AR-1242-5

R.T.: 5.588 min
Delta R.T.: -0.005 min
Response: 11265550
Conc: 56.28 ng/ml

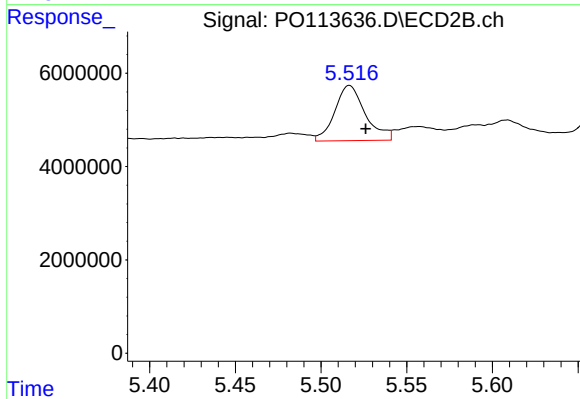

#20 AR-1242-5


R.T.: 5.517 min
Delta R.T.: -0.009 min
Response: 14665516
Conc: 98.34 ng/ml

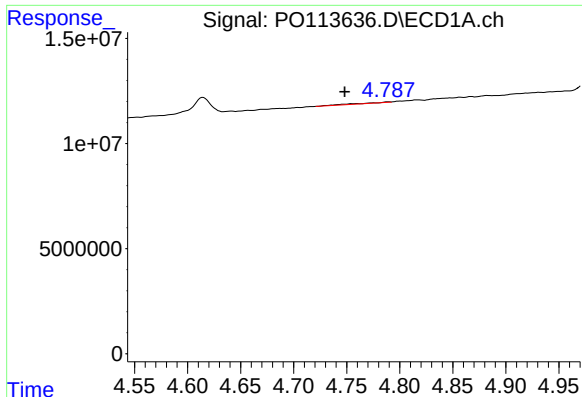

#21 AR-1248-1


R.T.: 4.789 min
Delta R.T.: 0.041 min
Response: 728824
Conc: 4.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

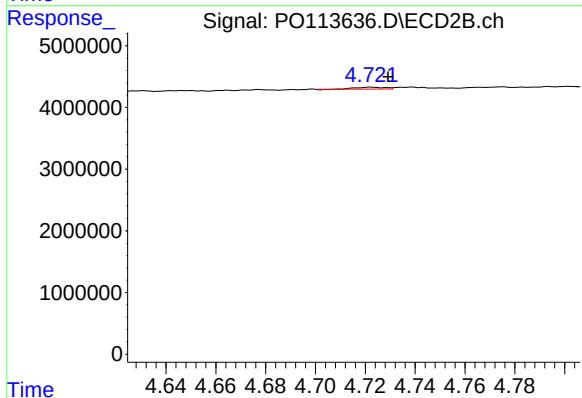


#21 AR-1248-1

R.T.: 4.722 min
Delta R.T.: -0.007 min
Response: 251025
Conc: 2.25 ng/ml

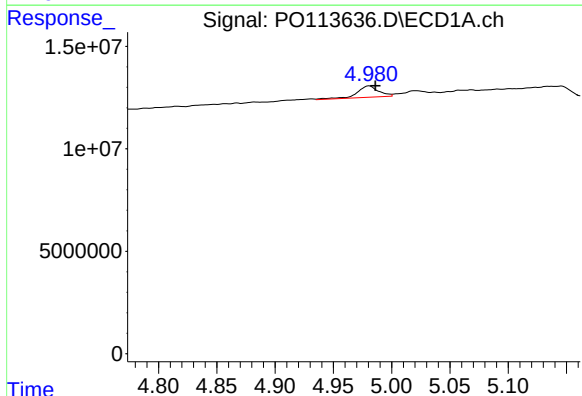


#22 AR-1248-2

R.T.: 4.981 min
Delta R.T.: -0.005 min
Response: 7191440
Conc: 29.73 ng/ml

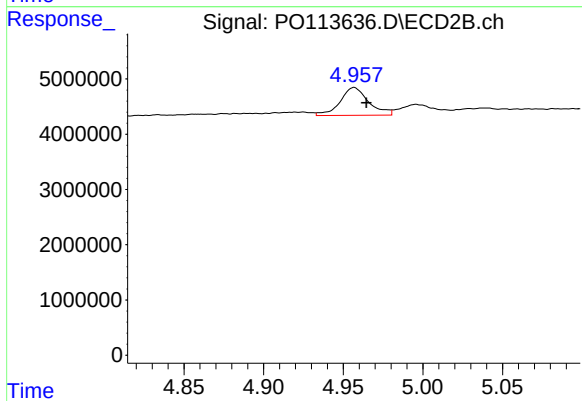

#22 AR-1248-2


R.T.: 4.957 min
Delta R.T.: -0.008 min
Response: 6307835
Conc: 39.25 ng/ml

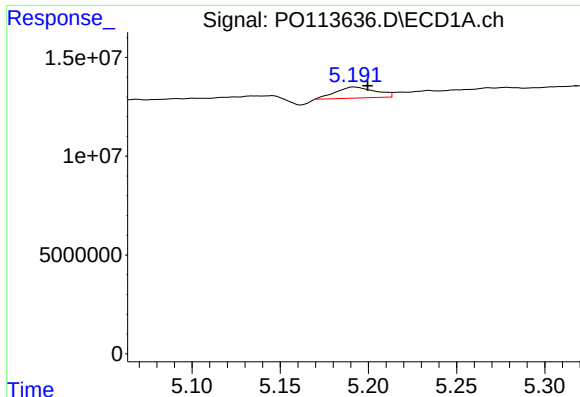

#23 AR-1248-3


R.T.: 5.192 min
Delta R.T.: -0.008 min
Response: 8693675
Conc: 27.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

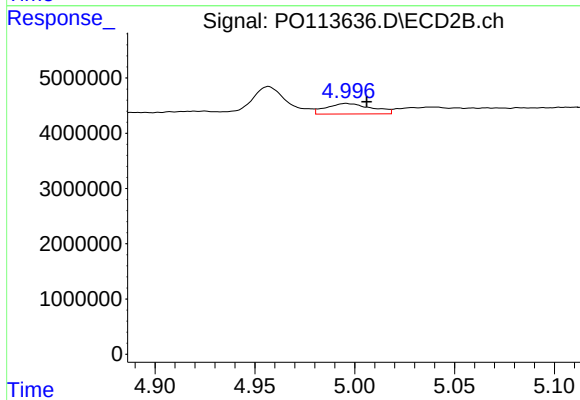


#23 AR-1248-3

R.T.: 4.996 min
Delta R.T.: -0.010 min
Response: 2995110
Conc: 17.65 ng/ml

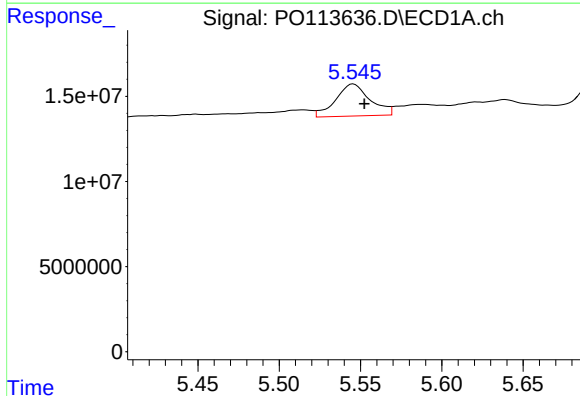


#24 AR-1248-4

R.T.: 5.546 min
Delta R.T.: -0.007 min
Response: 27679753
Conc: 55.40 ng/ml

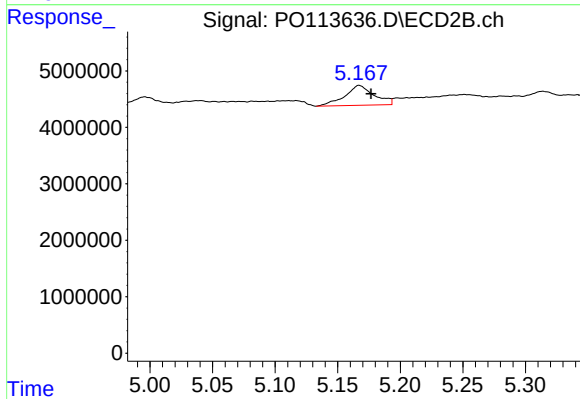

#24 AR-1248-4


R.T.: 5.167 min
Delta R.T.: -0.010 min
Response: 5755877
Conc: 28.89 ng/ml

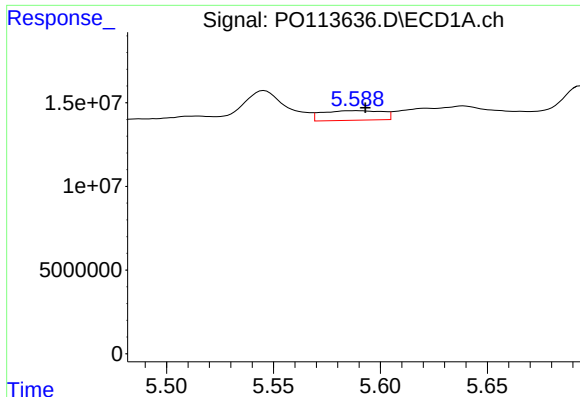

#25 AR-1248-5


R.T.: 5.588 min
Delta R.T.: -0.005 min
Response: 11265550
Conc: 32.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

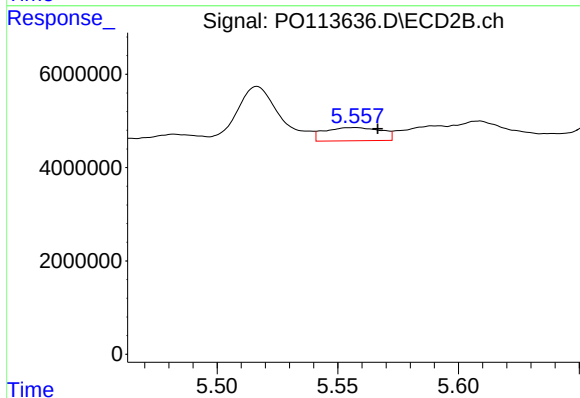


#25 AR-1248-5

R.T.: 5.557 min
Delta R.T.: -0.009 min
Response: 4630617
Conc: 21.81 ng/ml

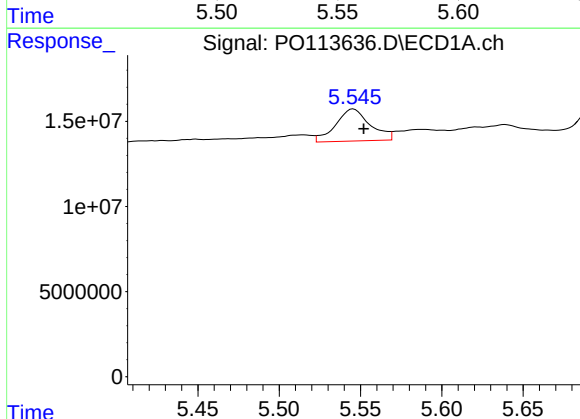


#26 AR-1254-1

R.T.: 5.546 min
Delta R.T.: -0.006 min
Response: 27679753
Conc: 51.26 ng/ml

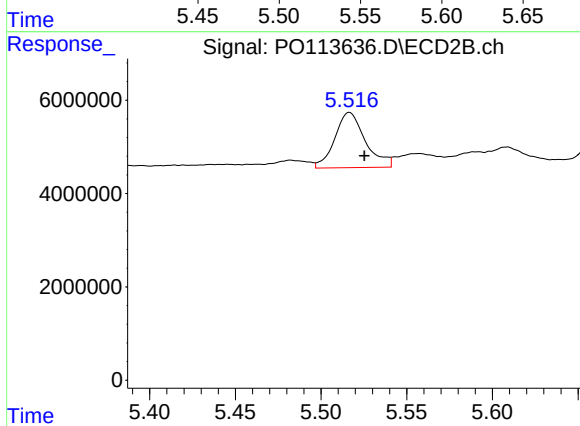

#26 AR-1254-1


R.T.: 5.517 min
Delta R.T.: -0.009 min
Response: 14665516
Conc: 46.50 ng/ml

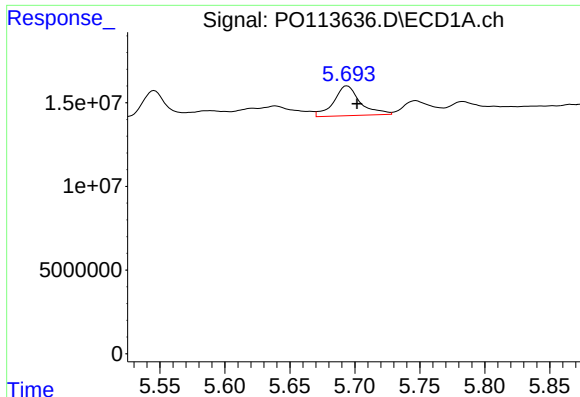

#27 AR-1254-2


R.T.: 5.694 min
Delta R.T.: -0.008 min
Response: 25363887
Conc: 51.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

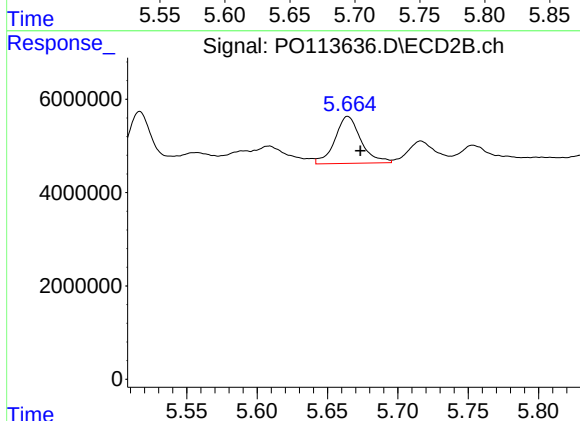


#27 AR-1254-2

R.T.: 5.664 min
Delta R.T.: -0.009 min
Response: 13002015
Conc: 46.38 ng/ml

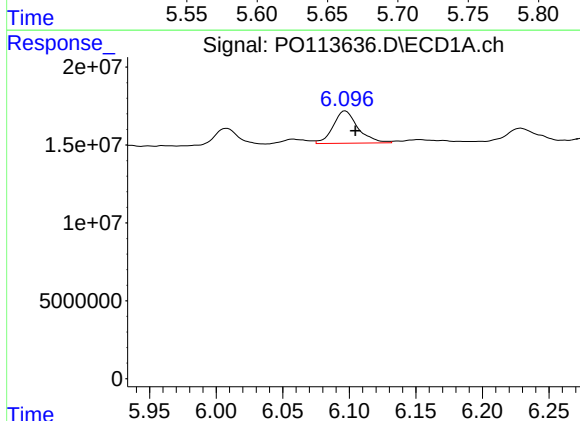


#28 AR-1254-3

R.T.: 6.097 min
Delta R.T.: -0.007 min
Response: 27079649
Conc: 36.65 ng/ml

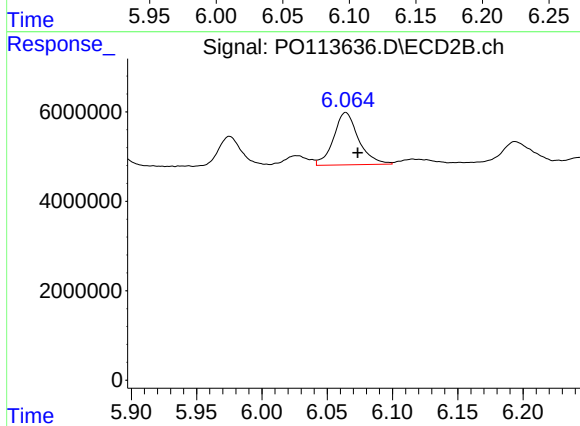

#28 AR-1254-3


R.T.: 6.064 min
Delta R.T.: -0.009 min
Response: 15620976
Conc: 37.47 ng/ml

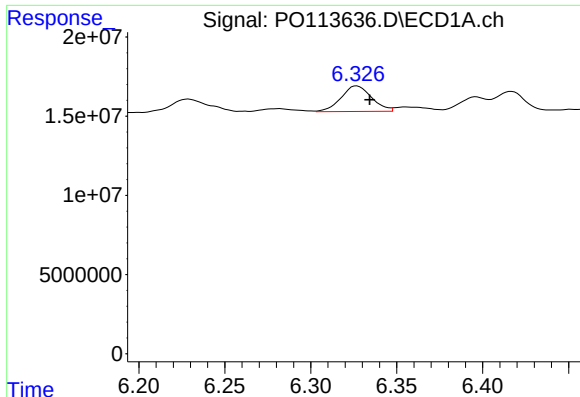

#29 AR-1254-4


R.T.: 6.327 min
Delta R.T.: -0.008 min
Response: 19959928
Conc: 35.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

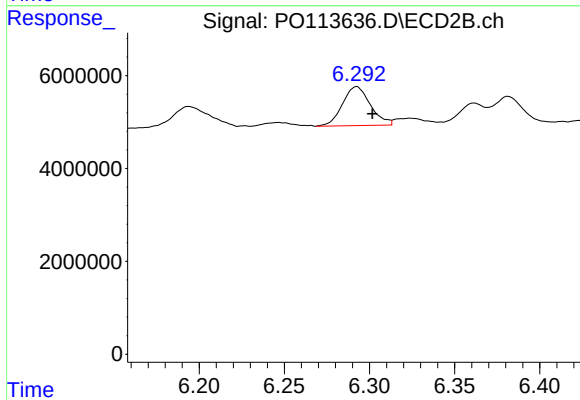


#29 AR-1254-4

R.T.: 6.293 min
Delta R.T.: -0.009 min
Response: 9574712
Conc: 34.84 ng/ml

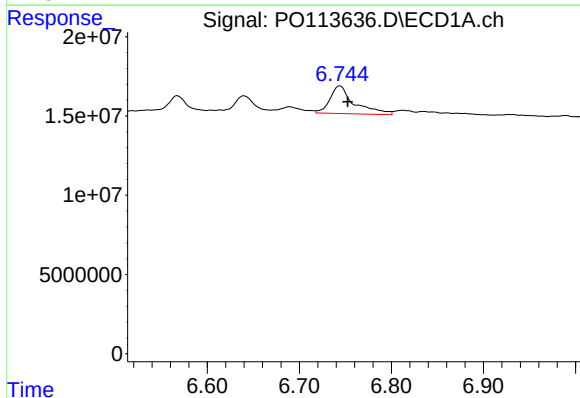


#30 AR-1254-5

R.T.: 6.744 min
Delta R.T.: -0.008 min
Response: 31983567
Conc: 45.63 ng/ml

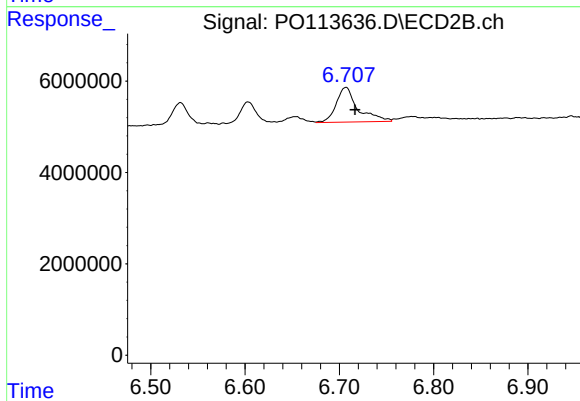

#30 AR-1254-5


R.T.: 6.707 min
Delta R.T.: -0.010 min
Response: 12201656
Conc: 34.13 ng/ml

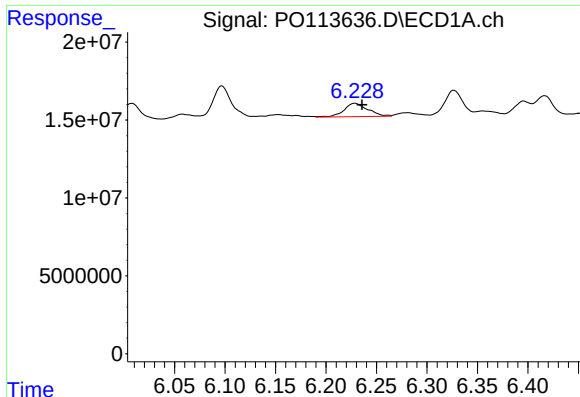

#31 AR-1260-1


R.T.: 6.229 min
Delta R.T.: -0.007 min
Response: 14201665
Conc: 31.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

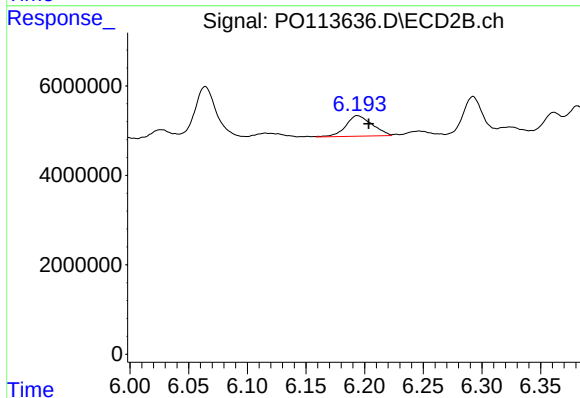


#31 AR-1260-1

R.T.: 6.194 min
Delta R.T.: -0.010 min
Response: 7171809
Conc: 28.12 ng/ml

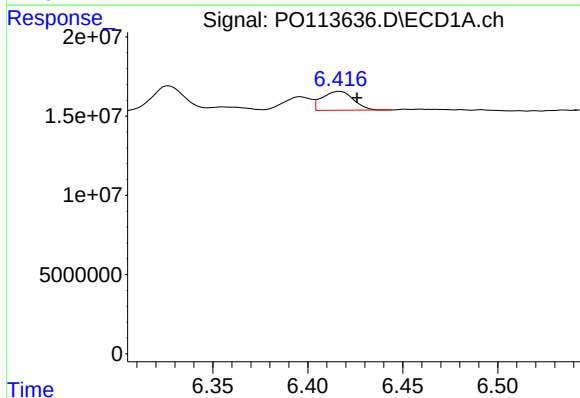


#32 AR-1260-2

R.T.: 6.417 min
Delta R.T.: -0.009 min
Response: 13722191
Conc: 19.98 ng/ml

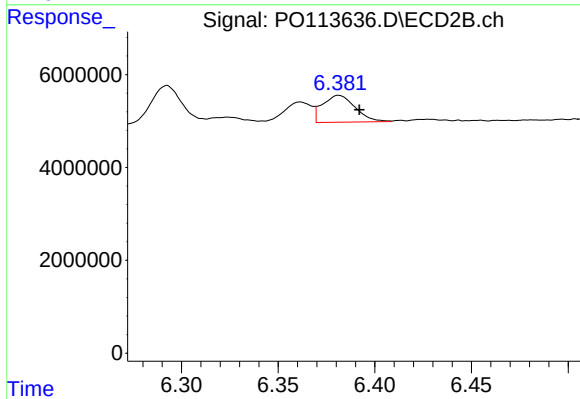

#32 AR-1260-2


R.T.: 6.381 min
Delta R.T.: -0.011 min
Response: 6824967
Conc: 19.74 ng/ml

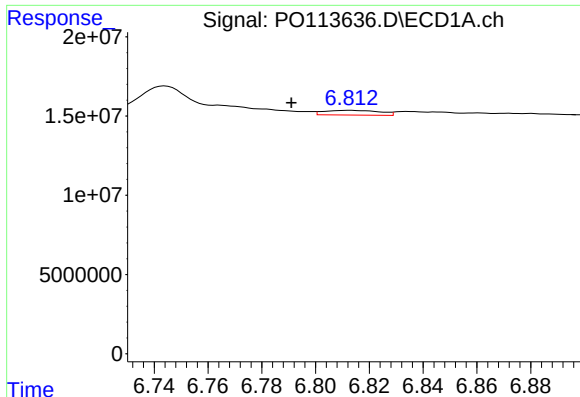

#33 AR-1260-3


R.T.: 6.813 min
Delta R.T.: 0.022 min
Response: 4314948
Conc: 6.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

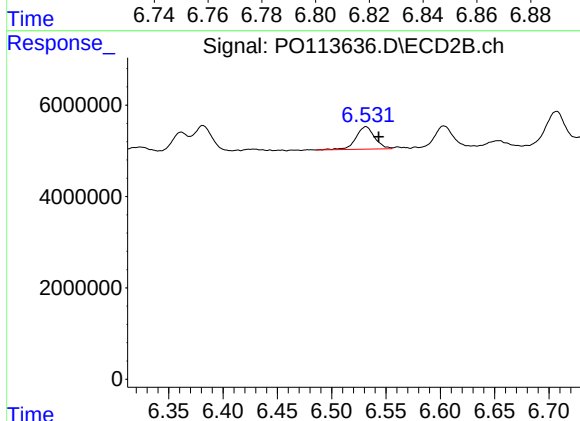


#33 AR-1260-3

R.T.: 6.532 min
Delta R.T.: -0.012 min
Response: 5904278
Conc: 19.85 ng/ml

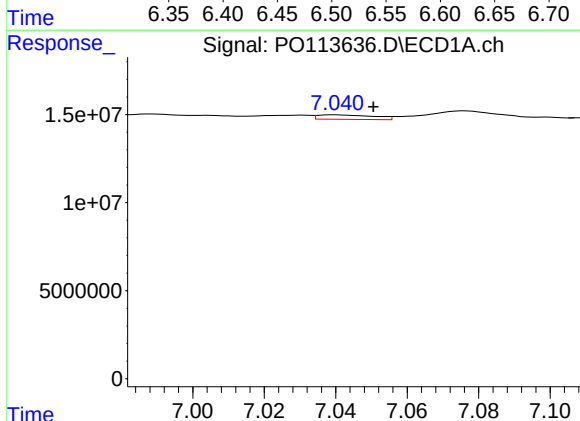


#34 AR-1260-4

R.T.: 7.040 min
Delta R.T.: -0.011 min
Response: 2762490
Conc: 6.17 ng/ml

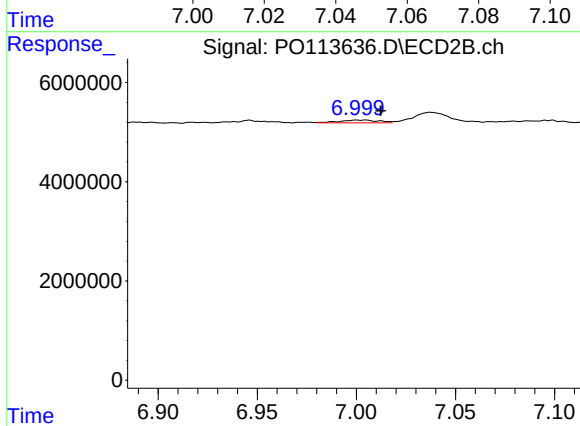

#34 AR-1260-4


R.T.: 7.004 min
Delta R.T.: -0.008 min
Response: 761088
Conc: 3.67 ng/ml

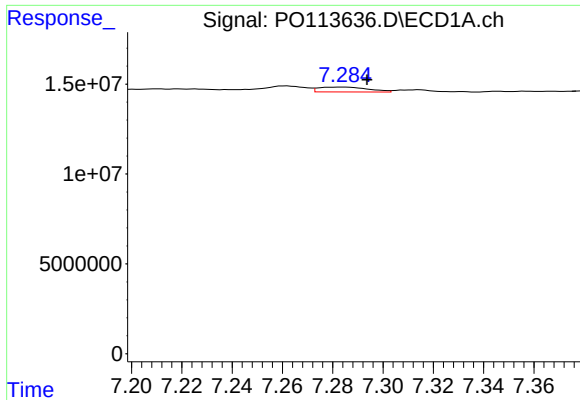

#35 AR-1260-5


R.T.: 7.284 min
Delta R.T.: -0.009 min
Response: 3743210
Conc: 3.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

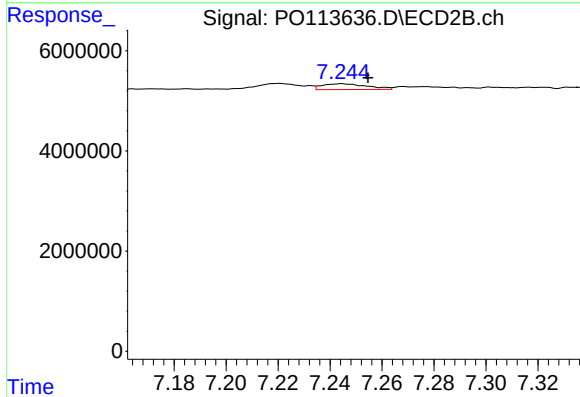


#35 AR-1260-5

R.T.: 7.244 min
Delta R.T.: -0.010 min
Response: 1389106
Conc: 2.97 ng/ml

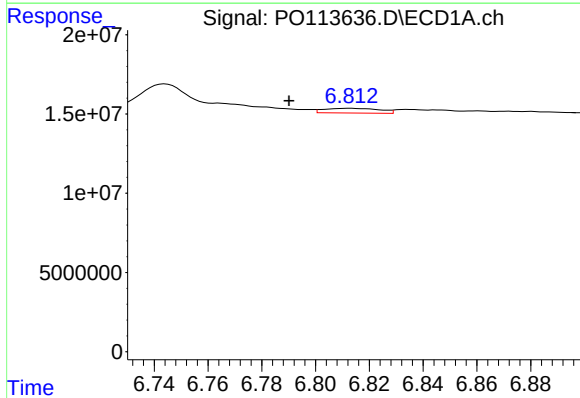


#36 AR-1262-1

R.T.: 6.813 min
Delta R.T.: 0.023 min
Response: 4314948
Conc: 4.71 ng/ml

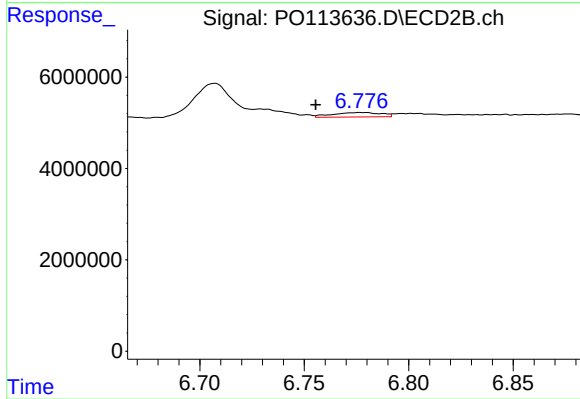

#36 AR-1262-1


R.T.: 6.777 min
Delta R.T.: 0.022 min
Response: 1574623
Conc: 3.80 ng/ml

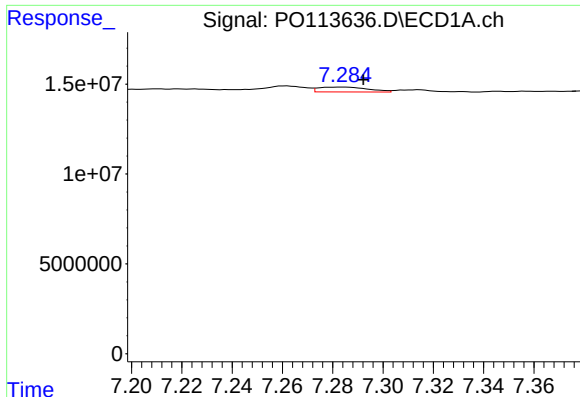

#37 AR-1262-2


R.T.: 7.284 min
Delta R.T.: -0.008 min
Response: 3743210
Conc: 2.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

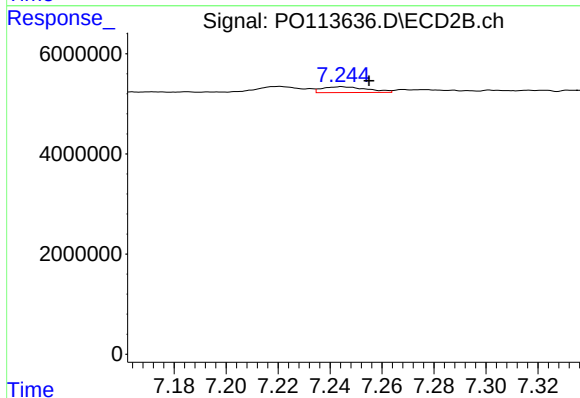


#37 AR-1262-2

R.T.: 7.244 min
Delta R.T.: -0.011 min
Response: 1389106
Conc: 2.68 ng/ml

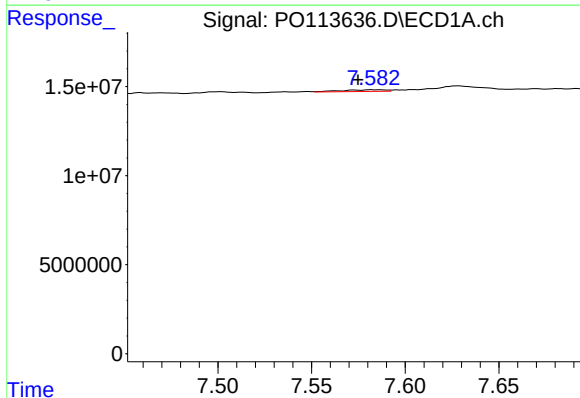


#38 AR-1262-3

R.T.: 7.582 min
Delta R.T.: 0.007 min
Response: 1564417
Conc: 2.82 ng/ml

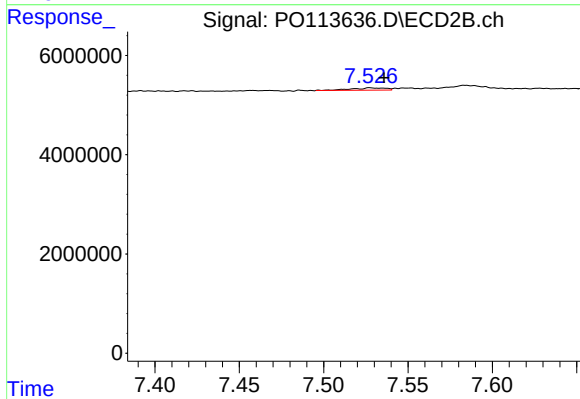

#38 AR-1262-3


R.T.: 7.527 min
Delta R.T.: -0.008 min
Response: 667649
Conc: 3.72 ng/ml

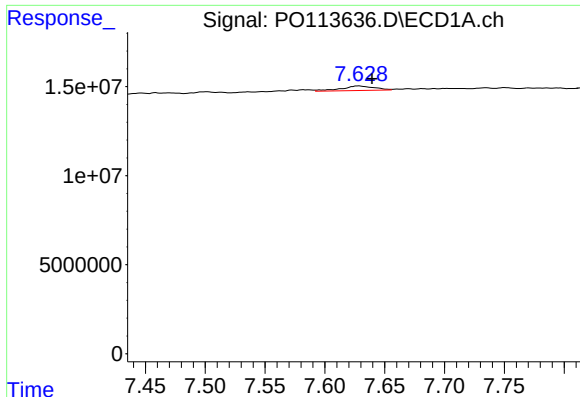

#39 AR-1262-4


R.T.: 7.628 min
Delta R.T.: -0.011 min
Response: 5040430
Conc: 5.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

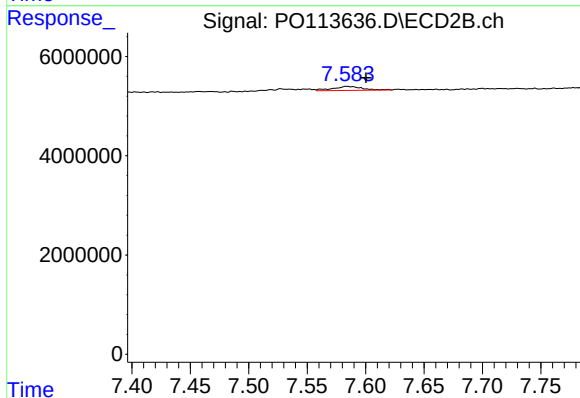


#39 AR-1262-4

R.T.: 7.584 min
Delta R.T.: -0.016 min
Response: 1463938
Conc: 5.05 ng/ml

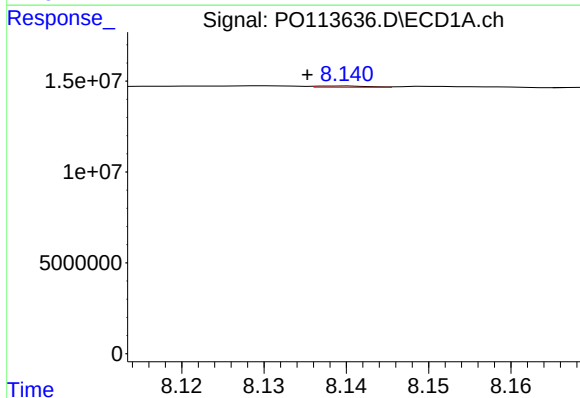


#40 AR-1262-5

R.T.: 8.140 min
Delta R.T.: 0.004 min
Response: 320002
Conc: 0.77 ng/ml

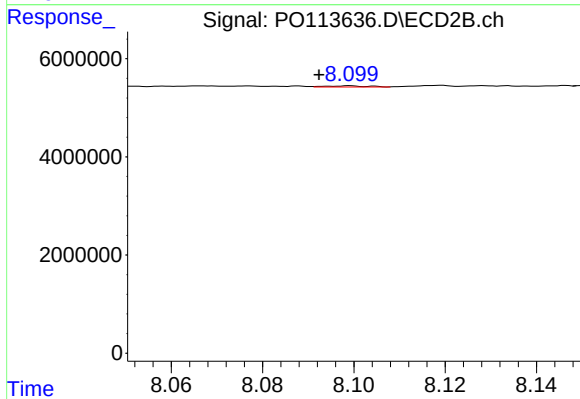

#40 AR-1262-5


R.T.: 8.099 min
Delta R.T.: 0.007 min
Response: 133894
Conc: 1.24 ng/ml

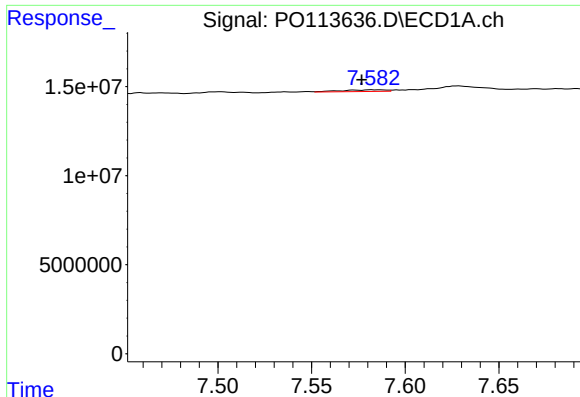

#41 AR-1268-1


R.T.: 7.582 min
Delta R.T.: 0.005 min
Response: 1564417
Conc: 0.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

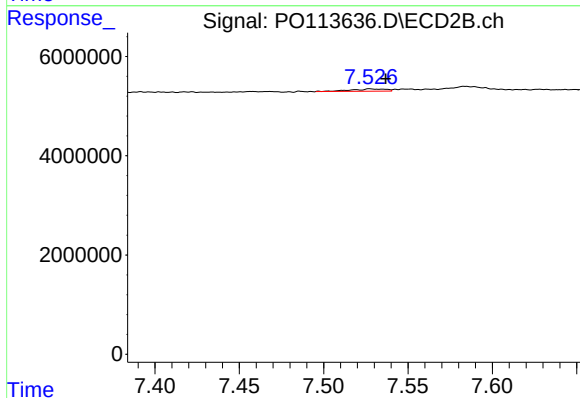


#41 AR-1268-1

R.T.: 7.527 min
Delta R.T.: -0.009 min
Response: 667649
Conc: 1.31 ng/ml

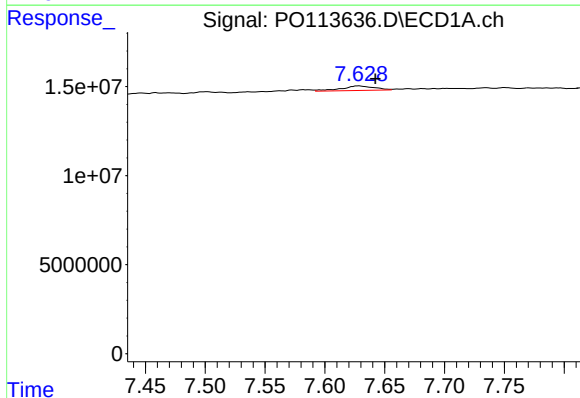


#42 AR-1268-2

R.T.: 7.628 min
Delta R.T.: -0.014 min
Response: 5040430
Conc: 3.48 ng/ml

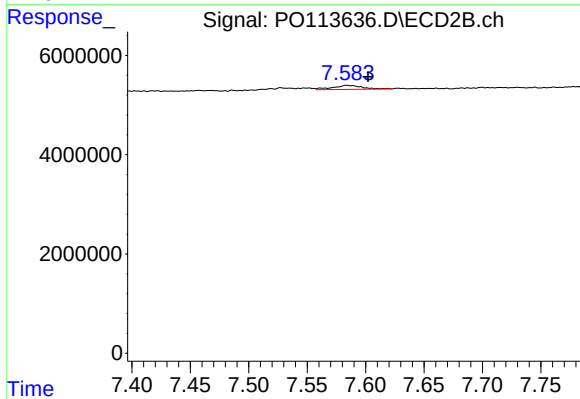

#42 AR-1268-2


R.T.: 7.584 min
Delta R.T.: -0.018 min
Response: 1463938
Conc: 3.52 ng/ml

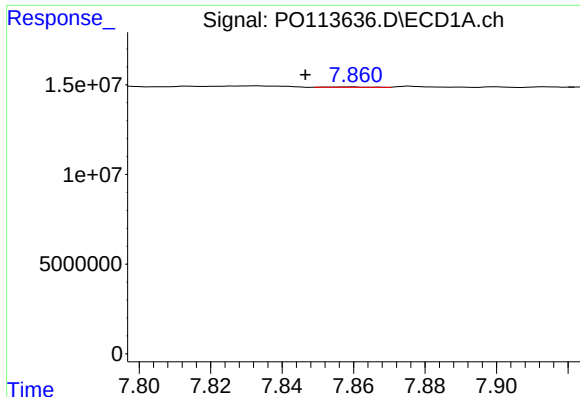

#43 AR-1268-3


R.T.: 7.860 min
Delta R.T.: 0.013 min
Response: 150542
Conc: 0.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

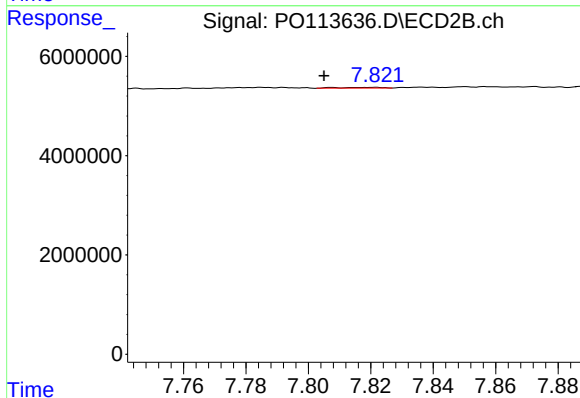


#43 AR-1268-3

R.T.: 7.821 min
Delta R.T.: 0.016 min
Response: 151611
Conc: 0.46 ng/ml

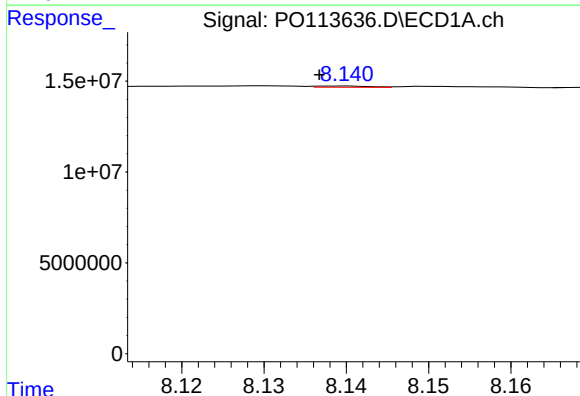


#44 AR-1268-4

R.T.: 8.140 min
Delta R.T.: 0.003 min
Response: 320002
Conc: 0.69 ng/ml

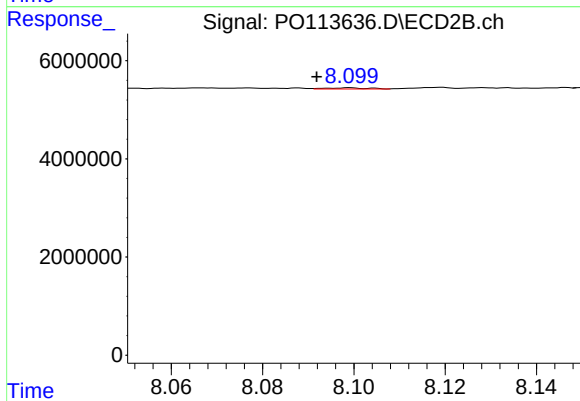

#44 AR-1268-4


R.T.: 8.099 min
Delta R.T.: 0.007 min
Response: 133894
Conc: 1.11 ng/ml

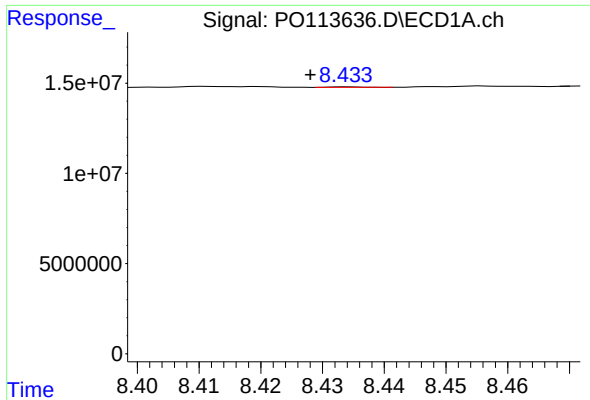

#45 AR-1268-5

R.T.: 8.434 min
Delta R.T.: 0.006 min
Response: 94063
Conc: 0.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

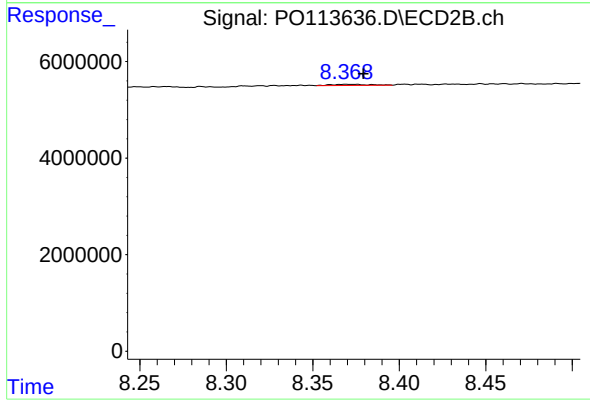

#45 AR-1268-5

R.T.: 8.369 min
Delta R.T.: -0.010 min
Response: 345709
Conc: 0.44 ng/ml