

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
 Data File : P0113637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 03:57
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1262 WATER LOD 40PPB
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:31:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.658	3.649	176.6E6	103.5E6	21.567	20.444
2)	SA Decachlor...	8.669	8.614	148.9E6	42050972	21.478	22.192
Target Compounds							
3)	L1 AR-1016-1	4.763	4.724	977545	374581	3.661	2.196 #
4)	L1 AR-1016-2	4.763	4.745	977545	94554	2.435	0.367 #
5)	L1 AR-1016-3	4.840	4.920	359758	370171	1.411	2.651 #
6)	L1 AR-1016-4	4.948	4.963	1203506	2155949	5.519	18.474 #
7)	L1 AR-1016-5	5.190	5.174	1952358	1166120	8.809	8.182
8)	L2 AR-1221-1	3.895	3.867	636167	119687	6.799	1.896 #
9)	L2 AR-1221-2	3.959	3.946	2336905	1815667	34.595	38.902
10)	L2 AR-1221-3	4.033	4.025	-85	83166	N.D.	0.560 #
11)	L3 AR-1232-1	4.033	4.018	-85	130500	N.D.	1.079 #
12)	L3 AR-1232-2	4.518	4.734	434487	387895	4.026	3.178
13)	L3 AR-1232-3	4.763	4.914	977545	576573	4.952	8.715 #
14)	L3 AR-1232-4	4.948	5.000	1203506	741481	12.244	12.373
15)	L3 AR-1232-5	4.989	5.174	1986175	1166120	30.193	17.246 #
16)	L4 AR-1242-1	4.763	4.734	977545	387895	4.251	2.684 #
17)	L4 AR-1242-2	4.763	4.745	977545	94554	2.845	0.436 #
18)	L4 AR-1242-3	4.840	4.920	359758	370171	1.621	3.165 #
19)	L4 AR-1242-4	4.948	5.008	1203506	301912	6.938	2.566 #
20)	L4 AR-1242-5	5.562	5.516	3027580	3969373	15.126	26.616 #
21)	L5 AR-1248-1	4.763	4.724	977545	374581	5.603	3.359 #
22)	L5 AR-1248-2	4.989	4.963	1986175	2155949	8.212	13.416 #
23)	L5 AR-1248-3	5.190	5.008	1952358	301912	6.123	1.780 #
24)	L5 AR-1248-4	5.546	5.174	9508352	1166120	19.032	5.853 #
25)	L5 AR-1248-5	5.562	5.568	3027580	1056106	8.866	4.975 #
26)	L6 AR-1254-1	5.546	5.516	9508352	3969373	17.609	12.587 #
27)	L6 AR-1254-2	5.696	5.664	13419128	5171318	27.194	18.447 #
28)	L6 AR-1254-3	6.112	6.080	14485220	7203678	19.604	17.278
29)	L6 AR-1254-4	6.321	6.290	4033688	231956	7.242	0.844 #
30)	L6 AR-1254-5	6.742	6.705	16517493	6566947	23.564	18.370
31)	L7 AR-1260-1	6.227	6.193	22061798	9503330	49.468	37.258
32)	L7 AR-1260-2	6.417	6.382	23948811	11015213	34.874	31.862
33)	L7 AR-1260-3	6.782	6.534	38623359	9488473	62.551	31.901 #
34)	L7 AR-1260-4	7.040	7.002	29499985	10003823	65.867	48.269 #
35)	L7 AR-1260-5	7.284	7.244	51661048	17245723	42.671	36.816
36)	L8 AR-1262-1	6.782	6.744	38623359	14539492	42.176	35.068
37)	L8 AR-1262-2	7.284	7.244	51661048	17245723	34.164	33.314
38)	L8 AR-1262-3	7.566	7.524	20413885	6056474	36.841	33.724
39)	L8 AR-1262-4	7.631	7.588	33700442	10238873	34.460	35.318
40)	L8 AR-1262-5	8.125	8.081	14789932	3706086	35.478	34.211
41)	L9 AR-1268-1	7.566	7.548	20413885	230350	11.862	0.452 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
Data File : P0113637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 03:57
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1262 WATER LOD 40PPB
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:31:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.631	7.588	33700442	10238873	23.271	24.648
43) L9	AR-1268-3	7.835	7.817	1788661	119351	1.483	0.366 #
44) L9	AR-1268-4	8.125	8.081	14789932	3706086	32.106	30.773
45) L9	AR-1268-5	8.416	8.367	4470105	1062820	1.402	1.361



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091025\
Data File : PO113637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 03:57
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1262 WATER LOD 40PPB
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:31:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

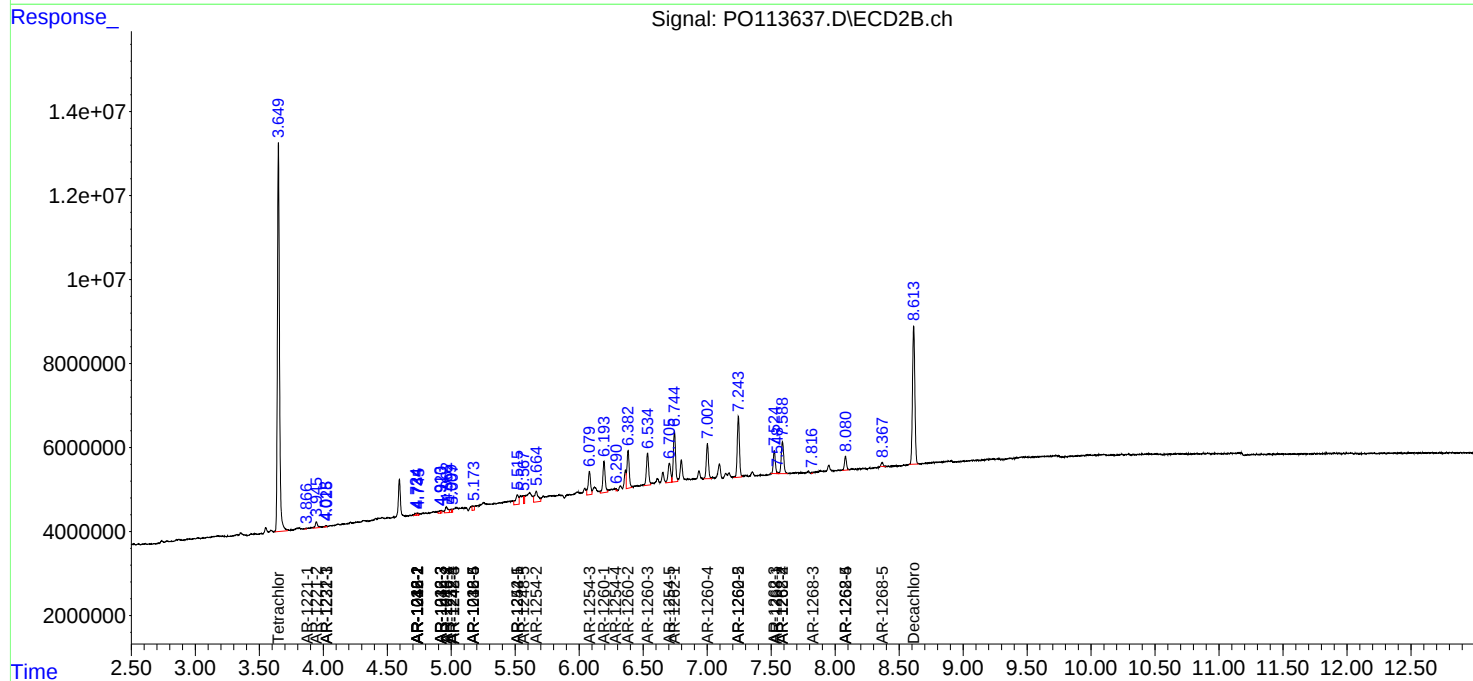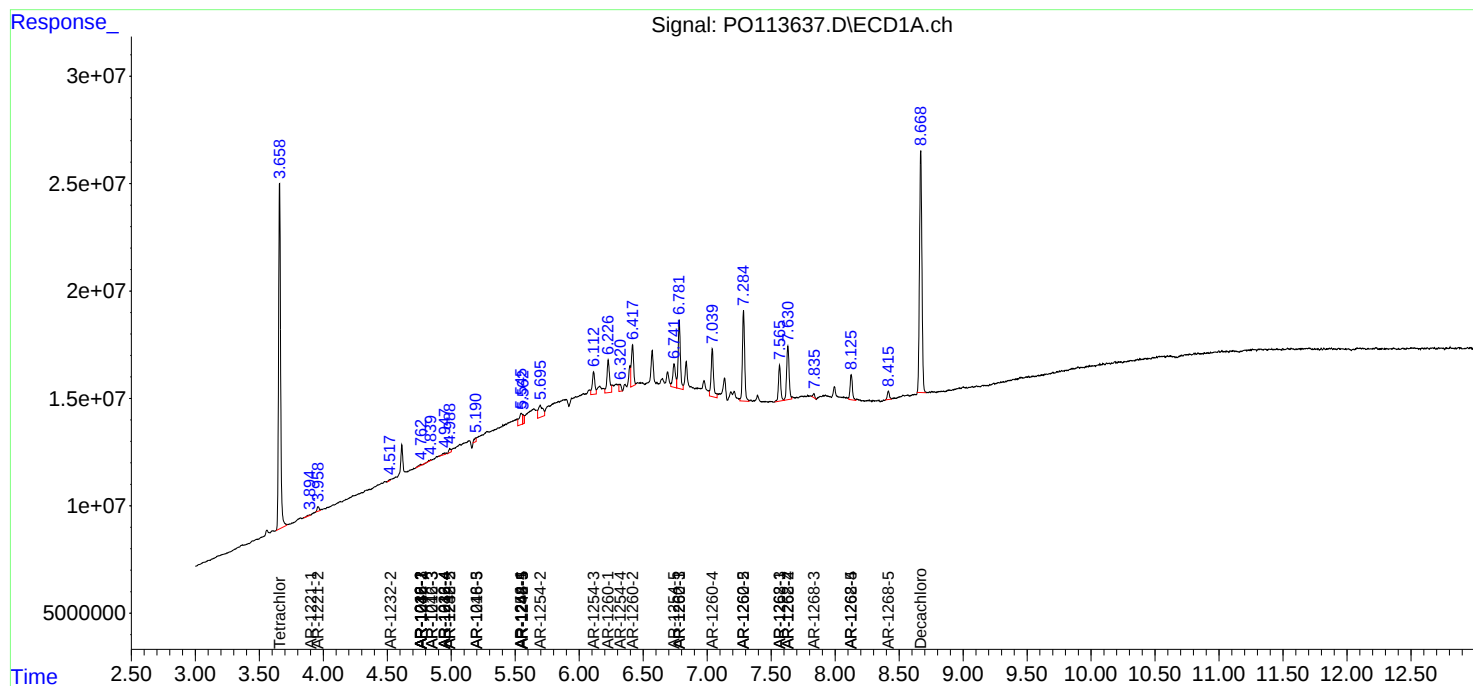


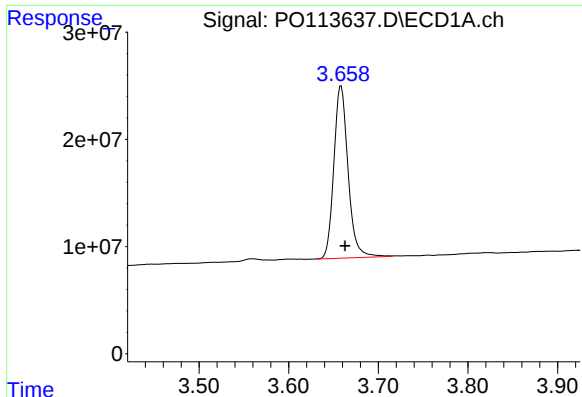

#1 Tetrachloro-m-xylene


R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 176563899
Conc: 21.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

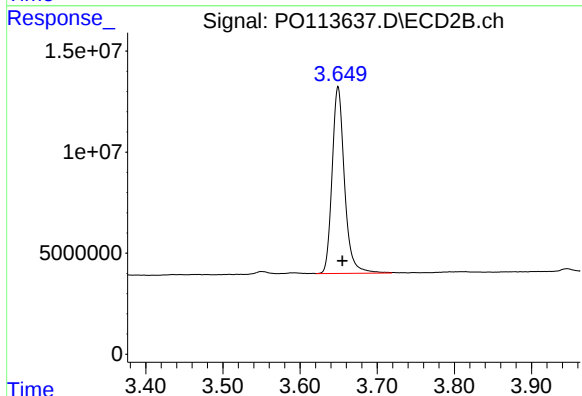


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.005 min
Response: 103459129
Conc: 20.44 ng/ml

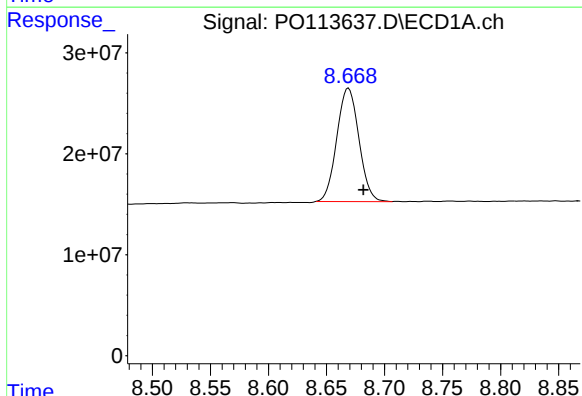


#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.013 min
Response: 148872793
Conc: 21.48 ng/ml

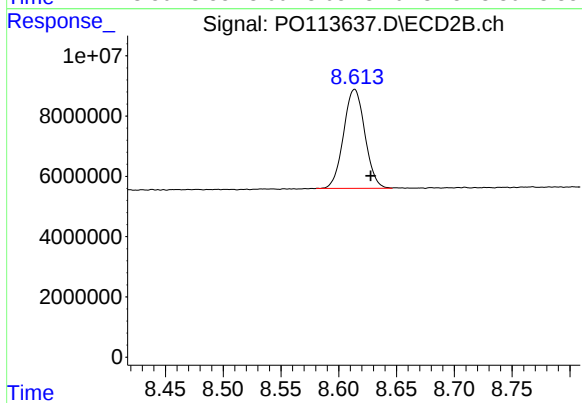

#2 Decachlorobiphenyl


R.T.: 8.614 min
Delta R.T.: -0.014 min
Response: 42050972
Conc: 22.19 ng/ml

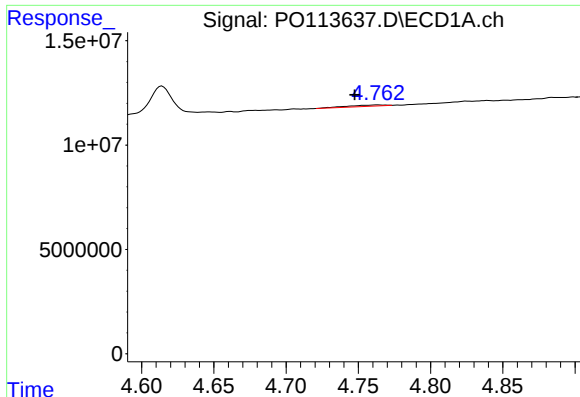

#3 AR-1016-1


R.T.: 4.763 min
Delta R.T.: 0.015 min
Response: 977545
Conc: 3.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

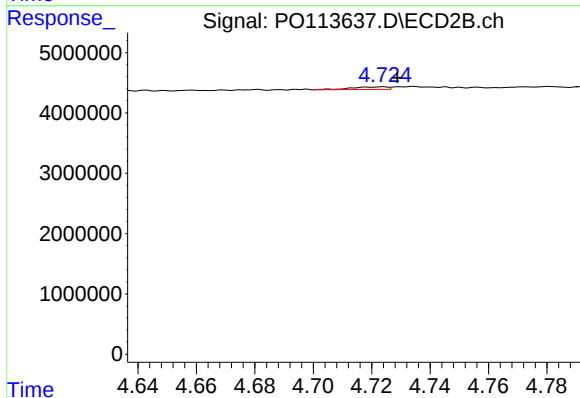


#3 AR-1016-1

R.T.: 4.724 min
Delta R.T.: -0.005 min
Response: 374581
Conc: 2.20 ng/ml

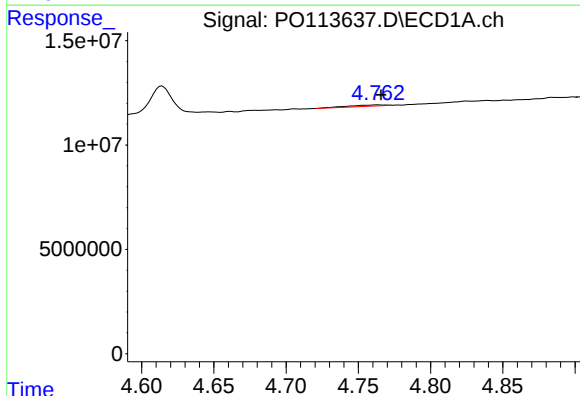


#4 AR-1016-2

R.T.: 4.763 min
Delta R.T.: -0.003 min
Response: 977545
Conc: 2.44 ng/ml

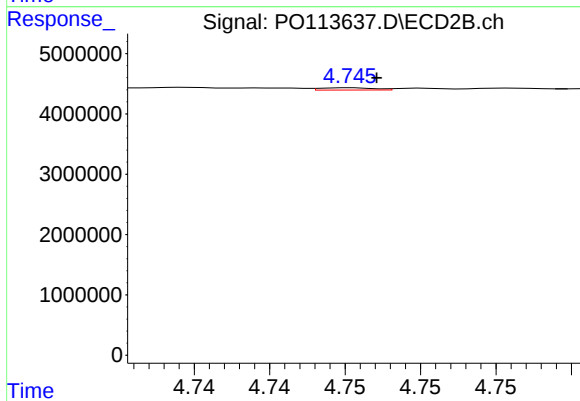

#4 AR-1016-2


R.T.: 4.745 min
Delta R.T.: -0.002 min
Response: 94554
Conc: 0.37 ng/ml

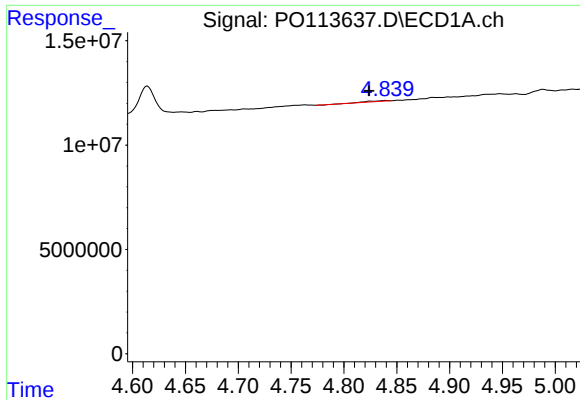

#5 AR-1016-3


R.T.: 4.840 min
Delta R.T.: 0.016 min
Response: 359758
Conc: 1.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

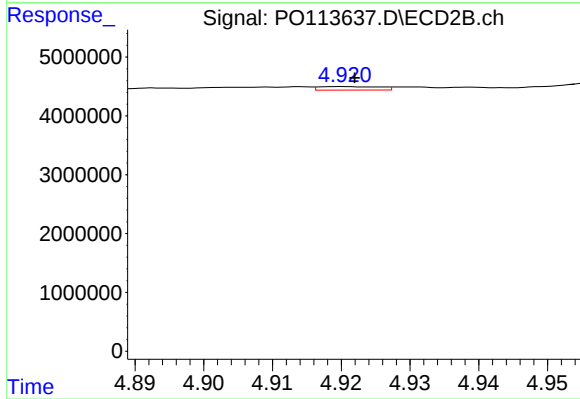


#5 AR-1016-3

R.T.: 4.920 min
Delta R.T.: -0.002 min
Response: 370171
Conc: 2.65 ng/ml

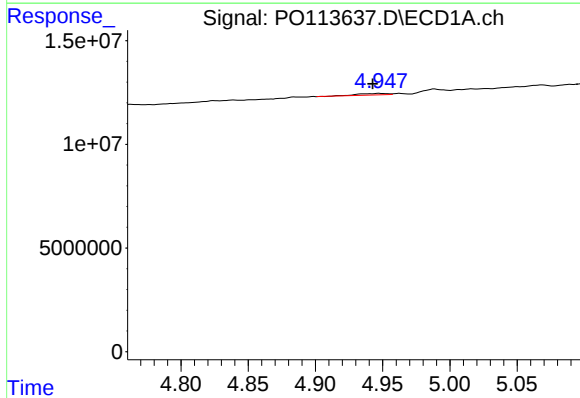


#6 AR-1016-4

R.T.: 4.948 min
Delta R.T.: 0.005 min
Response: 1203506
Conc: 5.52 ng/ml

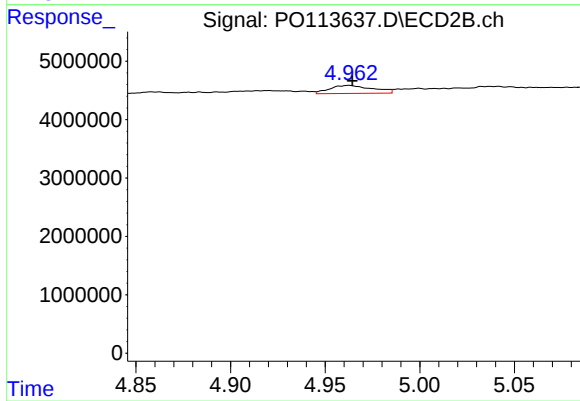

#6 AR-1016-4


R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 2155949
Conc: 18.47 ng/ml

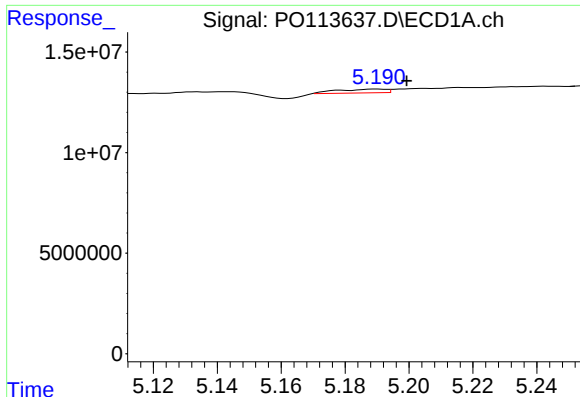

#7 AR-1016-5


R.T.: 5.190 min
Delta R.T.: -0.009 min
Response: 1952358
Conc: 8.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

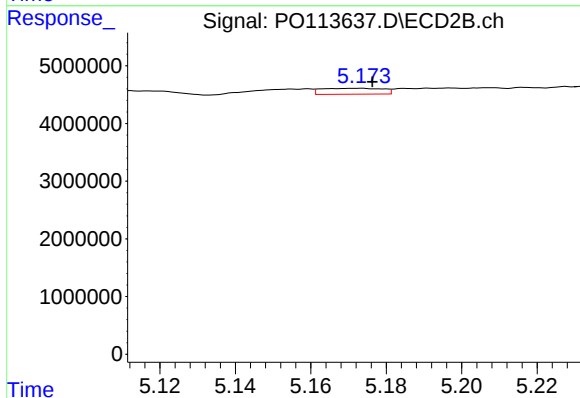


#7 AR-1016-5

R.T.: 5.174 min
Delta R.T.: -0.003 min
Response: 1166120
Conc: 8.18 ng/ml

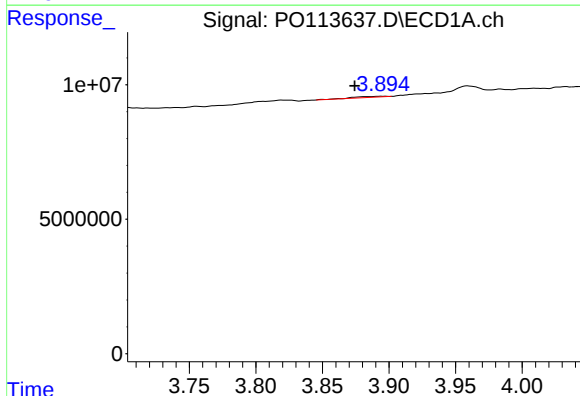


#8 AR-1221-1

R.T.: 3.895 min
Delta R.T.: 0.021 min
Response: 636167
Conc: 6.80 ng/ml

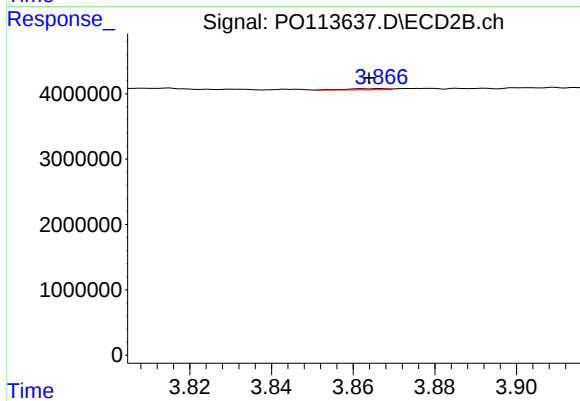

#8 AR-1221-1


R.T.: 3.867 min
Delta R.T.: 0.003 min
Response: 119687
Conc: 1.90 ng/ml

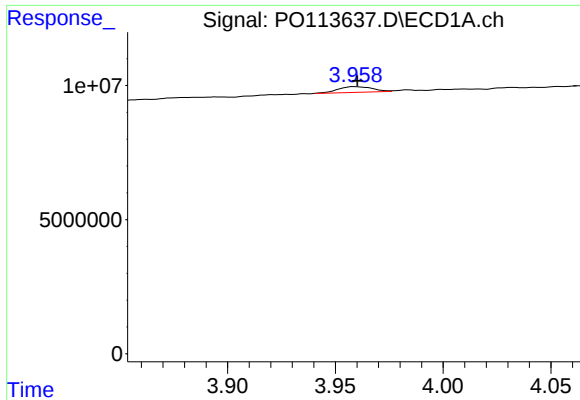

#9 AR-1221-2


R.T.: 3.959 min
Delta R.T.: -0.001 min
Response: 2336905
Conc: 34.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

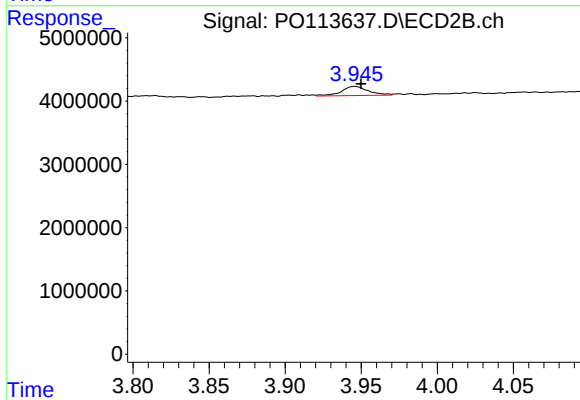


#9 AR-1221-2

R.T.: 3.946 min
Delta R.T.: -0.004 min
Response: 1815667
Conc: 38.90 ng/ml

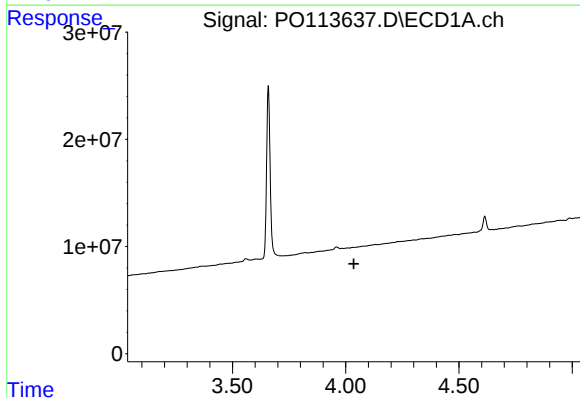


#10 AR-1221-3

R.T.: 4.033 min
Delta R.T.: -0.003 min
Response: -85
Conc: N.D.

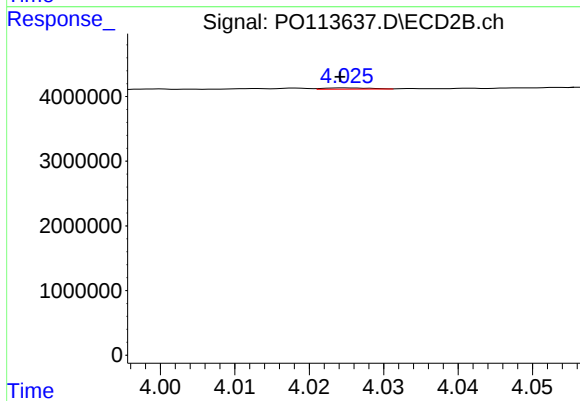

#10 AR-1221-3


R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 83166
Conc: 0.56 ng/ml

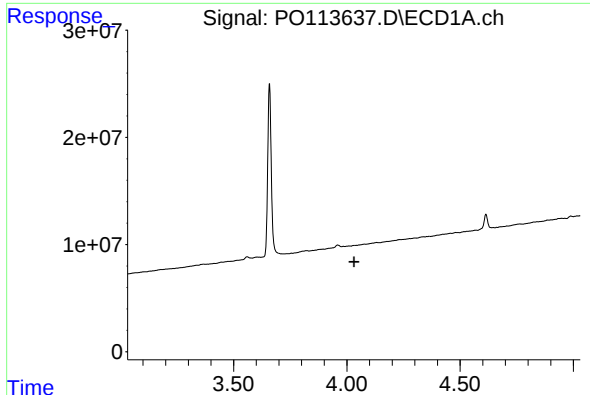

#11 AR-1232-1


R.T.: 4.033 min
Delta R.T.: 0.000 min
Response: -85
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

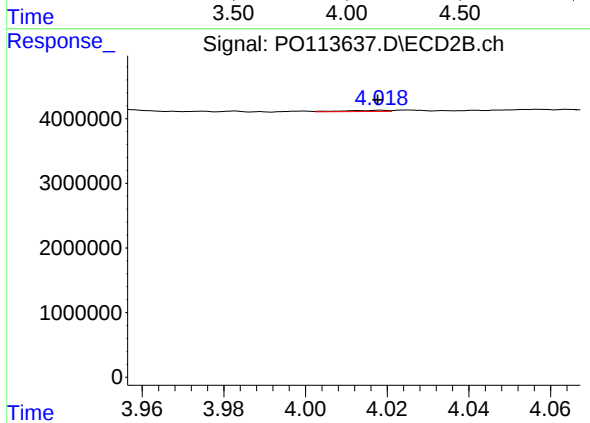


#11 AR-1232-1

R.T.: 4.018 min
Delta R.T.: 0.000 min
Response: 130500
Conc: 1.08 ng/ml

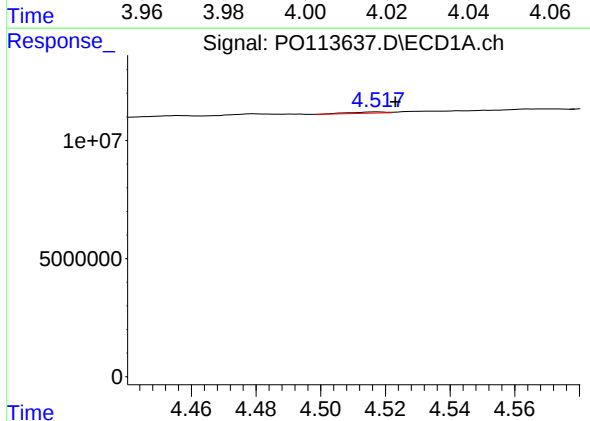


#12 AR-1232-2

R.T.: 4.518 min
Delta R.T.: -0.005 min
Response: 434487
Conc: 4.03 ng/ml

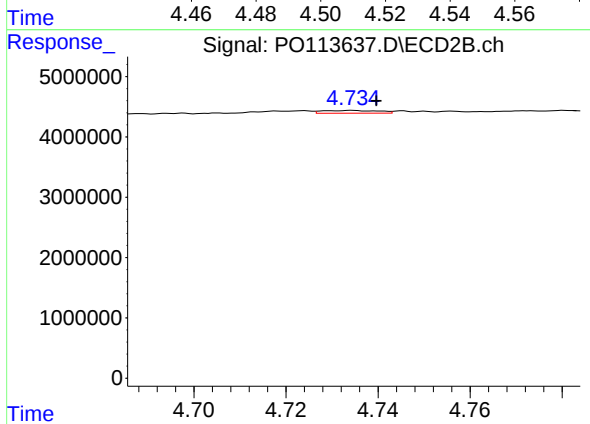

#12 AR-1232-2


R.T.: 4.734 min
Delta R.T.: -0.005 min
Response: 387895
Conc: 3.18 ng/ml

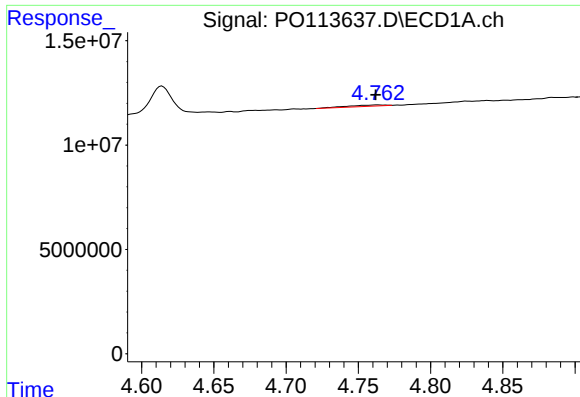

#13 AR-1232-3


R.T.: 4.763 min
Delta R.T.: 0.001 min
Response: 977545
Conc: 4.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

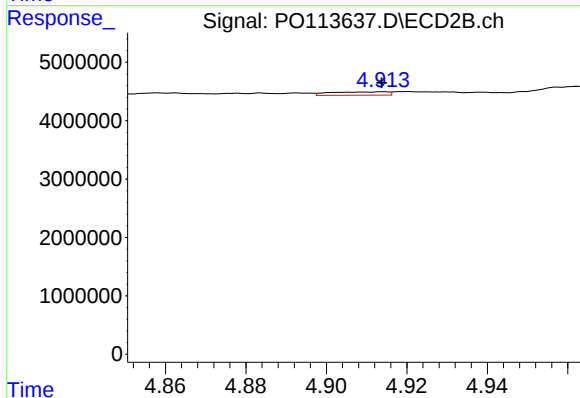


#13 AR-1232-3

R.T.: 4.914 min
Delta R.T.: 0.000 min
Response: 576573
Conc: 8.72 ng/ml

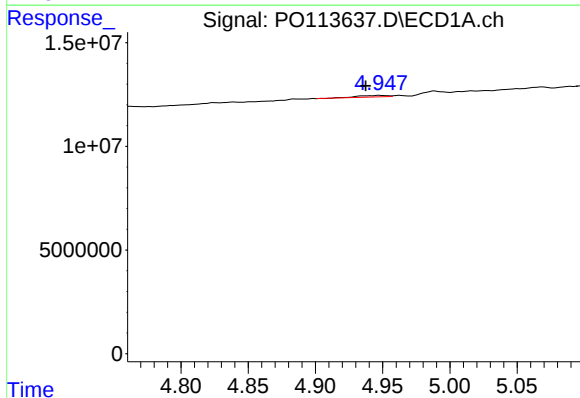


#14 AR-1232-4

R.T.: 4.948 min
Delta R.T.: 0.010 min
Response: 1203506
Conc: 12.24 ng/ml

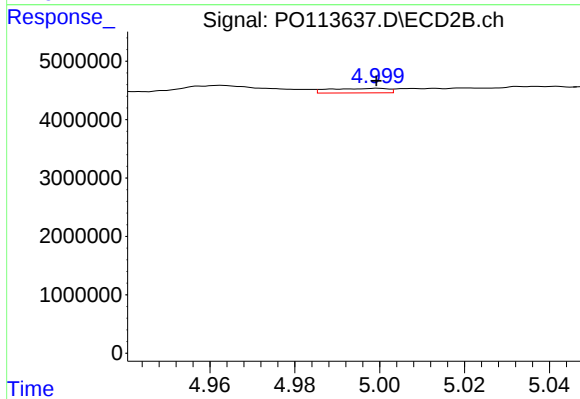

#14 AR-1232-4


R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 741481
Conc: 12.37 ng/ml

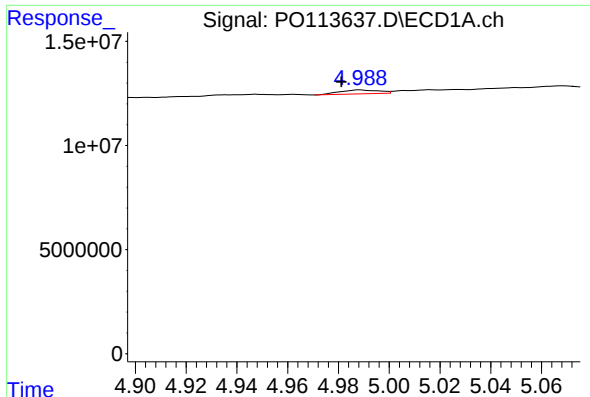

#15 AR-1232-5


R.T.: 4.989 min
Delta R.T.: 0.007 min
Response: 1986175
Conc: 30.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

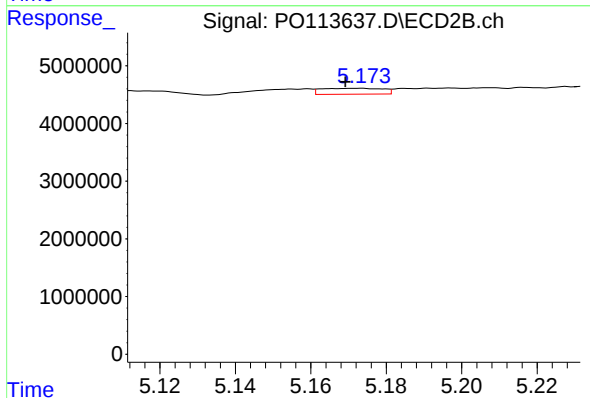


#15 AR-1232-5

R.T.: 5.174 min
Delta R.T.: 0.004 min
Response: 1166120
Conc: 17.25 ng/ml

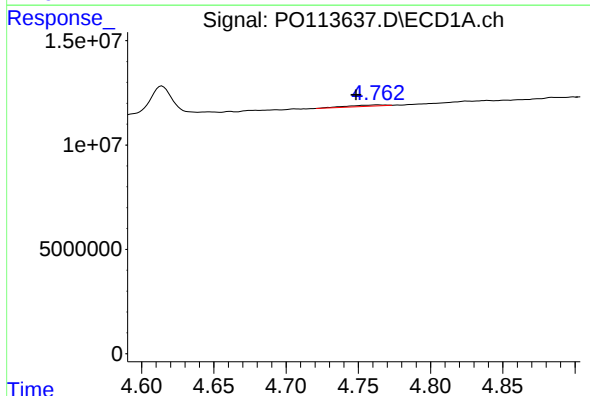


#16 AR-1242-1

R.T.: 4.763 min
Delta R.T.: 0.015 min
Response: 977545
Conc: 4.25 ng/ml

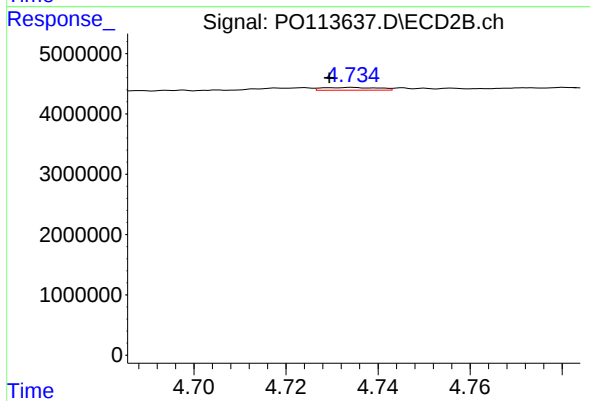

#16 AR-1242-1


R.T.: 4.734 min
Delta R.T.: 0.005 min
Response: 387895
Conc: 2.68 ng/ml

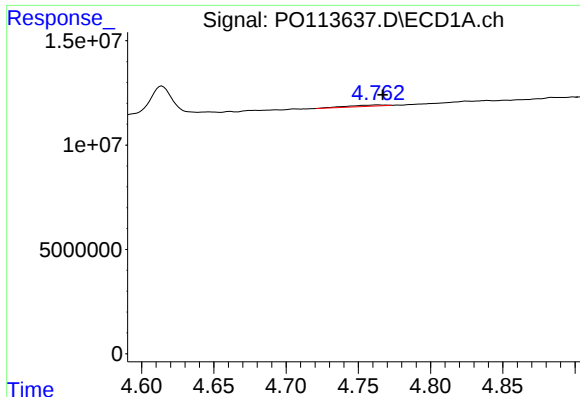

#17 AR-1242-2


R.T.: 4.763 min
Delta R.T.: -0.004 min
Response: 977545
Conc: 2.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

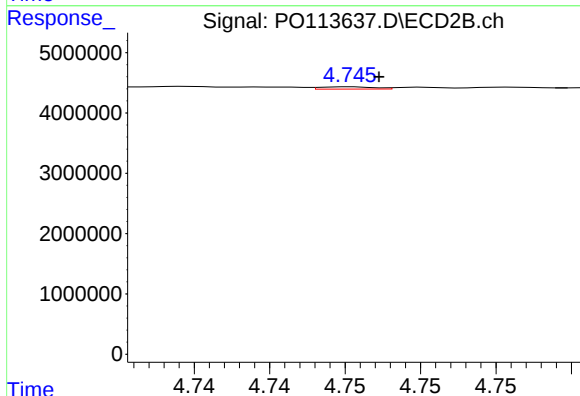


#17 AR-1242-2

R.T.: 4.745 min
Delta R.T.: -0.002 min
Response: 94554
Conc: 0.44 ng/ml

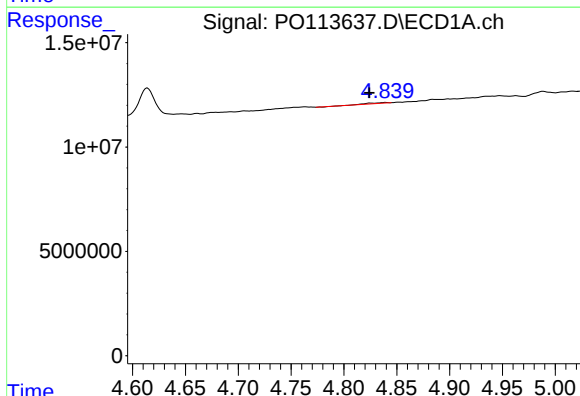


#18 AR-1242-3

R.T.: 4.840 min
Delta R.T.: 0.016 min
Response: 359758
Conc: 1.62 ng/ml

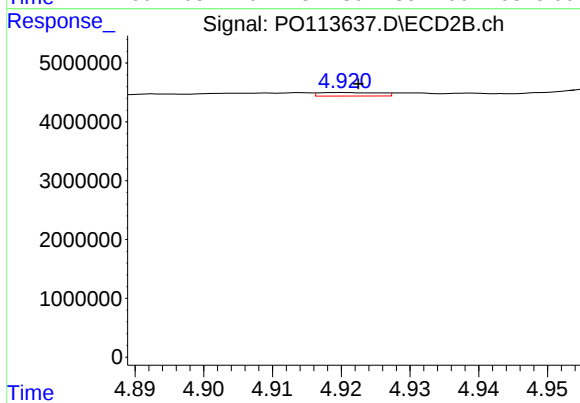

#18 AR-1242-3


R.T.: 4.920 min
Delta R.T.: -0.002 min
Response: 370171
Conc: 3.16 ng/ml

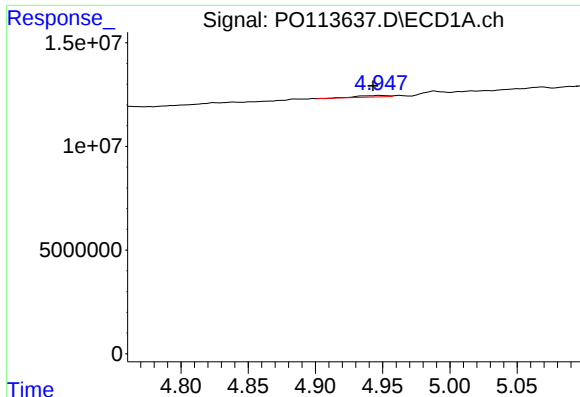

#19 AR-1242-4


R.T.: 4.948 min
Delta R.T.: 0.005 min
Response: 1203506
Conc: 6.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

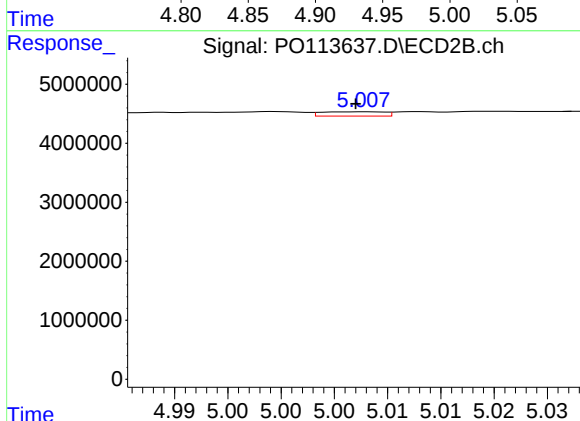


#19 AR-1242-4

R.T.: 5.008 min
Delta R.T.: 0.000 min
Response: 301912
Conc: 2.57 ng/ml

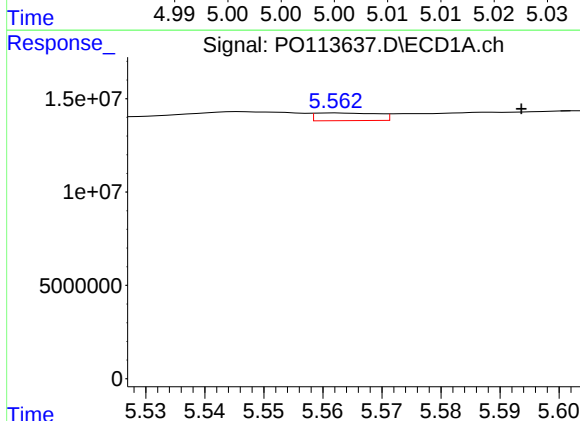


#20 AR-1242-5

R.T.: 5.562 min
Delta R.T.: -0.031 min
Response: 3027580
Conc: 15.13 ng/ml

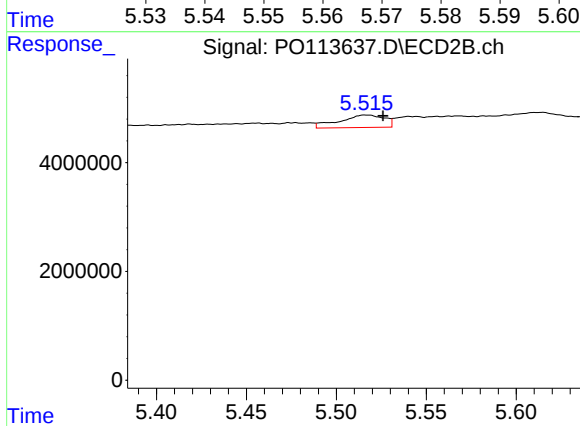

#20 AR-1242-5


R.T.: 5.516 min
Delta R.T.: -0.010 min
Response: 3969373
Conc: 26.62 ng/ml

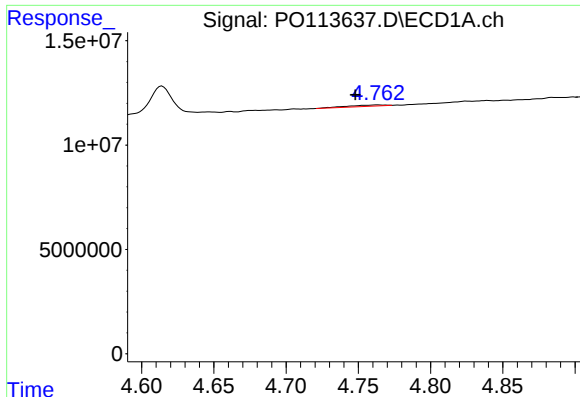

#21 AR-1248-1


R.T.: 4.763 min
Delta R.T.: 0.015 min
Response: 977545
Conc: 5.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

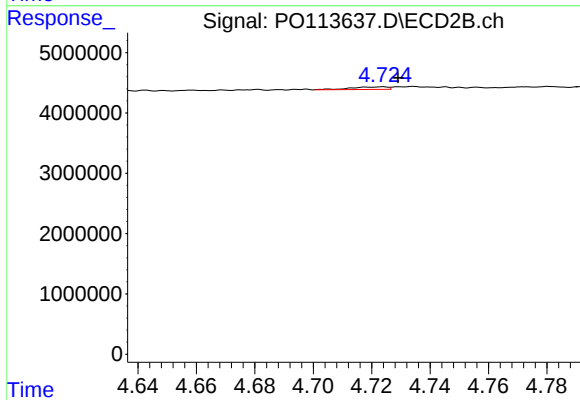


#21 AR-1248-1

R.T.: 4.724 min
Delta R.T.: -0.005 min
Response: 374581
Conc: 3.36 ng/ml

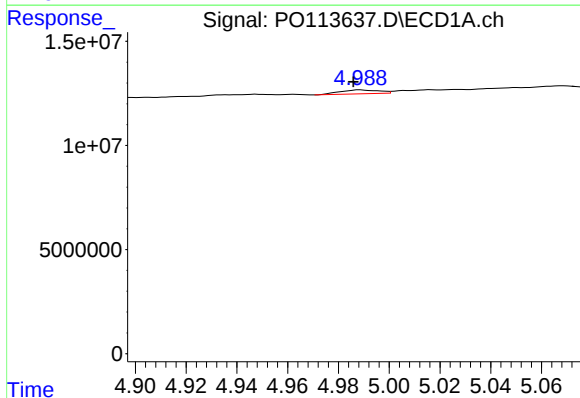


#22 AR-1248-2

R.T.: 4.989 min
Delta R.T.: 0.003 min
Response: 1986175
Conc: 8.21 ng/ml

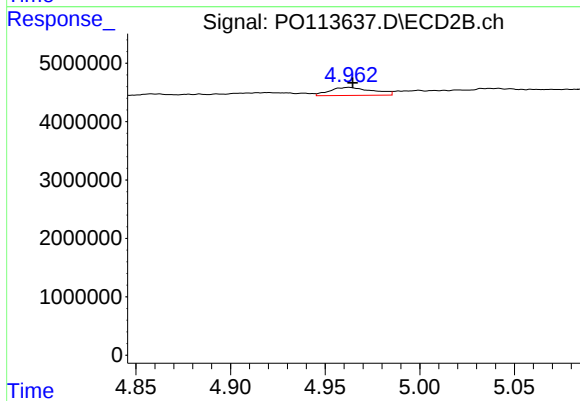

#22 AR-1248-2


R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 2155949
Conc: 13.42 ng/ml

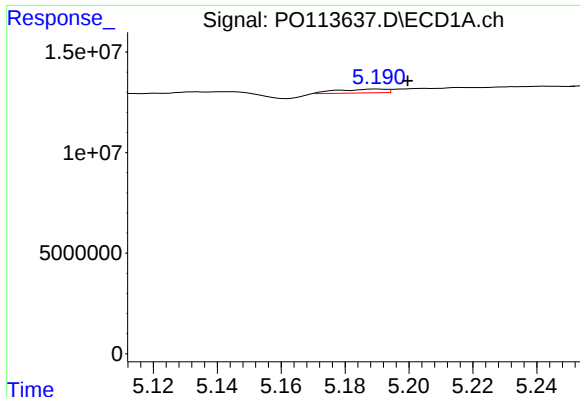

#23 AR-1248-3


R.T.: 5.190 min
Delta R.T.: -0.010 min
Response: 1952358
Conc: 6.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

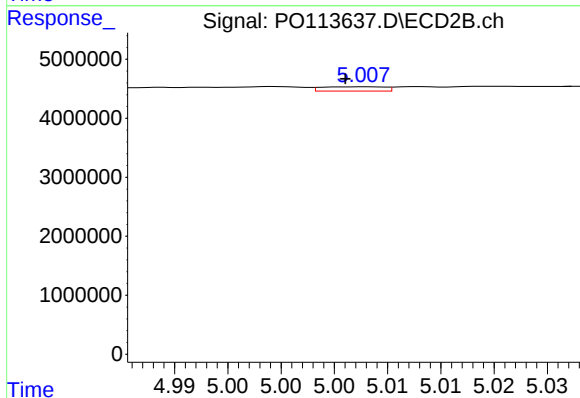


#23 AR-1248-3

R.T.: 5.008 min
Delta R.T.: 0.002 min
Response: 301912
Conc: 1.78 ng/ml

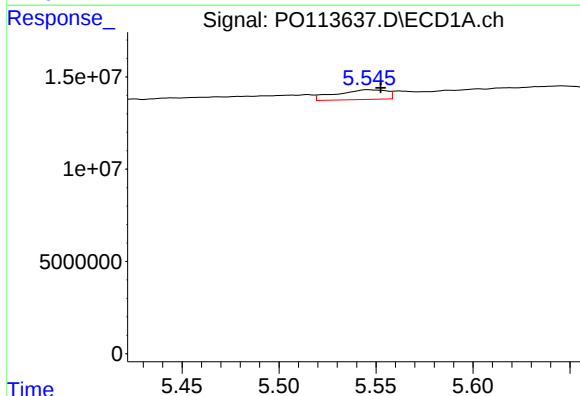


#24 AR-1248-4

R.T.: 5.546 min
Delta R.T.: -0.007 min
Response: 9508352
Conc: 19.03 ng/ml

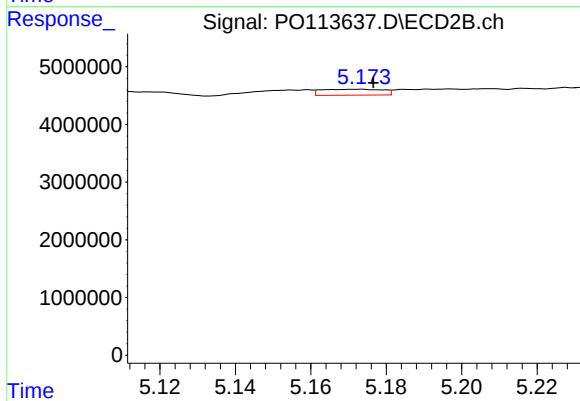

#24 AR-1248-4


R.T.: 5.174 min
Delta R.T.: -0.003 min
Response: 1166120
Conc: 5.85 ng/ml

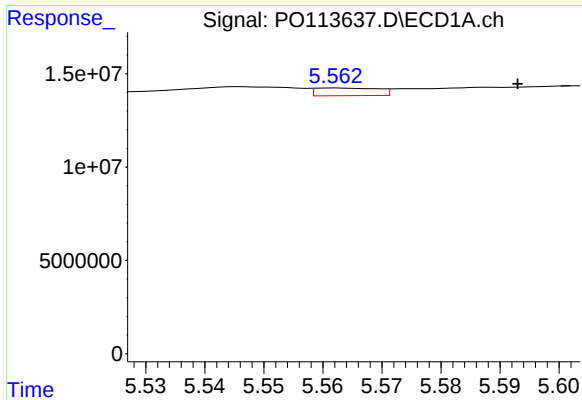

#25 AR-1248-5


R.T.: 5.562 min
Delta R.T.: -0.031 min
Response: 3027580
Conc: 8.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

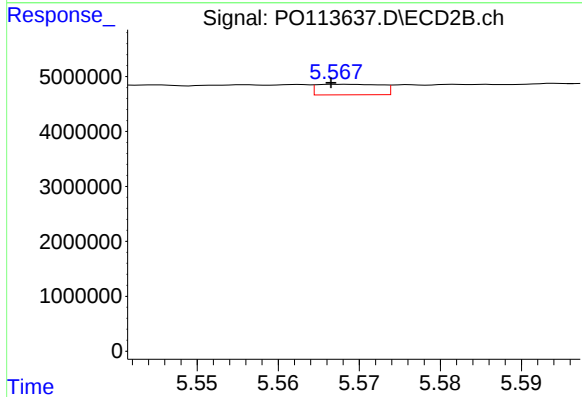


#25 AR-1248-5

R.T.: 5.568 min
Delta R.T.: 0.001 min
Response: 1056106
Conc: 4.97 ng/ml

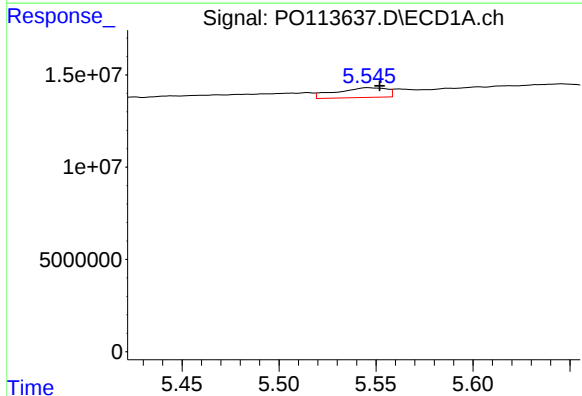


#26 AR-1254-1

R.T.: 5.546 min
Delta R.T.: -0.006 min
Response: 9508352
Conc: 17.61 ng/ml

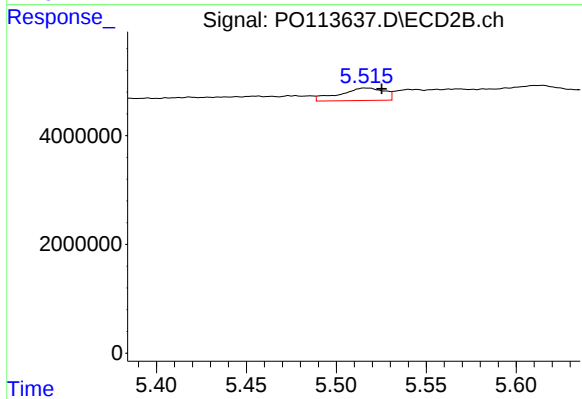

#26 AR-1254-1


R.T.: 5.516 min
Delta R.T.: -0.010 min
Response: 3969373
Conc: 12.59 ng/ml

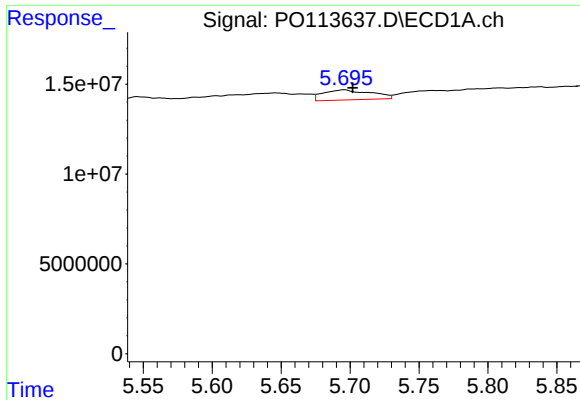

#27 AR-1254-2


R.T.: 5.696 min
Delta R.T.: -0.006 min
Response: 13419128
Conc: 27.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

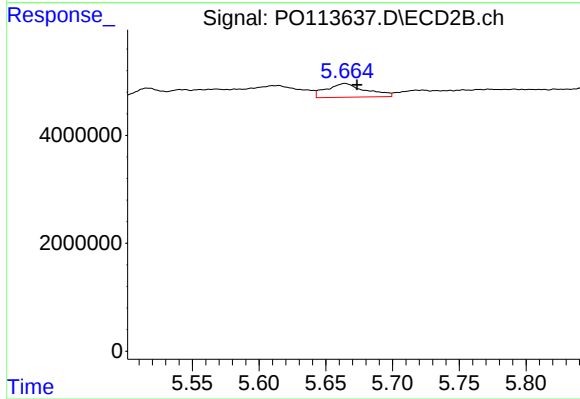


#27 AR-1254-2

R.T.: 5.664 min
Delta R.T.: -0.009 min
Response: 5171318
Conc: 18.45 ng/ml

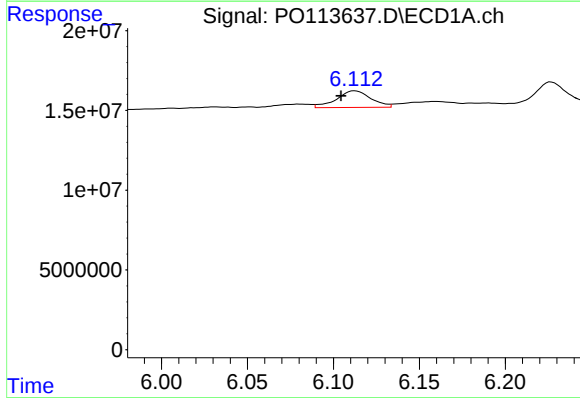


#28 AR-1254-3

R.T.: 6.112 min
Delta R.T.: 0.008 min
Response: 14485220
Conc: 19.60 ng/ml

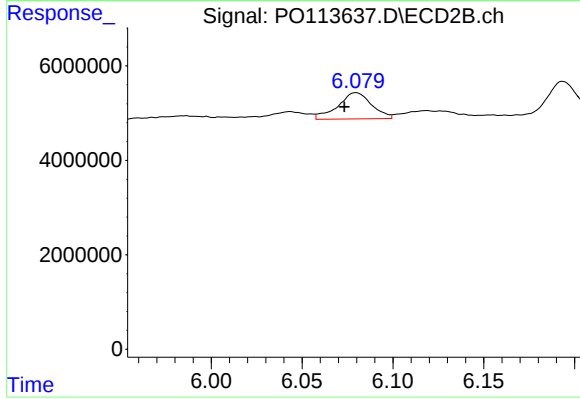

#28 AR-1254-3


R.T.: 6.080 min
Delta R.T.: 0.006 min
Response: 7203678
Conc: 17.28 ng/ml

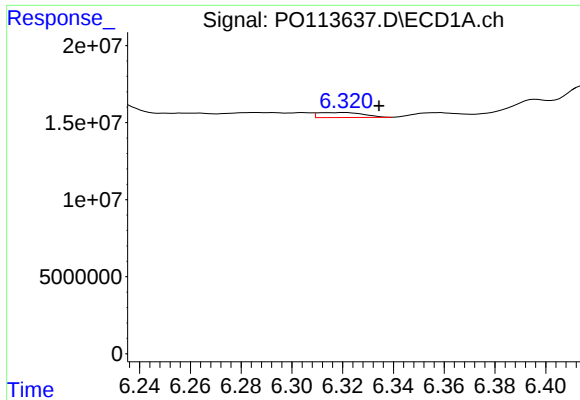

#29 AR-1254-4


R.T.: 6.321 min
Delta R.T.: -0.014 min
Response: 4033688
Conc: 7.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

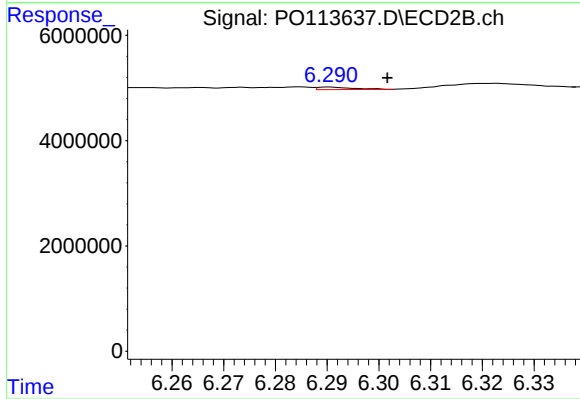


#29 AR-1254-4

R.T.: 6.290 min
Delta R.T.: -0.011 min
Response: 231956
Conc: 0.84 ng/ml

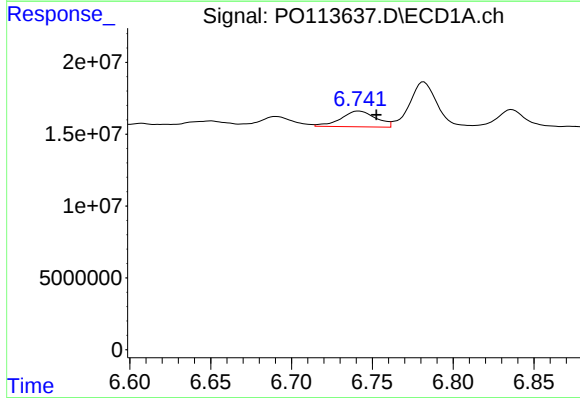


#30 AR-1254-5

R.T.: 6.742 min
Delta R.T.: -0.011 min
Response: 16517493
Conc: 23.56 ng/ml

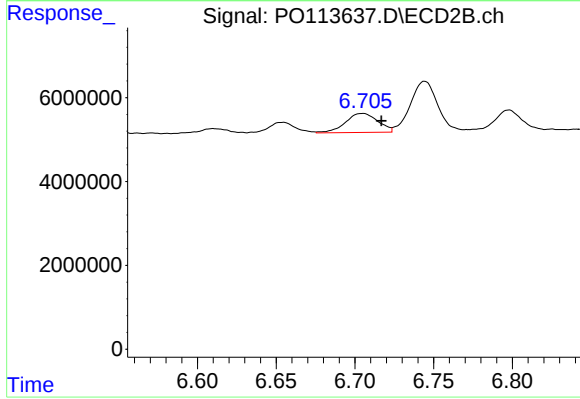

#30 AR-1254-5


R.T.: 6.705 min
Delta R.T.: -0.011 min
Response: 6566947
Conc: 18.37 ng/ml

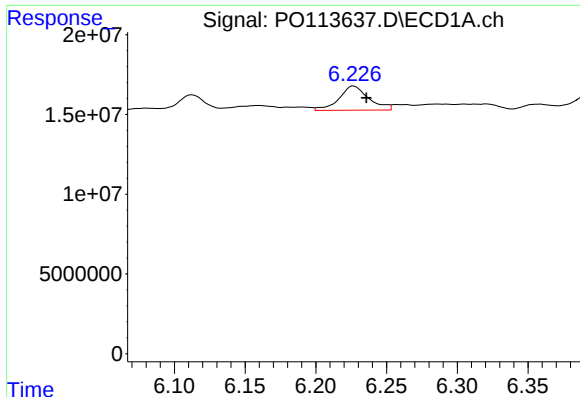

#31 AR-1260-1


R.T.: 6.227 min
Delta R.T.: -0.009 min
Response: 22061798
Conc: 49.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

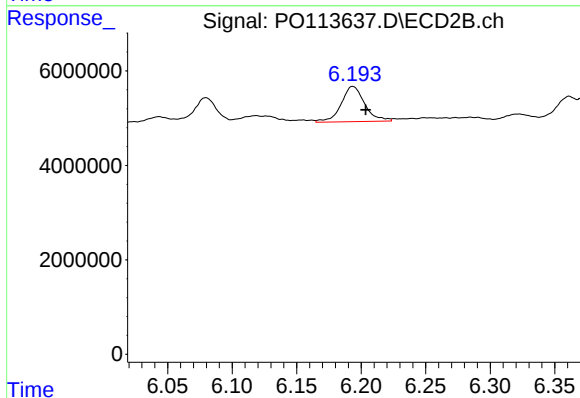


#31 AR-1260-1

R.T.: 6.193 min
Delta R.T.: -0.010 min
Response: 9503330
Conc: 37.26 ng/ml

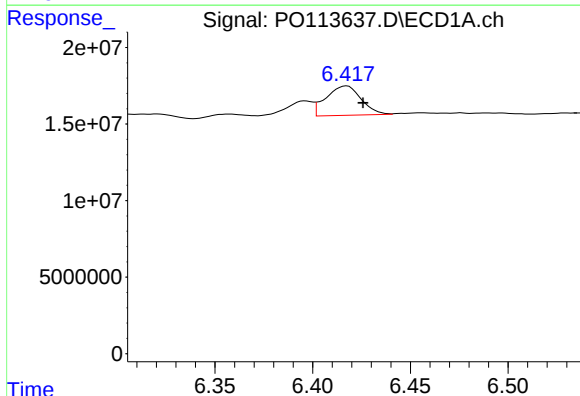


#32 AR-1260-2

R.T.: 6.417 min
Delta R.T.: -0.008 min
Response: 23948811
Conc: 34.87 ng/ml

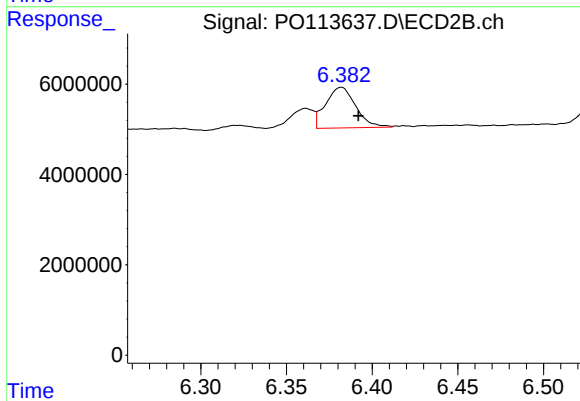

#32 AR-1260-2


R.T.: 6.382 min
Delta R.T.: -0.010 min
Response: 11015213
Conc: 31.86 ng/ml

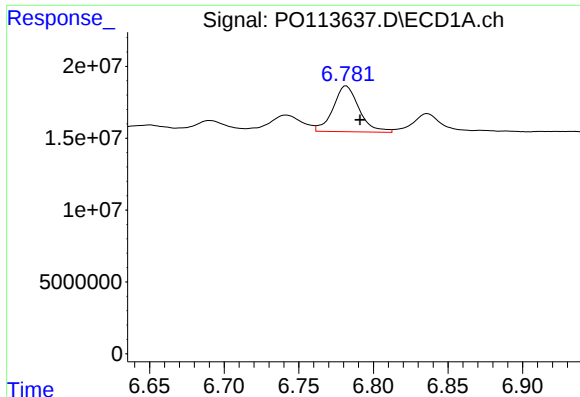

#33 AR-1260-3


R.T.: 6.782 min
Delta R.T.: -0.009 min
Response: 38623359
Conc: 62.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

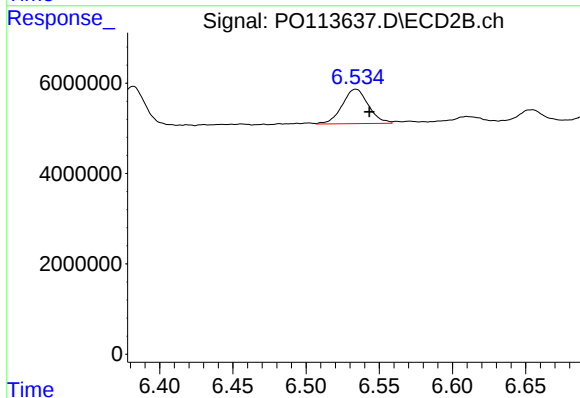


#33 AR-1260-3

R.T.: 6.534 min
Delta R.T.: -0.009 min
Response: 9488473
Conc: 31.90 ng/ml

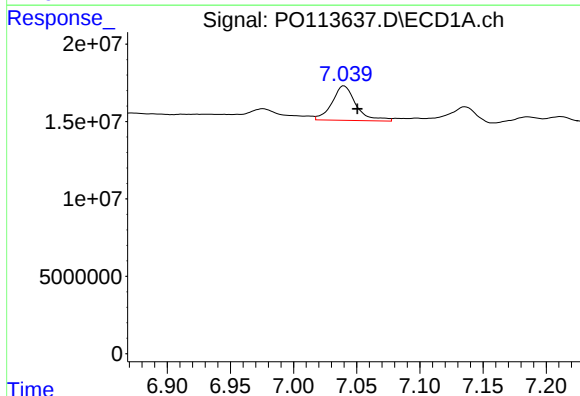


#34 AR-1260-4

R.T.: 7.040 min
Delta R.T.: -0.011 min
Response: 29499985
Conc: 65.87 ng/ml

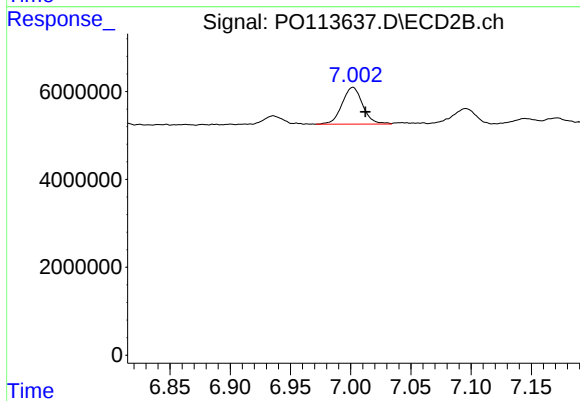

#34 AR-1260-4


R.T.: 7.002 min
Delta R.T.: -0.010 min
Response: 10003823
Conc: 48.27 ng/ml

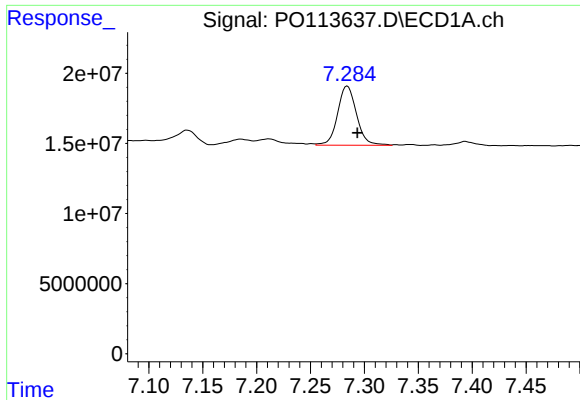

#35 AR-1260-5


R.T.: 7.284 min
Delta R.T.: -0.009 min
Response: 51661048
Conc: 42.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

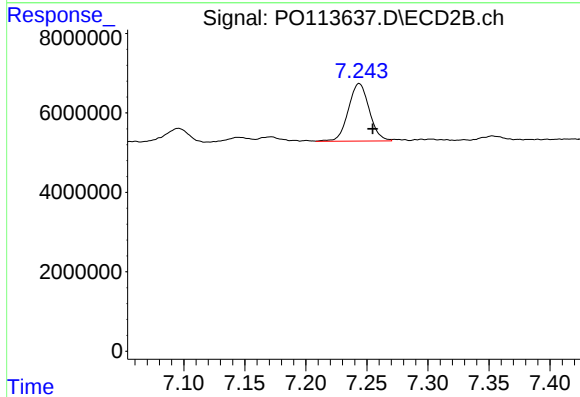


#35 AR-1260-5

R.T.: 7.244 min
Delta R.T.: -0.011 min
Response: 17245723
Conc: 36.82 ng/ml

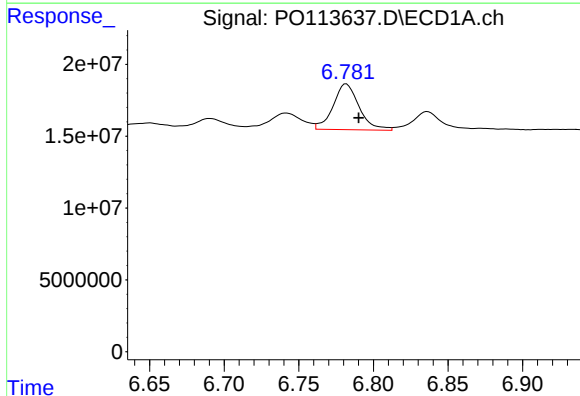


#36 AR-1262-1

R.T.: 6.782 min
Delta R.T.: -0.008 min
Response: 38623359
Conc: 42.18 ng/ml

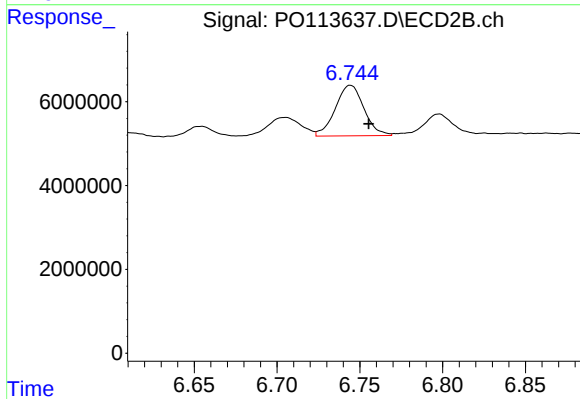

#36 AR-1262-1


R.T.: 6.744 min
Delta R.T.: -0.011 min
Response: 14539492
Conc: 35.07 ng/ml

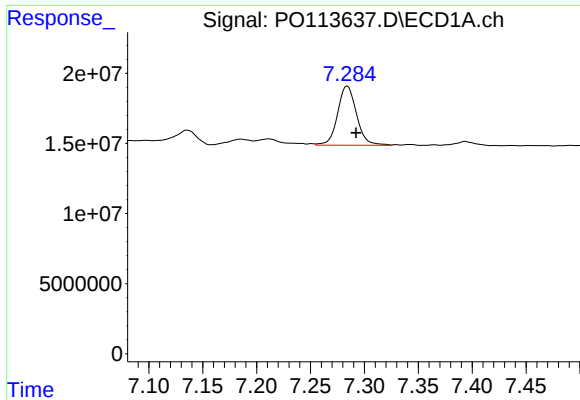

#37 AR-1262-2


R.T.: 7.284 min
Delta R.T.: -0.008 min
Response: 51661048
Conc: 34.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

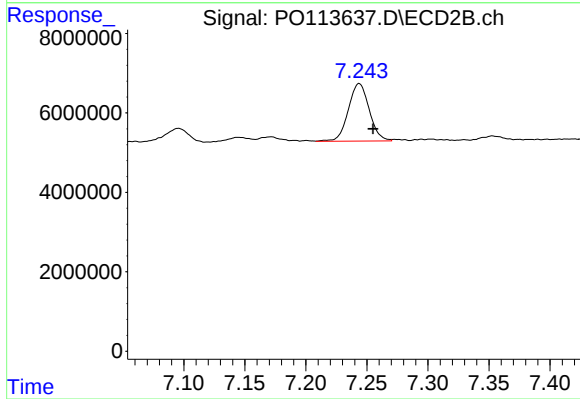


#37 AR-1262-2

R.T.: 7.244 min
Delta R.T.: -0.011 min
Response: 17245723
Conc: 33.31 ng/ml

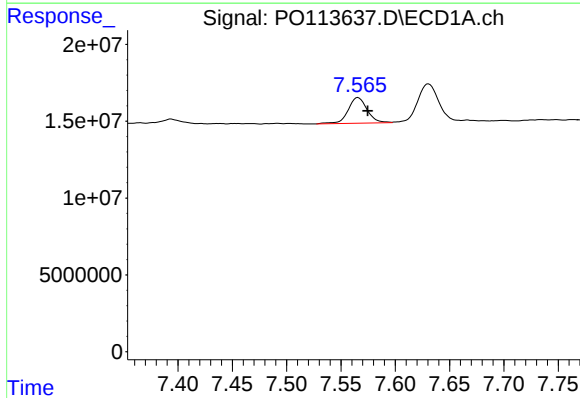


#38 AR-1262-3

R.T.: 7.566 min
Delta R.T.: -0.009 min
Response: 20413885
Conc: 36.84 ng/ml

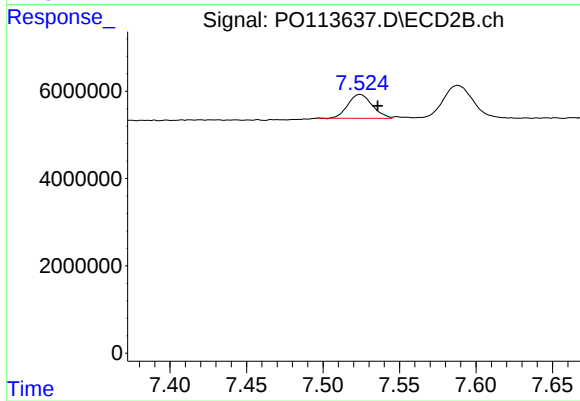

#38 AR-1262-3


R.T.: 7.524 min
Delta R.T.: -0.012 min
Response: 6056474
Conc: 33.72 ng/ml

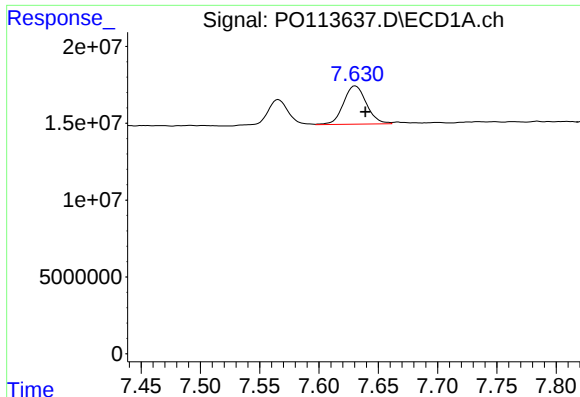

#39 AR-1262-4


R.T.: 7.631 min
Delta R.T.: -0.009 min
Response: 33700442
Conc: 34.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

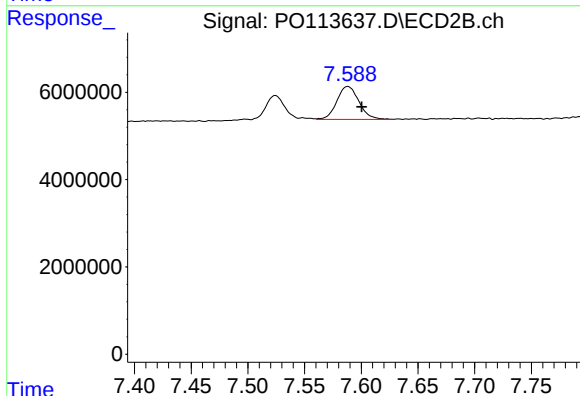


#39 AR-1262-4

R.T.: 7.588 min
Delta R.T.: -0.012 min
Response: 10238873
Conc: 35.32 ng/ml

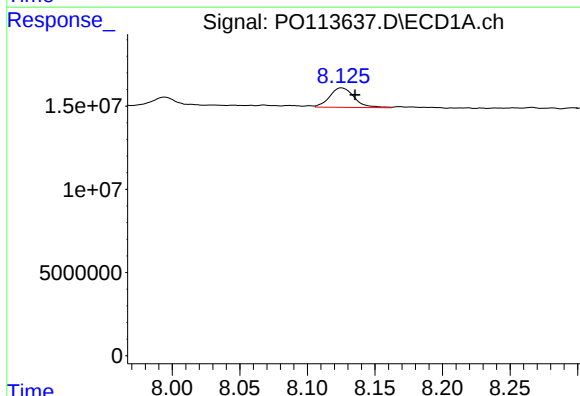


#40 AR-1262-5

R.T.: 8.125 min
Delta R.T.: -0.010 min
Response: 14789932
Conc: 35.48 ng/ml

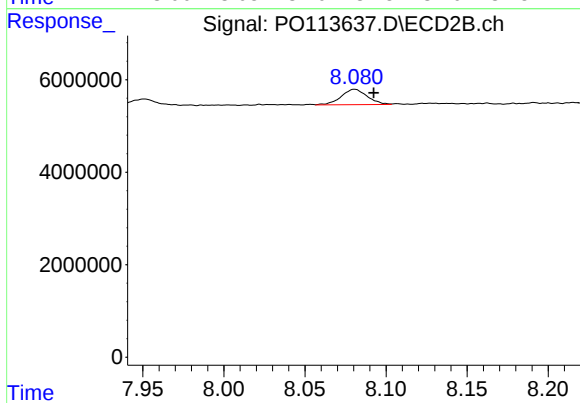

#40 AR-1262-5


R.T.: 8.081 min
Delta R.T.: -0.012 min
Response: 3706086
Conc: 34.21 ng/ml

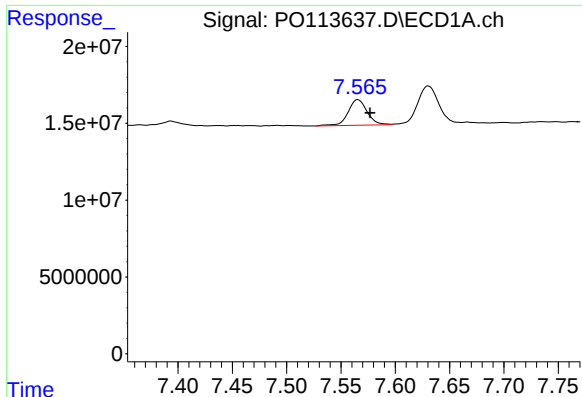

#41 AR-1268-1


R.T.: 7.566 min
Delta R.T.: -0.011 min
Response: 20413885
Conc: 11.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

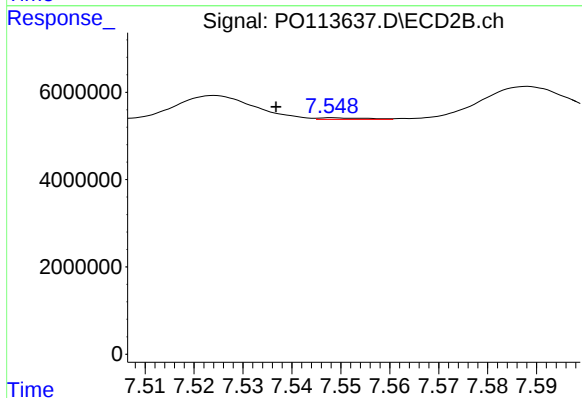


#41 AR-1268-1

R.T.: 7.548 min
Delta R.T.: 0.011 min
Response: 230350
Conc: 0.45 ng/ml

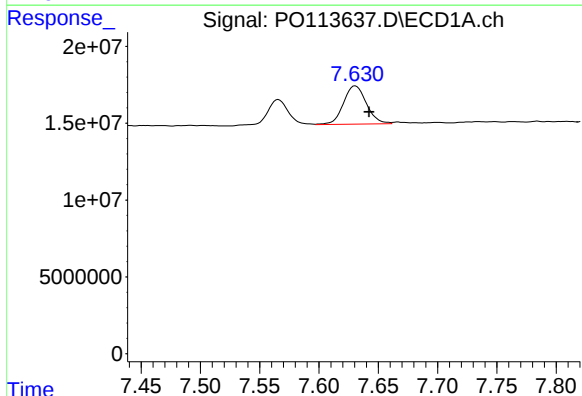


#42 AR-1268-2

R.T.: 7.631 min
Delta R.T.: -0.012 min
Response: 33700442
Conc: 23.27 ng/ml

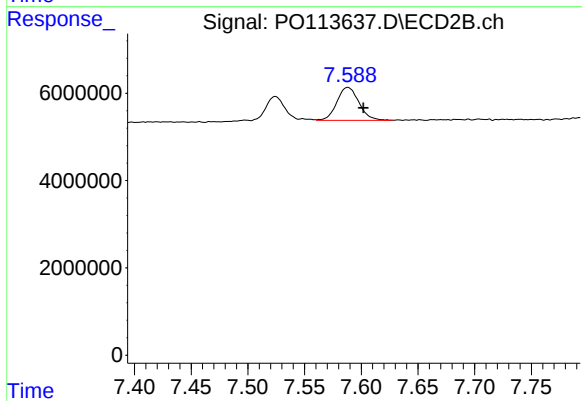

#42 AR-1268-2


R.T.: 7.588 min
Delta R.T.: -0.014 min
Response: 10238873
Conc: 24.65 ng/ml

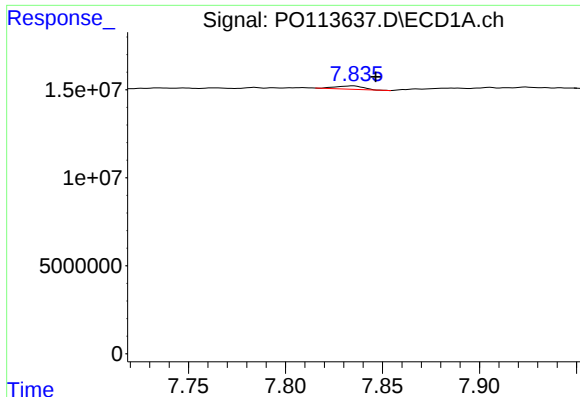

#43 AR-1268-3


R.T.: 7.835 min
Delta R.T.: -0.012 min
Response: 1788661
Conc: 1.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

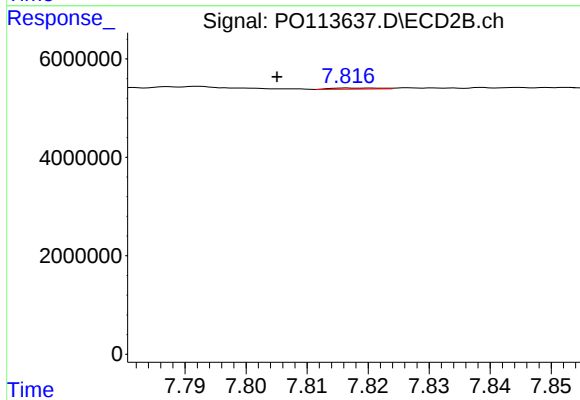


#43 AR-1268-3

R.T.: 7.817 min
Delta R.T.: 0.012 min
Response: 119351
Conc: 0.37 ng/ml

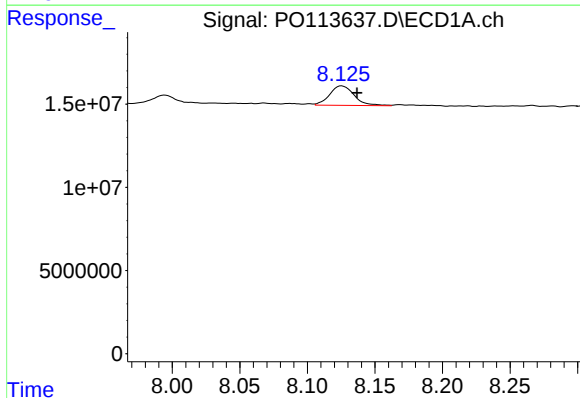


#44 AR-1268-4

R.T.: 8.125 min
Delta R.T.: -0.011 min
Response: 14789932
Conc: 32.11 ng/ml

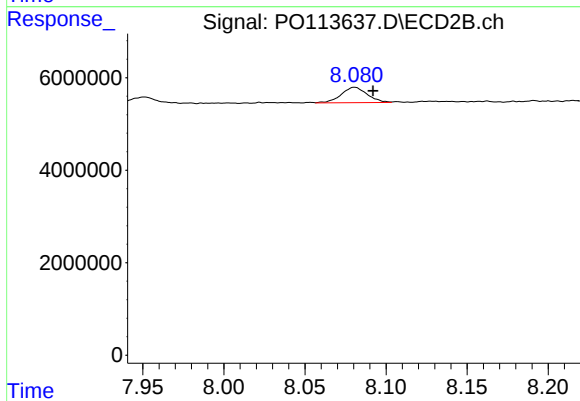

#44 AR-1268-4


R.T.: 8.081 min
Delta R.T.: -0.011 min
Response: 3706086
Conc: 30.77 ng/ml

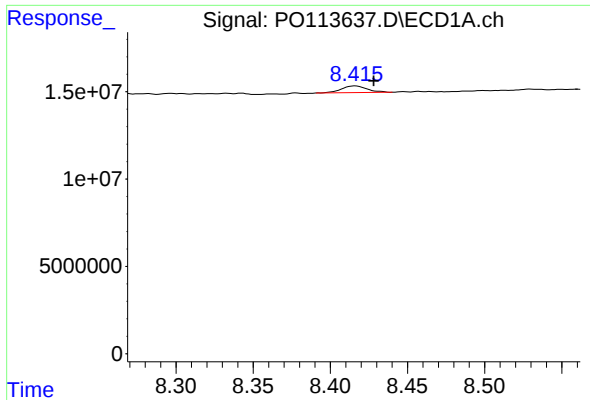

#45 AR-1268-5

R.T.: 8.416 min
Delta R.T.: -0.012 min
Response: 4470105
Conc: 1.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

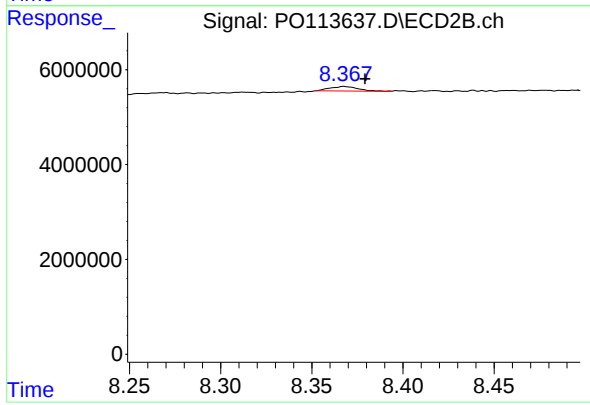

#45 AR-1268-5

R.T.: 8.367 min
Delta R.T.: -0.012 min
Response: 1062820
Conc: 1.36 ng/ml