

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
 Data File : P0113638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 04:16
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1268 WATER LOD 40PPB
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:31:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.658	3.649	177.1E6	103.5E6	21.639	20.461
2) SA Decachlor...	8.669	8.614	163.7E6	46491584	23.624	24.536
Target Compounds						
3) L1 AR-1016-1	4.756	4.738	463433	577594	1.736	3.386 #
4) L1 AR-1016-2	4.756	4.738	463433	577594	1.154	2.242 #
5) L1 AR-1016-3	4.813	4.922	97031	1191637	0.380	8.535 #
6) L1 AR-1016-4	4.936	4.962	921128	1950550	4.224	16.714 #
7) L1 AR-1016-5	5.251f	5.176	9664879	2471843	43.609	17.343 #
8) L2 AR-1221-1	3.928f	3.870	230605	196824	2.464	3.118 #
9) L2 AR-1221-2	3.960	3.946	2209848	1948001	32.714	41.737 #
10) L2 AR-1221-3	4.056	4.021	475326	92394	2.147	0.622 #
11) L3 AR-1232-1	4.056	4.021	475326	92394	2.648	0.764 #
12) L3 AR-1232-2	4.491	4.738	403333	577594	3.737	4.732 #
13) L3 AR-1232-3	4.756	4.922	463433	1191637	2.348	18.013 #
14) L3 AR-1232-4	4.936	5.003	921128	427843	9.371	7.139
15) L3 AR-1232-5	4.992	5.176	2508730	2471843	38.137	36.557
16) L4 AR-1242-1	4.756	4.738	463433	577594	2.016	3.997 #
17) L4 AR-1242-2	4.756	4.738	463433	577594	1.349	2.663 #
18) L4 AR-1242-3	4.813	4.922	97031	1191637	0.437	10.188 #
19) L4 AR-1242-4	4.936	5.003	921128	427843	5.310	3.637 #
20) L4 AR-1242-5	5.601	5.496	7198587	2870137	35.964	19.245 #
21) L5 AR-1248-1	4.756	4.738	463433	577594	2.656	5.180 #
22) L5 AR-1248-2	4.992	4.962	2508730	1950550	10.372	12.138
23) L5 AR-1248-3	5.251f	5.003	9664879	427843	30.310	2.522 #
24) L5 AR-1248-4	5.561	5.176	12208194	2471843	24.436	12.408 #
25) L5 AR-1248-5	5.586	5.570	5124749	6514873	15.007	30.688 #
26) L6 AR-1254-1	5.561	5.496	12208194	2870137	22.609	9.101 #
27) L6 AR-1254-2	5.706	5.680	10463751	1532183	21.205	5.465 #
28) L6 AR-1254-3	6.101	6.068	2680826	1471989	3.628	3.531
29) L6 AR-1254-4	6.353	6.313	618101	120907	1.110	0.440 #
30) L6 AR-1254-5	6.751	6.692	989874	570502	1.412	1.596
31) L7 AR-1260-1	6.242	6.187	2315043	1686813	5.191	6.613 #
32) L7 AR-1260-2	6.433	6.416	193070	486782	0.281	1.408 #
33) L7 AR-1260-3	6.781	6.540	16006233	1167925	25.922	3.927 #
34) L7 AR-1260-4	7.036	6.997	22531217	5956933	50.307	28.743 #
35) L7 AR-1260-5	7.284	7.243	8246254	2439651	6.811	5.208
36) L8 AR-1262-1	6.781	6.744	16006233	5893652	17.479	14.215
37) L8 AR-1262-2	7.284	7.243	8246254	2439651	5.453	4.713
38) L8 AR-1262-3	7.566	7.524	50874682	16076862	91.814	89.520
39) L8 AR-1262-4	7.632	7.590	41893870	13007070	42.838	44.867
40) L8 AR-1262-5	8.126	8.081	14642454	3680843	35.124	33.978
41) L9 AR-1268-1	7.566	7.524	50874682	16076862	29.563	31.556

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091025\
Data File : P0113638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 04:16
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1268 WATER LOD 40PPB
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:31:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.632	7.590	41893870	13007070	28.929	31.312
43)	L9 AR-1268-3	7.836	7.793	35041632	9724673	29.048	29.784
44)	L9 AR-1268-4	8.126	8.081	14642454	3680843	31.786	30.564
45)	L9 AR-1268-5	8.417	8.367	91328010	18888899	28.644	24.187



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091025\
Data File : PO113638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 04:16
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1268 WATER LOD 40PPB
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:31:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

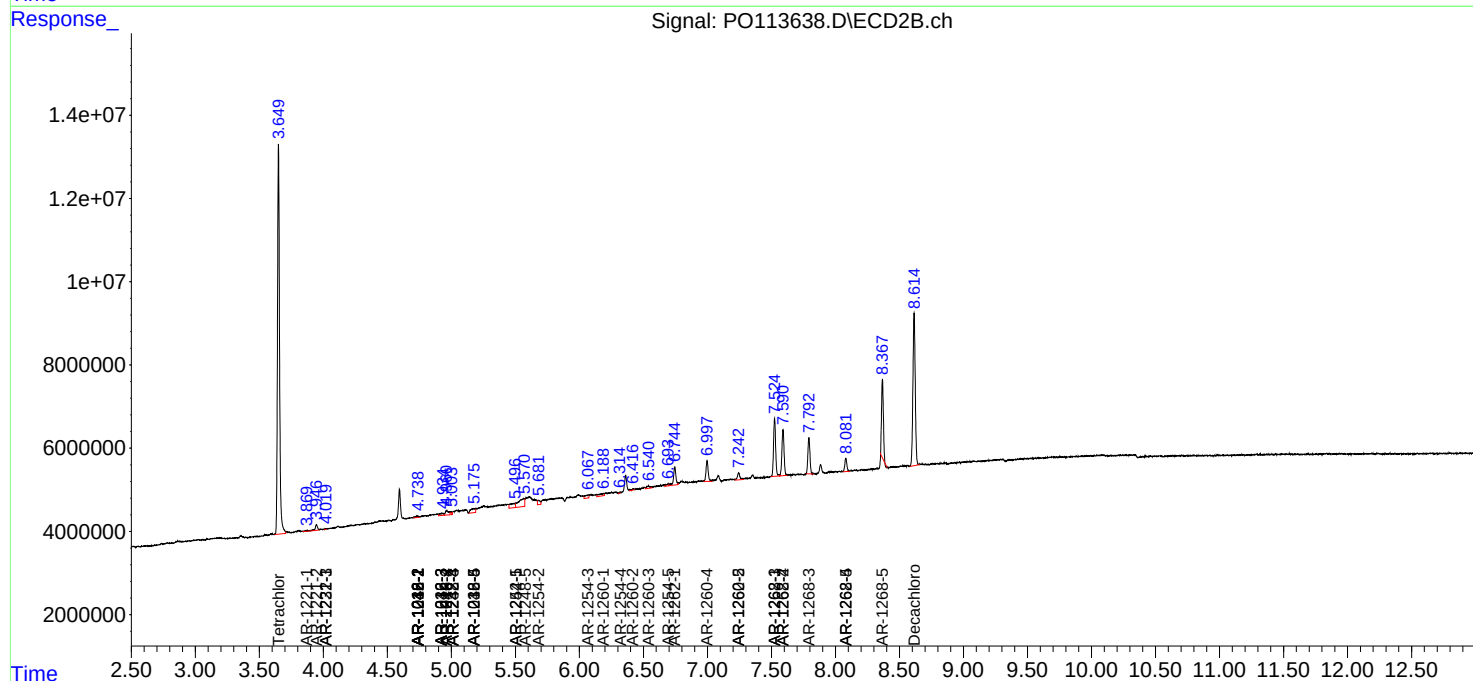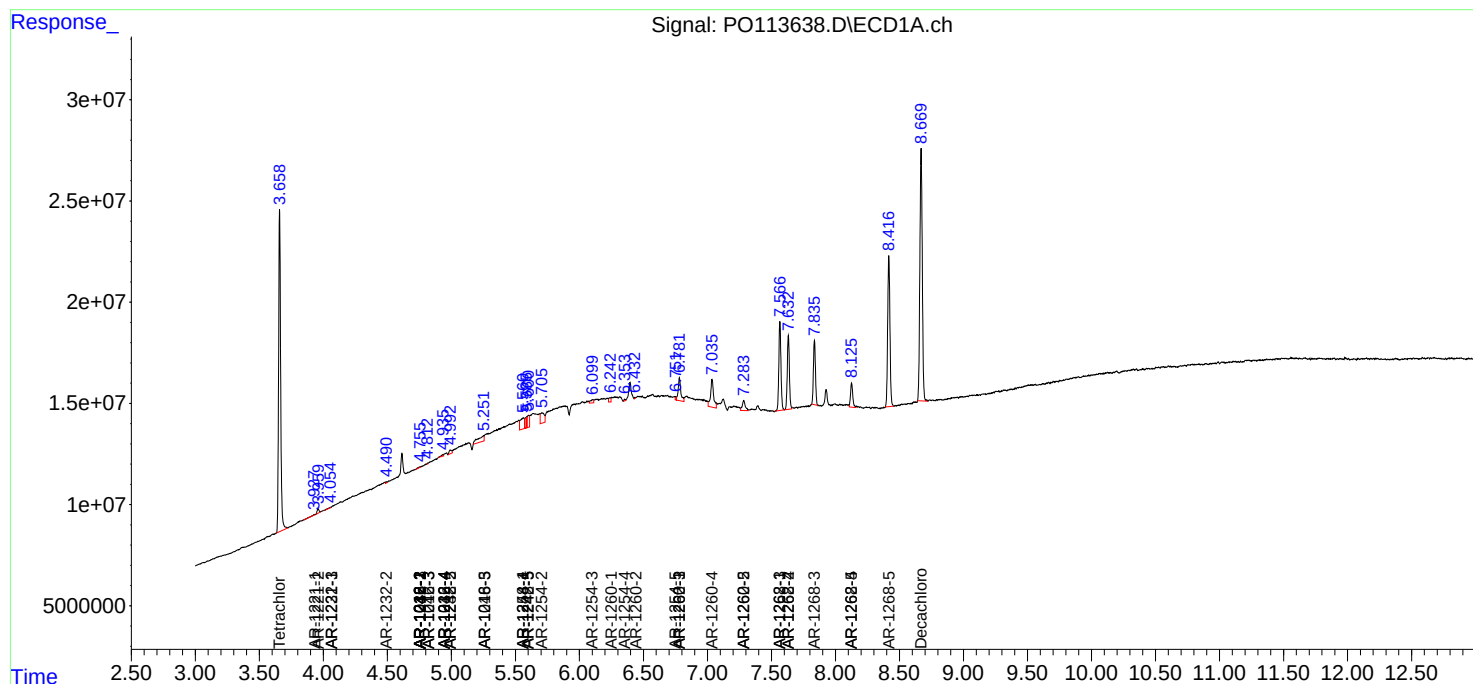


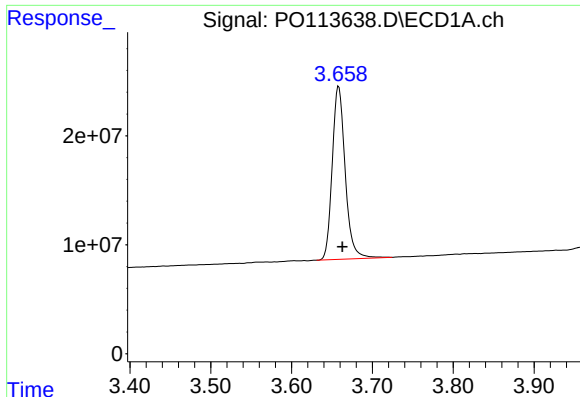

#1 Tetrachloro-m-xylene


R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 177148625
Conc: 21.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

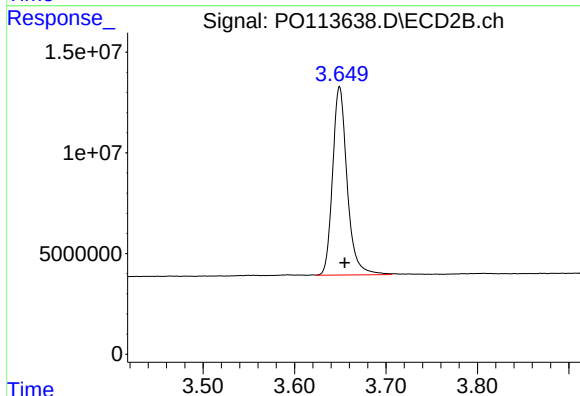


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.006 min
Response: 103547915
Conc: 20.46 ng/ml

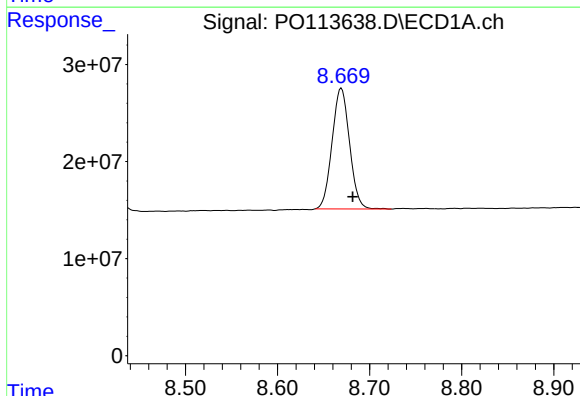


#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.012 min
Response: 163745687
Conc: 23.62 ng/ml

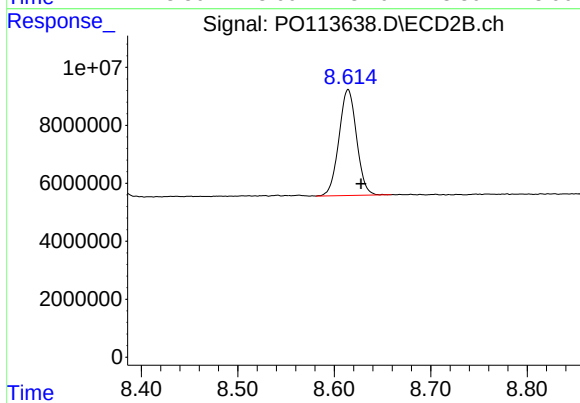

#2 Decachlorobiphenyl


R.T.: 8.614 min
Delta R.T.: -0.013 min
Response: 46491584
Conc: 24.54 ng/ml

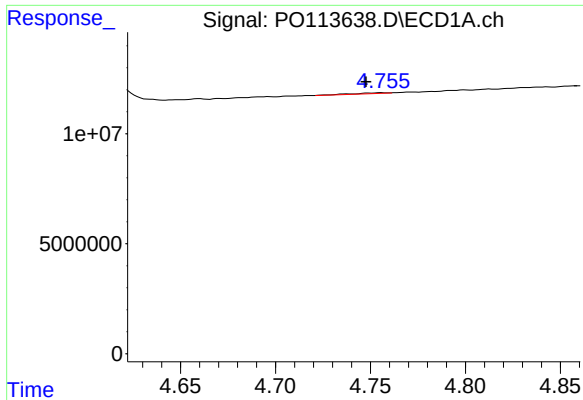

#3 AR-1016-1


R.T.: 4.756 min
Delta R.T.: 0.008 min
Response: 463433
Conc: 1.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

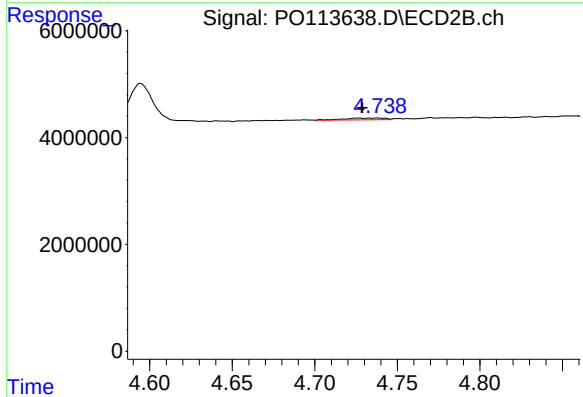


#3 AR-1016-1

R.T.: 4.738 min
Delta R.T.: 0.009 min
Response: 577594
Conc: 3.39 ng/ml

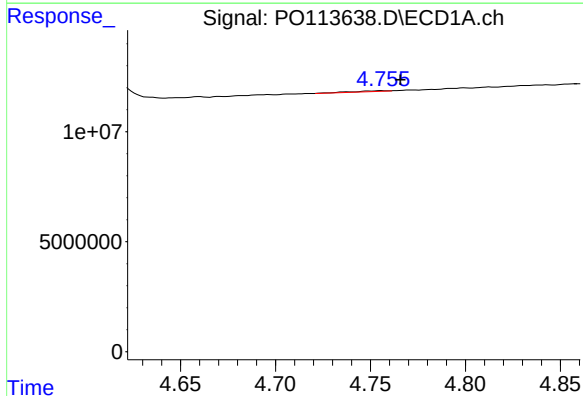


#4 AR-1016-2

R.T.: 4.756 min
Delta R.T.: -0.010 min
Response: 463433
Conc: 1.15 ng/ml

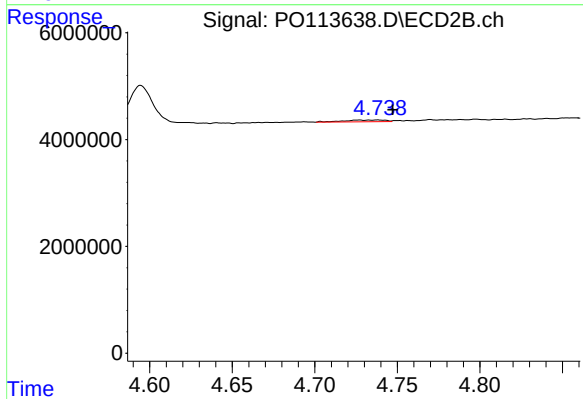

#4 AR-1016-2


R.T.: 4.738 min
Delta R.T.: -0.009 min
Response: 577594
Conc: 2.24 ng/ml

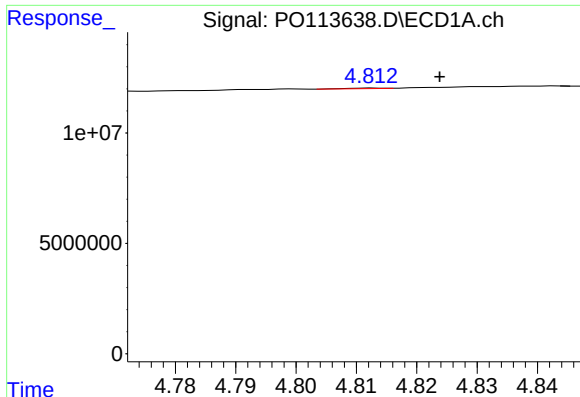

#5 AR-1016-3


R.T.: 4.813 min
Delta R.T.: -0.011 min
Response: 97031
Conc: 0.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

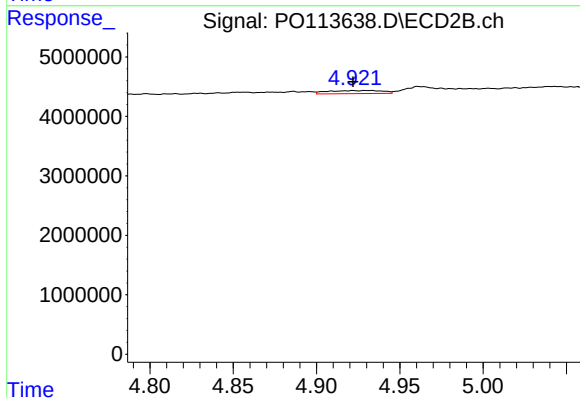


#5 AR-1016-3

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 1191637
Conc: 8.54 ng/ml

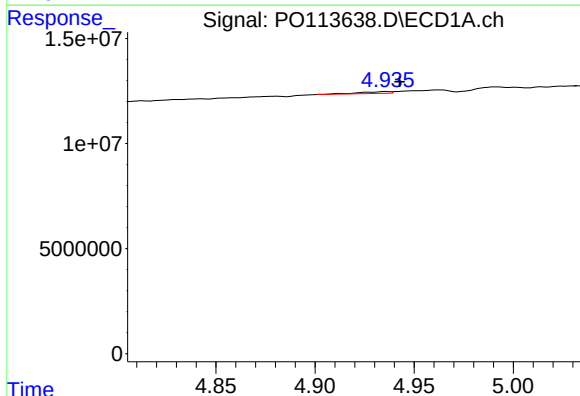


#6 AR-1016-4

R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 921128
Conc: 4.22 ng/ml

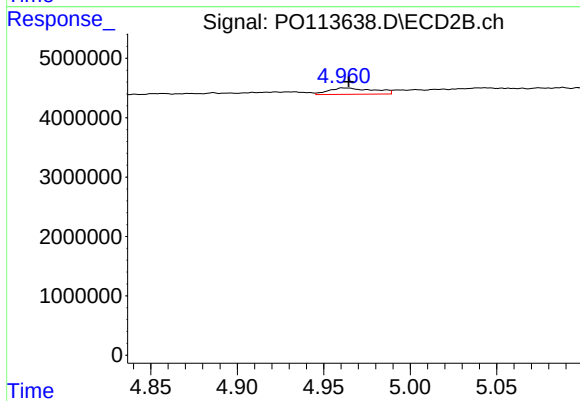

#6 AR-1016-4


R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 1950550
Conc: 16.71 ng/ml

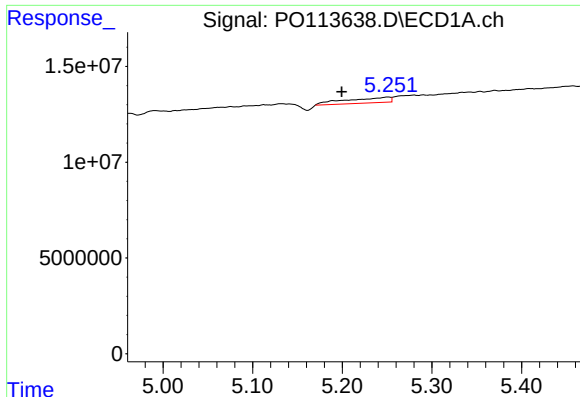

#7 AR-1016-5


R.T.: 5.251 min
Delta R.T.: 0.052 min
Response: 9664879
Conc: 43.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

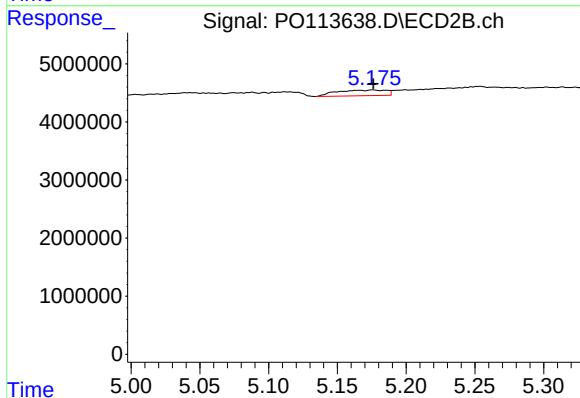


#7 AR-1016-5

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 2471843
Conc: 17.34 ng/ml

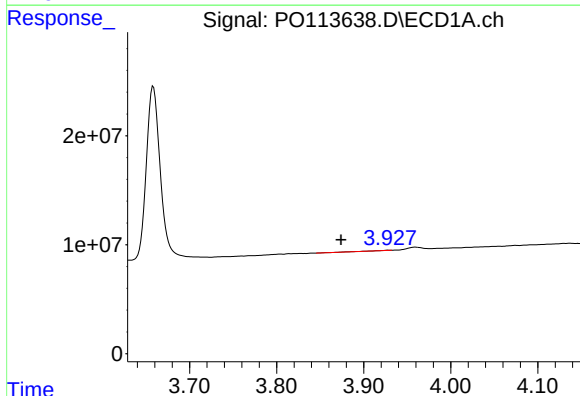


#8 AR-1221-1

R.T.: 3.928 min
Delta R.T.: 0.054 min
Response: 230605
Conc: 2.46 ng/ml

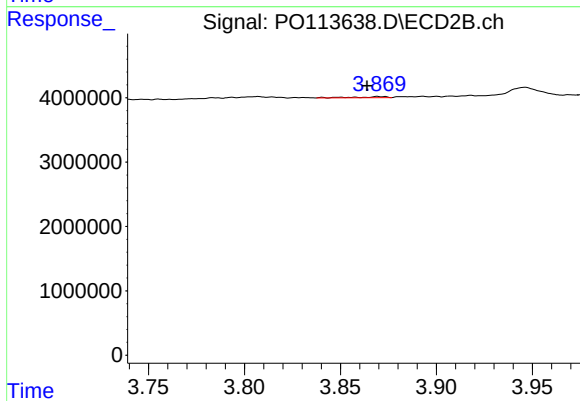

#8 AR-1221-1


R.T.: 3.870 min
Delta R.T.: 0.006 min
Response: 196824
Conc: 3.12 ng/ml

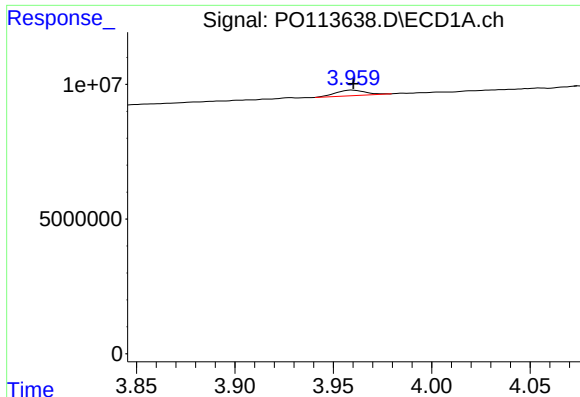

#9 AR-1221-2


R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 2209848
Conc: 32.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

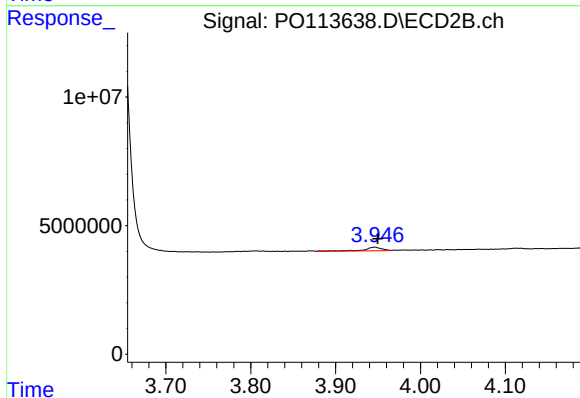


#9 AR-1221-2

R.T.: 3.946 min
Delta R.T.: -0.004 min
Response: 1948001
Conc: 41.74 ng/ml

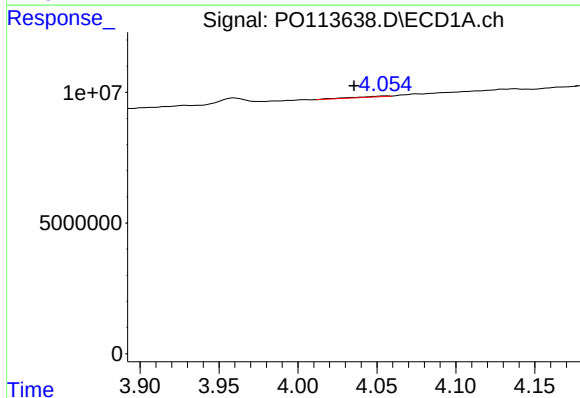


#10 AR-1221-3

R.T.: 4.056 min
Delta R.T.: 0.020 min
Response: 475326
Conc: 2.15 ng/ml

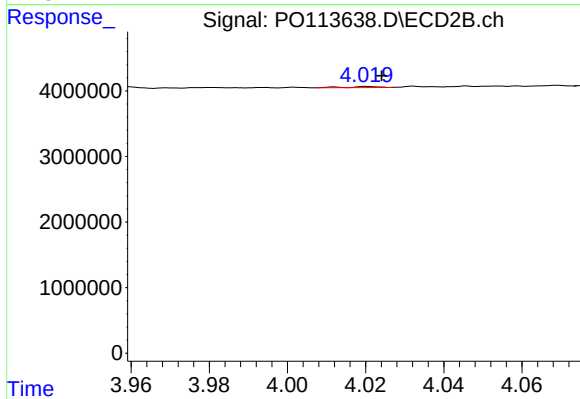

#10 AR-1221-3


R.T.: 4.021 min
Delta R.T.: -0.004 min
Response: 92394
Conc: 0.62 ng/ml

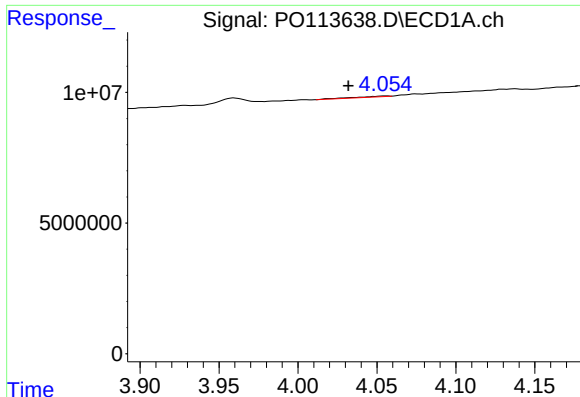

#11 AR-1232-1


R.T.: 4.056 min
Delta R.T.: 0.024 min
Response: 475326
Conc: 2.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

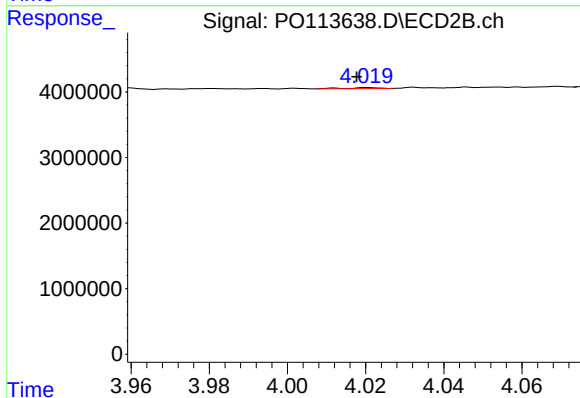


#11 AR-1232-1

R.T.: 4.021 min
Delta R.T.: 0.003 min
Response: 92394
Conc: 0.76 ng/ml

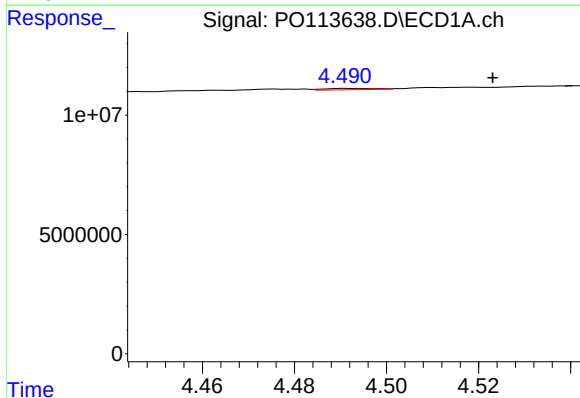


#12 AR-1232-2

R.T.: 4.491 min
Delta R.T.: -0.032 min
Response: 403333
Conc: 3.74 ng/ml

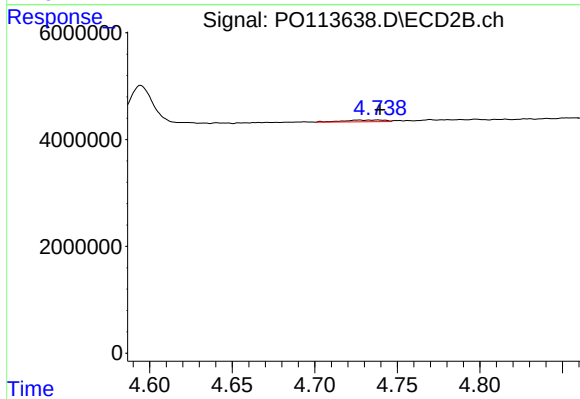

#12 AR-1232-2


R.T.: 4.738 min
Delta R.T.: -0.001 min
Response: 577594
Conc: 4.73 ng/ml

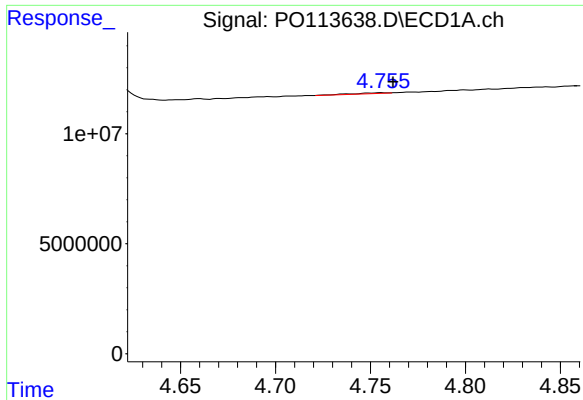

#13 AR-1232-3


R.T.: 4.756 min
Delta R.T.: -0.006 min
Response: 463433
Conc: 2.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

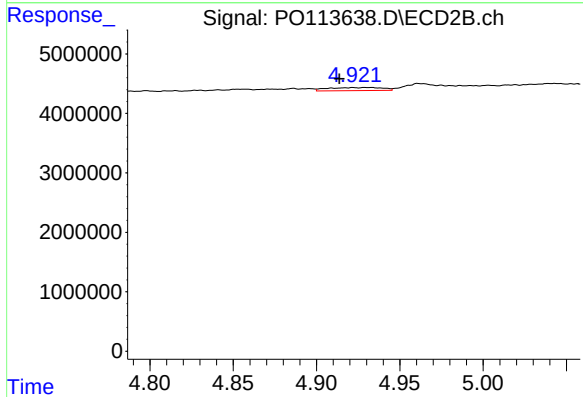


#13 AR-1232-3

R.T.: 4.922 min
Delta R.T.: 0.008 min
Response: 1191637
Conc: 18.01 ng/ml

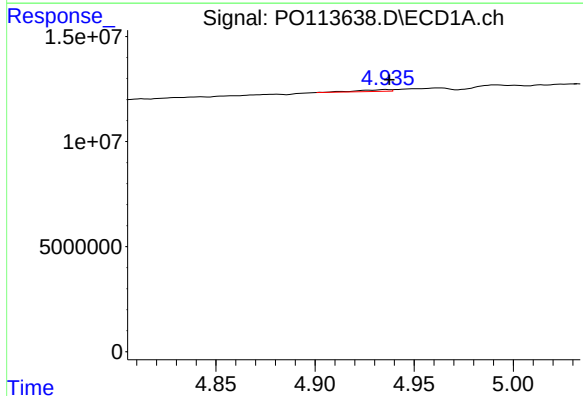


#14 AR-1232-4

R.T.: 4.936 min
Delta R.T.: -0.002 min
Response: 921128
Conc: 9.37 ng/ml

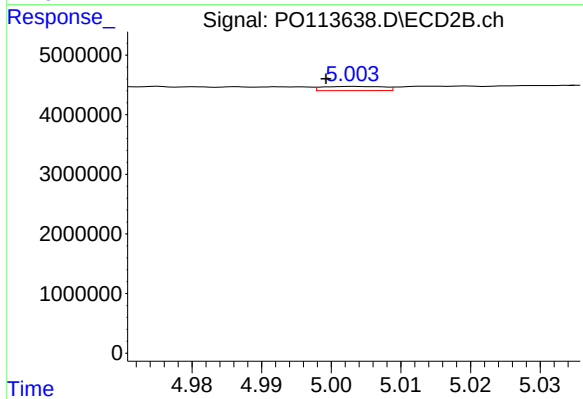

#14 AR-1232-4


R.T.: 5.003 min
Delta R.T.: 0.004 min
Response: 427843
Conc: 7.14 ng/ml

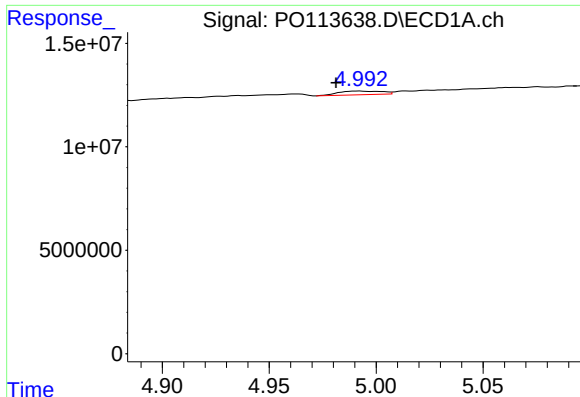

#15 AR-1232-5


R.T.: 4.992 min
Delta R.T.: 0.010 min
Response: 2508730
Conc: 38.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

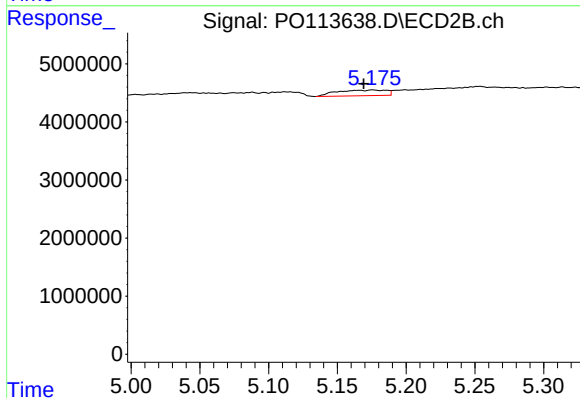


#15 AR-1232-5

R.T.: 5.176 min
Delta R.T.: 0.007 min
Response: 2471843
Conc: 36.56 ng/ml

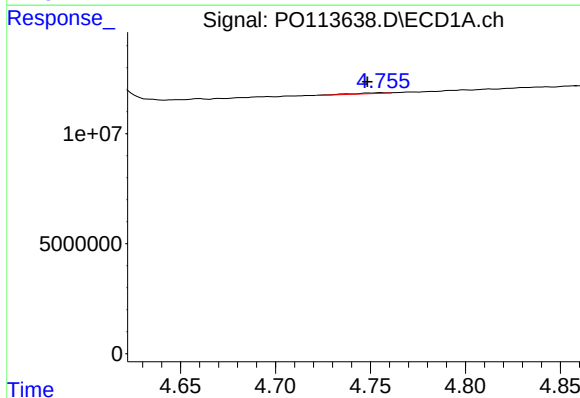


#16 AR-1242-1

R.T.: 4.756 min
Delta R.T.: 0.008 min
Response: 463433
Conc: 2.02 ng/ml

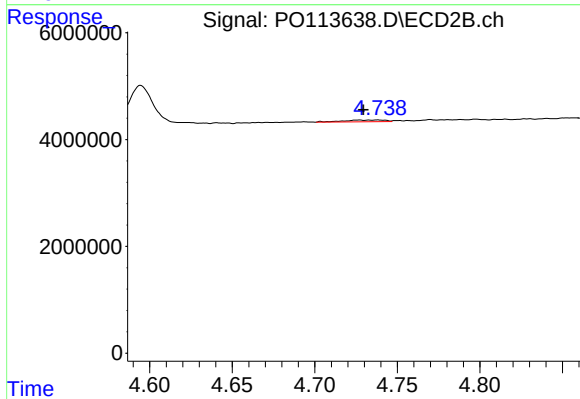

#16 AR-1242-1


R.T.: 4.738 min
Delta R.T.: 0.009 min
Response: 577594
Conc: 4.00 ng/ml

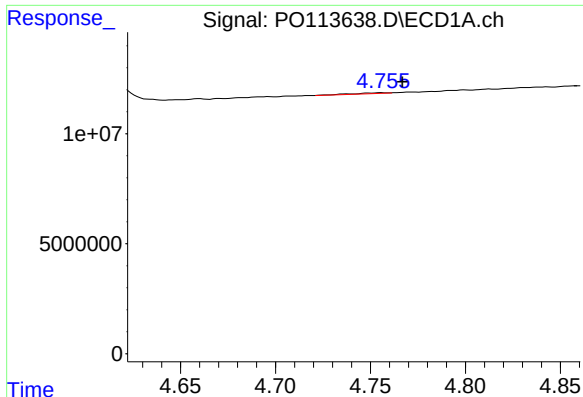

#17 AR-1242-2


R.T.: 4.756 min
Delta R.T.: -0.011 min
Response: 463433
Conc: 1.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

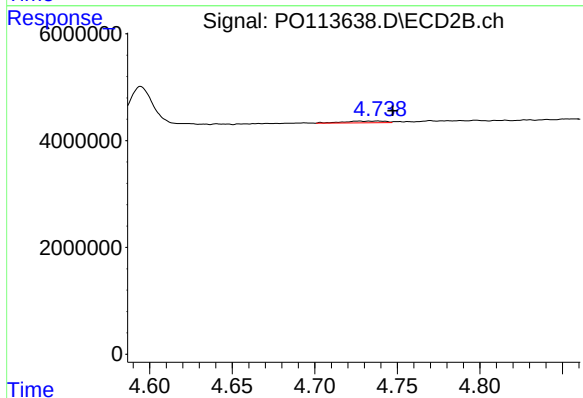


#17 AR-1242-2

R.T.: 4.738 min
Delta R.T.: -0.009 min
Response: 577594
Conc: 2.66 ng/ml

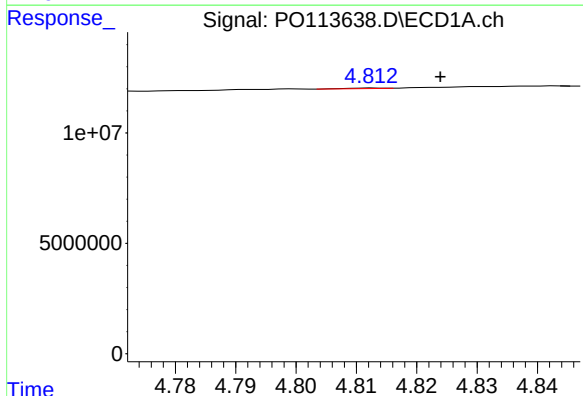


#18 AR-1242-3

R.T.: 4.813 min
Delta R.T.: -0.011 min
Response: 97031
Conc: 0.44 ng/ml

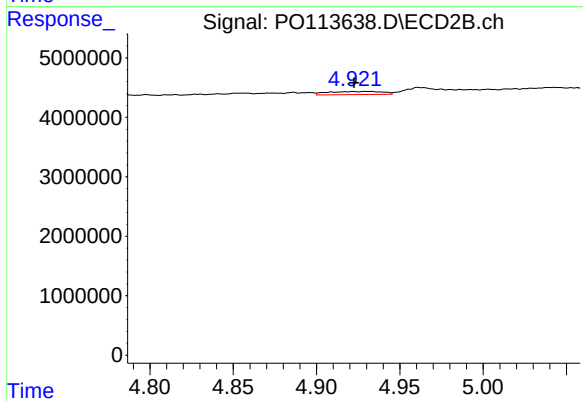

#18 AR-1242-3


R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 1191637
Conc: 10.19 ng/ml

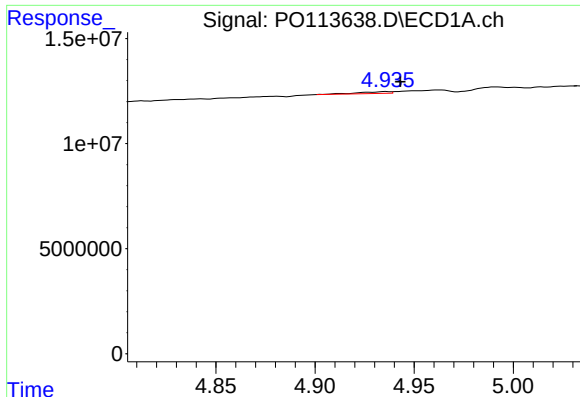

#19 AR-1242-4


R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 921128
Conc: 5.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

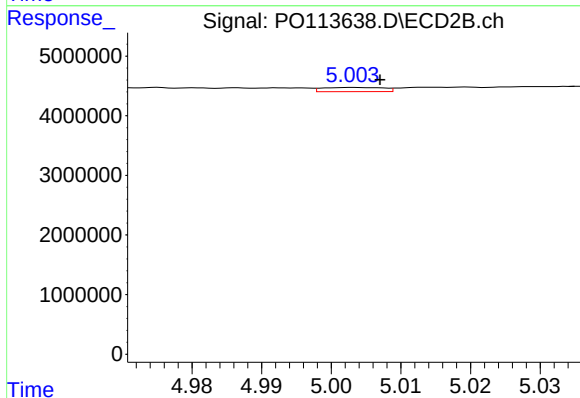


#19 AR-1242-4

R.T.: 5.003 min
Delta R.T.: -0.004 min
Response: 427843
Conc: 3.64 ng/ml

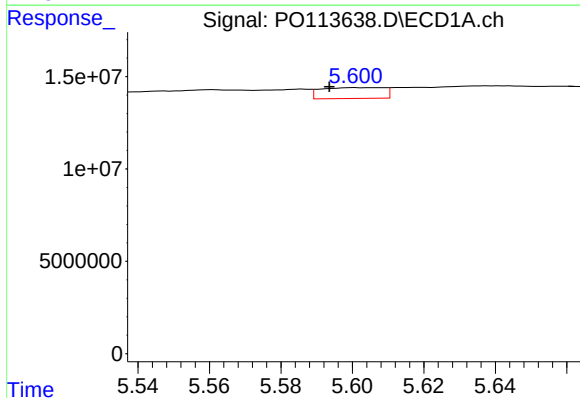


#20 AR-1242-5

R.T.: 5.601 min
Delta R.T.: 0.007 min
Response: 7198587
Conc: 35.96 ng/ml

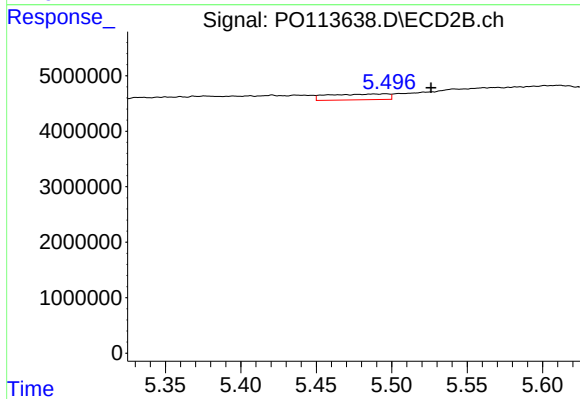

#20 AR-1242-5


R.T.: 5.496 min
Delta R.T.: -0.030 min
Response: 2870137
Conc: 19.25 ng/ml

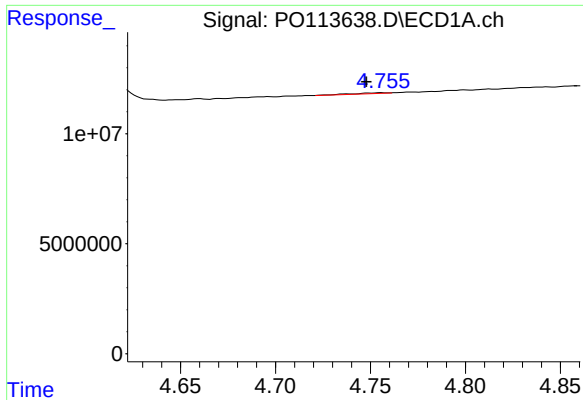

#21 AR-1248-1


R.T.: 4.756 min
Delta R.T.: 0.008 min
Response: 463433
Conc: 2.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

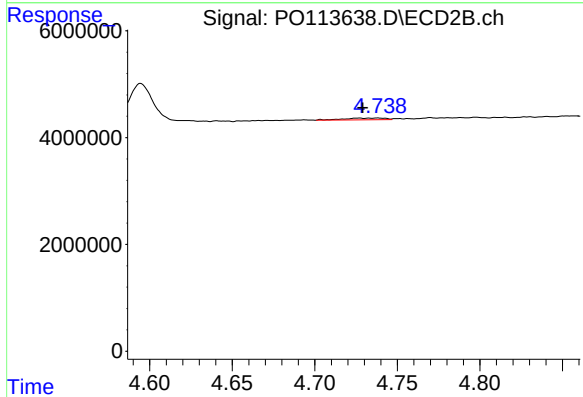


#21 AR-1248-1

R.T.: 4.738 min
Delta R.T.: 0.009 min
Response: 577594
Conc: 5.18 ng/ml

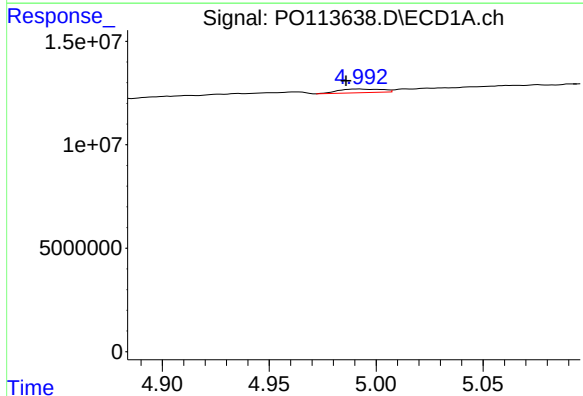


#22 AR-1248-2

R.T.: 4.992 min
Delta R.T.: 0.006 min
Response: 2508730
Conc: 10.37 ng/ml

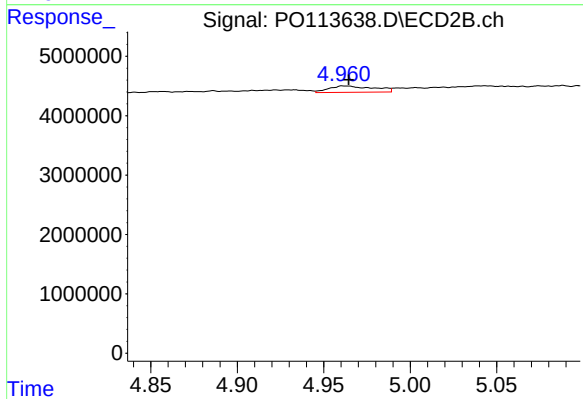

#22 AR-1248-2


R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 1950550
Conc: 12.14 ng/ml

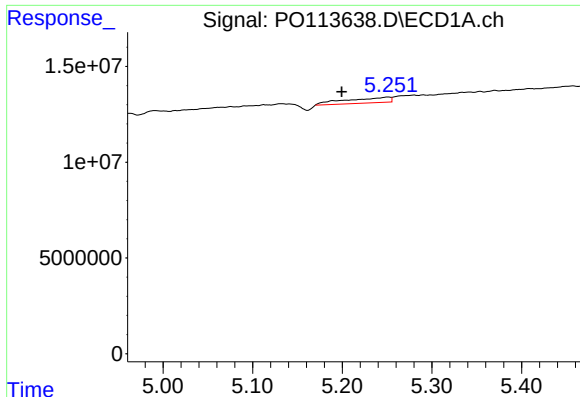

#23 AR-1248-3


R.T.: 5.251 min
Delta R.T.: 0.052 min
Response: 9664879
Conc: 30.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

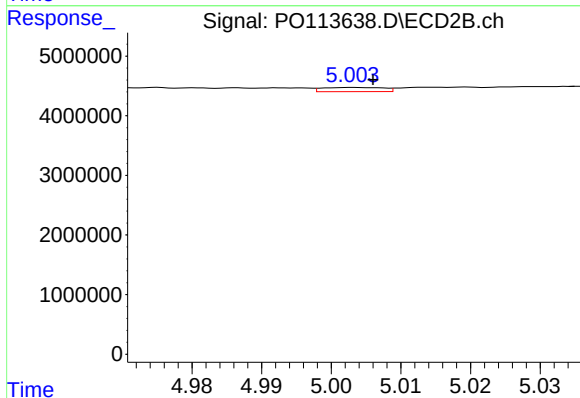


#23 AR-1248-3

R.T.: 5.003 min
Delta R.T.: -0.003 min
Response: 427843
Conc: 2.52 ng/ml

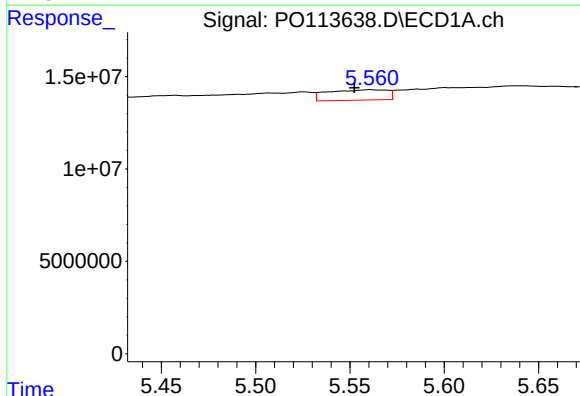


#24 AR-1248-4

R.T.: 5.561 min
Delta R.T.: 0.009 min
Response: 12208194
Conc: 24.44 ng/ml

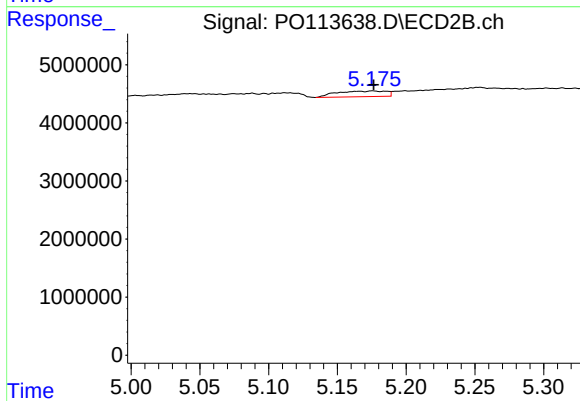

#24 AR-1248-4


R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 2471843
Conc: 12.41 ng/ml

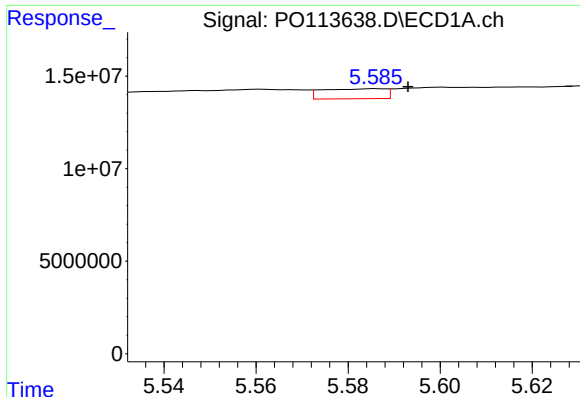

#25 AR-1248-5


R.T.: 5.586 min
Delta R.T.: -0.007 min
Response: 5124749
Conc: 15.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

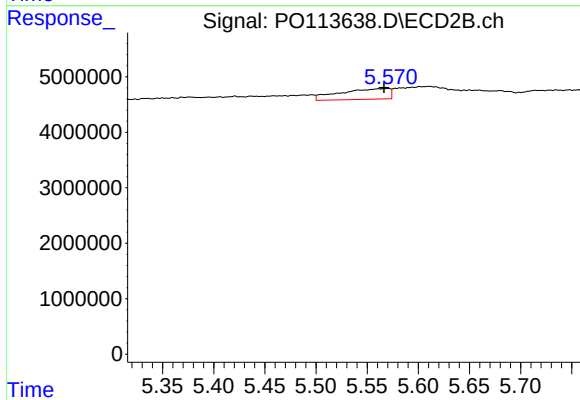


#25 AR-1248-5

R.T.: 5.570 min
Delta R.T.: 0.004 min
Response: 6514873
Conc: 30.69 ng/ml

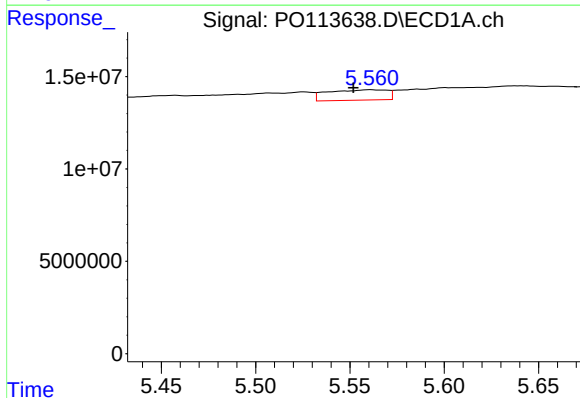


#26 AR-1254-1

R.T.: 5.561 min
Delta R.T.: 0.009 min
Response: 12208194
Conc: 22.61 ng/ml

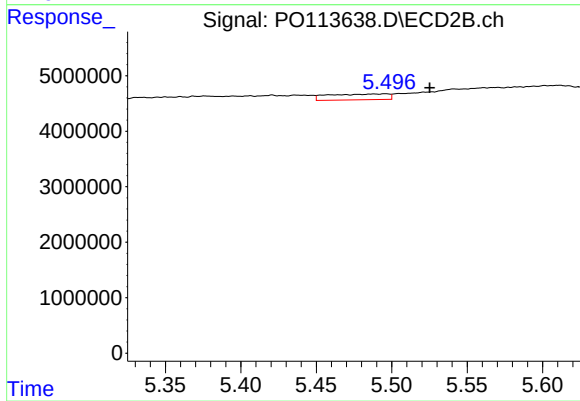

#26 AR-1254-1


R.T.: 5.496 min
Delta R.T.: -0.029 min
Response: 2870137
Conc: 9.10 ng/ml

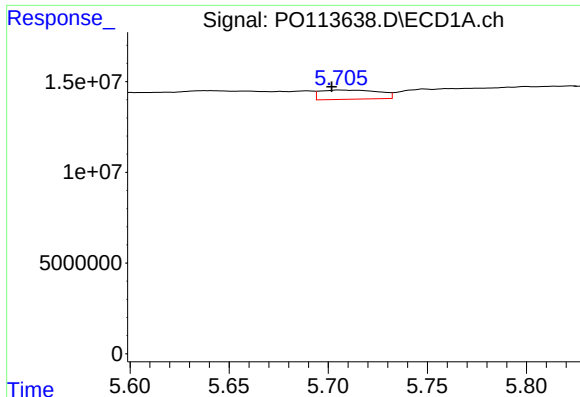

#27 AR-1254-2


R.T.: 5.706 min
Delta R.T.: 0.004 min
Response: 10463751
Conc: 21.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

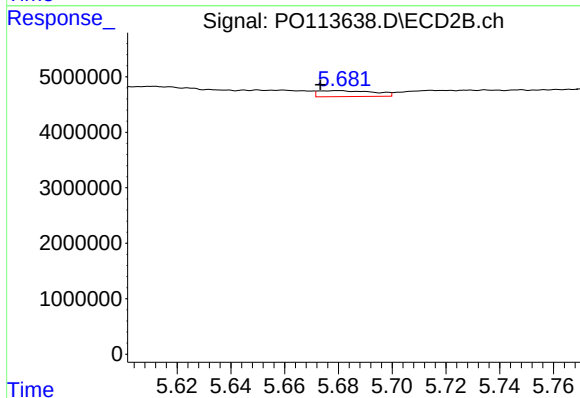


#27 AR-1254-2

R.T.: 5.680 min
Delta R.T.: 0.007 min
Response: 1532183
Conc: 5.47 ng/ml

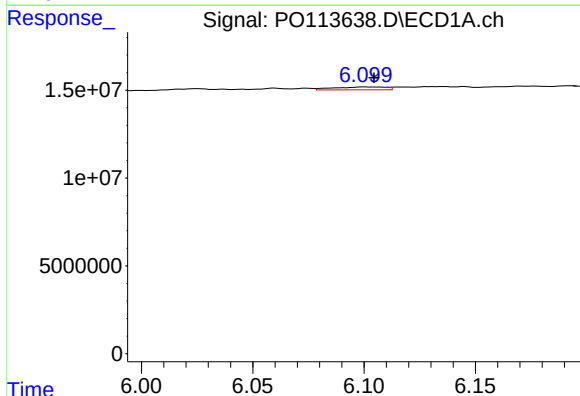


#28 AR-1254-3

R.T.: 6.101 min
Delta R.T.: -0.004 min
Response: 2680826
Conc: 3.63 ng/ml

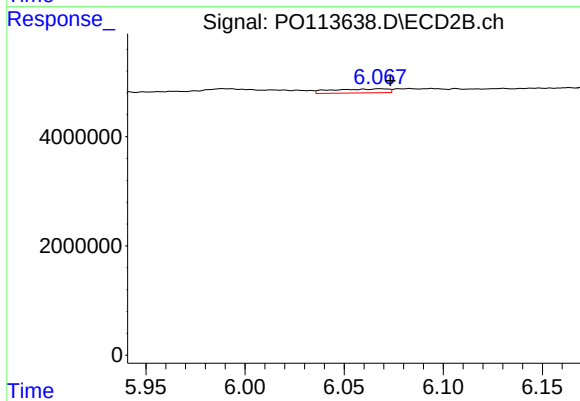

#28 AR-1254-3


R.T.: 6.068 min
Delta R.T.: -0.005 min
Response: 1471989
Conc: 3.53 ng/ml

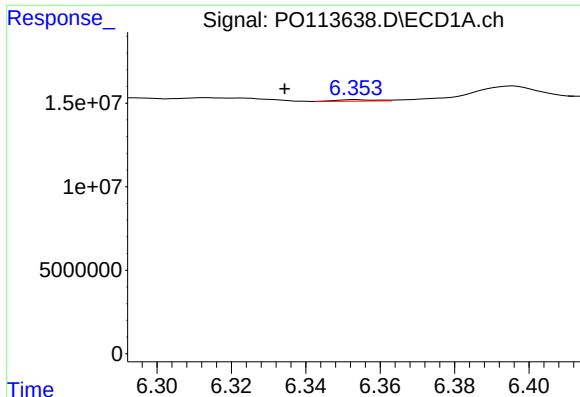

#29 AR-1254-4


R.T.: 6.353 min
Delta R.T.: 0.019 min
Response: 618101
Conc: 1.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

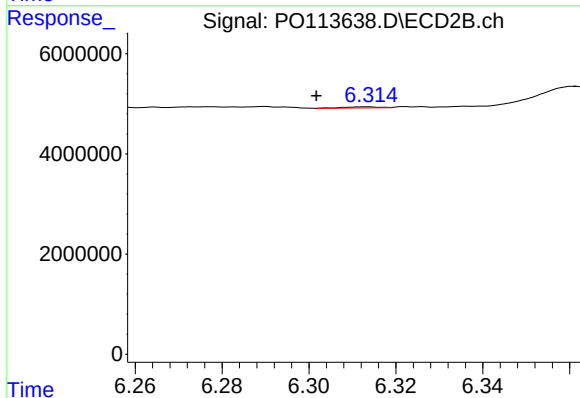


#29 AR-1254-4

R.T.: 6.313 min
Delta R.T.: 0.012 min
Response: 120907
Conc: 0.44 ng/ml

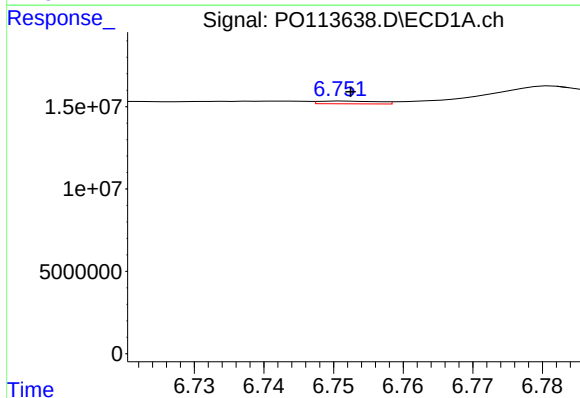


#30 AR-1254-5

R.T.: 6.751 min
Delta R.T.: -0.001 min
Response: 989874
Conc: 1.41 ng/ml

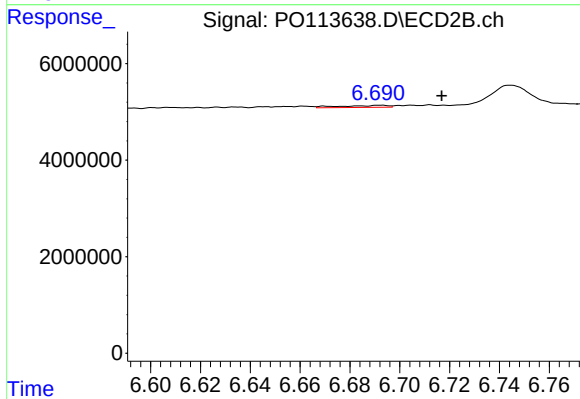

#30 AR-1254-5


R.T.: 6.692 min
Delta R.T.: -0.025 min
Response: 570502
Conc: 1.60 ng/ml

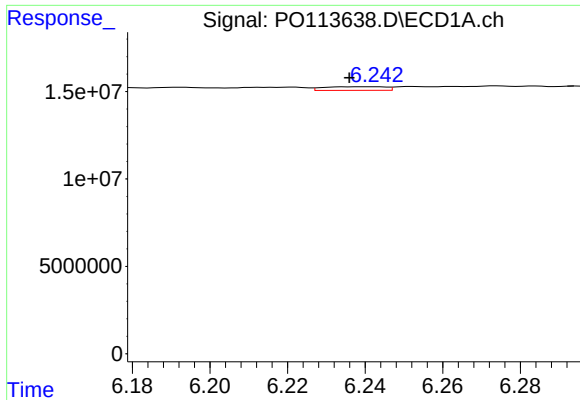

#31 AR-1260-1


R.T.: 6.242 min
Delta R.T.: 0.007 min
Response: 2315043
Conc: 5.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

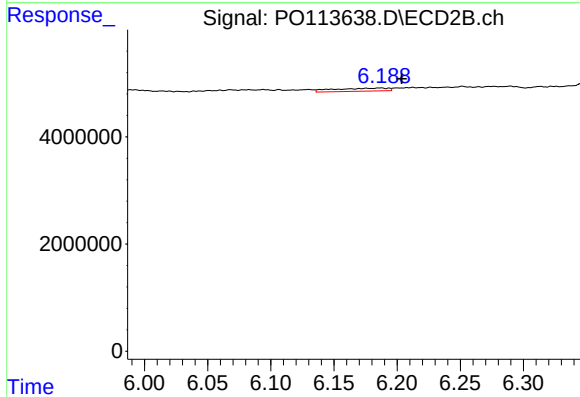


#31 AR-1260-1

R.T.: 6.187 min
Delta R.T.: -0.016 min
Response: 1686813
Conc: 6.61 ng/ml

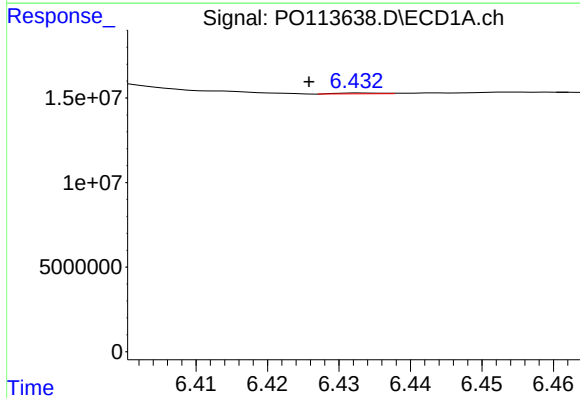


#32 AR-1260-2

R.T.: 6.433 min
Delta R.T.: 0.008 min
Response: 193070
Conc: 0.28 ng/ml

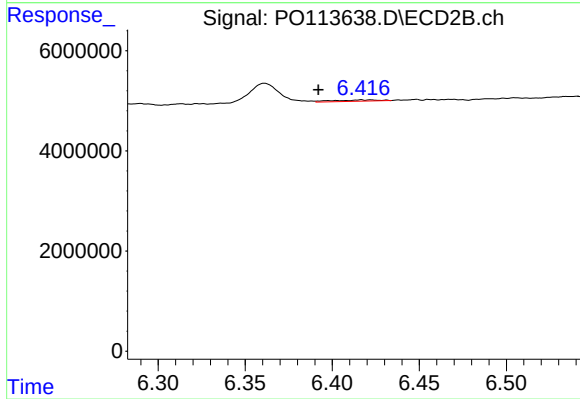

#32 AR-1260-2


R.T.: 6.416 min
Delta R.T.: 0.024 min
Response: 486782
Conc: 1.41 ng/ml

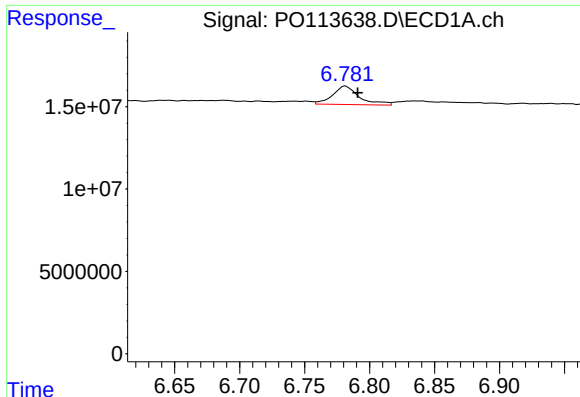

#33 AR-1260-3


R.T.: 6.781 min
Delta R.T.: -0.010 min
Response: 16006233
Conc: 25.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

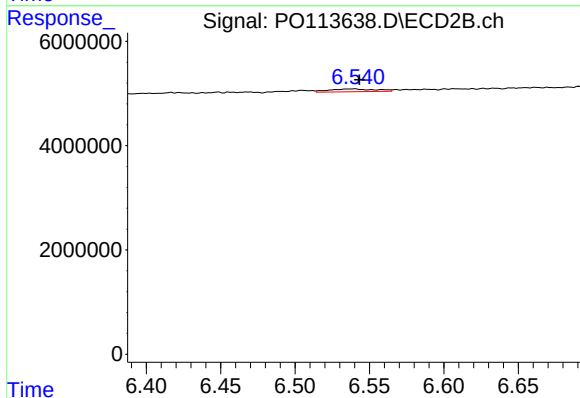


#33 AR-1260-3

R.T.: 6.540 min
Delta R.T.: -0.003 min
Response: 1167925
Conc: 3.93 ng/ml

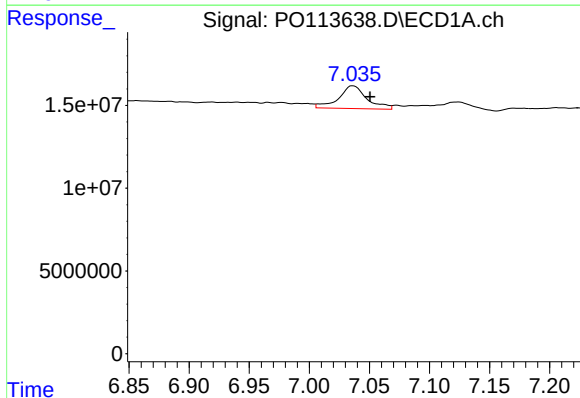


#34 AR-1260-4

R.T.: 7.036 min
Delta R.T.: -0.014 min
Response: 22531217
Conc: 50.31 ng/ml

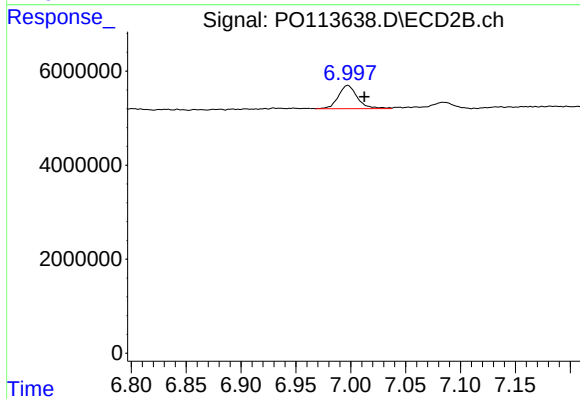

#34 AR-1260-4


R.T.: 6.997 min
Delta R.T.: -0.015 min
Response: 5956933
Conc: 28.74 ng/ml

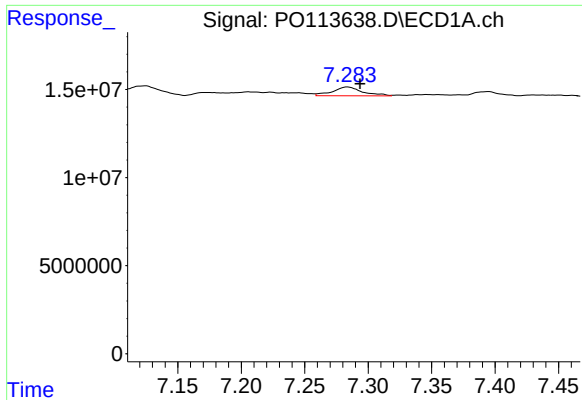

#35 AR-1260-5


R.T.: 7.284 min
Delta R.T.: -0.010 min
Response: 8246254
Conc: 6.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

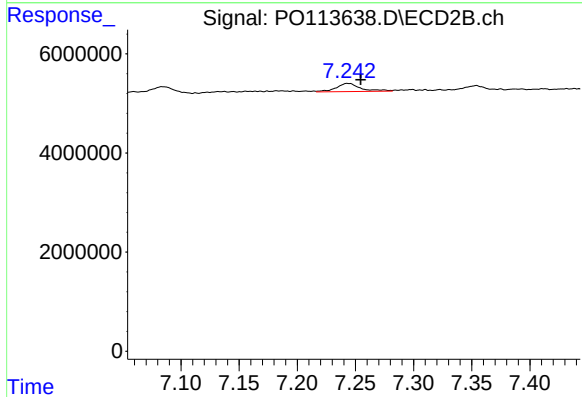


#35 AR-1260-5

R.T.: 7.243 min
Delta R.T.: -0.011 min
Response: 2439651
Conc: 5.21 ng/ml

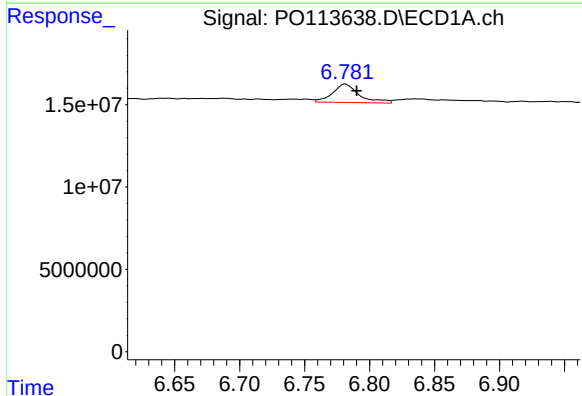


#36 AR-1262-1

R.T.: 6.781 min
Delta R.T.: -0.009 min
Response: 16006233
Conc: 17.48 ng/ml

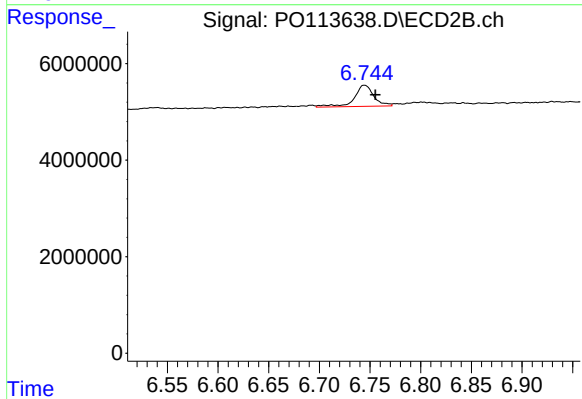

#36 AR-1262-1


R.T.: 6.744 min
Delta R.T.: -0.011 min
Response: 5893652
Conc: 14.21 ng/ml

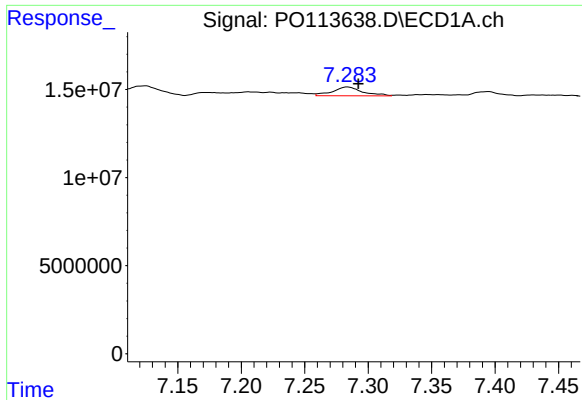

#37 AR-1262-2


R.T.: 7.284 min
Delta R.T.: -0.008 min
Response: 8246254
Conc: 5.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

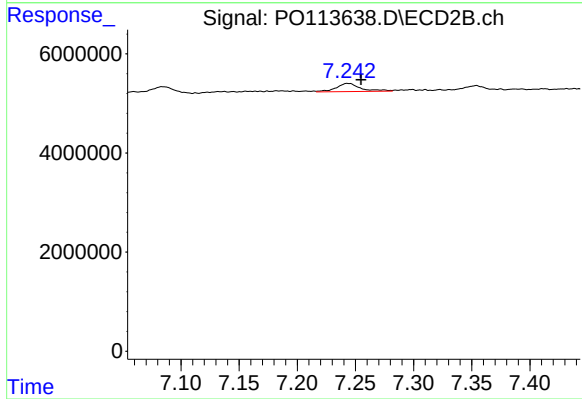


#37 AR-1262-2

R.T.: 7.243 min
Delta R.T.: -0.011 min
Response: 2439651
Conc: 4.71 ng/ml

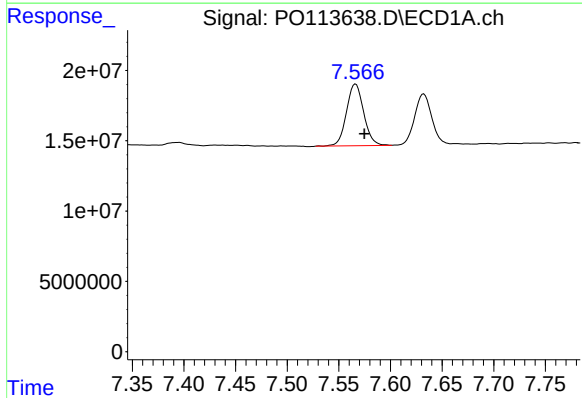


#38 AR-1262-3

R.T.: 7.566 min
Delta R.T.: -0.008 min
Response: 50874682
Conc: 91.81 ng/ml

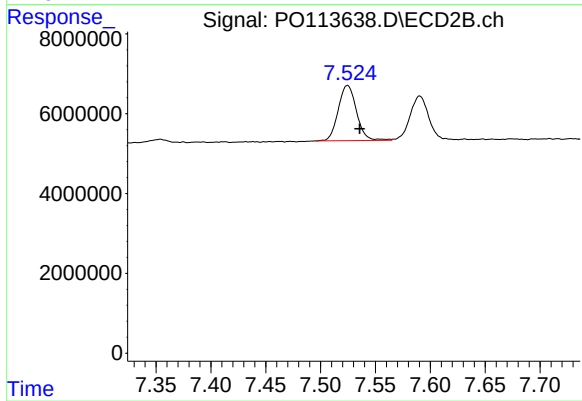

#38 AR-1262-3


R.T.: 7.524 min
Delta R.T.: -0.011 min
Response: 16076862
Conc: 89.52 ng/ml

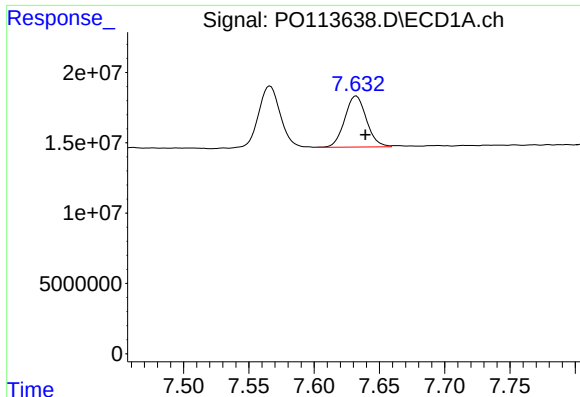

#39 AR-1262-4


R.T.: 7.632 min
Delta R.T.: -0.007 min
Response: 41893870
Conc: 42.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

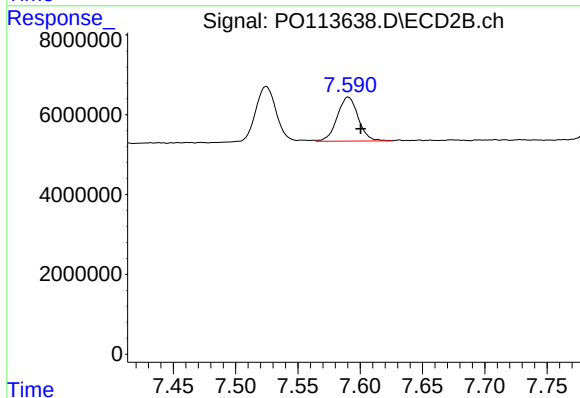


#39 AR-1262-4

R.T.: 7.590 min
Delta R.T.: -0.010 min
Response: 13007070
Conc: 44.87 ng/ml

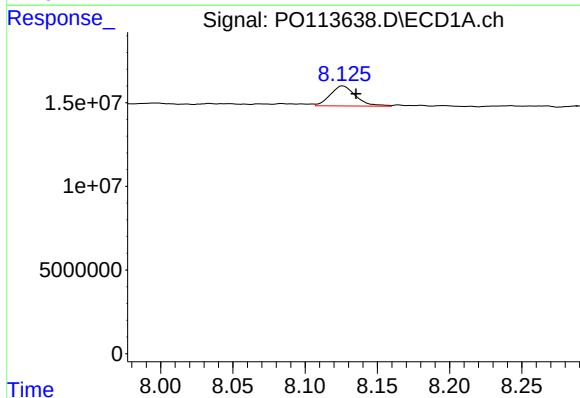


#40 AR-1262-5

R.T.: 8.126 min
Delta R.T.: -0.009 min
Response: 14642454
Conc: 35.12 ng/ml

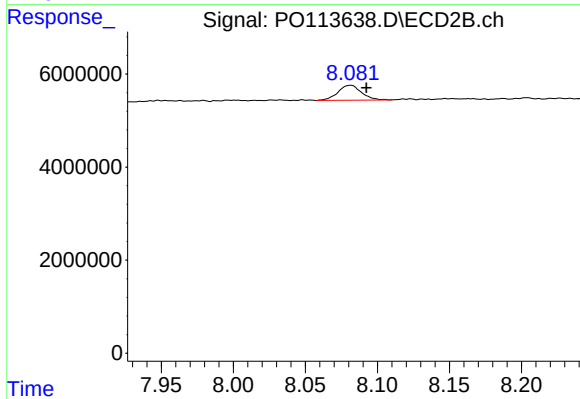

#40 AR-1262-5


R.T.: 8.081 min
Delta R.T.: -0.011 min
Response: 3680843
Conc: 33.98 ng/ml

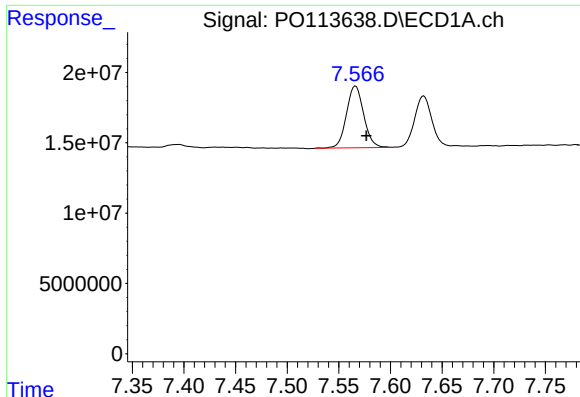

#41 AR-1268-1


R.T.: 7.566 min
Delta R.T.: -0.011 min
Response: 50874682
Conc: 29.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

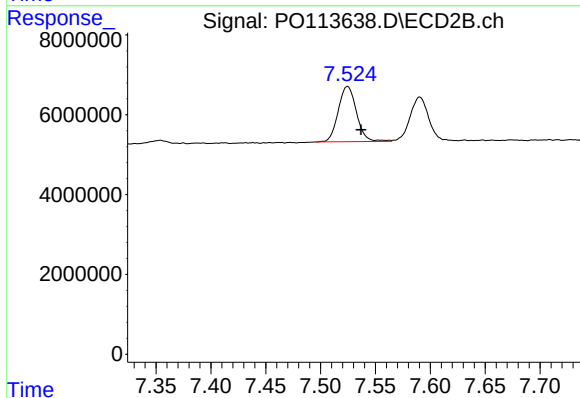


#41 AR-1268-1

R.T.: 7.524 min
Delta R.T.: -0.012 min
Response: 16076862
Conc: 31.56 ng/ml

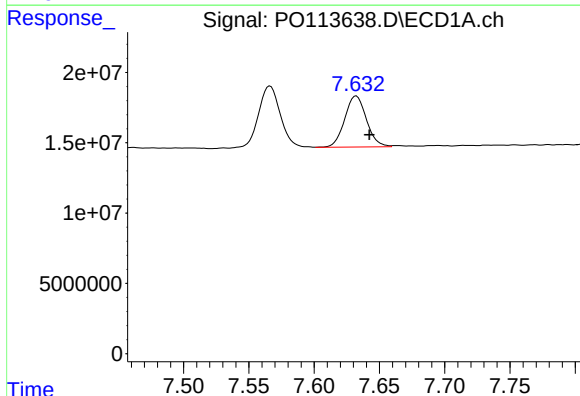


#42 AR-1268-2

R.T.: 7.632 min
Delta R.T.: -0.010 min
Response: 41893870
Conc: 28.93 ng/ml

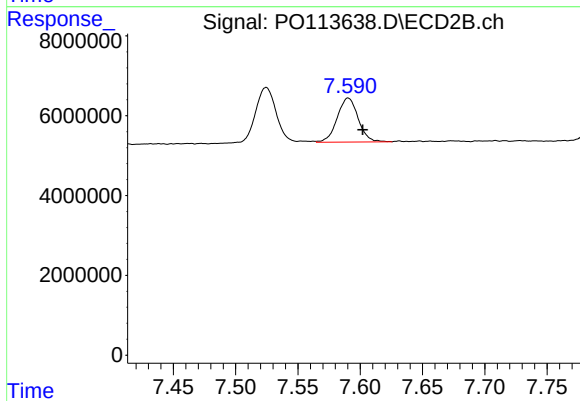

#42 AR-1268-2


R.T.: 7.590 min
Delta R.T.: -0.012 min
Response: 13007070
Conc: 31.31 ng/ml

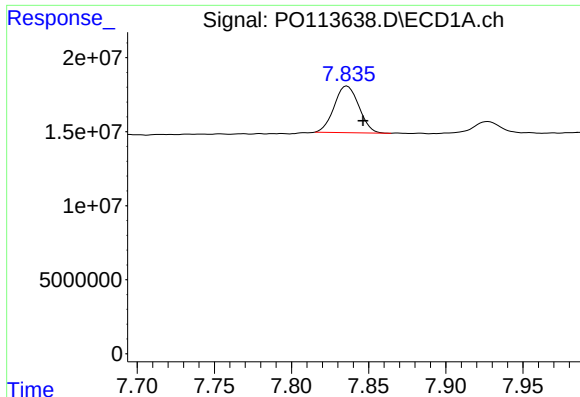

#43 AR-1268-3


R.T.: 7.836 min
Delta R.T.: -0.010 min
Response: 35041632
Conc: 29.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

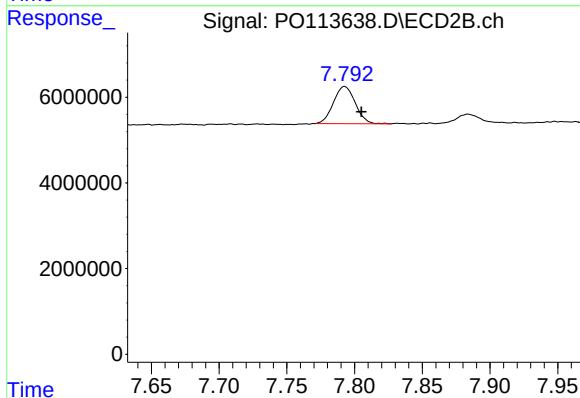


#43 AR-1268-3

R.T.: 7.793 min
Delta R.T.: -0.012 min
Response: 9724673
Conc: 29.78 ng/ml

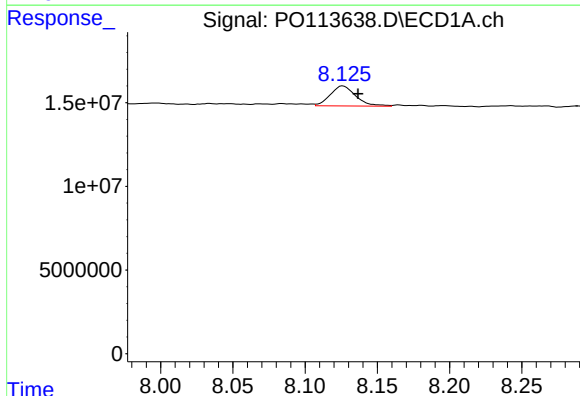


#44 AR-1268-4

R.T.: 8.126 min
Delta R.T.: -0.010 min
Response: 14642454
Conc: 31.79 ng/ml

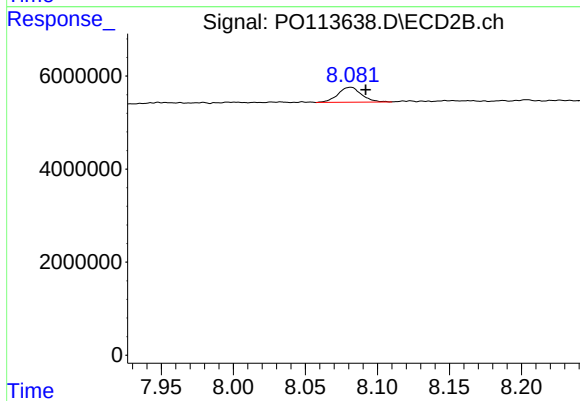

#44 AR-1268-4


R.T.: 8.081 min
Delta R.T.: -0.011 min
Response: 3680843
Conc: 30.56 ng/ml

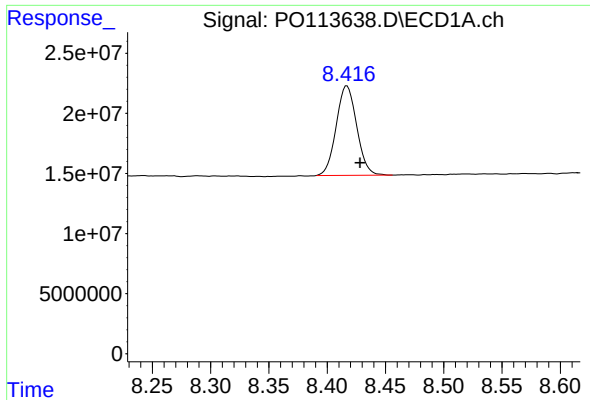

#45 AR-1268-5

R.T.: 8.417 min
Delta R.T.: -0.011 min
Response: 91328010
Conc: 28.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

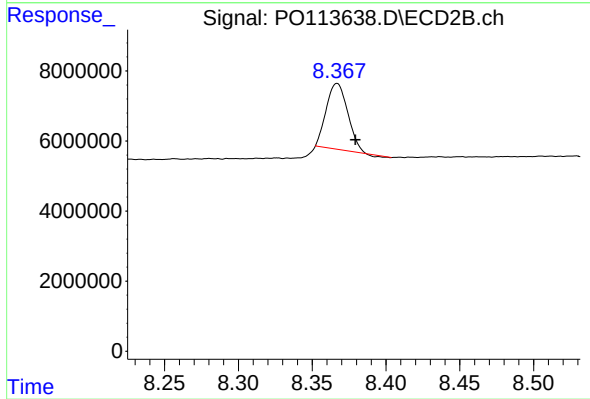

#45 AR-1268-5

R.T.: 8.367 min
Delta R.T.: -0.012 min
Response: 18888899
Conc: 24.19 ng/ml