

Data Path : P:\HPCHEM1\ECD_0\Data\P0091115\
Data File : P0024527.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2015 17:00
Operator : IZ/UA
Sample : G3617-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
090915-D534-E-D-B

Manual Integrations
APPROVED

ugo
9/14/2015 10:21:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 09:56:03 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.117	3.226	3214613	5043504	14.492m	17.926
2)	SA Decachlor...	9.649	8.026	1838601	3931303	15.090	14.541

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0091115\
Data File : P0024527.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2015 17:00
Operator : IZ/UA
Sample : G3617-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
090915-D534-E-D-B


Manual Integrations
APPROVED

ugo
9/14/2015 10:21:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 09:56:03 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

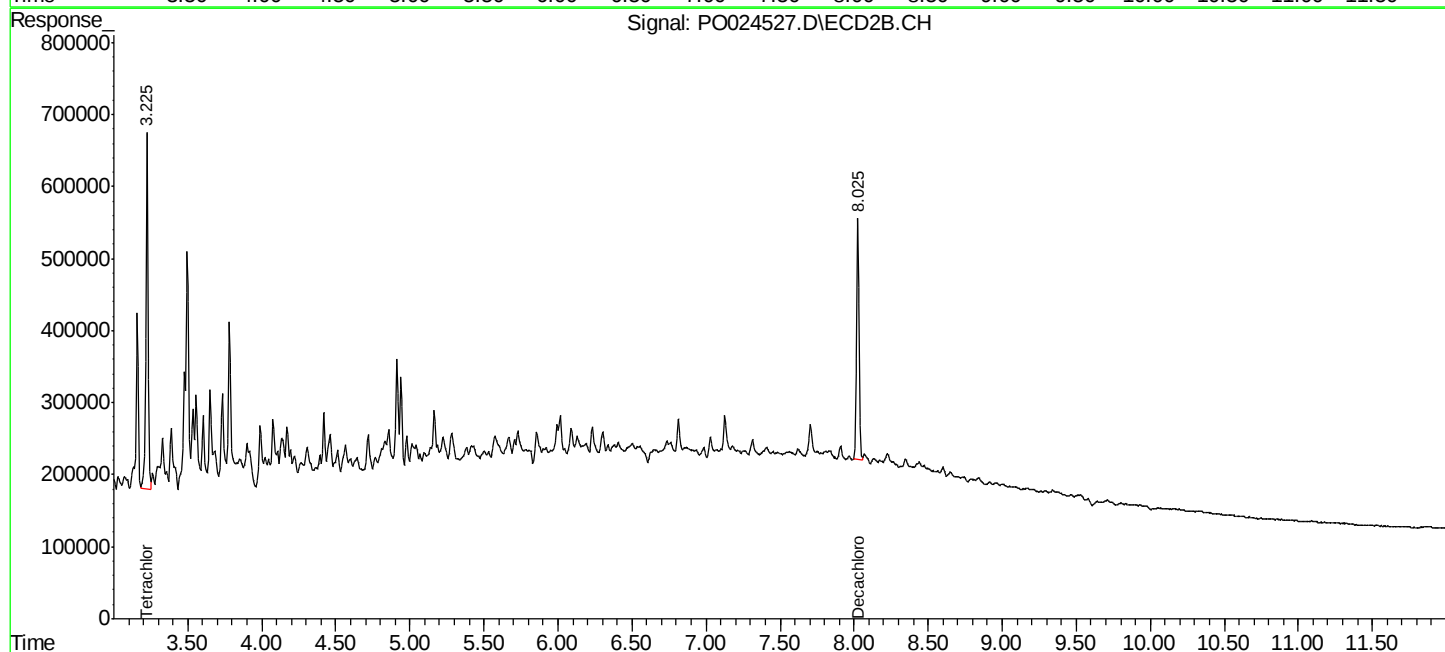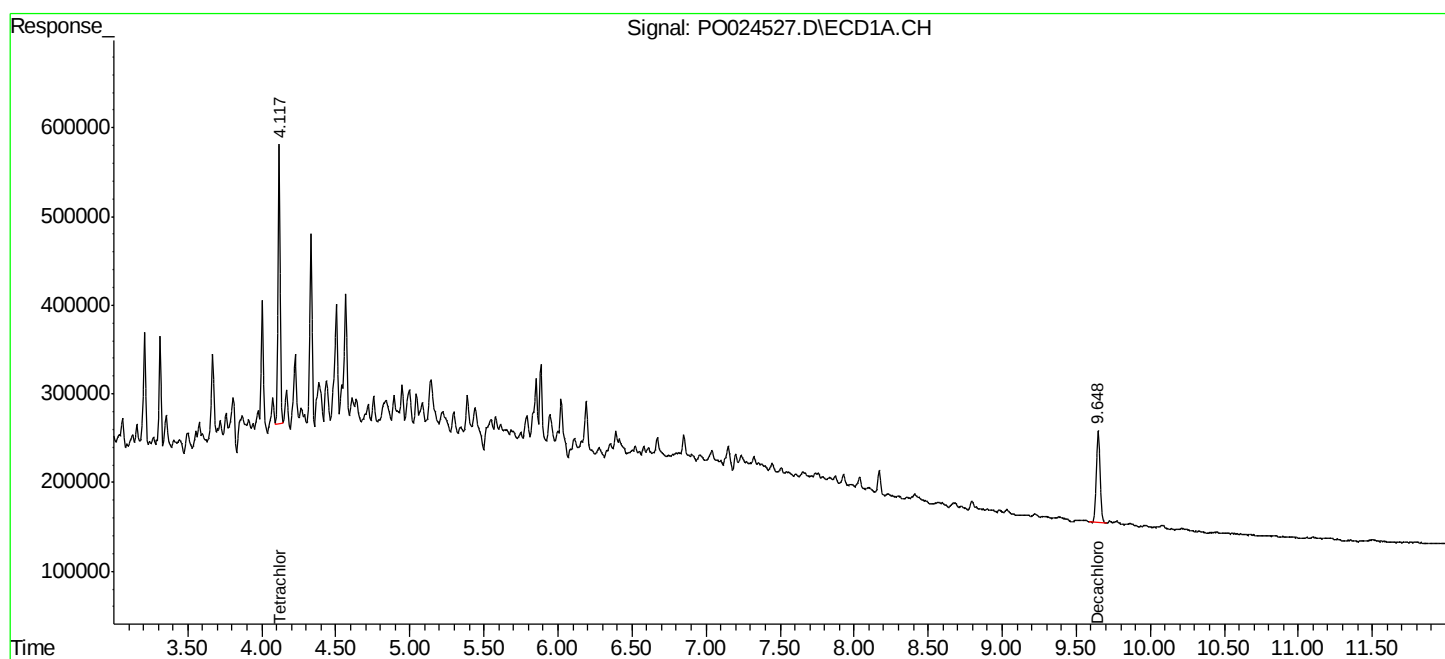

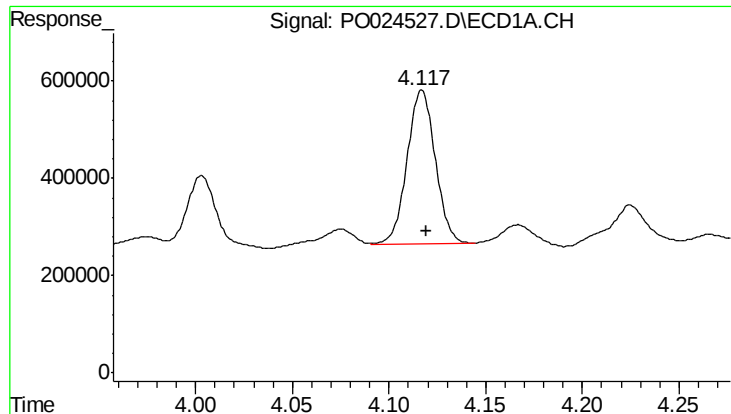


#1 Tetrachloro-m-xylene

R.T.: 4.117 min
Delta R.T.: -0.003 min
Response: 3214613
Conc: 14.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
090915-D534-E-D-B


Manual Integrations
APPROVED

ugo
9/14/2015 10:21:14 AM

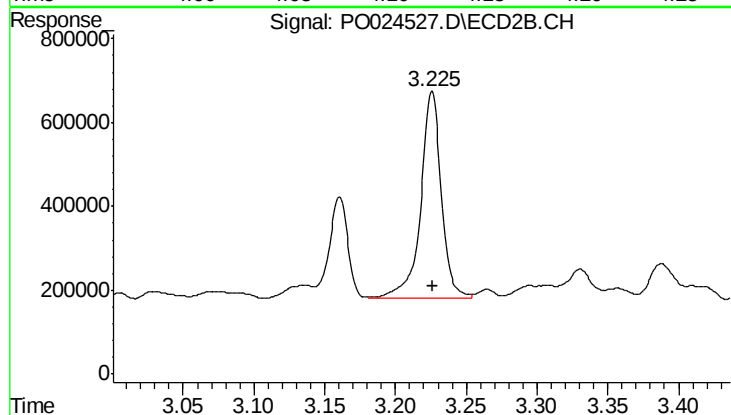


#1 Tetrachloro-m-xylene

R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 5043504
Conc: 17.93 ng/ml

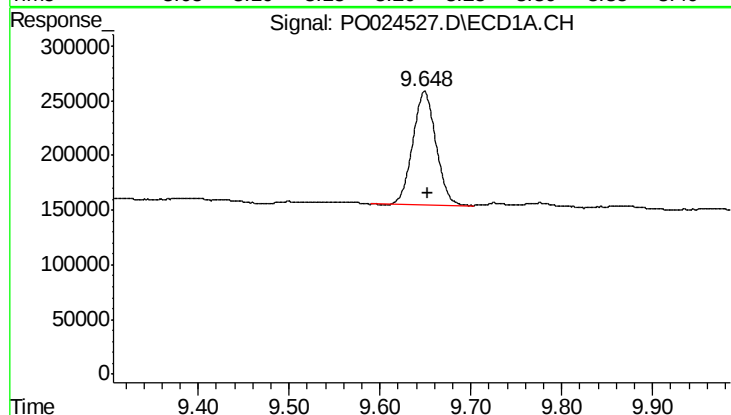

#2 Decachlorobiphenyl

R.T.: 9.649 min
Delta R.T.: -0.003 min
Response: 1838601
Conc: 15.09 ng/ml

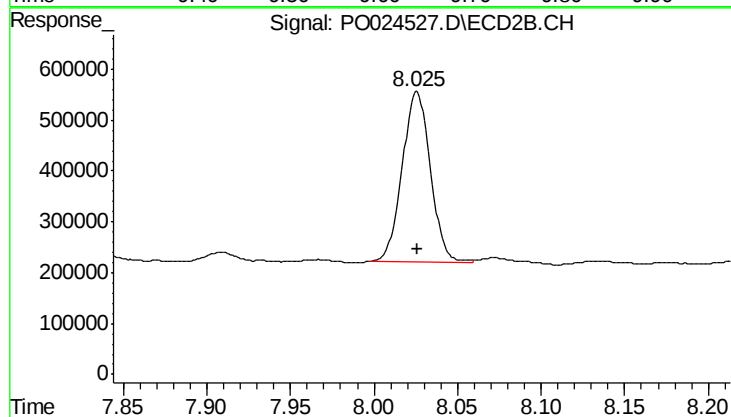

#2 Decachlorobiphenyl

R.T.: 8.026 min
Delta R.T.: 0.000 min
Response: 3931303
Conc: 14.54 ng/ml