

Data Path : P:\HPCHEM1\ECD_0\Data\P0091115\
Data File : P0024529.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2015 17:29
Operator : IZ/UA
Sample : G3617-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
090915-D534-E-U-B

Manual Integrations
APPROVED

ugo
9/14/2015 10:21:31 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 09:57:20 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.116	3.226	3550321	5269093	16.005m	18.728
2) SA Decachlor...	9.648	8.025	1953615	4081473	16.034	15.097

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0091115\
Data File : P0024529.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2015 17:29
Operator : IZ/UA
Sample : G3617-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
090915-D534-E-U-B


Manual Integrations
APPROVED

ugo
9/14/2015 10:21:31 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 09:57:20 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

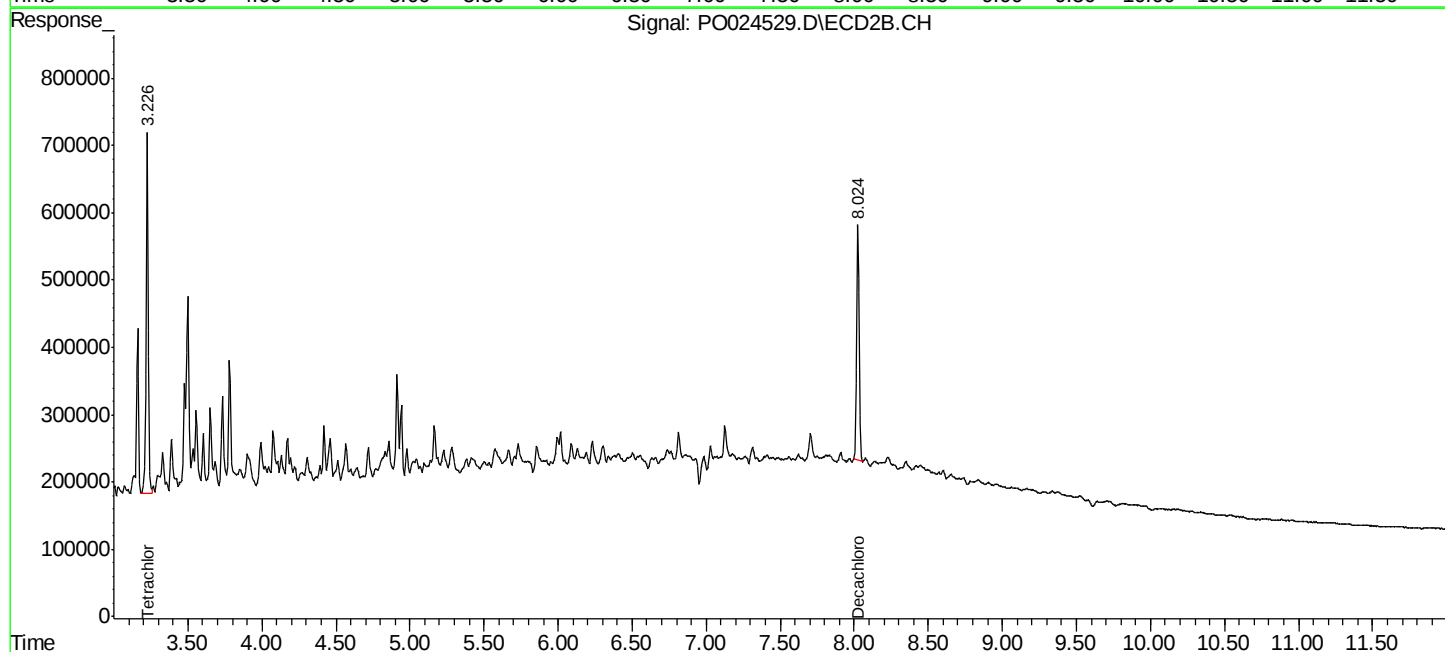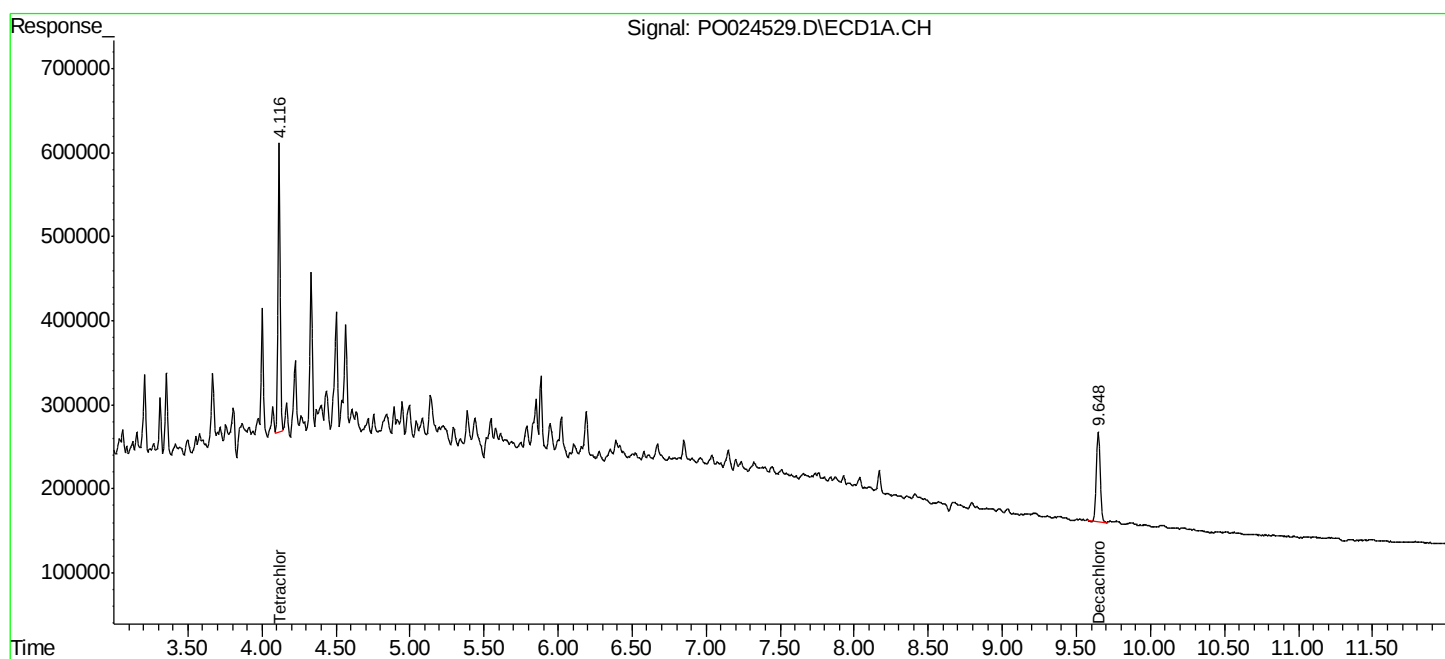

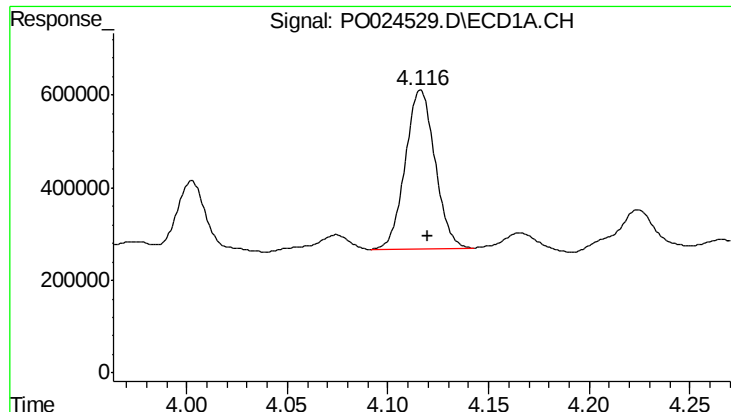


#1 Tetrachloro-m-xylene

R.T.: 4.116 min
Delta R.T.: -0.004 min
Response: 3550321
Conc: 16.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
090915-D534-E-U-B


Manual Integrations
APPROVED

ugo
9/14/2015 10:21:31 AM

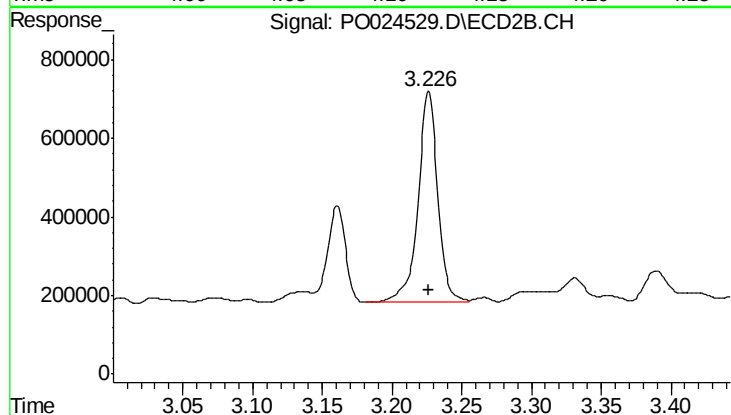


#1 Tetrachloro-m-xylene

R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 5269093
Conc: 18.73 ng/ml

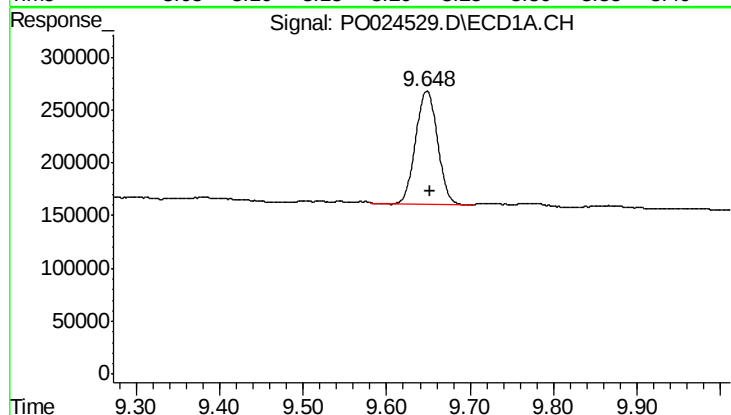

#2 Decachlorobiphenyl

R.T.: 9.648 min
Delta R.T.: -0.004 min
Response: 1953615
Conc: 16.03 ng/ml

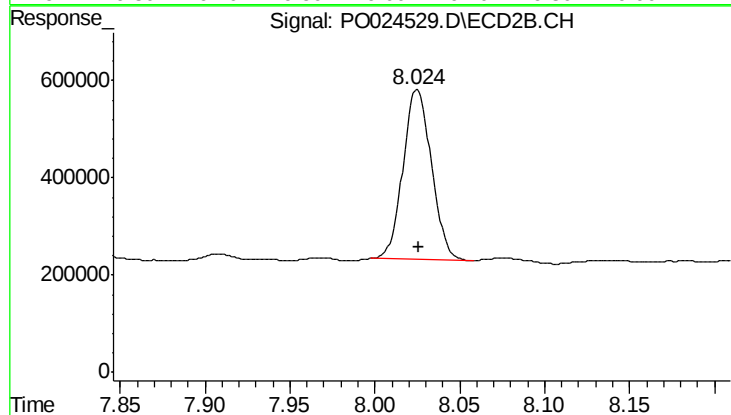

#2 Decachlorobiphenyl

R.T.: 8.025 min
Delta R.T.: -0.001 min
Response: 4081473
Conc: 15.10 ng/ml