

Data Path : P:\HPCHEM1\ECD_0\Data\P0091115\
Data File : P0024530.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2015 17:44
Operator : IZ/UA
Sample : G3617-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
090915-D534-E-U-S

Manual Integrations
APPROVED

ugo
9/14/2015 10:21:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 09:57:55 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.116	3.226	3463958	5199961	15.616m	18.482
2) SA Decachlor...	9.649	8.026	1865057	3914641	15.308	14.480

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0091115\
Data File : P0024530.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2015 17:44
Operator : IZ/UA
Sample : G3617-04
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
090915-D534-E-U-S


Manual Integrations
APPROVED

ugo
9/14/2015 10:21:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 09:57:55 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

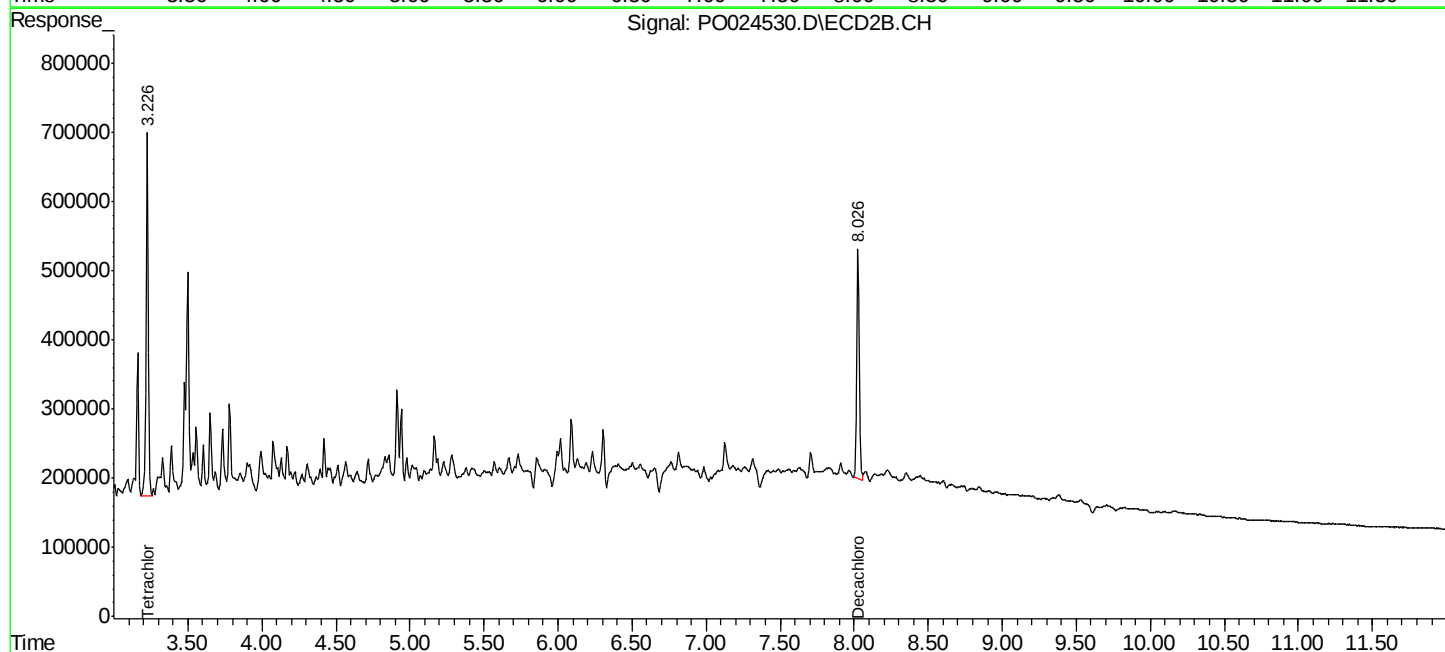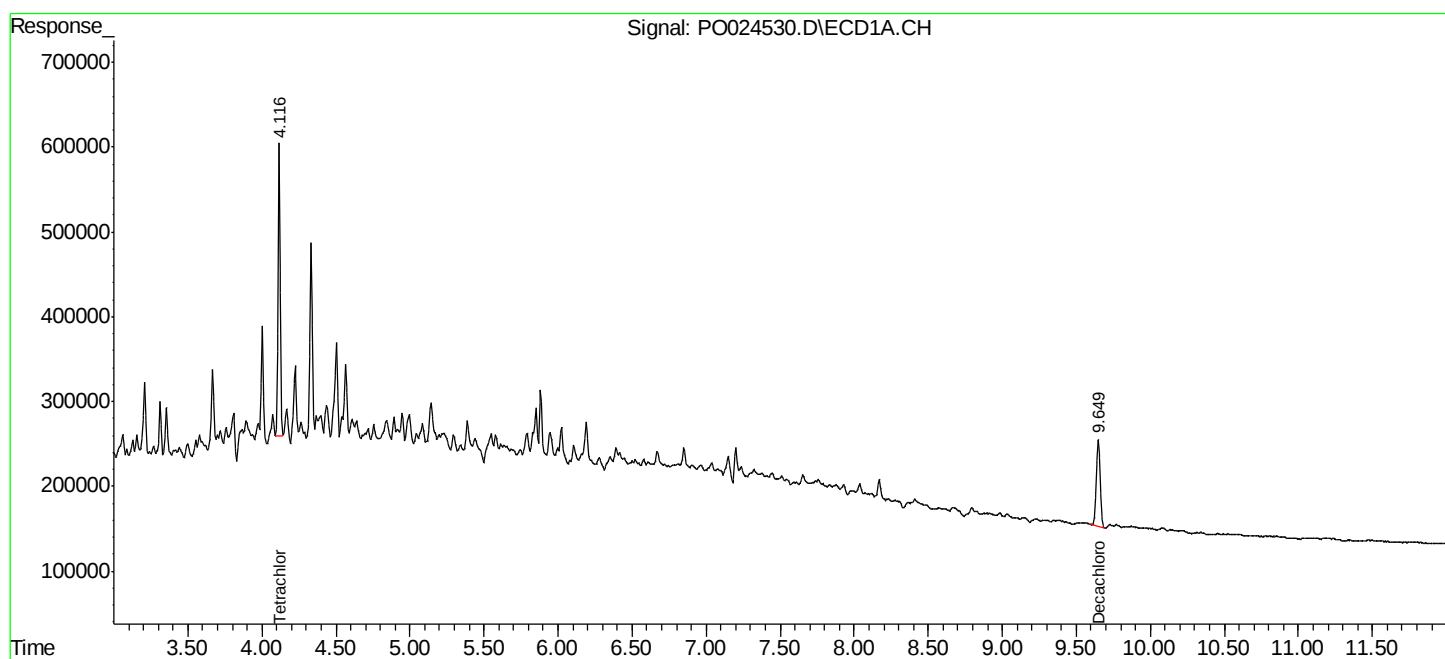

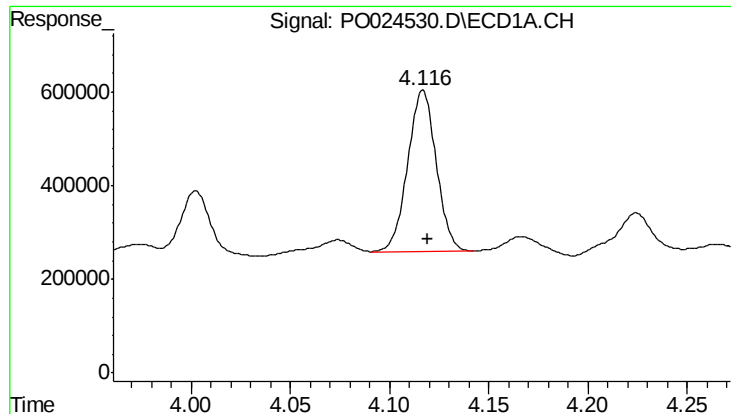


#1 Tetrachloro-m-xylene

R.T.: 4.116 min
Delta R.T.: -0.003 min
Response: 3463958
Conc: 15.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
090915-D534-E-U-S


Manual Integrations
APPROVED

ugo
9/14/2015 10:21:36 AM

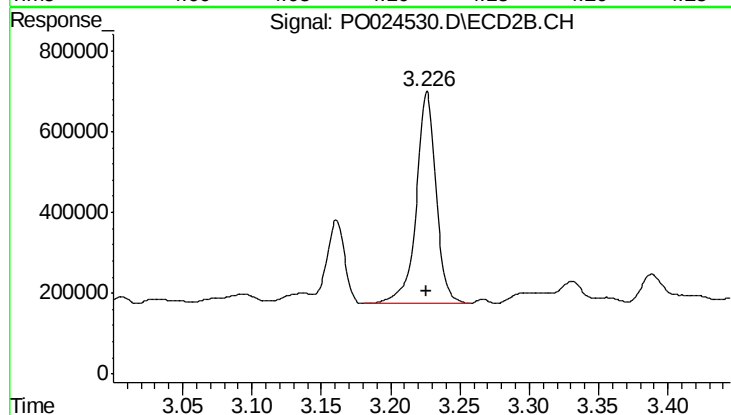


#1 Tetrachloro-m-xylene

R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 5199961
Conc: 18.48 ng/ml

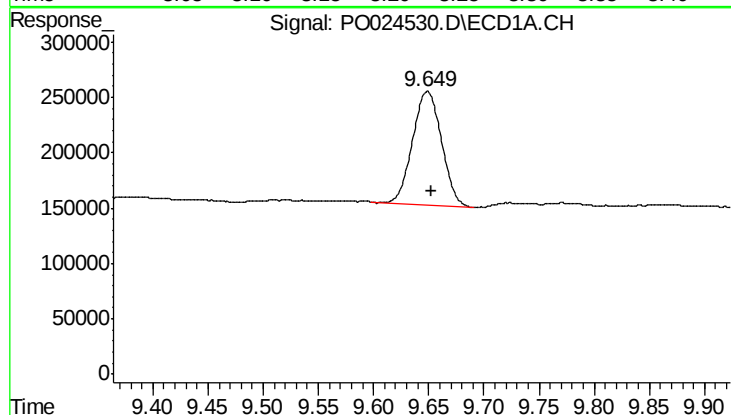

#2 Decachlorobiphenyl

R.T.: 9.649 min
Delta R.T.: -0.003 min
Response: 1865057
Conc: 15.31 ng/ml

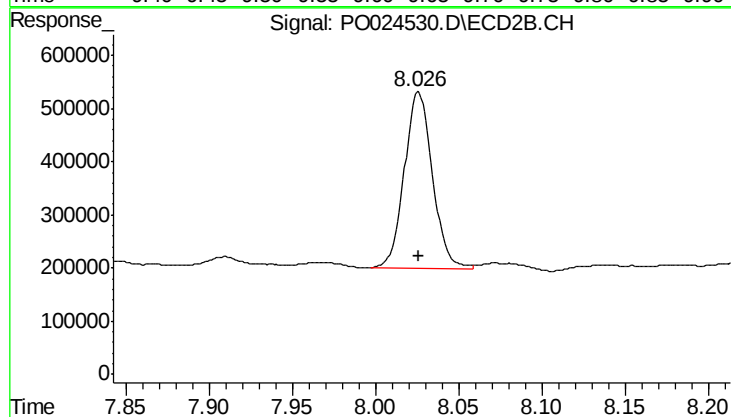

#2 Decachlorobiphenyl

R.T.: 8.026 min
Delta R.T.: 0.000 min
Response: 3914641
Conc: 14.48 ng/ml