

Data Path : P:\HPCHEM1\ECD_0\Data\P0091115\
 Data File : P0024532.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Sep 2015 18:14
 Operator : IZ/UA
 Sample : G3635-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 091015-D534-F-D-M

Manual Integrations
 APPROVED

ugo
 9/14/2015 10:21:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 09:59:34 2015
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 12 04:39:58 2015
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.116	3.225	3550540	5484852	16.006m	19.495m
2)	SA Decachlor...	9.647	8.025	1746323	3703216	14.333	13.698

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0091115\
Data File : P0024532.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2015 18:14
Operator : IZ/UA
Sample : G3635-02
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
091015-D534-F-D-M


Manual Integrations
APPROVED

ugo
9/14/2015 10:21:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 09:59:34 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

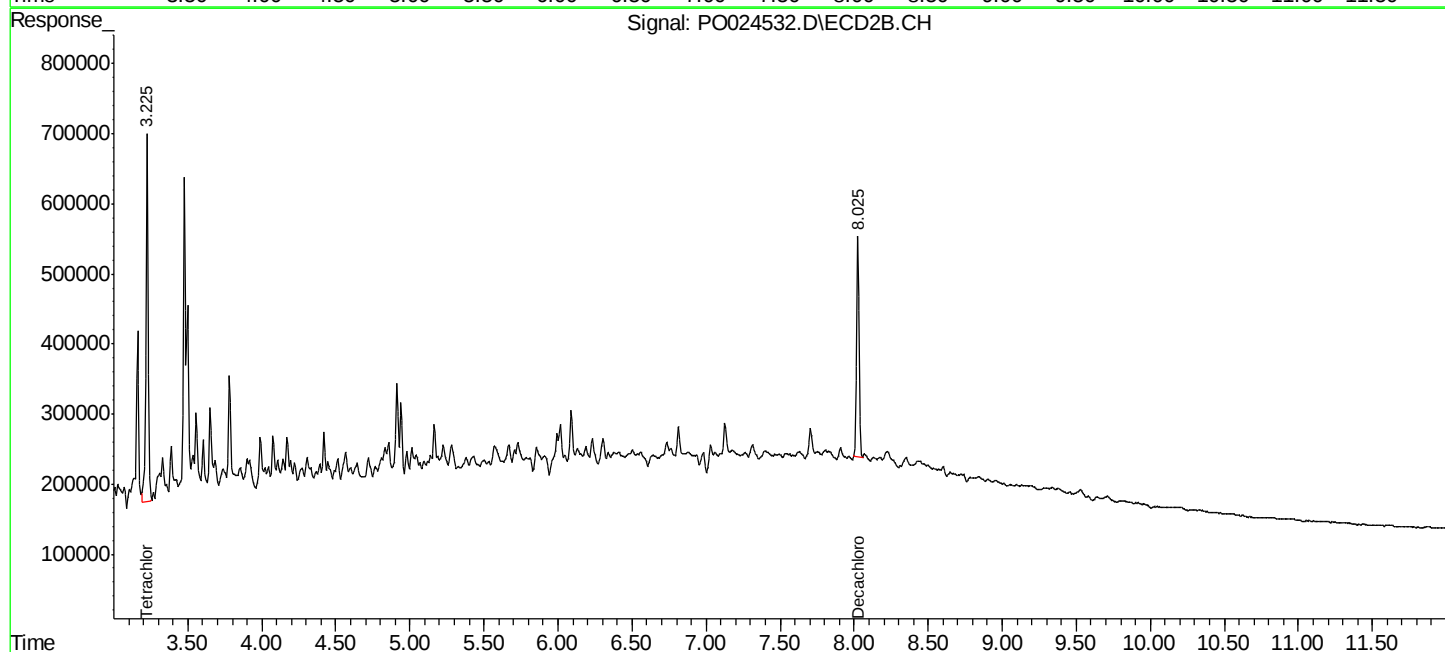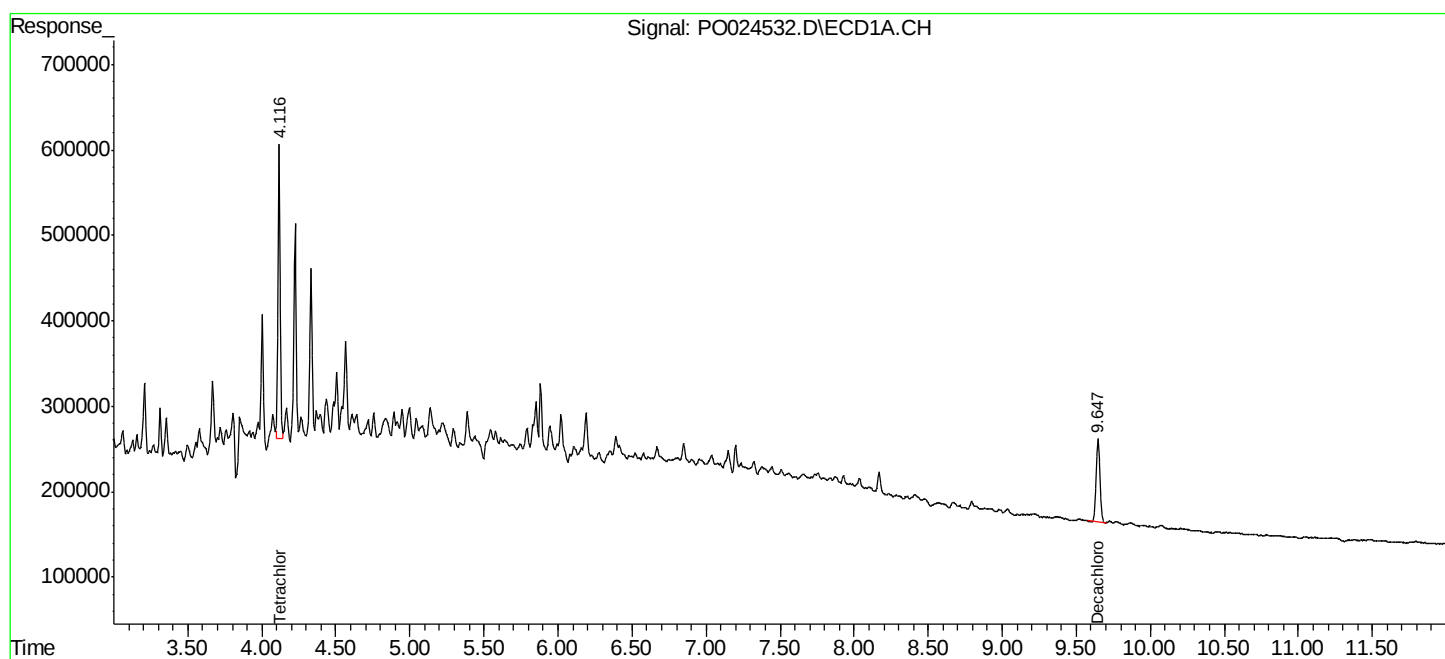

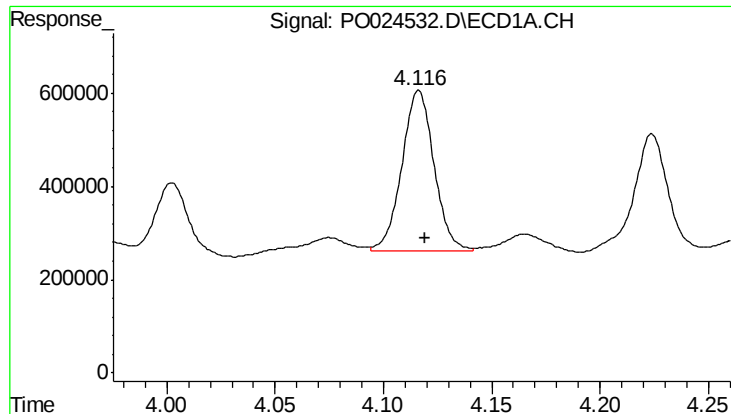


#1 Tetrachloro-m-xylene

R.T.: 4.116 min
Delta R.T.: -0.004 min
Response: 3550540
Conc: 16.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
091015-D534-F-D-M


Manual Integrations
APPROVED

ugo
9/14/2015 10:21:45 AM

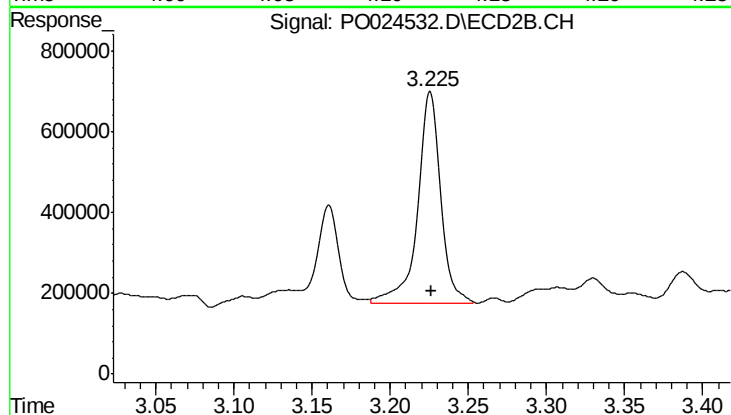


#1 Tetrachloro-m-xylene

R.T.: 3.225 min
Delta R.T.: 0.000 min
Response: 5484852
Conc: 19.49 ng/ml m

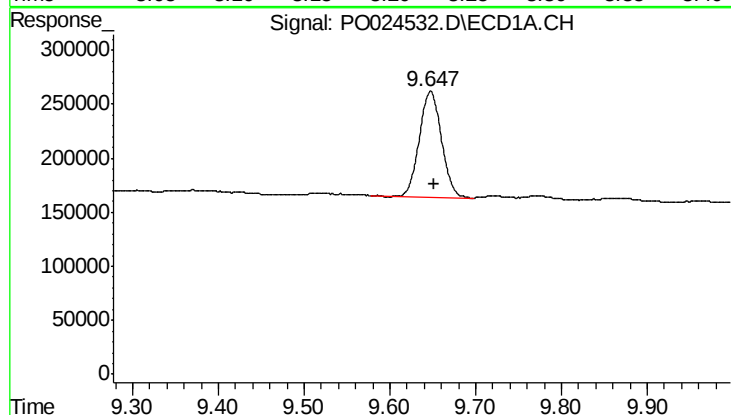

#2 Decachlorobiphenyl

R.T.: 9.647 min
Delta R.T.: -0.005 min
Response: 1746323
Conc: 14.33 ng/ml

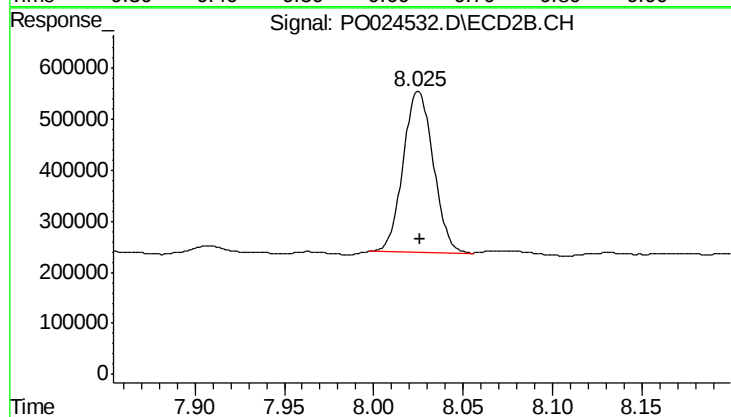

#2 Decachlorobiphenyl

R.T.: 8.025 min
Delta R.T.: -0.001 min
Response: 3703216
Conc: 13.70 ng/ml