

Data Path : P:\HPCHEM1\ECD_0\Data\P0091115\
Data File : P0024534.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2015 18:44
Operator : IZ/UA
Sample : G3635-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
091015-D534-F-U-B

Manual Integrations
APPROVED

ugo
9/14/2015 10:21:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 10:00:41 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.116	3.226	3487183	5352016	15.721m	19.023
2)	SA Decachlor...	9.649	8.026	1597642	3380014	13.113	12.502

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0091115\
Data File : P0024534.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2015 18:44
Operator : IZ/UA
Sample : G3635-04
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
091015-D534-F-U-B


Manual Integrations
APPROVED

ugo
9/14/2015 10:21:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 10:00:41 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

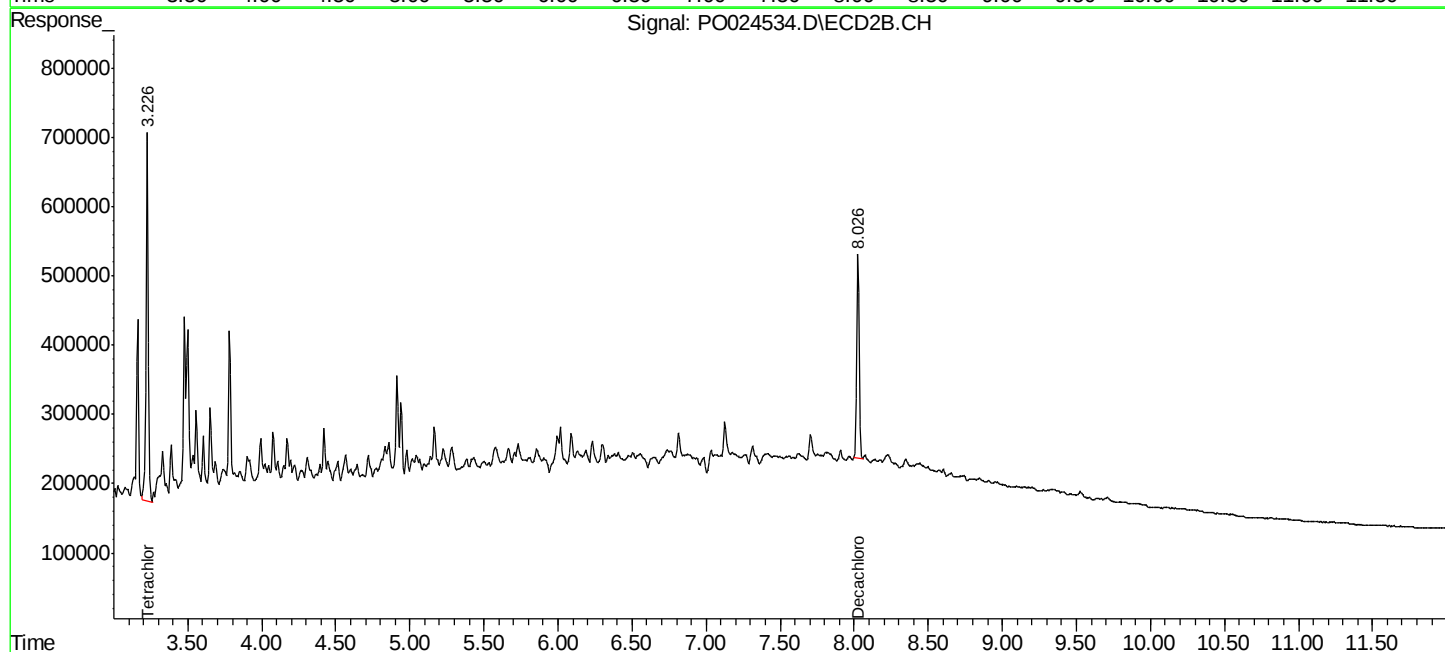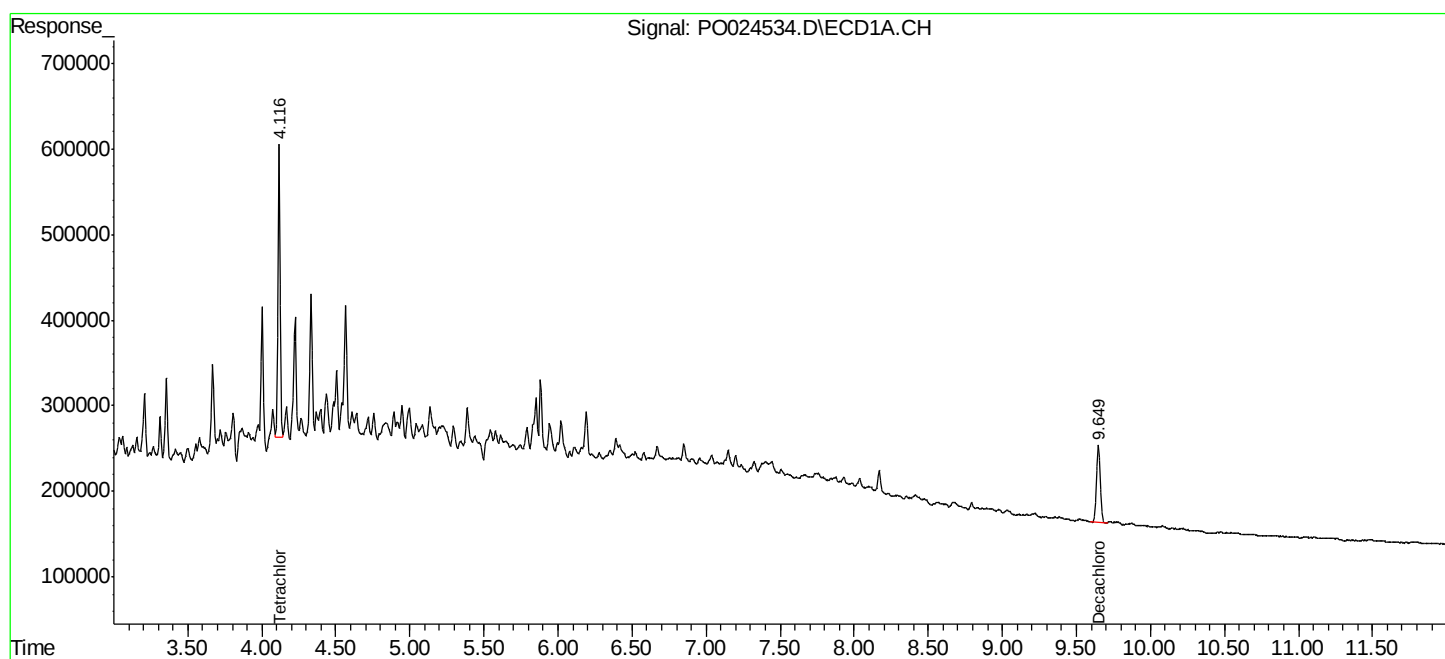

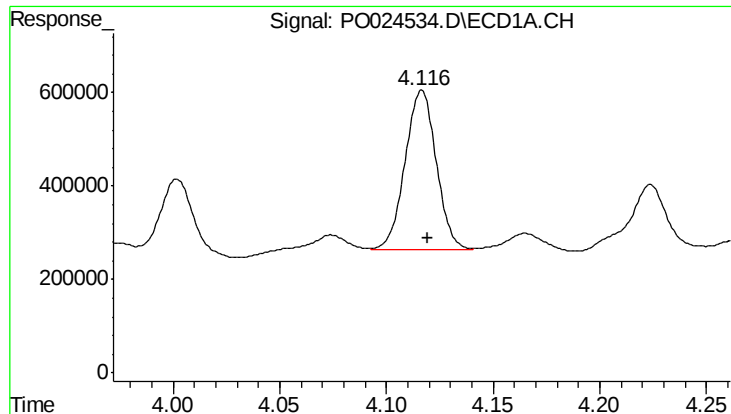


#1 Tetrachloro-m-xylene

R.T.: 4.116 min
Delta R.T.: -0.003 min
Response: 3487183
Conc: 15.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
091015-D534-F-U-B


Manual Integrations
APPROVED

ugo
9/14/2015 10:21:54 AM

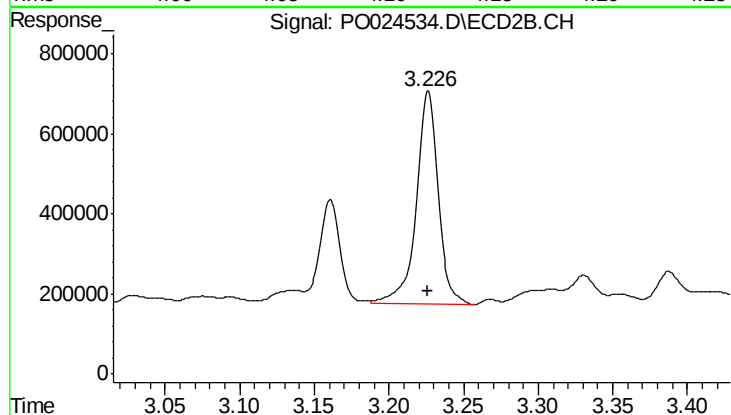


#1 Tetrachloro-m-xylene

R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 5352016
Conc: 19.02 ng/ml

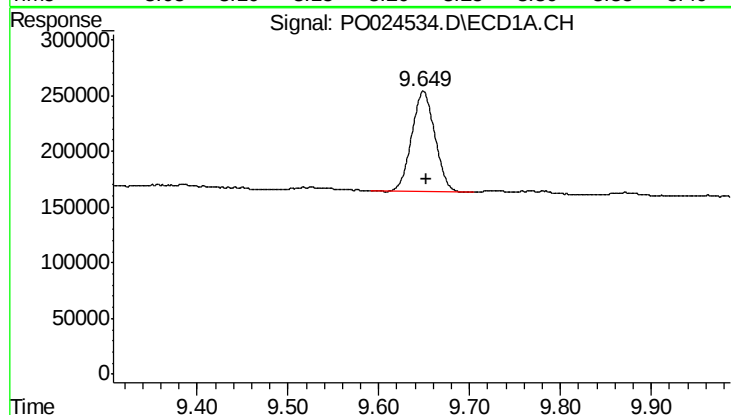

#2 Decachlorobiphenyl

R.T.: 9.649 min
Delta R.T.: -0.003 min
Response: 1597642
Conc: 13.11 ng/ml

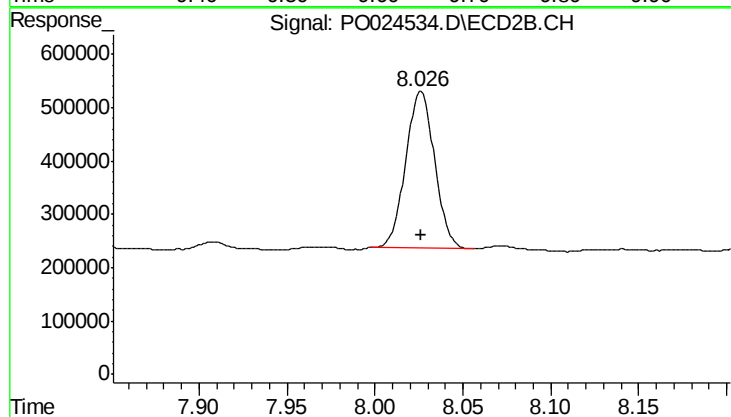

#2 Decachlorobiphenyl

R.T.: 8.026 min
Delta R.T.: 0.000 min
Response: 3380014
Conc: 12.50 ng/ml