

Data Path : P:\HPCHEM1\ECD_0\Data\P0091115\
Data File : P0024535.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2015 18:59
Operator : IZ/UA
Sample : G3635-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
091015-D534-F-U-M

Manual Integrations
APPROVED

ugo
9/14/2015 10:21:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 10:01:37 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.116	3.226	3494280	5479129	15.753m	19.474
2)	SA Decachlor...	9.649	8.026	1776663	3741950	14.582	13.841

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0091115\
Data File : P0024535.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2015 18:59
Operator : IZ/UA
Sample : G3635-05
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
091015-D534-F-U-M


Manual Integrations
APPROVED

ugo
9/14/2015 10:21:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 10:01:37 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

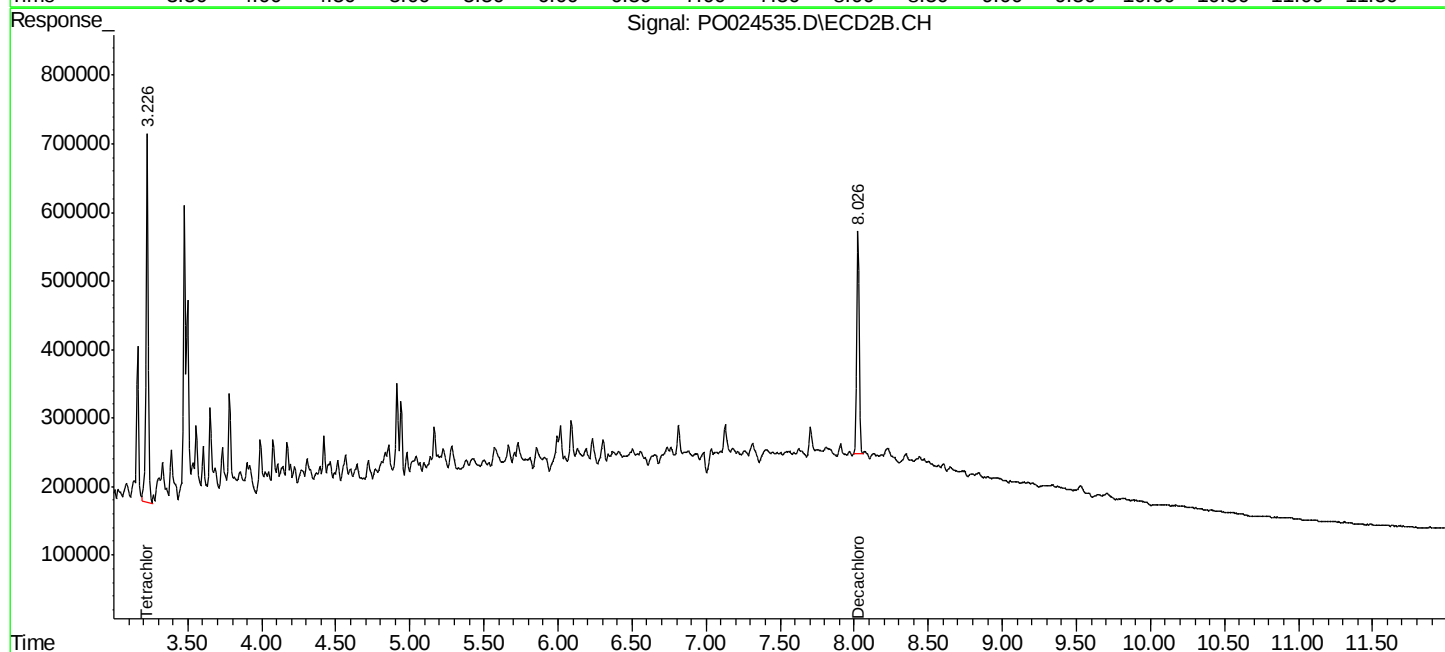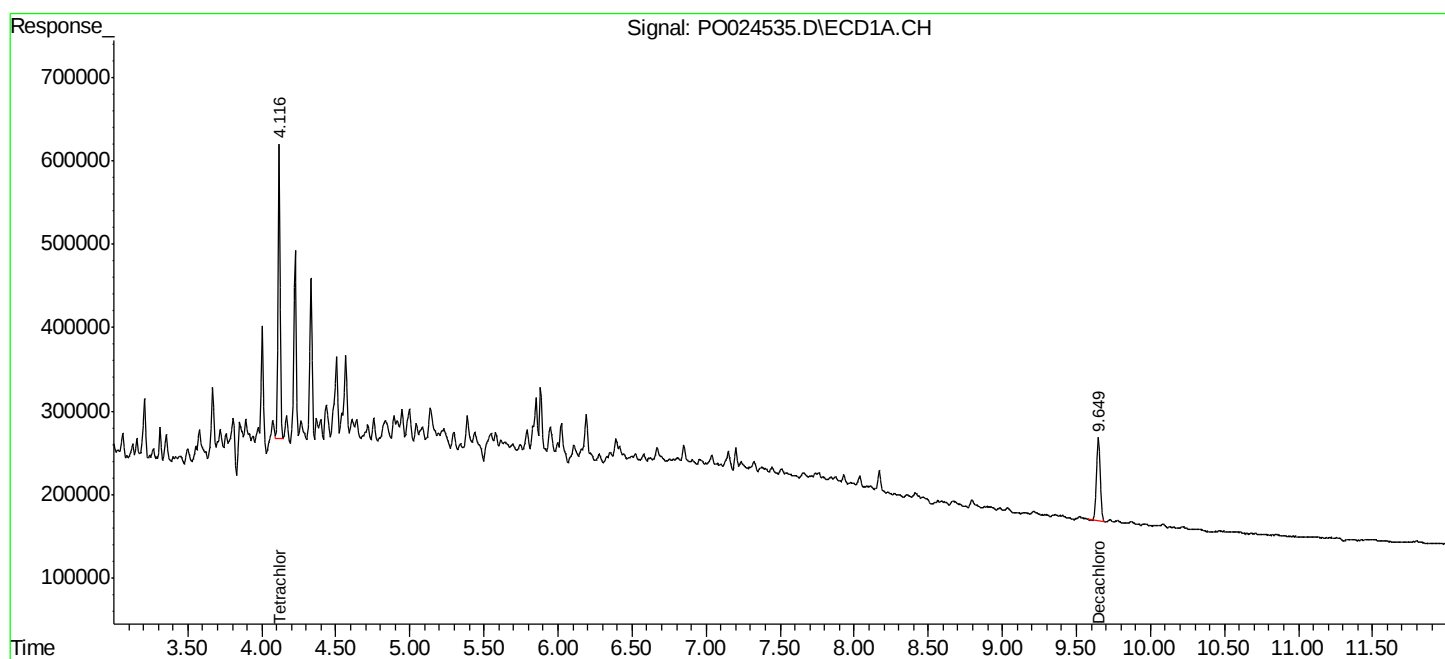

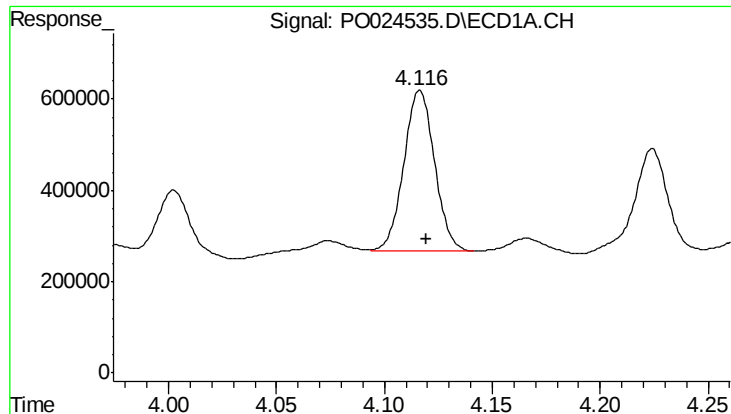


#1 Tetrachloro-m-xylene

R.T.: 4.116 min
Delta R.T.: -0.003 min
Response: 3494280
Conc: 15.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
091015-D534-F-U-M


Manual Integrations
APPROVED

ugo
9/14/2015 10:21:59 AM

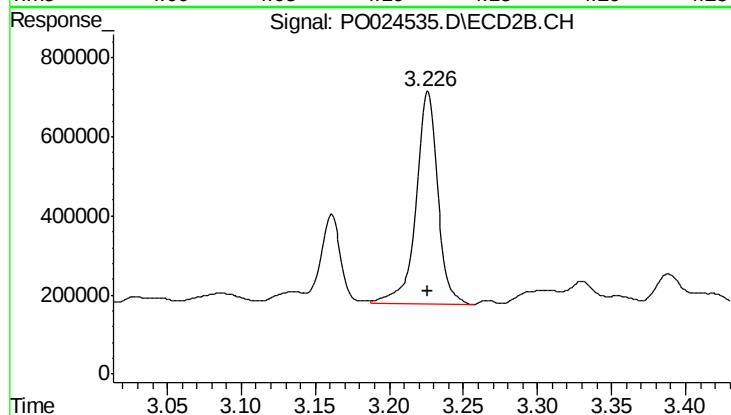


#1 Tetrachloro-m-xylene

R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 5479129
Conc: 19.47 ng/ml

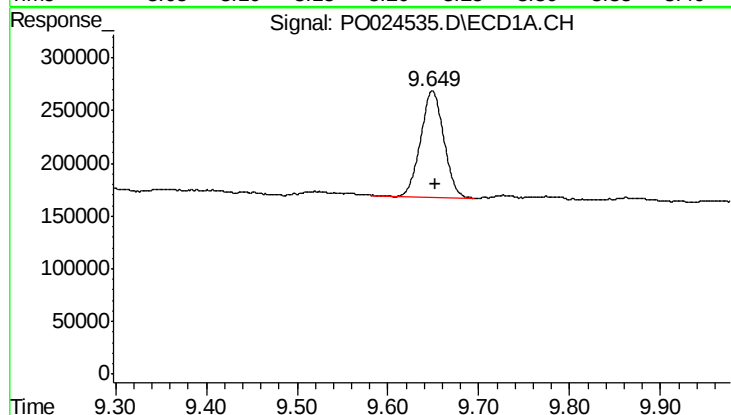

#2 Decachlorobiphenyl

R.T.: 9.649 min
Delta R.T.: -0.003 min
Response: 1776663
Conc: 14.58 ng/ml

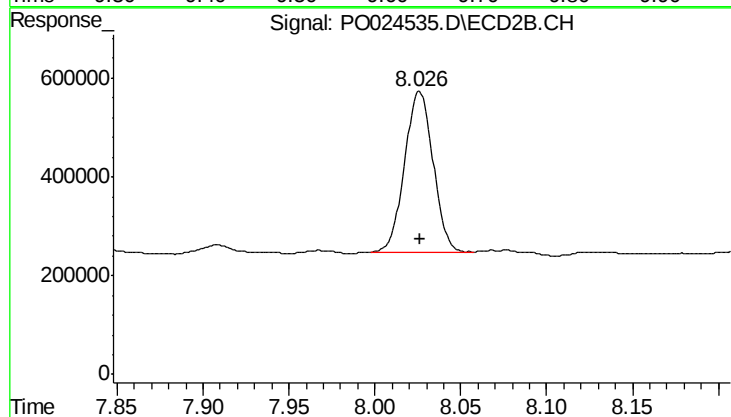

#2 Decachlorobiphenyl

R.T.: 8.026 min
Delta R.T.: 0.000 min
Response: 3741950
Conc: 13.84 ng/ml