

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091119\
 Data File : P0060659.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Sep 2019 10:31
 Operator : SM/AJ
 Sample : K4789-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RT5124

Manual Integrations
 APPROVED

Ankita
 9/12/2019 12:03:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 14:57:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Sep 08 02:12:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.369	3.532	924892	739214	22.291	24.067
2)	SA Decachlor...	10.029	8.416	1025491	777393	19.441m	21.000m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091119\
Data File : P0060659.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2019 10:31
Operator : SM/AJ
Sample : K4789-04
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
RT5124


Manual Integrations
APPROVED

Ankita
9/12/2019 12:03:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 14:57:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

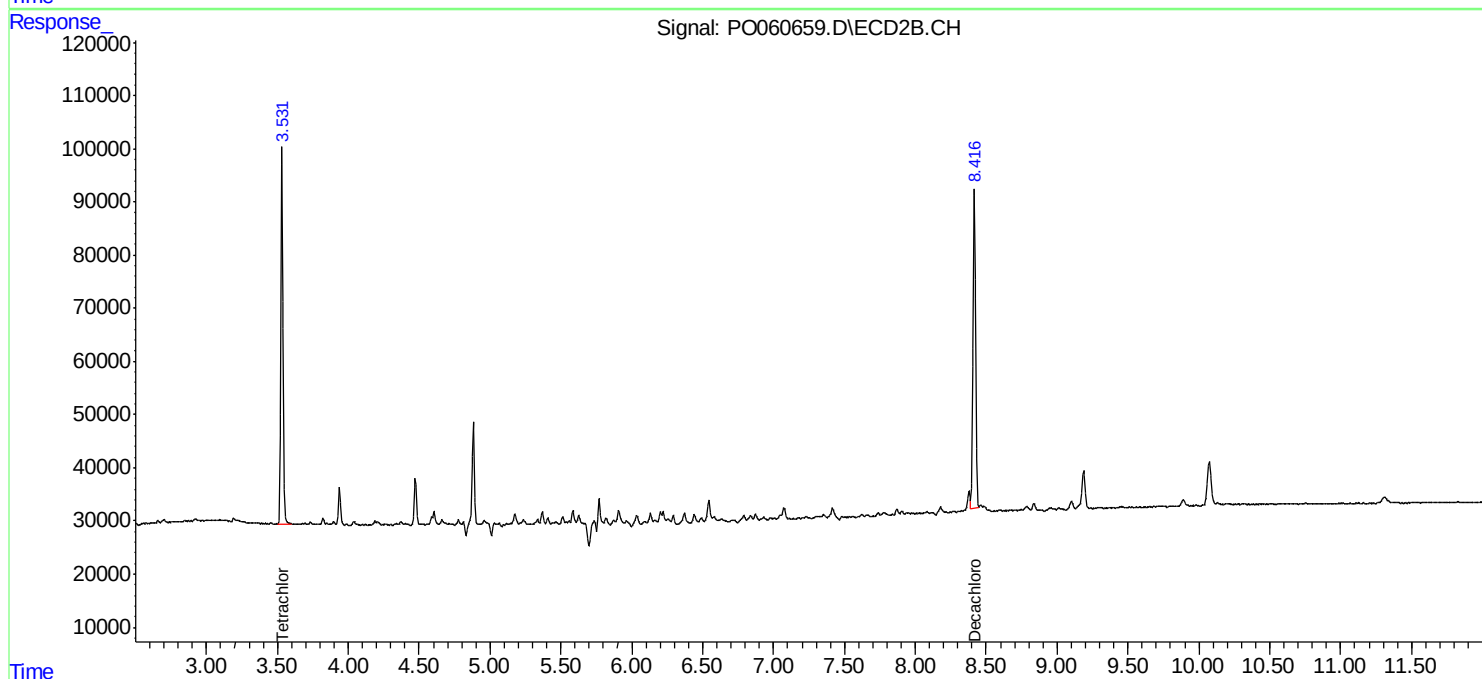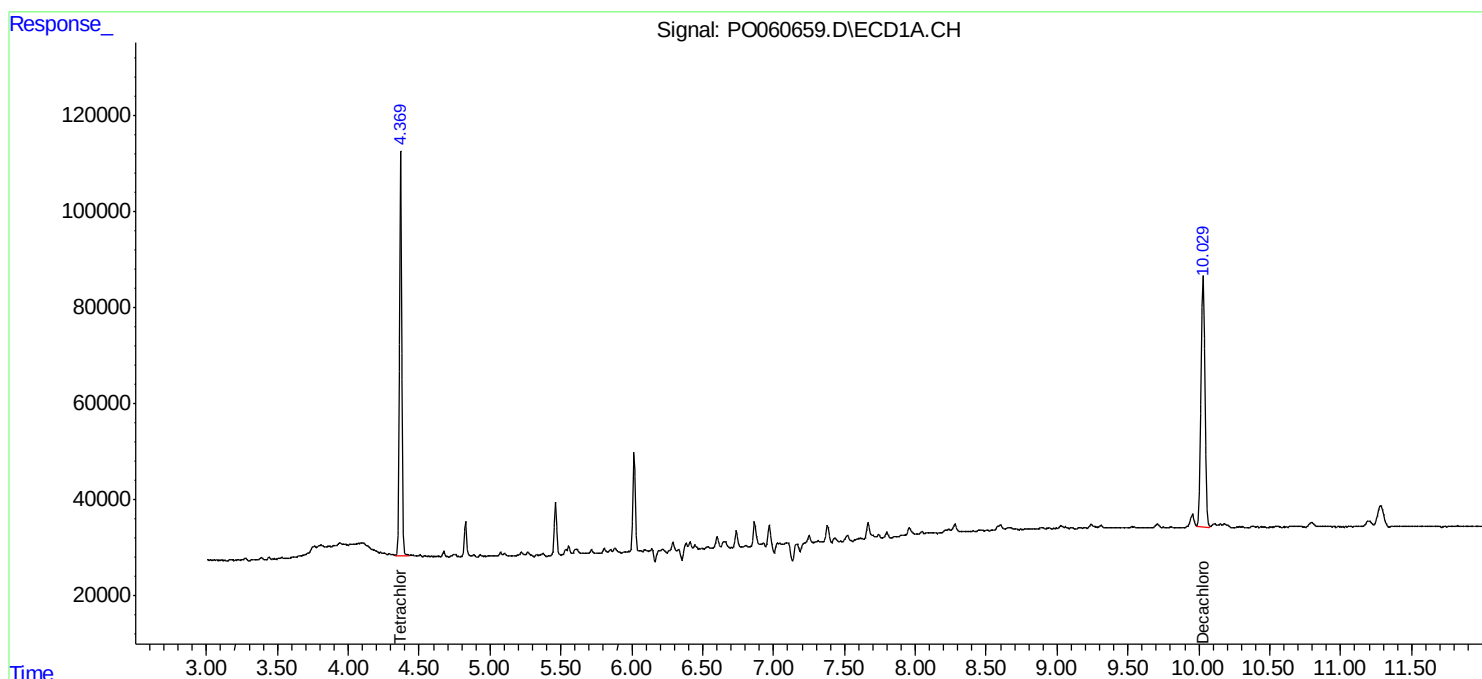

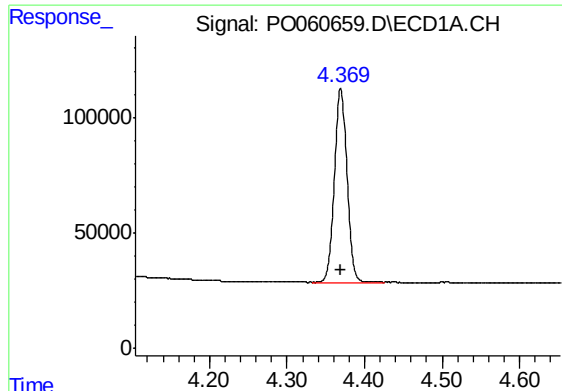


#1 Tetrachloro-m-xylene

R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 924892
Conc: 22.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT5124


Manual Integrations
APPROVED

Ankita
9/12/2019 12:03:47 PM

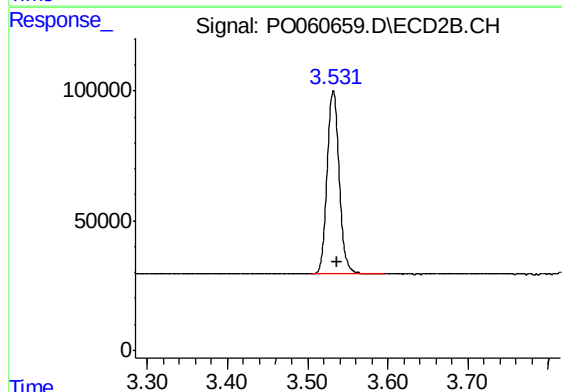


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: -0.004 min
Response: 739214
Conc: 24.07 ng/ml

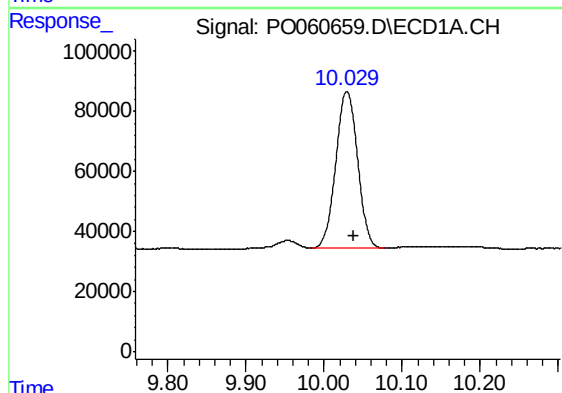

#2 Decachlorobiphenyl

R.T.: 10.029 min
Delta R.T.: -0.008 min
Response: 1025491
Conc: 19.44 ng/ml m

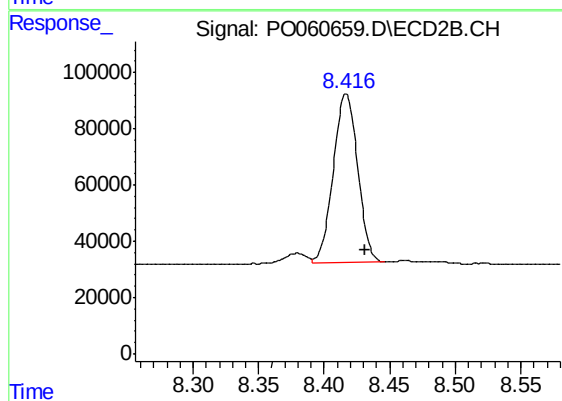

#2 Decachlorobiphenyl

R.T.: 8.416 min
Delta R.T.: -0.015 min
Response: 777393
Conc: 21.00 ng/ml m