

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091119\
Data File : P0060666.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2019 14:42
Operator : SM/AJ
Sample : K4819-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2-S(1-4)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 00:58:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.371	3.532	869372	712259	20.953	23.190
2)	SA Decachlor...	10.031	8.417	823578	614491	15.613	16.600

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091119\
Data File : P0060666.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2019 14:42
Operator : SM/AJ
Sample : K4819-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2-S(1-4)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 00:58:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

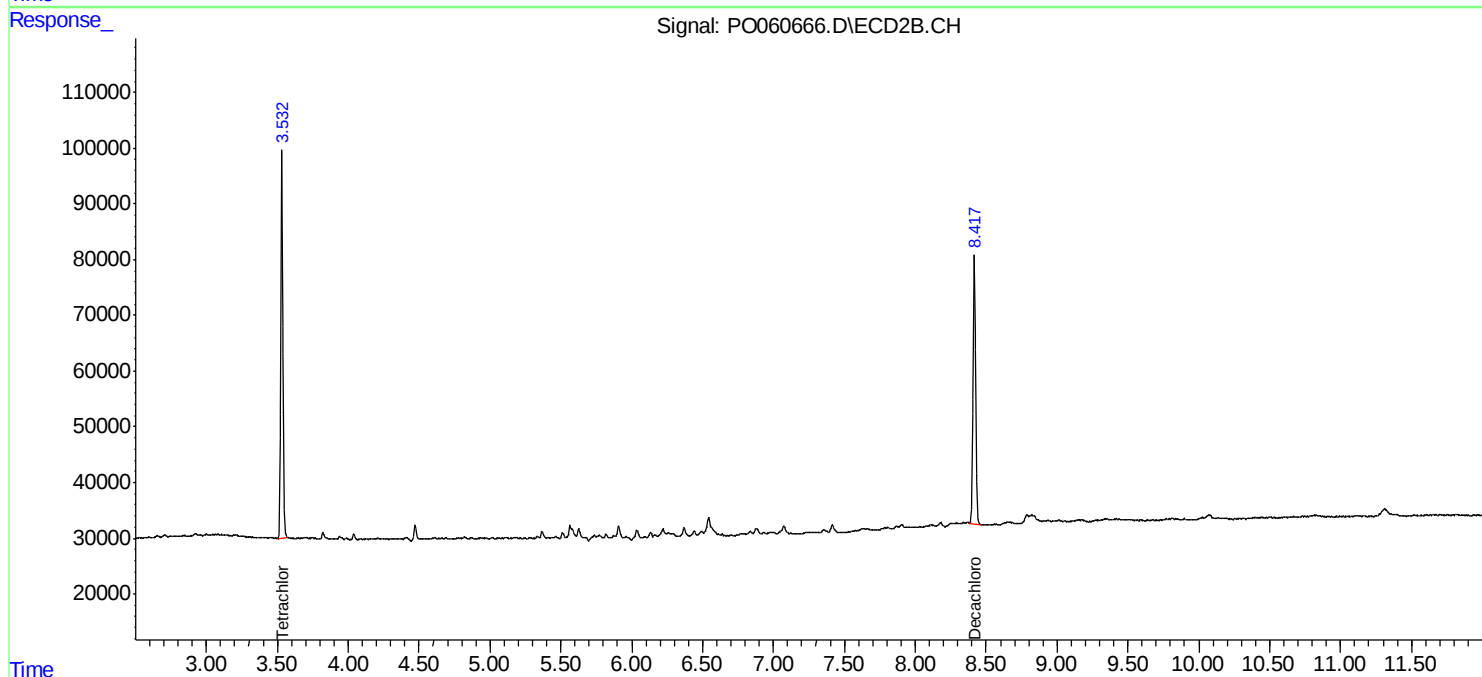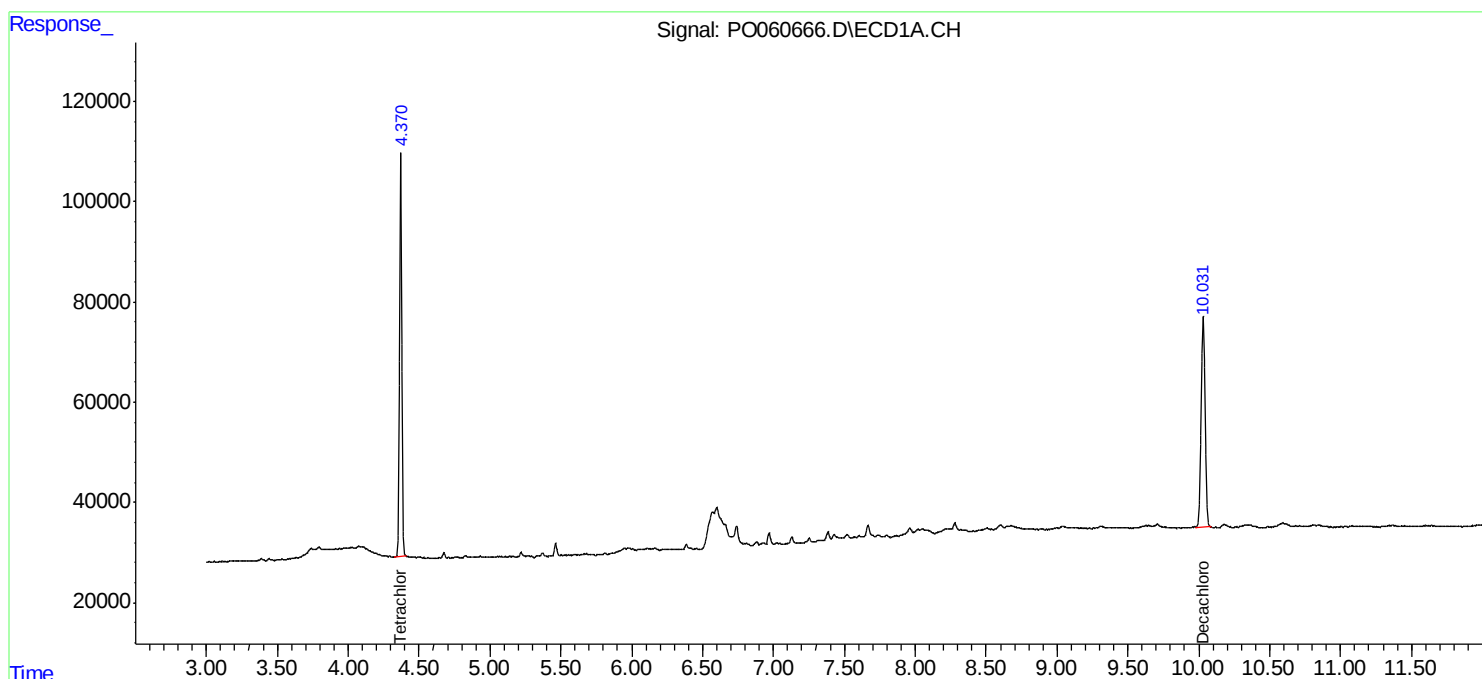


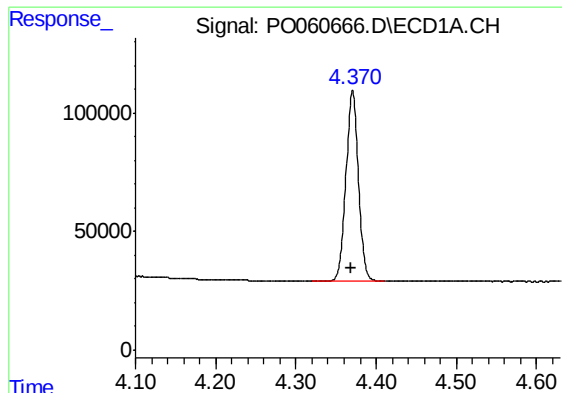

#1 Tetrachloro-m-xylene


R.T.: 4.371 min
Delta R.T.: 0.002 min
Response: 869372
Conc: 20.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2-S(1-4)

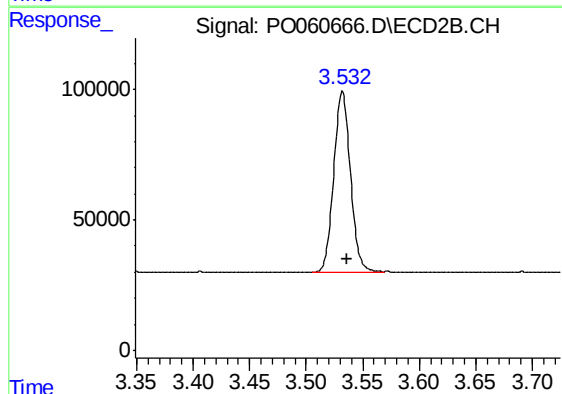


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: -0.004 min
Response: 712259
Conc: 23.19 ng/ml

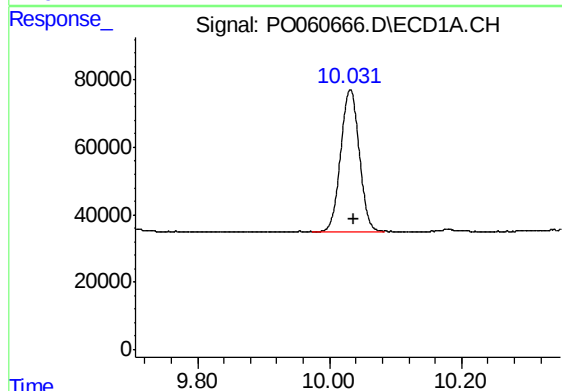

#2 Decachlorobiphenyl

R.T.: 10.031 min
Delta R.T.: -0.006 min
Response: 823578
Conc: 15.61 ng/ml

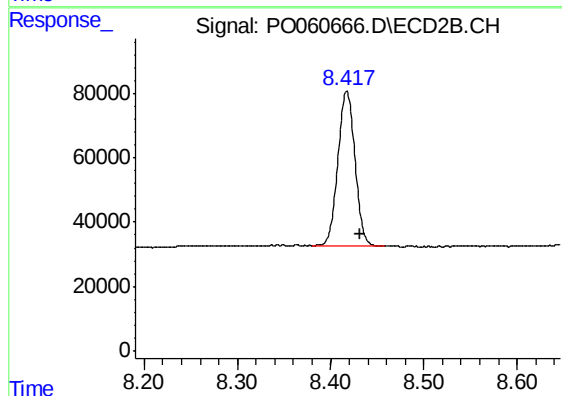

#2 Decachlorobiphenyl

R.T.: 8.417 min
Delta R.T.: -0.014 min
Response: 614491
Conc: 16.60 ng/ml