

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091120\
 Data File : P0071284.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Sep 2020 13:13
 Operator : DD\AJ
 Sample : L3943-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 357

Manual Integrations
 APPROVED

Ankita
 9/14/2020 11:02:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 17:09:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.346	3.530	1700334	909089	23.993	23.285
2) SA Decachlor...	9.959	8.709	1951596	1158149	20.928	21.025m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091120\
Data File : P0071284.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2020 13:13
Operator : DD\AJ
Sample : L3943-02
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
357


Manual Integrations
APPROVED

Ankita
9/14/2020 11:02:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 17:09:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

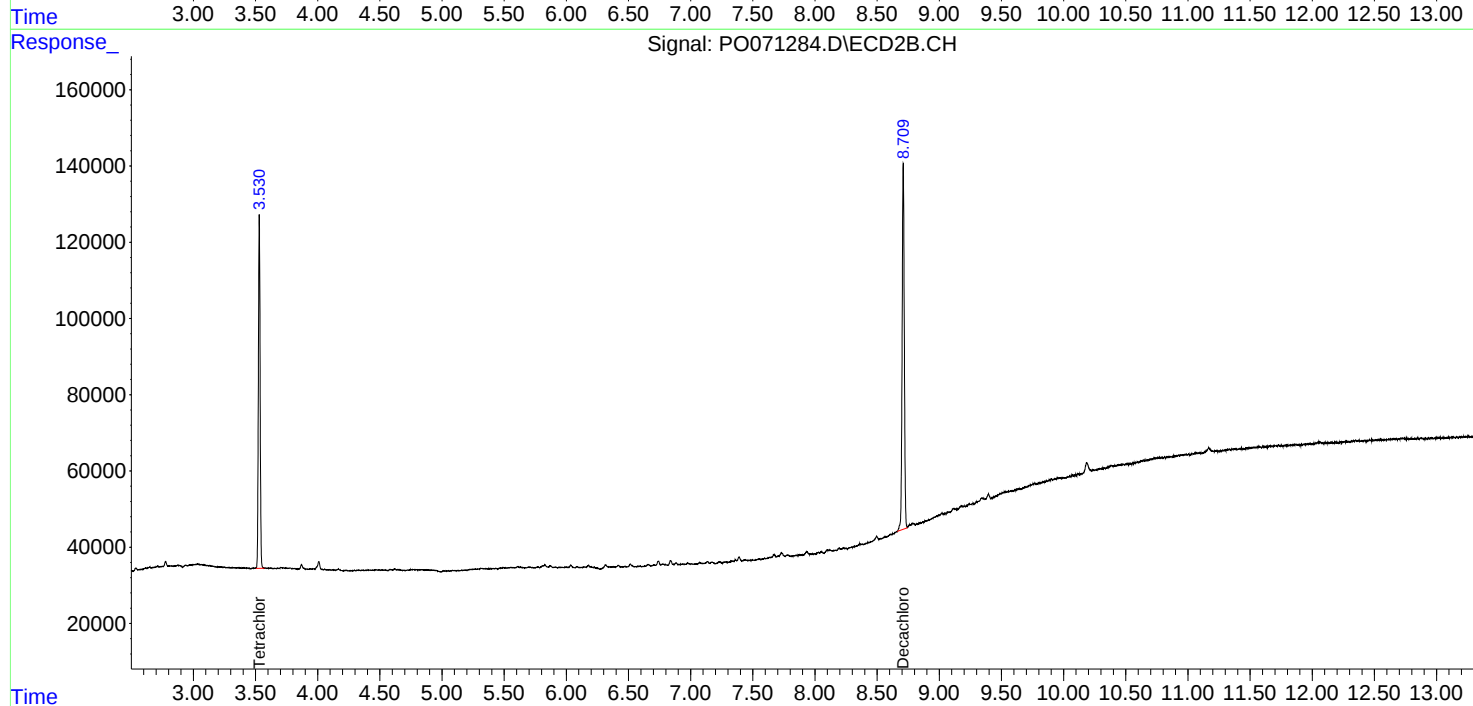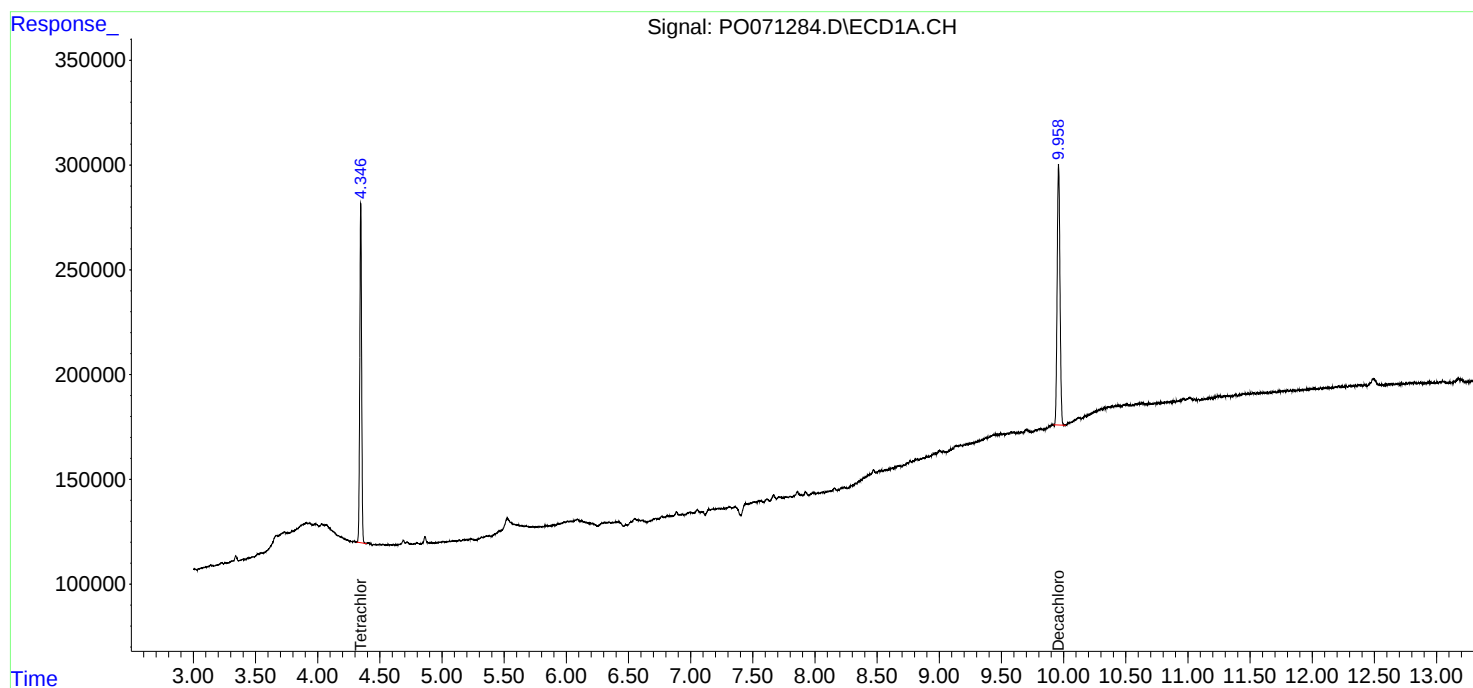

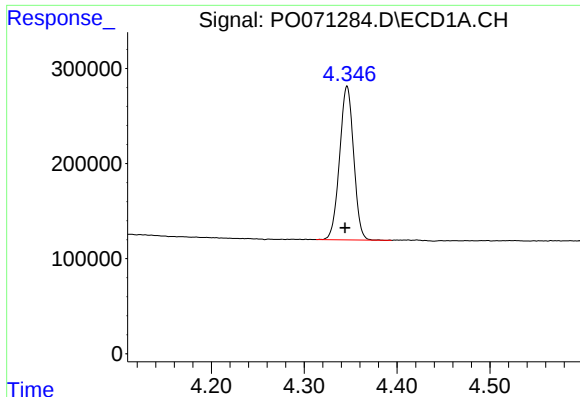


#1 Tetrachloro-m-xylene

R.T.: 4.346 min
Delta R.T.: 0.002 min
Response: 1700334
Conc: 23.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
357


Manual Integrations
APPROVED

Ankita
9/14/2020 11:02:06 AM

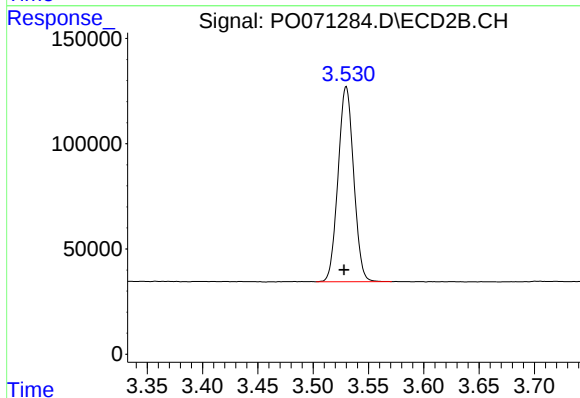


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: 0.002 min
Response: 909089
Conc: 23.29 ng/ml

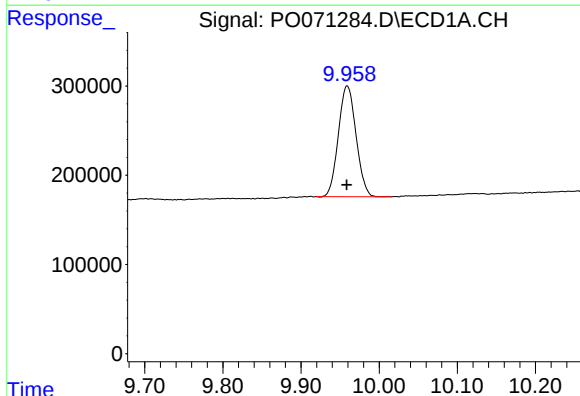

#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: 0.000 min
Response: 1951596
Conc: 20.93 ng/ml

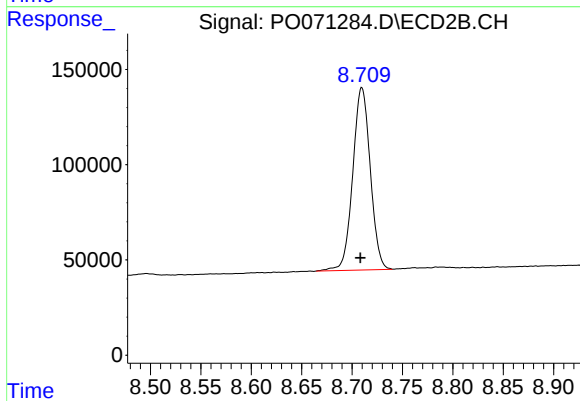

#2 Decachlorobiphenyl

R.T.: 8.709 min
Delta R.T.: 0.001 min
Response: 1158149
Conc: 21.03 ng/ml m