

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091120\
 Data File : P0071287.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Sep 2020 14:05
 Operator : DD\AJ
 Sample : L3952-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 16745

Manual Integrations
 APPROVED

Ankita
 9/14/2020 11:02:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 17:10:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.357	3.546f	1884620	811459	26.594m	20.785m
2) SA Decachlor...	9.959	8.710	2075064	1091359	22.252m	19.813m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091120\
Data File : P0071287.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2020 14:05
Operator : DD\AJ
Sample : L3952-11
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
16745


Manual Integrations
APPROVED

Ankita
9/14/2020 11:02:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 17:10:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

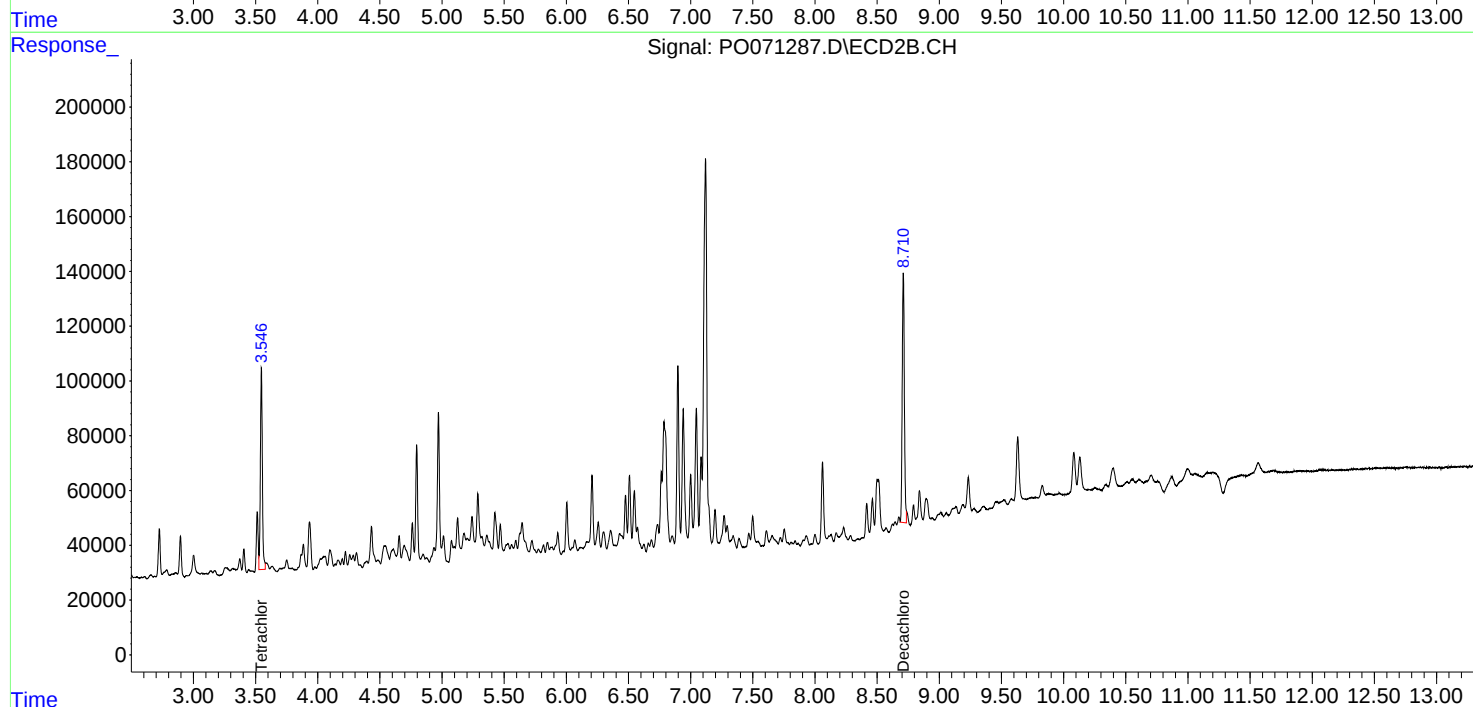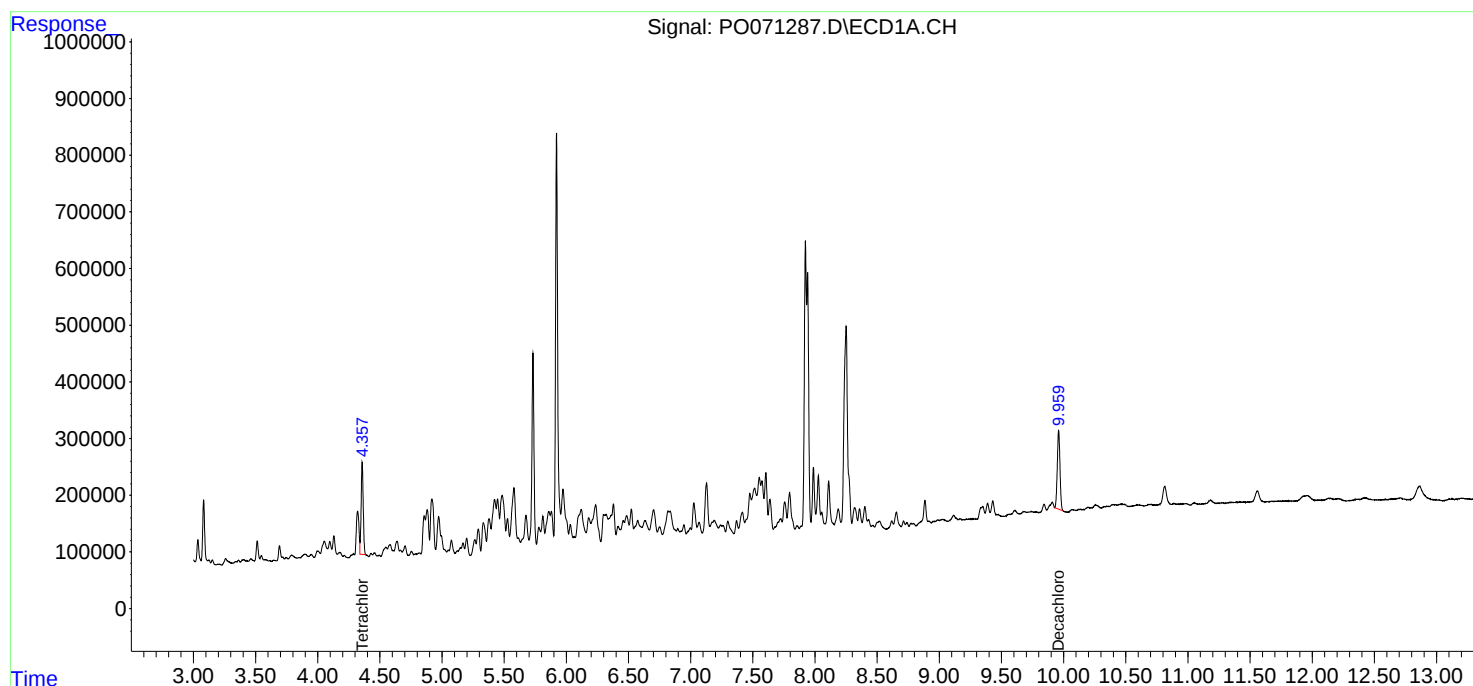

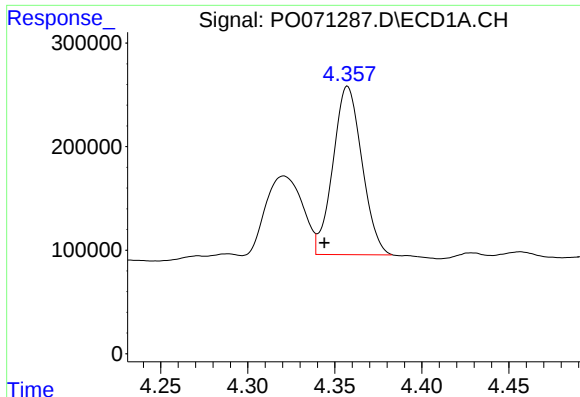


#1 Tetrachloro-m-xylene

R.T.: 4.357 min
Delta R.T.: 0.013 min
Response: 1884620
Conc: 26.59 ng/ml m

Instrument :
ECD_O
ClientSampleId :
16745


Manual Integrations
APPROVED

Ankita
9/14/2020 11:02:13 AM

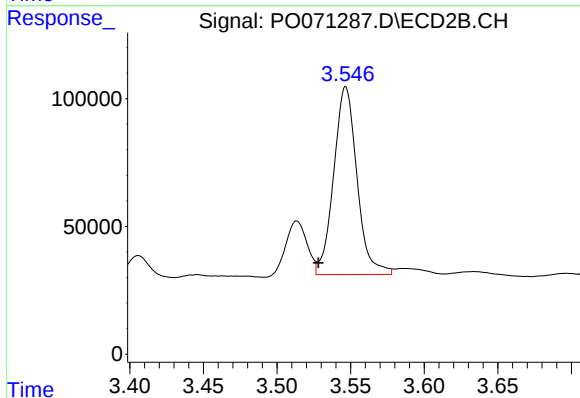


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: 0.018 min
Response: 811459
Conc: 20.78 ng/ml m

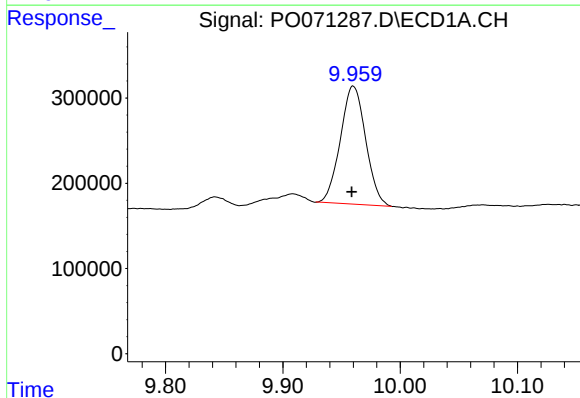

#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: 0.000 min
Response: 2075064
Conc: 22.25 ng/ml m

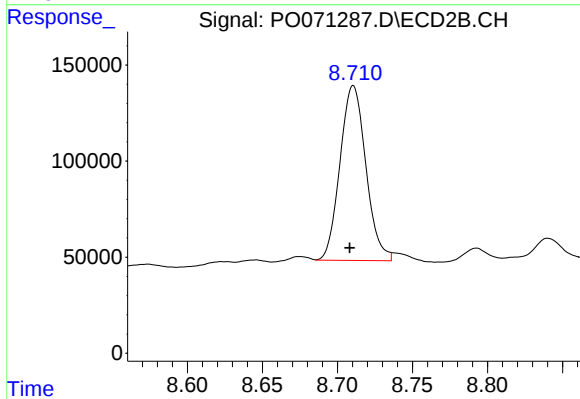

#2 Decachlorobiphenyl

R.T.: 8.710 min
Delta R.T.: 0.002 min
Response: 1091359
Conc: 19.81 ng/ml m