

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091120\
 Data File : P0071290.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Sep 2020 14:56
 Operator : DD\AJ
 Sample : L3975-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BSY-SB-03-0-17

Manual Integrations
 APPROVED

Ankita
 9/14/2020 11:02:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 17:11:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.528	1933426	1051251	27.283m	26.927
2) SA Decachlor...	9.957	8.706	1852406	1041349	19.864m	18.905m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091120\
Data File : PO071290.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2020 14:56
Operator : DD\AJ
Sample : L3975-04
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BSY-SB-03-0-17


Manual Integrations
APPROVED

Ankita
9/14/2020 11:02:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 17:11:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

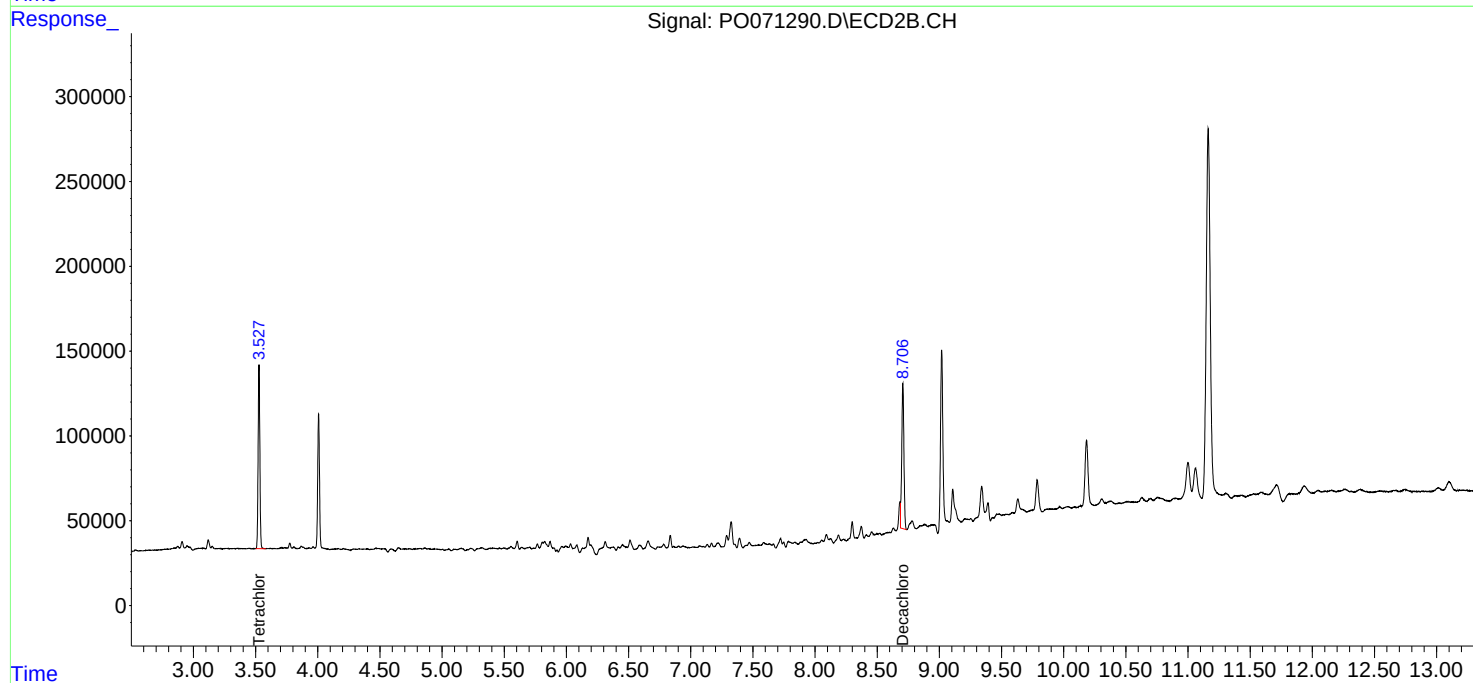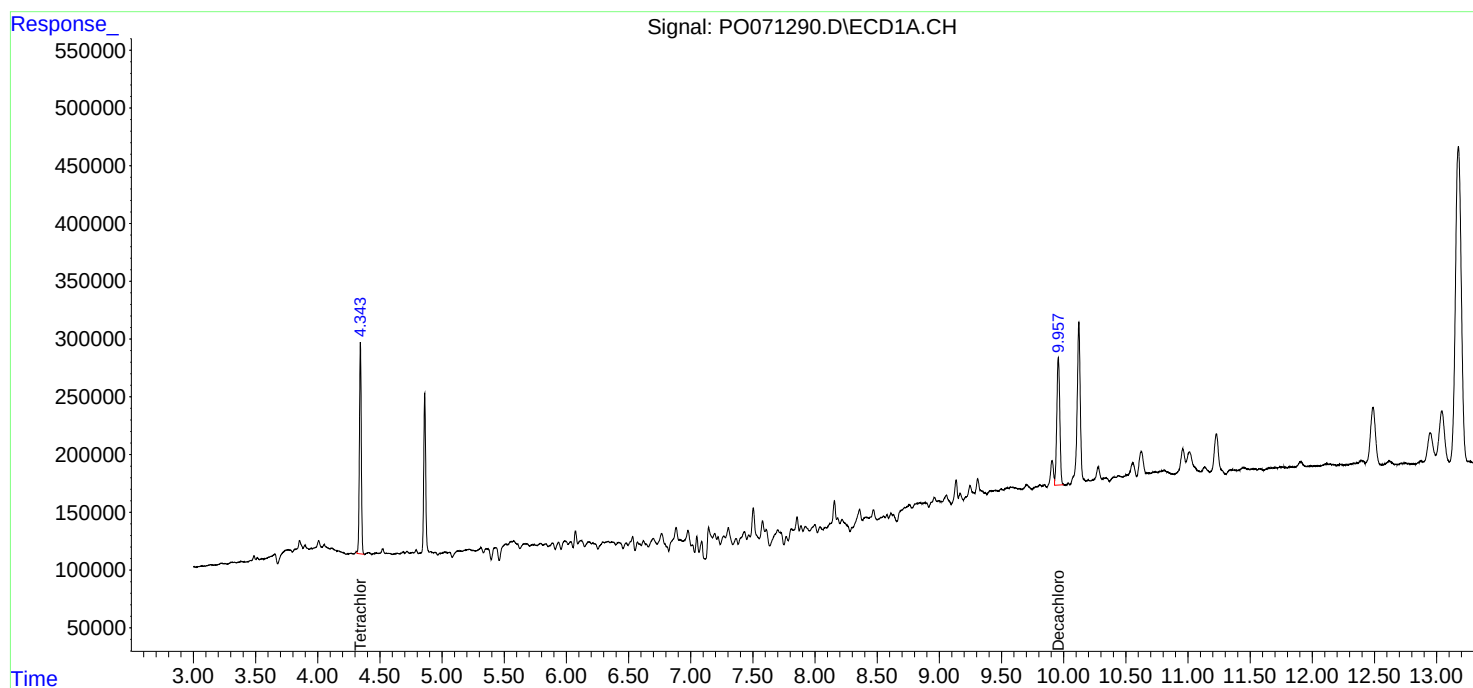

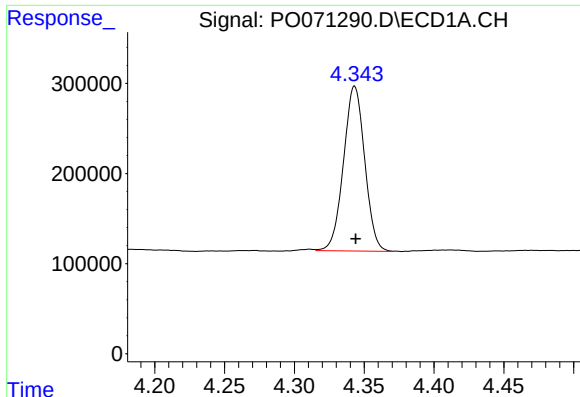


#1 Tetrachloro-m-xylene

R.T.: 4.343 min
Delta R.T.: -0.001 min
Response: 1933426
Conc: 27.28 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BSY-SB-03-0-17


Manual Integrations
APPROVED

Ankita
9/14/2020 11:02:17 AM

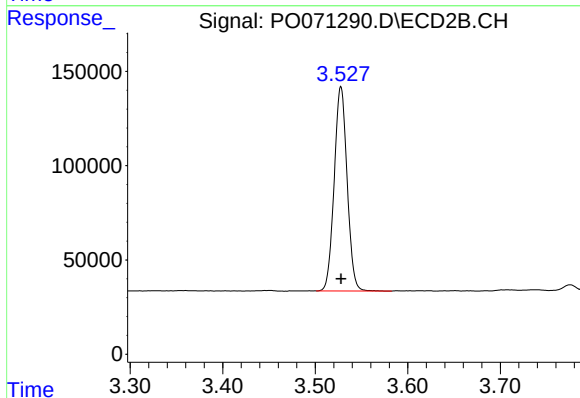


#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 1051251
Conc: 26.93 ng/ml

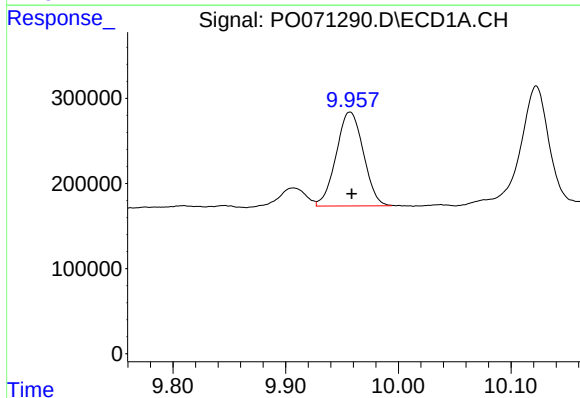

#2 Decachlorobiphenyl

R.T.: 9.957 min
Delta R.T.: -0.002 min
Response: 1852406
Conc: 19.86 ng/ml m

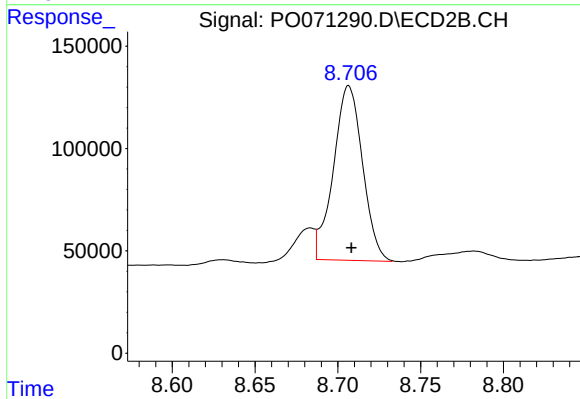

#2 Decachlorobiphenyl

R.T.: 8.706 min
Delta R.T.: -0.002 min
Response: 1041349
Conc: 18.90 ng/ml m