

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091123\
 Data File : P0097903.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2023 20:22
 Operator : YP/AJ
 Sample : 04369-02 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JEB800V-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/12/2023
 Supervised By :Ankita Jodhani 09/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 01:14:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 07 02:56:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.441	3.623	5200255	1700264	1.305m	1.775 #
2) SA Decachlor...	10.288	8.657	2924105	1481654	1.565m	1.734m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091123\
Data File : PO097903.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2023 20:22
Operator : YP/AJ
Sample : 04369-02 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
JEB800V-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/12/2023
Supervised By :Ankita Jodhani 09/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 01:14:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 07 02:56:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

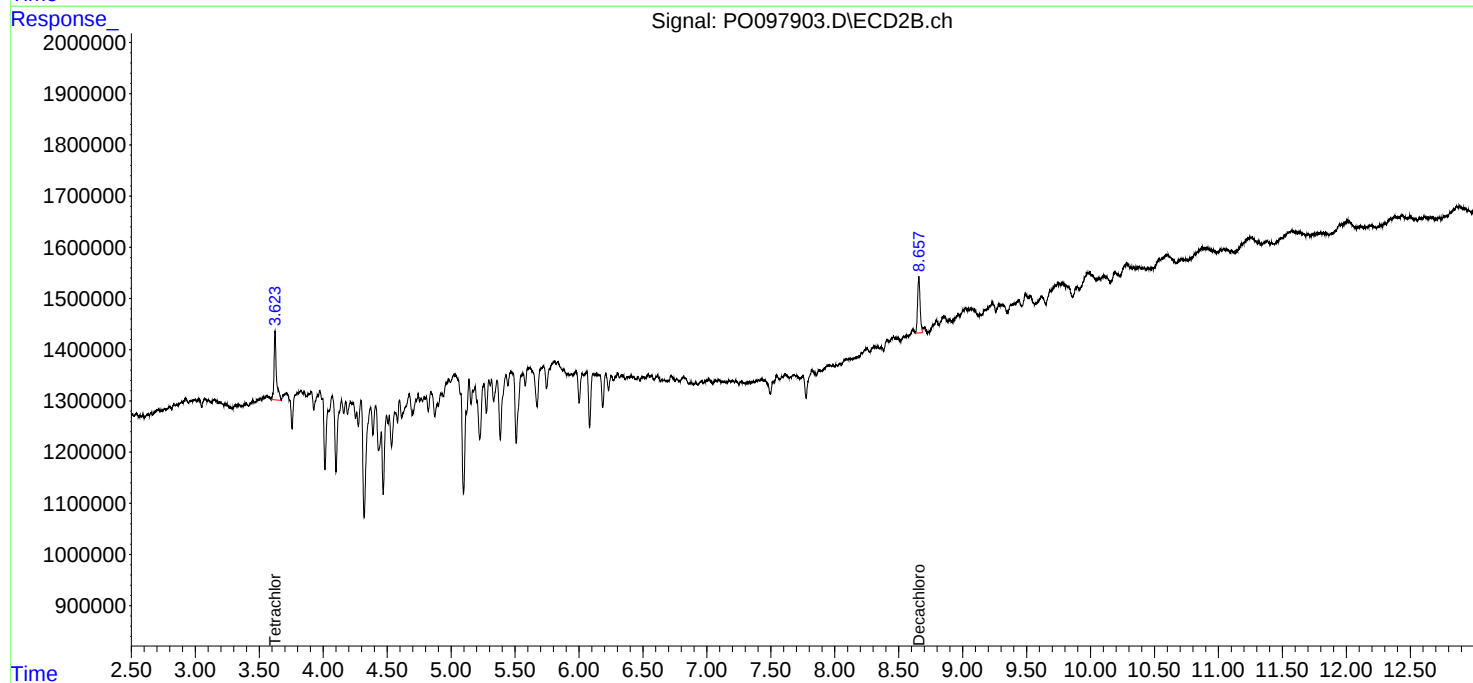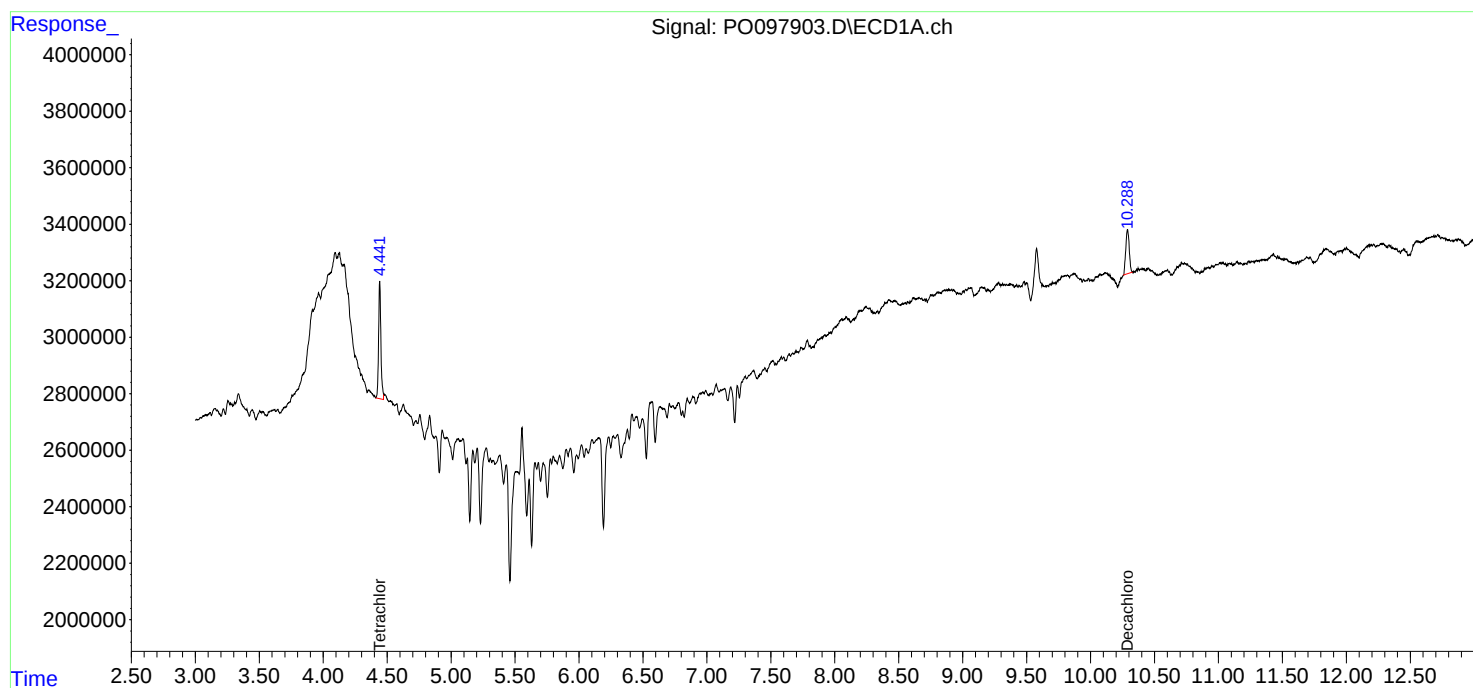

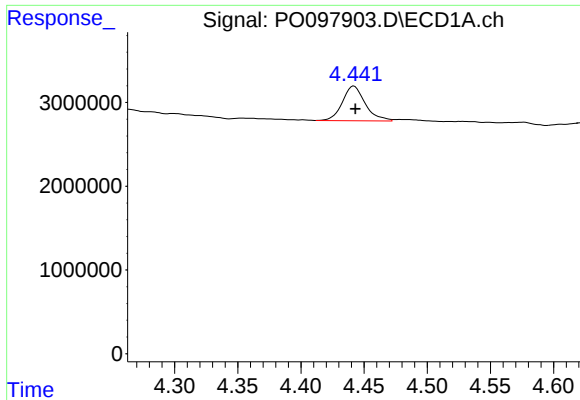


#1 Tetrachloro-m-xylene

R.T.: 4.441 min
Delta R.T.: -0.002 min
Response: 5200255
Conc: 1.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
JEB800V-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/12/2023
Supervised By :Ankita Jodhani 09/12/2023

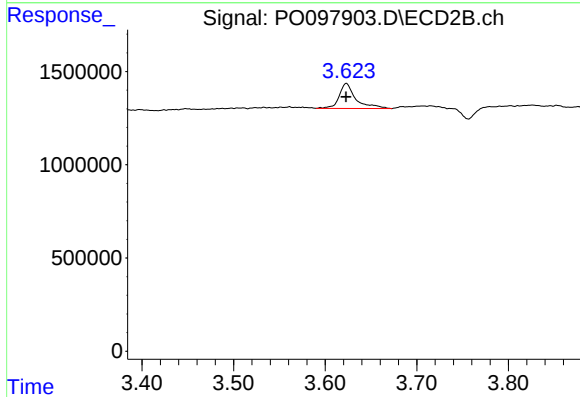


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: 0.000 min
Response: 1700264
Conc: 1.78 ng/ml

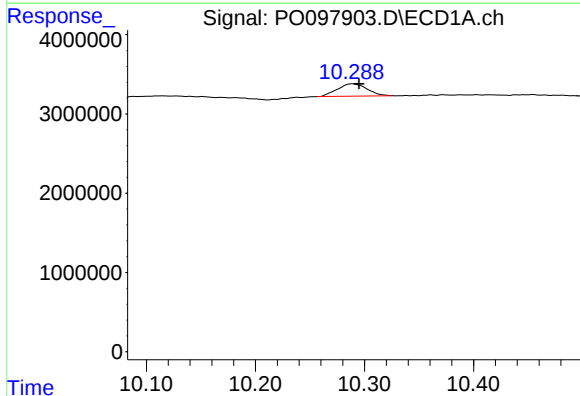

#2 Decachlorobiphenyl

R.T.: 10.288 min
Delta R.T.: -0.007 min
Response: 2924105
Conc: 1.56 ng/ml m

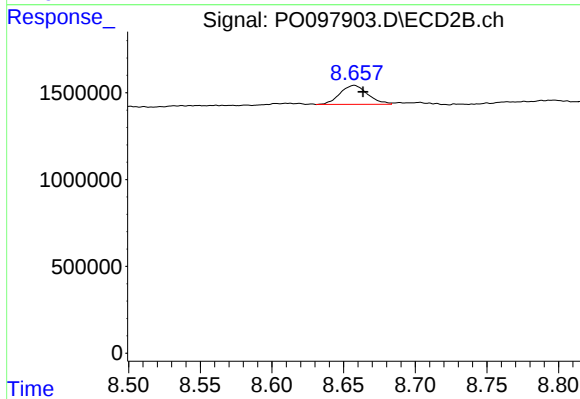

#2 Decachlorobiphenyl

R.T.: 8.657 min
Delta R.T.: -0.006 min
Response: 1481654
Conc: 1.73 ng/ml m