

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091123\
 Data File : P0097924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2023 03:15
 Operator : YP/AJ
 Sample : 04372-02 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KQAO72G-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/12/2023
 Supervised By :Ankita Jodhani 09/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 03:38:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 07 02:56:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.441	3.622	5281907	1538738	1.326m	1.607
2) SA Decachlor...	10.288	8.655	3546761	1529208	1.898	1.790m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091123\
Data File : PO097924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2023 03:15
Operator : YP/AJ
Sample : 04372-02 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KQAO72G-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/12/2023
Supervised By :Ankita Jodhani 09/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 03:38:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 07 02:56:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

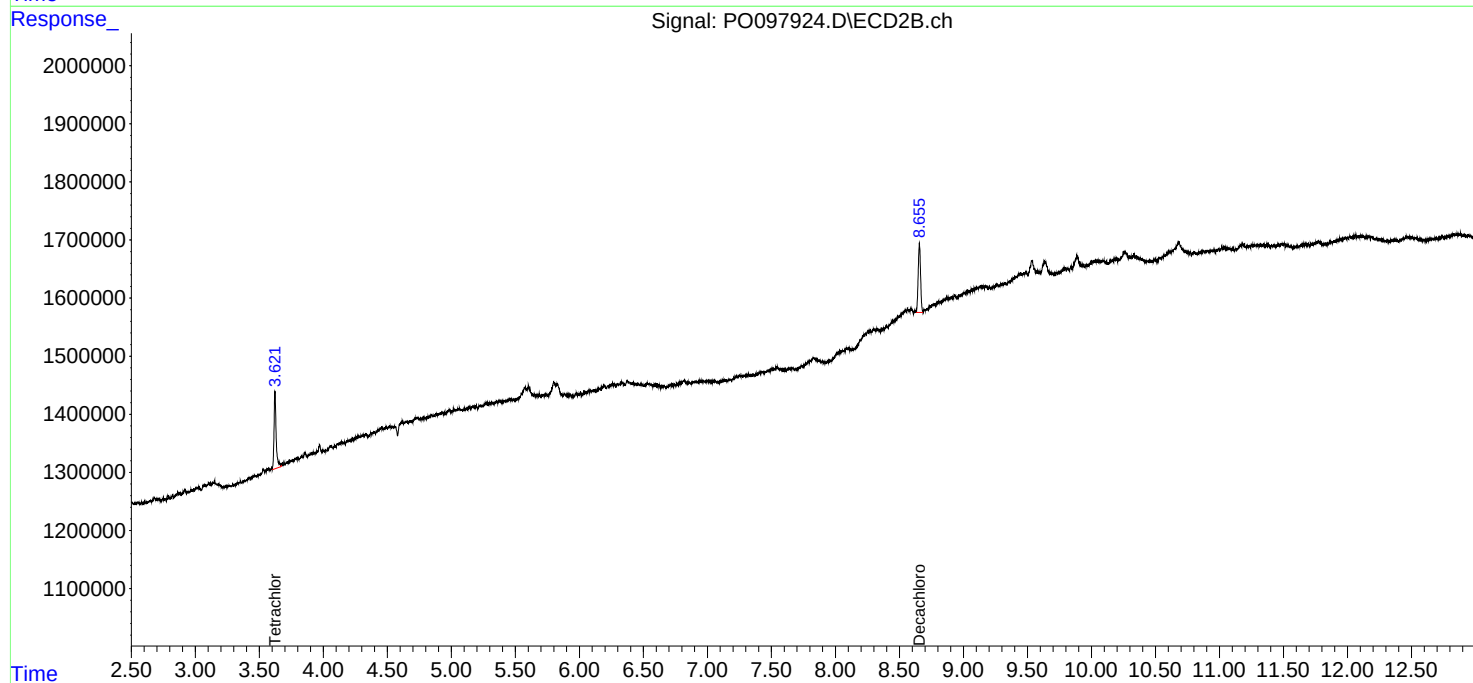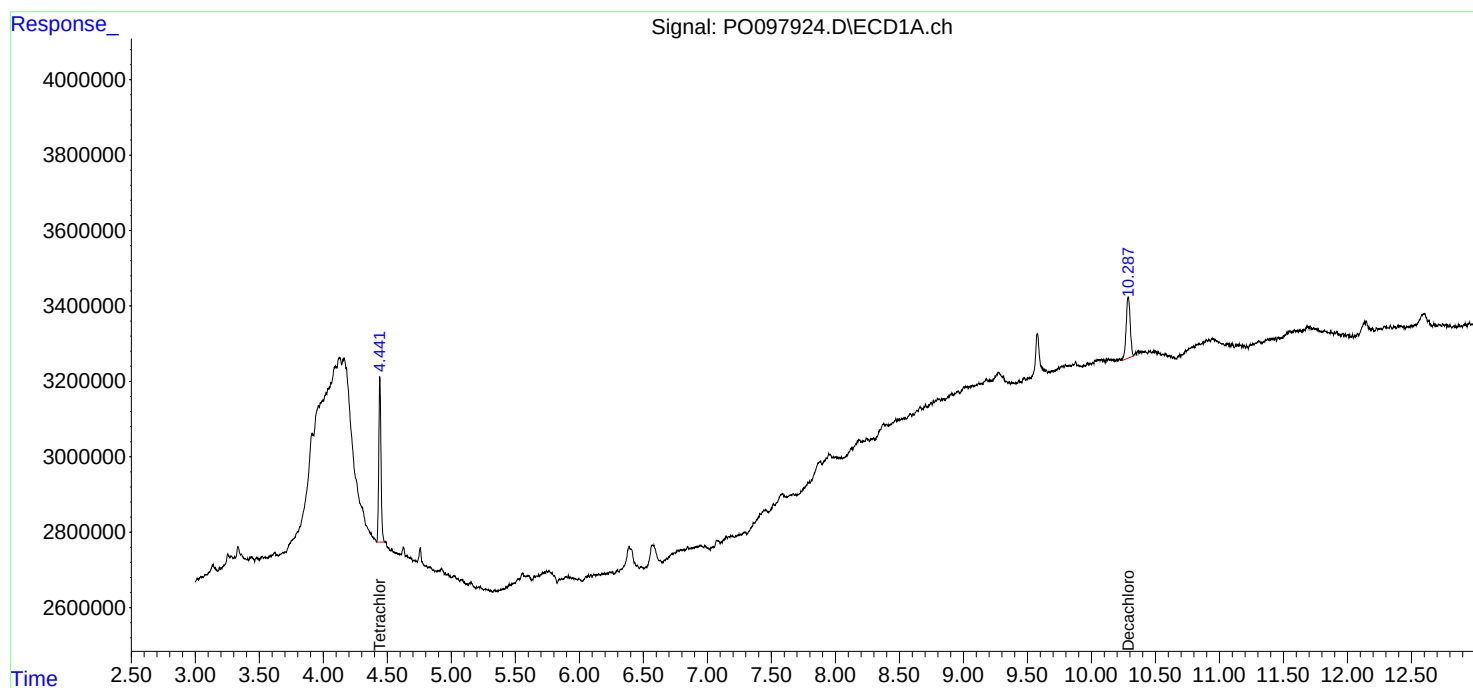

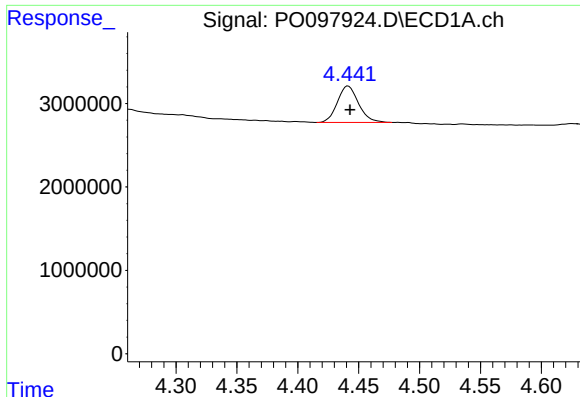


#1 Tetrachloro-m-xylene

R.T.: 4.441 min
Delta R.T.: -0.002 min
Response: 5281907
Conc: 1.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
KQA072G-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/12/2023
Supervised By :Ankita Jodhani 09/12/2023

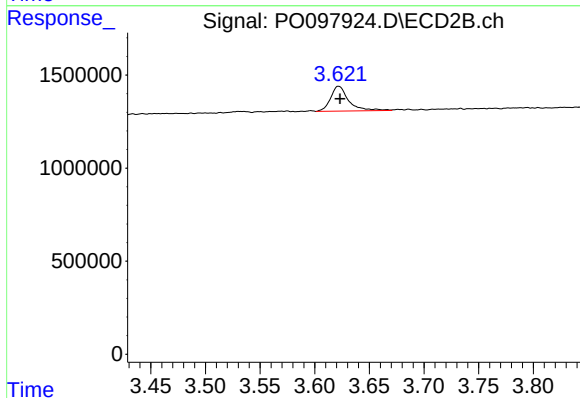


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.001 min
Response: 1538738
Conc: 1.61 ng/ml

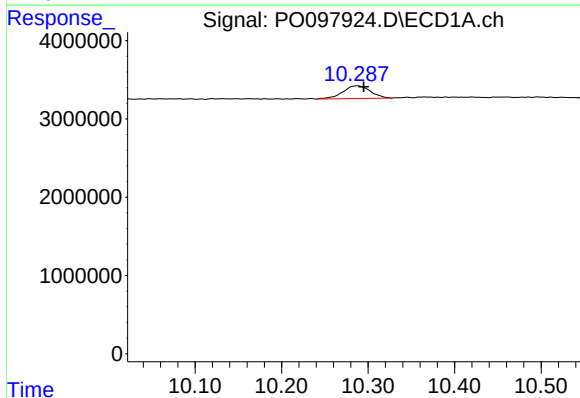

#2 Decachlorobiphenyl

R.T.: 10.288 min
Delta R.T.: -0.007 min
Response: 3546761
Conc: 1.90 ng/ml

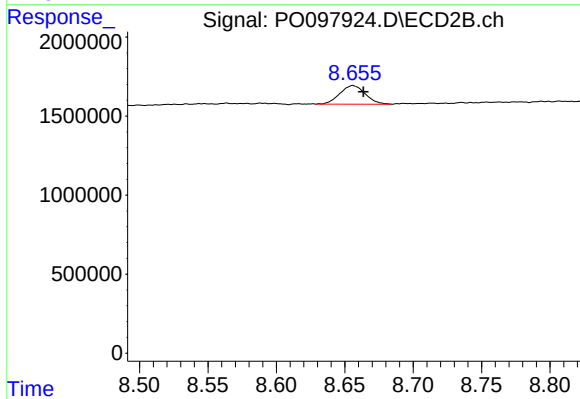

#2 Decachlorobiphenyl

R.T.: 8.655 min
Delta R.T.: -0.008 min
Response: 1529208
Conc: 1.79 ng/ml m