

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0091123\
 Data File : P0097931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2023 06:10
 Operator : YP/AJ
 Sample : 04372-04 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 KQAO72G-2-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/12/2023
 Supervised By :Ankita Jodhani 09/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 06:54:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0090623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 07 02:56:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.440	3.621	5178120	1388931	1.300m	1.450
2) SA Decachlor...	10.283	8.654	3760299	1691909	2.013m	1.980

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091123\
Data File : PO097931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2023 06:10
Operator : YP/AJ
Sample : 04372-04 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KQA072G-2-2


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 09/12/2023
Supervised By : Ankita Jodhani 09/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 06:54:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 07 02:56:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

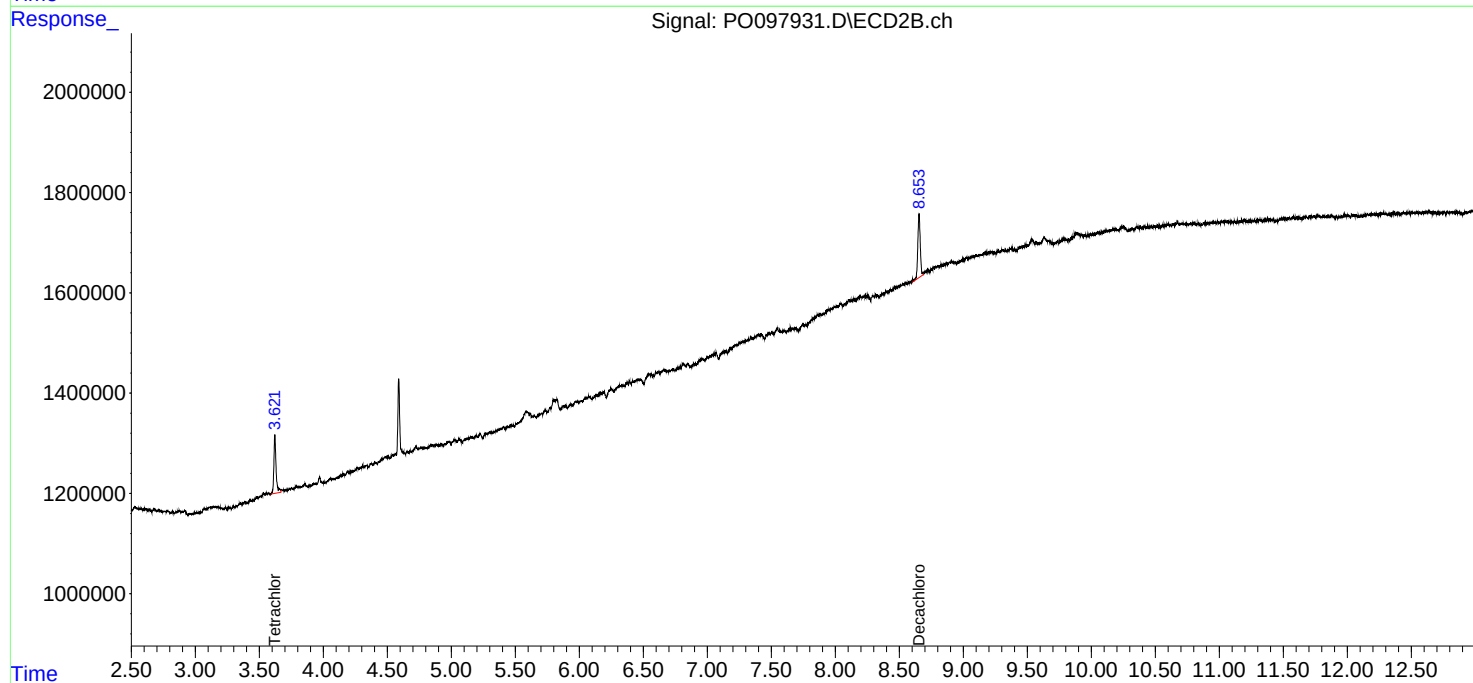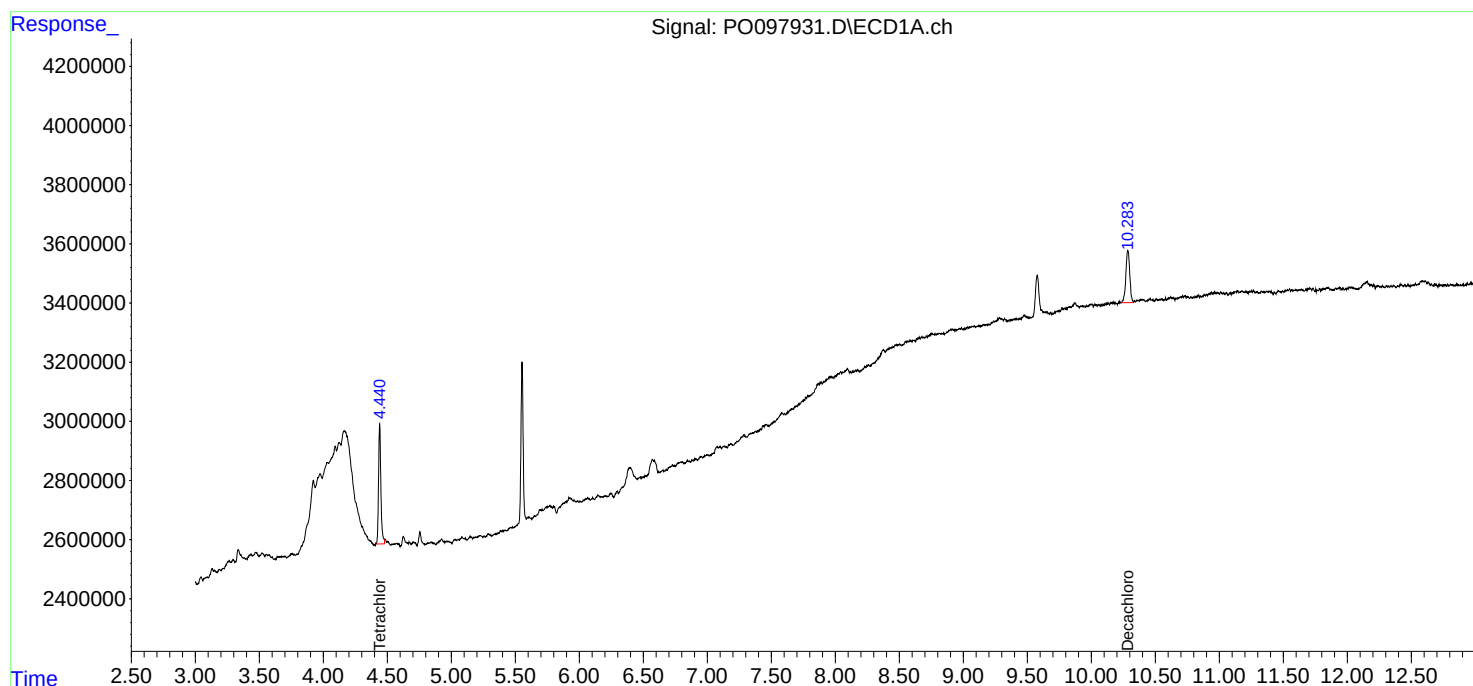

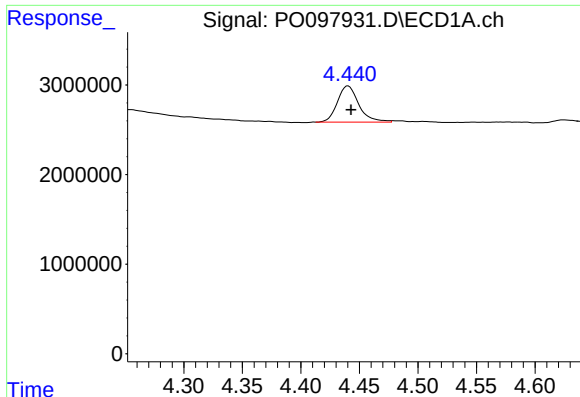


#1 Tetrachloro-m-xylene

R.T.: 4.440 min
Delta R.T.: -0.003 min
Response: 5178120
Conc: 1.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
KQA072G-2-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/12/2023
Supervised By :Ankita Jodhani 09/12/2023

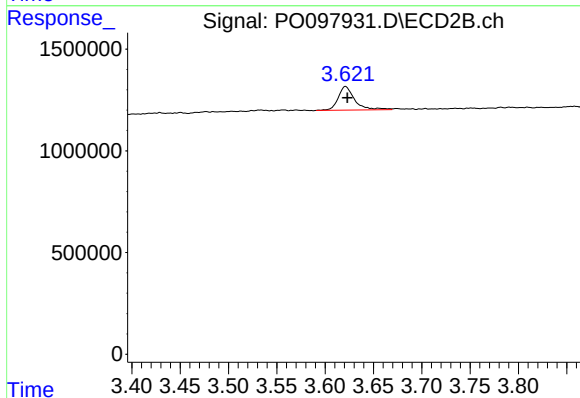


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.002 min
Response: 1388931
Conc: 1.45 ng/ml

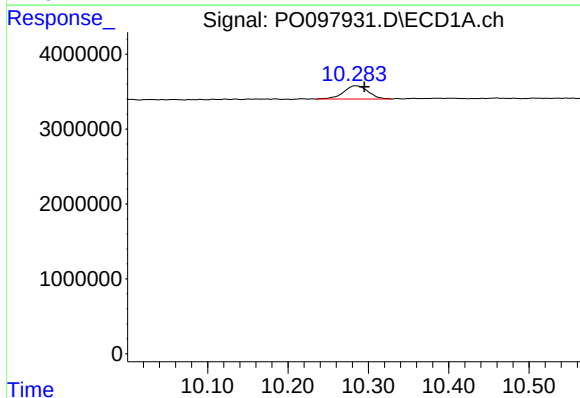

#2 Decachlorobiphenyl

R.T.: 10.283 min
Delta R.T.: -0.012 min
Response: 3760299
Conc: 2.01 ng/ml m

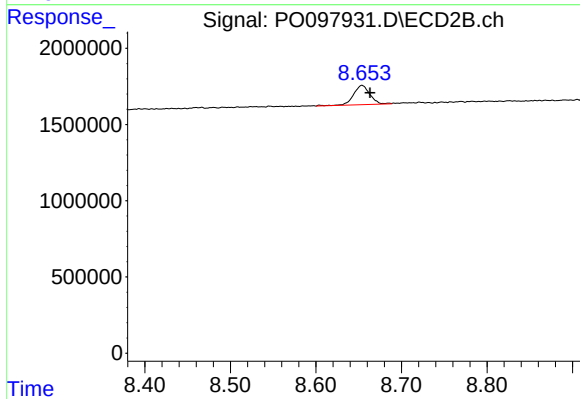

#2 Decachlorobiphenyl

R.T.: 8.654 min
Delta R.T.: -0.010 min
Response: 1691909
Conc: 1.98 ng/ml