

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091125\
 Data File : P0113652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 11:17
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1232 40PPB WATER MDL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 02:09:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.658	3.650	186.2E6	109.5E6	22.744	21.629
2)	SA Decachlor...	8.670	8.614	162.1E6	46039121	23.385	24.297
Target Compounds							
3)	L1 AR-1016-1	4.742	4.722	5113387	3743337	19.152	21.946
4)	L1 AR-1016-2	4.759	4.739	7781558	6571732	19.385	25.506 #
5)	L1 AR-1016-3	4.817	4.913	6431041	14676567	25.218	105.122 #
6)	L1 AR-1016-4	4.937	4.963	15467829	7819102	70.931	67.002
7)	L1 AR-1016-5	5.195	5.168	33323403	20979673	150.357	147.195
8)	L2 AR-1221-1	3.872	3.858	2150139	1719789	22.978	27.246
9)	L2 AR-1221-2	3.958	3.946	3615667	3571703	53.525	76.526 #
10)	L2 AR-1221-3	4.030	4.017	6248253	4779826	28.228	32.193
11)	L3 AR-1232-1	4.030	4.017	6248253	4779826	34.804	39.525
12)	L3 AR-1232-2	4.522	4.739	3495206	6571732	32.388	53.845 #
13)	L3 AR-1232-3	4.759	4.913	7781558	14676567	39.421	221.848 #
14)	L3 AR-1232-4	4.937	4.998	15467829	13417609	157.364	223.894 #
15)	L3 AR-1232-5	5.020f	5.168	46267768	20979673	703.348	310.276 #
16)	L4 AR-1242-1	4.742	4.722	5113387	3743337	22.239	25.905
17)	L4 AR-1242-2	4.759	4.739	7781558	6571732	22.645	30.297 #
18)	L4 AR-1242-3	4.817	4.913	6431041	14676567	28.984	125.479 #
19)	L4 AR-1242-4	4.937	4.998	15467829	13417609	89.171	114.059 #
20)	L4 AR-1242-5	5.616	5.518	19973089	12447109	99.784	83.463
21)	L5 AR-1248-1	4.742	4.722	5113387	3743337	29.309	33.569
22)	L5 AR-1248-2	5.020	4.963	46267768	7819102	191.295	48.657 #
23)	L5 AR-1248-3	5.195	4.998	33323403	13417609	104.507	79.085
24)	L5 AR-1248-4	5.546	5.168	38434650	20979673	76.930	105.309 #
25)	L5 AR-1248-5	5.616	5.541	19973089	33623657	58.488	158.381 #
26)	L6 AR-1254-1	5.546	5.518	38434650	12447109	71.178	39.470 #
27)	L6 AR-1254-2	5.702	5.667	62234821	18918612	126.121	67.485 #
28)	L6 AR-1254-3	6.096	6.062	4247206	8137421	5.748	19.518 #
29)	L6 AR-1254-4	6.324	6.306	4750629	2229430	8.529	8.112
30)	L6 AR-1254-5	6.751	6.724	4147146	1130649	5.916	3.163 #
31)	L7 AR-1260-1	6.228	6.208	1404973	14260213	3.150	55.907 #
32)	L7 AR-1260-2	6.452	6.414	1978064	791892	2.880	2.291
33)	L7 AR-1260-3	6.786	6.571	1081494	4510929	1.751	15.166 #
34)	L7 AR-1260-4	7.051	7.018	4124566	220138	9.209	1.062 #
35)	L7 AR-1260-5	7.295	7.249	908169	233593	0.750	0.499 #
36)	L8 AR-1262-1	6.786	6.746	1081494	632384	1.181	1.525 #
37)	L8 AR-1262-2	7.295	7.249	908169	233593	0.601	0.451
38)	L8 AR-1262-3	7.582	7.544	100.4E6	43567978	181.125	242.596 #
39)	L8 AR-1262-4	7.582f	7.544f	100.4E6	43567978	102.624	150.286 #
40)	L8 AR-1262-5	8.126	8.096	196274	185573	0.471	1.713 #
41)	L9 AR-1268-1	7.582	7.544	100.4E6	43567978	58.320	85.517 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091125\
Data File : P0113652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 11:17
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1232 40PPB WATER MDL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:09:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.582f	7.544f	100.4E6	43567978	69.304	104.881 #
43)	L9 AR-1268-3	7.853	7.815	356323	22480	0.295	0.069 #
44)	L9 AR-1268-4	8.145	8.096	898457	185573	1.950	1.541
45)	L9 AR-1268-5	8.416	8.384	892678	32324	0.280	0.041 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091125\
Data File : PO113652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 11:17
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1232 40PPB WATER MDL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:09:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

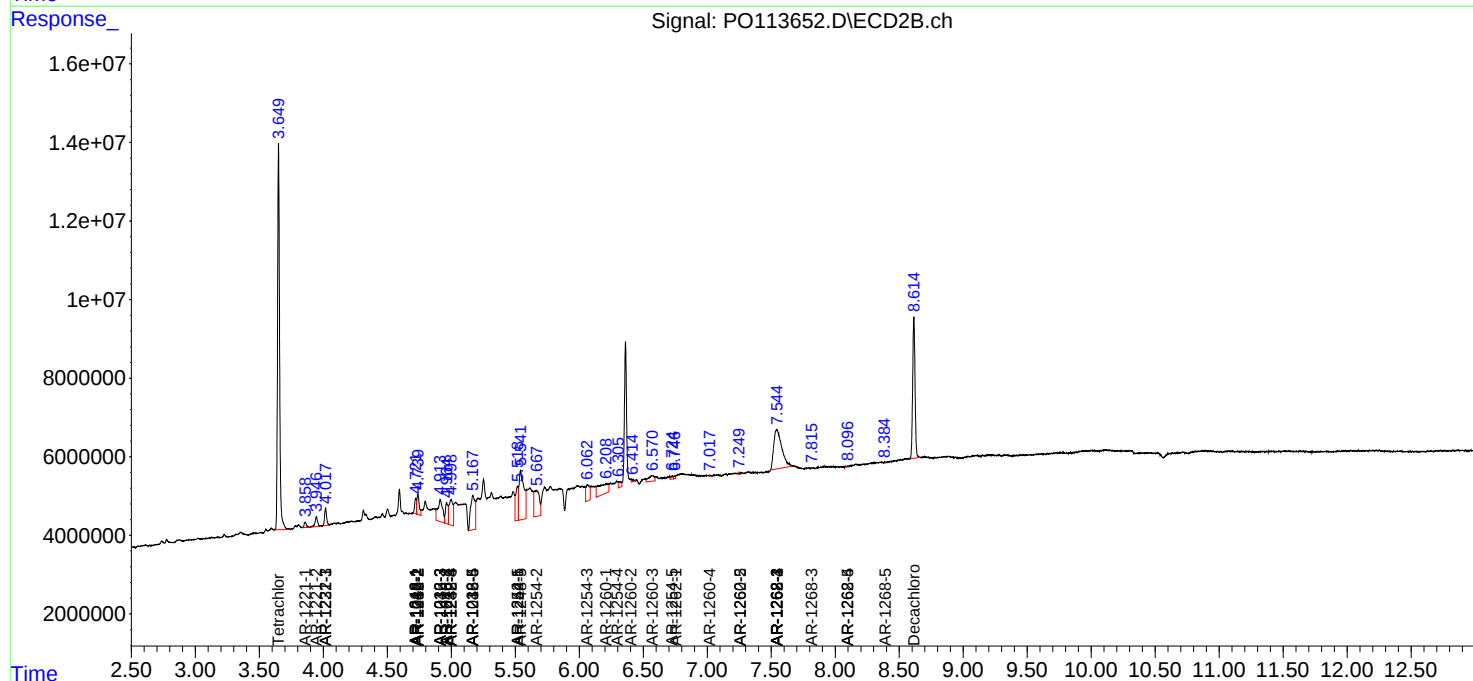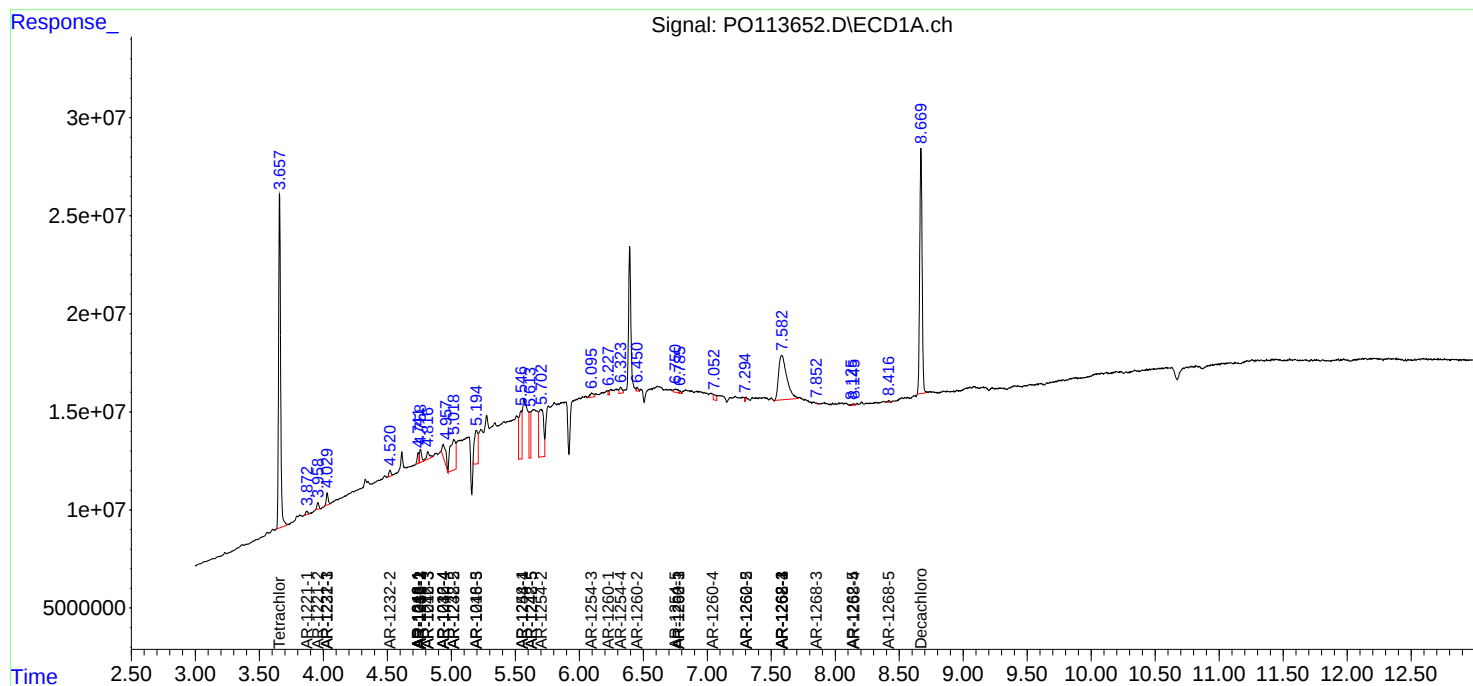


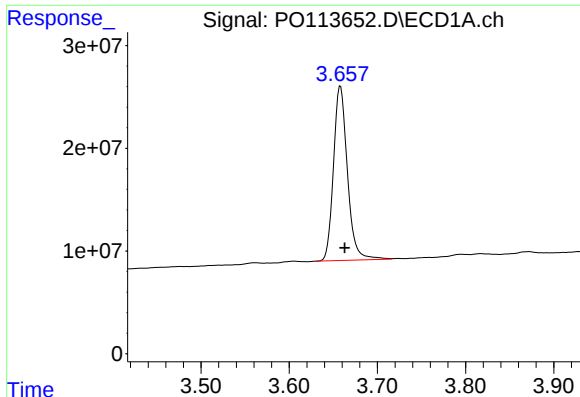

#1 Tetrachloro-m-xylene


R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 186198641
Conc: 22.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

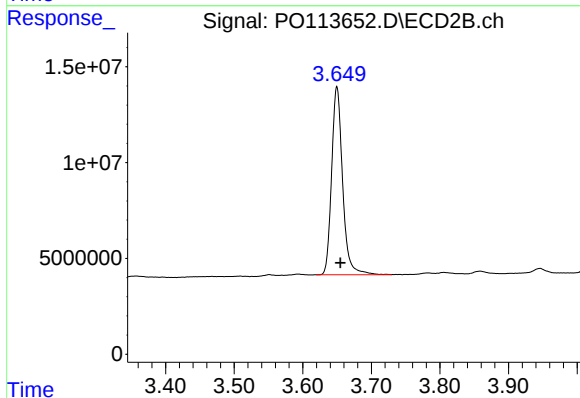


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: -0.005 min
Response: 109457274
Conc: 21.63 ng/ml

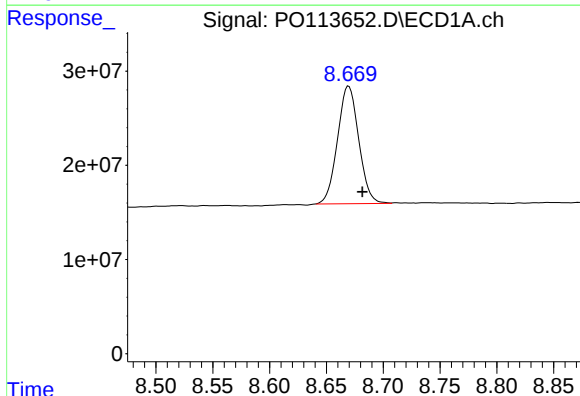


#2 Decachlorobiphenyl

R.T.: 8.670 min
Delta R.T.: -0.012 min
Response: 162093296
Conc: 23.39 ng/ml

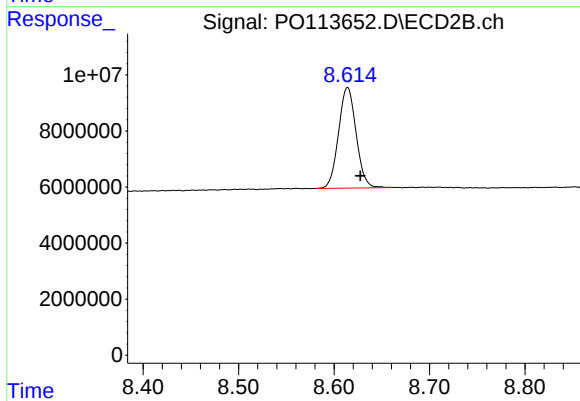

#2 Decachlorobiphenyl


R.T.: 8.614 min
Delta R.T.: -0.013 min
Response: 46039121
Conc: 24.30 ng/ml

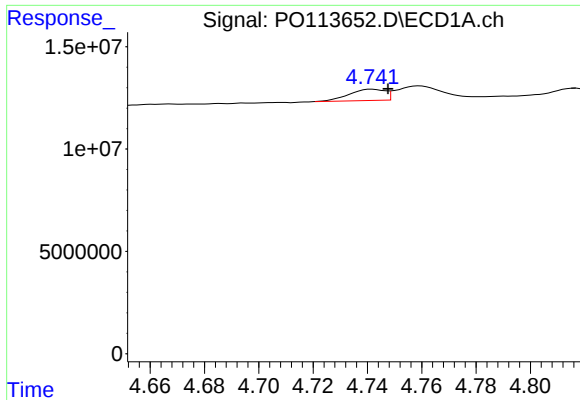

#3 AR-1016-1


R.T.: 4.742 min
Delta R.T.: -0.006 min
Response: 5113387
Conc: 19.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

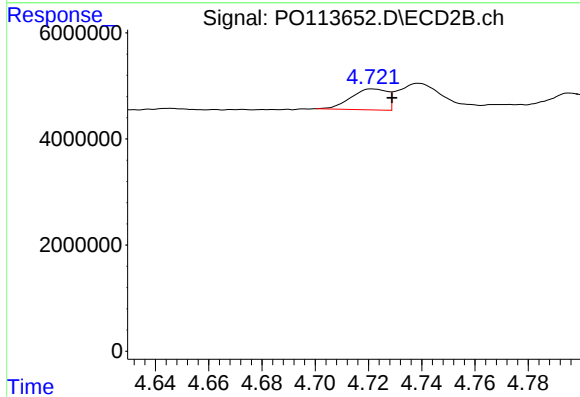


#3 AR-1016-1

R.T.: 4.722 min
Delta R.T.: -0.007 min
Response: 3743337
Conc: 21.95 ng/ml

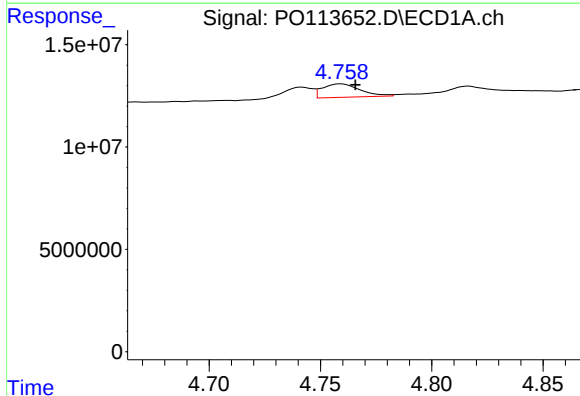


#4 AR-1016-2

R.T.: 4.759 min
Delta R.T.: -0.006 min
Response: 7781558
Conc: 19.38 ng/ml

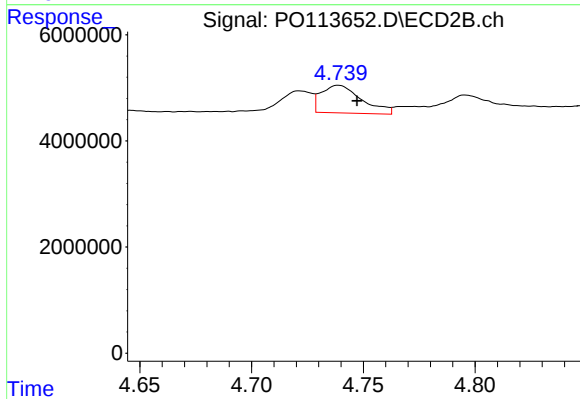

#4 AR-1016-2


R.T.: 4.739 min
Delta R.T.: -0.008 min
Response: 6571732
Conc: 25.51 ng/ml

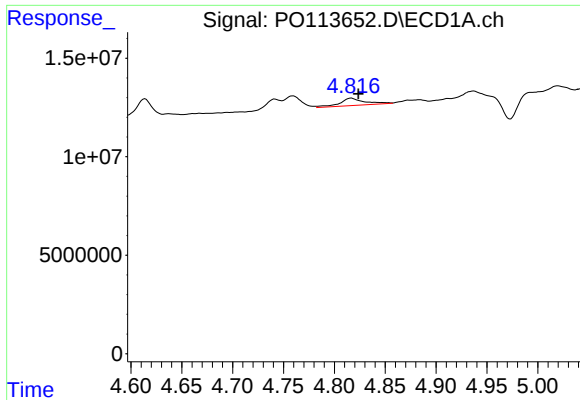

#5 AR-1016-3


R.T.: 4.817 min
Delta R.T.: -0.007 min
Response: 6431041
Conc: 25.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

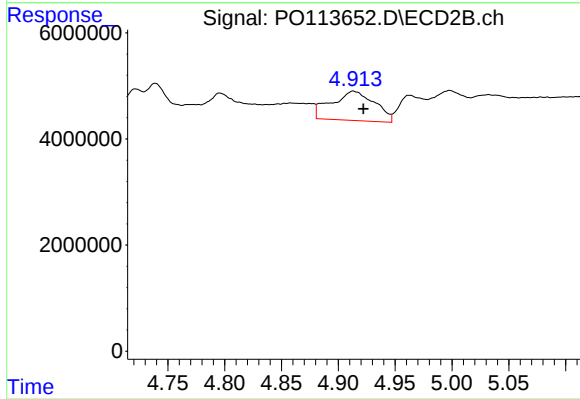


#5 AR-1016-3

R.T.: 4.913 min
Delta R.T.: -0.009 min
Response: 14676567
Conc: 105.12 ng/ml

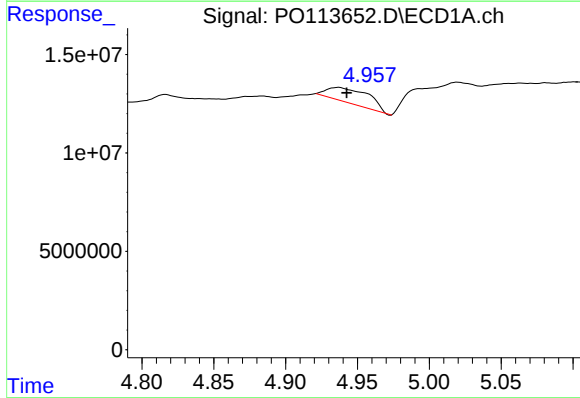


#6 AR-1016-4

R.T.: 4.937 min
Delta R.T.: -0.005 min
Response: 15467829
Conc: 70.93 ng/ml

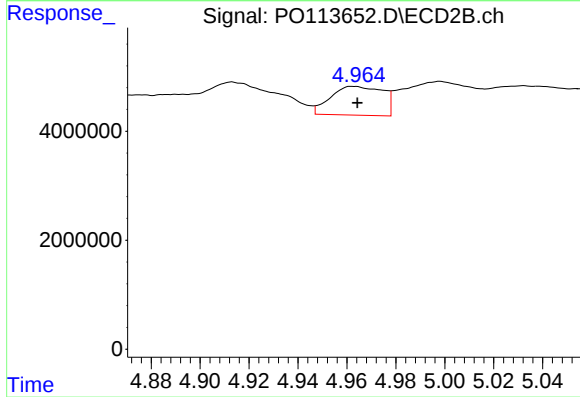

#6 AR-1016-4


R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 7819102
Conc: 67.00 ng/ml

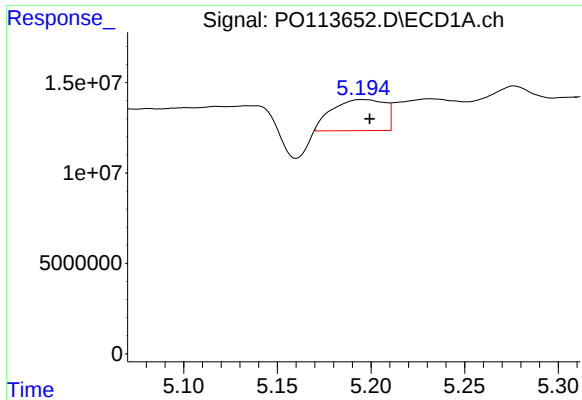

#7 AR-1016-5


R.T.: 5.195 min
Delta R.T.: -0.004 min
Response: 33323403
Conc: 150.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

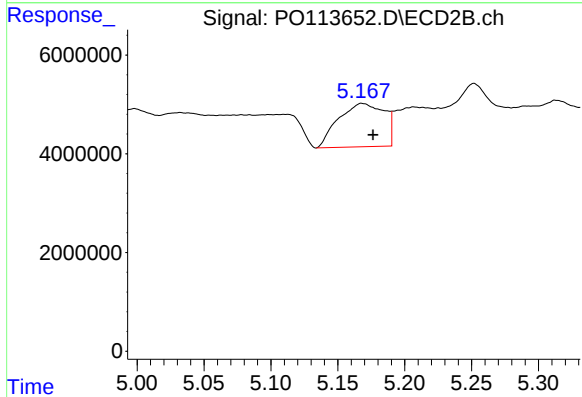


#7 AR-1016-5

R.T.: 5.168 min
Delta R.T.: -0.008 min
Response: 20979673
Conc: 147.19 ng/ml

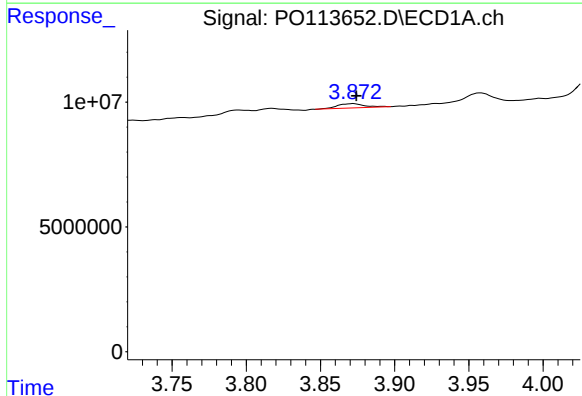


#8 AR-1221-1

R.T.: 3.872 min
Delta R.T.: -0.002 min
Response: 2150139
Conc: 22.98 ng/ml

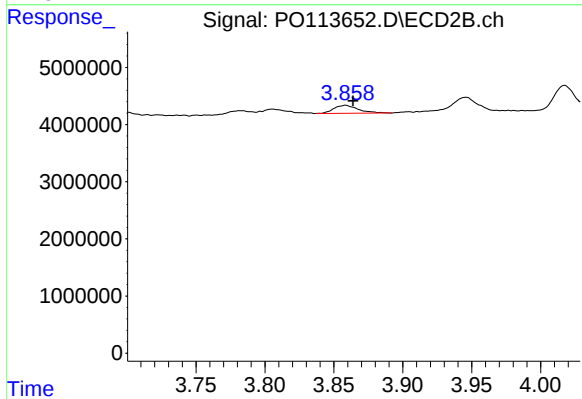

#8 AR-1221-1


R.T.: 3.858 min
Delta R.T.: -0.005 min
Response: 1719789
Conc: 27.25 ng/ml

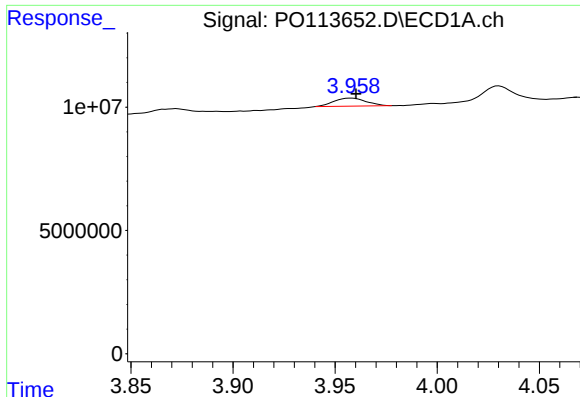

#9 AR-1221-2


R.T.: 3.958 min
Delta R.T.: -0.002 min
Response: 3615667
Conc: 53.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

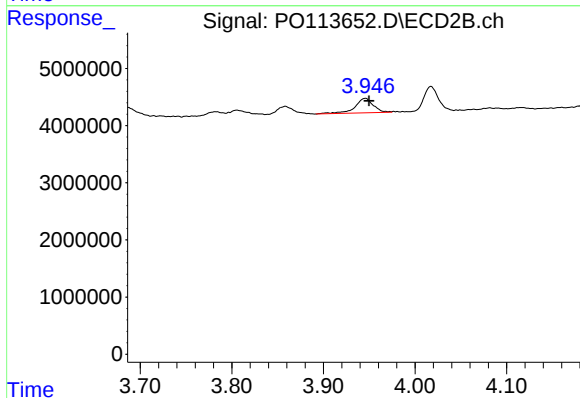


#9 AR-1221-2

R.T.: 3.946 min
Delta R.T.: -0.004 min
Response: 3571703
Conc: 76.53 ng/ml

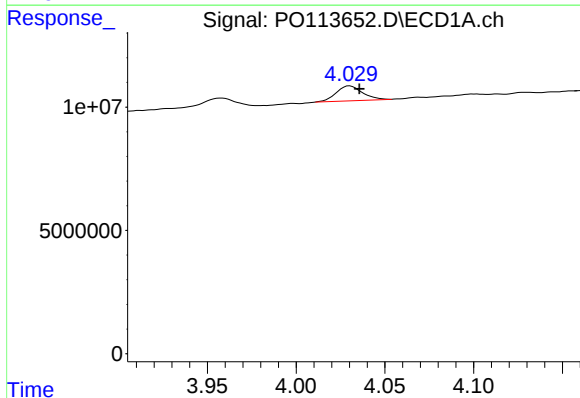


#10 AR-1221-3

R.T.: 4.030 min
Delta R.T.: -0.005 min
Response: 6248253
Conc: 28.23 ng/ml

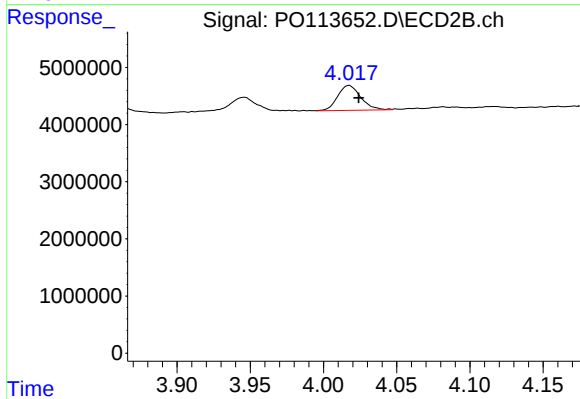

#10 AR-1221-3


R.T.: 4.017 min
Delta R.T.: -0.007 min
Response: 4779826
Conc: 32.19 ng/ml

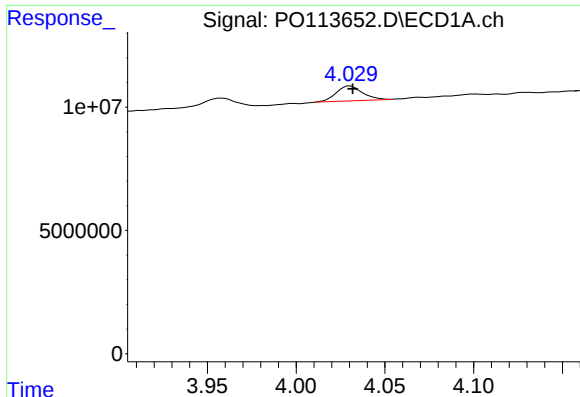

#11 AR-1232-1


R.T.: 4.030 min
Delta R.T.: -0.002 min
Response: 6248253
Conc: 34.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

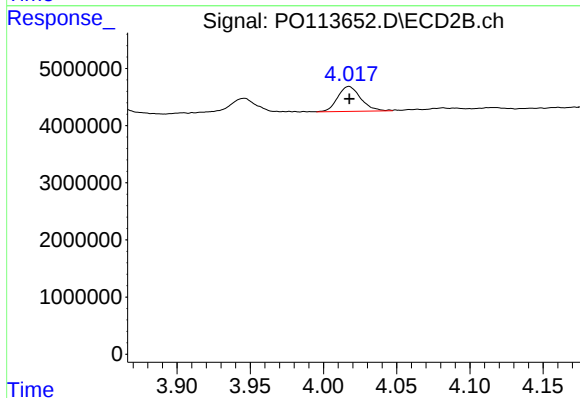


#11 AR-1232-1

R.T.: 4.017 min
Delta R.T.: 0.000 min
Response: 4779826
Conc: 39.52 ng/ml

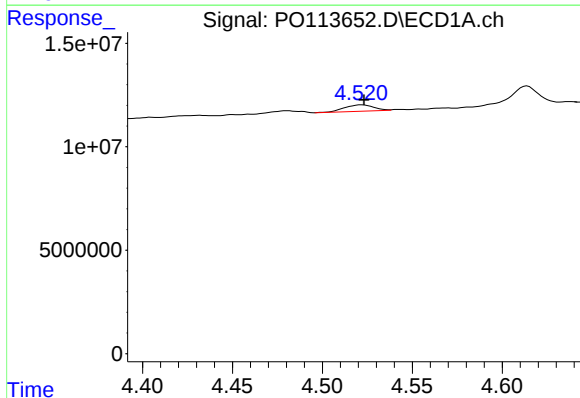


#12 AR-1232-2

R.T.: 4.522 min
Delta R.T.: -0.001 min
Response: 3495206
Conc: 32.39 ng/ml

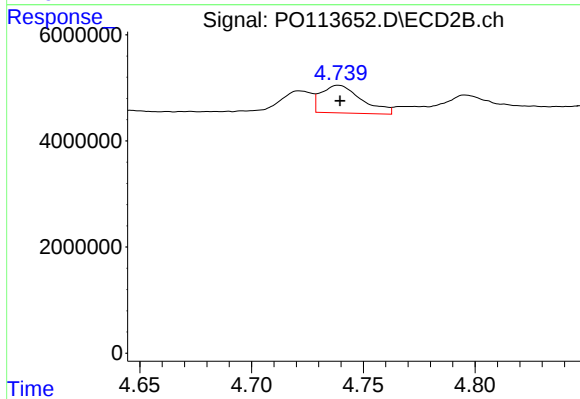

#12 AR-1232-2


R.T.: 4.739 min
Delta R.T.: 0.000 min
Response: 6571732
Conc: 53.84 ng/ml

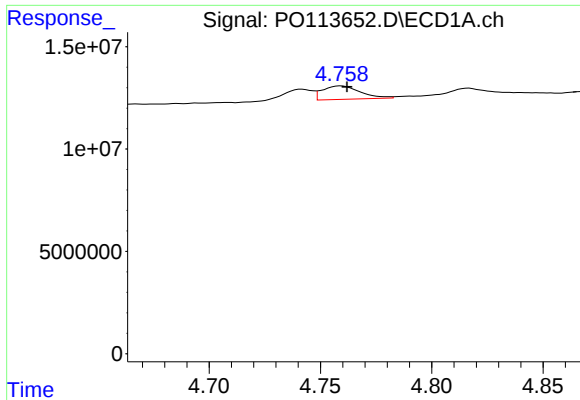

#13 AR-1232-3


R.T.: 4.759 min
Delta R.T.: -0.003 min
Response: 7781558
Conc: 39.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

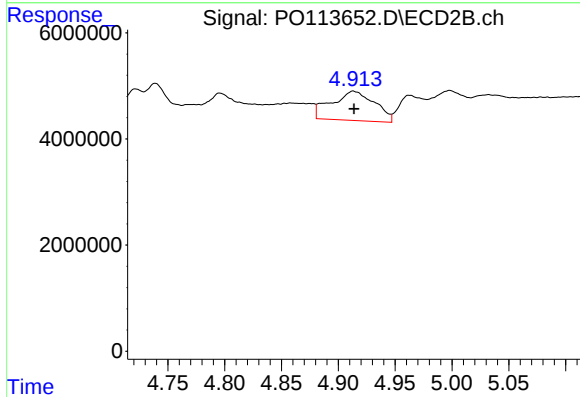


#13 AR-1232-3

R.T.: 4.913 min
Delta R.T.: 0.000 min
Response: 14676567
Conc: 221.85 ng/ml

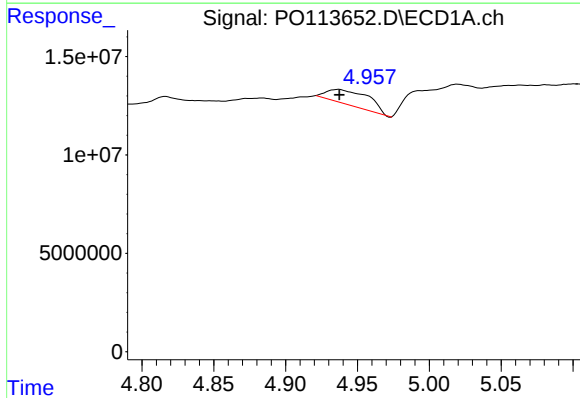


#14 AR-1232-4

R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 15467829
Conc: 157.36 ng/ml

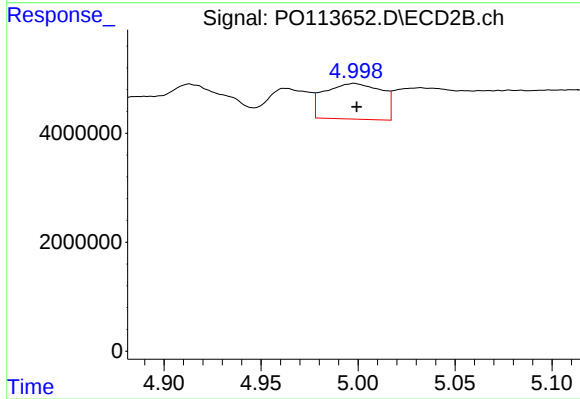

#14 AR-1232-4


R.T.: 4.998 min
Delta R.T.: -0.001 min
Response: 13417609
Conc: 223.89 ng/ml

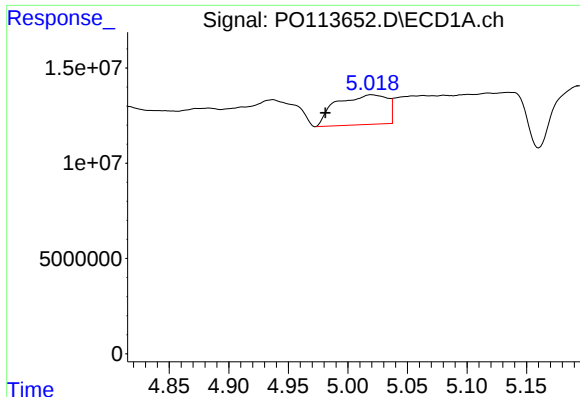

#15 AR-1232-5


R.T.: 5.020 min
Delta R.T.: 0.039 min
Response: 46267768
Conc: 703.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

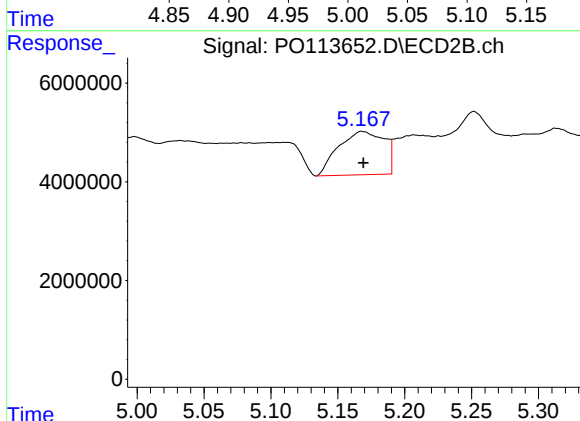


#15 AR-1232-5

R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 20979673
Conc: 310.28 ng/ml

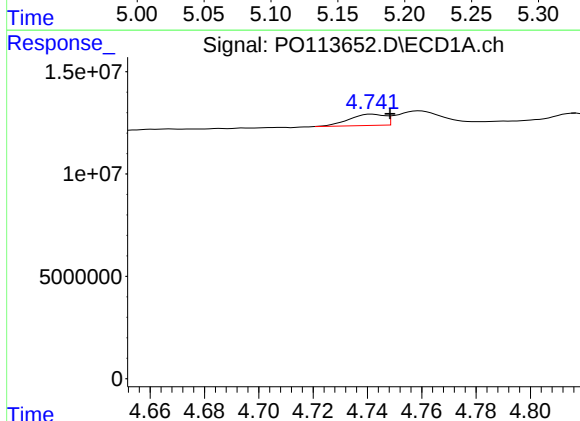


#16 AR-1242-1

R.T.: 4.742 min
Delta R.T.: -0.007 min
Response: 5113387
Conc: 22.24 ng/ml

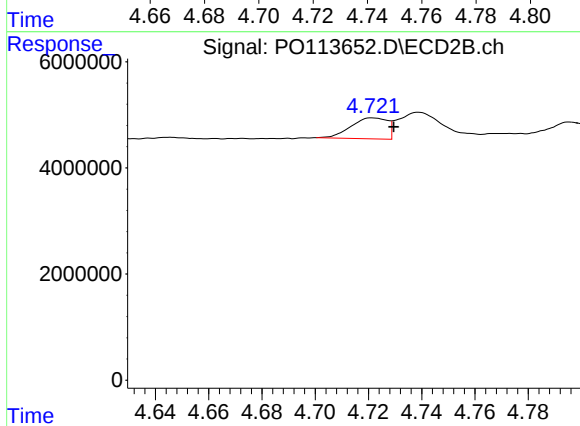

#16 AR-1242-1


R.T.: 4.722 min
Delta R.T.: -0.008 min
Response: 3743337
Conc: 25.90 ng/ml

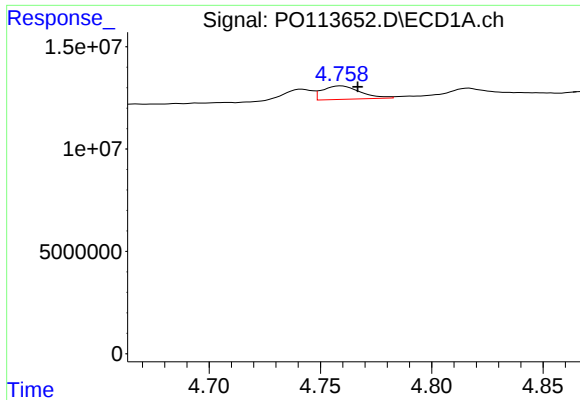

#17 AR-1242-2


R.T.: 4.759 min
Delta R.T.: -0.008 min
Response: 7781558
Conc: 22.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

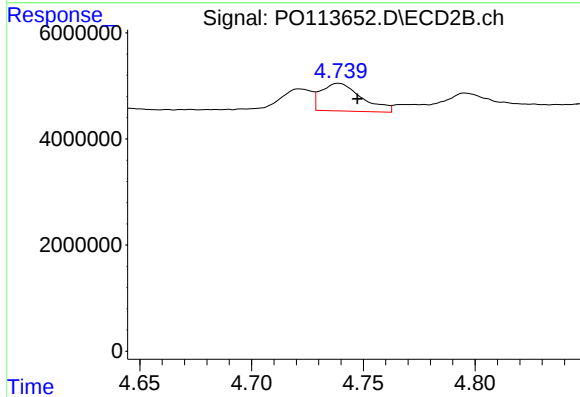


#17 AR-1242-2

R.T.: 4.739 min
Delta R.T.: -0.008 min
Response: 6571732
Conc: 30.30 ng/ml

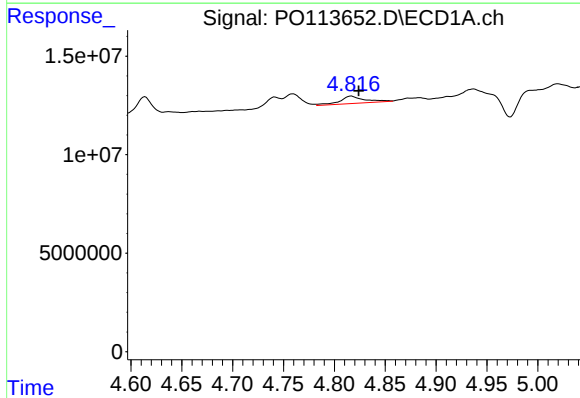


#18 AR-1242-3

R.T.: 4.817 min
Delta R.T.: -0.007 min
Response: 6431041
Conc: 28.98 ng/ml

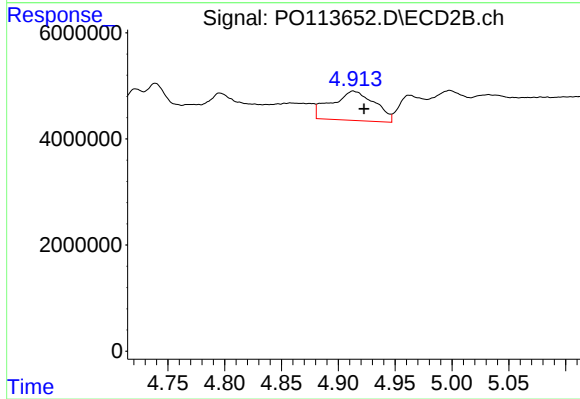

#18 AR-1242-3


R.T.: 4.913 min
Delta R.T.: -0.009 min
Response: 14676567
Conc: 125.48 ng/ml

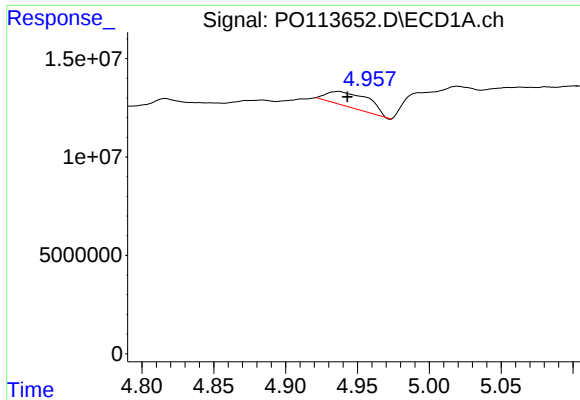

#19 AR-1242-4


R.T.: 4.937 min
Delta R.T.: -0.006 min
Response: 15467829
Conc: 89.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

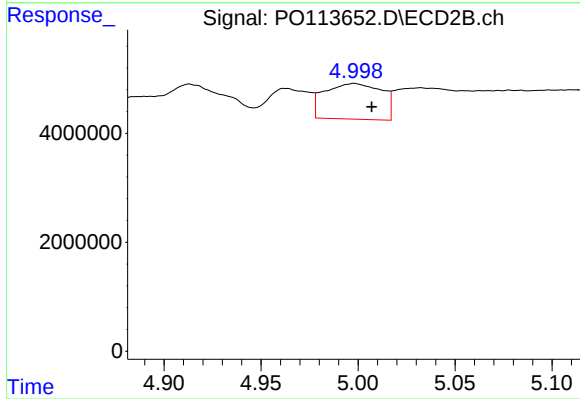


#19 AR-1242-4

R.T.: 4.998 min
Delta R.T.: -0.009 min
Response: 13417609
Conc: 114.06 ng/ml

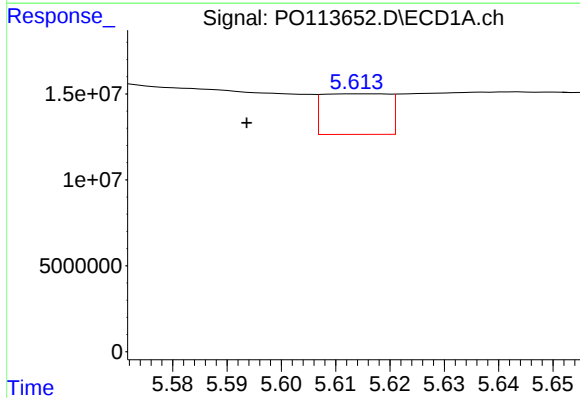


#20 AR-1242-5

R.T.: 5.616 min
Delta R.T.: 0.022 min
Response: 19973089
Conc: 99.78 ng/ml

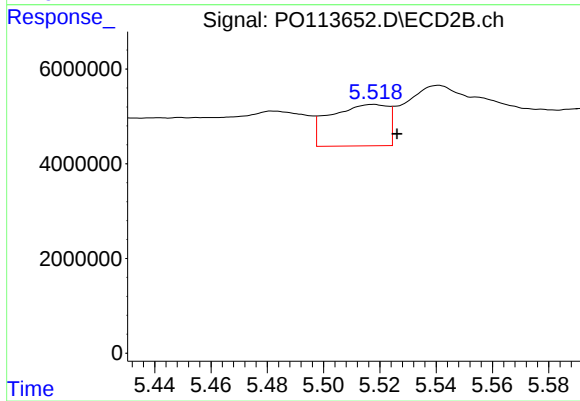

#20 AR-1242-5


R.T.: 5.518 min
Delta R.T.: -0.008 min
Response: 12447109
Conc: 83.46 ng/ml

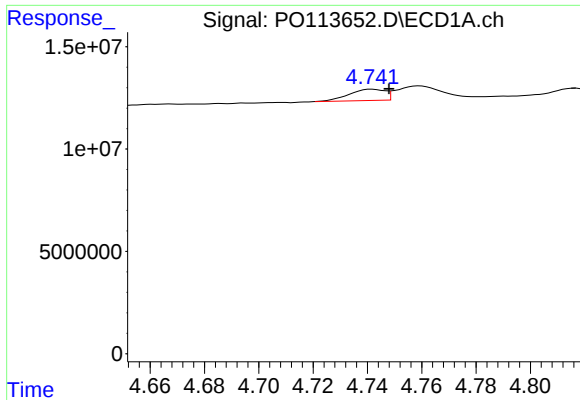

#21 AR-1248-1


R.T.: 4.742 min
Delta R.T.: -0.006 min
Response: 5113387
Conc: 29.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

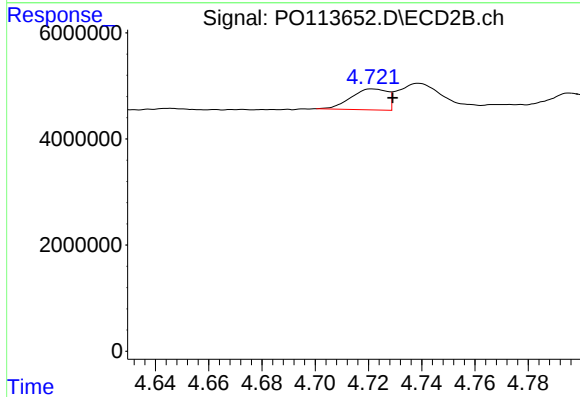


#21 AR-1248-1

R.T.: 4.722 min
Delta R.T.: -0.007 min
Response: 3743337
Conc: 33.57 ng/ml

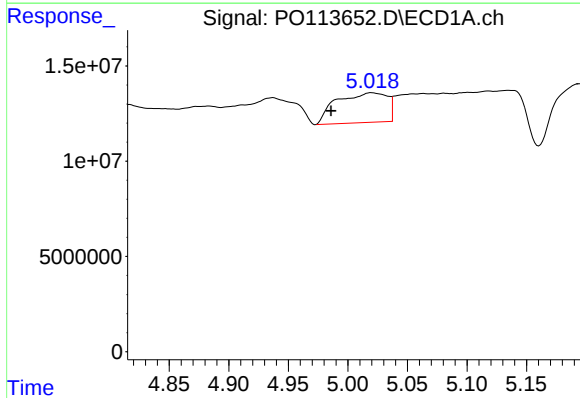


#22 AR-1248-2

R.T.: 5.020 min
Delta R.T.: 0.034 min
Response: 46267768
Conc: 191.30 ng/ml

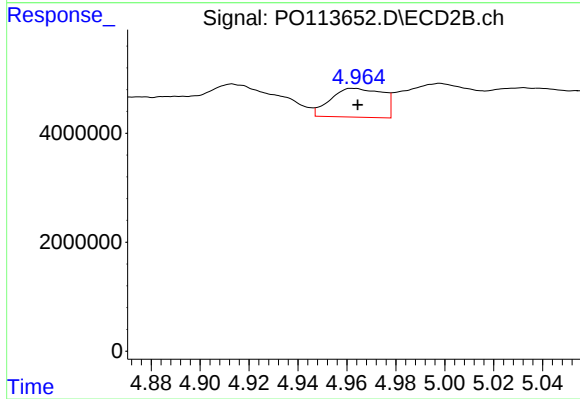

#22 AR-1248-2


R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 7819102
Conc: 48.66 ng/ml

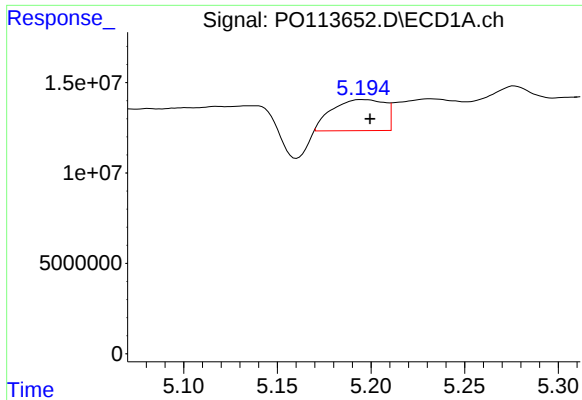

#23 AR-1248-3


R.T.: 5.195 min
Delta R.T.: -0.004 min
Response: 33323403
Conc: 104.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

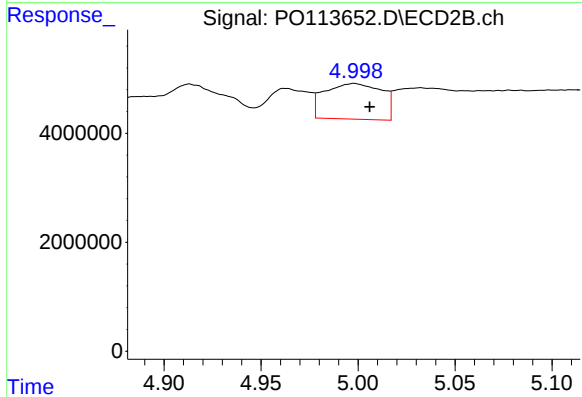


#23 AR-1248-3

R.T.: 4.998 min
Delta R.T.: -0.008 min
Response: 13417609
Conc: 79.08 ng/ml

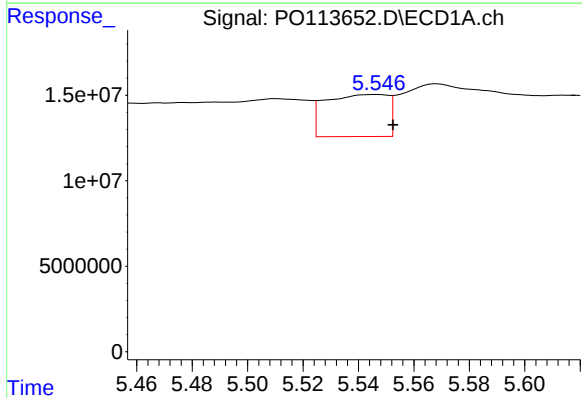


#24 AR-1248-4

R.T.: 5.546 min
Delta R.T.: -0.006 min
Response: 38434650
Conc: 76.93 ng/ml

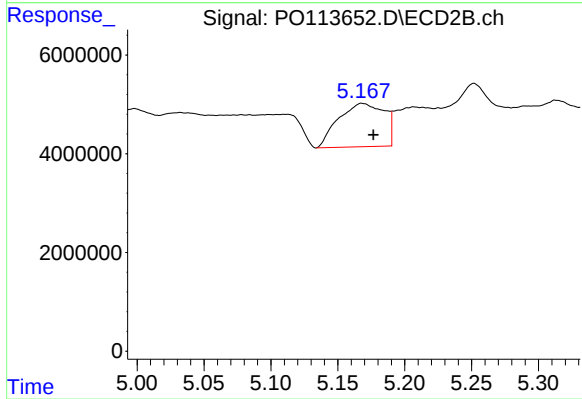

#24 AR-1248-4


R.T.: 5.168 min
Delta R.T.: -0.008 min
Response: 20979673
Conc: 105.31 ng/ml

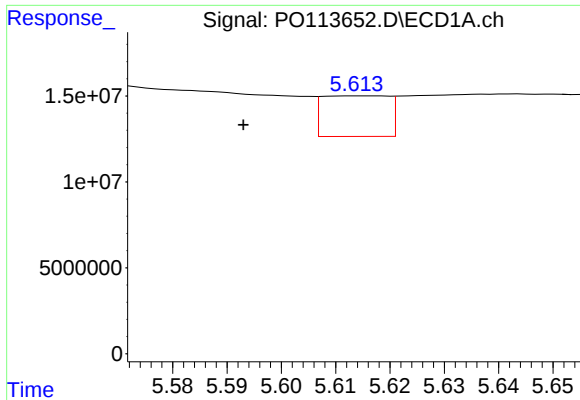

#25 AR-1248-5


R.T.: 5.616 min
Delta R.T.: 0.023 min
Response: 19973089
Conc: 58.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

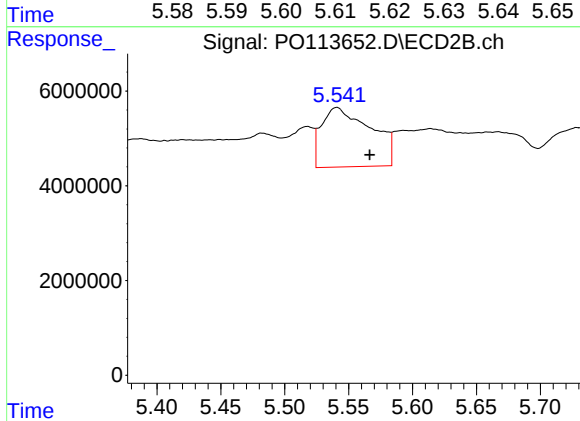


#25 AR-1248-5

R.T.: 5.541 min
Delta R.T.: -0.026 min
Response: 33623657
Conc: 158.38 ng/ml

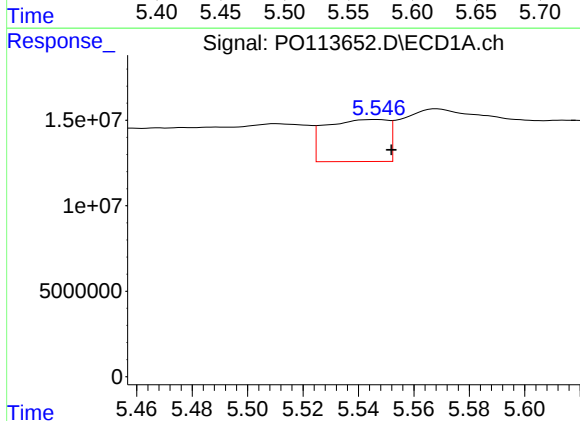


#26 AR-1254-1

R.T.: 5.546 min
Delta R.T.: -0.005 min
Response: 38434650
Conc: 71.18 ng/ml

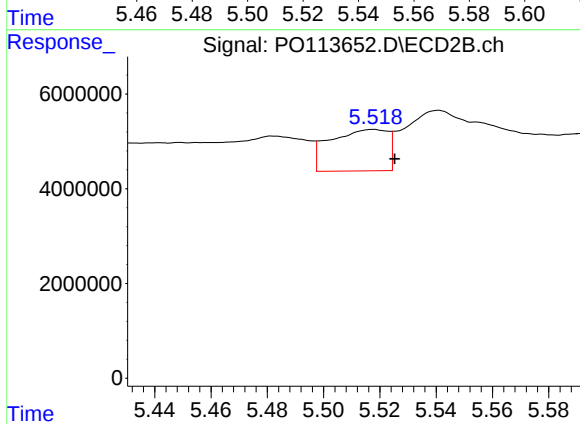

#26 AR-1254-1


R.T.: 5.518 min
Delta R.T.: -0.008 min
Response: 12447109
Conc: 39.47 ng/ml

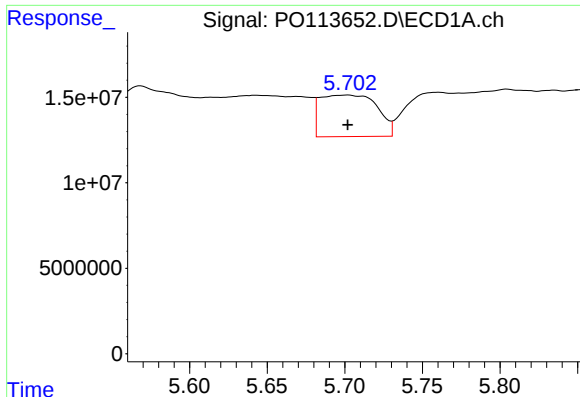

#27 AR-1254-2


R.T.: 5.702 min
Delta R.T.: 0.000 min
Response: 62234821
Conc: 126.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

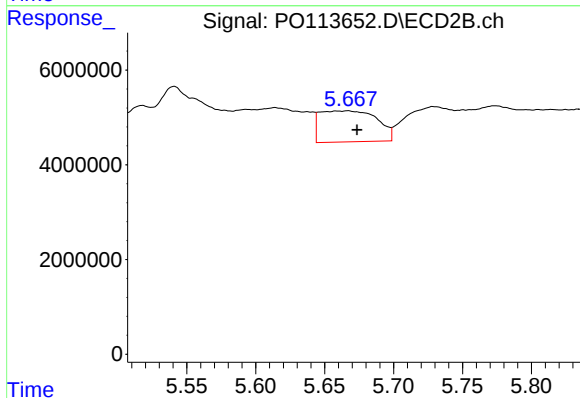


#27 AR-1254-2

R.T.: 5.667 min
Delta R.T.: -0.007 min
Response: 18918612
Conc: 67.48 ng/ml

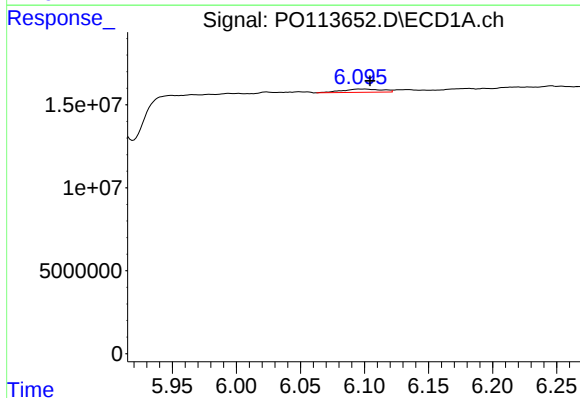


#28 AR-1254-3

R.T.: 6.096 min
Delta R.T.: -0.009 min
Response: 4247206
Conc: 5.75 ng/ml

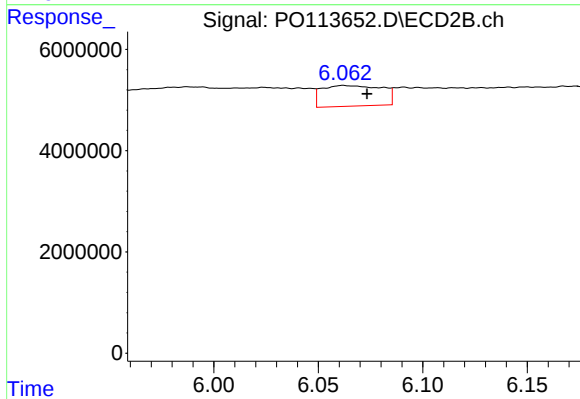

#28 AR-1254-3


R.T.: 6.062 min
Delta R.T.: -0.011 min
Response: 8137421
Conc: 19.52 ng/ml

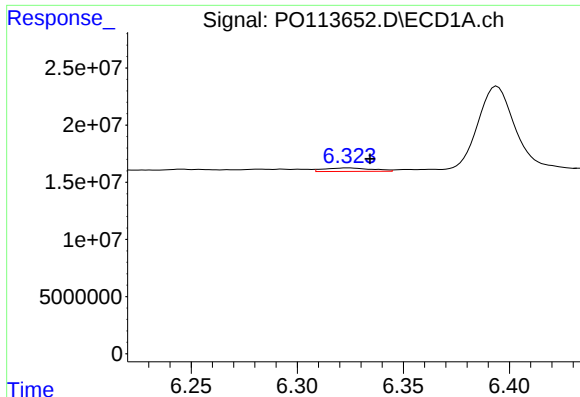

#29 AR-1254-4


R.T.: 6.324 min
Delta R.T.: -0.010 min
Response: 4750629
Conc: 8.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

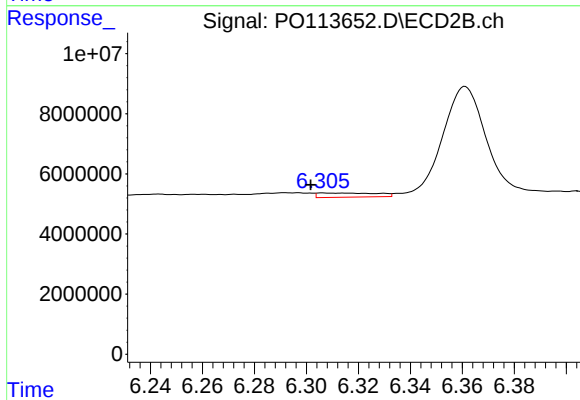


#29 AR-1254-4

R.T.: 6.306 min
Delta R.T.: 0.004 min
Response: 2229430
Conc: 8.11 ng/ml

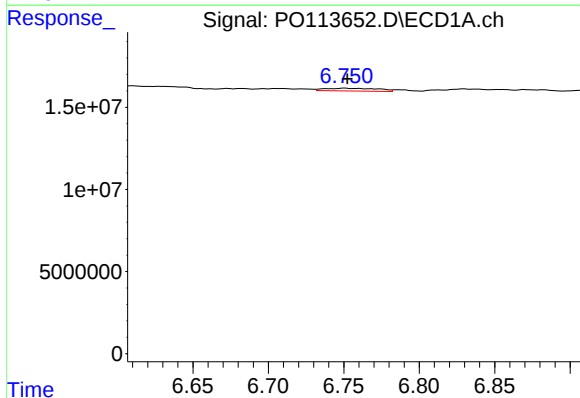


#30 AR-1254-5

R.T.: 6.751 min
Delta R.T.: -0.002 min
Response: 4147146
Conc: 5.92 ng/ml

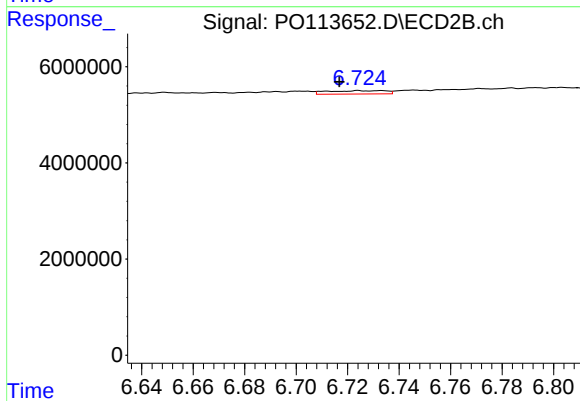

#30 AR-1254-5


R.T.: 6.724 min
Delta R.T.: 0.008 min
Response: 1130649
Conc: 3.16 ng/ml

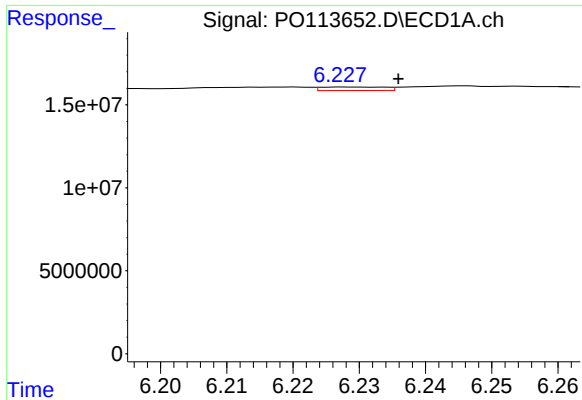

#31 AR-1260-1


R.T.: 6.228 min
Delta R.T.: -0.008 min
Response: 1404973
Conc: 3.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

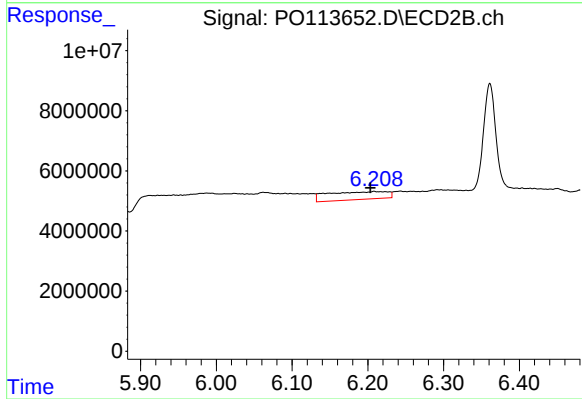


#31 AR-1260-1

R.T.: 6.208 min
Delta R.T.: 0.005 min
Response: 14260213
Conc: 55.91 ng/ml

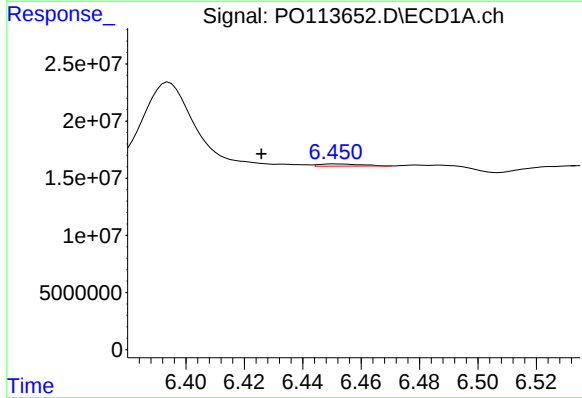


#32 AR-1260-2

R.T.: 6.452 min
Delta R.T.: 0.026 min
Response: 1978064
Conc: 2.88 ng/ml

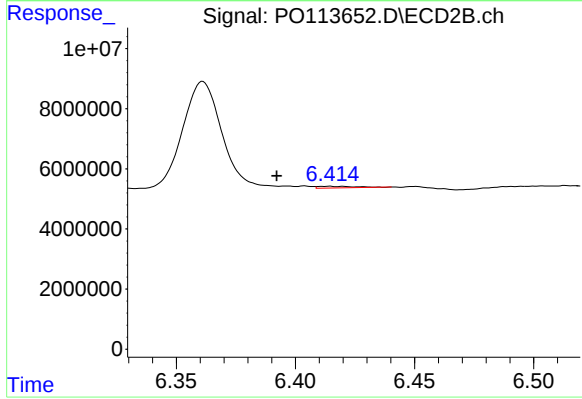

#32 AR-1260-2


R.T.: 6.414 min
Delta R.T.: 0.022 min
Response: 791892
Conc: 2.29 ng/ml

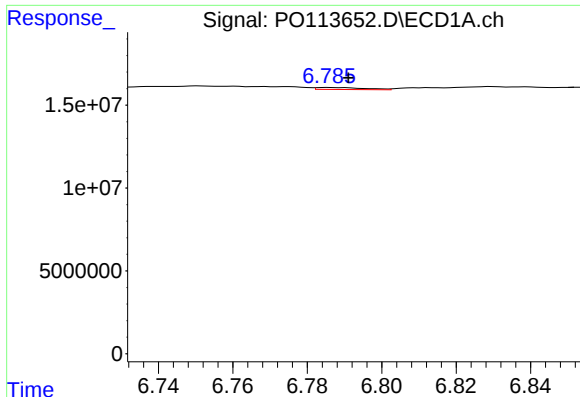

#33 AR-1260-3


R.T.: 6.786 min
Delta R.T.: -0.005 min
Response: 1081494
Conc: 1.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

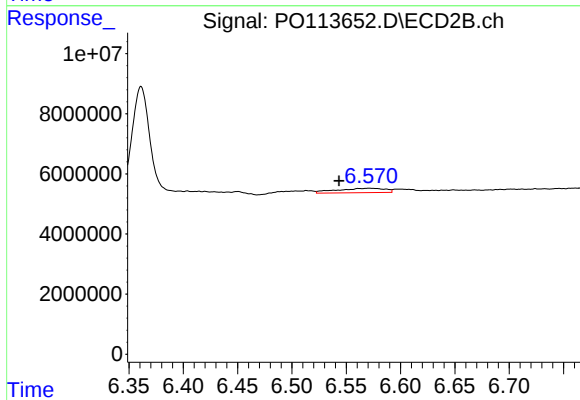


#33 AR-1260-3

R.T.: 6.571 min
Delta R.T.: 0.028 min
Response: 4510929
Conc: 15.17 ng/ml

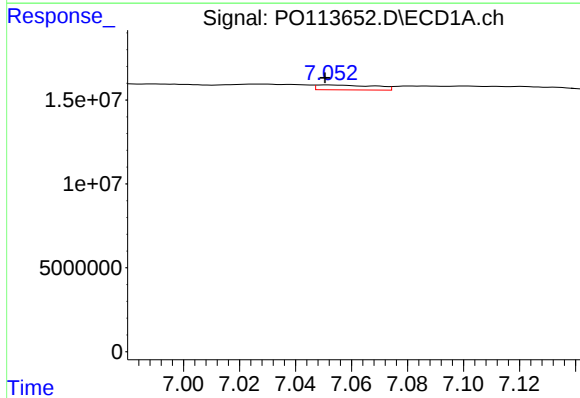


#34 AR-1260-4

R.T.: 7.051 min
Delta R.T.: 0.000 min
Response: 4124566
Conc: 9.21 ng/ml

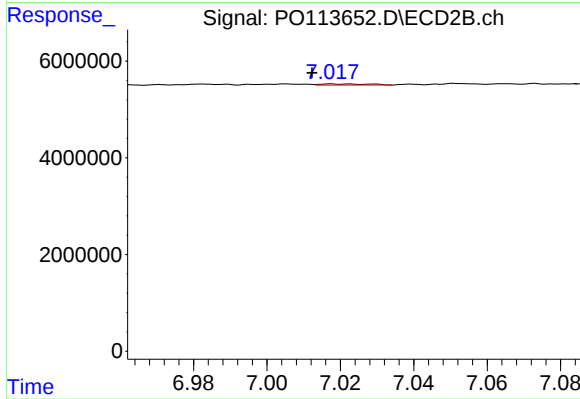

#34 AR-1260-4


R.T.: 7.018 min
Delta R.T.: 0.005 min
Response: 220138
Conc: 1.06 ng/ml

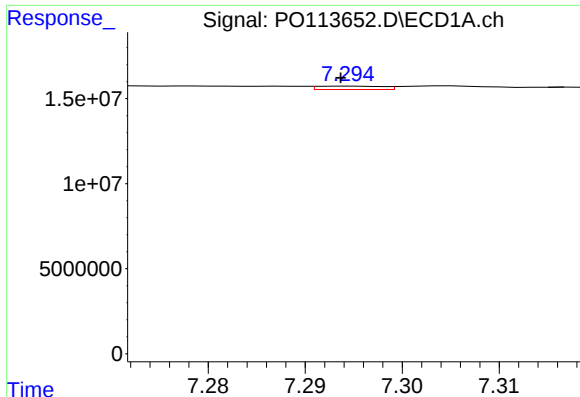

#35 AR-1260-5


R.T.: 7.295 min
Delta R.T.: 0.001 min
Response: 908169
Conc: 0.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

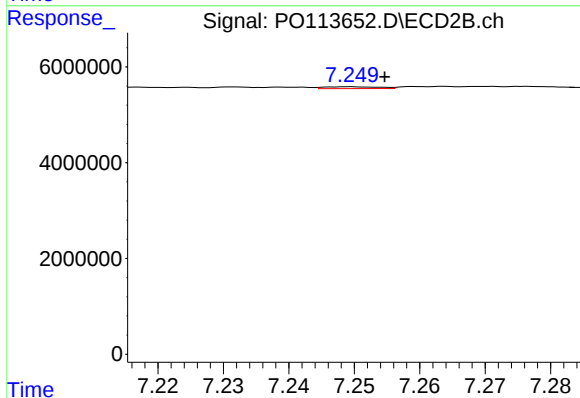


#35 AR-1260-5

R.T.: 7.249 min
Delta R.T.: -0.005 min
Response: 233593
Conc: 0.50 ng/ml

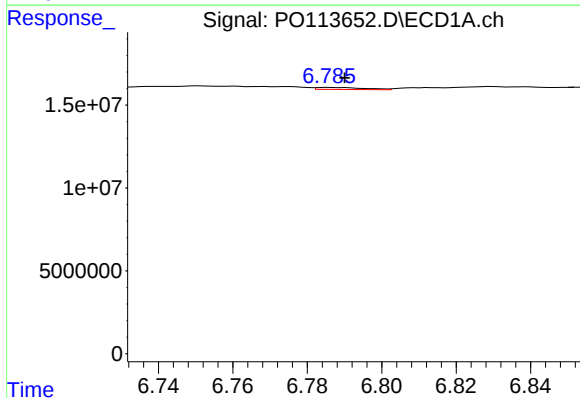


#36 AR-1262-1

R.T.: 6.786 min
Delta R.T.: -0.004 min
Response: 1081494
Conc: 1.18 ng/ml

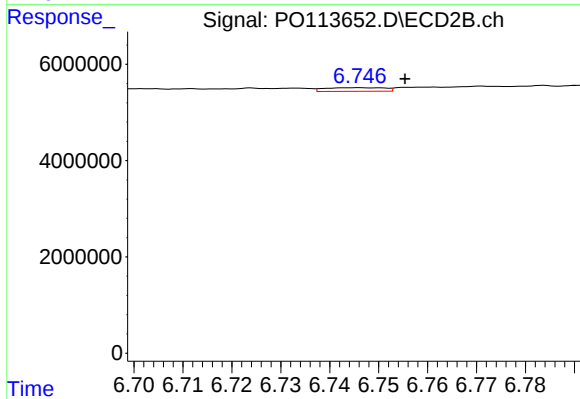

#36 AR-1262-1


R.T.: 6.746 min
Delta R.T.: -0.010 min
Response: 632384
Conc: 1.53 ng/ml

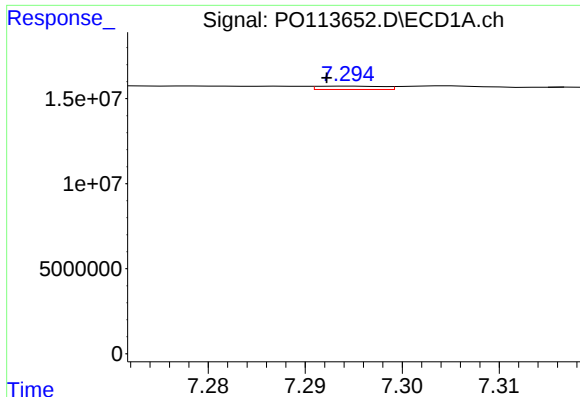

#37 AR-1262-2


R.T.: 7.295 min
Delta R.T.: 0.003 min
Response: 908169
Conc: 0.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

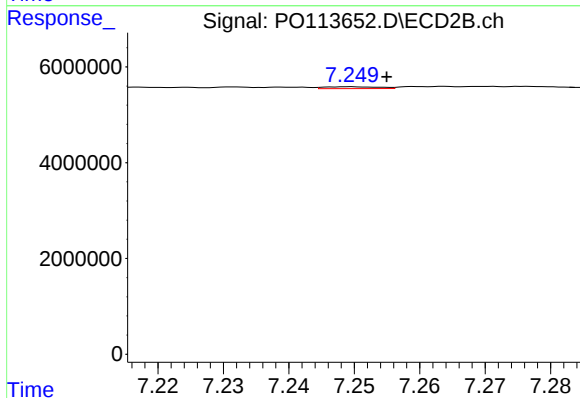


#37 AR-1262-2

R.T.: 7.249 min
Delta R.T.: -0.006 min
Response: 233593
Conc: 0.45 ng/ml

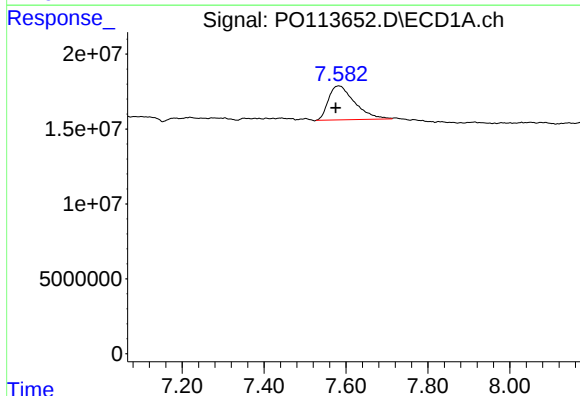


#38 AR-1262-3

R.T.: 7.582 min
Delta R.T.: 0.008 min
Response: 100362571
Conc: 181.12 ng/ml

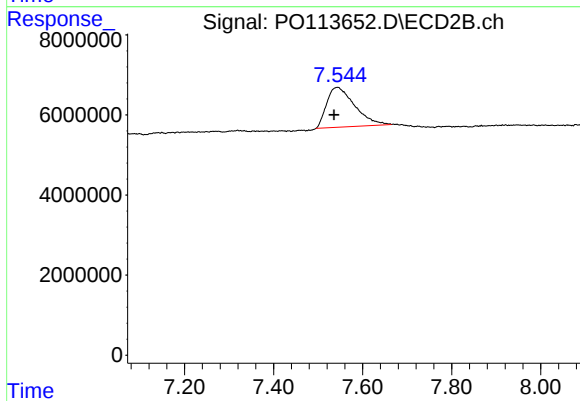

#38 AR-1262-3


R.T.: 7.544 min
Delta R.T.: 0.008 min
Response: 43567978
Conc: 242.60 ng/ml

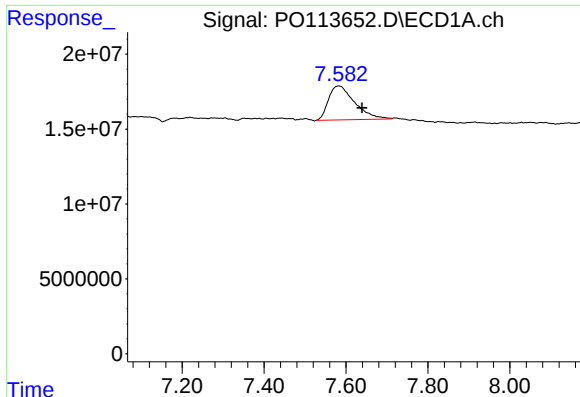

#39 AR-1262-4


R.T.: 7.582 min
Delta R.T.: -0.057 min
Response: 100362571
Conc: 102.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

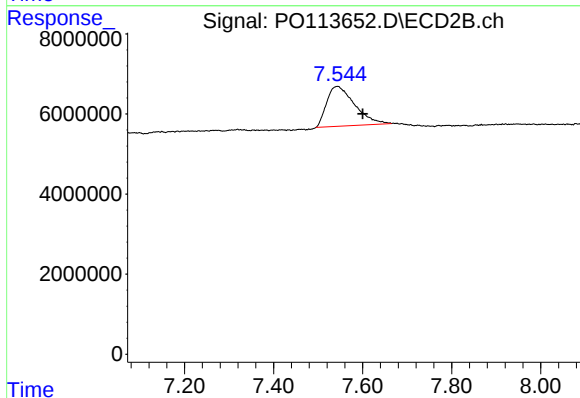


#39 AR-1262-4

R.T.: 7.544 min
Delta R.T.: -0.056 min
Response: 43567978
Conc: 150.29 ng/ml

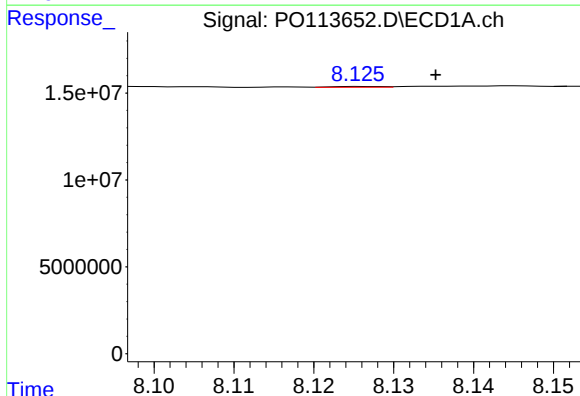


#40 AR-1262-5

R.T.: 8.126 min
Delta R.T.: -0.009 min
Response: 196274
Conc: 0.47 ng/ml

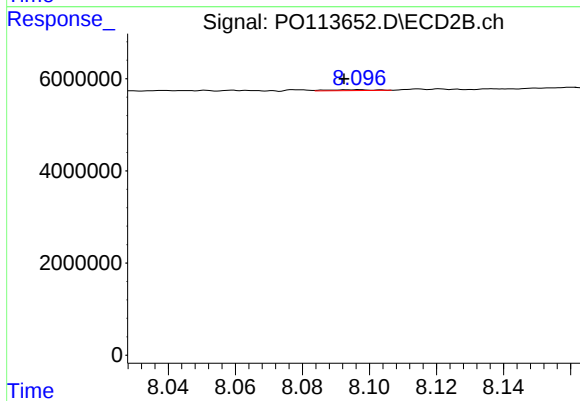

#40 AR-1262-5


R.T.: 8.096 min
Delta R.T.: 0.004 min
Response: 185573
Conc: 1.71 ng/ml

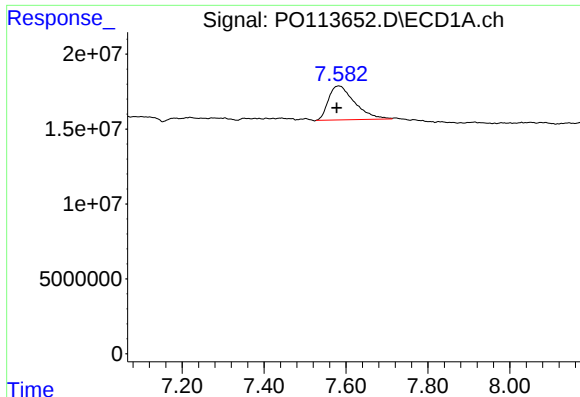

#41 AR-1268-1


R.T.: 7.582 min
Delta R.T.: 0.005 min
Response: 100362571
Conc: 58.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

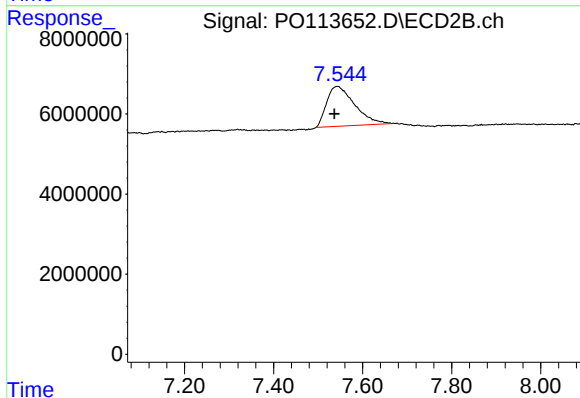


#41 AR-1268-1

R.T.: 7.544 min
Delta R.T.: 0.007 min
Response: 43567978
Conc: 85.52 ng/ml

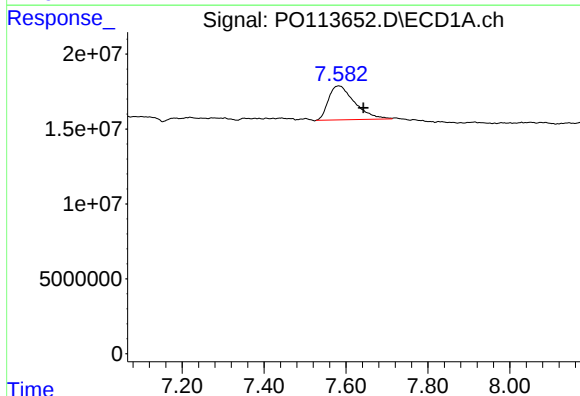


#42 AR-1268-2

R.T.: 7.582 min
Delta R.T.: -0.060 min
Response: 100362571
Conc: 69.30 ng/ml

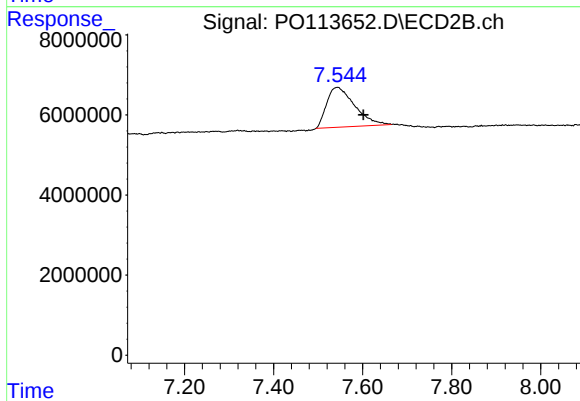

#42 AR-1268-2


R.T.: 7.544 min
Delta R.T.: -0.058 min
Response: 43567978
Conc: 104.88 ng/ml

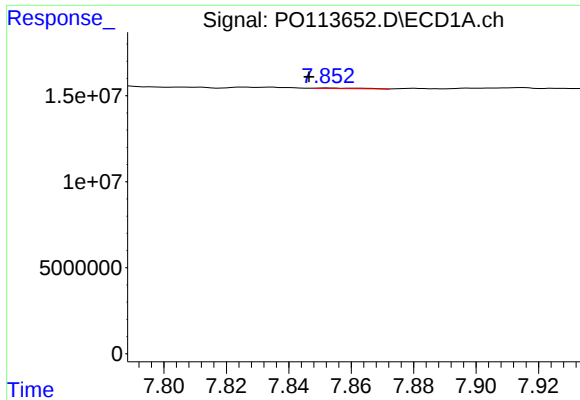

#43 AR-1268-3


R.T.: 7.853 min
Delta R.T.: 0.006 min
Response: 356323
Conc: 0.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

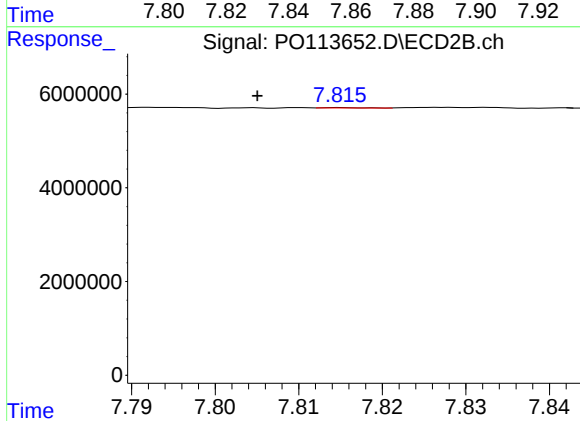


#43 AR-1268-3

R.T.: 7.815 min
Delta R.T.: 0.010 min
Response: 22480
Conc: 0.07 ng/ml

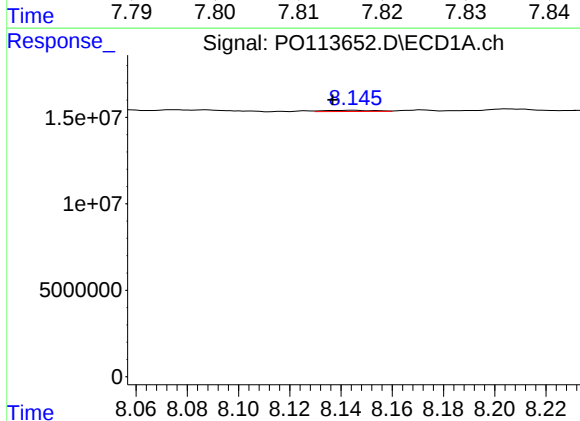


#44 AR-1268-4

R.T.: 8.145 min
Delta R.T.: 0.008 min
Response: 898457
Conc: 1.95 ng/ml

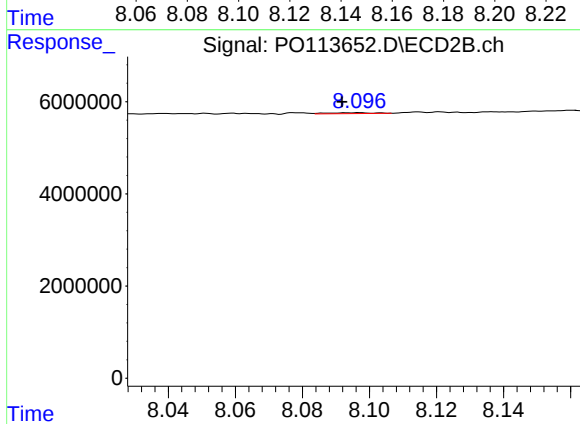

#44 AR-1268-4


R.T.: 8.096 min
Delta R.T.: 0.005 min
Response: 185573
Conc: 1.54 ng/ml

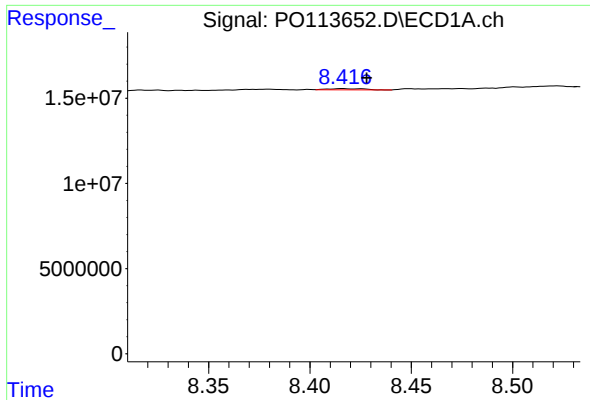

#45 AR-1268-5

R.T.: 8.416 min
Delta R.T.: -0.012 min
Response: 892678
Conc: 0.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

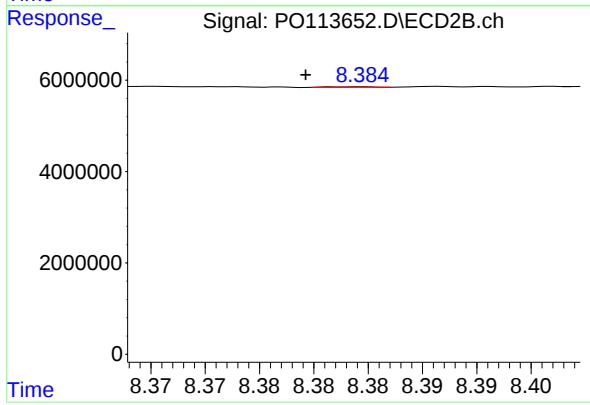

#45 AR-1268-5

R.T.: 8.384 min
Delta R.T.: 0.004 min
Response: 32324
Conc: 0.04 ng/ml