

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091125\
 Data File : P0113653.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 11:35
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1242 40PPB WATER MDL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 02:09:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.658	3.649	185.4E6	108.9E6	22.650	21.511
2)	SA Decachlor...	8.669	8.614	161.5E6	44676408	23.299	23.578
Target Compounds							
3)	L1 AR-1016-1	4.742	4.721	9557405	6632580	35.798	38.884
4)	L1 AR-1016-2	4.760	4.739	14463889	10035476	36.031	38.949
5)	L1 AR-1016-3	4.817	4.914	9331767	8471066	36.592	60.675 #
6)	L1 AR-1016-4	4.935	4.958	7783903	6926917	35.695	59.357 #
7)	L1 AR-1016-5	5.192	5.168	19925196	12383180	89.904	86.881
8)	L2 AR-1221-1	3.872	3.857	788245	609001	8.424	9.648
9)	L2 AR-1221-2	3.957	3.944	1972702	3086927	29.203	66.139 #
10)	L2 AR-1221-3	4.031	4.017	4569824	3618140	20.645	24.369
11)	L3 AR-1232-1	4.031	4.017	4569824	3618140	25.455	29.919
12)	L3 AR-1232-2	4.521	4.739	7676119	10035476	71.130	82.224
13)	L3 AR-1232-3	4.760	4.914	14463889	8471066	73.274	128.047 #
14)	L3 AR-1232-4	4.935	4.997	7783903	9455147	79.191	157.774 #
15)	L3 AR-1232-5	4.986	5.168	5871011	12383180	89.249	183.139 #
16)	L4 AR-1242-1	4.742	4.721	9557405	6632580	41.566	45.899
17)	L4 AR-1242-2	4.760	4.739	14463889	10035476	42.092	46.265
18)	L4 AR-1242-3	4.817	4.914	9331767	8471066	42.057	72.424 #
19)	L4 AR-1242-4	4.935	4.997	7783903	9455147	44.874	80.375 #
20)	L4 AR-1242-5	5.586	5.516	39888877	11479190	199.283	76.973 #
21)	L5 AR-1248-1	4.742	4.721	9557405	6632580	54.781	59.479
22)	L5 AR-1248-2	4.986	4.958	5871011	6926917	24.274	43.105 #
23)	L5 AR-1248-3	5.192	4.997	19925196	9455147	62.488	55.730
24)	L5 AR-1248-4	5.545	5.168	29447354	12383180	58.941	62.158
25)	L5 AR-1248-5	5.586	5.557	39888877	15712432	116.808	74.012 #
26)	L6 AR-1254-1	5.545	5.516	29447354	11479190	54.534	36.401 #
27)	L6 AR-1254-2	5.694	5.666	28986077	6807062	58.741	24.282 #
28)	L6 AR-1254-3	6.097	6.062	4500468	4335138	6.091	10.398 #
29)	L6 AR-1254-4	6.325	6.292	6517544	2558014	11.701	9.307
30)	L6 AR-1254-5	6.759	6.716	2987736	189450	4.262	0.530 #
31)	L7 AR-1260-1	6.239	6.207	2630447	1748588	5.898	6.855
32)	L7 AR-1260-2	6.455	6.392	1654202	128509	2.409	0.372 #
33)	L7 AR-1260-3	6.782	6.543	2012658	146410	3.260	0.492 #
34)	L7 AR-1260-4	7.054	7.017	7459037	348663	16.654	1.682 #
35)	L7 AR-1260-5	7.291	7.260	4456978	247177	3.681	0.528 #
36)	L8 AR-1262-1	6.782	6.762	2012658	342705	2.198	0.827 #
37)	L8 AR-1262-2	7.291	7.260	4456978	247177	2.947	0.477 #
38)	L8 AR-1262-3	7.577	7.541	18484879	4288533	33.360	23.880 #
39)	L8 AR-1262-4	7.677f	7.608	78084	265721	0.080	0.917 #
40)	L8 AR-1262-5	8.136	8.114	628122	189538	1.507	1.750
41)	L9 AR-1268-1	7.577	7.541	18484879	4288533	10.741	8.418

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091125\
 Data File : P0113653.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 11:35
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1242 40PPB WATER MDL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 02:09:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.677f	7.608	78084	265721	0.054	0.640 #
43) L9	AR-1268-3	7.856	7.791	64442	226087	0.053	0.692 #
44) L9	AR-1268-4	8.136	8.114	628122	189538	1.364	1.574
45) L9	AR-1268-5	8.431	8.375	82836	42183	0.026	0.054 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091125\
Data File : PO113653.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 11:35
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1242 40PPB WATER MDL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:09:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

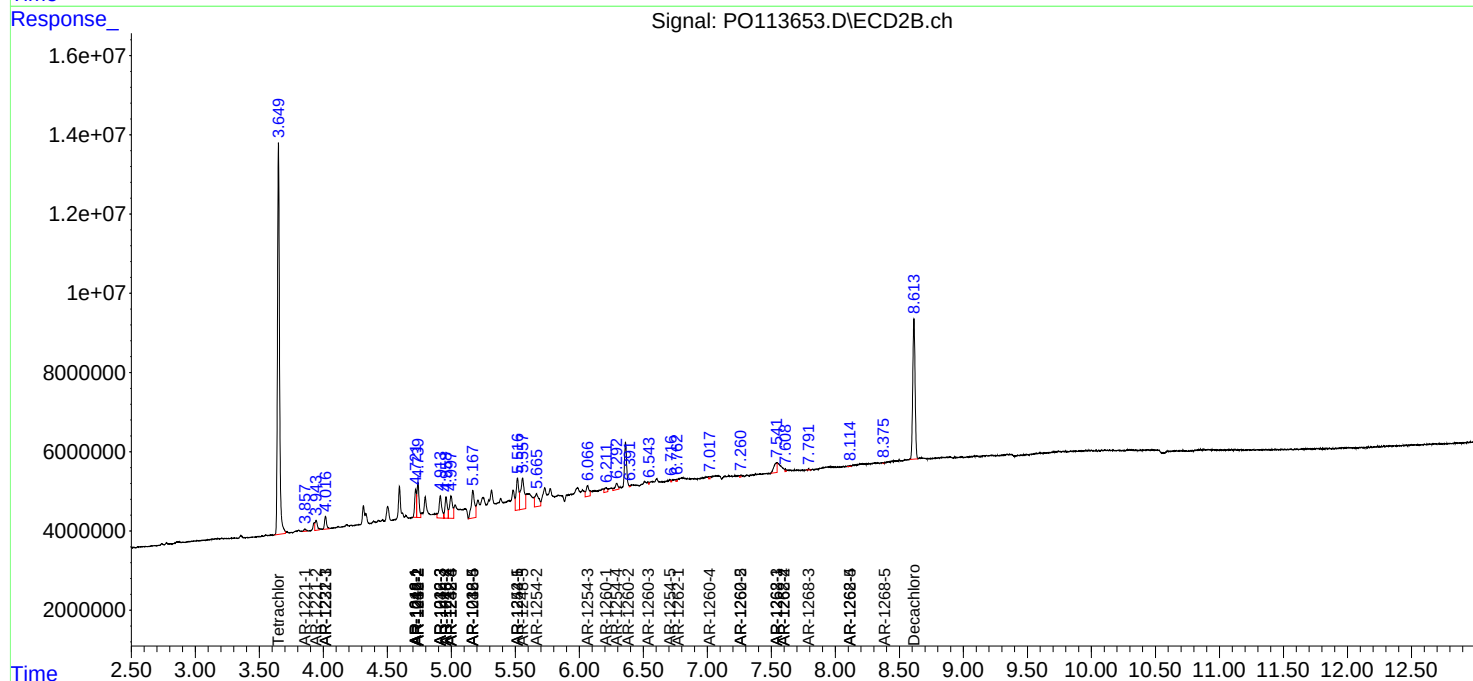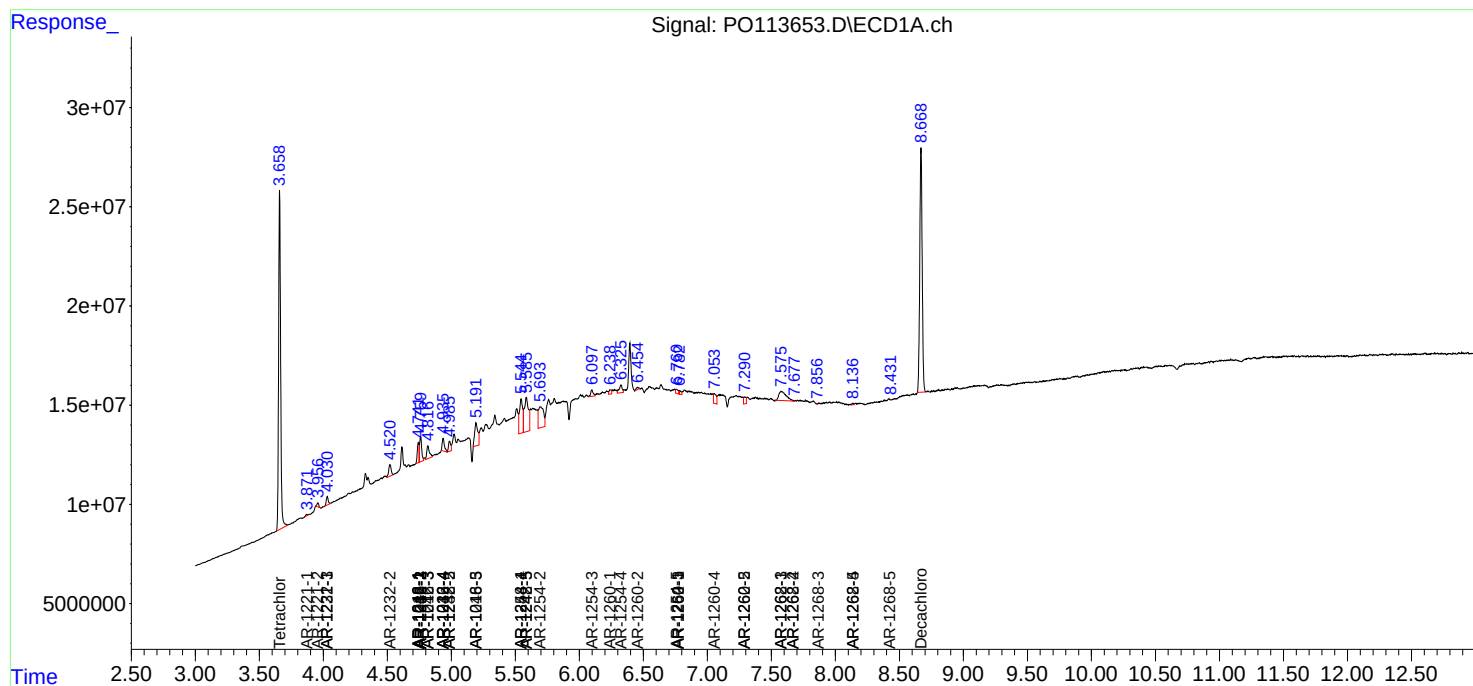


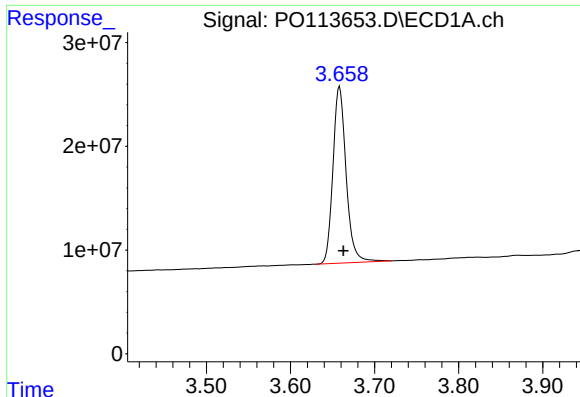

#1 Tetrachloro-m-xylene


R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 185423893
Conc: 22.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

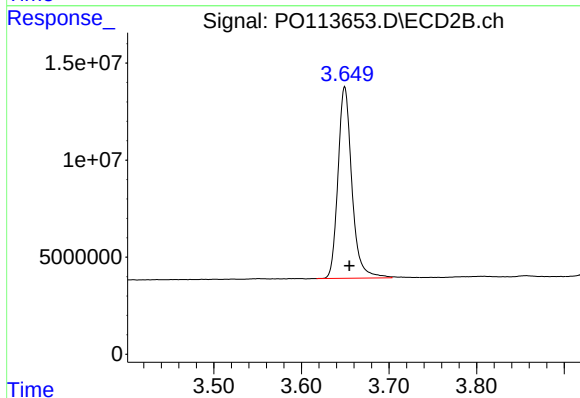


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.005 min
Response: 108860356
Conc: 21.51 ng/ml

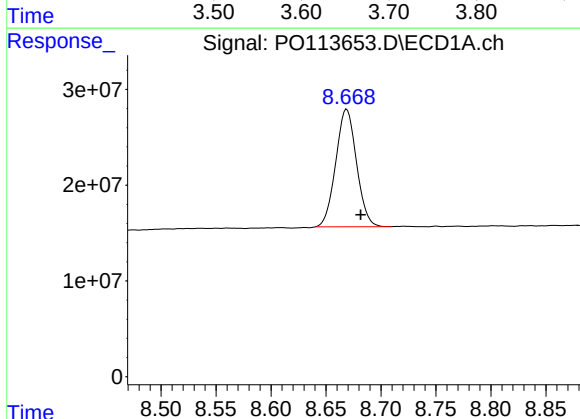


#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.013 min
Response: 161498489
Conc: 23.30 ng/ml

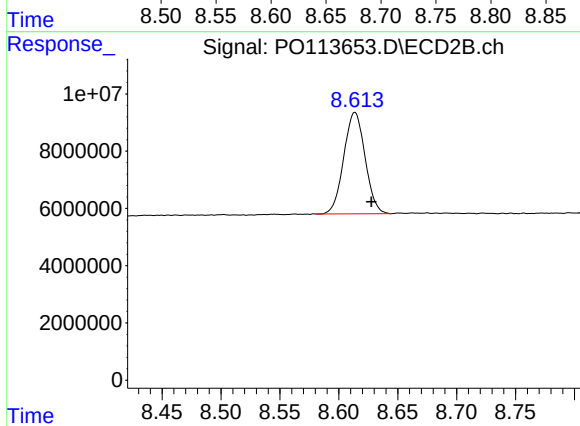

#2 Decachlorobiphenyl


R.T.: 8.614 min
Delta R.T.: -0.014 min
Response: 44676408
Conc: 23.58 ng/ml

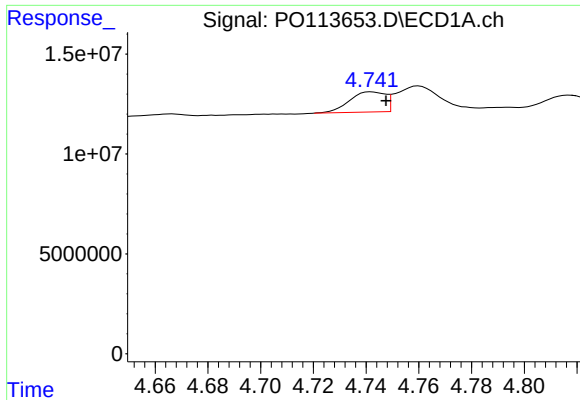

#3 AR-1016-1


R.T.: 4.742 min
Delta R.T.: -0.006 min
Response: 9557405
Conc: 35.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

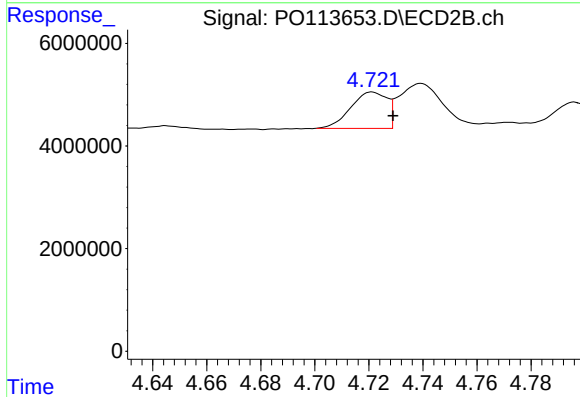


#3 AR-1016-1

R.T.: 4.721 min
Delta R.T.: -0.008 min
Response: 6632580
Conc: 38.88 ng/ml

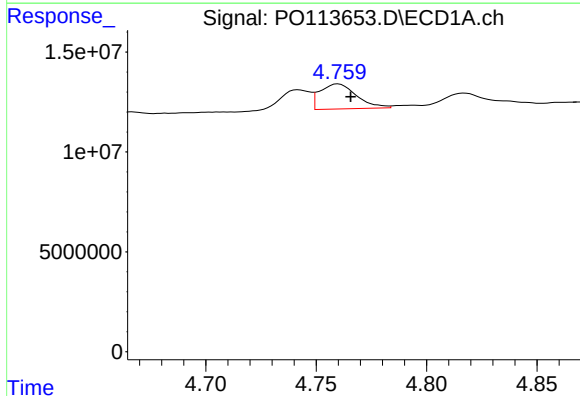


#4 AR-1016-2

R.T.: 4.760 min
Delta R.T.: -0.006 min
Response: 14463889
Conc: 36.03 ng/ml

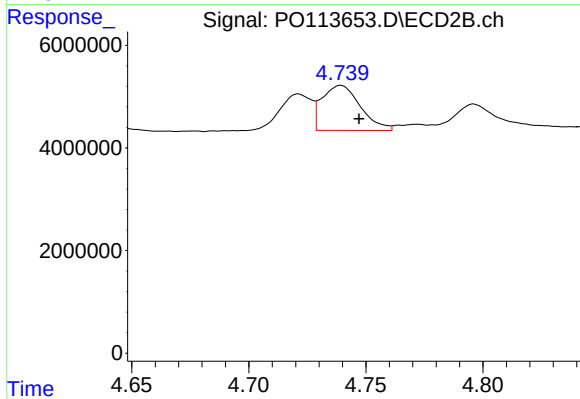

#4 AR-1016-2


R.T.: 4.739 min
Delta R.T.: -0.008 min
Response: 10035476
Conc: 38.95 ng/ml

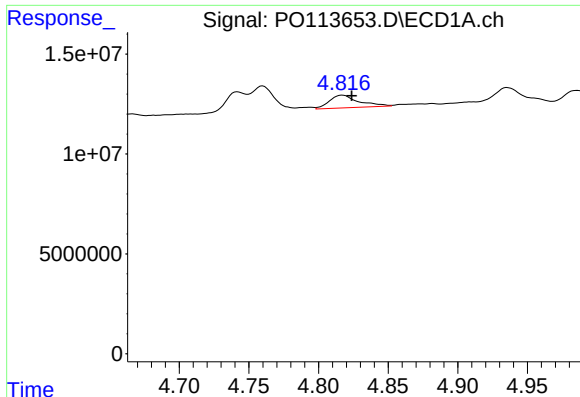

#5 AR-1016-3


R.T.: 4.817 min
Delta R.T.: -0.007 min
Response: 9331767
Conc: 36.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

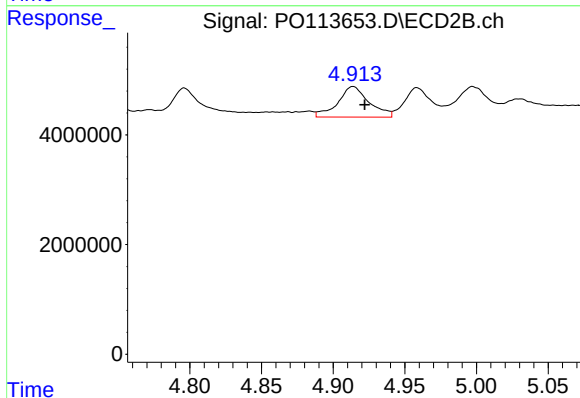


#5 AR-1016-3

R.T.: 4.914 min
Delta R.T.: -0.008 min
Response: 8471066
Conc: 60.67 ng/ml

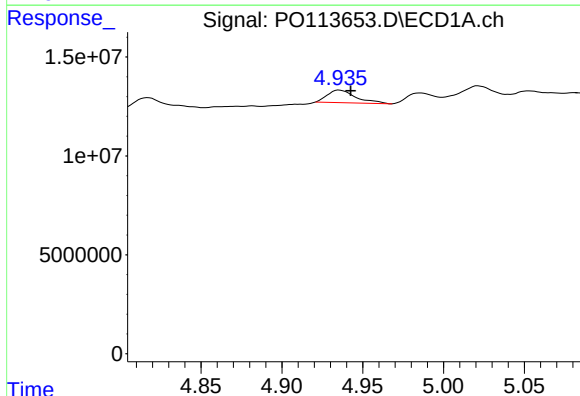


#6 AR-1016-4

R.T.: 4.935 min
Delta R.T.: -0.007 min
Response: 7783903
Conc: 35.69 ng/ml

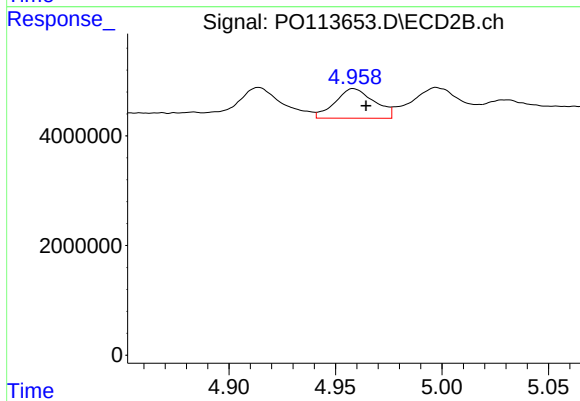

#6 AR-1016-4


R.T.: 4.958 min
Delta R.T.: -0.006 min
Response: 6926917
Conc: 59.36 ng/ml

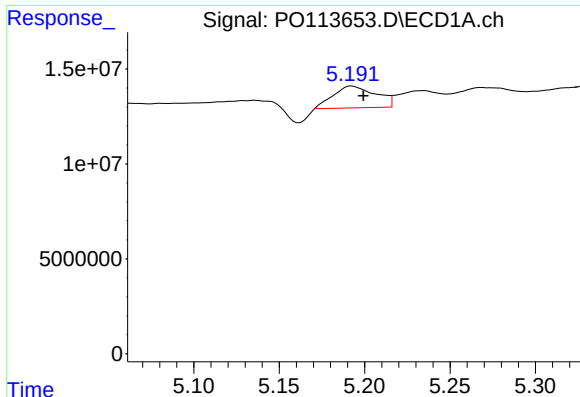

#7 AR-1016-5


R.T.: 5.192 min
Delta R.T.: -0.007 min
Response: 19925196
Conc: 89.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

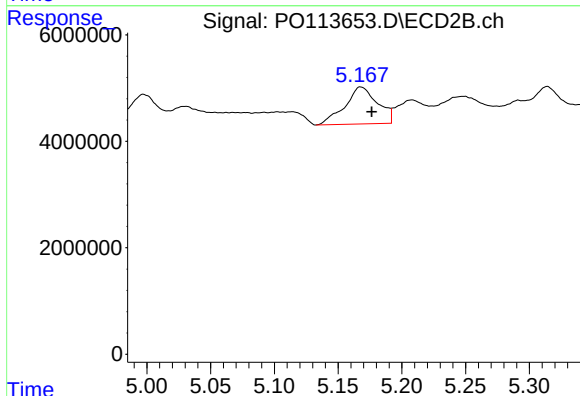


#7 AR-1016-5

R.T.: 5.168 min
Delta R.T.: -0.009 min
Response: 12383180
Conc: 86.88 ng/ml

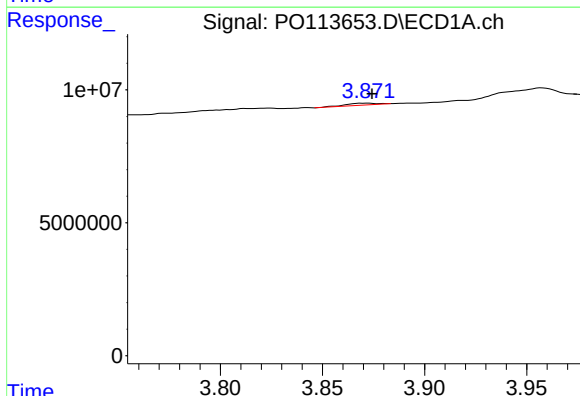


#8 AR-1221-1

R.T.: 3.872 min
Delta R.T.: -0.002 min
Response: 788245
Conc: 8.42 ng/ml

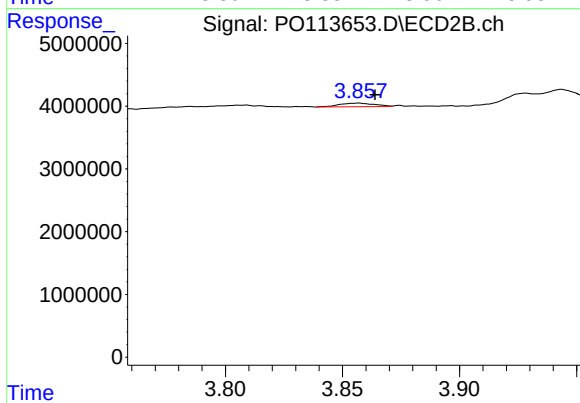

#8 AR-1221-1


R.T.: 3.857 min
Delta R.T.: -0.007 min
Response: 609001
Conc: 9.65 ng/ml

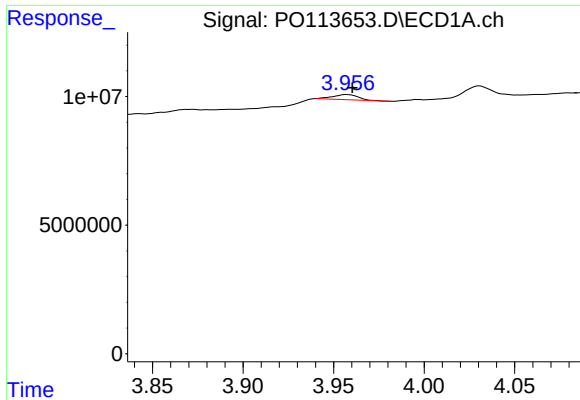

#9 AR-1221-2


R.T.: 3.957 min
Delta R.T.: -0.003 min
Response: 1972702
Conc: 29.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

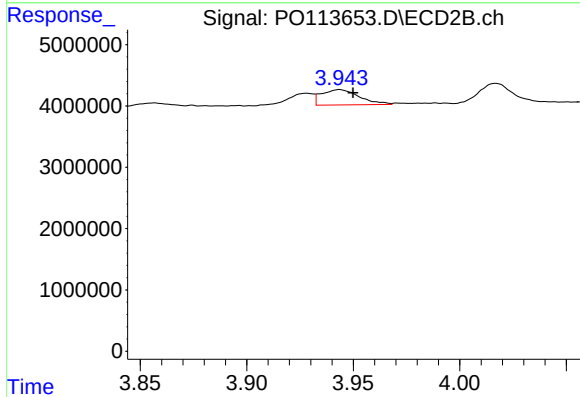


#9 AR-1221-2

R.T.: 3.944 min
Delta R.T.: -0.006 min
Response: 3086927
Conc: 66.14 ng/ml

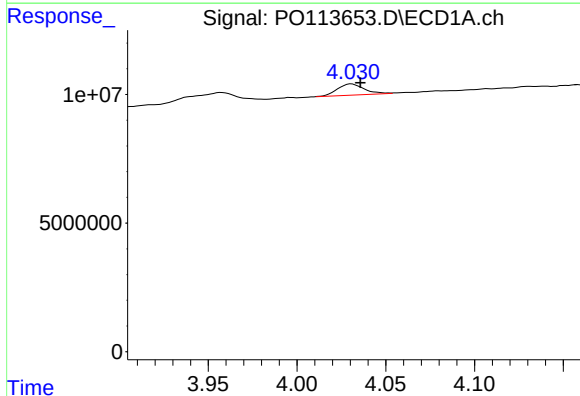


#10 AR-1221-3

R.T.: 4.031 min
Delta R.T.: -0.005 min
Response: 4569824
Conc: 20.65 ng/ml

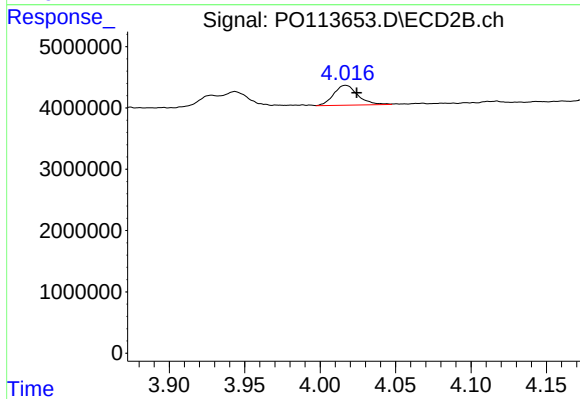

#10 AR-1221-3


R.T.: 4.017 min
Delta R.T.: -0.007 min
Response: 3618140
Conc: 24.37 ng/ml

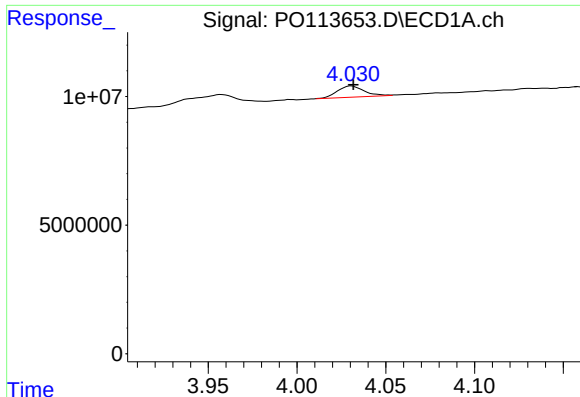

#11 AR-1232-1


R.T.: 4.031 min
Delta R.T.: -0.001 min
Response: 4569824
Conc: 25.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

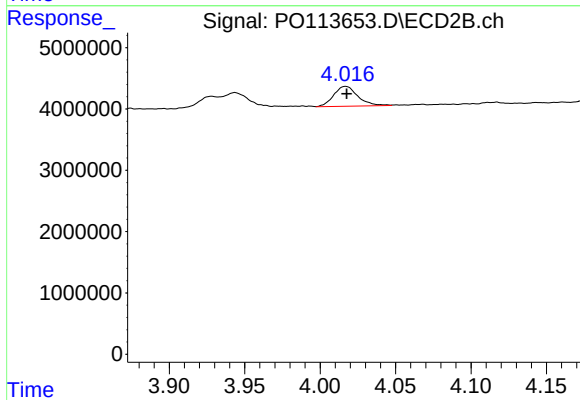


#11 AR-1232-1

R.T.: 4.017 min
Delta R.T.: 0.000 min
Response: 3618140
Conc: 29.92 ng/ml

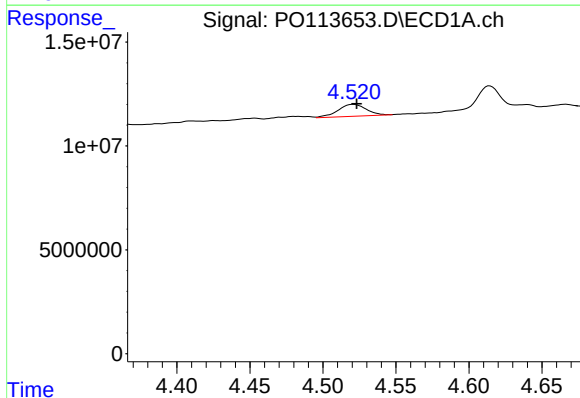


#12 AR-1232-2

R.T.: 4.521 min
Delta R.T.: -0.002 min
Response: 7676119
Conc: 71.13 ng/ml

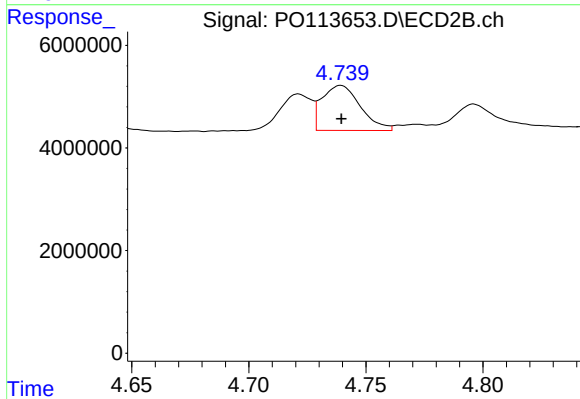

#12 AR-1232-2


R.T.: 4.739 min
Delta R.T.: 0.000 min
Response: 10035476
Conc: 82.22 ng/ml

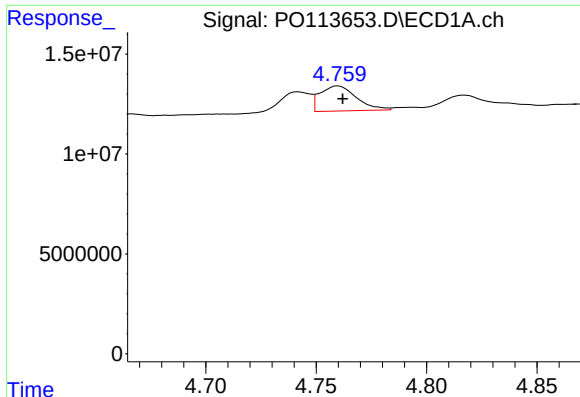

#13 AR-1232-3


R.T.: 4.760 min
Delta R.T.: -0.002 min
Response: 14463889
Conc: 73.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

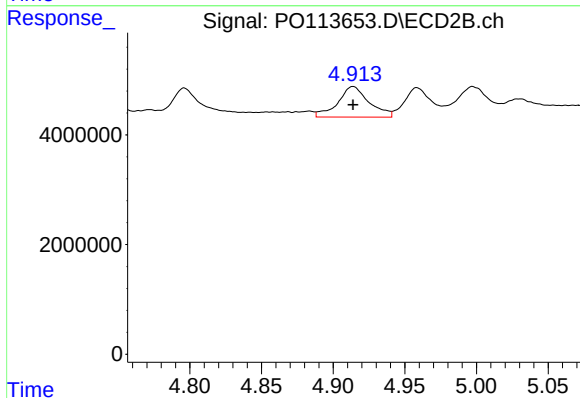


#13 AR-1232-3

R.T.: 4.914 min
Delta R.T.: 0.000 min
Response: 8471066
Conc: 128.05 ng/ml

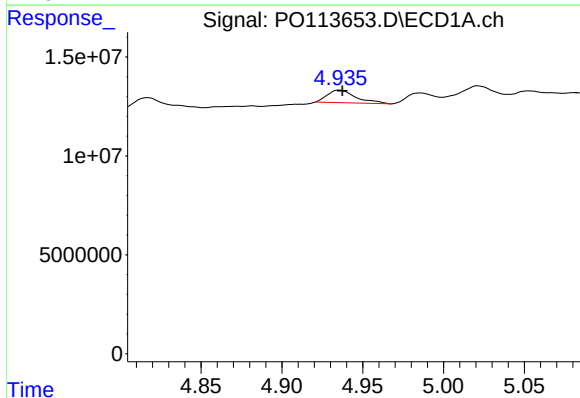


#14 AR-1232-4

R.T.: 4.935 min
Delta R.T.: -0.002 min
Response: 7783903
Conc: 79.19 ng/ml

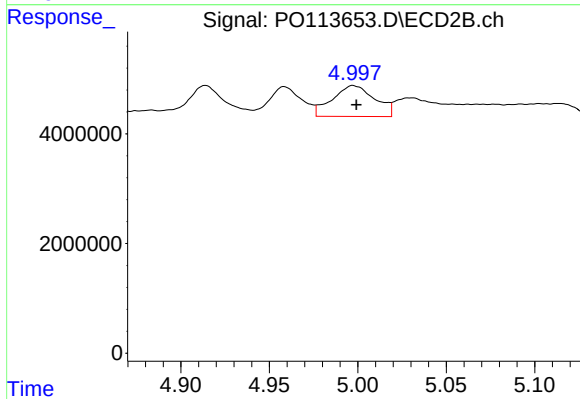

#14 AR-1232-4


R.T.: 4.997 min
Delta R.T.: -0.002 min
Response: 9455147
Conc: 157.77 ng/ml

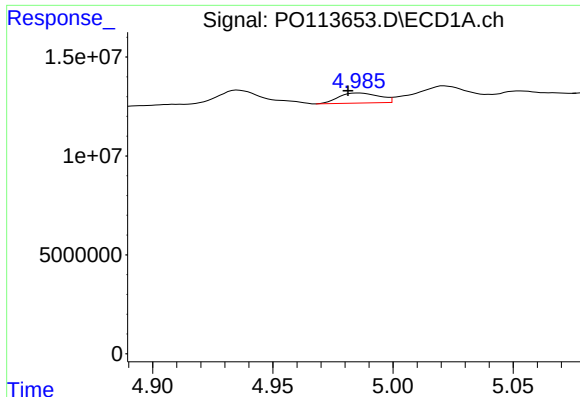

#15 AR-1232-5


R.T.: 4.986 min
Delta R.T.: 0.005 min
Response: 5871011
Conc: 89.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

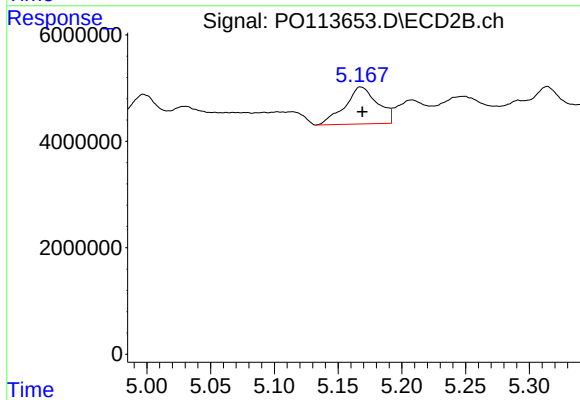


#15 AR-1232-5

R.T.: 5.168 min
Delta R.T.: -0.002 min
Response: 12383180
Conc: 183.14 ng/ml

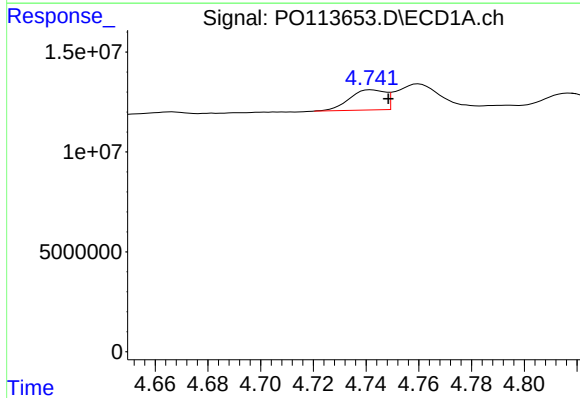


#16 AR-1242-1

R.T.: 4.742 min
Delta R.T.: -0.006 min
Response: 9557405
Conc: 41.57 ng/ml

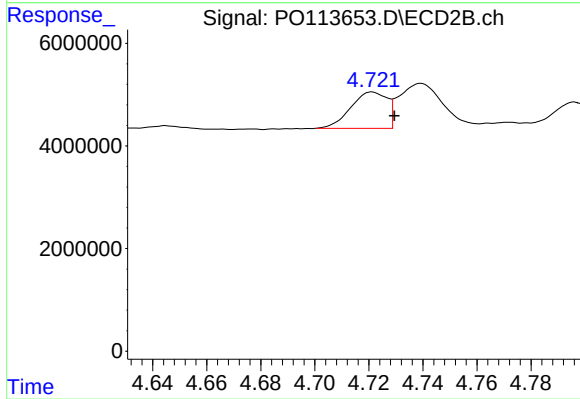

#16 AR-1242-1


R.T.: 4.721 min
Delta R.T.: -0.008 min
Response: 6632580
Conc: 45.90 ng/ml

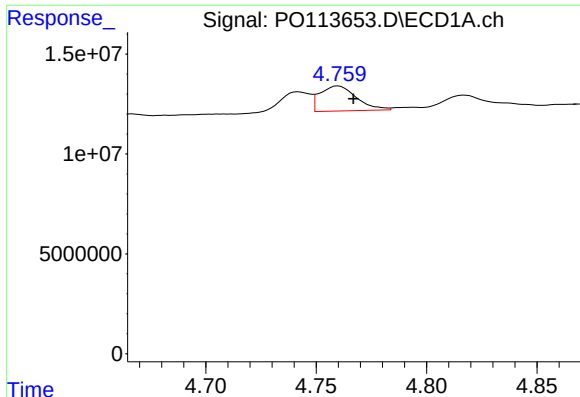

#17 AR-1242-2


R.T.: 4.760 min
Delta R.T.: -0.007 min
Response: 14463889
Conc: 42.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

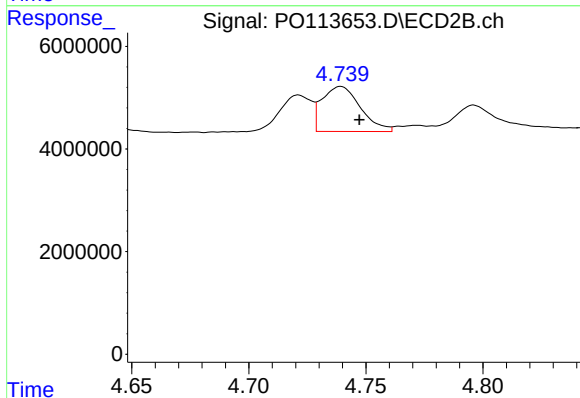


#17 AR-1242-2

R.T.: 4.739 min
Delta R.T.: -0.008 min
Response: 10035476
Conc: 46.27 ng/ml

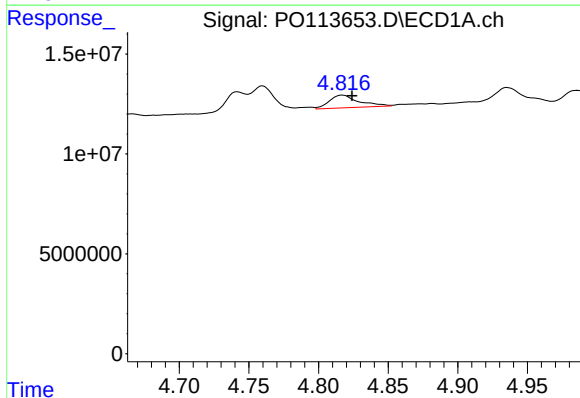


#18 AR-1242-3

R.T.: 4.817 min
Delta R.T.: -0.007 min
Response: 9331767
Conc: 42.06 ng/ml

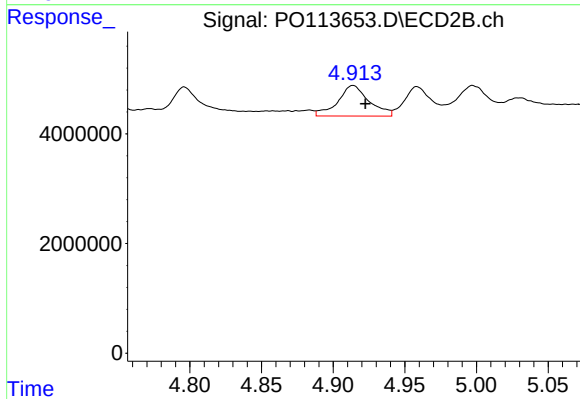

#18 AR-1242-3


R.T.: 4.914 min
Delta R.T.: -0.009 min
Response: 8471066
Conc: 72.42 ng/ml

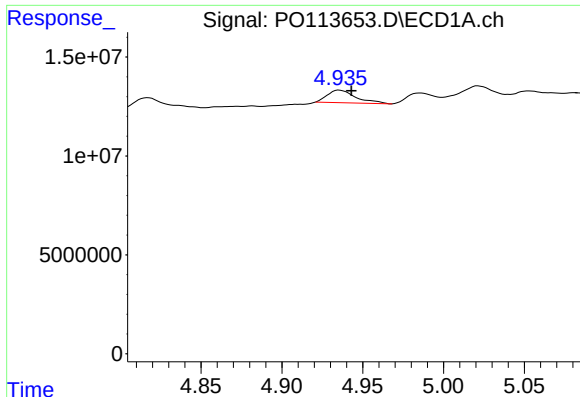

#19 AR-1242-4


R.T.: 4.935 min
Delta R.T.: -0.008 min
Response: 7783903
Conc: 44.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

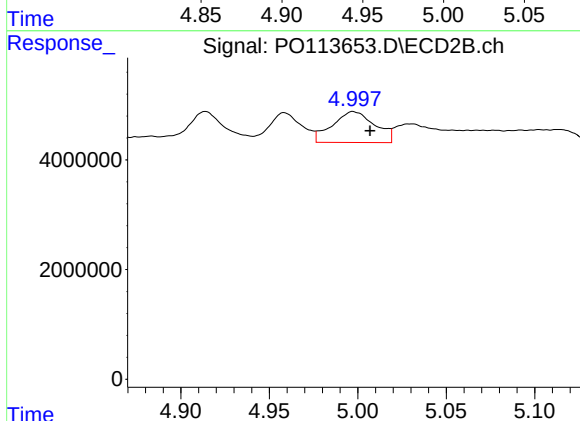


#19 AR-1242-4

R.T.: 4.997 min
Delta R.T.: -0.010 min
Response: 9455147
Conc: 80.38 ng/ml

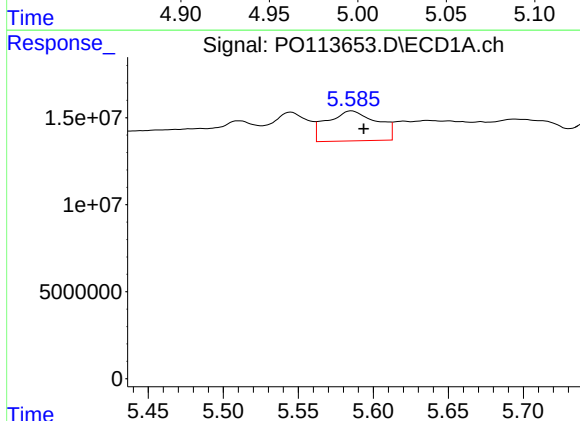


#20 AR-1242-5

R.T.: 5.586 min
Delta R.T.: -0.008 min
Response: 39888877
Conc: 199.28 ng/ml

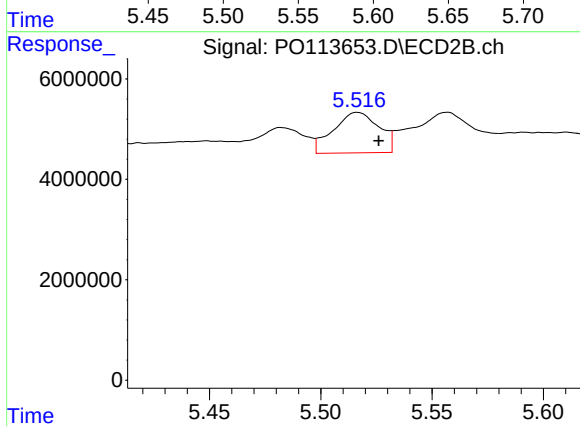

#20 AR-1242-5


R.T.: 5.516 min
Delta R.T.: -0.010 min
Response: 11479190
Conc: 76.97 ng/ml

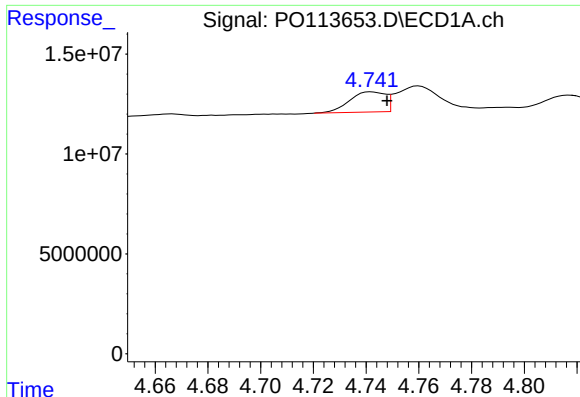

#21 AR-1248-1


R.T.: 4.742 min
Delta R.T.: -0.006 min
Response: 9557405
Conc: 54.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

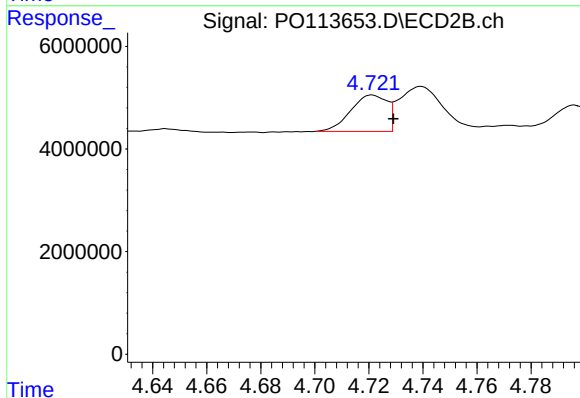


#21 AR-1248-1

R.T.: 4.721 min
Delta R.T.: -0.008 min
Response: 6632580
Conc: 59.48 ng/ml

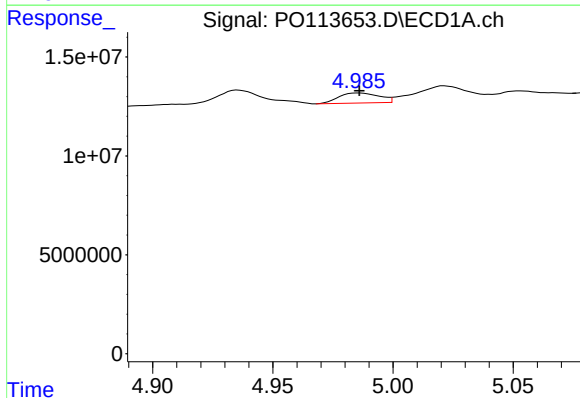


#22 AR-1248-2

R.T.: 4.986 min
Delta R.T.: 0.000 min
Response: 5871011
Conc: 24.27 ng/ml

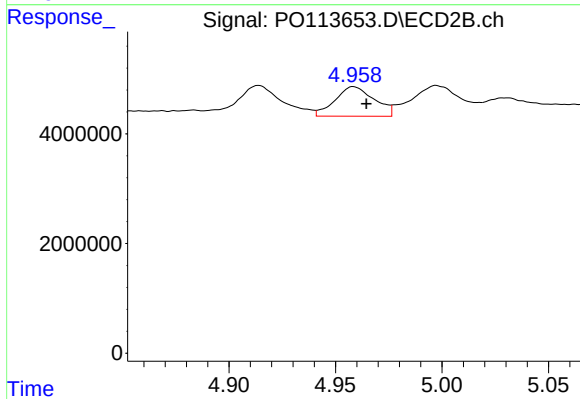

#22 AR-1248-2


R.T.: 4.958 min
Delta R.T.: -0.006 min
Response: 6926917
Conc: 43.10 ng/ml

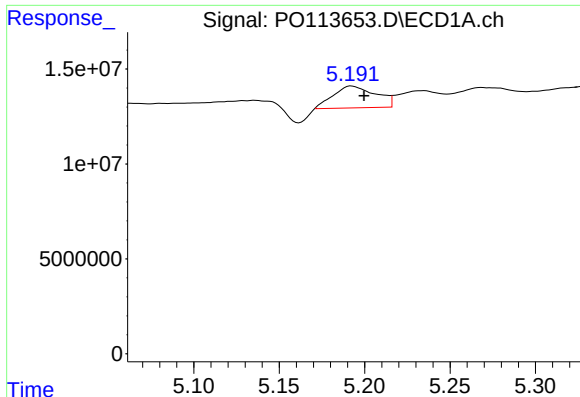

#23 AR-1248-3


R.T.: 5.192 min
Delta R.T.: -0.007 min
Response: 19925196
Conc: 62.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

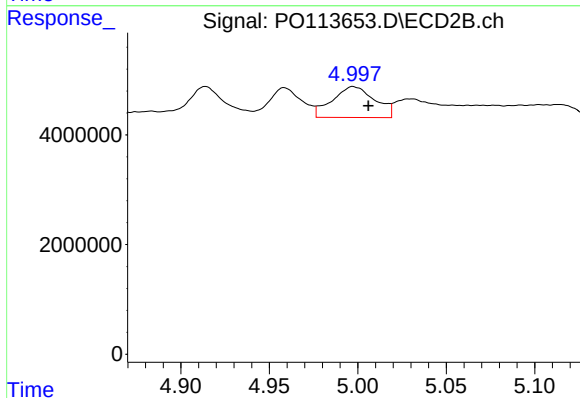


#23 AR-1248-3

R.T.: 4.997 min
Delta R.T.: -0.009 min
Response: 9455147
Conc: 55.73 ng/ml

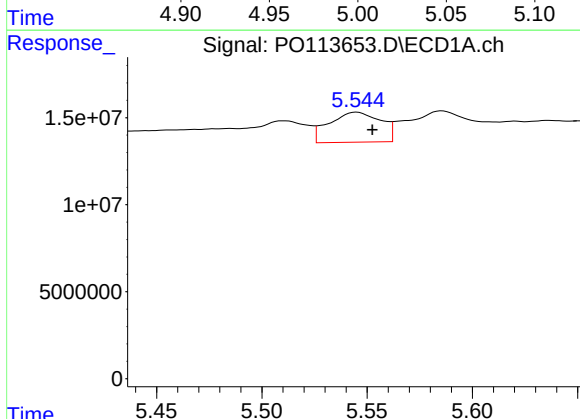


#24 AR-1248-4

R.T.: 5.545 min
Delta R.T.: -0.007 min
Response: 29447354
Conc: 58.94 ng/ml

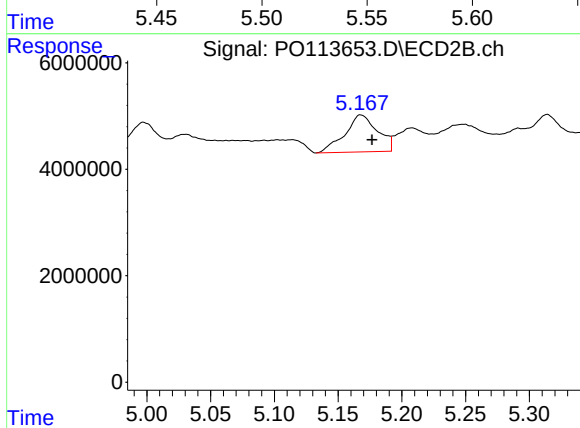

#24 AR-1248-4


R.T.: 5.168 min
Delta R.T.: -0.009 min
Response: 12383180
Conc: 62.16 ng/ml

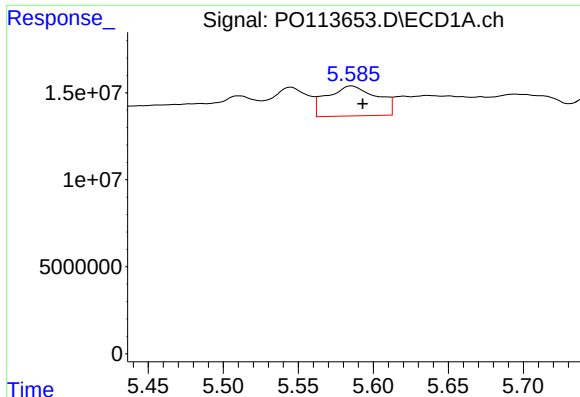

#25 AR-1248-5


R.T.: 5.586 min
Delta R.T.: -0.007 min
Response: 39888877
Conc: 116.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

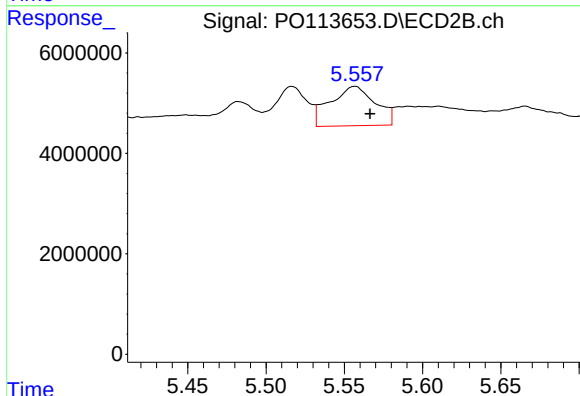


#25 AR-1248-5

R.T.: 5.557 min
Delta R.T.: -0.010 min
Response: 15712432
Conc: 74.01 ng/ml

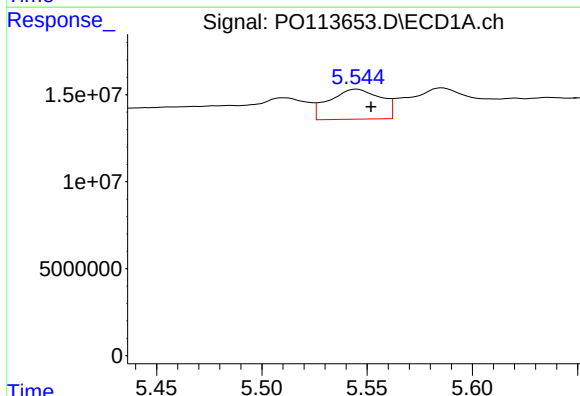


#26 AR-1254-1

R.T.: 5.545 min
Delta R.T.: -0.007 min
Response: 29447354
Conc: 54.53 ng/ml

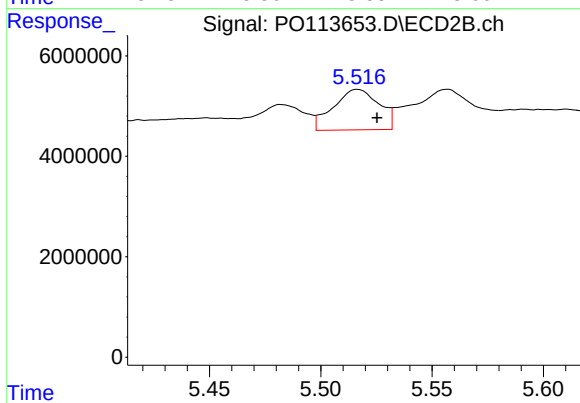

#26 AR-1254-1


R.T.: 5.516 min
Delta R.T.: -0.009 min
Response: 11479190
Conc: 36.40 ng/ml

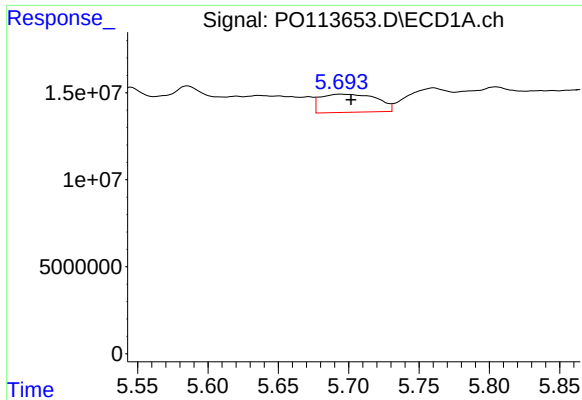

#27 AR-1254-2


R.T.: 5.694 min
Delta R.T.: -0.008 min
Response: 28986077
Conc: 58.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

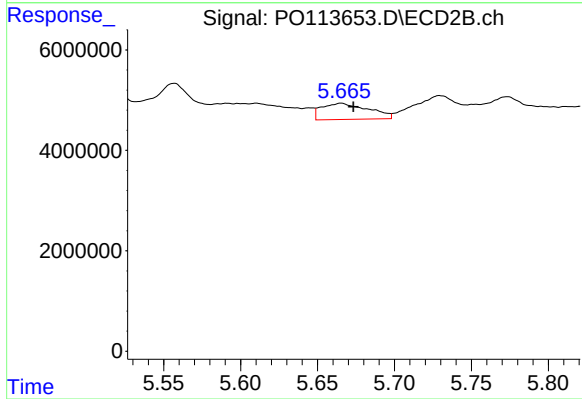


#27 AR-1254-2

R.T.: 5.666 min
Delta R.T.: -0.008 min
Response: 6807062
Conc: 24.28 ng/ml

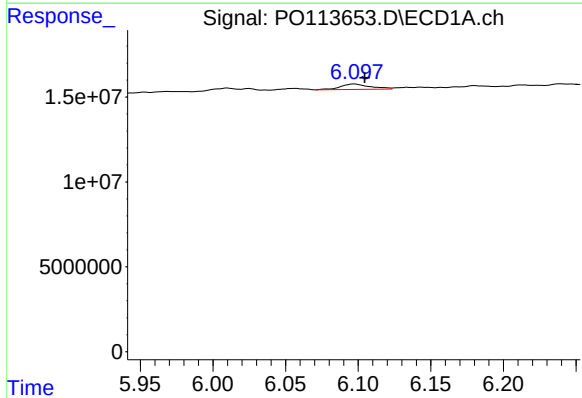


#28 AR-1254-3

R.T.: 6.097 min
Delta R.T.: -0.007 min
Response: 4500468
Conc: 6.09 ng/ml

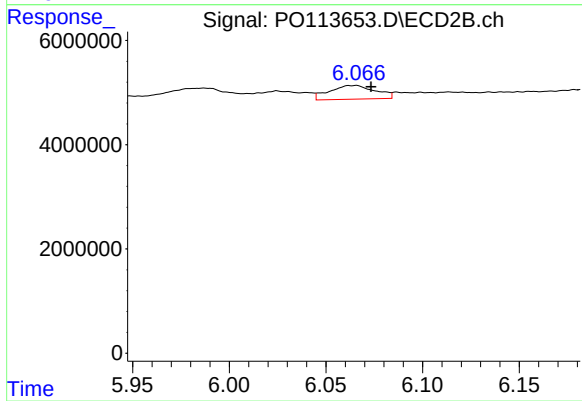

#28 AR-1254-3


R.T.: 6.062 min
Delta R.T.: -0.011 min
Response: 4335138
Conc: 10.40 ng/ml

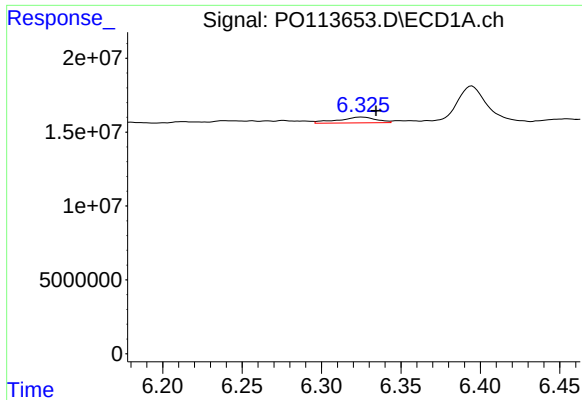

#29 AR-1254-4


R.T.: 6.325 min
Delta R.T.: -0.009 min
Response: 6517544
Conc: 11.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

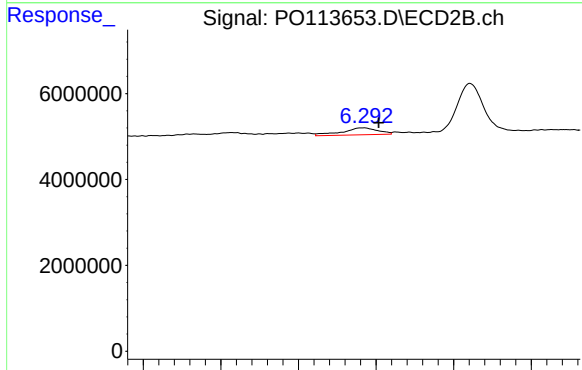


#29 AR-1254-4

R.T.: 6.292 min
Delta R.T.: -0.009 min
Response: 2558014
Conc: 9.31 ng/ml

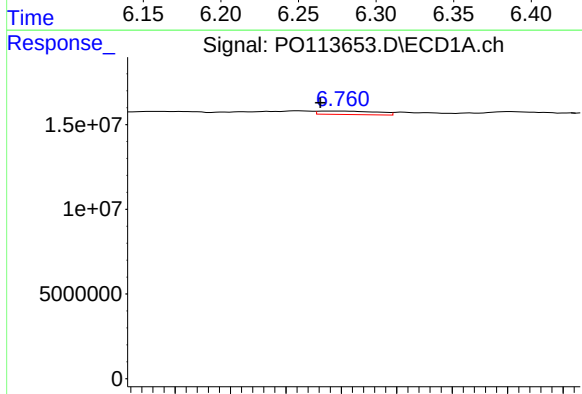


#30 AR-1254-5

R.T.: 6.759 min
Delta R.T.: 0.007 min
Response: 2987736
Conc: 4.26 ng/ml

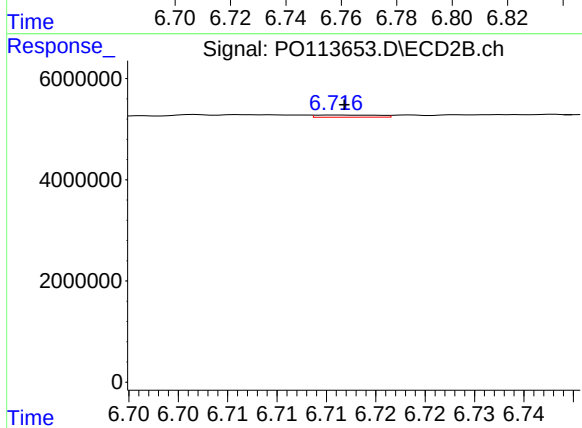

#30 AR-1254-5


R.T.: 6.716 min
Delta R.T.: 0.000 min
Response: 189450
Conc: 0.53 ng/ml

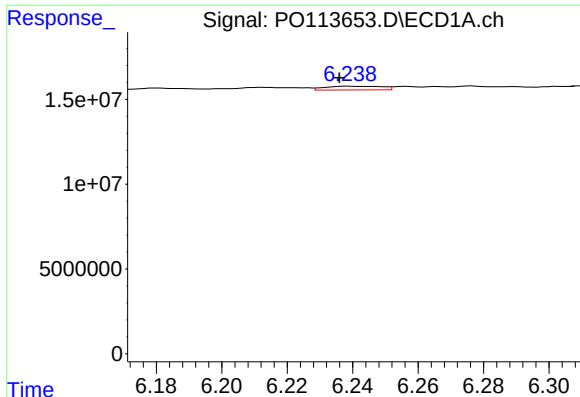

#31 AR-1260-1


R.T.: 6.239 min
Delta R.T.: 0.003 min
Response: 2630447
Conc: 5.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

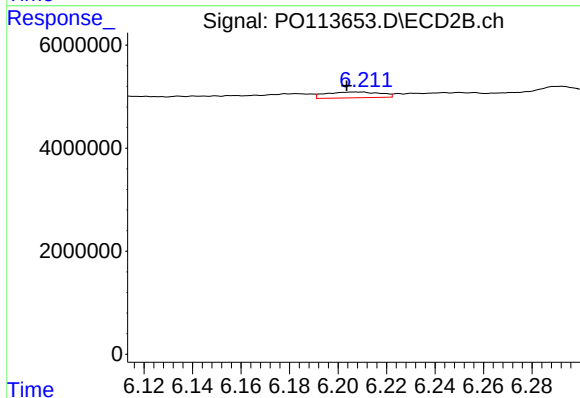


#31 AR-1260-1

R.T.: 6.207 min
Delta R.T.: 0.004 min
Response: 1748588
Conc: 6.86 ng/ml

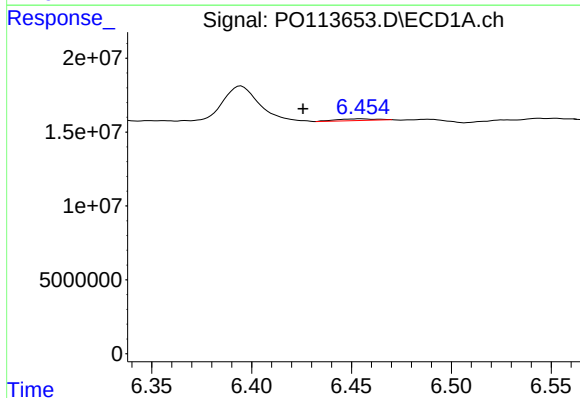


#32 AR-1260-2

R.T.: 6.455 min
Delta R.T.: 0.029 min
Response: 1654202
Conc: 2.41 ng/ml

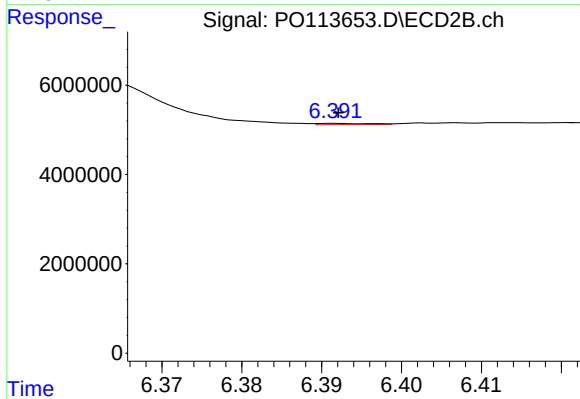

#32 AR-1260-2


R.T.: 6.392 min
Delta R.T.: 0.000 min
Response: 128509
Conc: 0.37 ng/ml

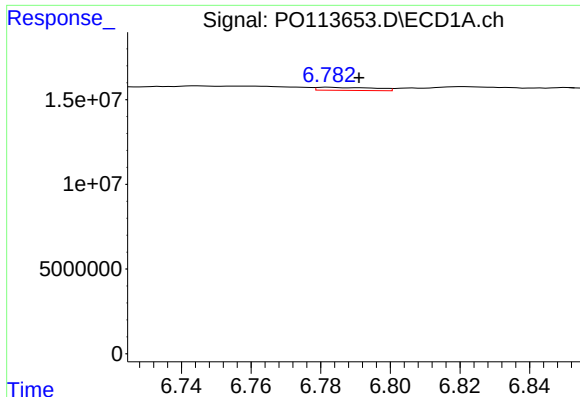

#33 AR-1260-3


R.T.: 6.782 min
Delta R.T.: -0.009 min
Response: 2012658
Conc: 3.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

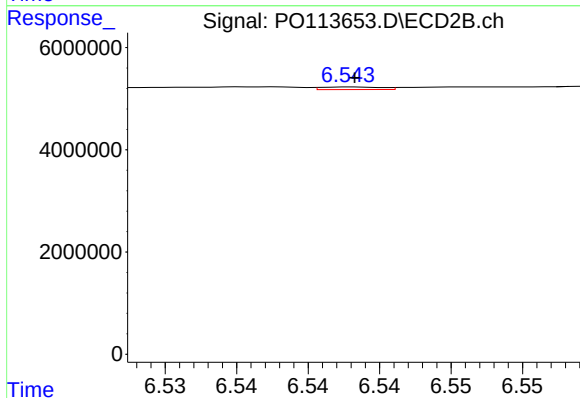


#33 AR-1260-3

R.T.: 6.543 min
Delta R.T.: 0.000 min
Response: 146410
Conc: 0.49 ng/ml

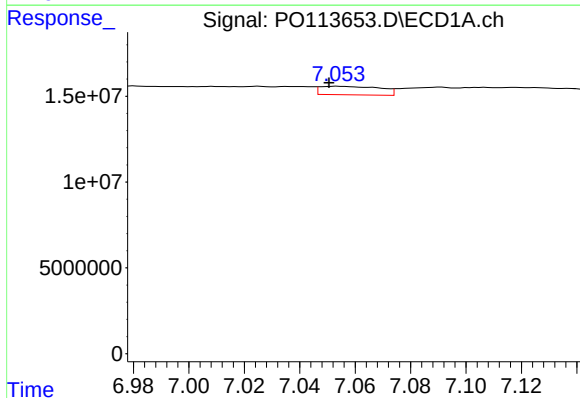


#34 AR-1260-4

R.T.: 7.054 min
Delta R.T.: 0.003 min
Response: 7459037
Conc: 16.65 ng/ml

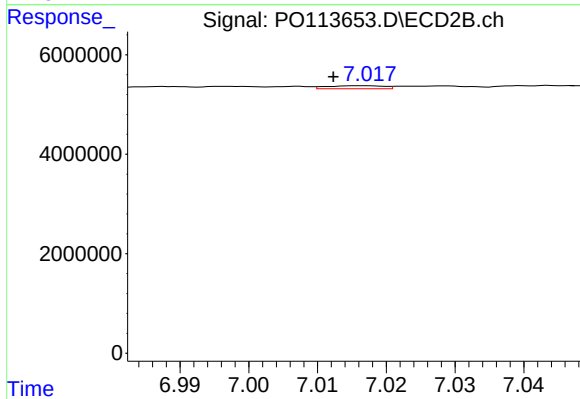

#34 AR-1260-4


R.T.: 7.017 min
Delta R.T.: 0.005 min
Response: 348663
Conc: 1.68 ng/ml

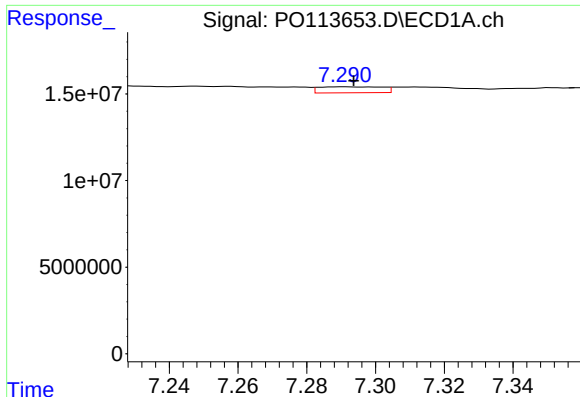

#35 AR-1260-5


R.T.: 7.291 min
Delta R.T.: -0.002 min
Response: 4456978
Conc: 3.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

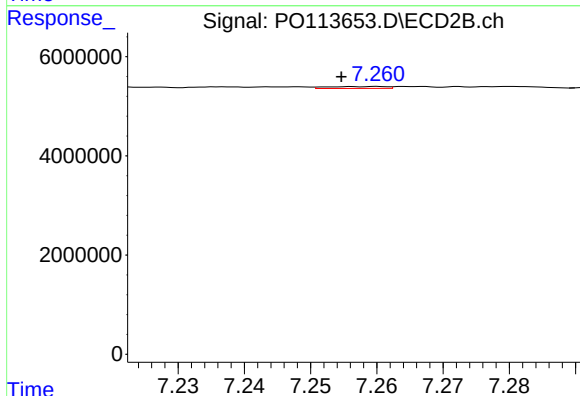


#35 AR-1260-5

R.T.: 7.260 min
Delta R.T.: 0.006 min
Response: 247177
Conc: 0.53 ng/ml

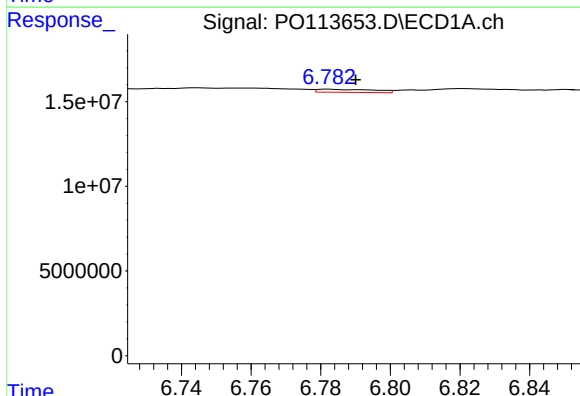


#36 AR-1262-1

R.T.: 6.782 min
Delta R.T.: -0.008 min
Response: 2012658
Conc: 2.20 ng/ml

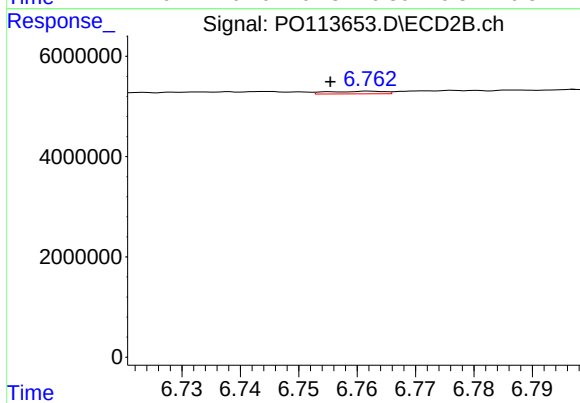

#36 AR-1262-1


R.T.: 6.762 min
Delta R.T.: 0.007 min
Response: 342705
Conc: 0.83 ng/ml

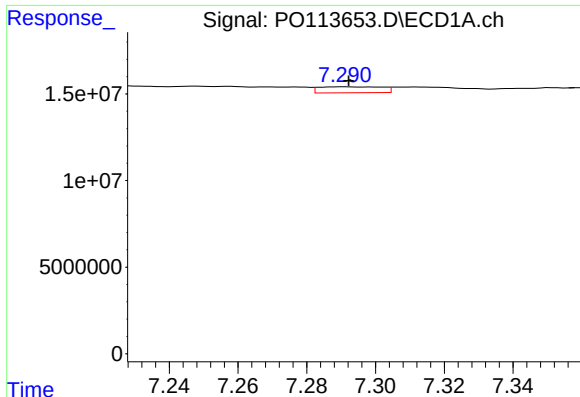

#37 AR-1262-2


R.T.: 7.291 min
Delta R.T.: 0.000 min
Response: 4456978
Conc: 2.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

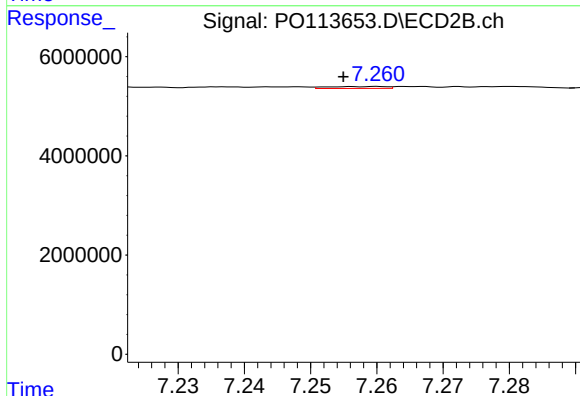


#37 AR-1262-2

R.T.: 7.260 min
Delta R.T.: 0.005 min
Response: 247177
Conc: 0.48 ng/ml

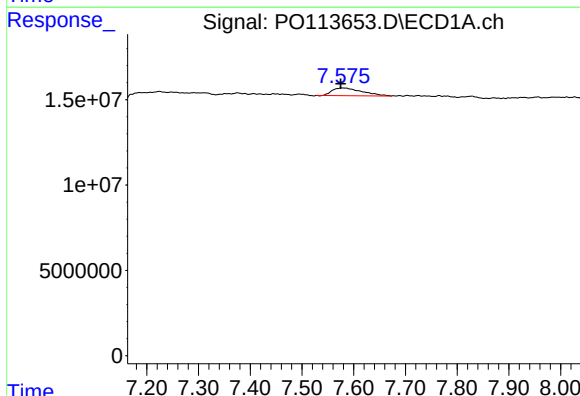


#38 AR-1262-3

R.T.: 7.577 min
Delta R.T.: 0.002 min
Response: 18484879
Conc: 33.36 ng/ml

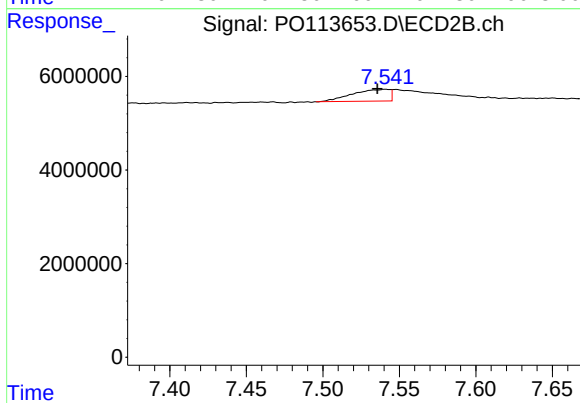

#38 AR-1262-3


R.T.: 7.541 min
Delta R.T.: 0.005 min
Response: 4288533
Conc: 23.88 ng/ml

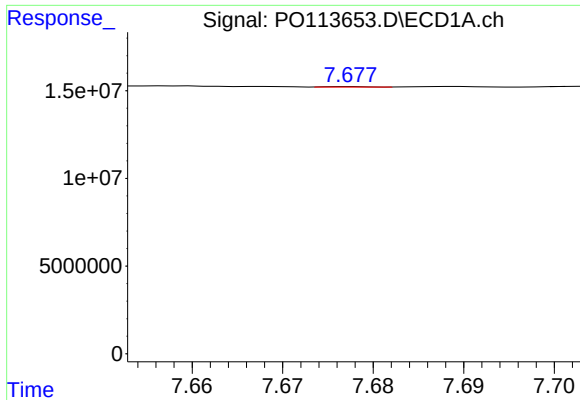

#39 AR-1262-4


R.T.: 7.677 min
Delta R.T.: 0.038 min
Response: 78084
Conc: 0.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

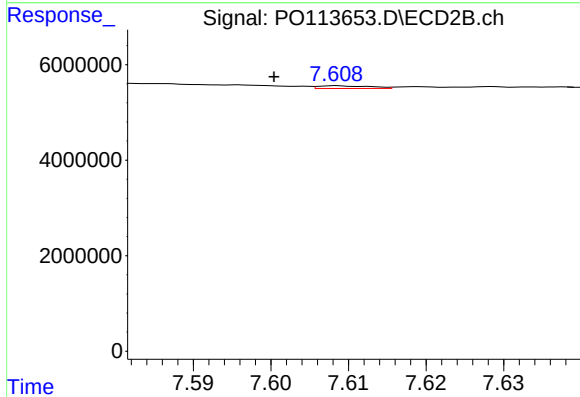


#39 AR-1262-4

R.T.: 7.608 min
Delta R.T.: 0.008 min
Response: 265721
Conc: 0.92 ng/ml

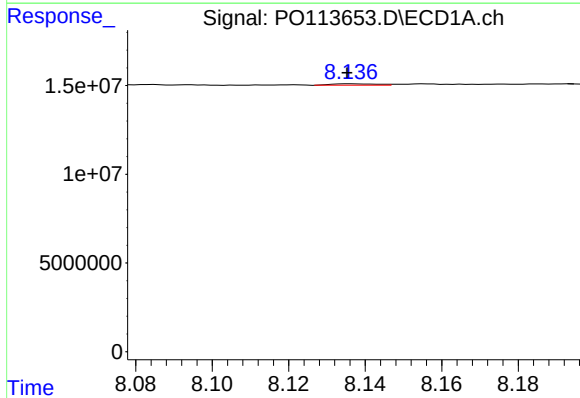


#40 AR-1262-5

R.T.: 8.136 min
Delta R.T.: 0.001 min
Response: 628122
Conc: 1.51 ng/ml

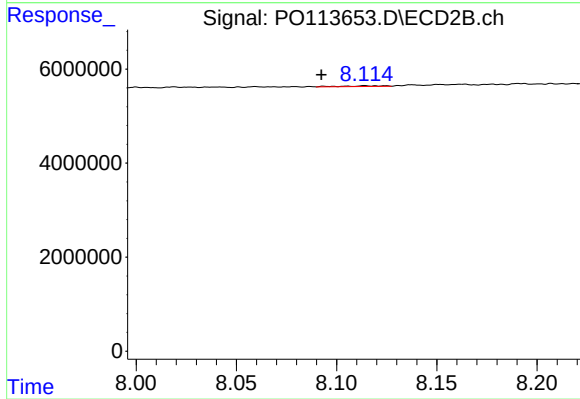

#40 AR-1262-5


R.T.: 8.114 min
Delta R.T.: 0.022 min
Response: 189538
Conc: 1.75 ng/ml

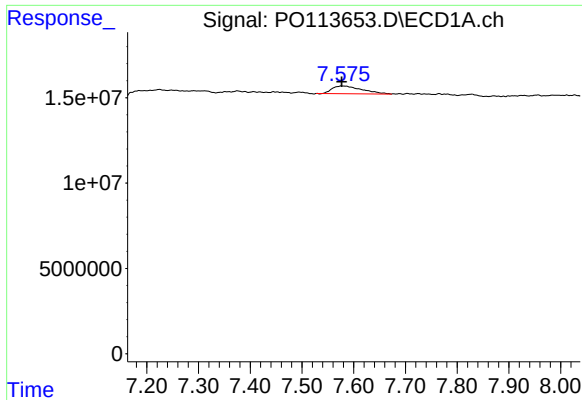

#41 AR-1268-1


R.T.: 7.577 min
Delta R.T.: 0.000 min
Response: 18484879
Conc: 10.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

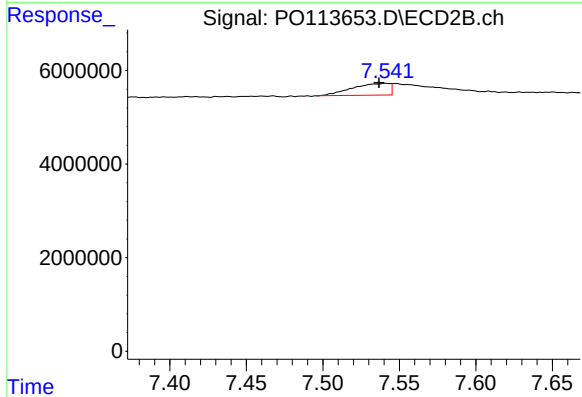


#41 AR-1268-1

R.T.: 7.541 min
Delta R.T.: 0.004 min
Response: 4288533
Conc: 8.42 ng/ml

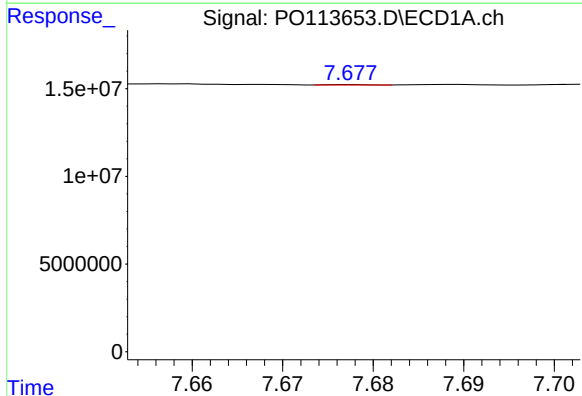


#42 AR-1268-2

R.T.: 7.677 min
Delta R.T.: 0.035 min
Response: 78084
Conc: 0.05 ng/ml

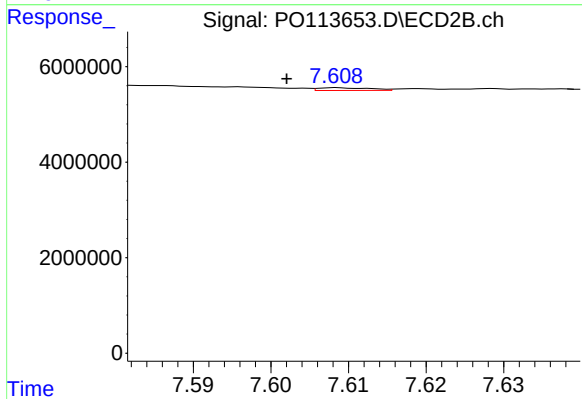

#42 AR-1268-2


R.T.: 7.608 min
Delta R.T.: 0.006 min
Response: 265721
Conc: 0.64 ng/ml

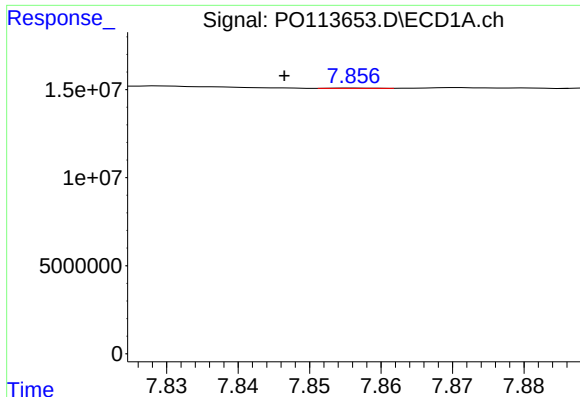

#43 AR-1268-3


R.T.: 7.856 min
Delta R.T.: 0.010 min
Response: 64442
Conc: 0.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

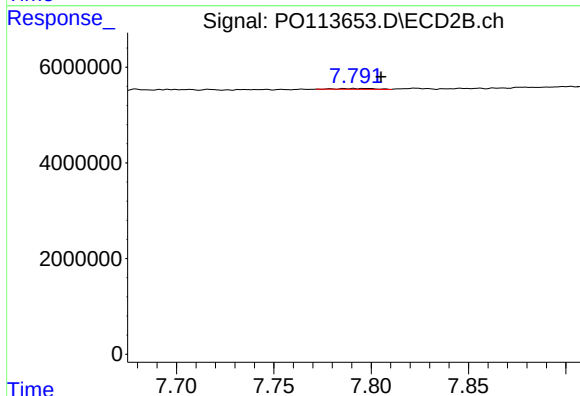


#43 AR-1268-3

R.T.: 7.791 min
Delta R.T.: -0.014 min
Response: 226087
Conc: 0.69 ng/ml

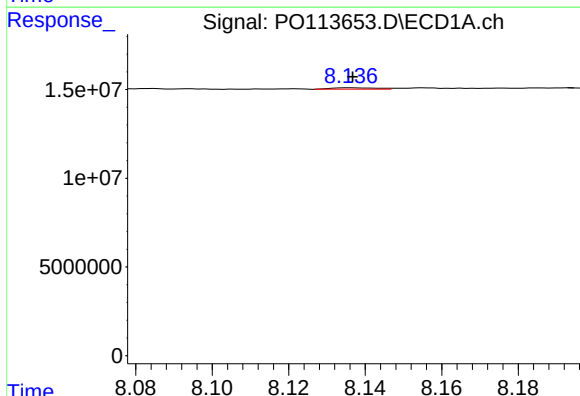


#44 AR-1268-4

R.T.: 8.136 min
Delta R.T.: 0.000 min
Response: 628122
Conc: 1.36 ng/ml

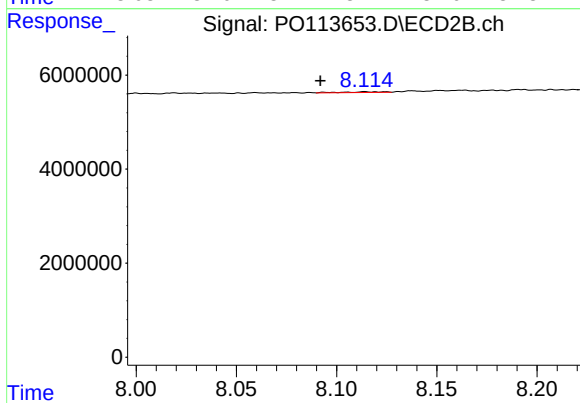

#44 AR-1268-4


R.T.: 8.114 min
Delta R.T.: 0.022 min
Response: 189538
Conc: 1.57 ng/ml

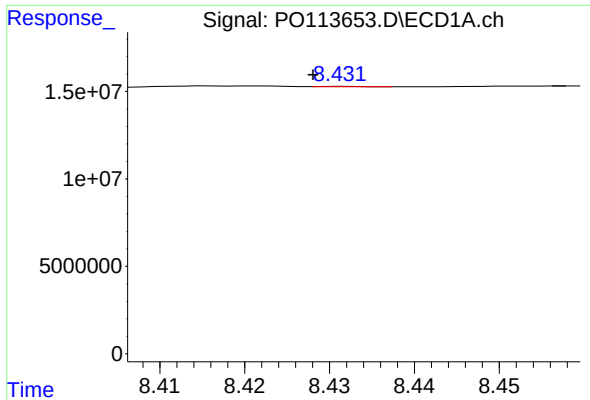

#45 AR-1268-5

R.T.: 8.431 min
Delta R.T.: 0.003 min
Response: 82836
Conc: 0.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

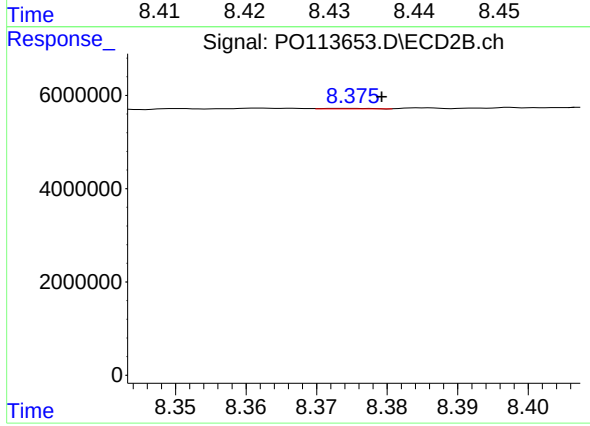

#45 AR-1268-5

R.T.: 8.375 min
Delta R.T.: -0.005 min
Response: 42183
Conc: 0.05 ng/ml