

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091125\
 Data File : P0113654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 11:53
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1248 40PPB WATER MDL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 02:10:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.658	3.649	182.8E6	108.5E6	22.331	21.434
2)	SA Decachlor...	8.668	8.614	161.1E6	45296072	23.238	23.905
Target Compounds							
3)	L1 AR-1016-1	4.741	4.721	6819156	4490446	25.541	26.326
4)	L1 AR-1016-2	4.759	4.738	7135788	5266623	17.776	20.441
5)	L1 AR-1016-3	4.816	4.914	4232061	5369858	16.595	38.462 #
6)	L1 AR-1016-4	4.937	4.956	4748271	9051792	21.774	77.565 #
7)	L1 AR-1016-5	5.192	5.167	20518612	13680944	92.581	95.986
8)	L2 AR-1221-1	0.000	3.868	0	79850	N.D.	1.265 #
9)	L2 AR-1221-2	3.958	3.945	1886242	2586972	27.923	55.427 #
10)	L2 AR-1221-3	4.038	4.017	506513	440357	2.288	2.966 #
11)	L3 AR-1232-1	4.038	4.017	506513	440357	2.821	3.641 #
12)	L3 AR-1232-2	4.521	4.738	3452937	5266623	31.996	43.151 #
13)	L3 AR-1232-3	4.759	4.914	7135788	5369858	36.150	81.170 #
14)	L3 AR-1232-4	4.937	4.997	4748271	9995212	48.307	166.786 #
15)	L3 AR-1232-5	4.981	5.167	7983209	13680944	121.358	202.333 #
16)	L4 AR-1242-1	4.741	4.721	6819156	4490446	29.657	31.075
17)	L4 AR-1242-2	4.759	4.738	7135788	5266623	20.766	24.280
18)	L4 AR-1242-3	4.816	4.914	4232061	5369858	19.073	45.910 #
19)	L4 AR-1242-4	4.937	4.997	4748271	9995212	27.373	84.966 #
20)	L4 AR-1242-5	5.585	5.516	34317195	16376649	171.447	109.812 #
21)	L5 AR-1248-1	4.741	4.721	6819156	4490446	39.086	40.269
22)	L5 AR-1248-2	4.981	4.956	7983209	9051792	33.007	56.328 #
23)	L5 AR-1248-3	5.192	4.997	20518612	9995212	64.349	58.913
24)	L5 AR-1248-4	5.544	5.167	35441165	13680944	70.938	68.673
25)	L5 AR-1248-5	5.585	5.556	34317195	14916949	100.492	70.265 #
26)	L6 AR-1254-1	5.544	5.516	35441165	16376649	65.634	51.931
27)	L6 AR-1254-2	5.693	5.664	28321854	7979888	57.395	28.465 #
28)	L6 AR-1254-3	6.096	6.063	8932417	5938983	12.089	14.245
29)	L6 AR-1254-4	6.325	6.310	9204871	60558	16.526	0.220 #
30)	L6 AR-1254-5	6.744	6.713	3040977	309782	4.338	0.867 #
31)	L7 AR-1260-1	6.241	6.208	8214162	2325272	18.418	9.116 #
32)	L7 AR-1260-2	6.394	6.397	21773046	93837	31.706	0.271 #
33)	L7 AR-1260-3	6.780	6.544	2947383	205517	4.773	0.691 #
34)	L7 AR-1260-4	7.050	7.015	6683028	352928	14.922	1.703 #
35)	L7 AR-1260-5	7.298	7.262	2687860	480038	2.220	1.025 #
36)	L8 AR-1262-1	6.780	6.761	2947383	286973	3.218	0.692 #
37)	L8 AR-1262-2	7.298	7.262	2687860	480038	1.778	0.927 #
38)	L8 AR-1262-3	7.570	7.528	3850868	1395285	6.950	7.769
39)	L8 AR-1262-4	7.617	7.614	3463886	195698	3.542	0.675 #
40)	L8 AR-1262-5	8.139	8.089	753049	43166	1.806	0.398 #
41)	L9 AR-1268-1	7.583	7.544	4196129	1277754	2.438	2.508

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091125\
Data File : P0113654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 11:53
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1248 40PPB WATER MDL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:10:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.617	7.614	3463886	195698	2.392	0.471 #
43)	L9 AR-1268-3	7.832	7.805	1004964	11924	0.833	0.037 #
44)	L9 AR-1268-4	8.139	8.089	753049	43166	1.635	0.358 #
45)	L9 AR-1268-5	8.434	8.381	248676	70816	0.078	0.091



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091125\
Data File : PO113654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 11:53
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1248 40PPB WATER MDL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:10:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

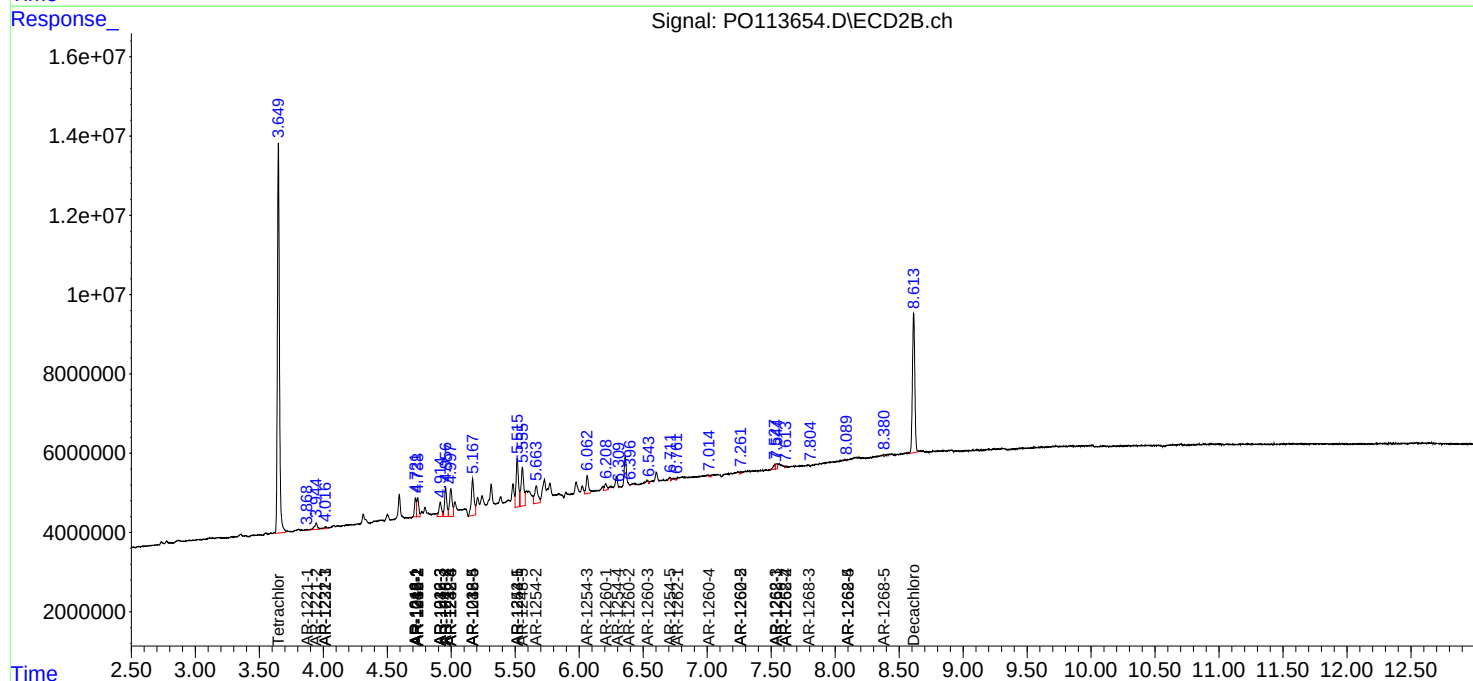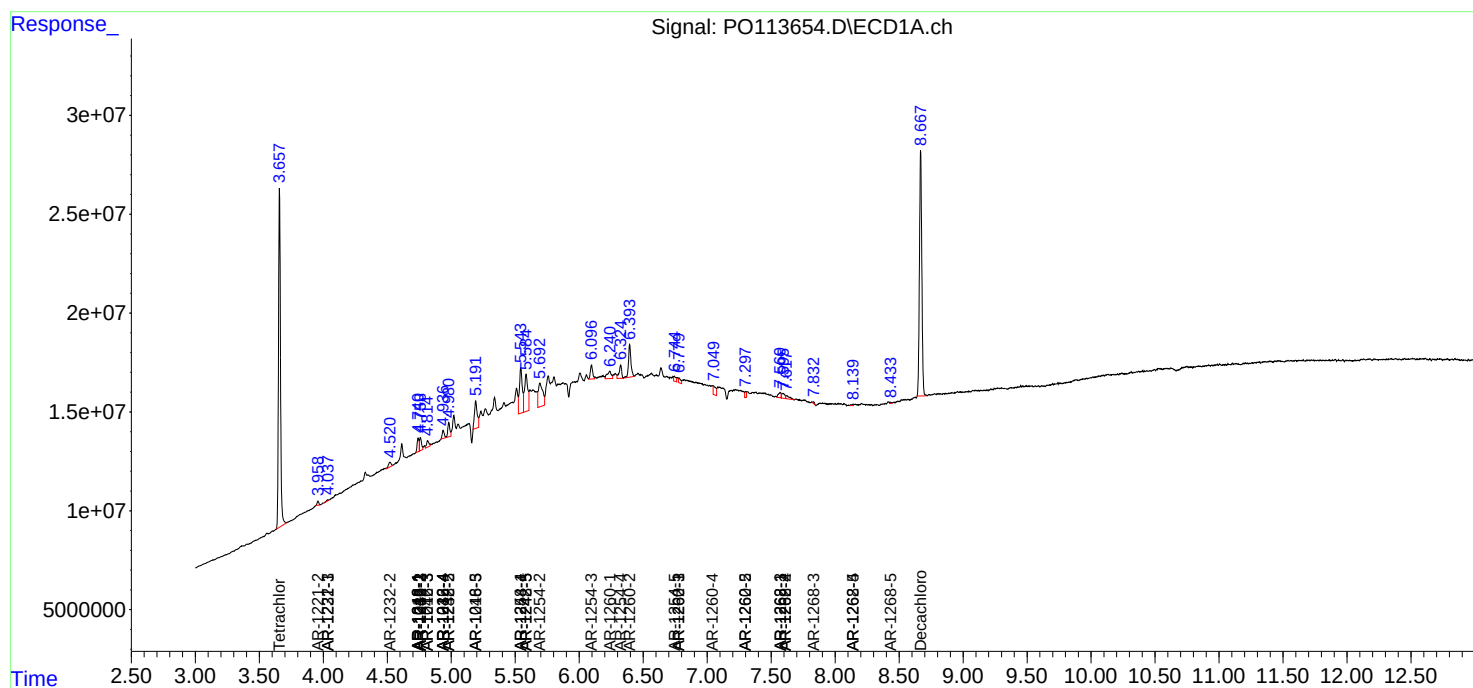


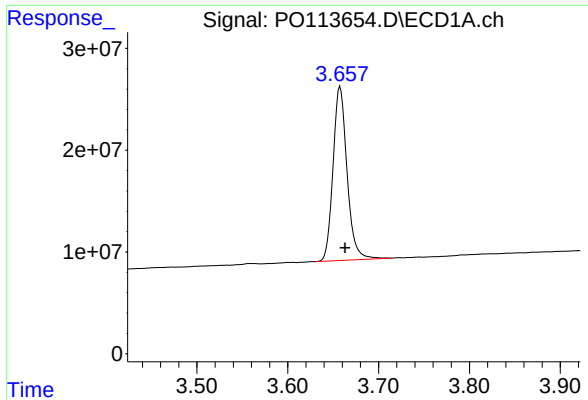

#1 Tetrachloro-m-xylene


R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 182814887
Conc: 22.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

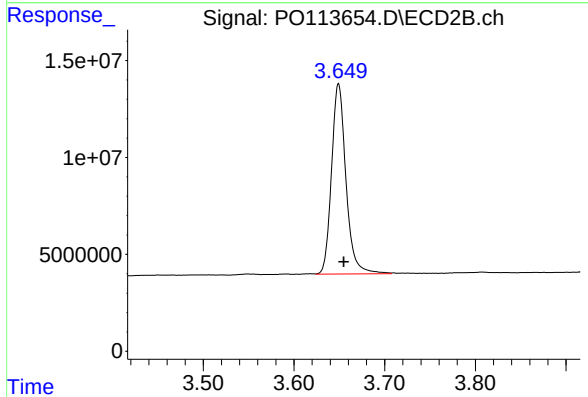


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.006 min
Response: 108471081
Conc: 21.43 ng/ml

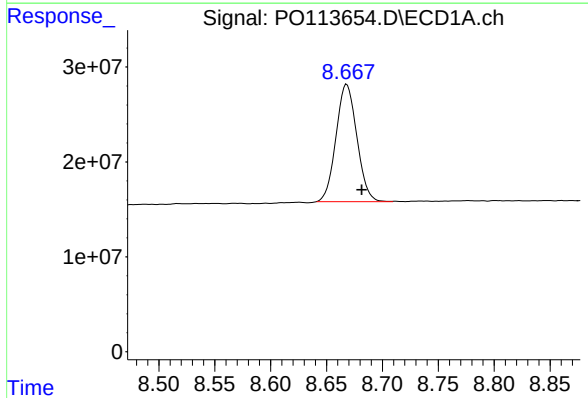


#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: -0.014 min
Response: 161071225
Conc: 23.24 ng/ml

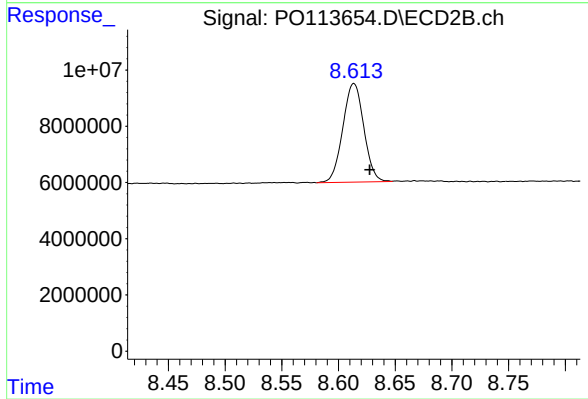

#2 Decachlorobiphenyl


R.T.: 8.614 min
Delta R.T.: -0.014 min
Response: 45296072
Conc: 23.90 ng/ml

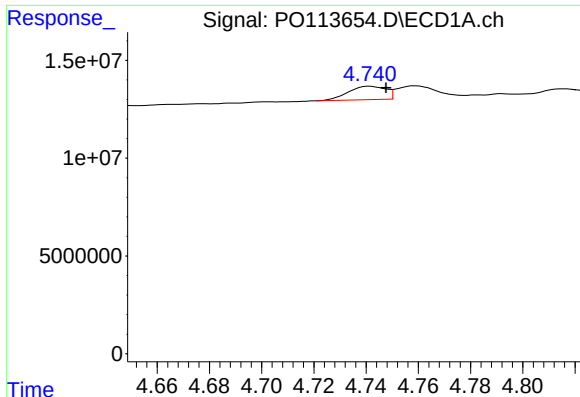

#3 AR-1016-1


R.T.: 4.741 min
Delta R.T.: -0.006 min
Response: 6819156
Conc: 25.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

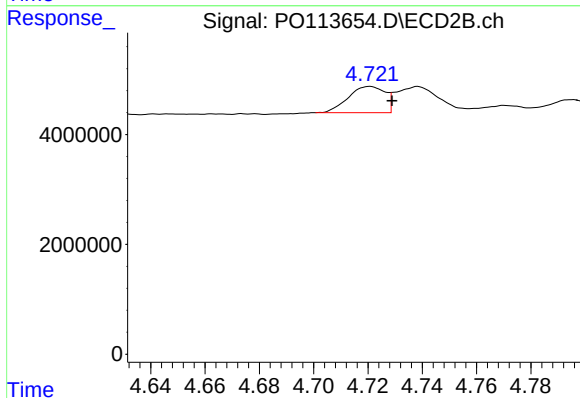


#3 AR-1016-1

R.T.: 4.721 min
Delta R.T.: -0.008 min
Response: 4490446
Conc: 26.33 ng/ml

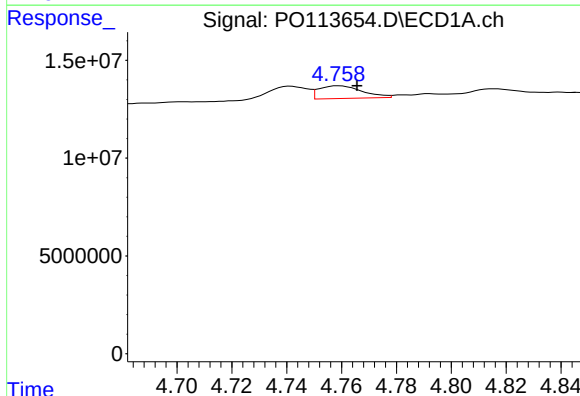


#4 AR-1016-2

R.T.: 4.759 min
Delta R.T.: -0.007 min
Response: 7135788
Conc: 17.78 ng/ml

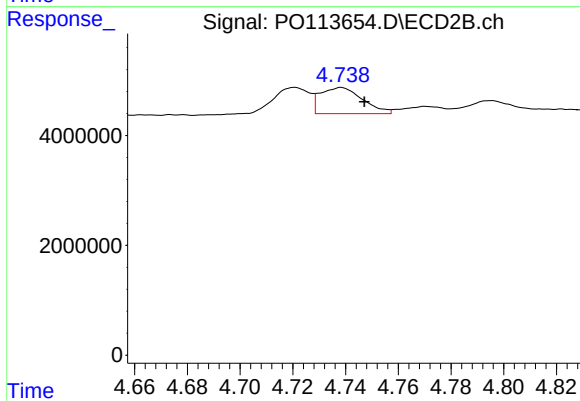

#4 AR-1016-2


R.T.: 4.738 min
Delta R.T.: -0.009 min
Response: 5266623
Conc: 20.44 ng/ml

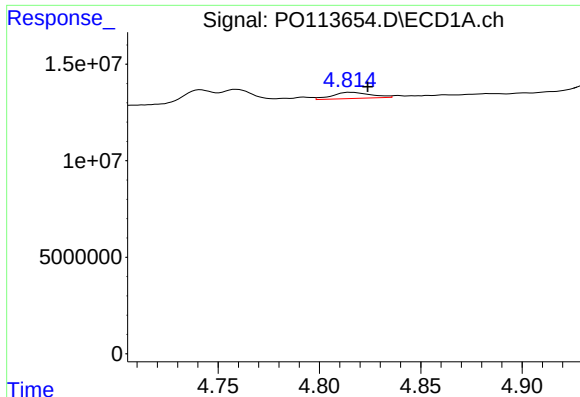

#5 AR-1016-3


R.T.: 4.816 min
Delta R.T.: -0.008 min
Response: 4232061
Conc: 16.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

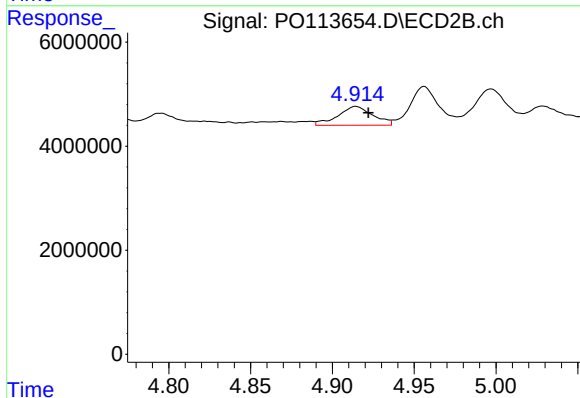


#5 AR-1016-3

R.T.: 4.914 min
Delta R.T.: -0.008 min
Response: 5369858
Conc: 38.46 ng/ml

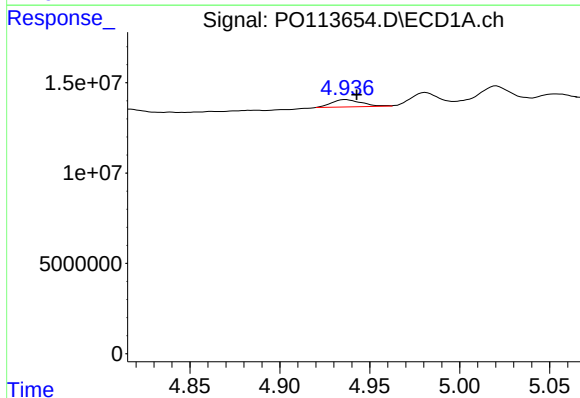


#6 AR-1016-4

R.T.: 4.937 min
Delta R.T.: -0.006 min
Response: 4748271
Conc: 21.77 ng/ml

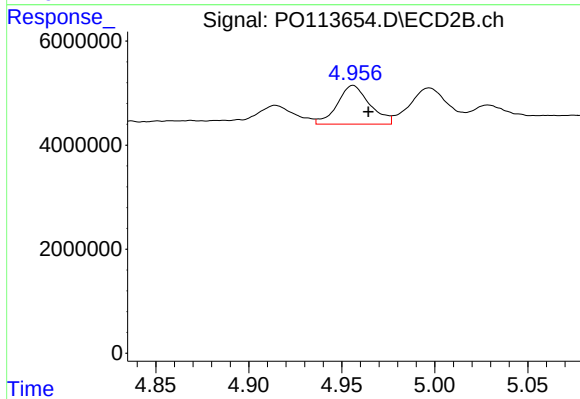

#6 AR-1016-4


R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 9051792
Conc: 77.57 ng/ml

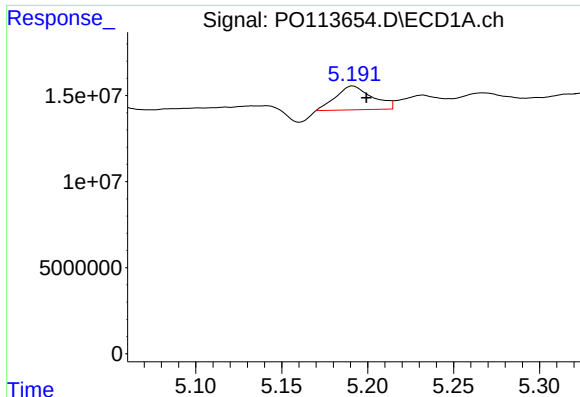

#7 AR-1016-5


R.T.: 5.192 min
Delta R.T.: -0.008 min
Response: 20518612
Conc: 92.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

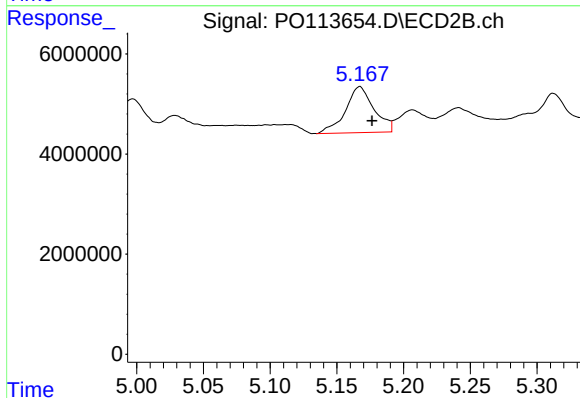


#7 AR-1016-5

R.T.: 5.167 min
Delta R.T.: -0.009 min
Response: 13680944
Conc: 95.99 ng/ml

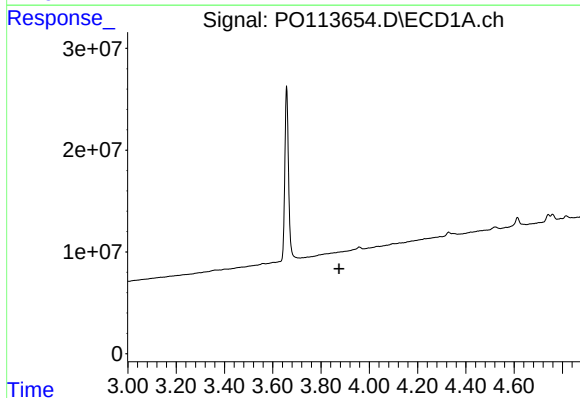


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 3.874 min
Response: 0
Conc: N.D.

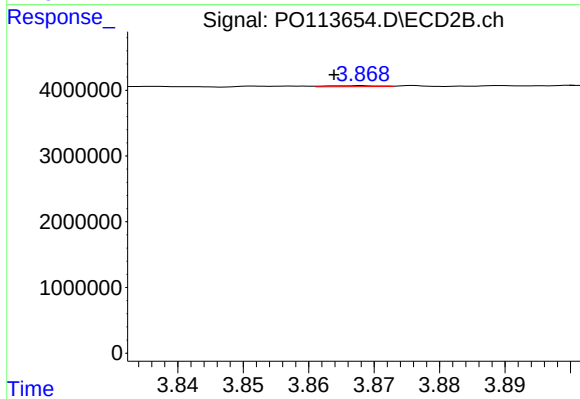

#8 AR-1221-1


R.T.: 3.868 min
Delta R.T.: 0.004 min
Response: 79850
Conc: 1.27 ng/ml

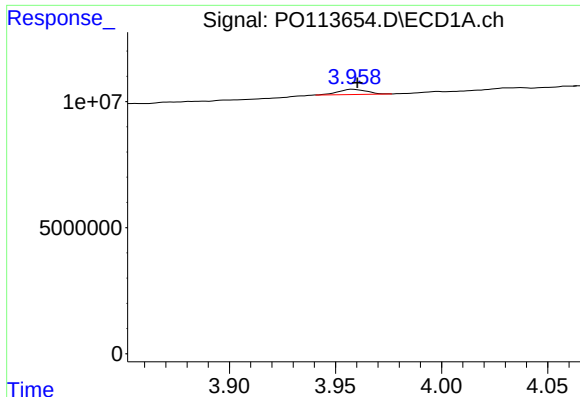

#9 AR-1221-2


R.T.: 3.958 min
Delta R.T.: -0.002 min
Response: 1886242
Conc: 27.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

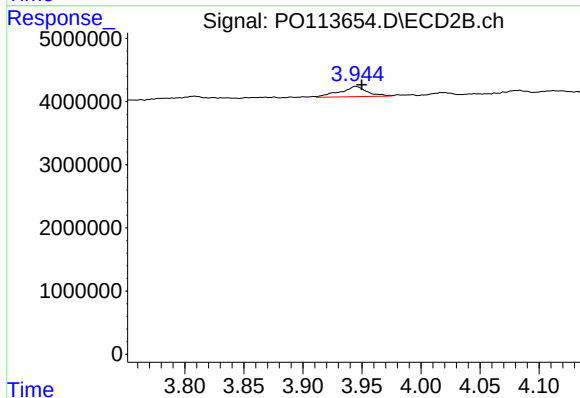


#9 AR-1221-2

R.T.: 3.945 min
Delta R.T.: -0.005 min
Response: 2586972
Conc: 55.43 ng/ml

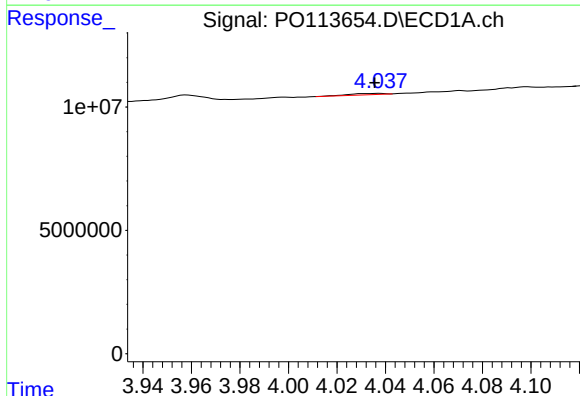


#10 AR-1221-3

R.T.: 4.038 min
Delta R.T.: 0.002 min
Response: 506513
Conc: 2.29 ng/ml

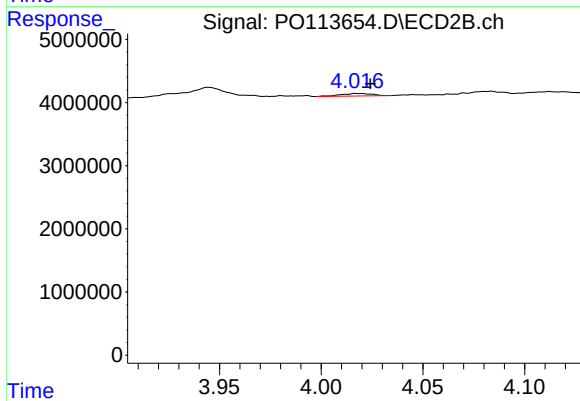

#10 AR-1221-3


R.T.: 4.017 min
Delta R.T.: -0.007 min
Response: 440357
Conc: 2.97 ng/ml

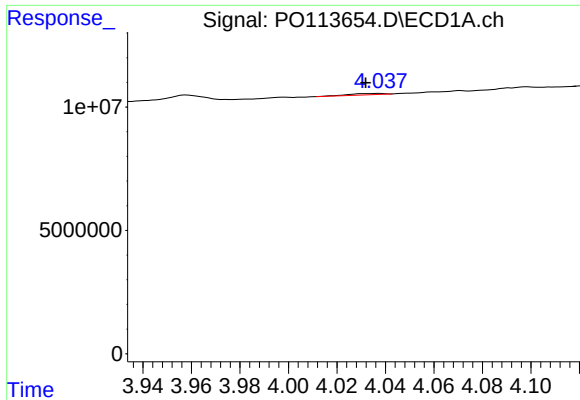

#11 AR-1232-1


R.T.: 4.038 min
Delta R.T.: 0.006 min
Response: 506513
Conc: 2.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

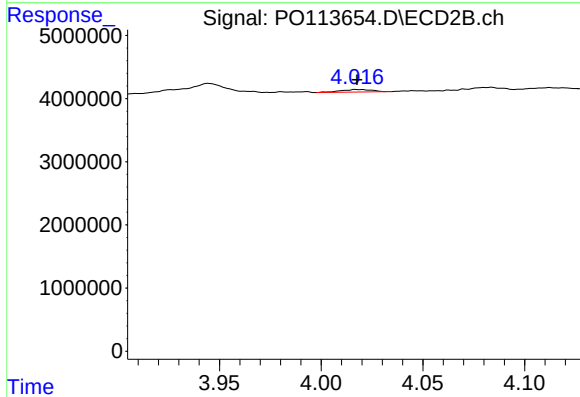


#11 AR-1232-1

R.T.: 4.017 min
Delta R.T.: 0.000 min
Response: 440357
Conc: 3.64 ng/ml

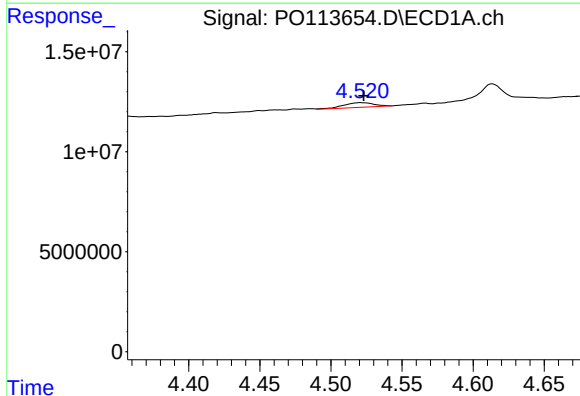


#12 AR-1232-2

R.T.: 4.521 min
Delta R.T.: -0.002 min
Response: 3452937
Conc: 32.00 ng/ml

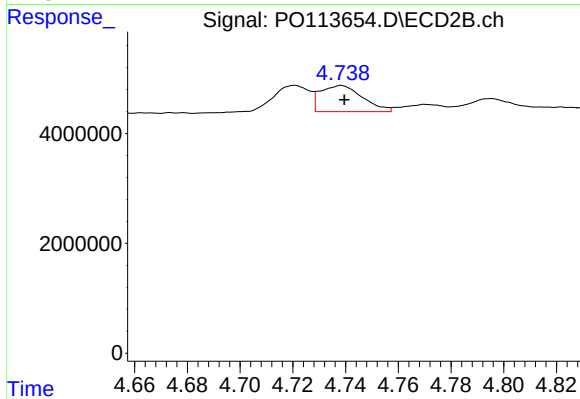

#12 AR-1232-2


R.T.: 4.738 min
Delta R.T.: -0.001 min
Response: 5266623
Conc: 43.15 ng/ml

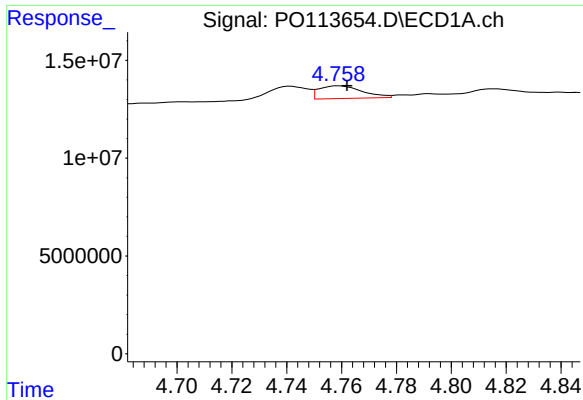

#13 AR-1232-3


R.T.: 4.759 min
Delta R.T.: -0.003 min
Response: 7135788
Conc: 36.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

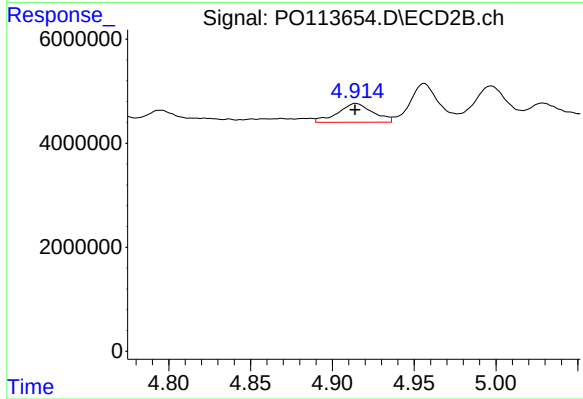


#13 AR-1232-3

R.T.: 4.914 min
Delta R.T.: 0.000 min
Response: 5369858
Conc: 81.17 ng/ml

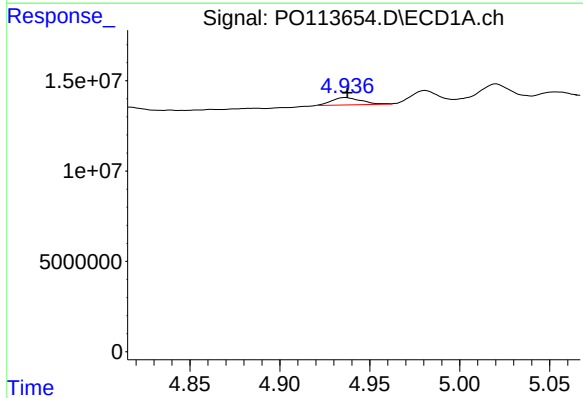


#14 AR-1232-4

R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 4748271
Conc: 48.31 ng/ml

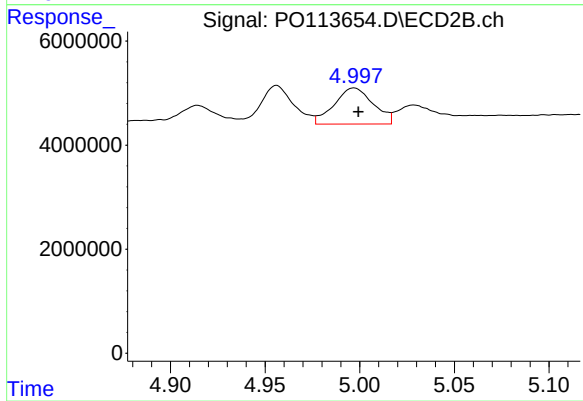

#14 AR-1232-4


R.T.: 4.997 min
Delta R.T.: -0.002 min
Response: 9995212
Conc: 166.79 ng/ml

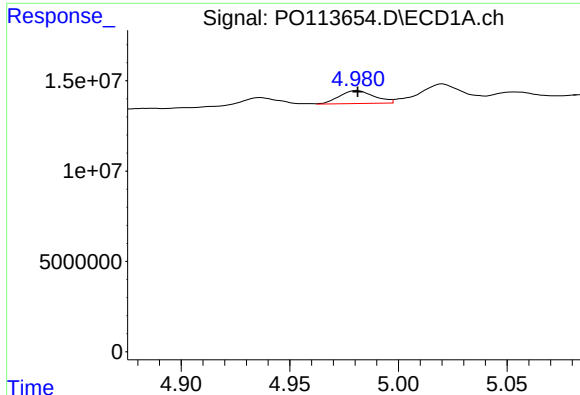

#15 AR-1232-5


R.T.: 4.981 min
Delta R.T.: 0.000 min
Response: 7983209
Conc: 121.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

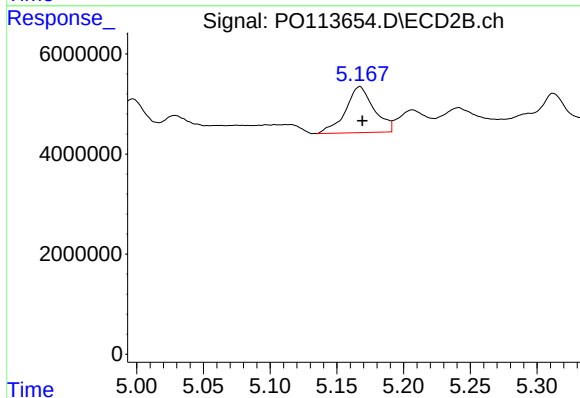


#15 AR-1232-5

R.T.: 5.167 min
Delta R.T.: -0.002 min
Response: 13680944
Conc: 202.33 ng/ml

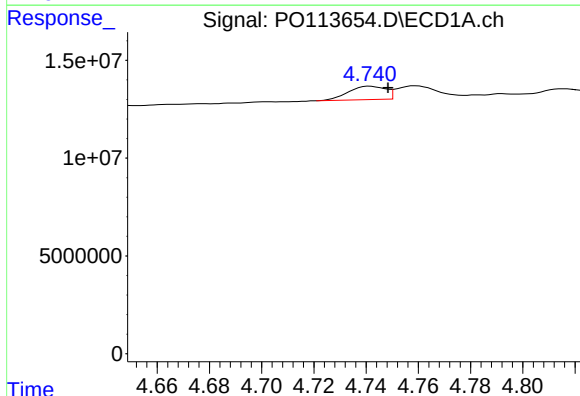


#16 AR-1242-1

R.T.: 4.741 min
Delta R.T.: -0.007 min
Response: 6819156
Conc: 29.66 ng/ml

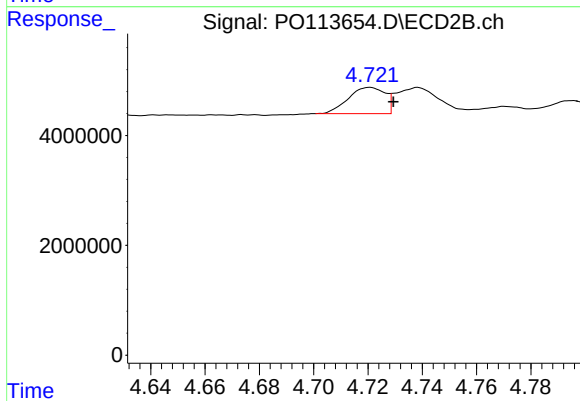

#16 AR-1242-1


R.T.: 4.721 min
Delta R.T.: -0.009 min
Response: 4490446
Conc: 31.07 ng/ml

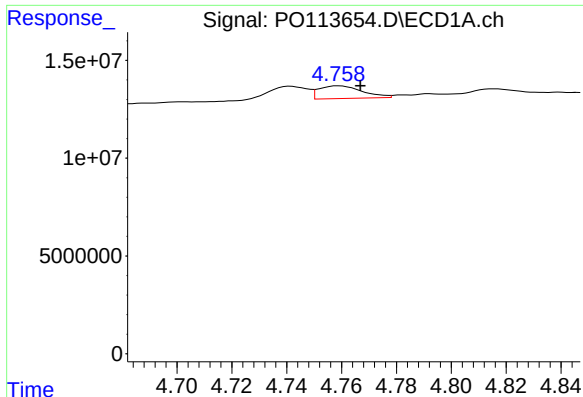

#17 AR-1242-2


R.T.: 4.759 min
Delta R.T.: -0.008 min
Response: 7135788
Conc: 20.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

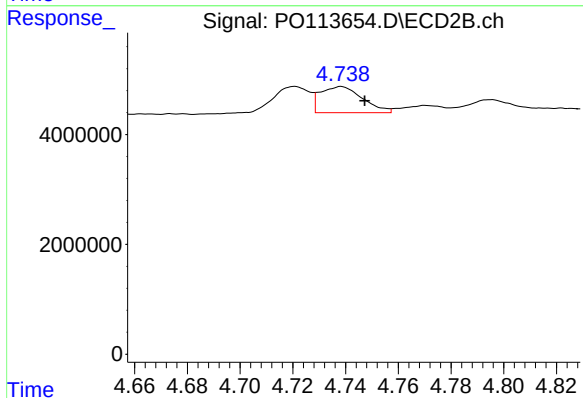


#17 AR-1242-2

R.T.: 4.738 min
Delta R.T.: -0.009 min
Response: 5266623
Conc: 24.28 ng/ml

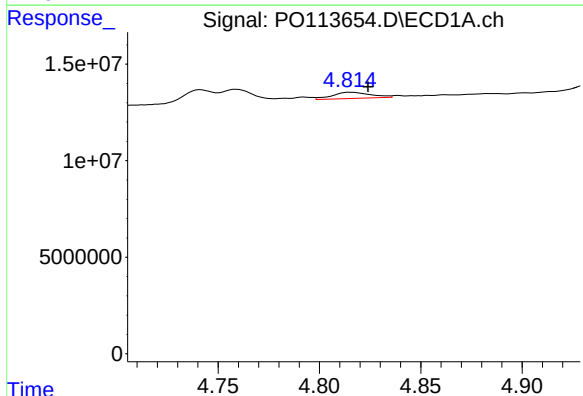


#18 AR-1242-3

R.T.: 4.816 min
Delta R.T.: -0.008 min
Response: 4232061
Conc: 19.07 ng/ml

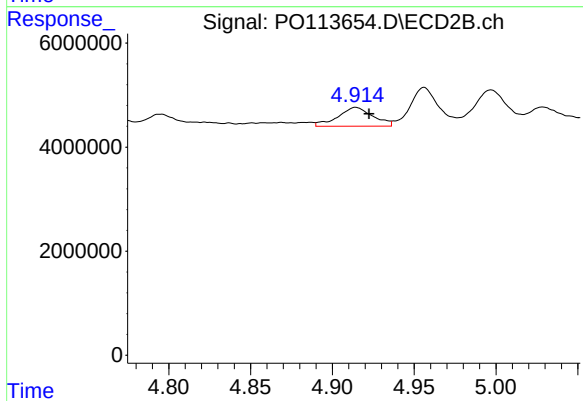

#18 AR-1242-3


R.T.: 4.914 min
Delta R.T.: -0.008 min
Response: 5369858
Conc: 45.91 ng/ml

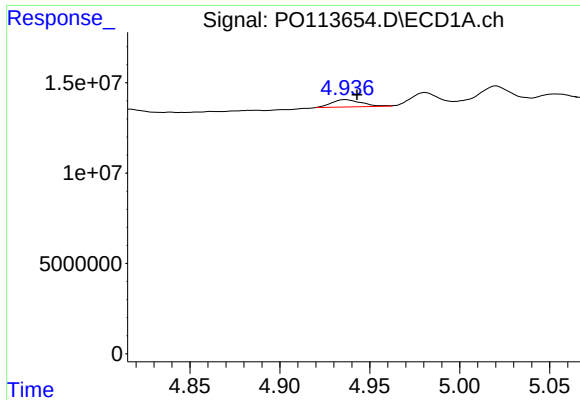

#19 AR-1242-4


R.T.: 4.937 min
Delta R.T.: -0.006 min
Response: 4748271
Conc: 27.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

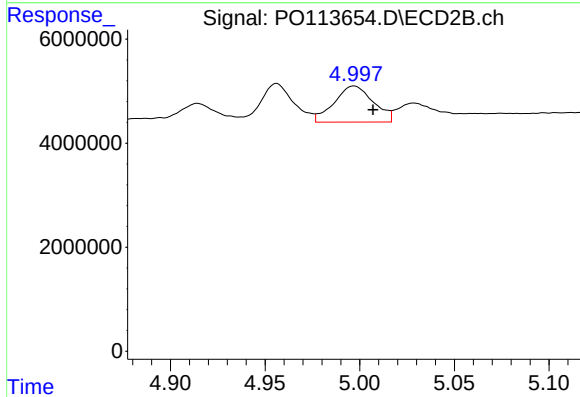


#19 AR-1242-4

R.T.: 4.997 min
Delta R.T.: -0.010 min
Response: 9995212
Conc: 84.97 ng/ml

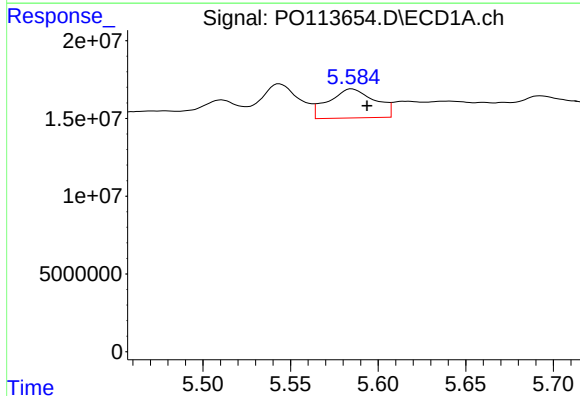


#20 AR-1242-5

R.T.: 5.585 min
Delta R.T.: -0.009 min
Response: 34317195
Conc: 171.45 ng/ml

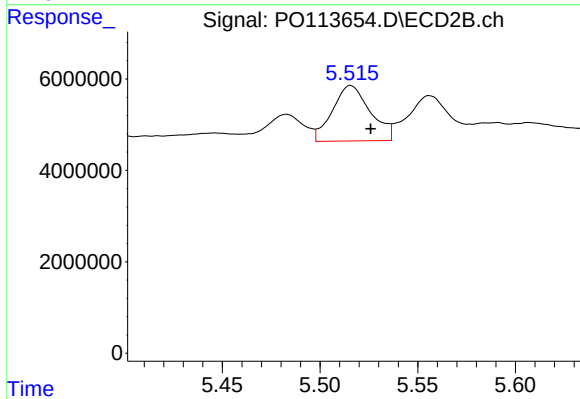

#20 AR-1242-5


R.T.: 5.516 min
Delta R.T.: -0.010 min
Response: 16376649
Conc: 109.81 ng/ml

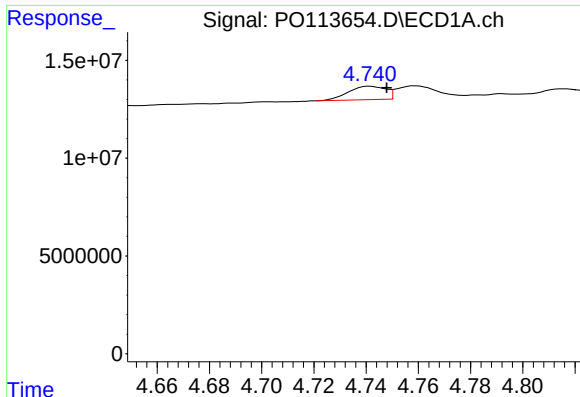

#21 AR-1248-1


R.T.: 4.741 min
Delta R.T.: -0.006 min
Response: 6819156
Conc: 39.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

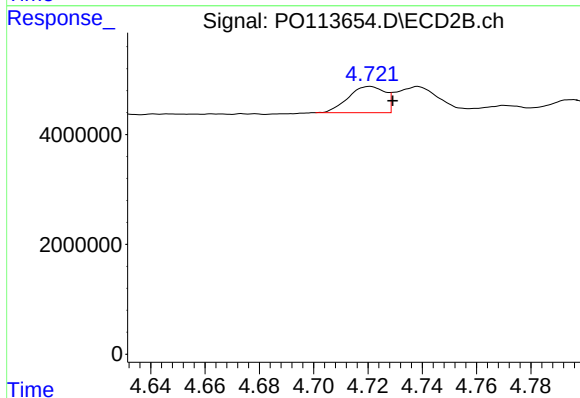


#21 AR-1248-1

R.T.: 4.721 min
Delta R.T.: -0.008 min
Response: 4490446
Conc: 40.27 ng/ml

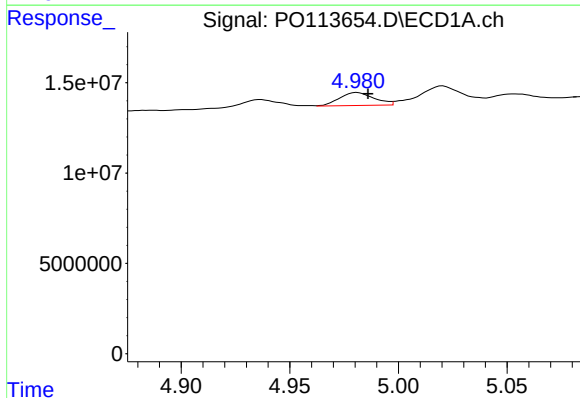


#22 AR-1248-2

R.T.: 4.981 min
Delta R.T.: -0.005 min
Response: 7983209
Conc: 33.01 ng/ml

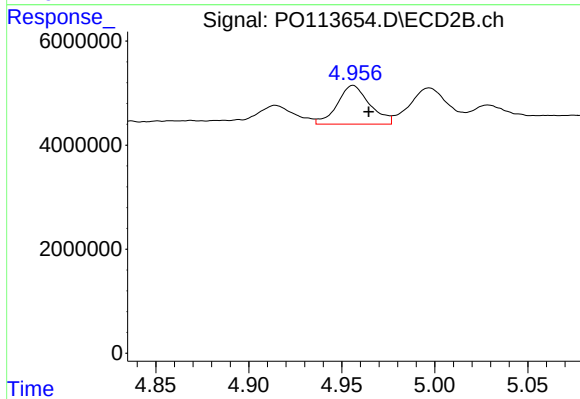

#22 AR-1248-2


R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 9051792
Conc: 56.33 ng/ml

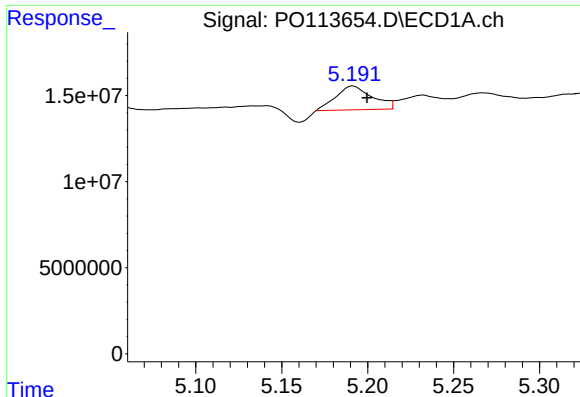

#23 AR-1248-3


R.T.: 5.192 min
Delta R.T.: -0.008 min
Response: 20518612
Conc: 64.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

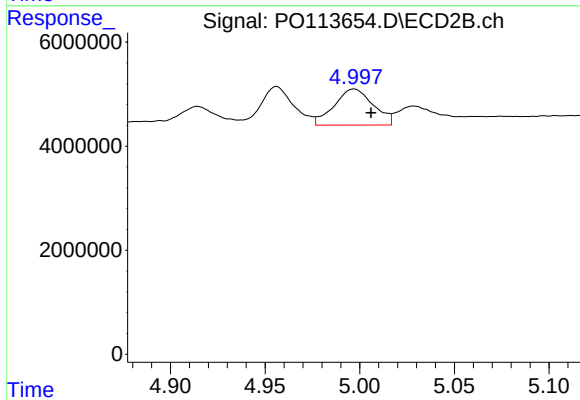


#23 AR-1248-3

R.T.: 4.997 min
Delta R.T.: -0.009 min
Response: 9995212
Conc: 58.91 ng/ml

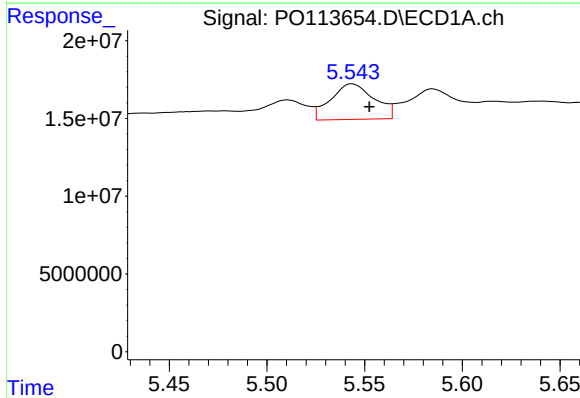


#24 AR-1248-4

R.T.: 5.544 min
Delta R.T.: -0.009 min
Response: 35441165
Conc: 70.94 ng/ml

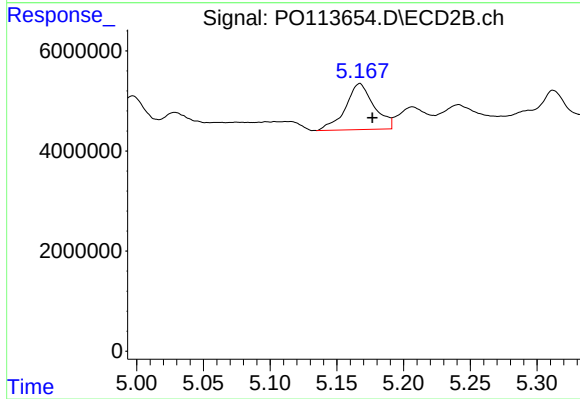

#24 AR-1248-4


R.T.: 5.167 min
Delta R.T.: -0.009 min
Response: 13680944
Conc: 68.67 ng/ml

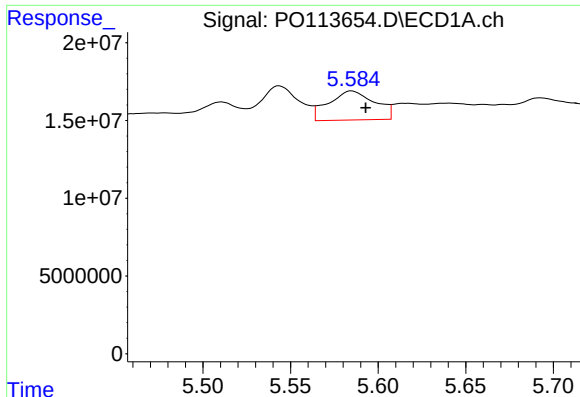

#25 AR-1248-5


R.T.: 5.585 min
Delta R.T.: -0.008 min
Response: 34317195
Conc: 100.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

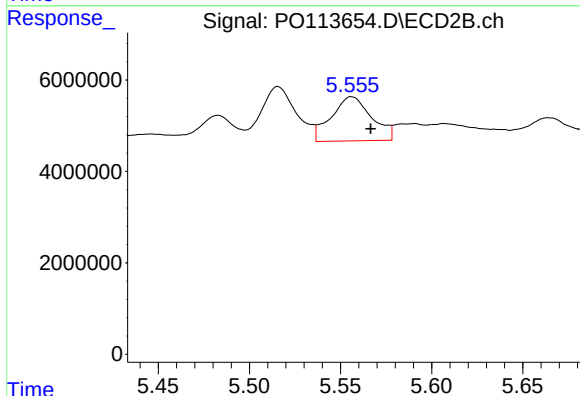


#25 AR-1248-5

R.T.: 5.556 min
Delta R.T.: -0.011 min
Response: 14916949
Conc: 70.26 ng/ml

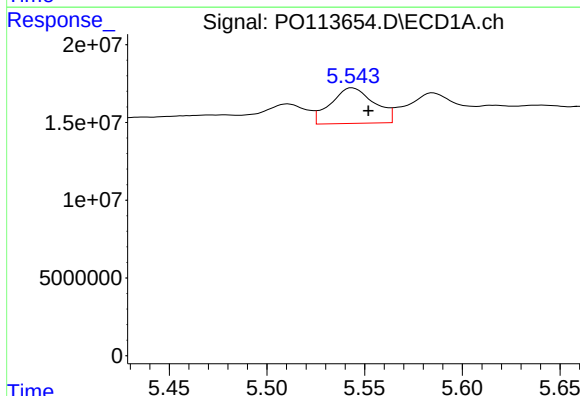


#26 AR-1254-1

R.T.: 5.544 min
Delta R.T.: -0.008 min
Response: 35441165
Conc: 65.63 ng/ml

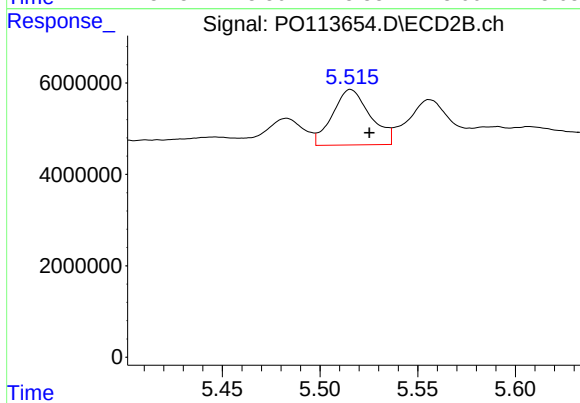

#26 AR-1254-1


R.T.: 5.516 min
Delta R.T.: -0.010 min
Response: 16376649
Conc: 51.93 ng/ml

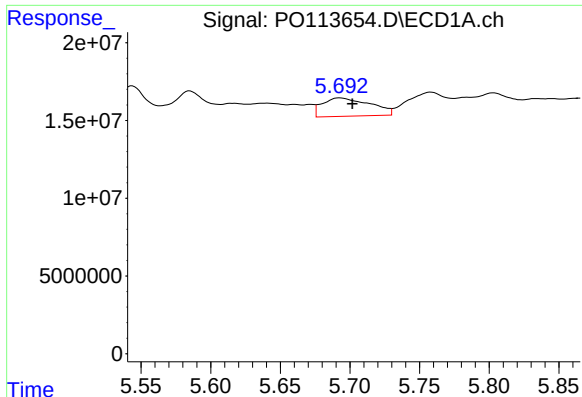

#27 AR-1254-2


R.T.: 5.693 min
Delta R.T.: -0.009 min
Response: 28321854
Conc: 57.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

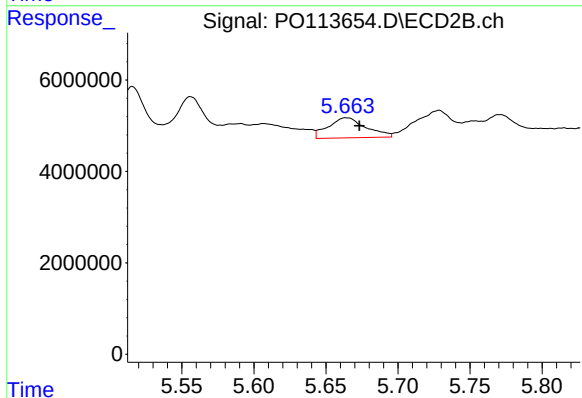


#27 AR-1254-2

R.T.: 5.664 min
Delta R.T.: -0.010 min
Response: 7979888
Conc: 28.47 ng/ml

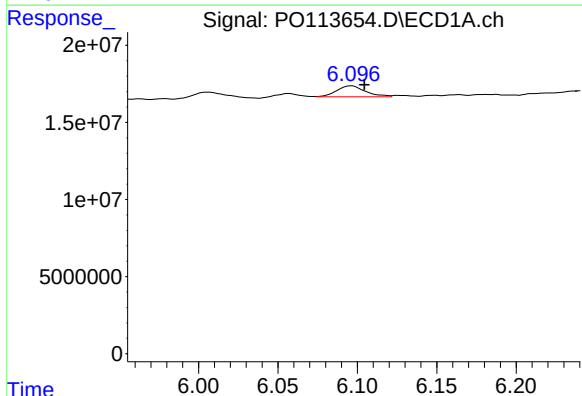


#28 AR-1254-3

R.T.: 6.096 min
Delta R.T.: -0.008 min
Response: 8932417
Conc: 12.09 ng/ml

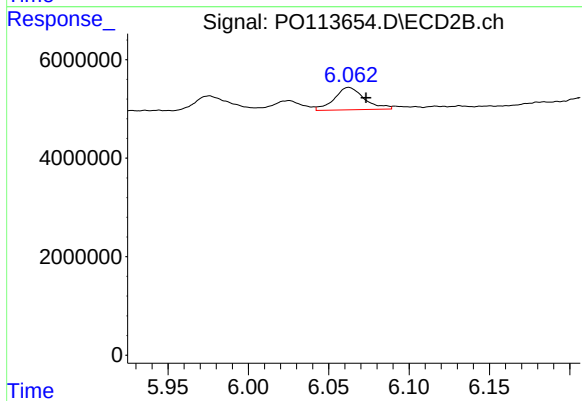

#28 AR-1254-3


R.T.: 6.063 min
Delta R.T.: -0.011 min
Response: 5938983
Conc: 14.24 ng/ml

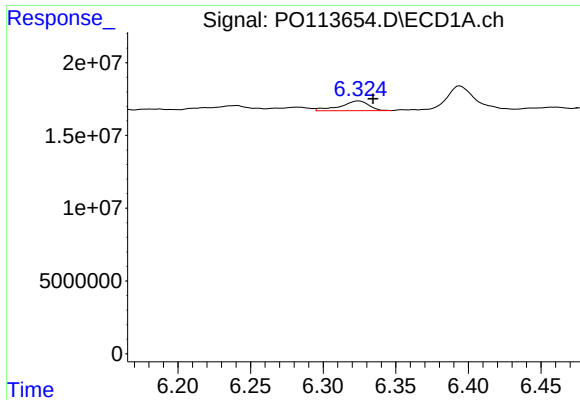

#29 AR-1254-4


R.T.: 6.325 min
Delta R.T.: -0.010 min
Response: 9204871
Conc: 16.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

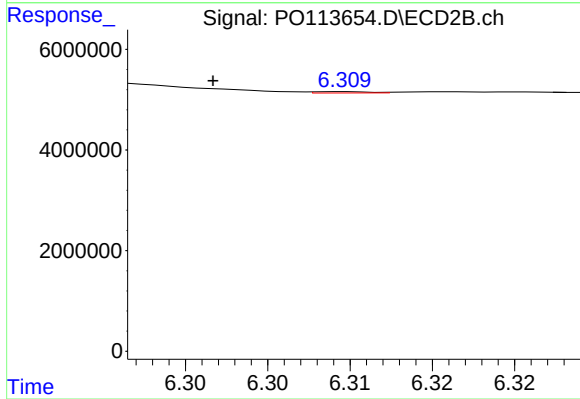


#29 AR-1254-4

R.T.: 6.310 min
Delta R.T.: 0.008 min
Response: 60558
Conc: 0.22 ng/ml

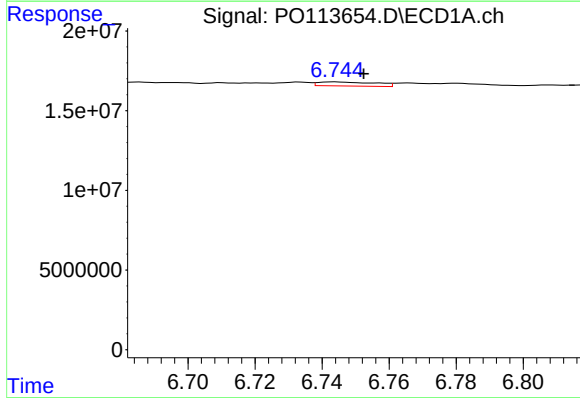


#30 AR-1254-5

R.T.: 6.744 min
Delta R.T.: -0.009 min
Response: 3040977
Conc: 4.34 ng/ml

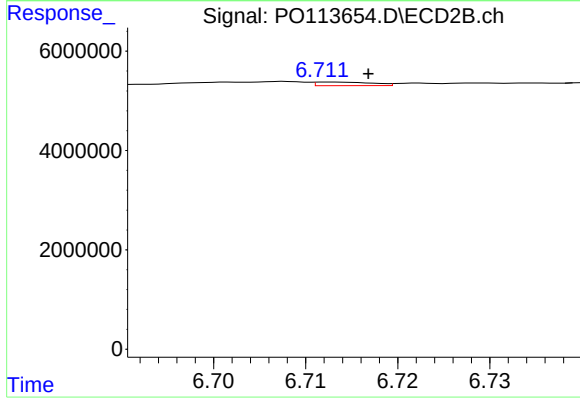

#30 AR-1254-5


R.T.: 6.713 min
Delta R.T.: -0.004 min
Response: 309782
Conc: 0.87 ng/ml

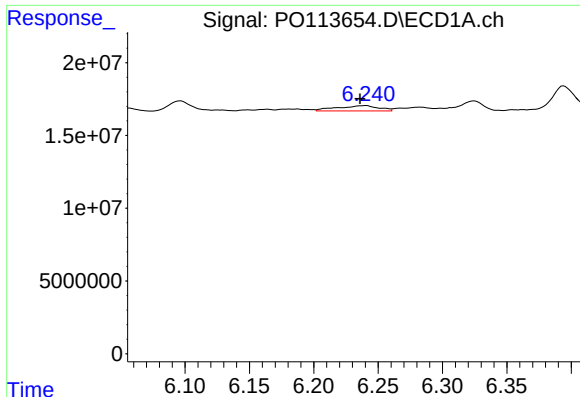

#31 AR-1260-1


R.T.: 6.241 min
Delta R.T.: 0.005 min
Response: 8214162
Conc: 18.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

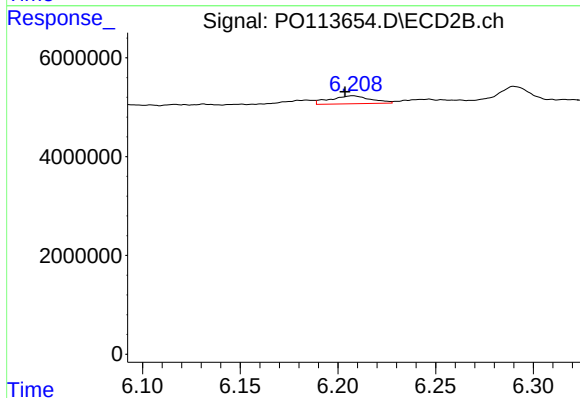


#31 AR-1260-1

R.T.: 6.208 min
Delta R.T.: 0.004 min
Response: 2325272
Conc: 9.12 ng/ml

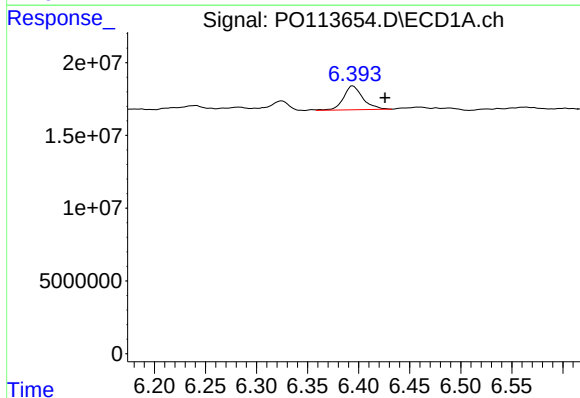


#32 AR-1260-2

R.T.: 6.394 min
Delta R.T.: -0.032 min
Response: 21773046
Conc: 31.71 ng/ml

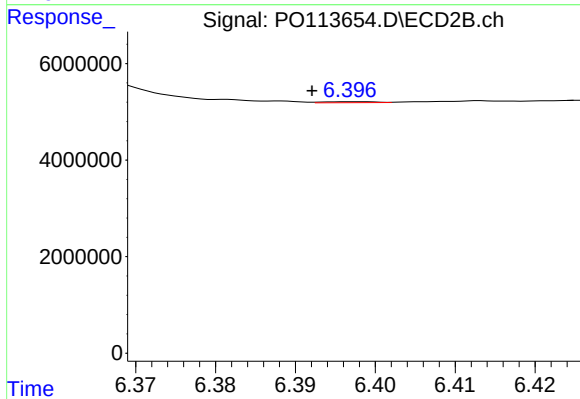

#32 AR-1260-2


R.T.: 6.397 min
Delta R.T.: 0.005 min
Response: 93837
Conc: 0.27 ng/ml

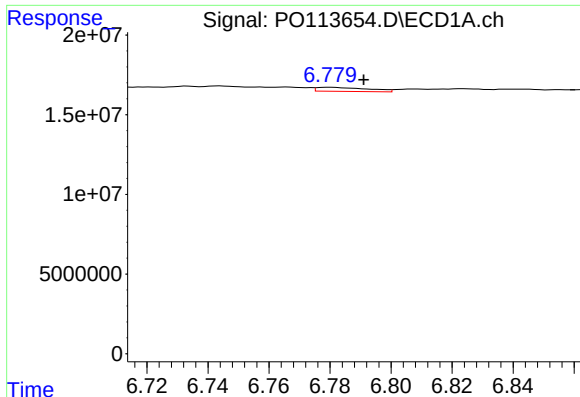

#33 AR-1260-3


R.T.: 6.780 min
Delta R.T.: -0.011 min
Response: 2947383
Conc: 4.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

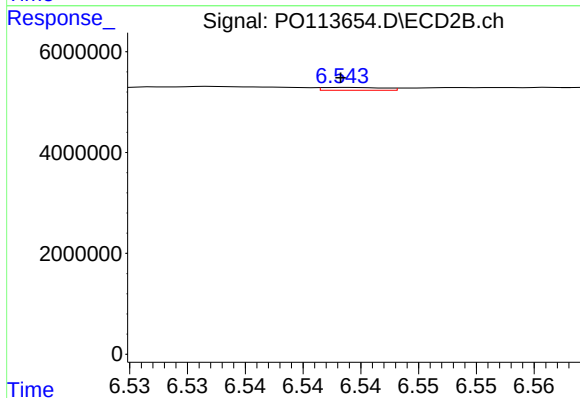


#33 AR-1260-3

R.T.: 6.544 min
Delta R.T.: 0.000 min
Response: 205517
Conc: 0.69 ng/ml

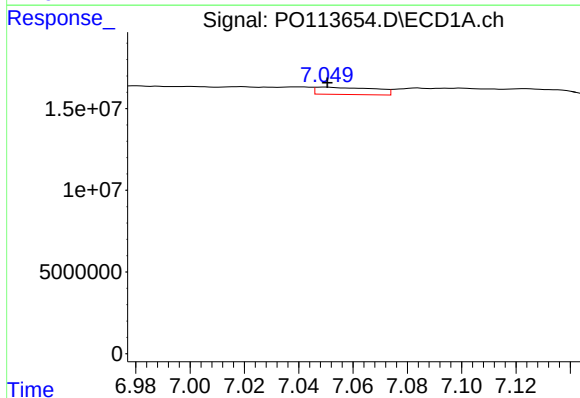


#34 AR-1260-4

R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 6683028
Conc: 14.92 ng/ml

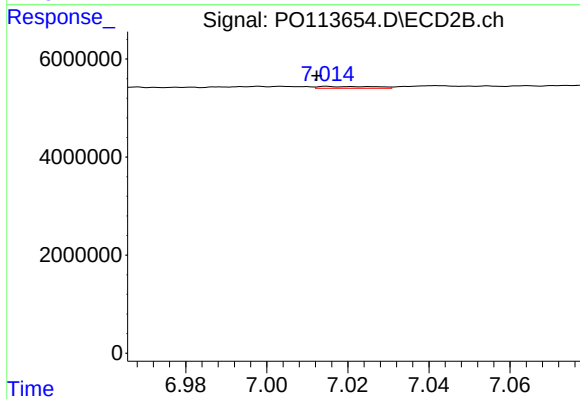

#34 AR-1260-4


R.T.: 7.015 min
Delta R.T.: 0.003 min
Response: 352928
Conc: 1.70 ng/ml

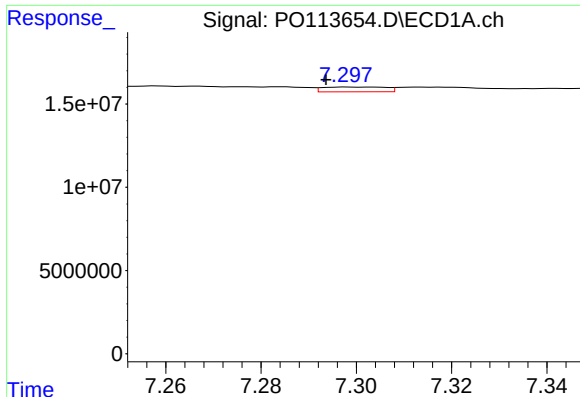

#35 AR-1260-5


R.T.: 7.298 min
Delta R.T.: 0.004 min
Response: 2687860
Conc: 2.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

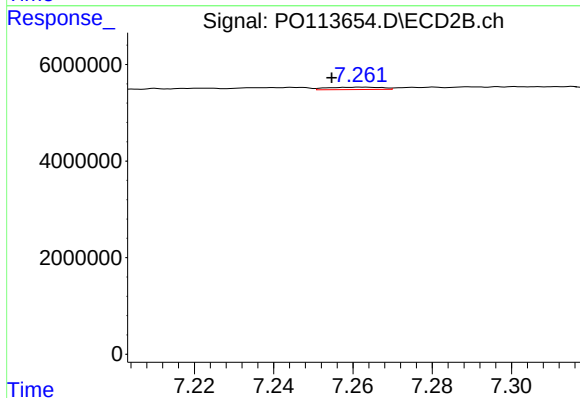


#35 AR-1260-5

R.T.: 7.262 min
Delta R.T.: 0.007 min
Response: 480038
Conc: 1.02 ng/ml

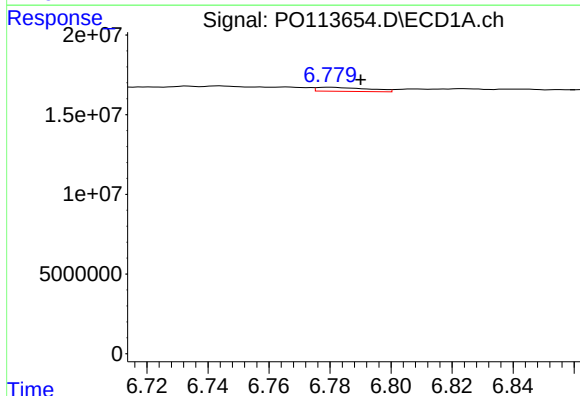


#36 AR-1262-1

R.T.: 6.780 min
Delta R.T.: -0.010 min
Response: 2947383
Conc: 3.22 ng/ml

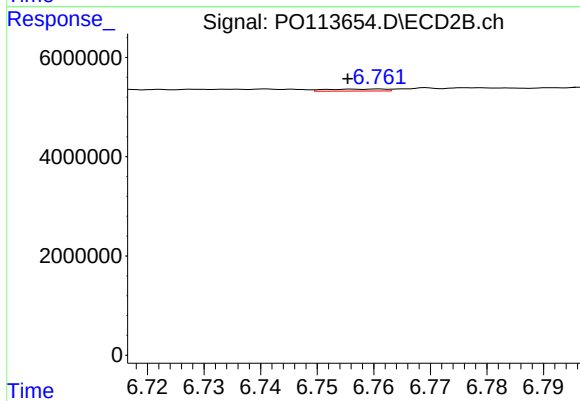

#36 AR-1262-1


R.T.: 6.761 min
Delta R.T.: 0.005 min
Response: 286973
Conc: 0.69 ng/ml

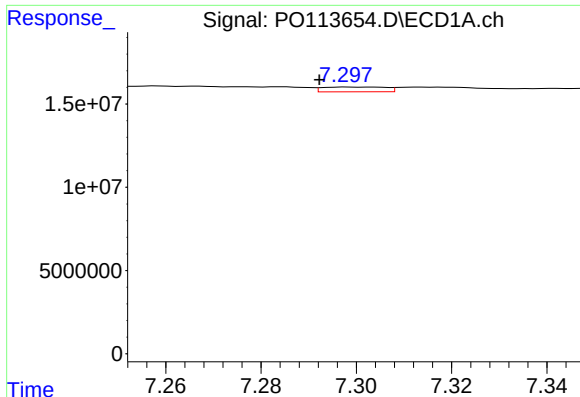

#37 AR-1262-2


R.T.: 7.298 min
Delta R.T.: 0.006 min
Response: 2687860
Conc: 1.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

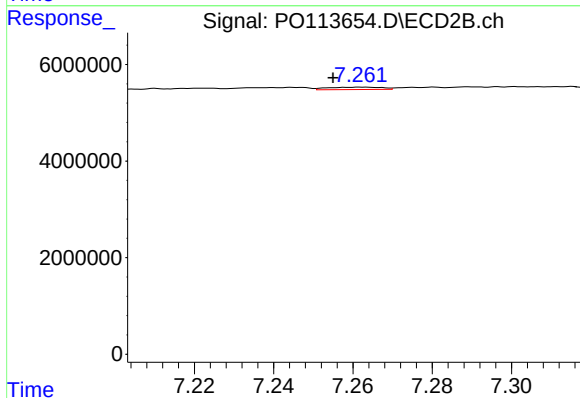


#37 AR-1262-2

R.T.: 7.262 min
Delta R.T.: 0.007 min
Response: 480038
Conc: 0.93 ng/ml

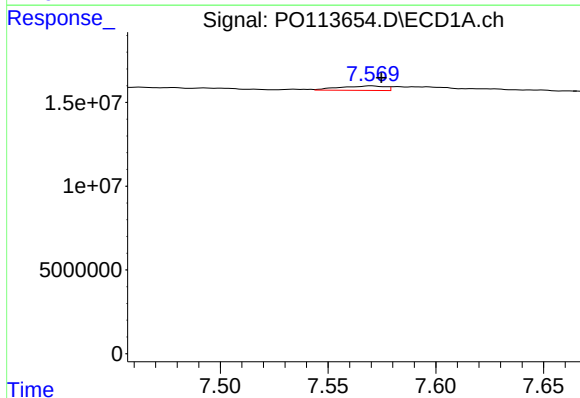


#38 AR-1262-3

R.T.: 7.570 min
Delta R.T.: -0.005 min
Response: 3850868
Conc: 6.95 ng/ml

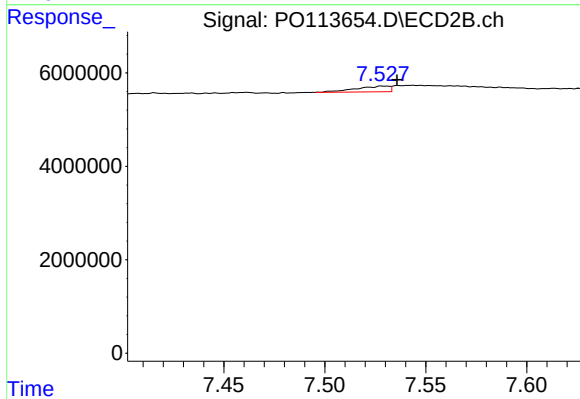

#38 AR-1262-3


R.T.: 7.528 min
Delta R.T.: -0.008 min
Response: 1395285
Conc: 7.77 ng/ml

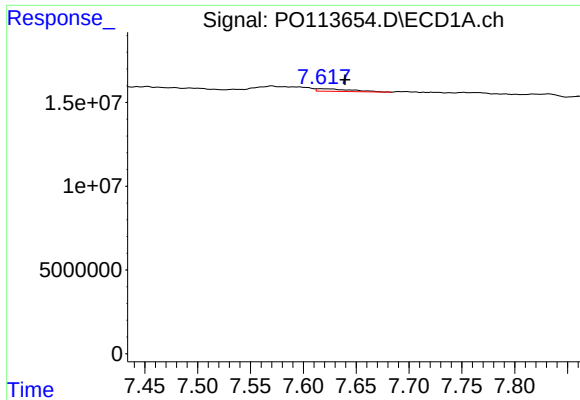

#39 AR-1262-4


R.T.: 7.617 min
Delta R.T.: -0.022 min
Response: 3463886
Conc: 3.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

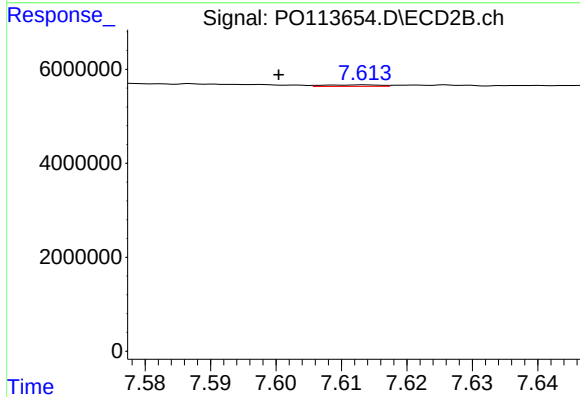


#39 AR-1262-4

R.T.: 7.614 min
Delta R.T.: 0.013 min
Response: 195698
Conc: 0.68 ng/ml

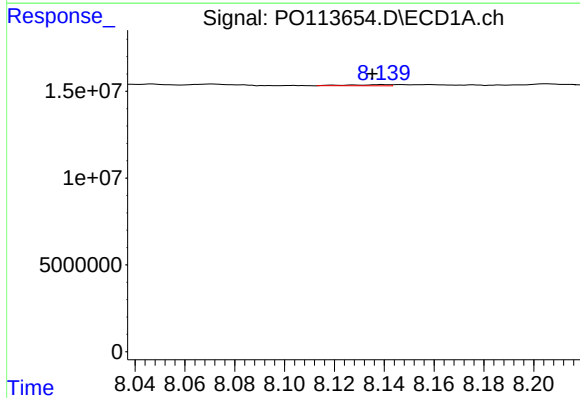


#40 AR-1262-5

R.T.: 8.139 min
Delta R.T.: 0.004 min
Response: 753049
Conc: 1.81 ng/ml

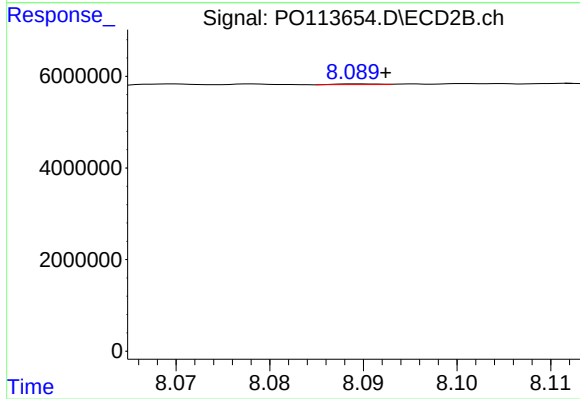

#40 AR-1262-5


R.T.: 8.089 min
Delta R.T.: -0.003 min
Response: 43166
Conc: 0.40 ng/ml

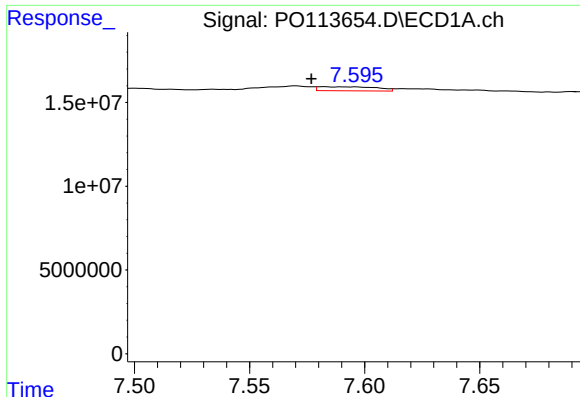

#41 AR-1268-1


R.T.: 7.583 min
Delta R.T.: 0.006 min
Response: 4196129
Conc: 2.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

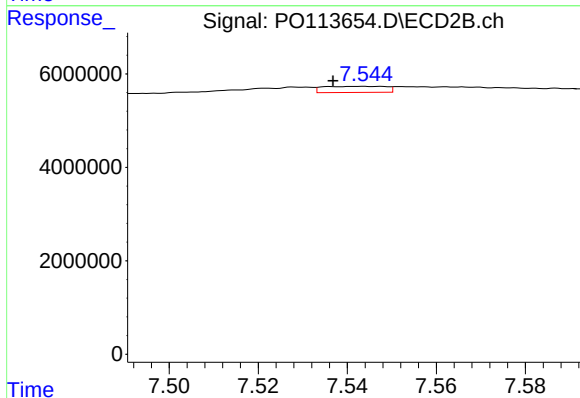


#41 AR-1268-1

R.T.: 7.544 min
Delta R.T.: 0.007 min
Response: 1277754
Conc: 2.51 ng/ml

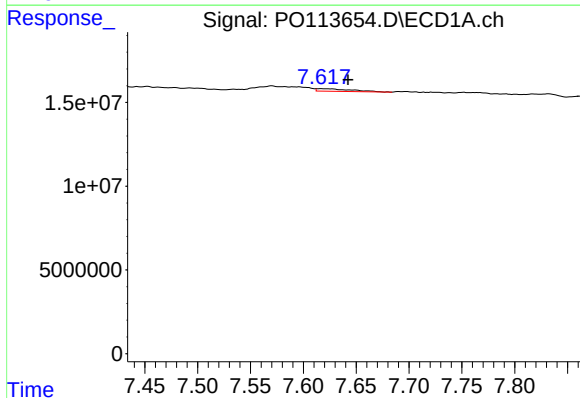


#42 AR-1268-2

R.T.: 7.617 min
Delta R.T.: -0.025 min
Response: 3463886
Conc: 2.39 ng/ml

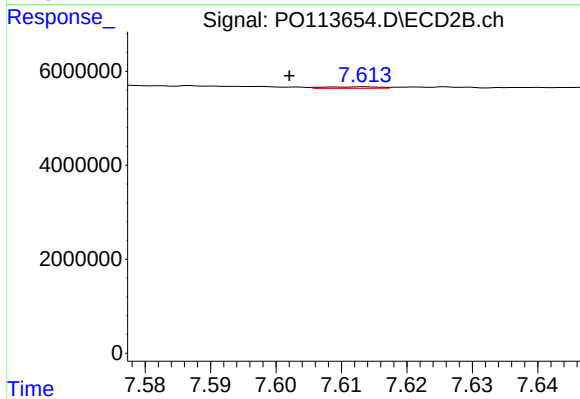

#42 AR-1268-2


R.T.: 7.614 min
Delta R.T.: 0.012 min
Response: 195698
Conc: 0.47 ng/ml

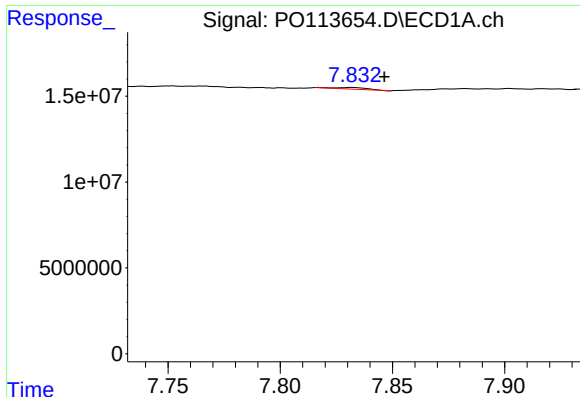

#43 AR-1268-3


R.T.: 7.832 min
Delta R.T.: -0.014 min
Response: 1004964
Conc: 0.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

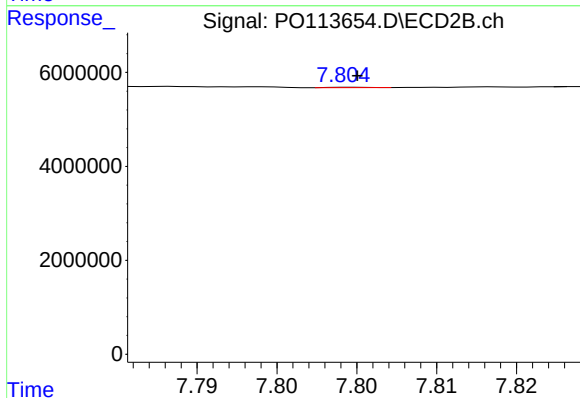


#43 AR-1268-3

R.T.: 7.805 min
Delta R.T.: 0.000 min
Response: 11924
Conc: 0.04 ng/ml

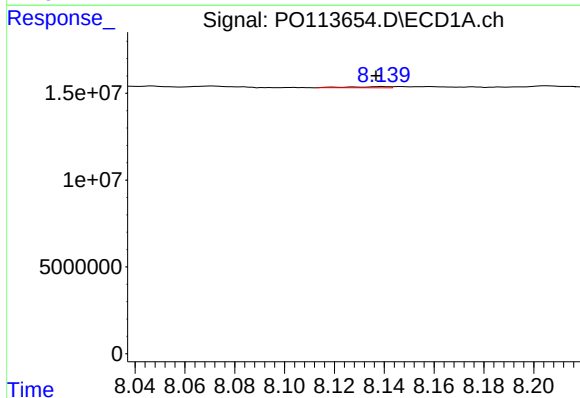


#44 AR-1268-4

R.T.: 8.139 min
Delta R.T.: 0.003 min
Response: 753049
Conc: 1.63 ng/ml

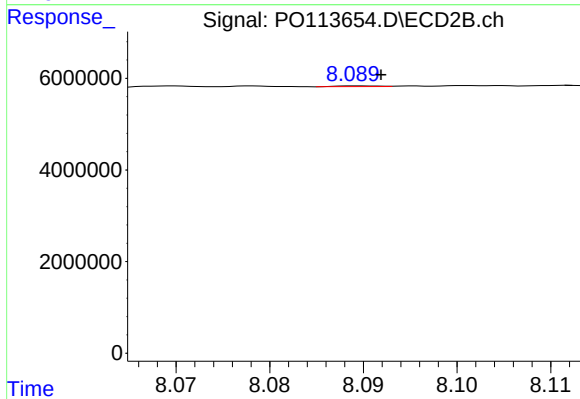

#44 AR-1268-4


R.T.: 8.089 min
Delta R.T.: -0.002 min
Response: 43166
Conc: 0.36 ng/ml

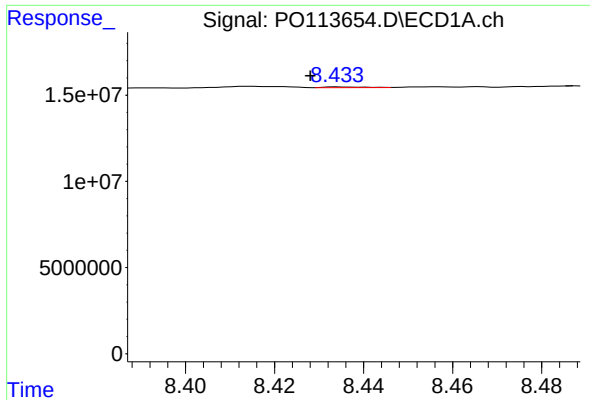

#45 AR-1268-5

R.T.: 8.434 min
Delta R.T.: 0.006 min
Response: 248676
Conc: 0.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

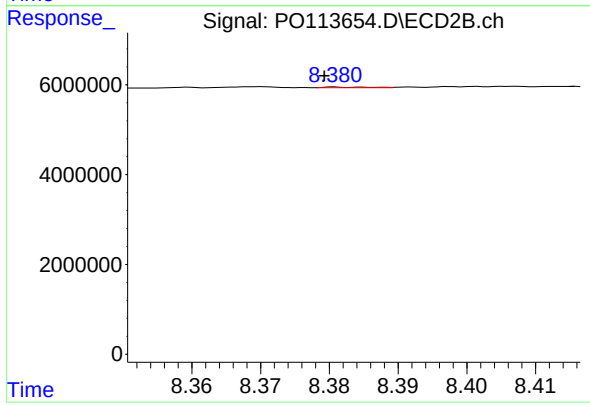

#45 AR-1268-5

R.T.: 8.381 min
Delta R.T.: 0.002 min
Response: 70816
Conc: 0.09 ng/ml