

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091125\
 Data File : P0113655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 12:12
 Operator : YP/AJ
 Sample : Q2893-07
 Misc : AR1254 40PPB WATER MDL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 02:10:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.659	3.666	173.3E6	101.2E6	21.171	20.006
2)	SA Decachlor...	8.670	8.630	155.3E6	42731003	22.403	22.551
Target Compounds							
3)	L1 AR-1016-1	4.753	4.738	742920	1311485	2.783	7.689 #
4)	L1 AR-1016-2	4.772	4.738	231127	1311485	0.576	5.090 #
5)	L1 AR-1016-3	4.817	4.938	584519	5290341	2.292	37.893 #
6)	L1 AR-1016-4	4.954	4.973	1829513	8597781	8.390	73.675 #
7)	L1 AR-1016-5	5.193	5.183	17550838	11200930	79.191	78.586
8)	L2 AR-1221-1	3.884	3.881	-60102	463808	N.D.	7.348 #
9)	L2 AR-1221-2	3.959	3.963	1791256	2680532	26.517	57.432 #
10)	L2 AR-1221-3	4.074f	4.012	-195590	231737	N.D.	1.561 #
11)	L3 AR-1232-1	4.074f	4.012	-195590	231737	N.D.	1.916 #
12)	L3 AR-1232-2	4.525	4.738	1706971	1311485	15.817	10.745 #
13)	L3 AR-1232-3	4.753	4.938	742920	5290341	3.764	79.968 #
14)	L3 AR-1232-4	4.954	5.013	1829513	6329547	18.613	105.618 #
15)	L3 AR-1232-5	4.983	5.183	5558422	11200930	84.497	165.655 #
16)	L4 AR-1242-1	4.753	4.738	742920	1311485	3.231	9.076 #
17)	L4 AR-1242-2	4.772	4.738	231127	1311485	0.673	6.046 #
18)	L4 AR-1242-3	4.817	4.938	584519	5290341	2.634	45.230 #
19)	L4 AR-1242-4	4.954	5.013	1829513	6329547	10.547	53.806 #
20)	L4 AR-1242-5	5.584	5.532	14749518	26376305	73.688	176.864 #
21)	L5 AR-1248-1	4.753	4.738	742920	1311485	4.258	11.761 #
22)	L5 AR-1248-2	4.983	4.973	5558422	8597781	22.981	53.502 #
23)	L5 AR-1248-3	5.193	5.013	17550838	6329547	55.042	37.307 #
24)	L5 AR-1248-4	5.545	5.183	44087760	11200930	88.245	56.224 #
25)	L5 AR-1248-5	5.584	5.532	14749518	26376305	43.191	124.243 #
26)	L6 AR-1254-1	5.545	5.532	44087760	26376305	81.647	83.640
27)	L6 AR-1254-2	5.694	5.681	40164602	16597175	81.395	59.204 #
28)	L6 AR-1254-3	6.097	6.079	24777796	17075359	33.534	40.956
29)	L6 AR-1254-4	6.326	6.307	20217355	9306936	36.297	33.864
30)	L6 AR-1254-5	6.744	6.723	30970179	12829781	44.182	35.888
31)	L7 AR-1260-1	6.228	6.210	14377541	8163717	32.238	32.006
32)	L7 AR-1260-2	6.415	6.398	12271084	5655626	17.869	16.359
33)	L7 AR-1260-3	6.819	6.547	3707615	8100426	6.004	27.234 #
34)	L7 AR-1260-4	7.043	7.016	3666901	982450	8.187	4.740 #
35)	L7 AR-1260-5	7.283	7.259	7472852	1441964	6.172	3.078 #
36)	L8 AR-1262-1	6.819	6.723	3707615	12829781	4.049	30.944 #
37)	L8 AR-1262-2	7.283	7.259	7472852	1441964	4.942	2.785 #
38)	L8 AR-1262-3	7.581	7.557	15576673	7081629	28.111	39.432 #
39)	L8 AR-1262-4	7.621	7.600	8693599	2503627	8.889	8.636
40)	L8 AR-1262-5	8.137	8.115	1046699	250101	2.511	2.309
41)	L9 AR-1268-1	7.581	7.557	15576673	7081629	9.052	13.900 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091125\
Data File : P0113655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 12:12
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1254 40PPB WATER MDL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:10:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.661	7.600	995817	2503627	0.688	6.027 #
43)	L9 AR-1268-3	7.864	7.801	527644	300410	0.437	0.920 #
44)	L9 AR-1268-4	8.137	8.115	1046699	250101	2.272	2.077
45)	L9 AR-1268-5	8.424	8.387	1745441	317847	0.547	0.407 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091125\
Data File : PO113655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 12:12
Operator : YP/AJ
Sample : Q2893-07
Misc : AR1254 40PPB WATER MDL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:10:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

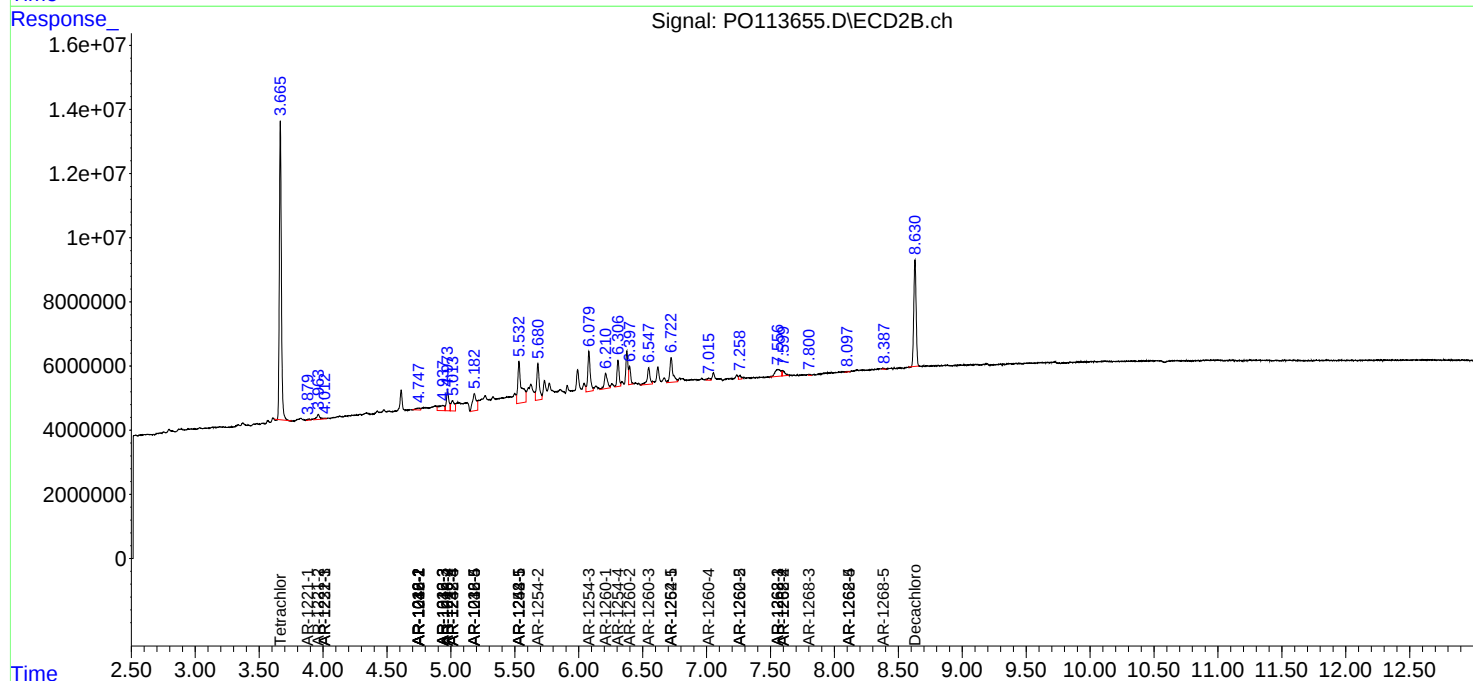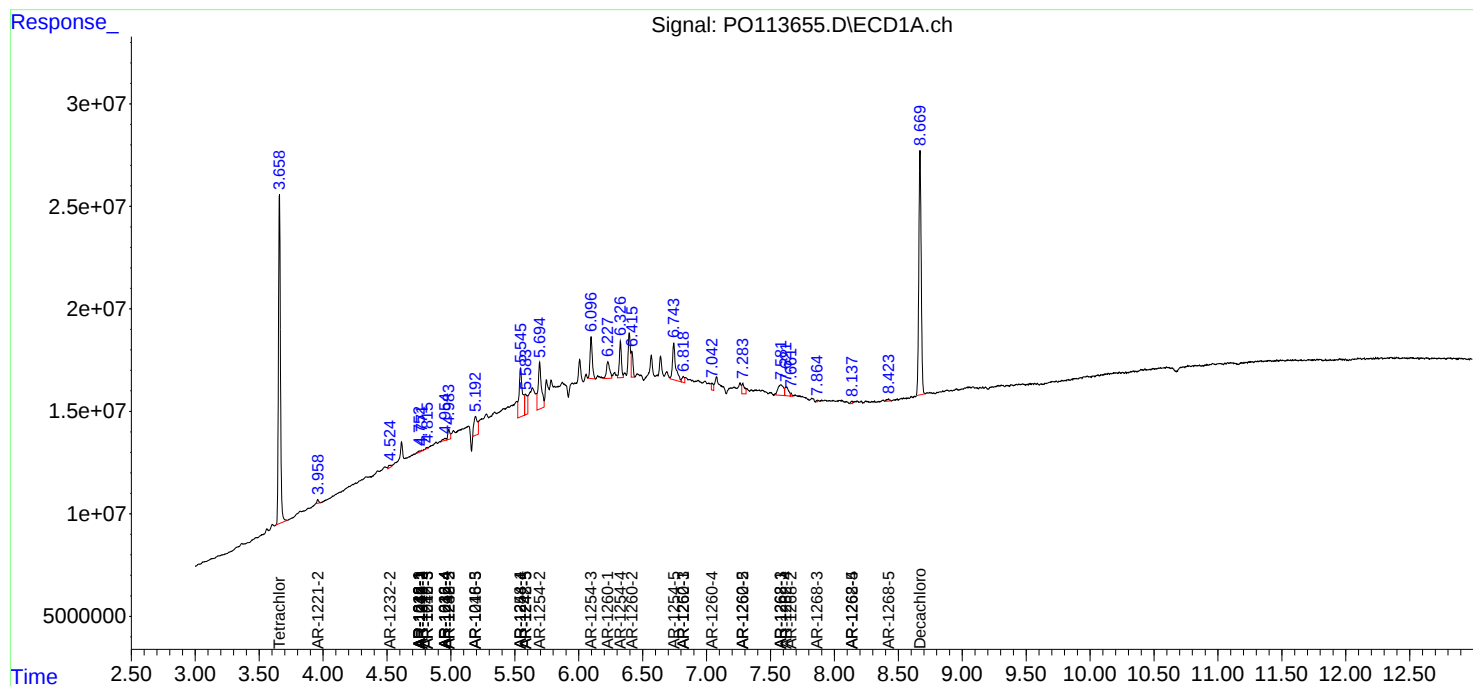


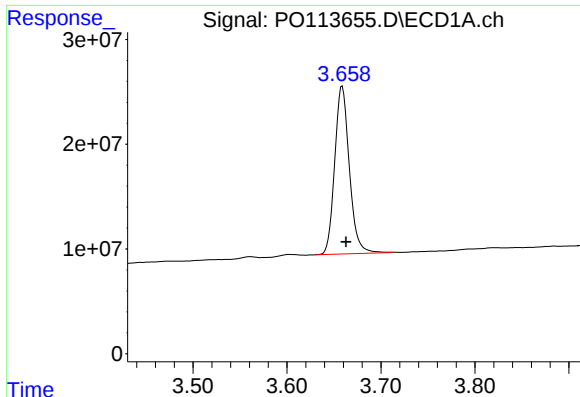

#1 Tetrachloro-m-xylene


R.T.: 3.659 min
Delta R.T.: -0.004 min
Response: 173318503
Conc: 21.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

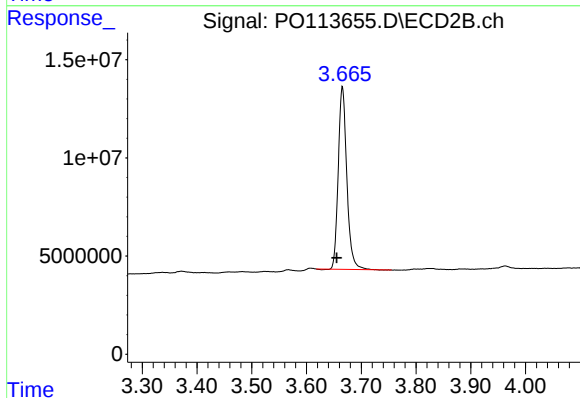


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: 0.011 min
Response: 101244947
Conc: 20.01 ng/ml

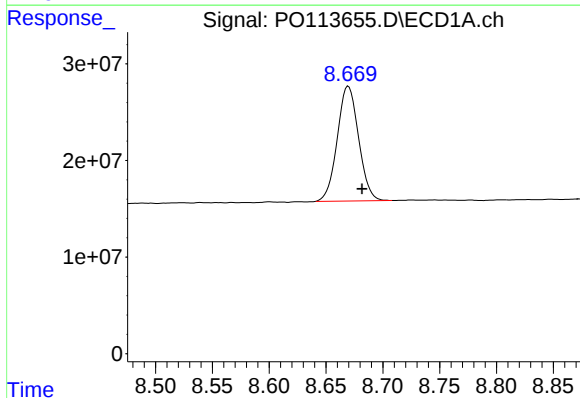


#2 Decachlorobiphenyl

R.T.: 8.670 min
Delta R.T.: -0.012 min
Response: 155283122
Conc: 22.40 ng/ml

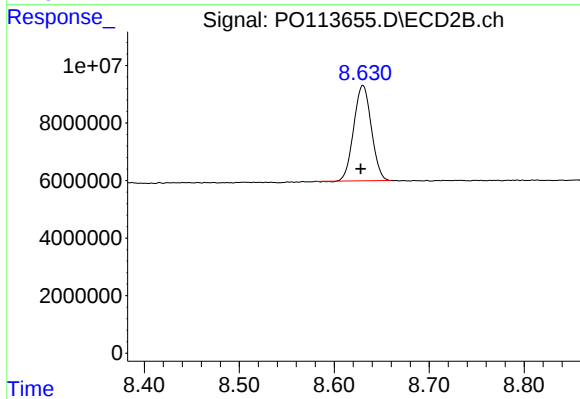

#2 Decachlorobiphenyl


R.T.: 8.630 min
Delta R.T.: 0.003 min
Response: 42731003
Conc: 22.55 ng/ml

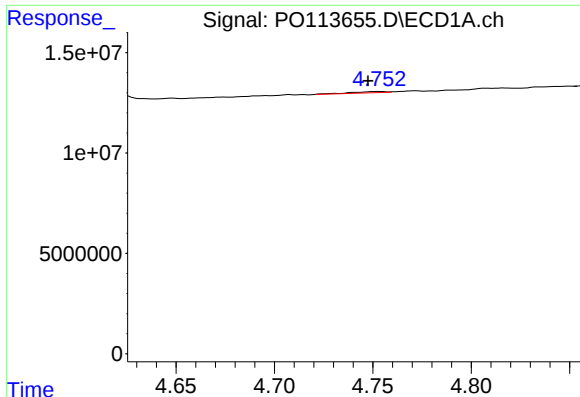

#3 AR-1016-1


R.T.: 4.753 min
Delta R.T.: 0.005 min
Response: 742920
Conc: 2.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

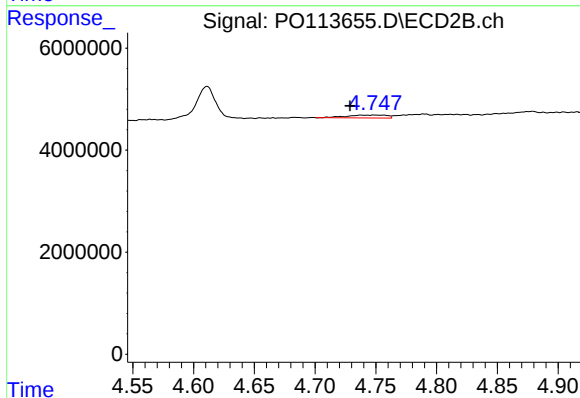


#3 AR-1016-1

R.T.: 4.738 min
Delta R.T.: 0.009 min
Response: 1311485
Conc: 7.69 ng/ml

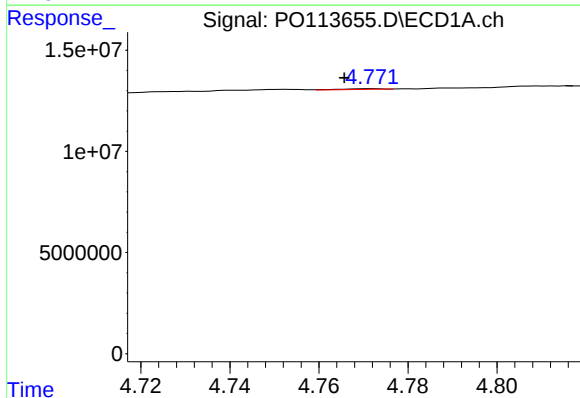


#4 AR-1016-2

R.T.: 4.772 min
Delta R.T.: 0.006 min
Response: 231127
Conc: 0.58 ng/ml

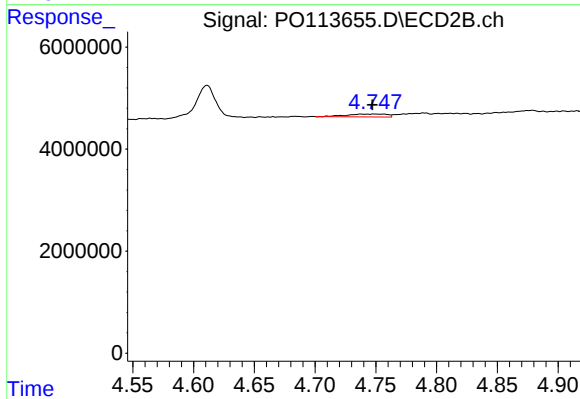

#4 AR-1016-2


R.T.: 4.738 min
Delta R.T.: -0.009 min
Response: 1311485
Conc: 5.09 ng/ml

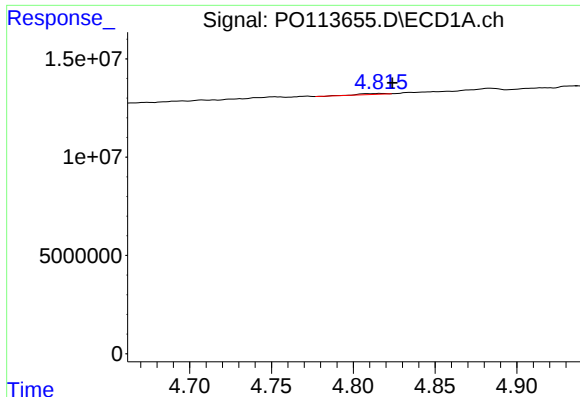

#5 AR-1016-3


R.T.: 4.817 min
Delta R.T.: -0.007 min
Response: 584519
Conc: 2.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

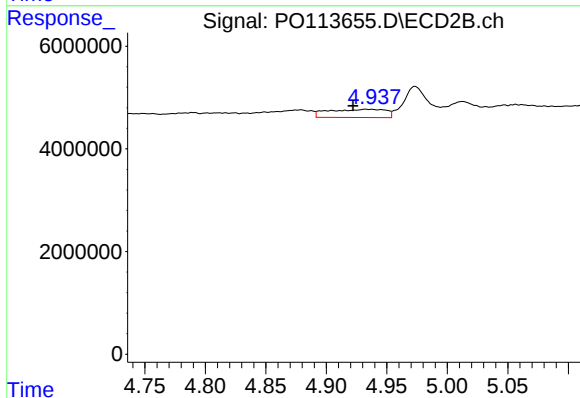


#5 AR-1016-3

R.T.: 4.938 min
Delta R.T.: 0.016 min
Response: 5290341
Conc: 37.89 ng/ml

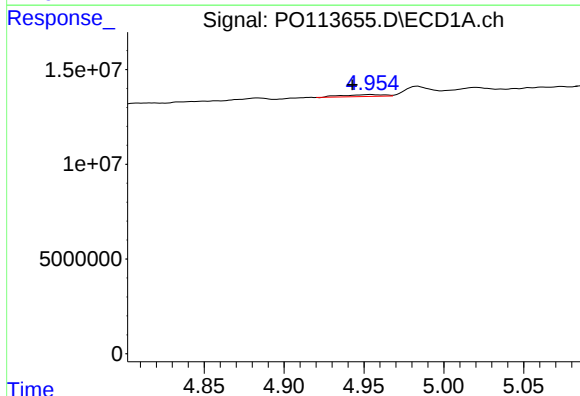


#6 AR-1016-4

R.T.: 4.954 min
Delta R.T.: 0.012 min
Response: 1829513
Conc: 8.39 ng/ml

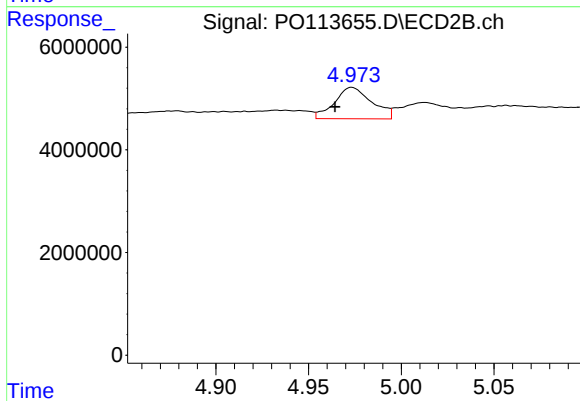

#6 AR-1016-4


R.T.: 4.973 min
Delta R.T.: 0.009 min
Response: 8597781
Conc: 73.67 ng/ml

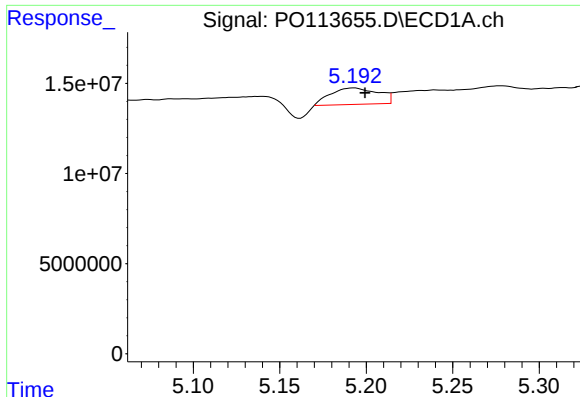

#7 AR-1016-5


R.T.: 5.193 min
Delta R.T.: -0.006 min
Response: 17550838
Conc: 79.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

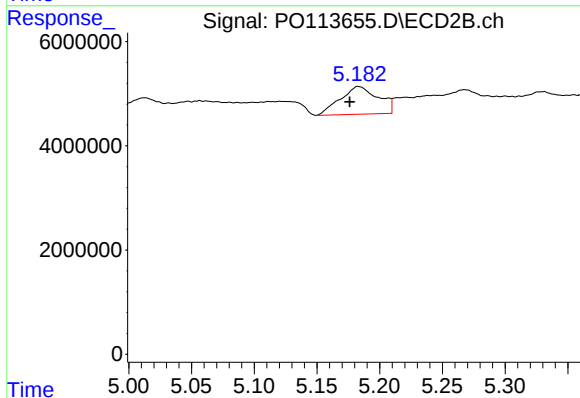


#7 AR-1016-5

R.T.: 5.183 min
Delta R.T.: 0.007 min
Response: 11200930
Conc: 78.59 ng/ml

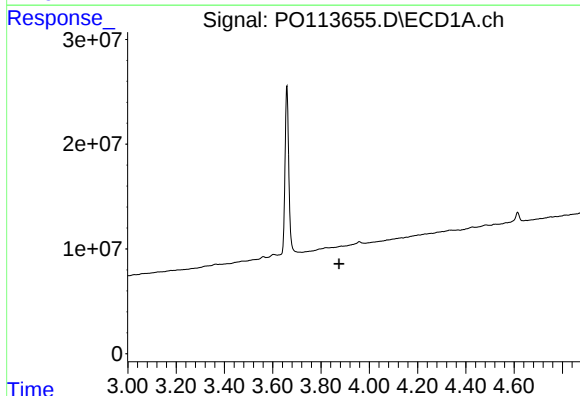


#8 AR-1221-1

R.T.: 3.884 min
Delta R.T.: 0.010 min
Response: -60102
Conc: N.D.

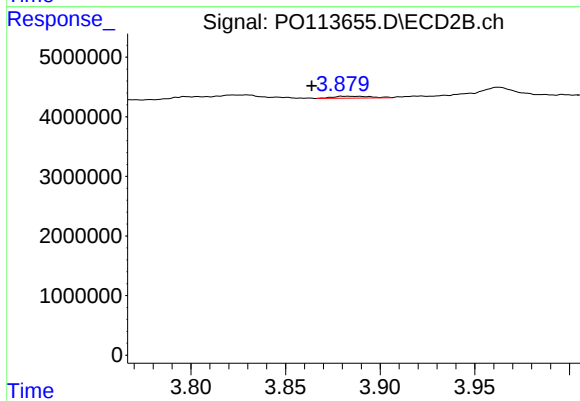

#8 AR-1221-1


R.T.: 3.881 min
Delta R.T.: 0.017 min
Response: 463808
Conc: 7.35 ng/ml

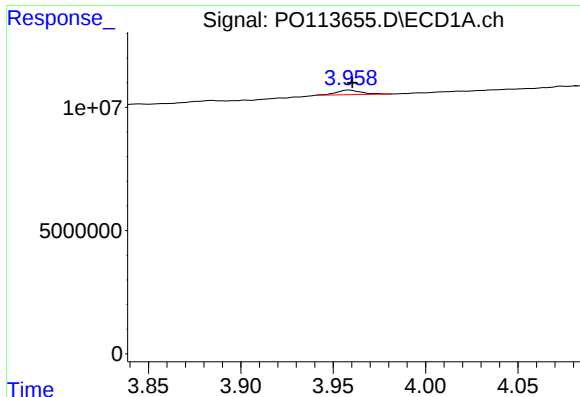

#9 AR-1221-2


R.T.: 3.959 min
Delta R.T.: -0.002 min
Response: 1791256
Conc: 26.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

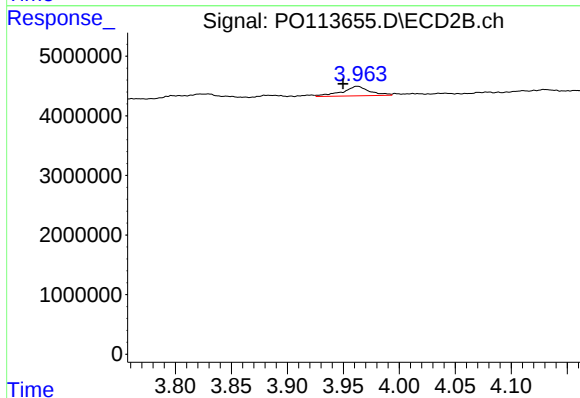


#9 AR-1221-2

R.T.: 3.963 min
Delta R.T.: 0.013 min
Response: 2680532
Conc: 57.43 ng/ml

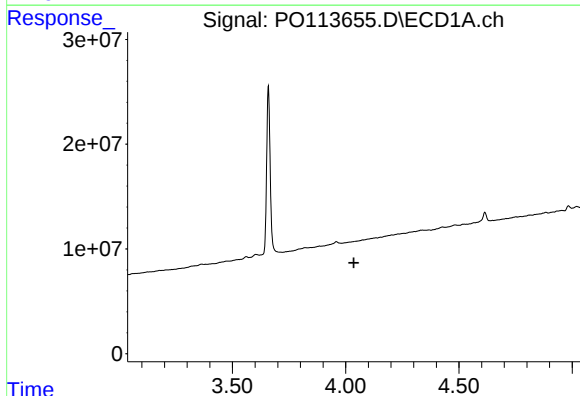


#10 AR-1221-3

R.T.: 4.074 min
Delta R.T.: 0.038 min
Response: -195590
Conc: N.D.

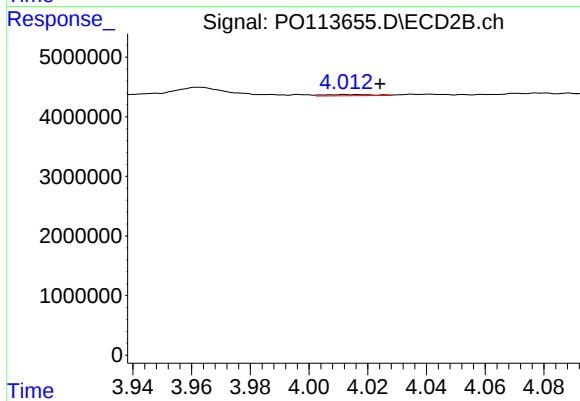

#10 AR-1221-3


R.T.: 4.012 min
Delta R.T.: -0.012 min
Response: 231737
Conc: 1.56 ng/ml

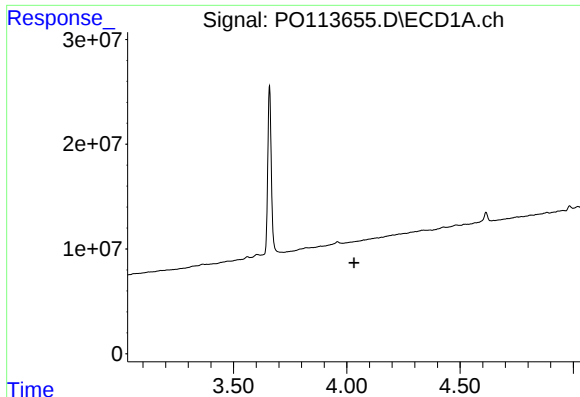

#11 AR-1232-1


R.T.: 4.074 min
Delta R.T.: 0.042 min
Response: -195590
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

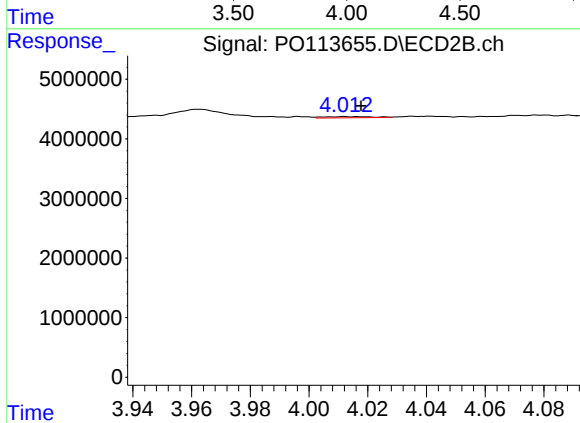


#11 AR-1232-1

R.T.: 4.012 min
Delta R.T.: -0.006 min
Response: 231737
Conc: 1.92 ng/ml

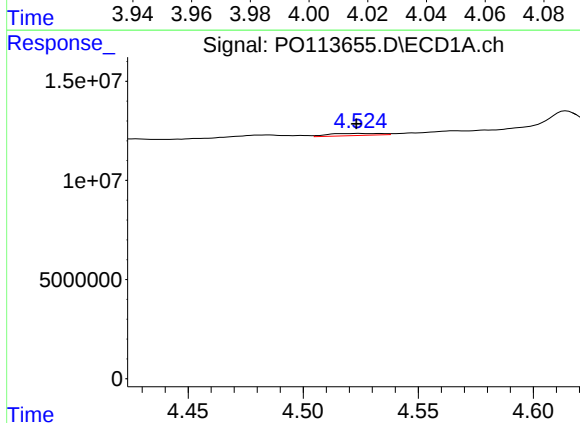


#12 AR-1232-2

R.T.: 4.525 min
Delta R.T.: 0.001 min
Response: 1706971
Conc: 15.82 ng/ml

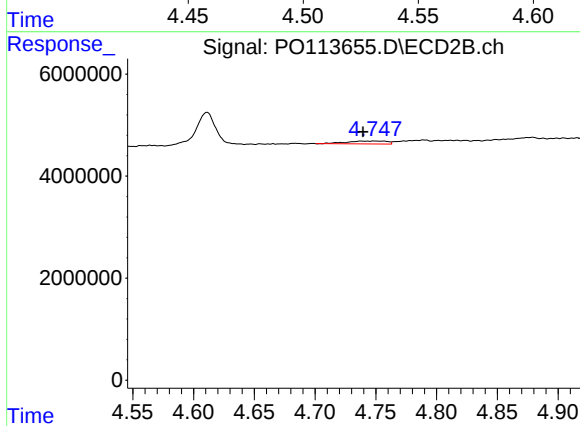

#12 AR-1232-2


R.T.: 4.738 min
Delta R.T.: -0.002 min
Response: 1311485
Conc: 10.75 ng/ml

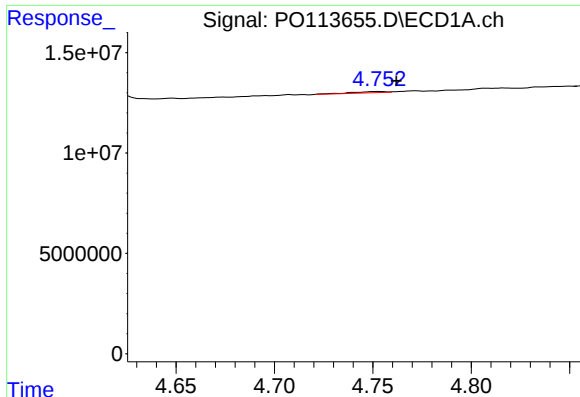

#13 AR-1232-3


R.T.: 4.753 min
Delta R.T.: -0.009 min
Response: 742920
Conc: 3.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

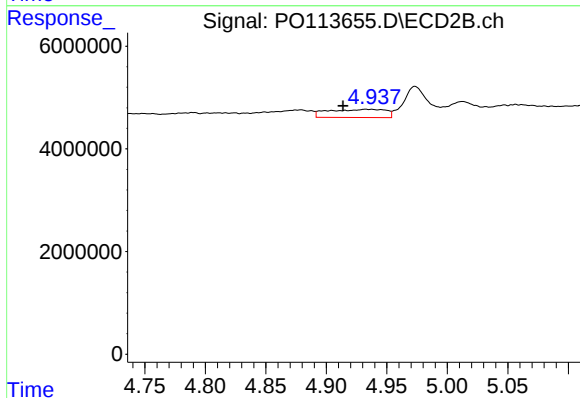


#13 AR-1232-3

R.T.: 4.938 min
Delta R.T.: 0.024 min
Response: 5290341
Conc: 79.97 ng/ml

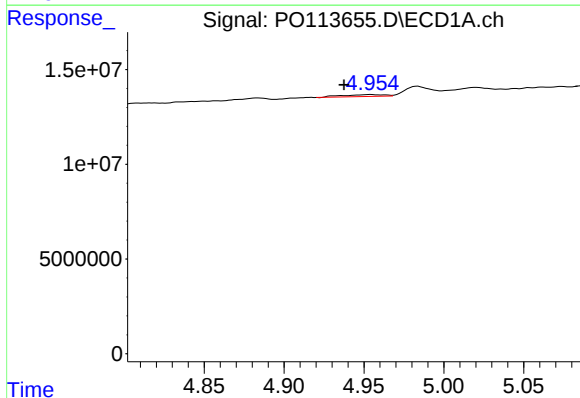


#14 AR-1232-4

R.T.: 4.954 min
Delta R.T.: 0.017 min
Response: 1829513
Conc: 18.61 ng/ml

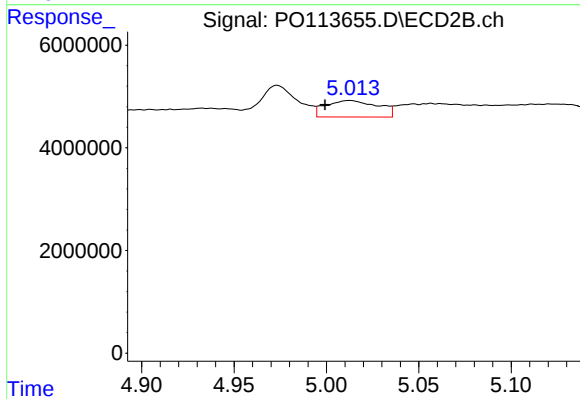

#14 AR-1232-4


R.T.: 5.013 min
Delta R.T.: 0.013 min
Response: 6329547
Conc: 105.62 ng/ml

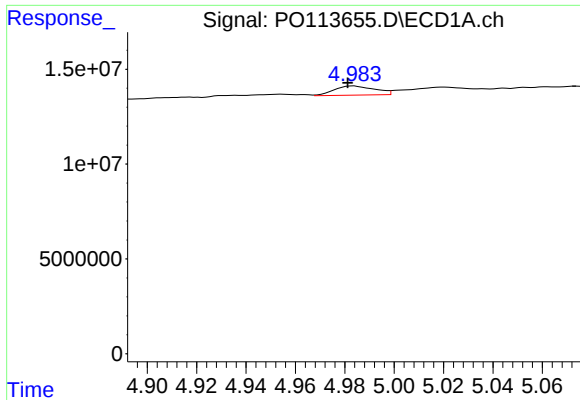

#15 AR-1232-5


R.T.: 4.983 min
Delta R.T.: 0.002 min
Response: 5558422
Conc: 84.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

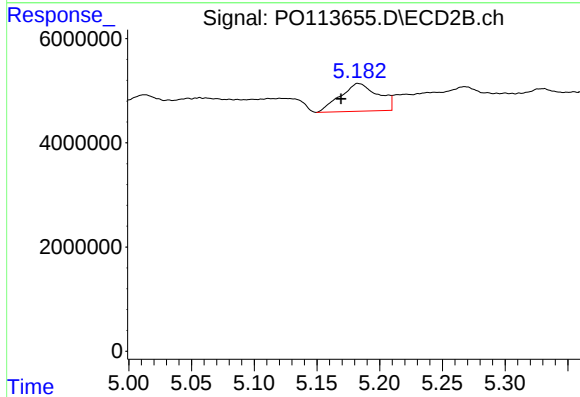


#15 AR-1232-5

R.T.: 5.183 min
Delta R.T.: 0.014 min
Response: 11200930
Conc: 165.65 ng/ml

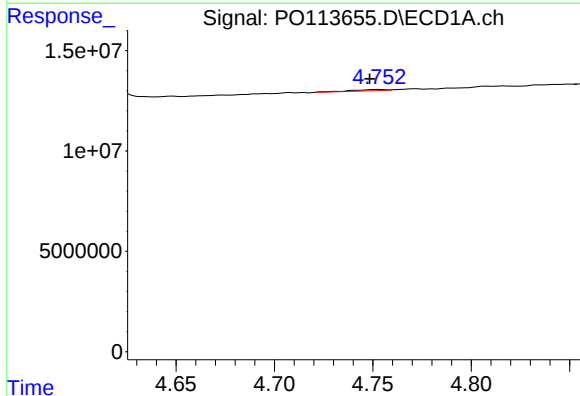


#16 AR-1242-1

R.T.: 4.753 min
Delta R.T.: 0.004 min
Response: 742920
Conc: 3.23 ng/ml

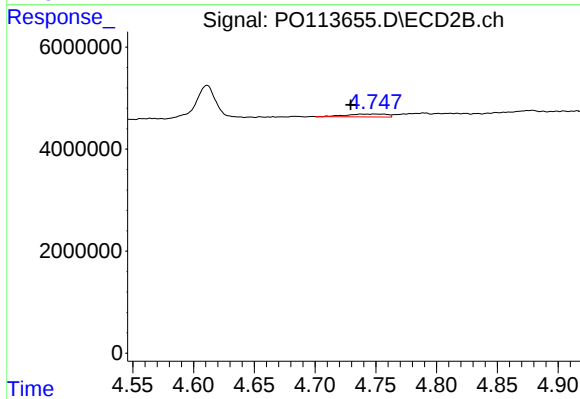

#16 AR-1242-1


R.T.: 4.738 min
Delta R.T.: 0.009 min
Response: 1311485
Conc: 9.08 ng/ml

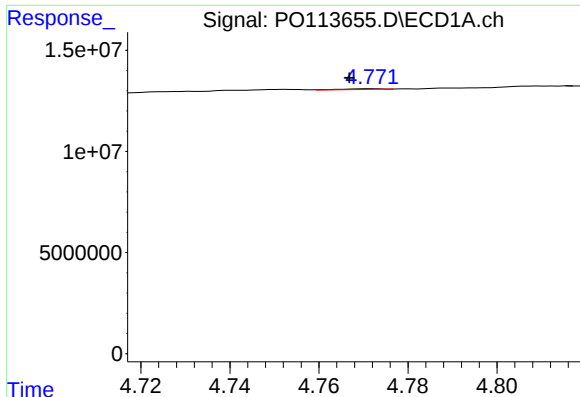

#17 AR-1242-2


R.T.: 4.772 min
Delta R.T.: 0.005 min
Response: 231127
Conc: 0.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

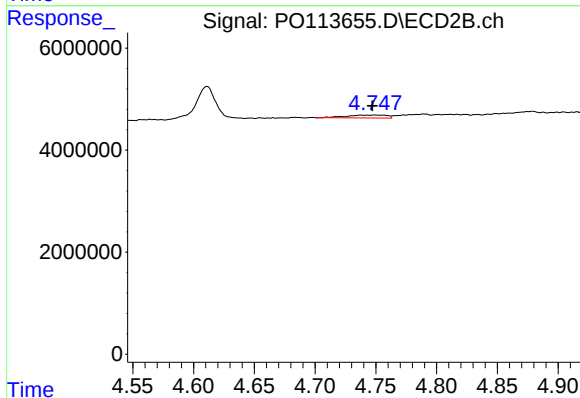


#17 AR-1242-2

R.T.: 4.738 min
Delta R.T.: -0.009 min
Response: 1311485
Conc: 6.05 ng/ml

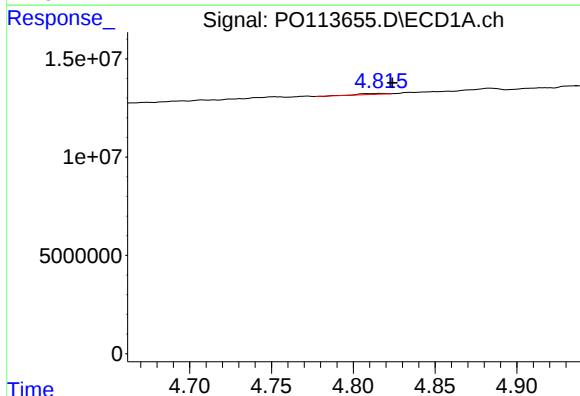


#18 AR-1242-3

R.T.: 4.817 min
Delta R.T.: -0.007 min
Response: 584519
Conc: 2.63 ng/ml

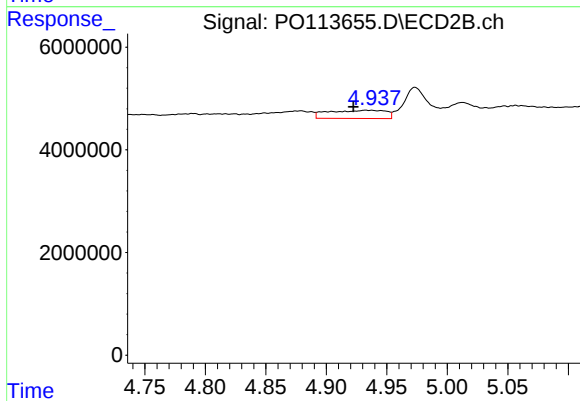

#18 AR-1242-3


R.T.: 4.938 min
Delta R.T.: 0.015 min
Response: 5290341
Conc: 45.23 ng/ml

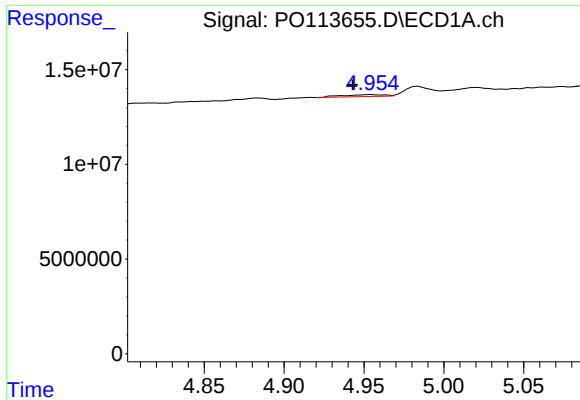

#19 AR-1242-4


R.T.: 4.954 min
Delta R.T.: 0.011 min
Response: 1829513
Conc: 10.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

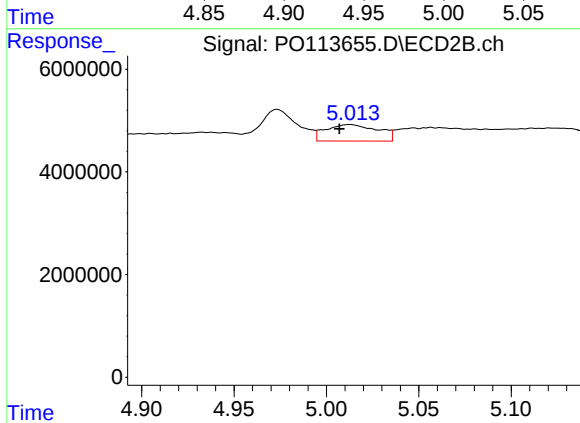


#19 AR-1242-4

R.T.: 5.013 min
Delta R.T.: 0.006 min
Response: 6329547
Conc: 53.81 ng/ml

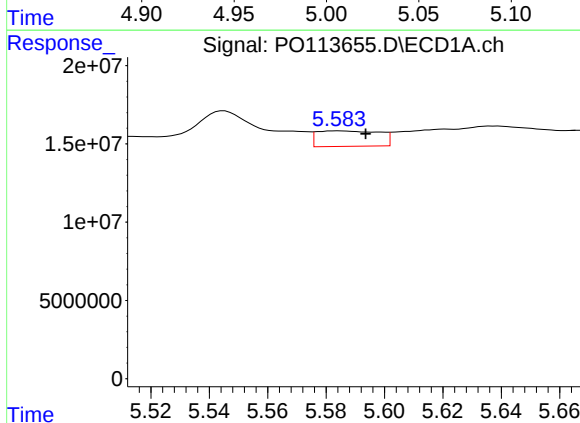


#20 AR-1242-5

R.T.: 5.584 min
Delta R.T.: -0.010 min
Response: 14749518
Conc: 73.69 ng/ml

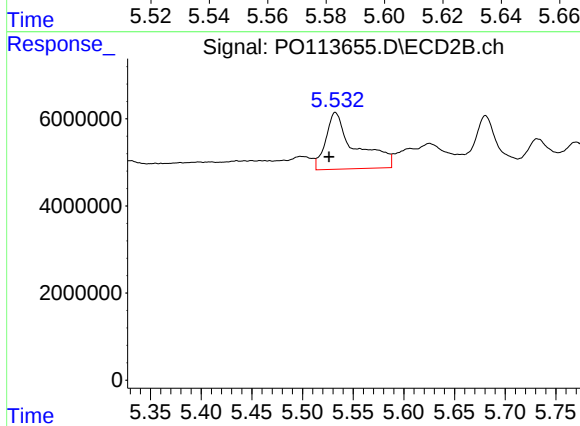

#20 AR-1242-5


R.T.: 5.532 min
Delta R.T.: 0.006 min
Response: 26376305
Conc: 176.86 ng/ml

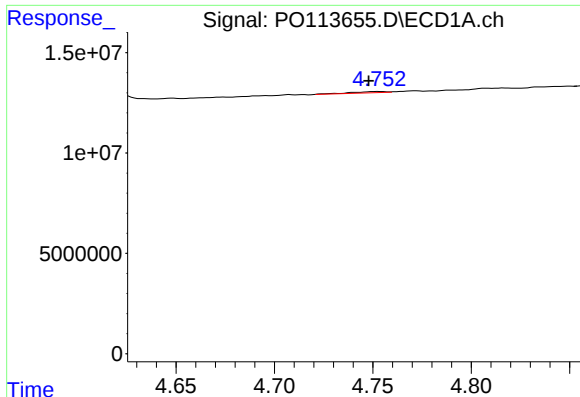

#21 AR-1248-1


R.T.: 4.753 min
Delta R.T.: 0.005 min
Response: 742920
Conc: 4.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

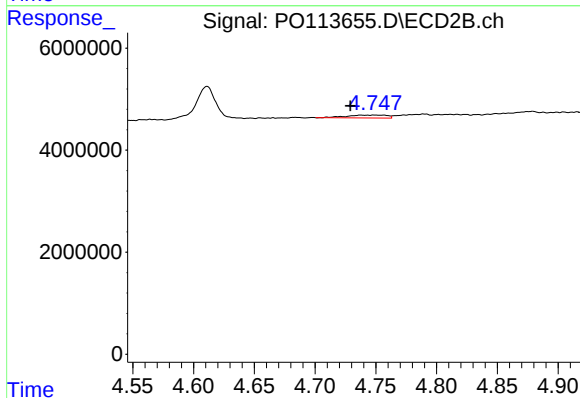


#21 AR-1248-1

R.T.: 4.738 min
Delta R.T.: 0.009 min
Response: 1311485
Conc: 11.76 ng/ml

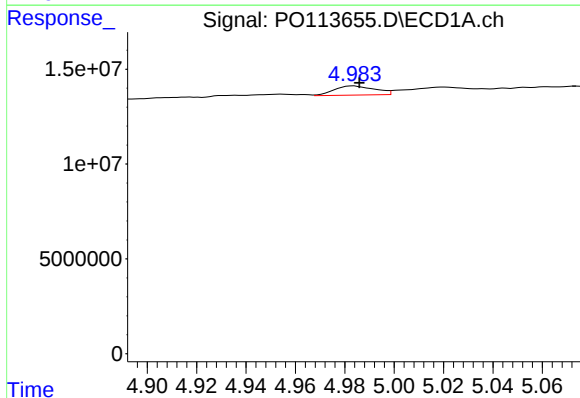


#22 AR-1248-2

R.T.: 4.983 min
Delta R.T.: -0.002 min
Response: 5558422
Conc: 22.98 ng/ml

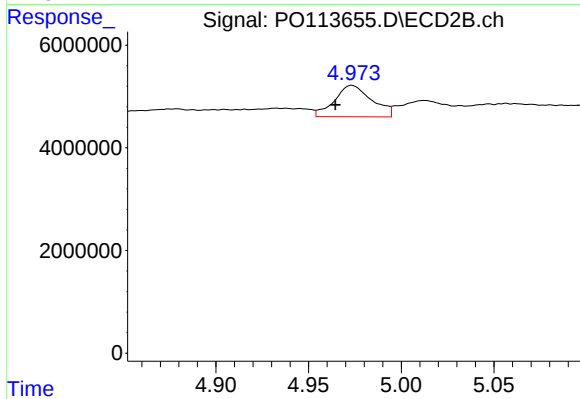

#22 AR-1248-2


R.T.: 4.973 min
Delta R.T.: 0.009 min
Response: 8597781
Conc: 53.50 ng/ml

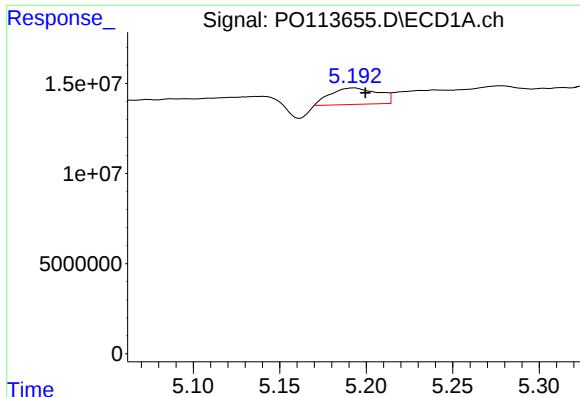

#23 AR-1248-3


R.T.: 5.193 min
Delta R.T.: -0.007 min
Response: 17550838
Conc: 55.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

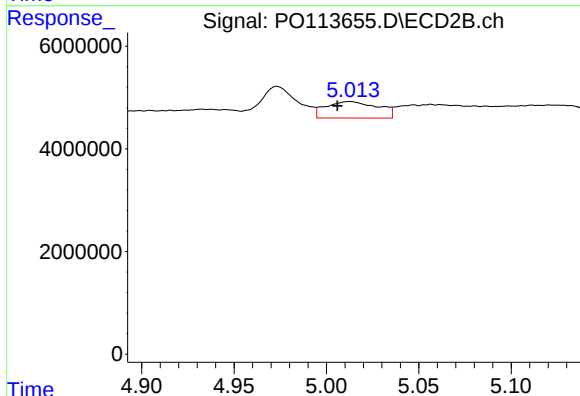


#23 AR-1248-3

R.T.: 5.013 min
Delta R.T.: 0.007 min
Response: 6329547
Conc: 37.31 ng/ml

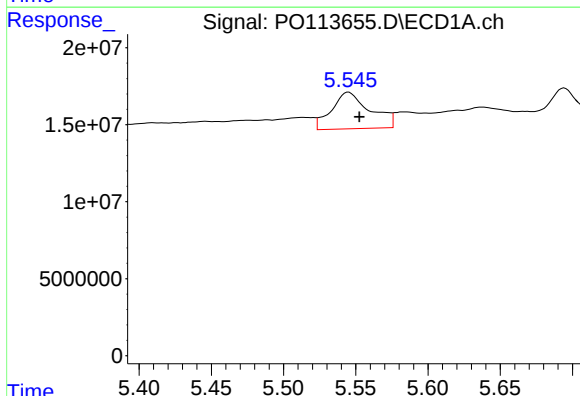


#24 AR-1248-4

R.T.: 5.545 min
Delta R.T.: -0.007 min
Response: 44087760
Conc: 88.25 ng/ml

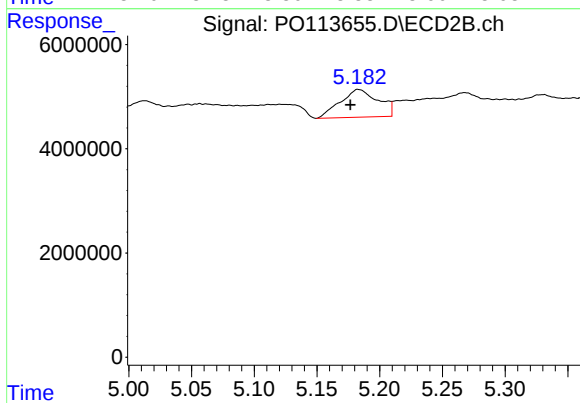

#24 AR-1248-4


R.T.: 5.183 min
Delta R.T.: 0.007 min
Response: 11200930
Conc: 56.22 ng/ml

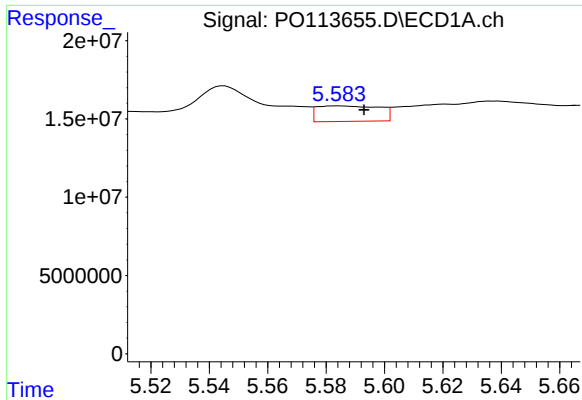

#25 AR-1248-5


R.T.: 5.584 min
Delta R.T.: -0.009 min
Response: 14749518
Conc: 43.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

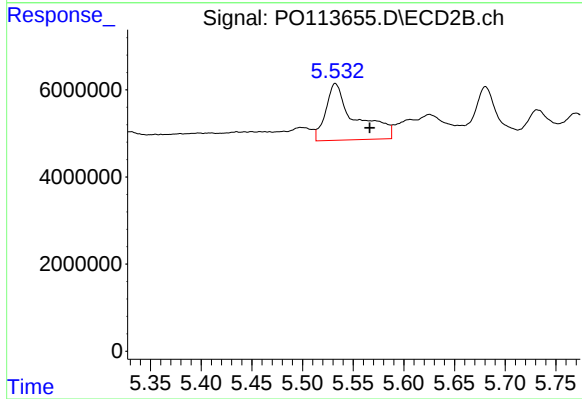


#25 AR-1248-5

R.T.: 5.532 min
Delta R.T.: -0.034 min
Response: 26376305
Conc: 124.24 ng/ml

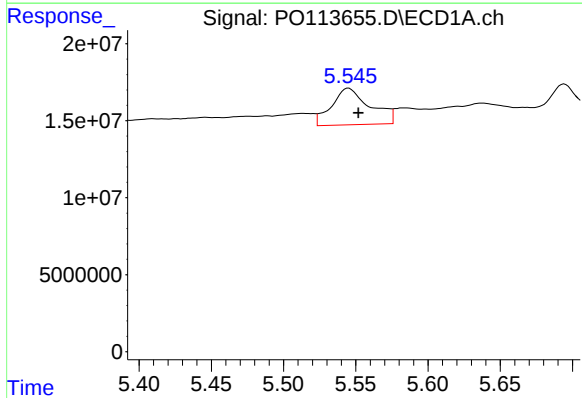


#26 AR-1254-1

R.T.: 5.545 min
Delta R.T.: -0.007 min
Response: 44087760
Conc: 81.65 ng/ml

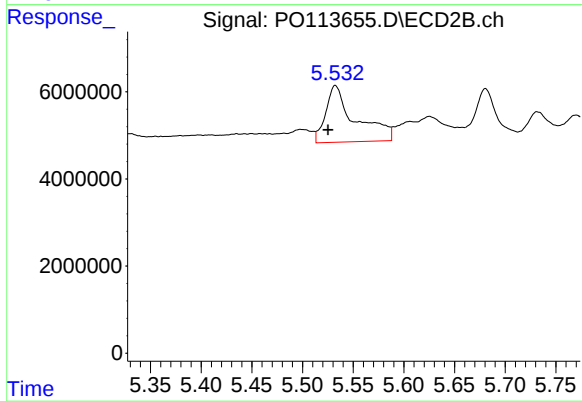

#26 AR-1254-1


R.T.: 5.532 min
Delta R.T.: 0.007 min
Response: 26376305
Conc: 83.64 ng/ml

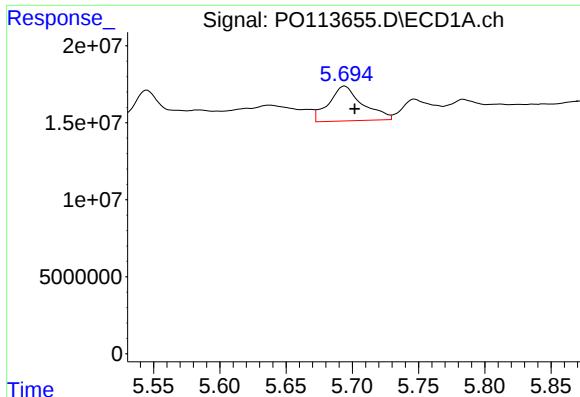

#27 AR-1254-2


R.T.: 5.694 min
Delta R.T.: -0.007 min
Response: 40164602
Conc: 81.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

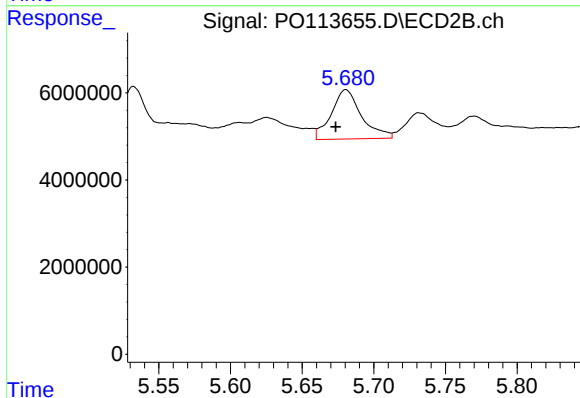


#27 AR-1254-2

R.T.: 5.681 min
Delta R.T.: 0.007 min
Response: 16597175
Conc: 59.20 ng/ml

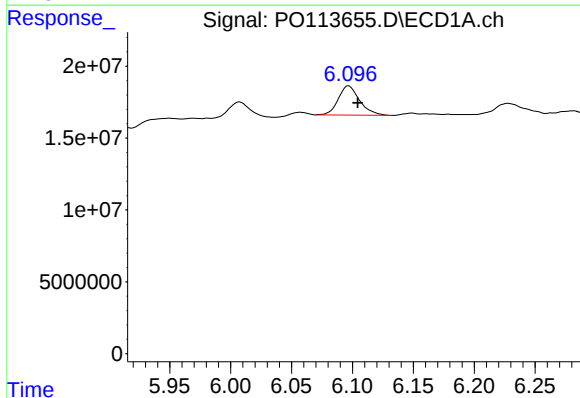


#28 AR-1254-3

R.T.: 6.097 min
Delta R.T.: -0.008 min
Response: 24777796
Conc: 33.53 ng/ml

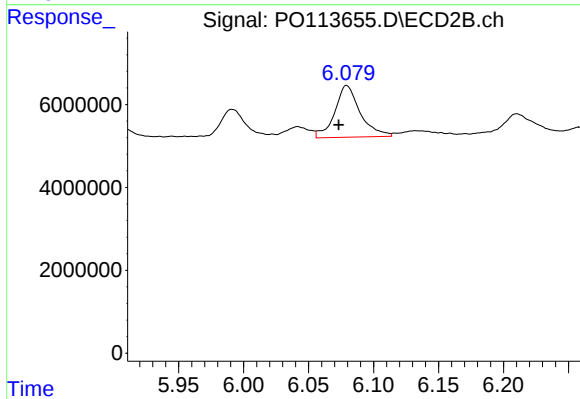

#28 AR-1254-3


R.T.: 6.079 min
Delta R.T.: 0.006 min
Response: 17075359
Conc: 40.96 ng/ml

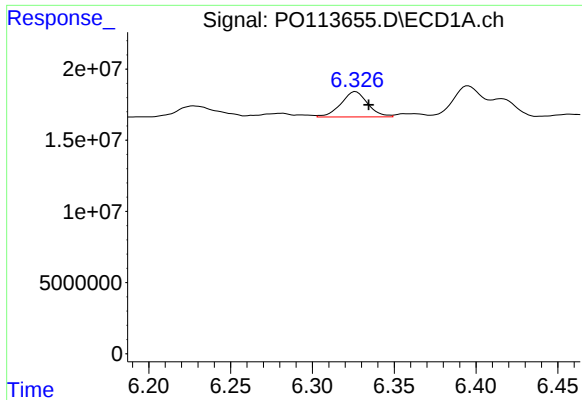

#29 AR-1254-4


R.T.: 6.326 min
Delta R.T.: -0.008 min
Response: 20217355
Conc: 36.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

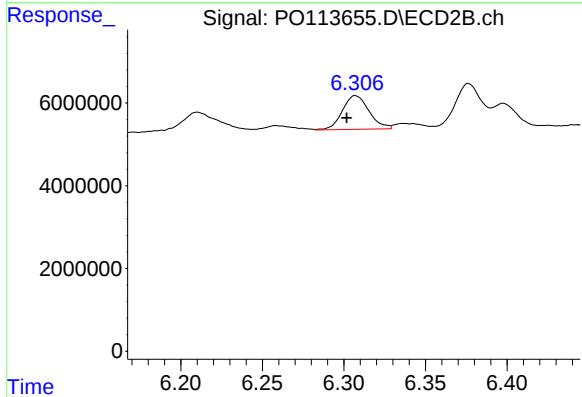


#29 AR-1254-4

R.T.: 6.307 min
Delta R.T.: 0.005 min
Response: 9306936
Conc: 33.86 ng/ml

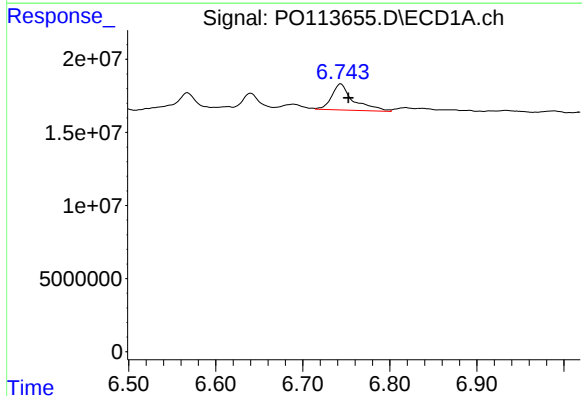


#30 AR-1254-5

R.T.: 6.744 min
Delta R.T.: -0.009 min
Response: 30970179
Conc: 44.18 ng/ml

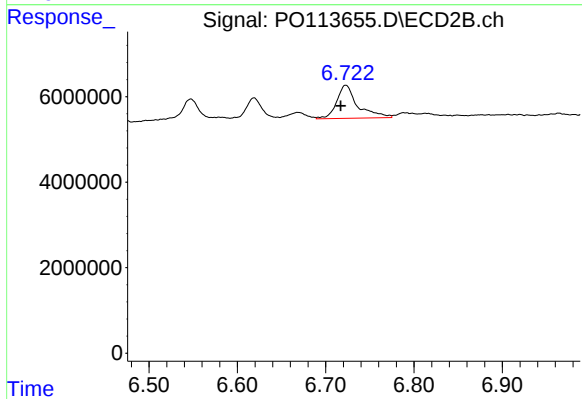

#30 AR-1254-5


R.T.: 6.723 min
Delta R.T.: 0.006 min
Response: 12829781
Conc: 35.89 ng/ml

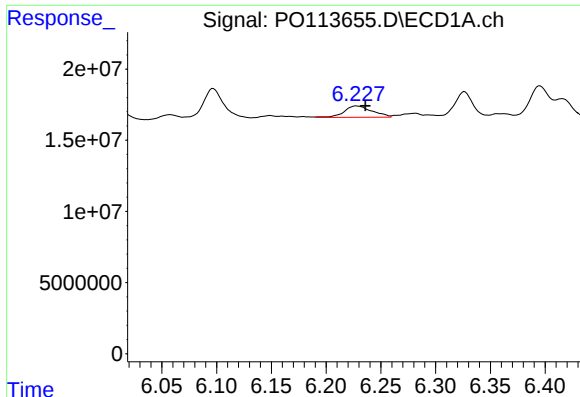

#31 AR-1260-1


R.T.: 6.228 min
Delta R.T.: -0.008 min
Response: 14377541
Conc: 32.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

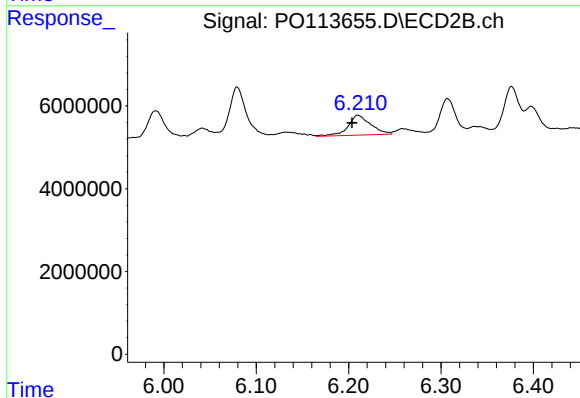


#31 AR-1260-1

R.T.: 6.210 min
Delta R.T.: 0.007 min
Response: 8163717
Conc: 32.01 ng/ml

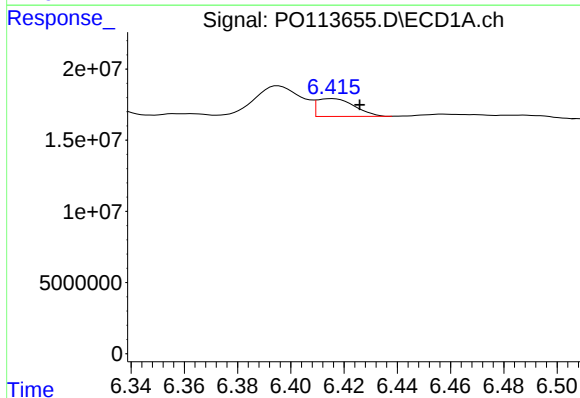


#32 AR-1260-2

R.T.: 6.415 min
Delta R.T.: -0.010 min
Response: 12271084
Conc: 17.87 ng/ml

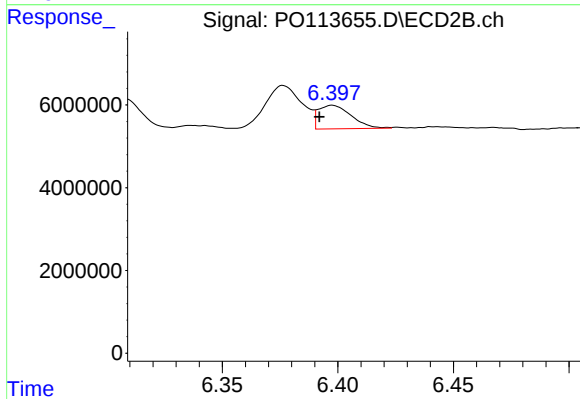

#32 AR-1260-2


R.T.: 6.398 min
Delta R.T.: 0.006 min
Response: 5655626
Conc: 16.36 ng/ml

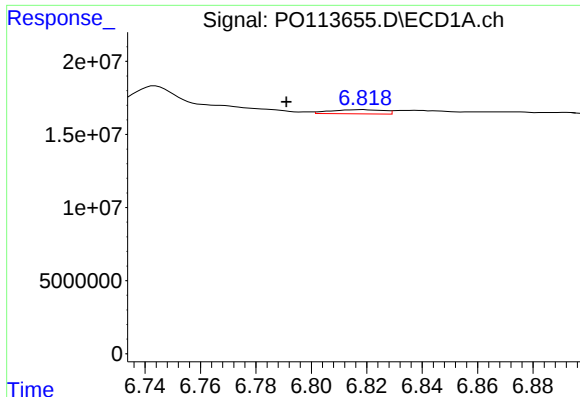

#33 AR-1260-3


R.T.: 6.819 min
Delta R.T.: 0.028 min
Response: 3707615
Conc: 6.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

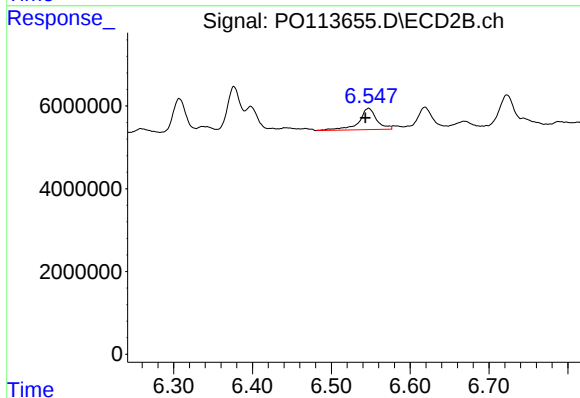


#33 AR-1260-3

R.T.: 6.547 min
Delta R.T.: 0.004 min
Response: 8100426
Conc: 27.23 ng/ml

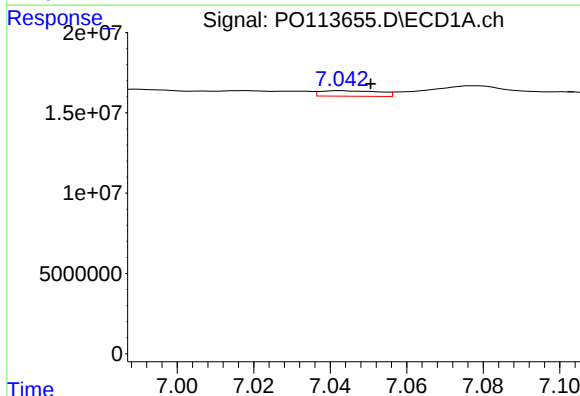


#34 AR-1260-4

R.T.: 7.043 min
Delta R.T.: -0.008 min
Response: 3666901
Conc: 8.19 ng/ml

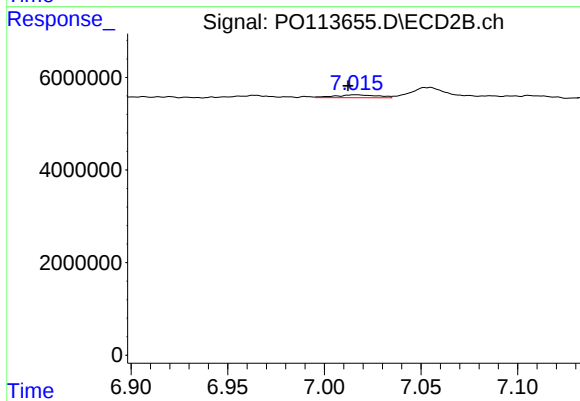

#34 AR-1260-4


R.T.: 7.016 min
Delta R.T.: 0.004 min
Response: 982450
Conc: 4.74 ng/ml

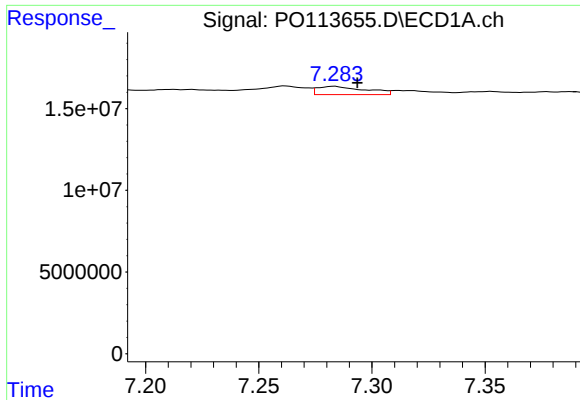

#35 AR-1260-5


R.T.: 7.283 min
Delta R.T.: -0.010 min
Response: 7472852
Conc: 6.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

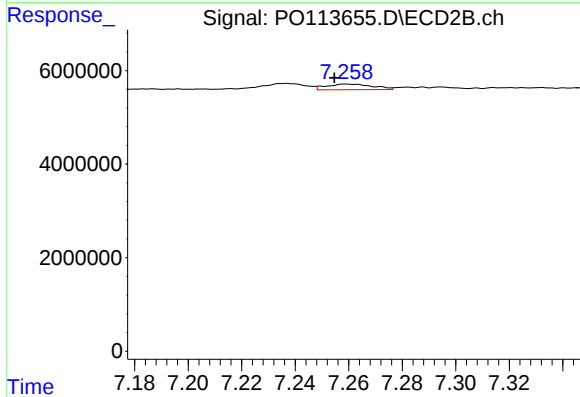


#35 AR-1260-5

R.T.: 7.259 min
Delta R.T.: 0.005 min
Response: 1441964
Conc: 3.08 ng/ml

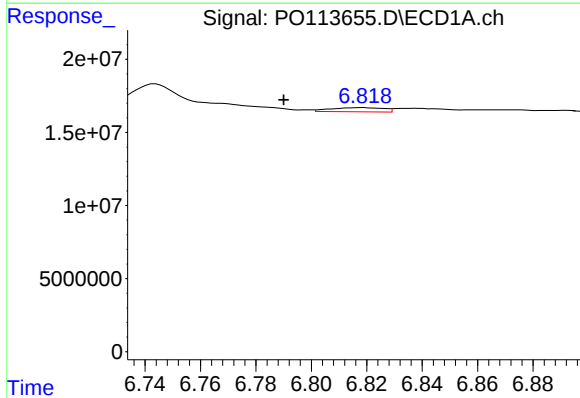


#36 AR-1262-1

R.T.: 6.819 min
Delta R.T.: 0.029 min
Response: 3707615
Conc: 4.05 ng/ml

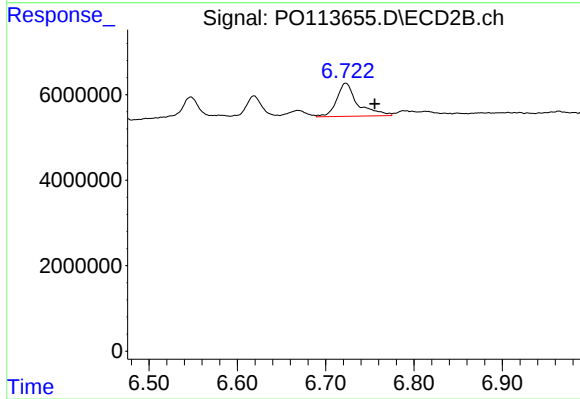

#36 AR-1262-1


R.T.: 6.723 min
Delta R.T.: -0.033 min
Response: 12829781
Conc: 30.94 ng/ml

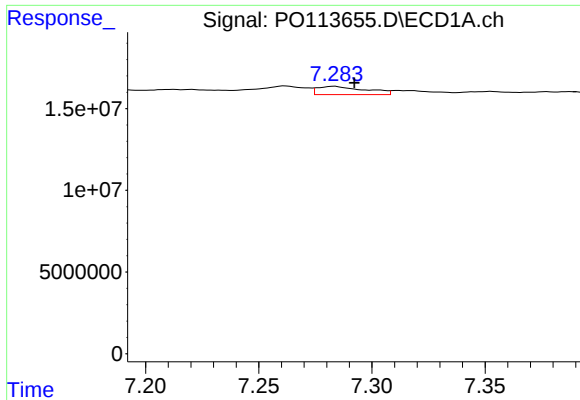

#37 AR-1262-2


R.T.: 7.283 min
Delta R.T.: -0.009 min
Response: 7472852
Conc: 4.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

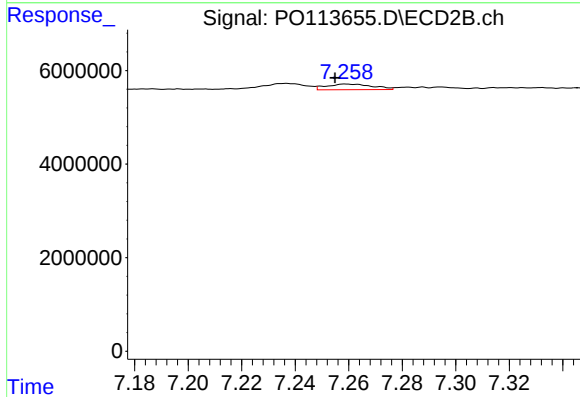


#37 AR-1262-2

R.T.: 7.259 min
Delta R.T.: 0.004 min
Response: 1441964
Conc: 2.79 ng/ml

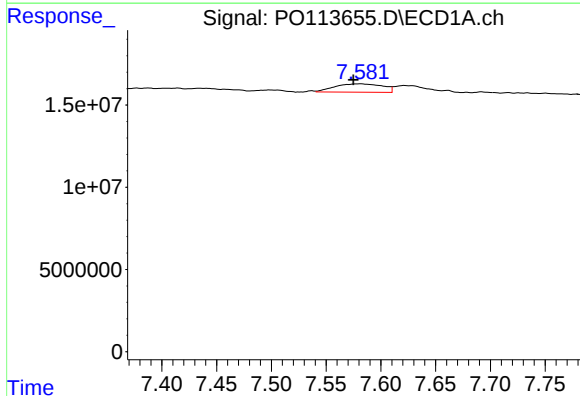


#38 AR-1262-3

R.T.: 7.581 min
Delta R.T.: 0.007 min
Response: 15576673
Conc: 28.11 ng/ml

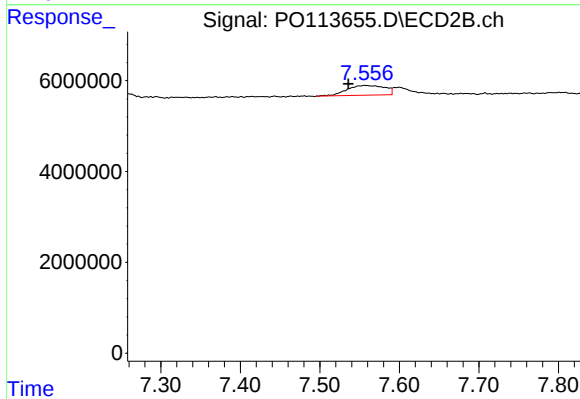

#38 AR-1262-3


R.T.: 7.557 min
Delta R.T.: 0.021 min
Response: 7081629
Conc: 39.43 ng/ml

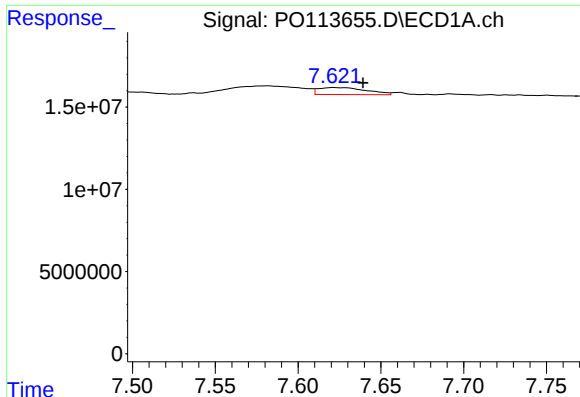

#39 AR-1262-4


R.T.: 7.621 min
Delta R.T.: -0.018 min
Response: 8693599
Conc: 8.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

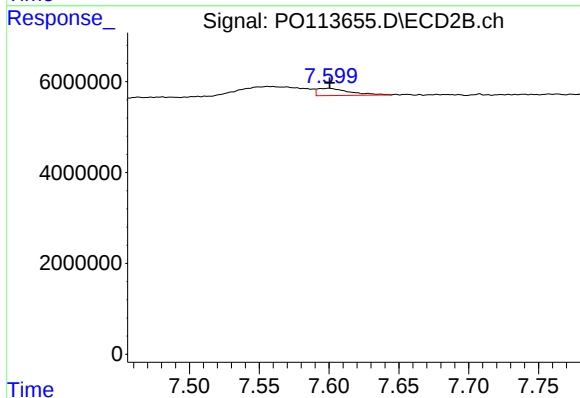


#39 AR-1262-4

R.T.: 7.600 min
Delta R.T.: 0.000 min
Response: 2503627
Conc: 8.64 ng/ml

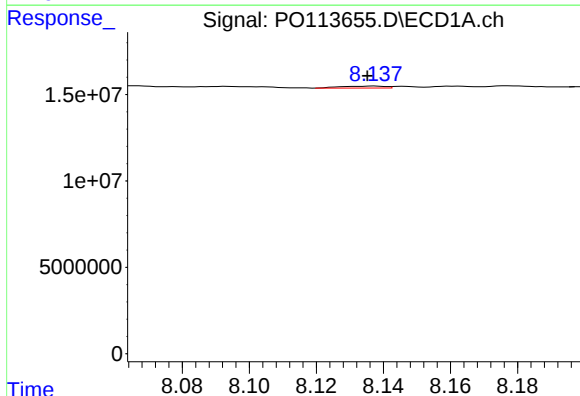


#40 AR-1262-5

R.T.: 8.137 min
Delta R.T.: 0.002 min
Response: 1046699
Conc: 2.51 ng/ml

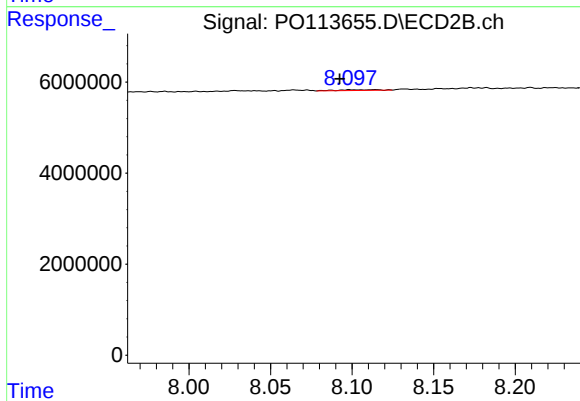

#40 AR-1262-5


R.T.: 8.115 min
Delta R.T.: 0.022 min
Response: 250101
Conc: 2.31 ng/ml

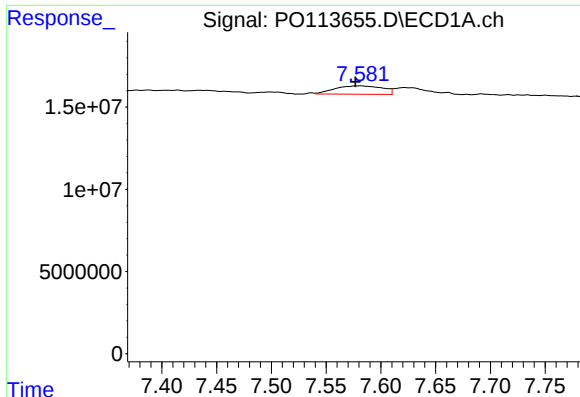

#41 AR-1268-1


R.T.: 7.581 min
Delta R.T.: 0.004 min
Response: 15576673
Conc: 9.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

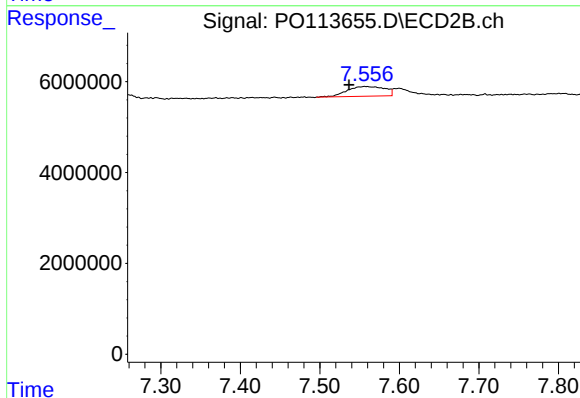


#41 AR-1268-1

R.T.: 7.557 min
Delta R.T.: 0.020 min
Response: 7081629
Conc: 13.90 ng/ml

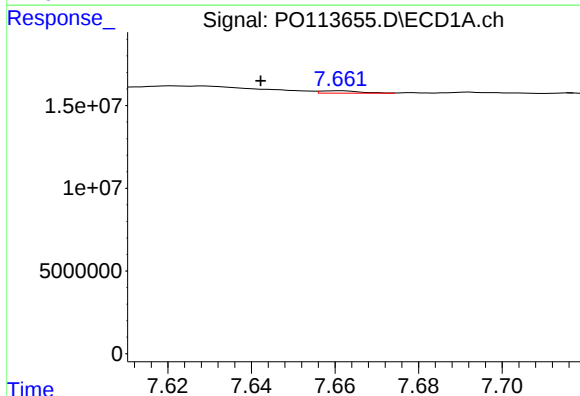


#42 AR-1268-2

R.T.: 7.661 min
Delta R.T.: 0.019 min
Response: 995817
Conc: 0.69 ng/ml

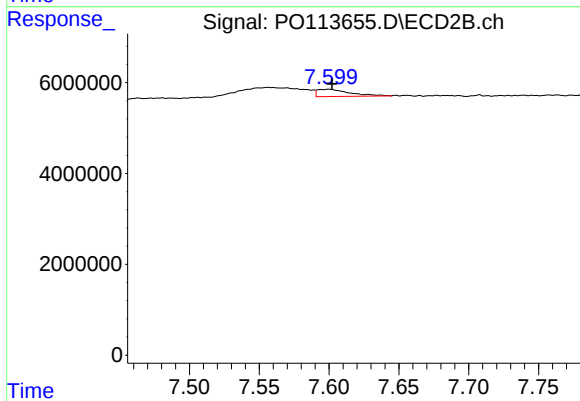

#42 AR-1268-2


R.T.: 7.600 min
Delta R.T.: -0.002 min
Response: 2503627
Conc: 6.03 ng/ml

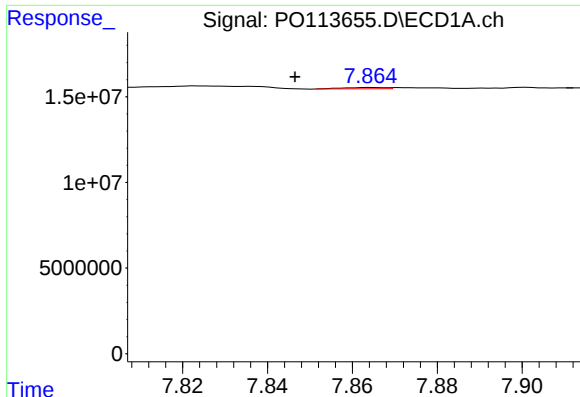

#43 AR-1268-3


R.T.: 7.864 min
Delta R.T.: 0.018 min
Response: 527644
Conc: 0.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

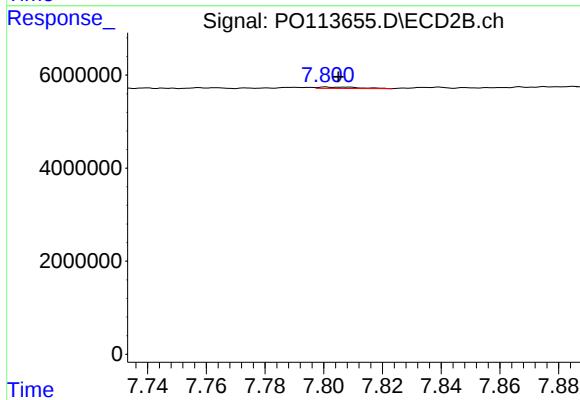


#43 AR-1268-3

R.T.: 7.801 min
Delta R.T.: -0.004 min
Response: 300410
Conc: 0.92 ng/ml

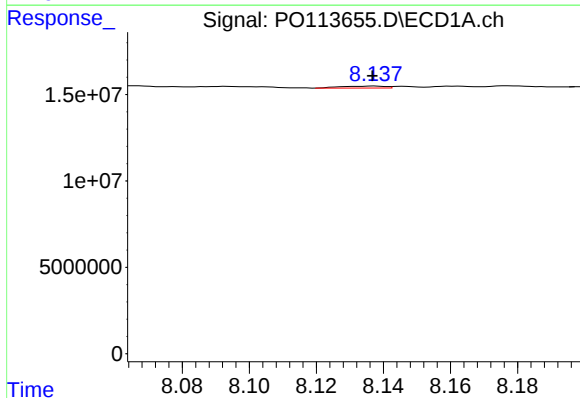


#44 AR-1268-4

R.T.: 8.137 min
Delta R.T.: 0.000 min
Response: 1046699
Conc: 2.27 ng/ml

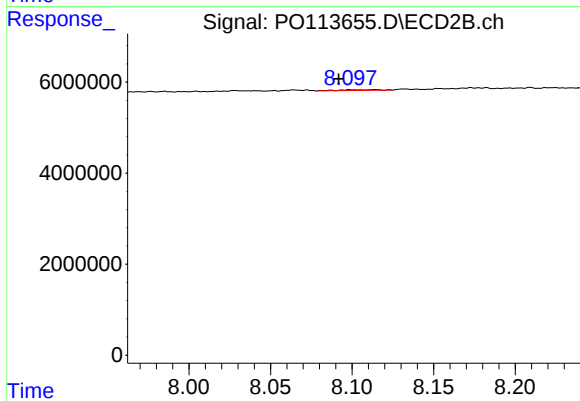

#44 AR-1268-4


R.T.: 8.115 min
Delta R.T.: 0.023 min
Response: 250101
Conc: 2.08 ng/ml

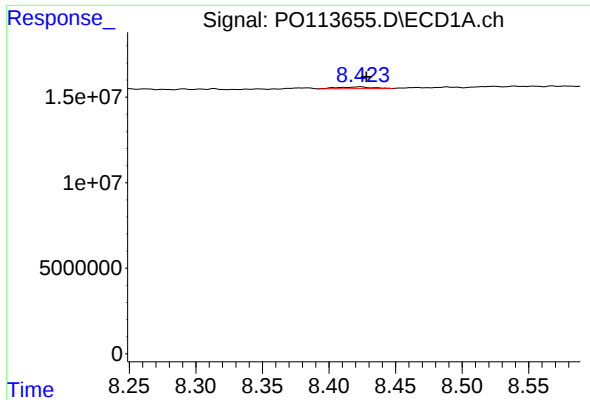

#45 AR-1268-5

R.T.: 8.424 min
Delta R.T.: -0.004 min
Response: 1745441
Conc: 0.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

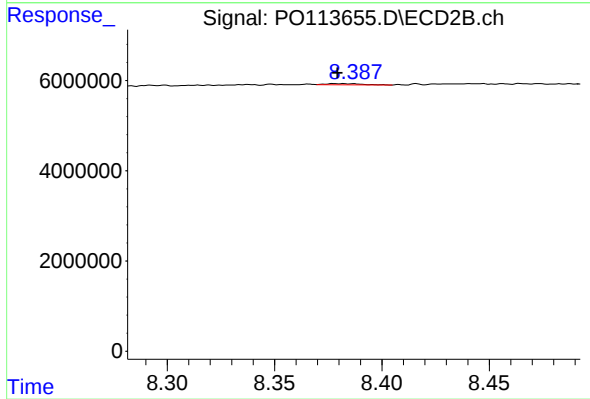

#45 AR-1268-5

R.T.: 8.387 min
Delta R.T.: 0.007 min
Response: 317847
Conc: 0.41 ng/ml