

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091125\
 Data File : P0113668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 17:25
 Operator : YP/AJ
 Sample : Q3055-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-03-090925

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/11/2025
 Supervised By :mohammad ahmed 09/15/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 02:13:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.656	3.648	176.9E6	104.8E6	21.605m	20.712
2) SA Decachlor...	8.669	8.614	104.4E6	31944765	15.062	16.859

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091125\
Data File : PO113668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 17:25
Operator : YP/AJ
Sample : Q3055-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-03-090925


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2025
Supervised By :mohammad ahmed 09/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:13:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

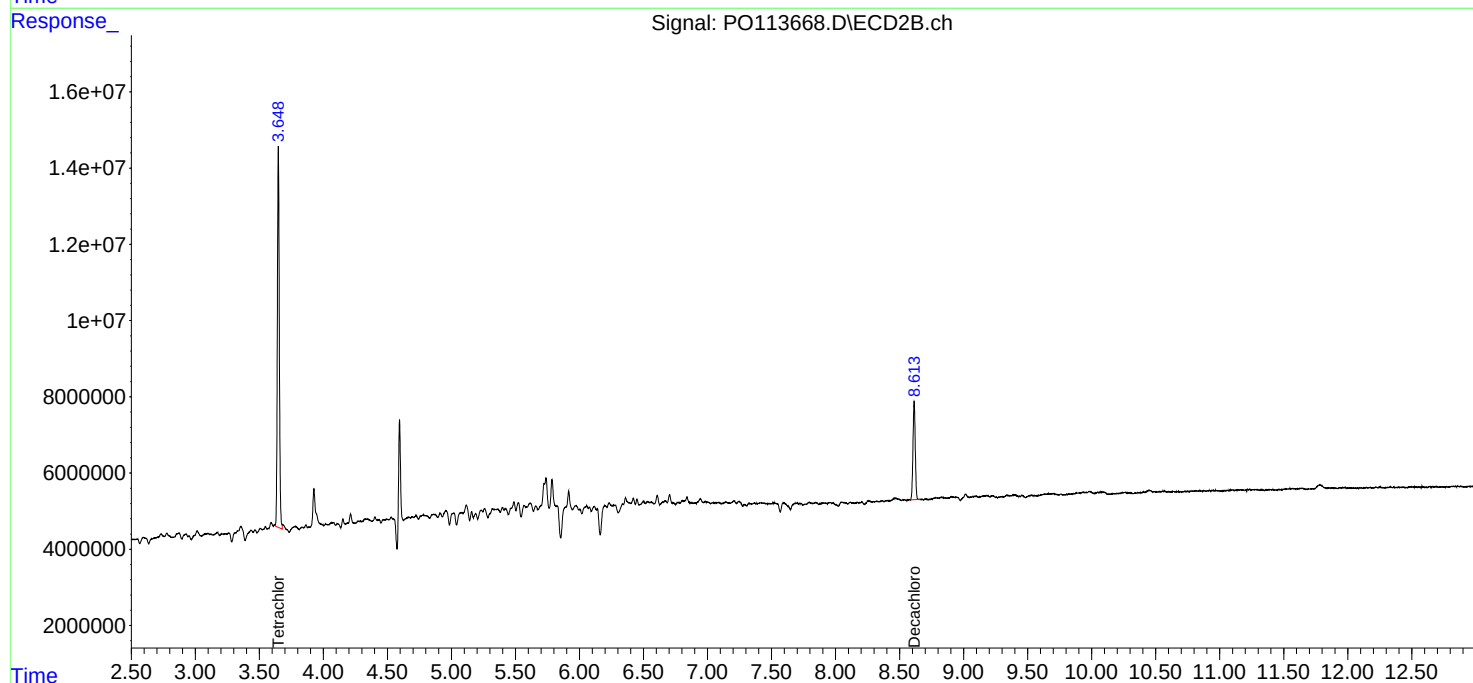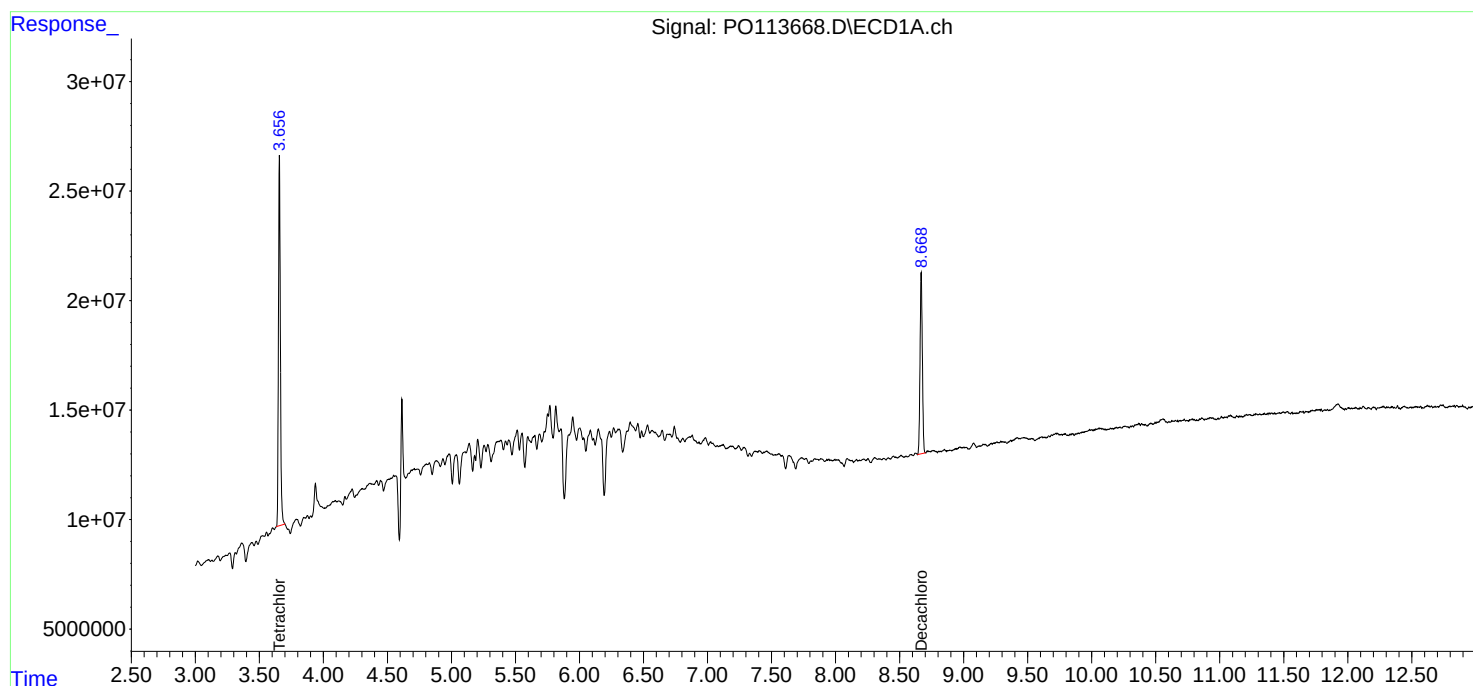

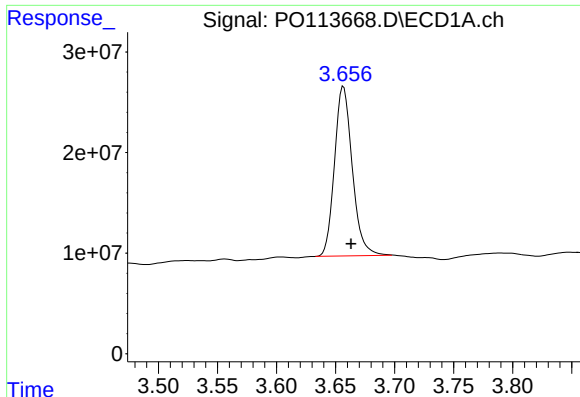

#1 Tetrachloro-m-xylene

R.T.: 3.656 min
Delta R.T.: -0.007 min
Response: 176870175
Conc: 21.60 ng/ml

Instrument :


ECD_O

ClientSampleId :

OR-03-090925


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2025
Supervised By :mohammad ahmed 09/15/2025

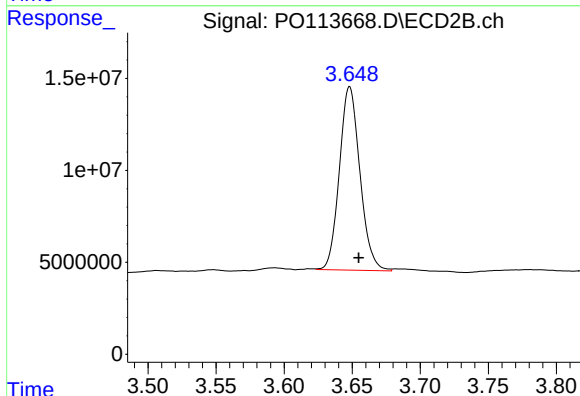


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: -0.007 min
Response: 104816726
Conc: 20.71 ng/ml

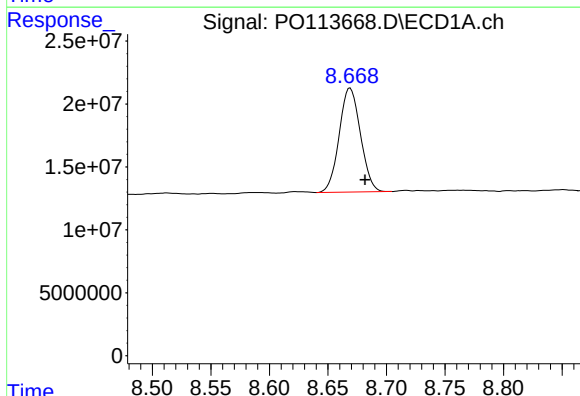

#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.013 min
Response: 104404356
Conc: 15.06 ng/ml

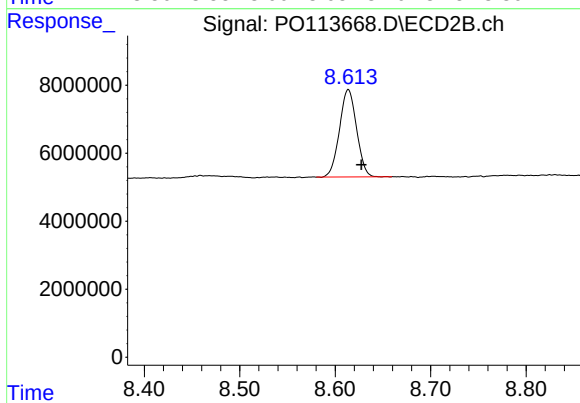

#2 Decachlorobiphenyl

R.T.: 8.614 min
Delta R.T.: -0.014 min
Response: 31944765
Conc: 16.86 ng/ml