

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091125\
 Data File : P0113669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 17:43
 Operator : YP/AJ
 Sample : Q3056-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-02-090925

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/11/2025
 Supervised By :mohammad ahmed 09/15/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 02:14:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.657	3.648	155.1E6	92564772	18.951m	18.291m
2) SA Decachlor...	8.669	8.614	106.1E6	34203861	15.313	18.051

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091125\
Data File : PO113669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 17:43
Operator : YP/AJ
Sample : Q3056-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-02-090925


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2025
Supervised By :mohammad ahmed 09/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:14:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

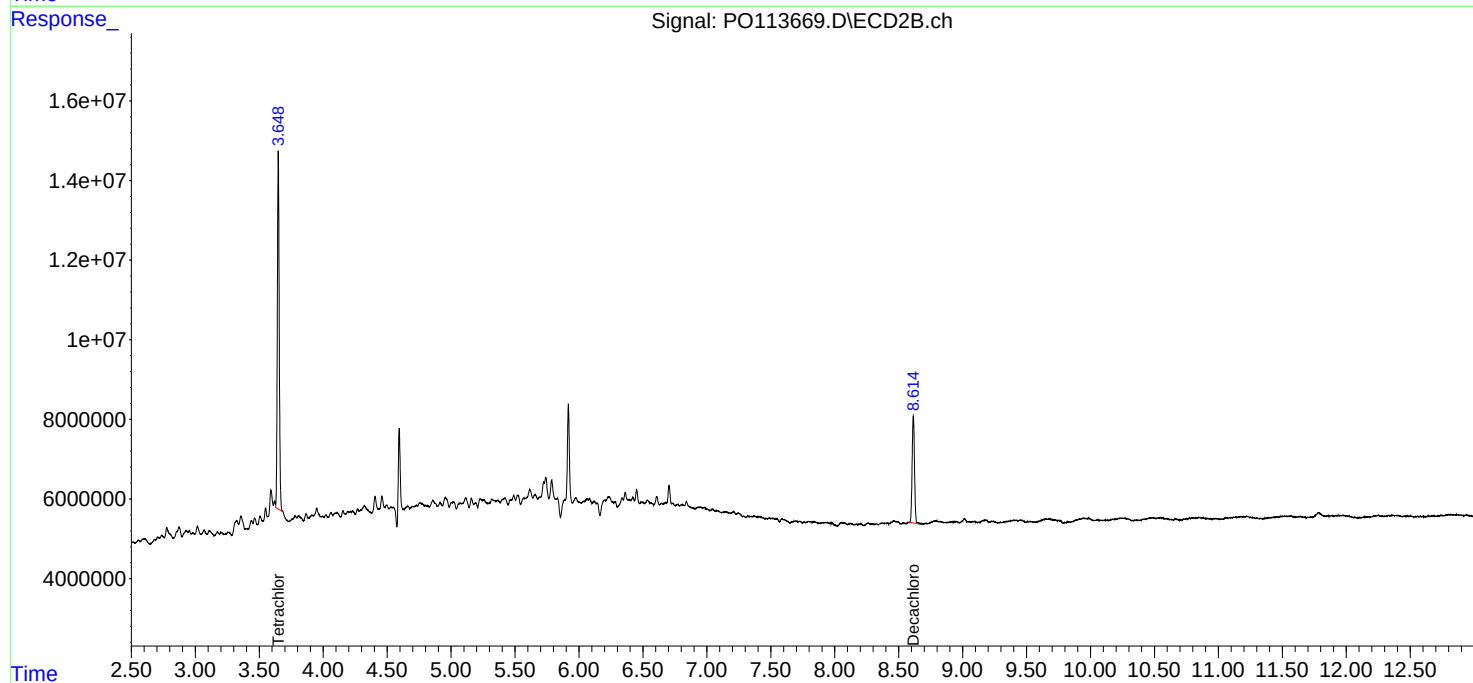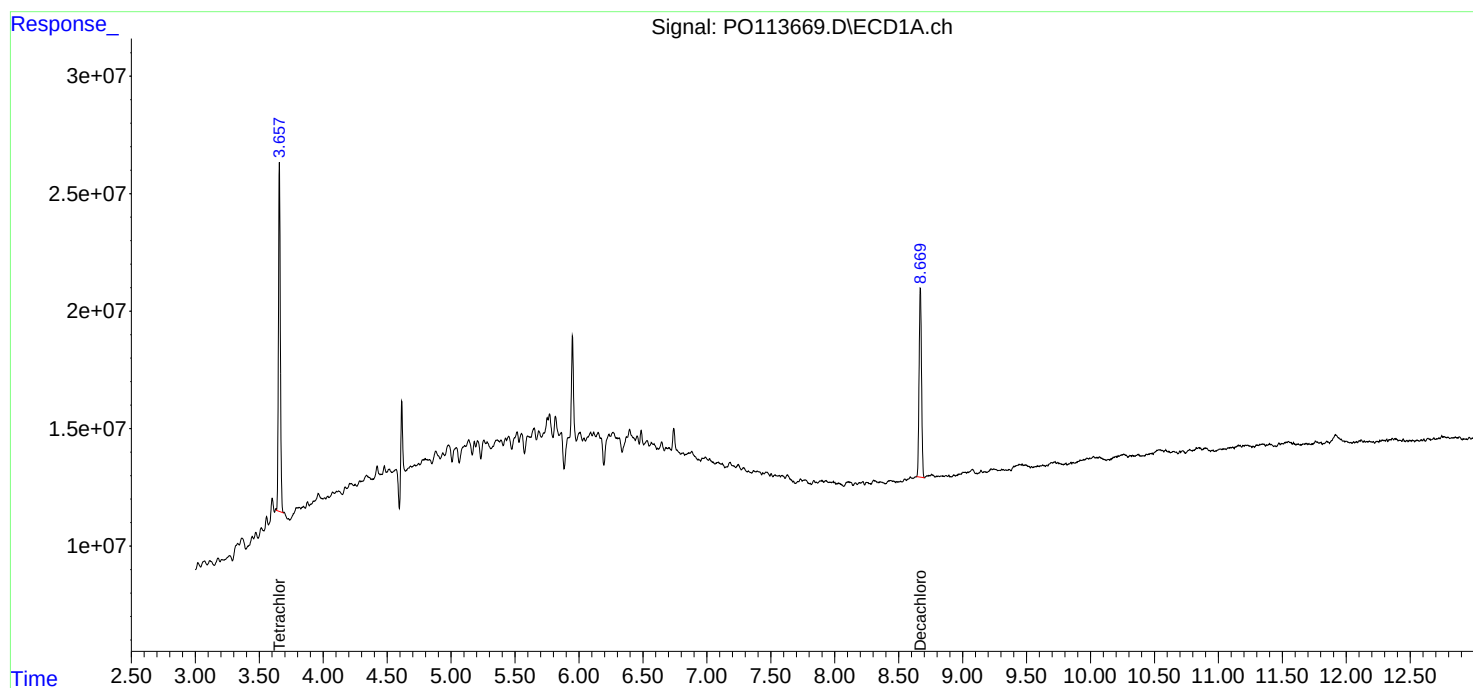

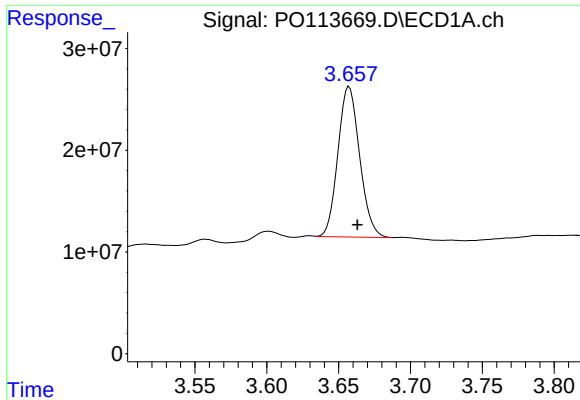


#1 Tetrachloro-m-xylene

R.T.: 3.657 min
Delta R.T.: -0.006 min
Response: 155145164
Conc: 18.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-02-090925


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2025
Supervised By :mohammad ahmed 09/15/2025

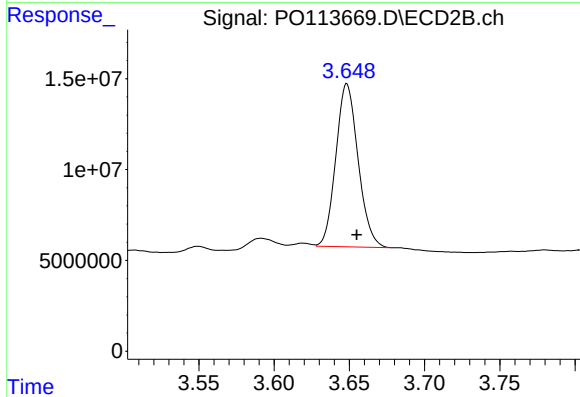


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: -0.007 min
Response: 92564772
Conc: 18.29 ng/ml m

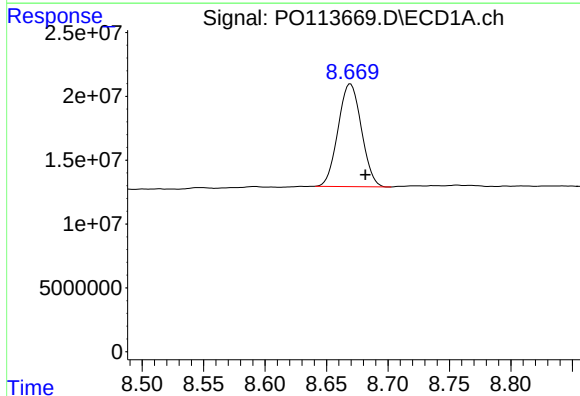

#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.012 min
Response: 106143931
Conc: 15.31 ng/ml

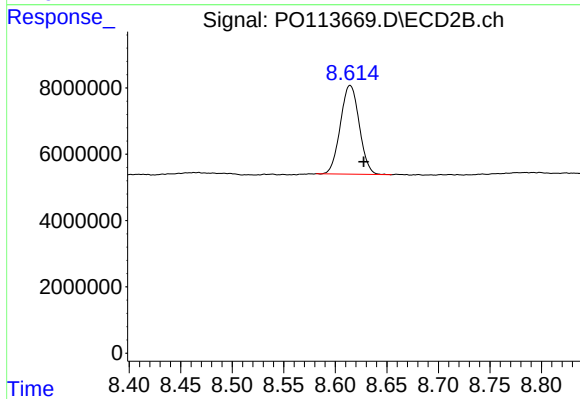

#2 Decachlorobiphenyl

R.T.: 8.614 min
Delta R.T.: -0.013 min
Response: 34203861
Conc: 18.05 ng/ml