

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091219\
Data File : P0060717.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Sep 2019 22:31
Operator : SM/AJ
Sample : K4857-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 04:32:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.367	3.532	710815	586962	17.131	19.110
2)	SA Decachlor...	10.027	8.414	649525	505594	12.313	13.658

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091219\
Data File : P0060717.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Sep 2019 22:31
Operator : SM/AJ
Sample : K4857-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 04:32:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

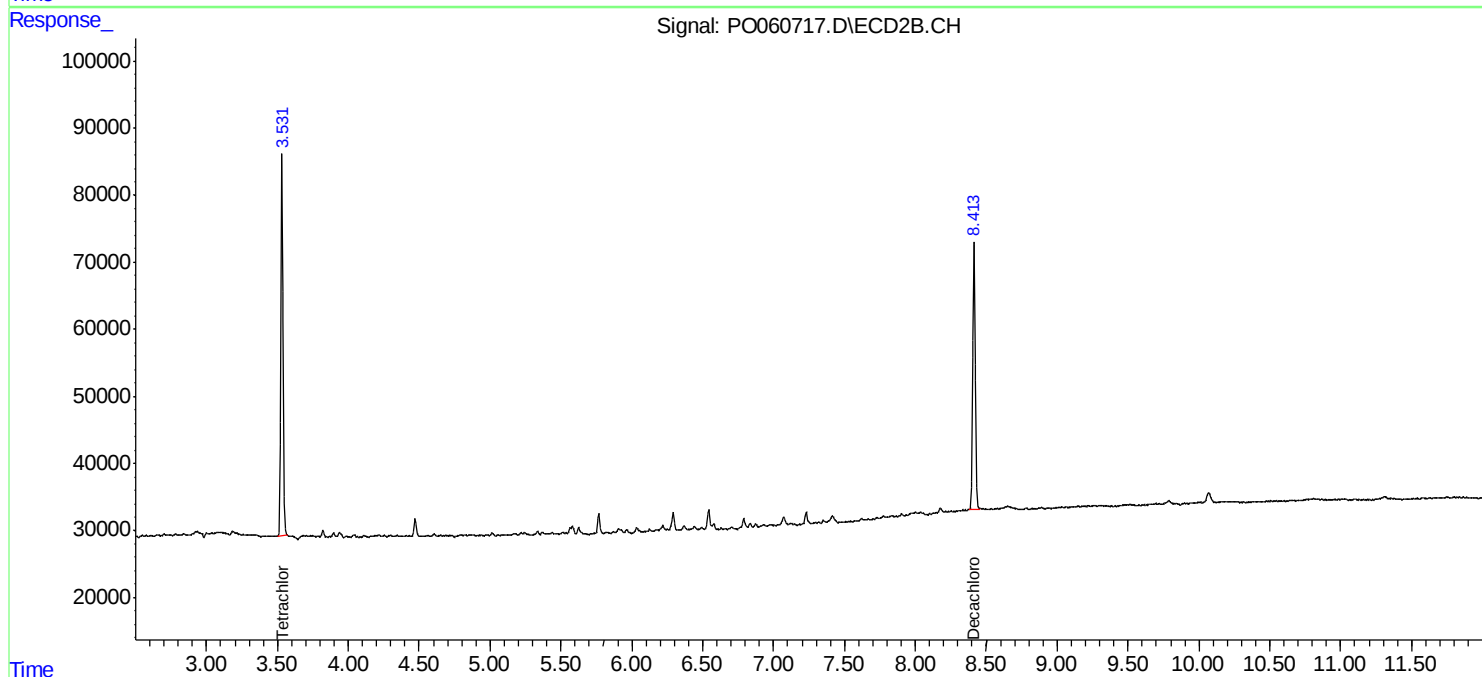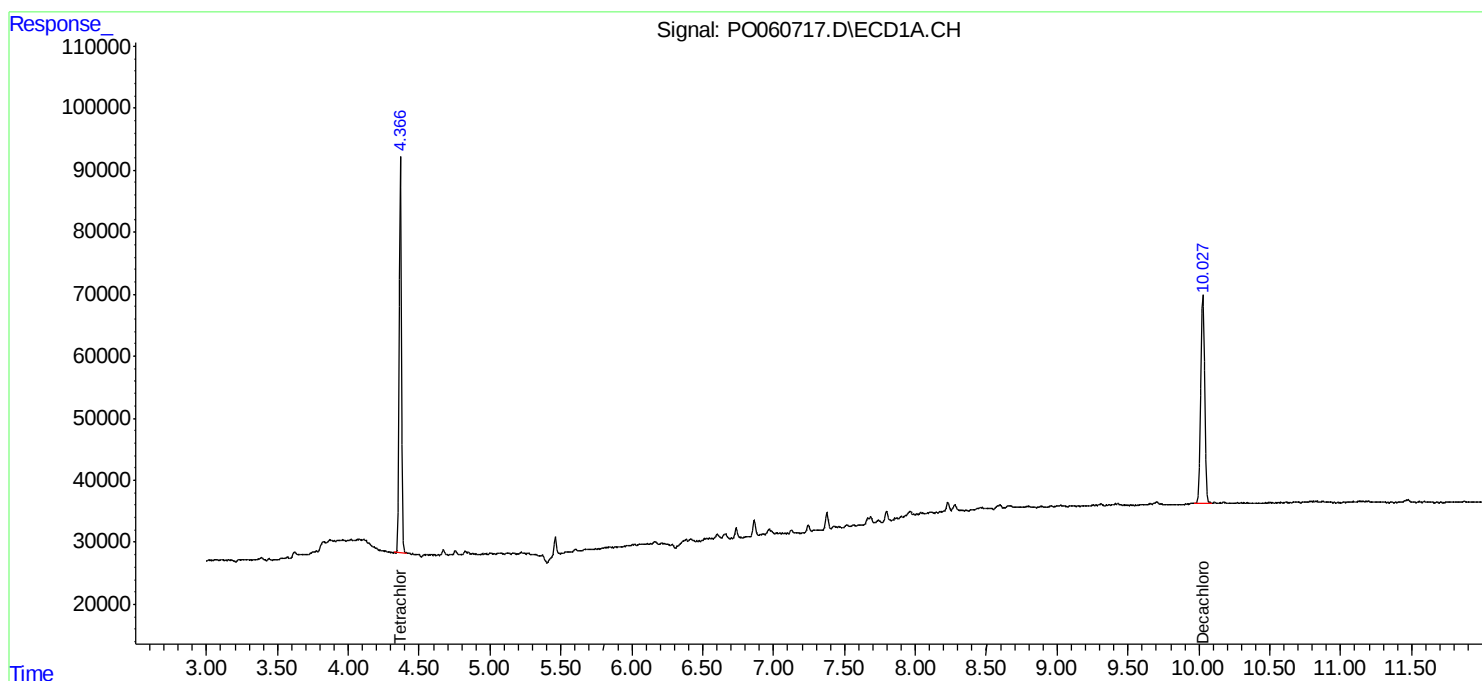


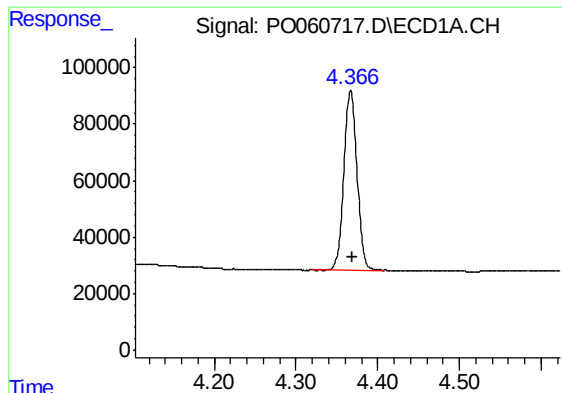

#1 Tetrachloro-m-xylene


R.T.: 4.367 min
Delta R.T.: -0.002 min
Response: 710815
Conc: 17.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-1

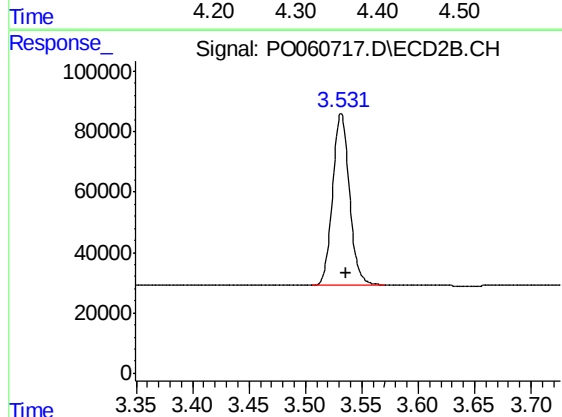


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: -0.004 min
Response: 586962
Conc: 19.11 ng/ml

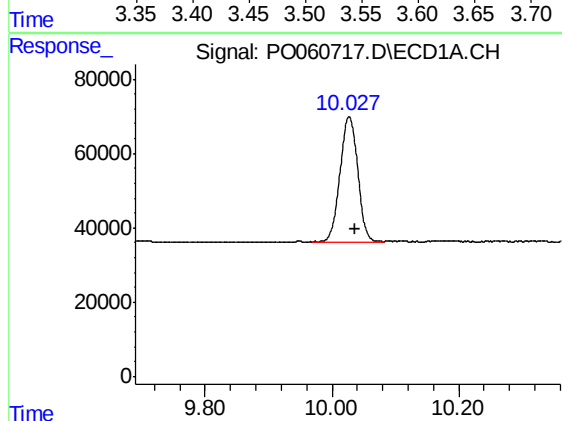

#2 Decachlorobiphenyl

R.T.: 10.027 min
Delta R.T.: -0.010 min
Response: 649525
Conc: 12.31 ng/ml

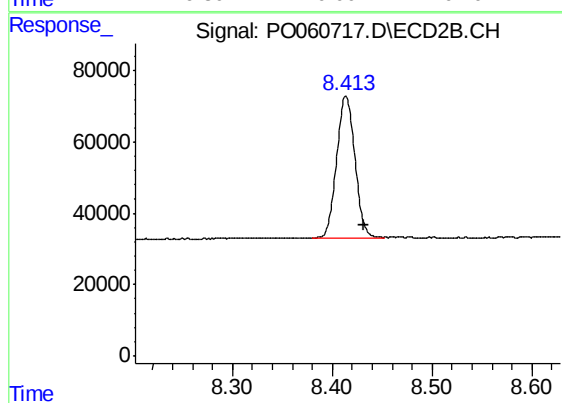

#2 Decachlorobiphenyl

R.T.: 8.414 min
Delta R.T.: -0.017 min
Response: 505594
Conc: 13.66 ng/ml