

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091219\
Data File : P0060748.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Sep 2019 8:56
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 12:29:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.365	3.530	819120	660727	19.741	21.512
2)	SA Decachlor...	10.021	8.411	1006113	732865	19.073	19.798

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091219\
Data File : P0060748.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Sep 2019 8:56
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 12:29:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

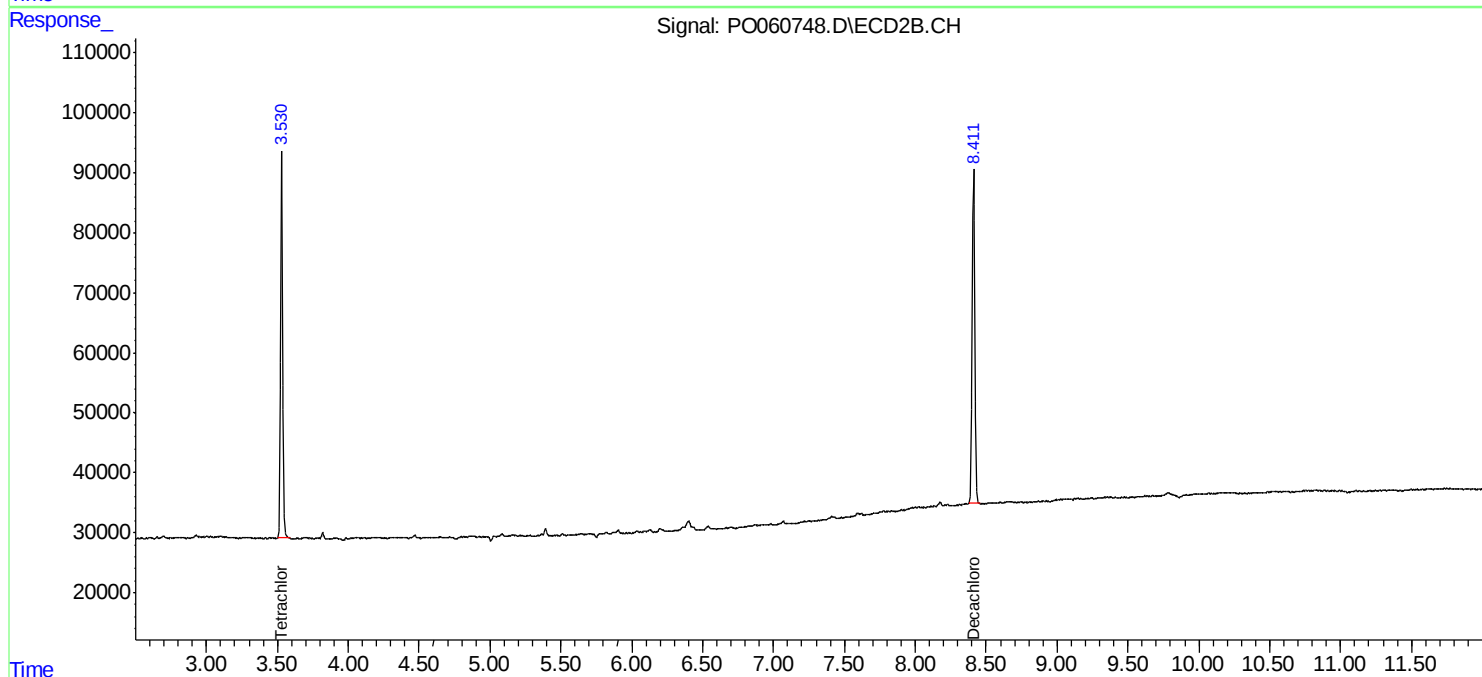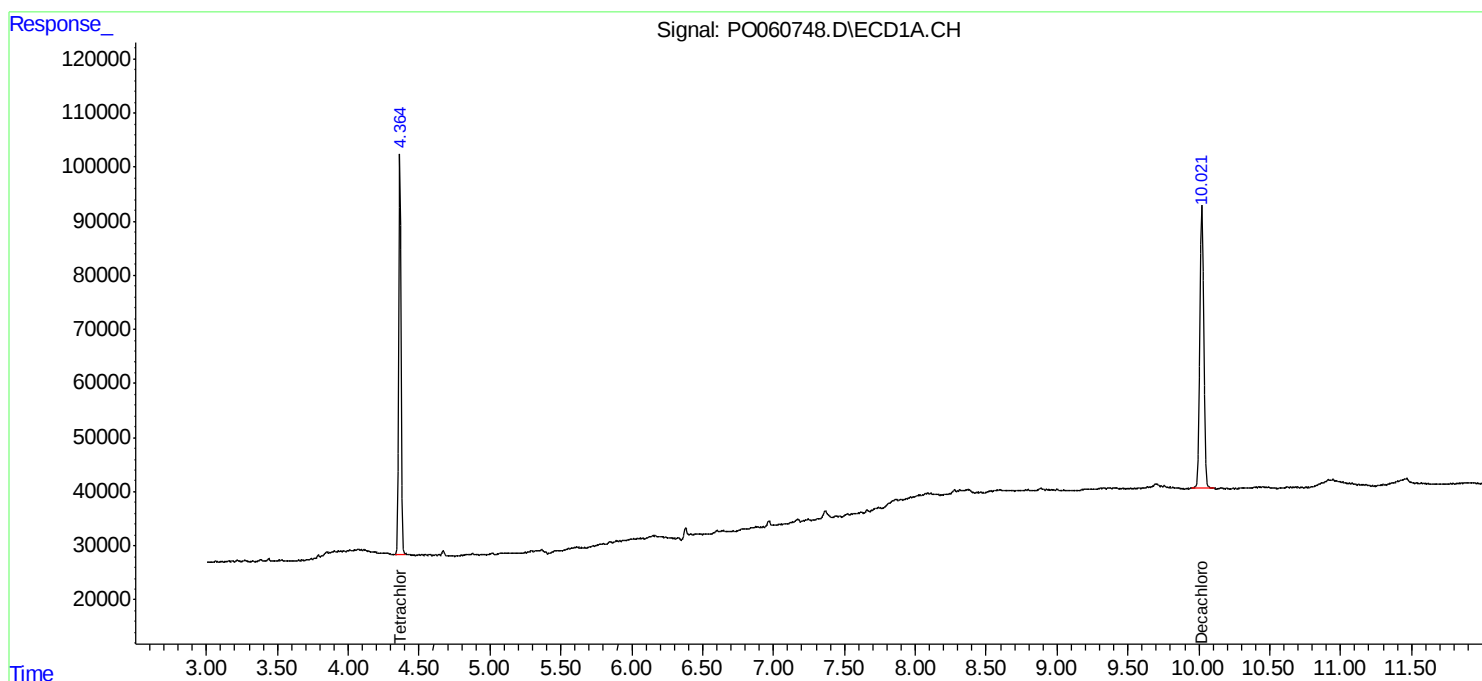


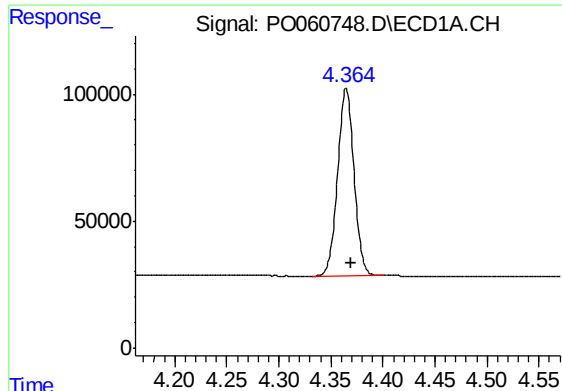

#1 Tetrachloro-m-xylene


R.T.: 4.365 min
Delta R.T.: -0.004 min
Response: 819120
Conc: 19.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

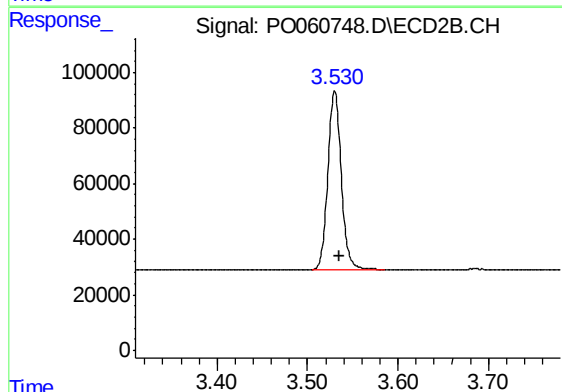


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.006 min
Response: 660727
Conc: 21.51 ng/ml

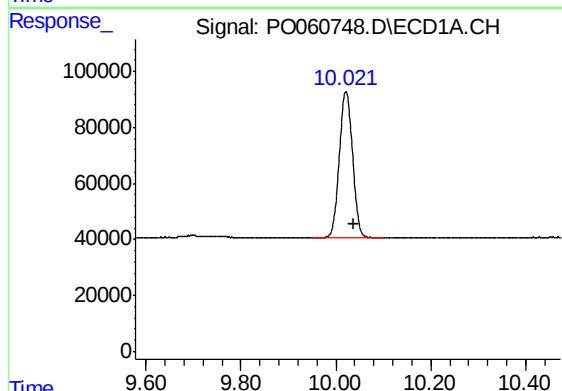

#2 Decachlorobiphenyl

R.T.: 10.021 min
Delta R.T.: -0.016 min
Response: 1006113
Conc: 19.07 ng/ml

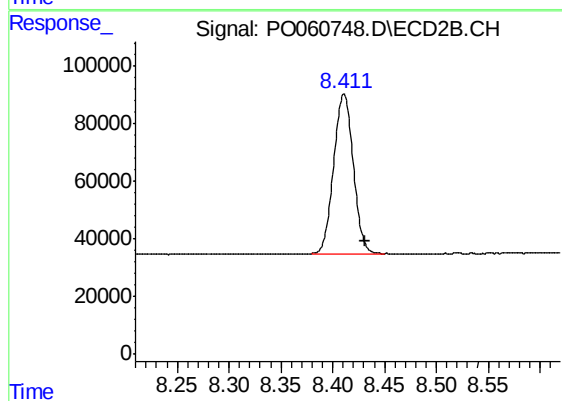

#2 Decachlorobiphenyl

R.T.: 8.411 min
Delta R.T.: -0.020 min
Response: 732865
Conc: 19.80 ng/ml