

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091224\
 Data File : P0106499.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2024 23:56
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 05:20:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.451	3.714	166.4E6	55687244	22.180	20.847
2) SA Decachlor...	10.192	8.738	102.2E6	43565578	20.673	21.780

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091224\
Data File : PO106499.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2024 23:56
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 05:20:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

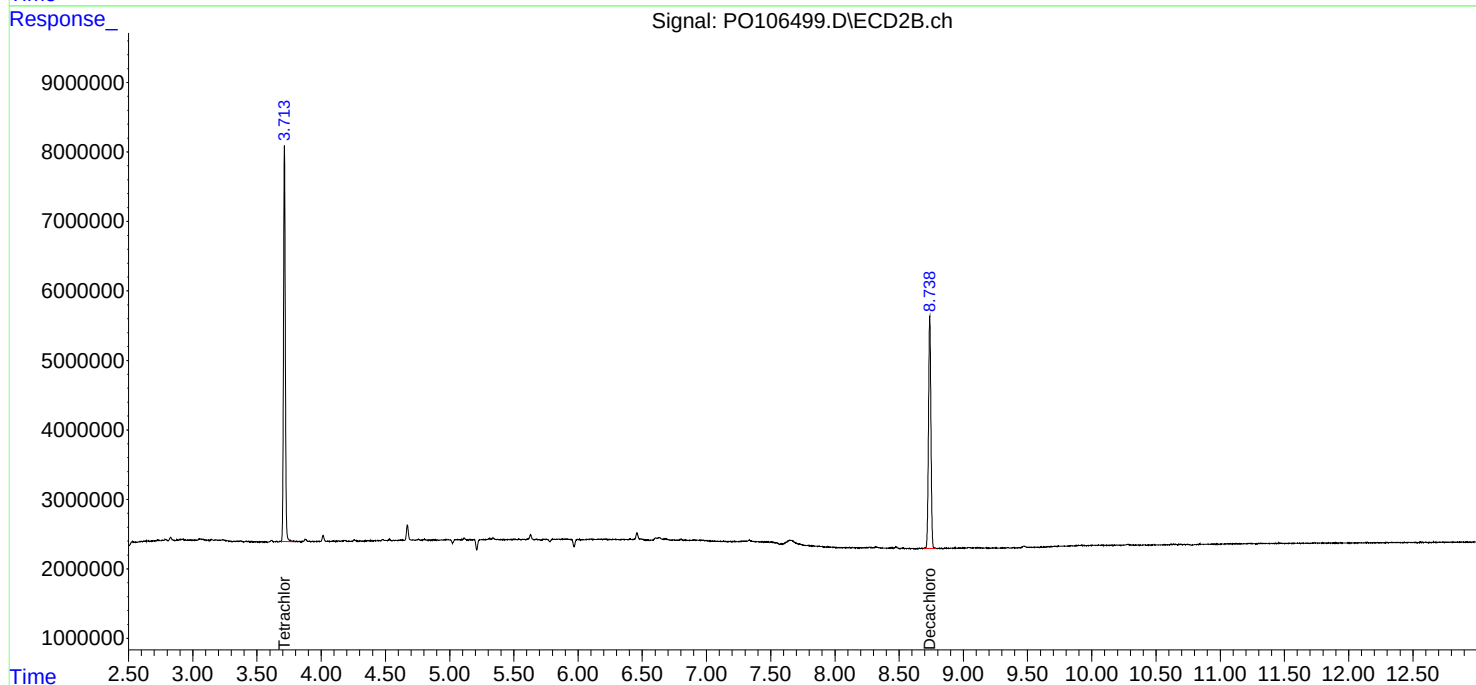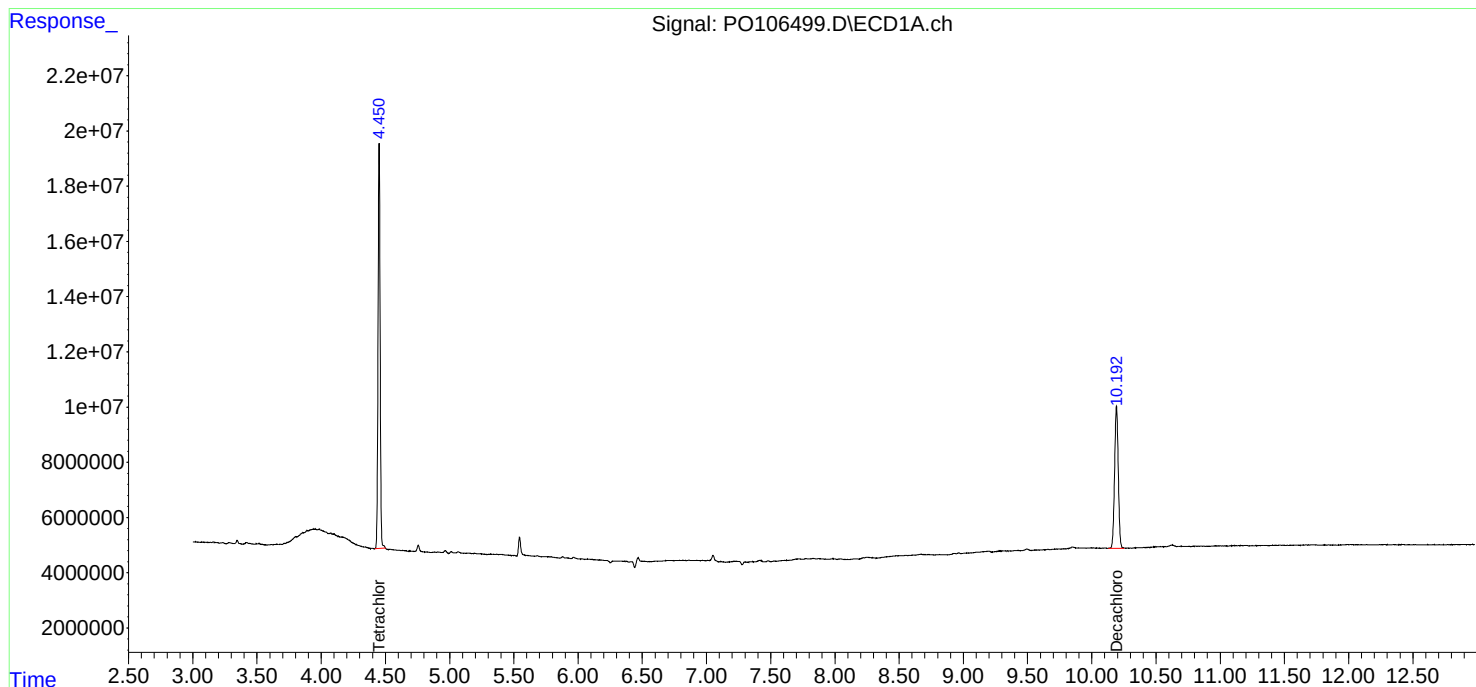


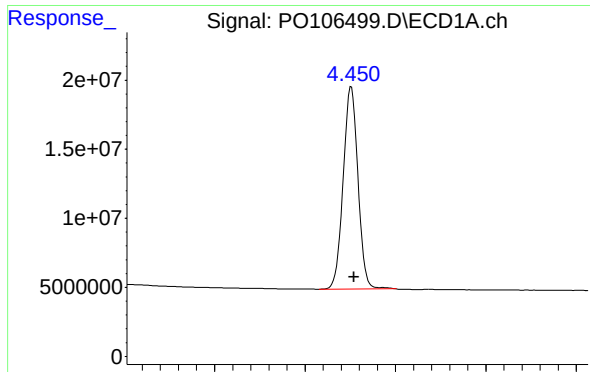

#1 Tetrachloro-m-xylene


R.T.: 4.451 min
Delta R.T.: -0.003 min
Response: 166378501
Conc: 22.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

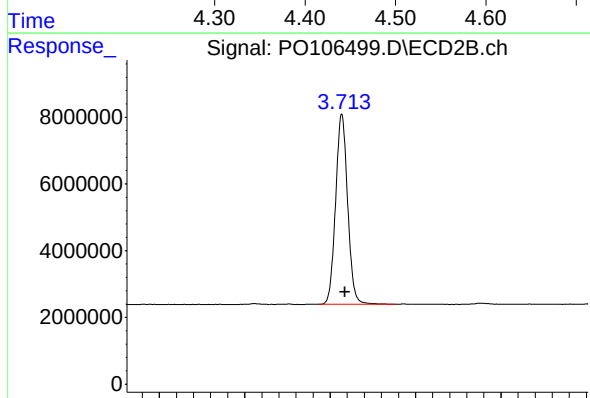


#1 Tetrachloro-m-xylene

R.T.: 3.714 min
Delta R.T.: -0.004 min
Response: 55687244
Conc: 20.85 ng/ml

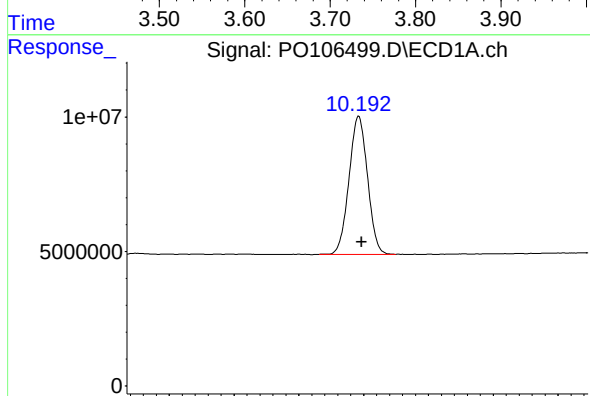

#2 Decachlorobiphenyl

R.T.: 10.192 min
Delta R.T.: -0.005 min
Response: 102181295
Conc: 20.67 ng/ml

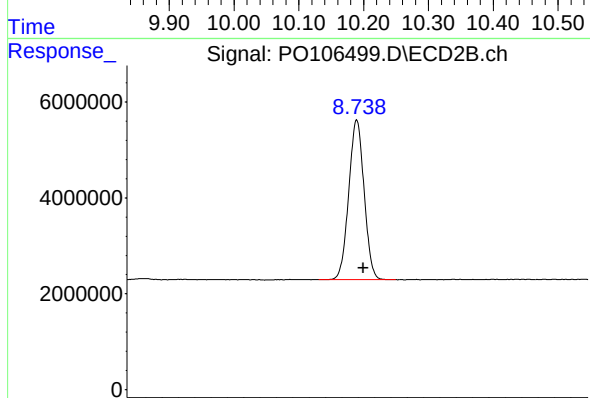

#2 Decachlorobiphenyl

R.T.: 8.738 min
Delta R.T.: -0.008 min
Response: 43565578
Conc: 21.78 ng/ml