

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091319\
 Data File : P0060770.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Sep 2019 16:39
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 00:16:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.369	3.530	779065	609706	21.175	21.836
2)	SA Decachlor...	10.028	8.411	1057465	829664	23.015	23.670
Target Compounds							
9)	L2 AR-1221-2	0.000	3.819	0	9916	N.D.	35.284 #
20)	L4 AR-1242-5	0.000	5.390	0	7899	N.D.	7.980 #
25)	L5 AR-1248-5	0.000	5.390	0	7899	N.D.	6.249 #
26)	L6 AR-1254-1	0.000	5.390	0	7899	N.D.	3.833 #
29)	L6 AR-1254-4	0.000	6.198	0	4809	N.D.	2.310 #
30)	L6 AR-1254-5	0.000	6.537	0	719	N.D.	0.227 #
32)	L7 AR-1260-2	0.000	6.198	0	4809	N.D.	1.864 #
35)	L7 AR-1260-5	0.000	7.064	0	1939	N.D.	0.401 #
36)	L8 AR-1262-1	0.000	6.537	0	719	N.D.	0.241 #
37)	L8 AR-1262-2	0.000	7.064	0	1939	N.D.	0.373 #
38)	L8 AR-1262-3	0.000	7.407	0	7617	N.D.	3.589 #
39)	L8 AR-1262-4	0.000	7.407	0	7617	N.D.	1.994 #
41)	L9 AR-1268-1	0.000	7.407	0	7617	N.D.	1.299 #
42)	L9 AR-1268-2	0.000	7.407	0	7617	N.D.	1.429 #
43)	L9 AR-1268-3	0.000	7.620	0	9447	N.D.	2.131 #
45)	L9 AR-1268-5	0.000	8.175	0	10428	N.D.	0.867 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091319\
Data File : P0060770.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Sep 2019 16:39
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 00:16:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

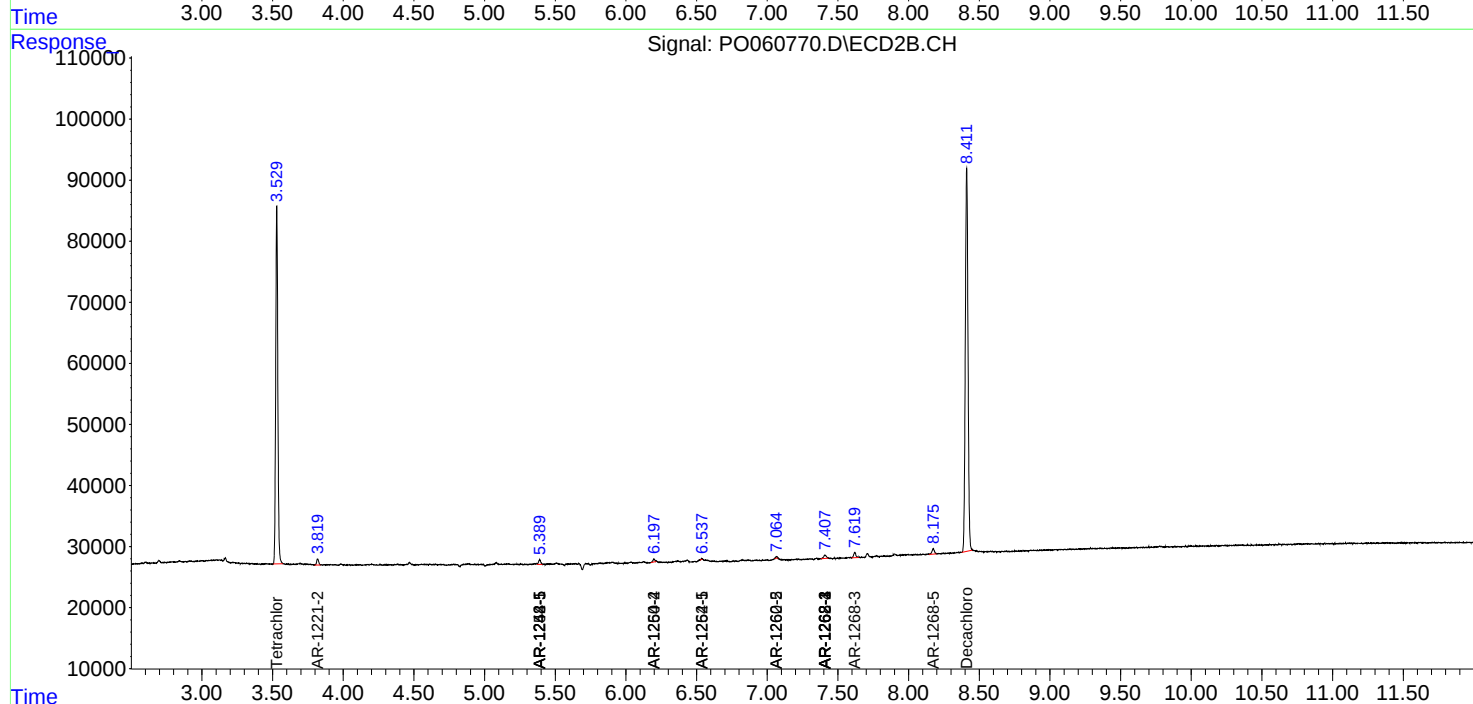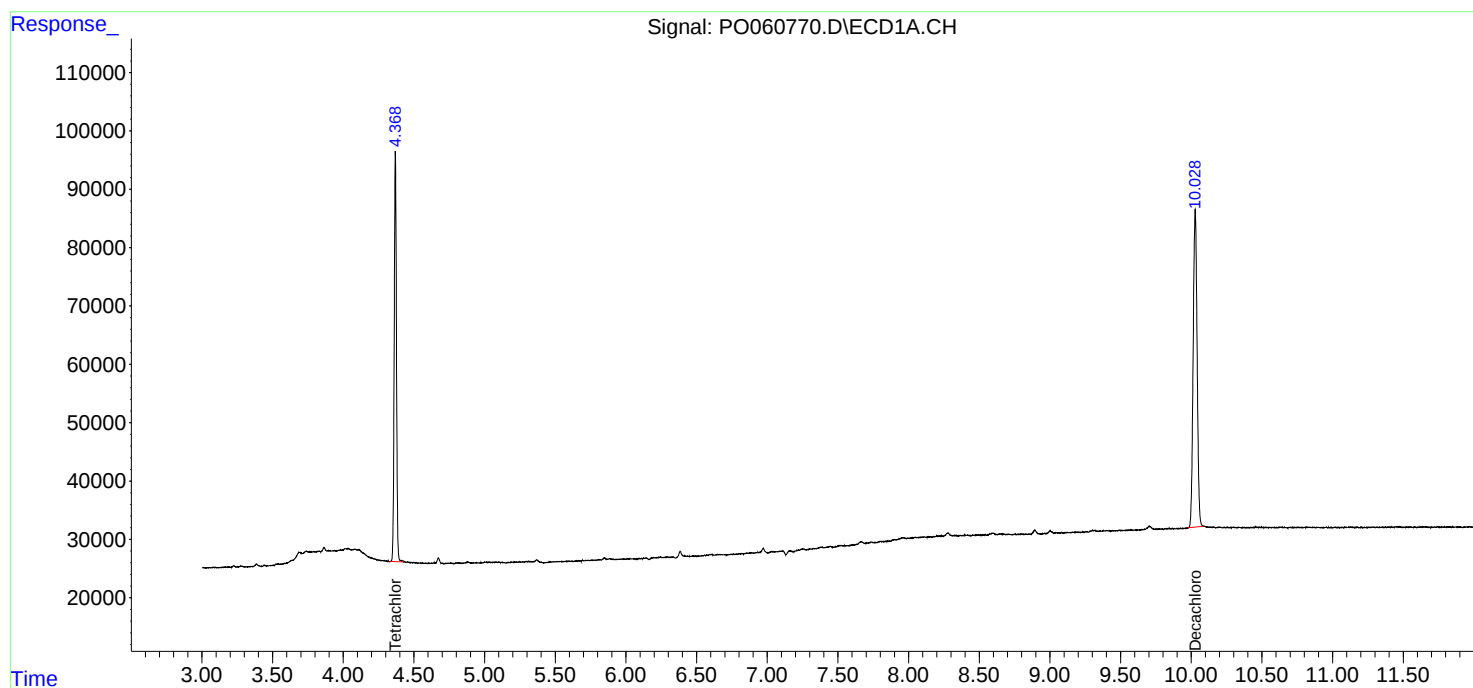


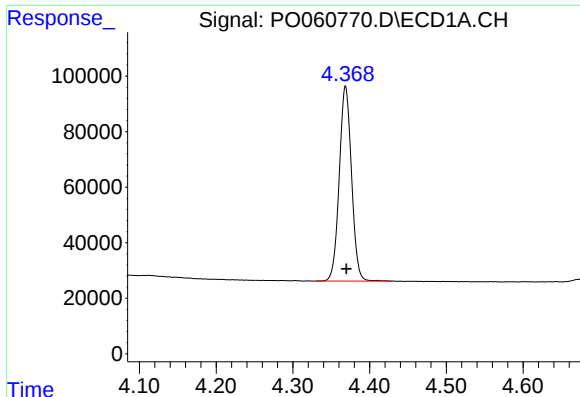

#1 Tetrachloro-m-xylene


R.T.: 4.369 min
Delta R.T.: -0.001 min
Response: 779065
Conc: 21.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

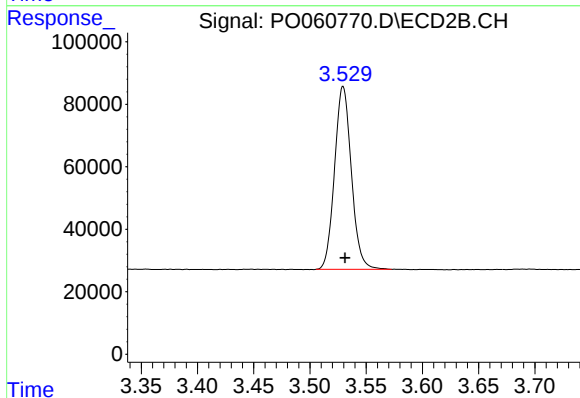


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.002 min
Response: 609706
Conc: 21.84 ng/ml

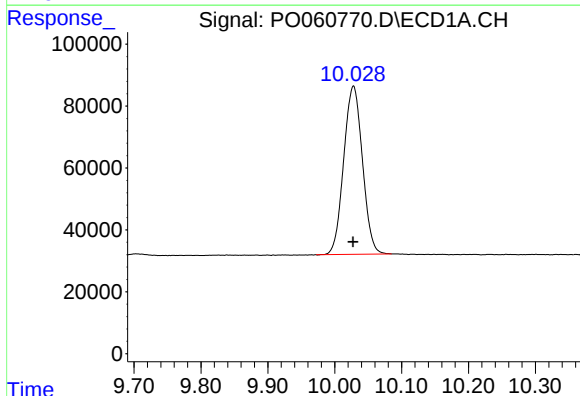


#2 Decachlorobiphenyl

R.T.: 10.028 min
Delta R.T.: 0.000 min
Response: 1057465
Conc: 23.02 ng/ml

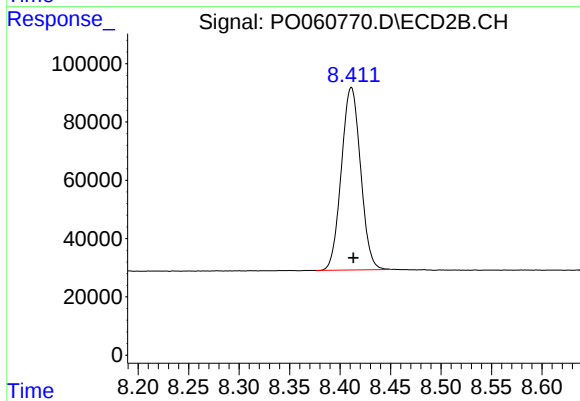

#2 Decachlorobiphenyl


R.T.: 8.411 min
Delta R.T.: -0.002 min
Response: 829664
Conc: 23.67 ng/ml

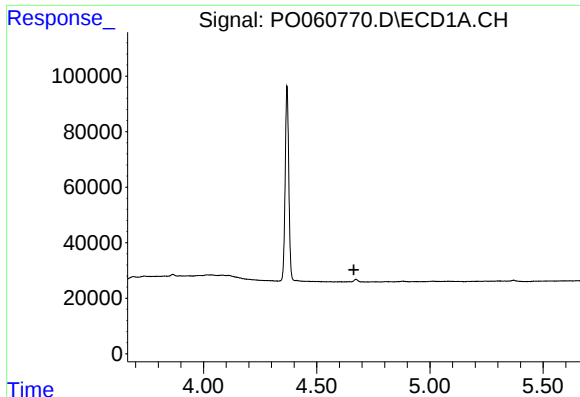

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.664 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

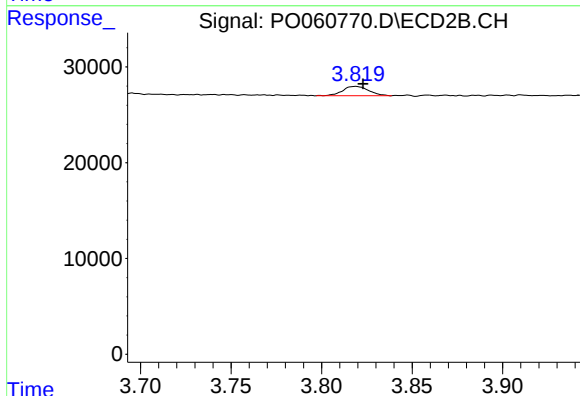


#9 AR-1221-2

R.T.: 3.819 min
Delta R.T.: -0.004 min
Response: 9916
Conc: 35.28 ng/ml

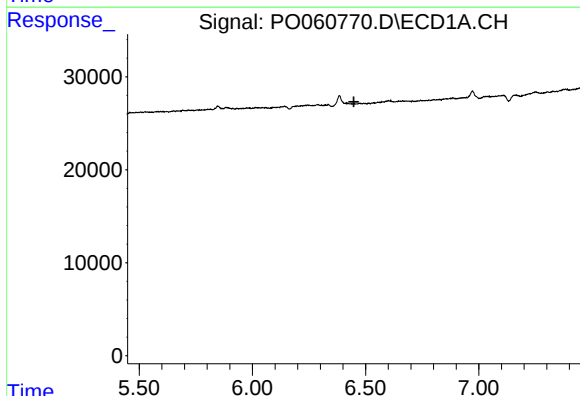


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.448 min
Response: 0
Conc: N.D.

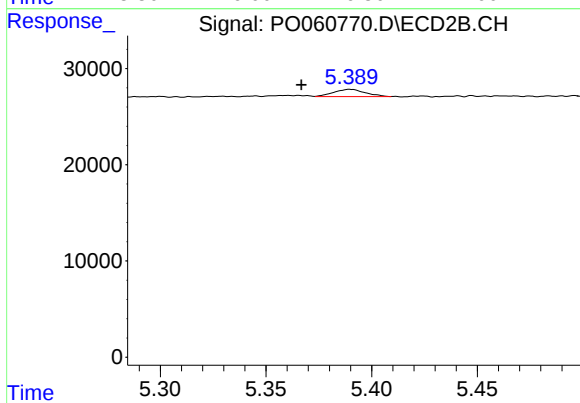

#20 AR-1242-5


R.T.: 5.390 min
Delta R.T.: 0.023 min
Response: 7899
Conc: 7.98 ng/ml

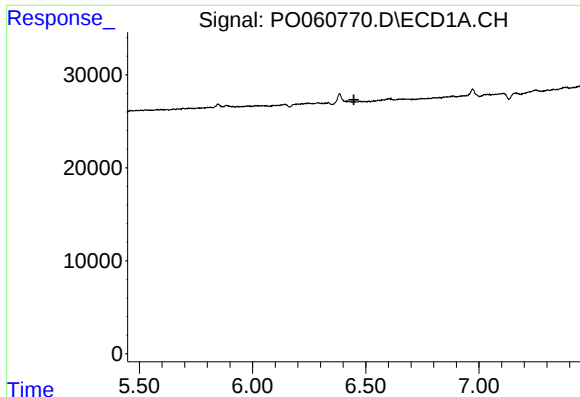

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

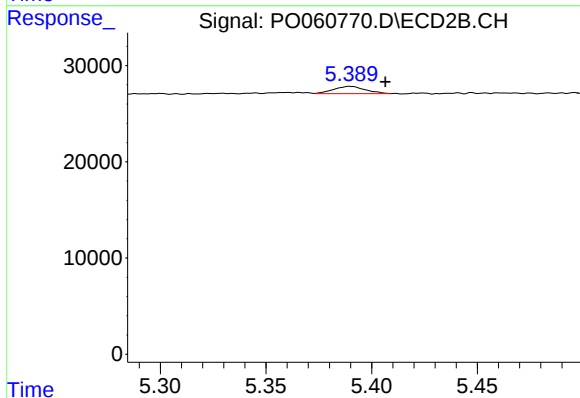


#25 AR-1248-5

R.T.: 5.390 min
Delta R.T.: -0.017 min
Response: 7899
Conc: 6.25 ng/ml

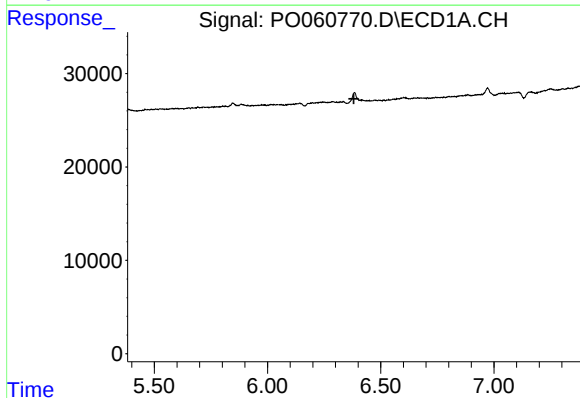


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.382 min
Response: 0
Conc: N.D.

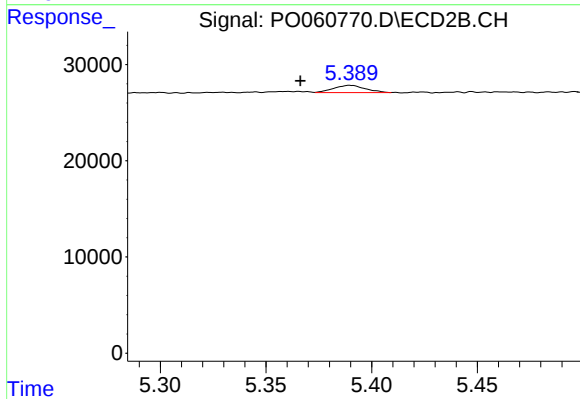

#26 AR-1254-1


R.T.: 5.390 min
Delta R.T.: 0.023 min
Response: 7899
Conc: 3.83 ng/ml

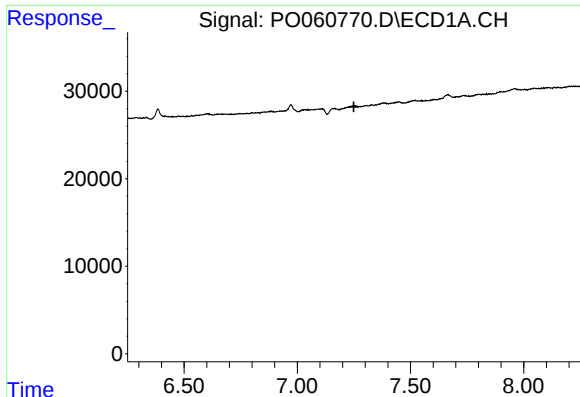

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.250 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

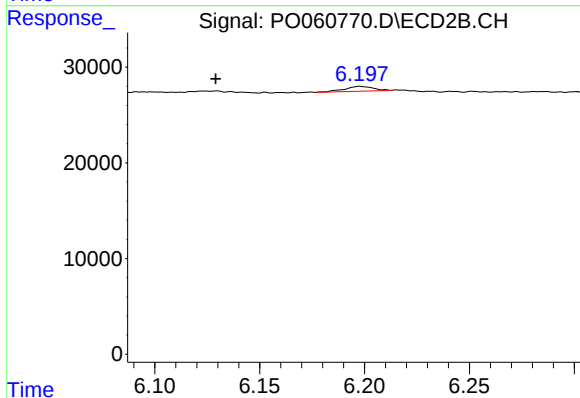


#29 AR-1254-4

R.T.: 6.198 min
Delta R.T.: 0.069 min
Response: 4809
Conc: 2.31 ng/ml

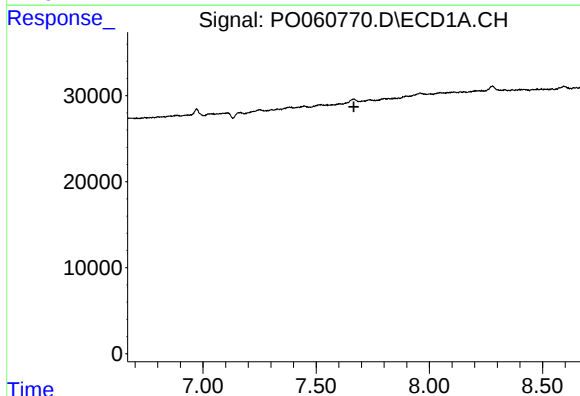


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.667 min
Response: 0
Conc: N.D.

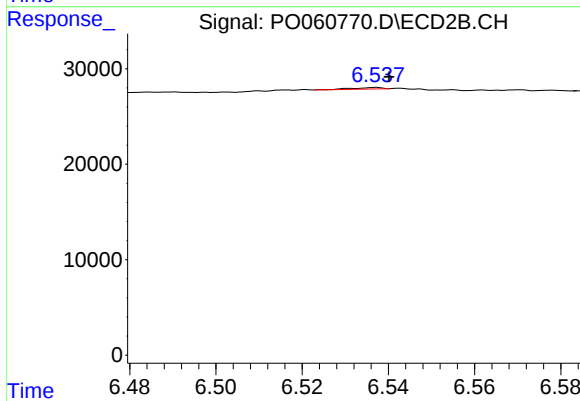

#30 AR-1254-5


R.T.: 6.537 min
Delta R.T.: -0.003 min
Response: 719
Conc: 0.23 ng/ml

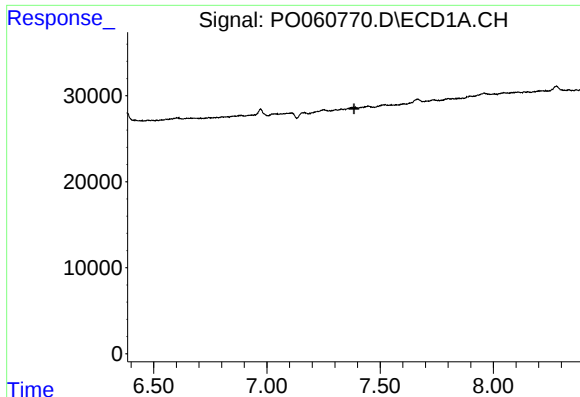

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.384 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

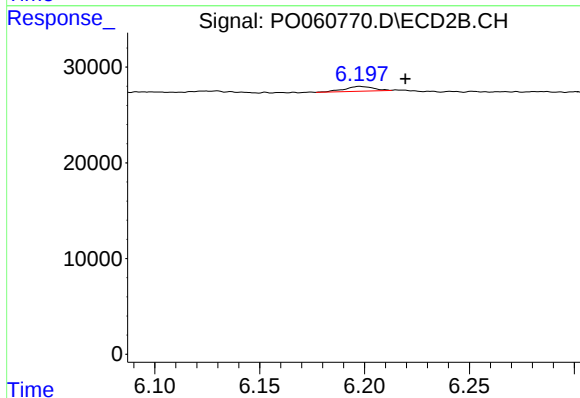


#32 AR-1260-2

R.T.: 6.198 min
Delta R.T.: -0.022 min
Response: 4809
Conc: 1.86 ng/ml

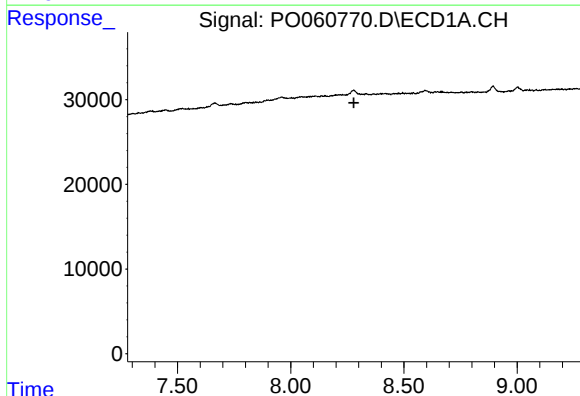


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.279 min
Response: 0
Conc: N.D.

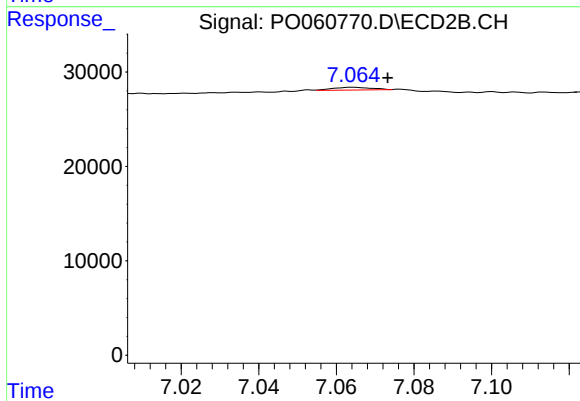

#35 AR-1260-5


R.T.: 7.064 min
Delta R.T.: -0.009 min
Response: 1939
Conc: 0.40 ng/ml

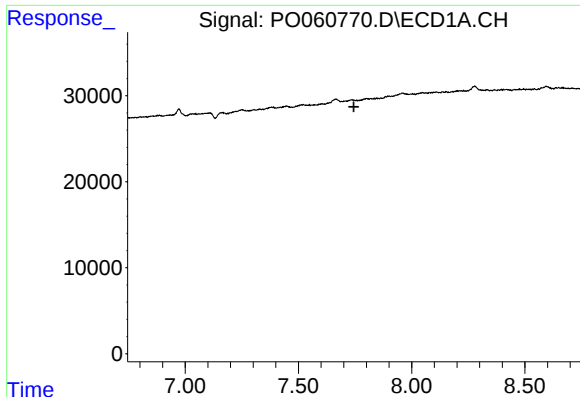

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

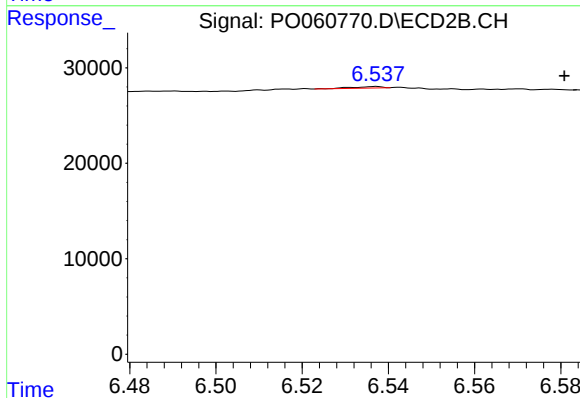


#36 AR-1262-1

R.T.: 6.537 min
Delta R.T.: -0.043 min
Response: 719
Conc: 0.24 ng/ml

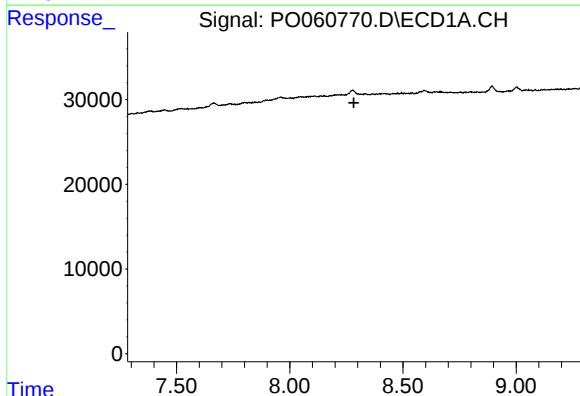


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

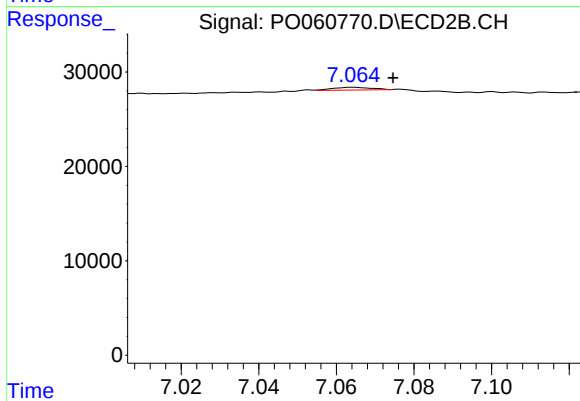

#37 AR-1262-2


R.T.: 7.064 min
Delta R.T.: -0.010 min
Response: 1939
Conc: 0.37 ng/ml

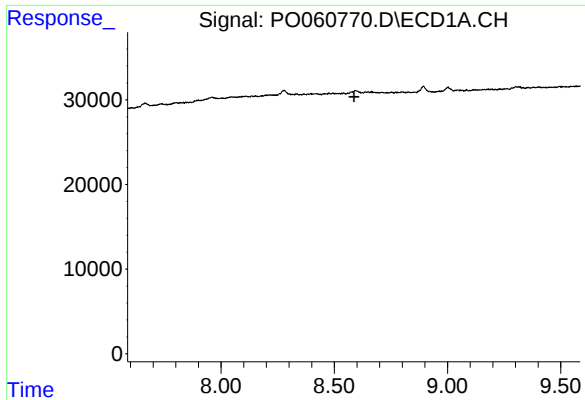

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.587 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

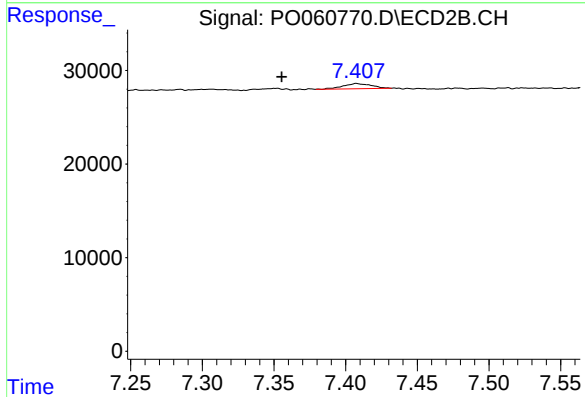


#38 AR-1262-3

R.T.: 7.407 min
Delta R.T.: 0.052 min
Response: 7617
Conc: 3.59 ng/ml

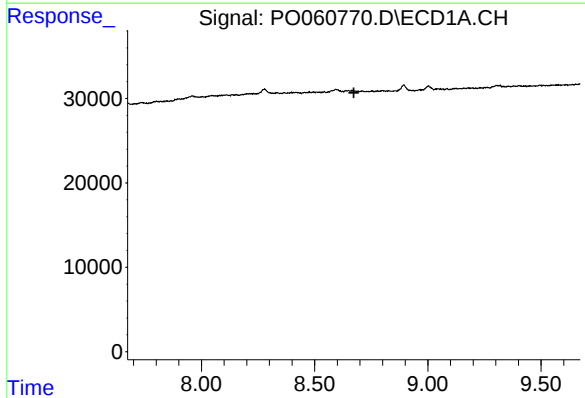


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.673 min
Response: 0
Conc: N.D.

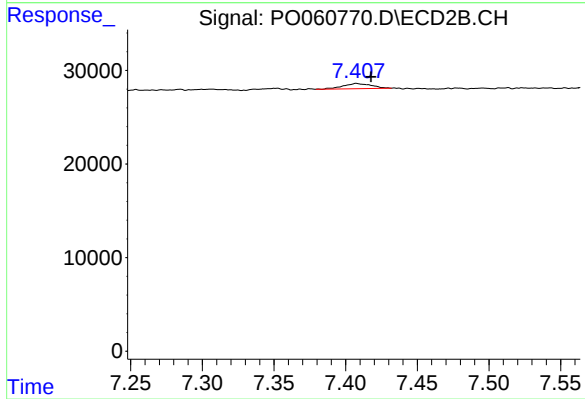

#39 AR-1262-4


R.T.: 7.407 min
Delta R.T.: -0.010 min
Response: 7617
Conc: 1.99 ng/ml

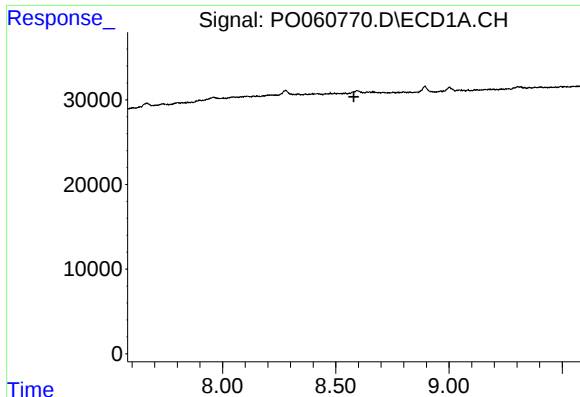

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.580 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

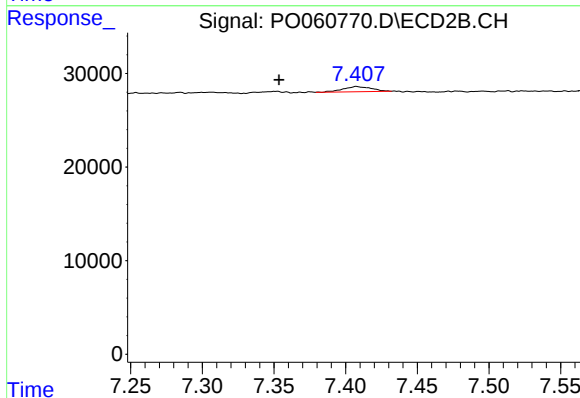


#41 AR-1268-1

R.T.: 7.407 min
Delta R.T.: 0.054 min
Response: 7617
Conc: 1.30 ng/ml

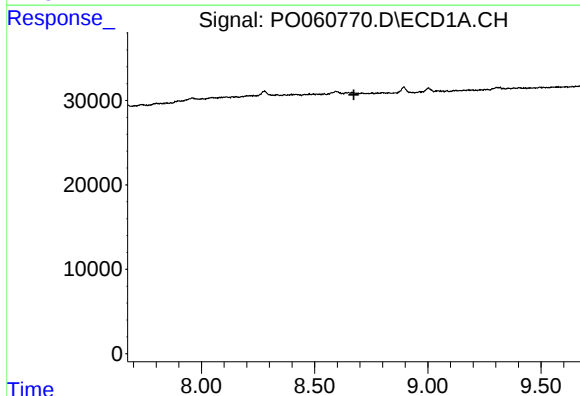


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.673 min
Response: 0
Conc: N.D.

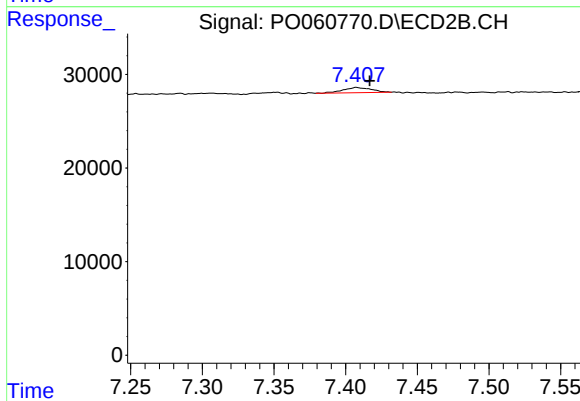

#42 AR-1268-2

R.T.: 7.407 min
Delta R.T.: -0.009 min
Response: 7617
Conc: 1.43 ng/ml

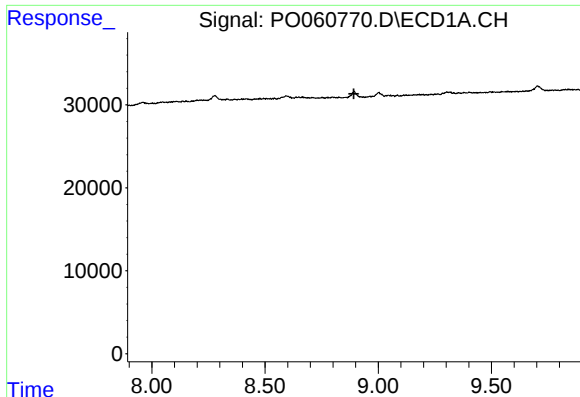


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 8.893 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

#43 AR-1268-3

R.T.: 7.620 min
Delta R.T.: -0.002 min
Response: 9447
Conc: 2.13 ng/ml

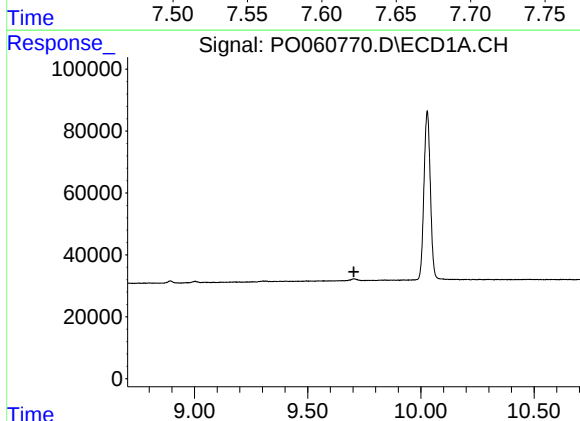

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.704 min
Response: 0
Conc: N.D.

#45 AR-1268-5

R.T.: 8.175 min
Delta R.T.: -0.001 min
Response: 10428
Conc: 0.87 ng/ml