

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091319\
 Data File : P0060821.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Sep 2019 10:22
 Operator : SM/AJ
 Sample : K4846-02
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-19-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 00:42:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.363	3.528	843687	706789	22.932	25.313
2)	SA Decachlor...	10.022	8.407	745724	550824	16.230	15.715
Target Compounds							
9)	L2 AR-1221-2	0.000	3.819	0	8758	N.D.	31.162 #
29)	L6 AR-1254-4	0.000	6.195	0	931	N.D.	0.447 #
30)	L6 AR-1254-5	0.000	6.533	0	9172	N.D.	2.898 #
32)	L7 AR-1260-2	0.000	6.210	0	556	N.D.	0.215 #
35)	L7 AR-1260-5	0.000	7.069	0	4187	N.D.	0.866 #
36)	L8 AR-1262-1	0.000	6.533	0	9172	N.D.	3.071 #
37)	L8 AR-1262-2	0.000	7.069	0	4187	N.D.	0.805 #
45)	L9 AR-1268-5	0.000	8.173	0	6656	N.D.	0.553 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091319\
Data File : P0060821.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Sep 2019 10:22
Operator : SM/AJ
Sample : K4846-02
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-19-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 00:42:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

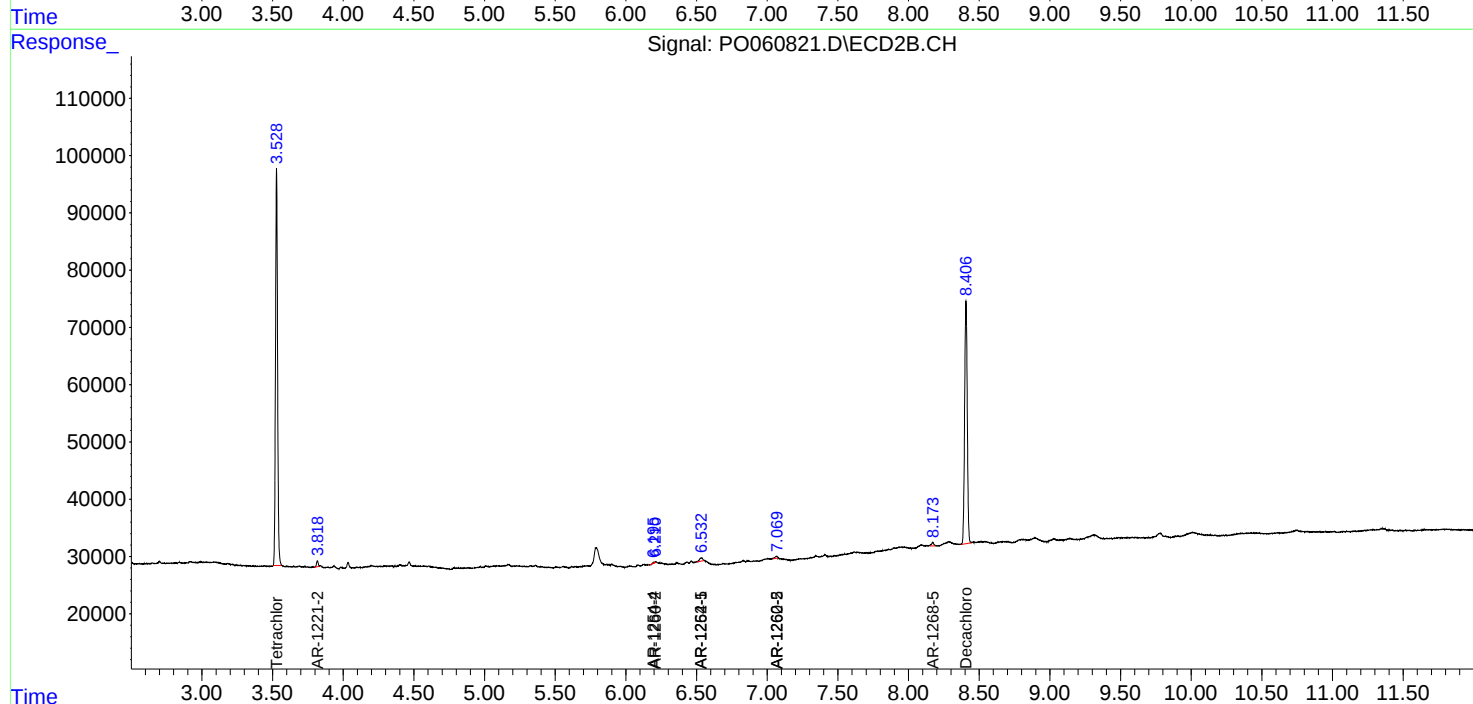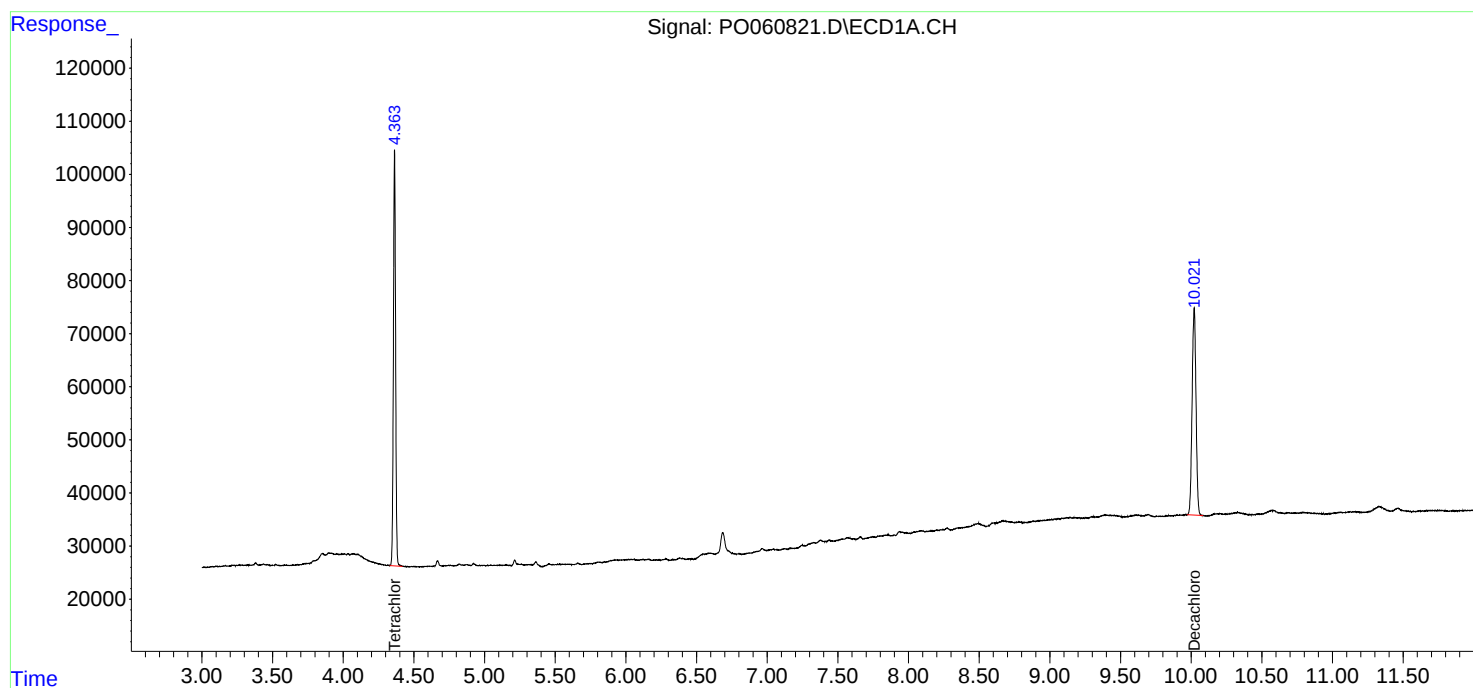


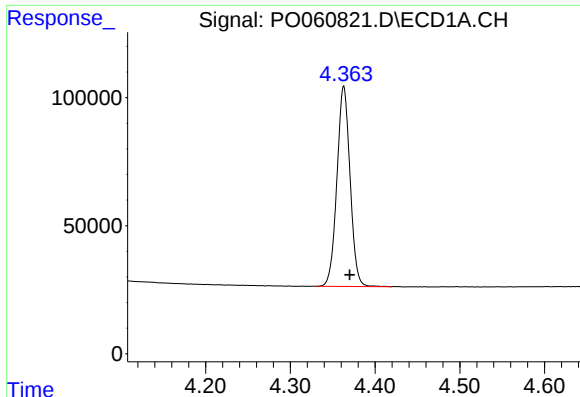

#1 Tetrachloro-m-xylene


R.T.: 4.363 min
Delta R.T.: -0.007 min
Response: 843687
Conc: 22.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-19-COMP

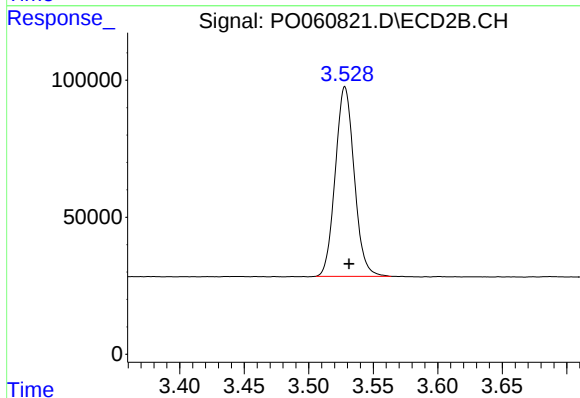


#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: -0.003 min
Response: 706789
Conc: 25.31 ng/ml

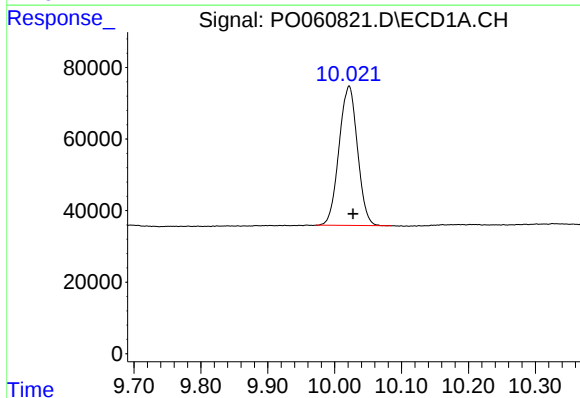


#2 Decachlorobiphenyl

R.T.: 10.022 min
Delta R.T.: -0.006 min
Response: 745724
Conc: 16.23 ng/ml

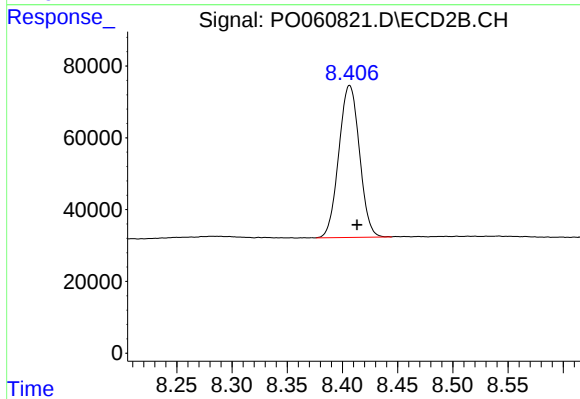

#2 Decachlorobiphenyl


R.T.: 8.407 min
Delta R.T.: -0.007 min
Response: 550824
Conc: 15.71 ng/ml

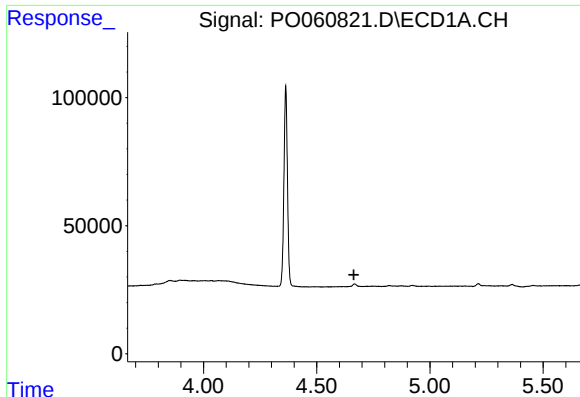

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.664 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-19-COMP

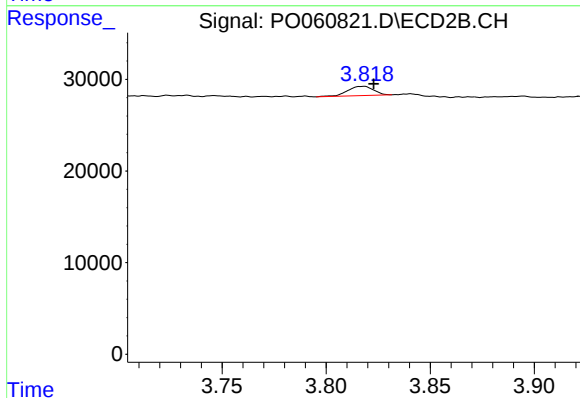


#9 AR-1221-2

R.T.: 3.819 min
Delta R.T.: -0.004 min
Response: 8758
Conc: 31.16 ng/ml

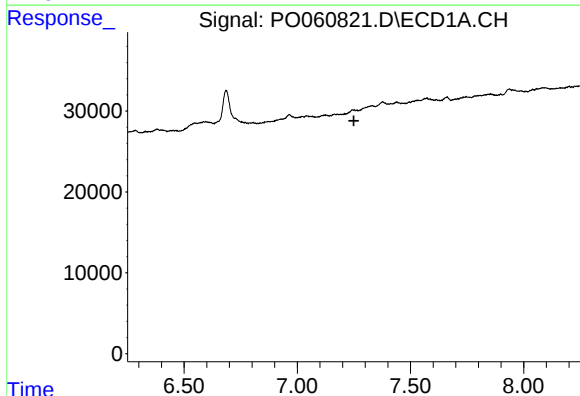


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T.: 7.250 min
Response: 0
Conc: N.D.

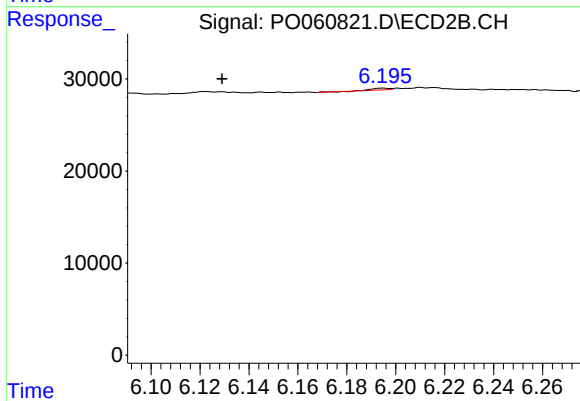

#29 AR-1254-4


R.T.: 6.195 min
Delta R.T.: 0.066 min
Response: 931
Conc: 0.45 ng/ml

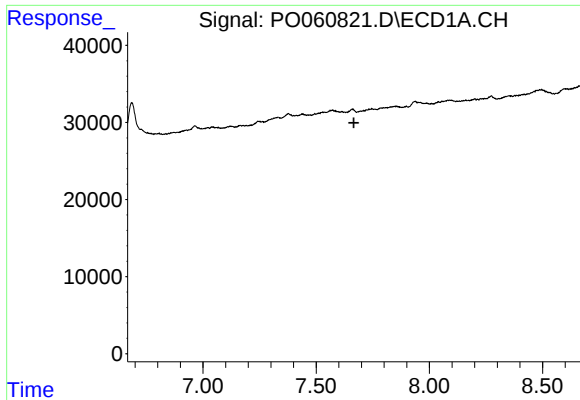

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 7.667 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-19-COMP

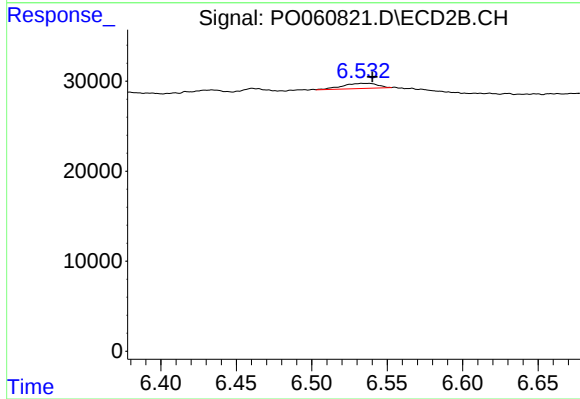


#30 AR-1254-5

R.T.: 6.533 min
Delta R.T.: -0.007 min
Response: 9172
Conc: 2.90 ng/ml

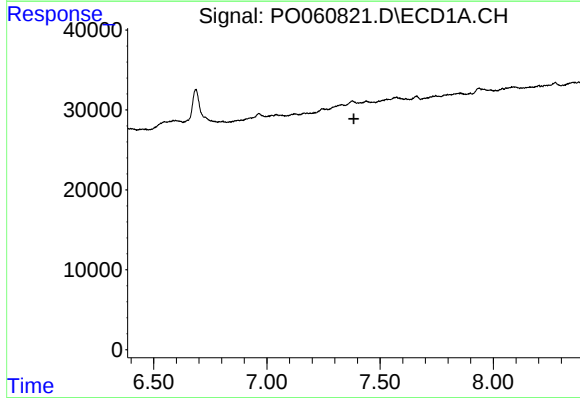


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.384 min
Response: 0
Conc: N.D.

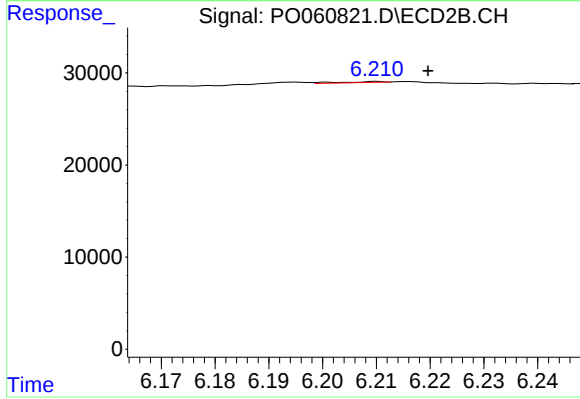

#32 AR-1260-2


R.T.: 6.210 min
Delta R.T.: -0.010 min
Response: 556
Conc: 0.22 ng/ml

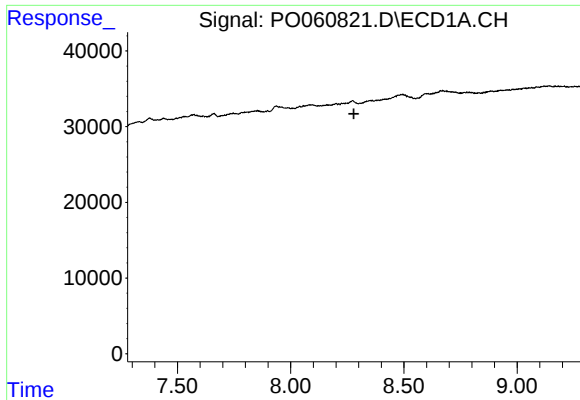

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.279 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-19-COMP

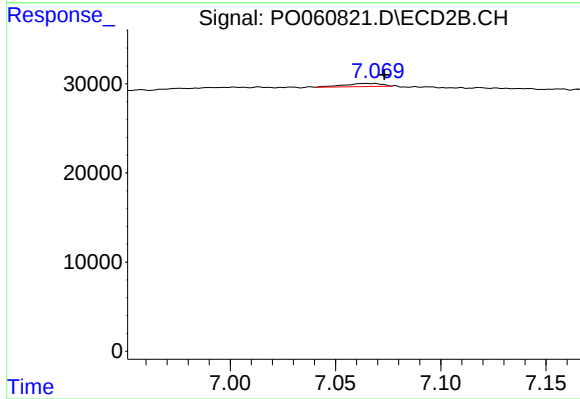


#35 AR-1260-5

R.T.: 7.069 min
Delta R.T.: -0.004 min
Response: 4187
Conc: 0.87 ng/ml

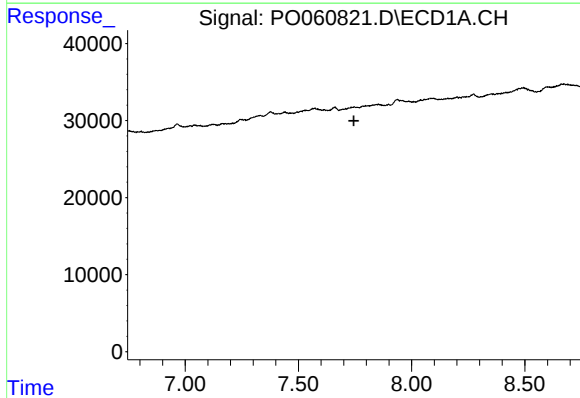


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.745 min
Response: 0
Conc: N.D.

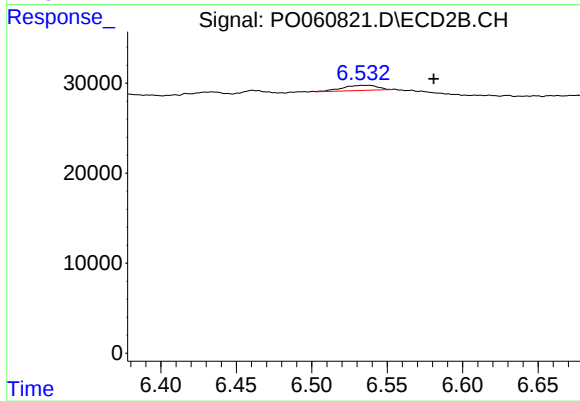

#36 AR-1262-1


R.T.: 6.533 min
Delta R.T.: -0.048 min
Response: 9172
Conc: 3.07 ng/ml

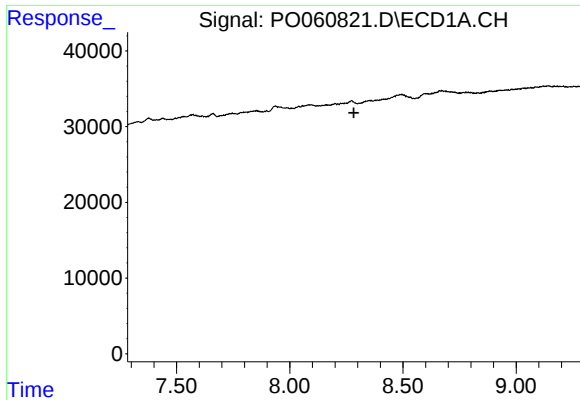

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-19-COMP

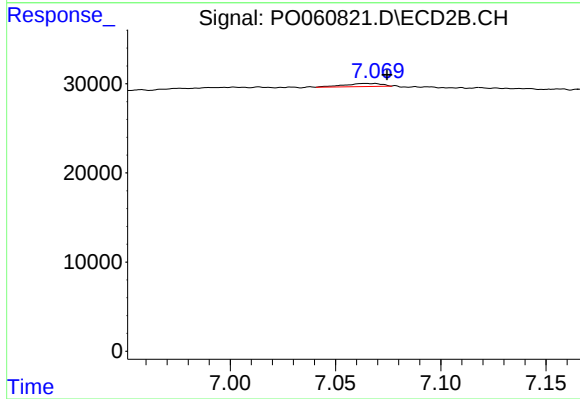


#37 AR-1262-2

R.T.: 7.069 min
Delta R.T.: -0.005 min
Response: 4187
Conc: 0.81 ng/ml

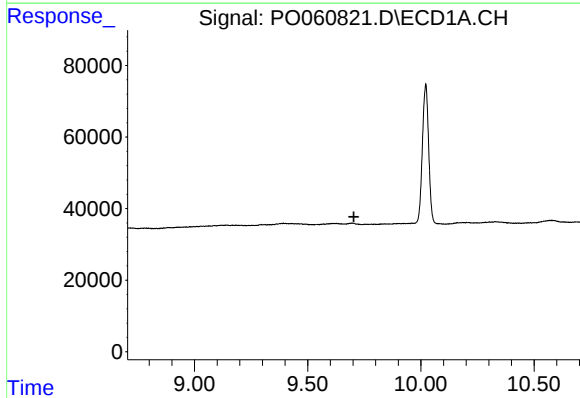

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.704 min
Response: 0
Conc: N.D.

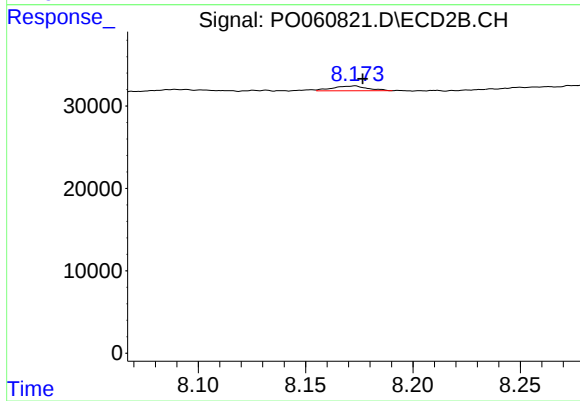

#45 AR-1268-5

R.T.: 8.173 min
Delta R.T.: -0.003 min
Response: 6656
Conc: 0.55 ng/ml