

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091319\
 Data File : P0060791.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Sep 2019 22:24
 Operator : SM/AJ
 Sample : K4859-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDW-GW200A-B4-091119

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 00:23:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.365	3.530	770915	606014	20.954	21.704
2)	SA Decachlor...	10.022	8.408	578813	455096	12.598	12.984

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091319\
Data File : P0060791.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Sep 2019 22:24
Operator : SM/AJ
Sample : K4859-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IDW-GW200A-B4-091119

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 00:23:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

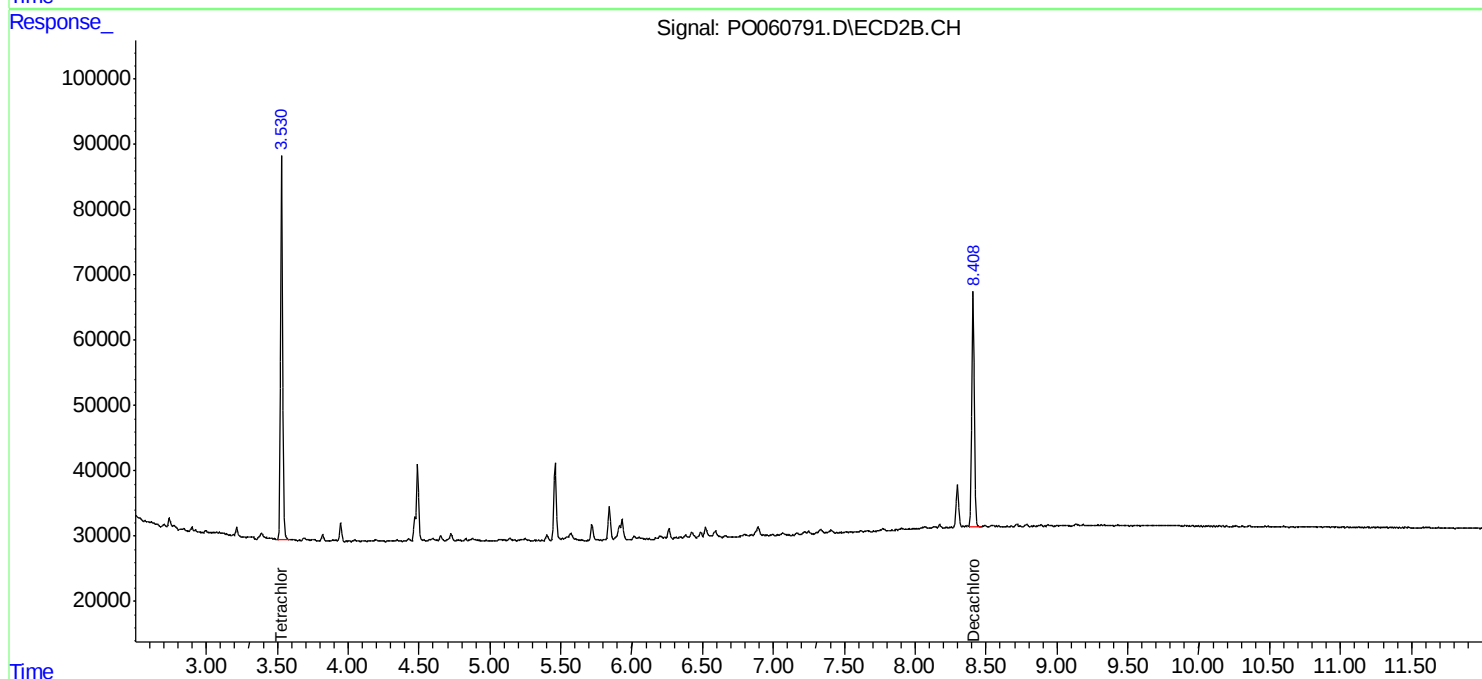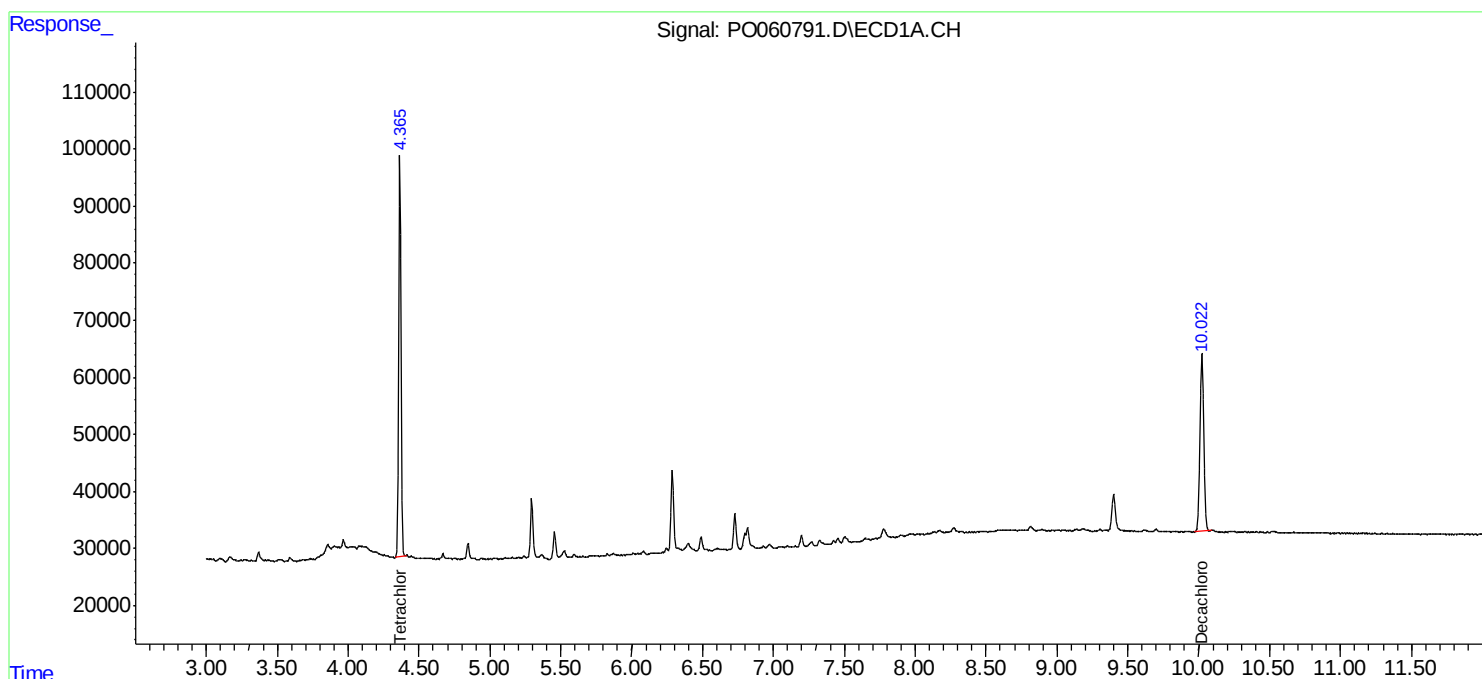


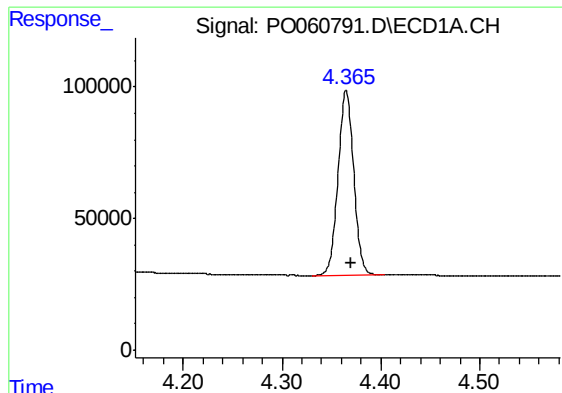

#1 Tetrachloro-m-xylene


R.T.: 4.365 min
Delta R.T.: -0.005 min
Response: 770915
Conc: 20.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
IDW-GW200A-B4-091119

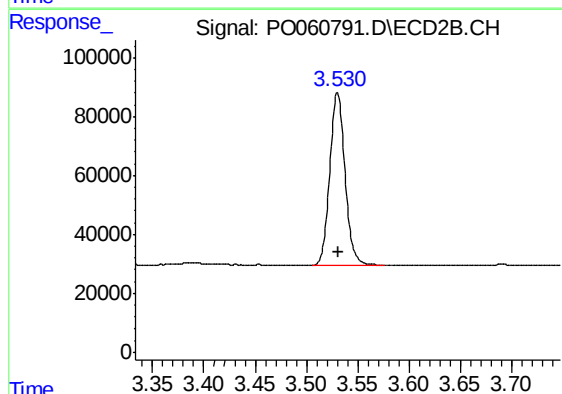


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.001 min
Response: 606014
Conc: 21.70 ng/ml

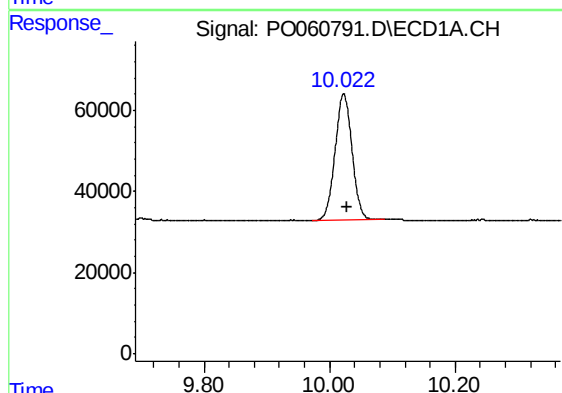

#2 Decachlorobiphenyl

R.T.: 10.022 min
Delta R.T.: -0.005 min
Response: 578813
Conc: 12.60 ng/ml

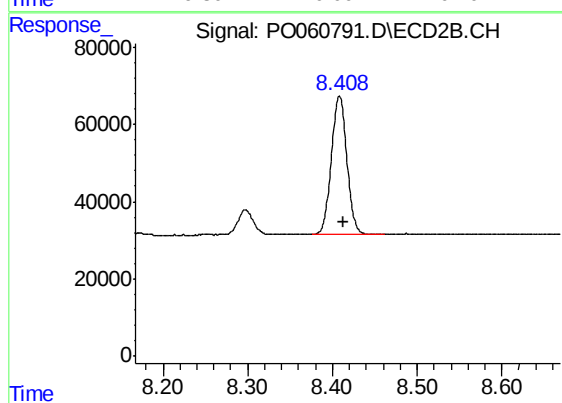

#2 Decachlorobiphenyl

R.T.: 8.408 min
Delta R.T.: -0.005 min
Response: 455096
Conc: 12.98 ng/ml