

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091319\
 Data File : P0060810.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Sep 2019 3:47
 Operator : SM/AJ
 Sample : K4855-10
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RI14-07-(0-6)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 04:46:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.367	3.532	1421795	1094083	38.645	39.183
2)	SA Decachlor...	10.026	8.410	871407	667928	18.966	19.055

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091319\
Data File : P0060810.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Sep 2019 3:47
Operator : SM/AJ
Sample : K4855-10
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RI14-07-(0-6)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 04:46:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

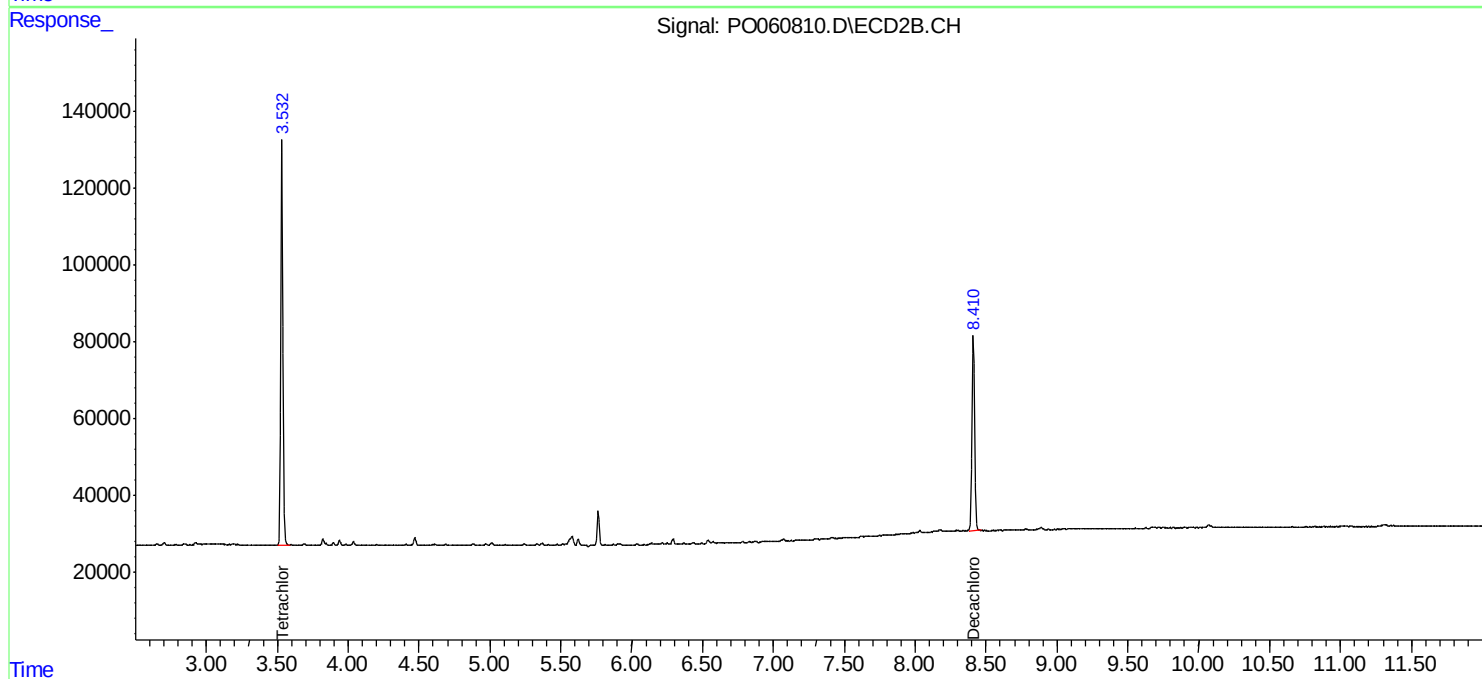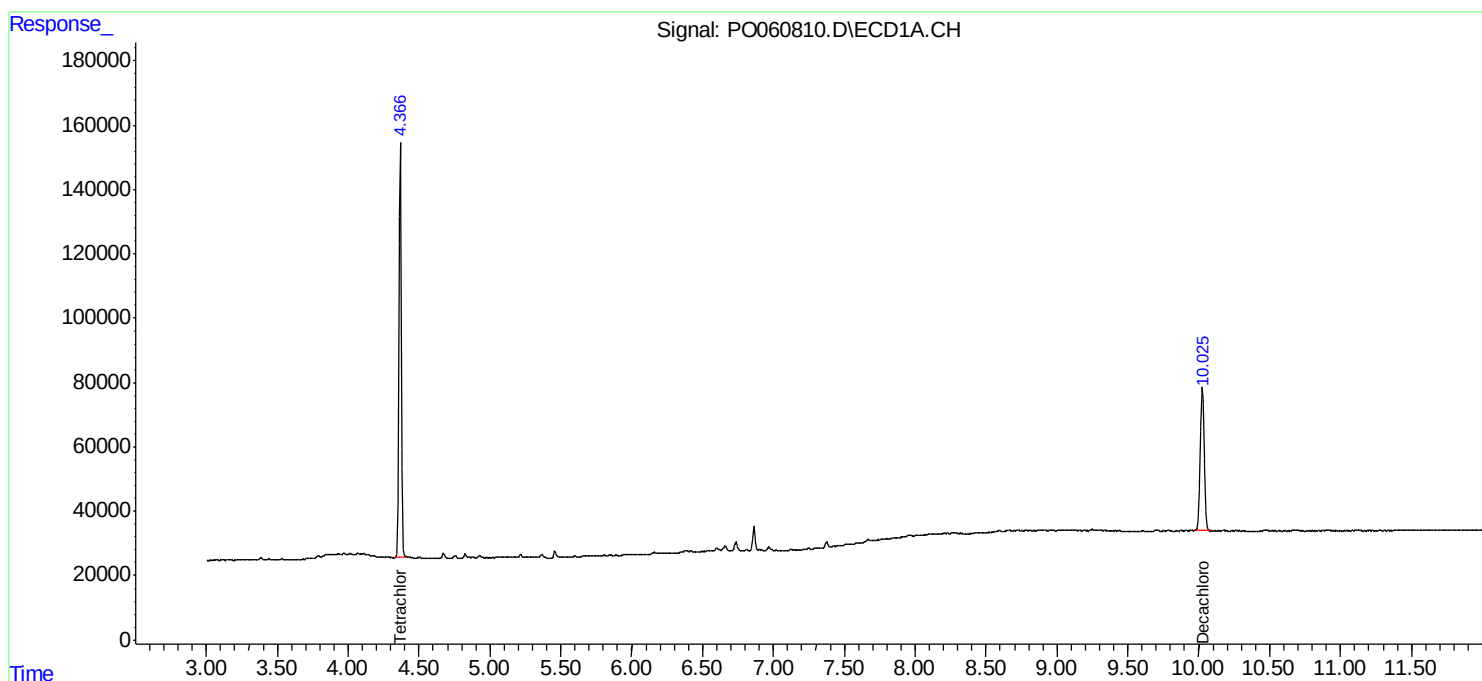


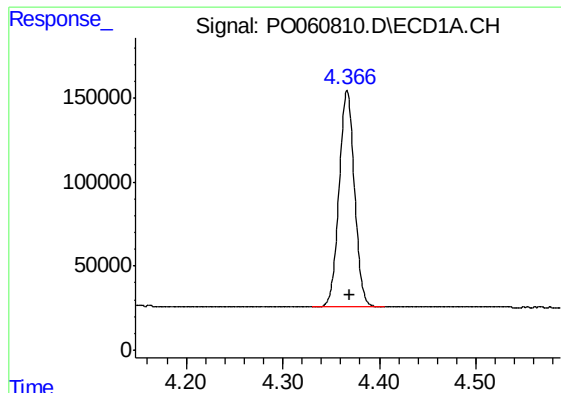

#1 Tetrachloro-m-xylene


R.T.: 4.367 min
Delta R.T.: -0.003 min
Response: 1421795
Conc: 38.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
RI14-07-(0-6)

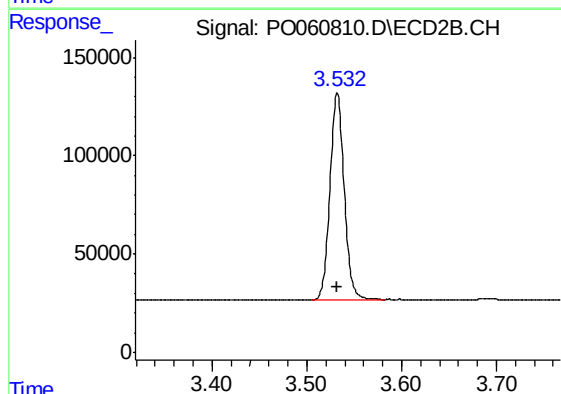


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 1094083
Conc: 39.18 ng/ml

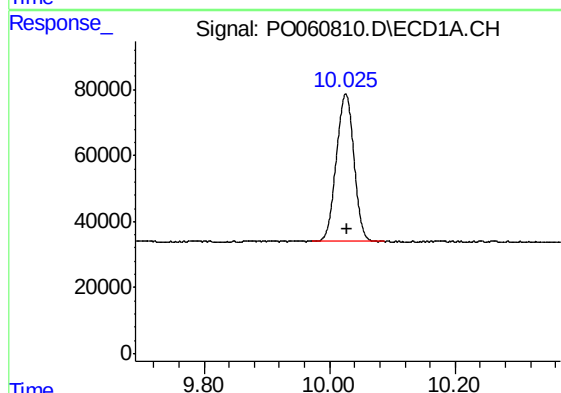

#2 Decachlorobiphenyl

R.T.: 10.026 min
Delta R.T.: -0.002 min
Response: 871407
Conc: 18.97 ng/ml

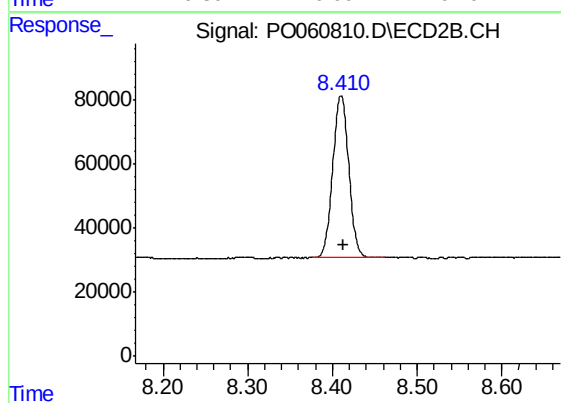

#2 Decachlorobiphenyl

R.T.: 8.410 min
Delta R.T.: -0.003 min
Response: 667928
Conc: 19.06 ng/ml