

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091319\
 Data File : P0060811.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Sep 2019 4:03
 Operator : SM/AJ
 Sample : K4855-11
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RI14-07-(6-12)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 06:46:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.367	3.531	1281854	982758	34.842	35.196
2)	SA Decachlor...	10.025	8.410	790000	603327	17.194	17.212

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091319\
Data File : P0060811.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Sep 2019 4:03
Operator : SM/AJ
Sample : K4855-11
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RI14-07-(6-12)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 06:46:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

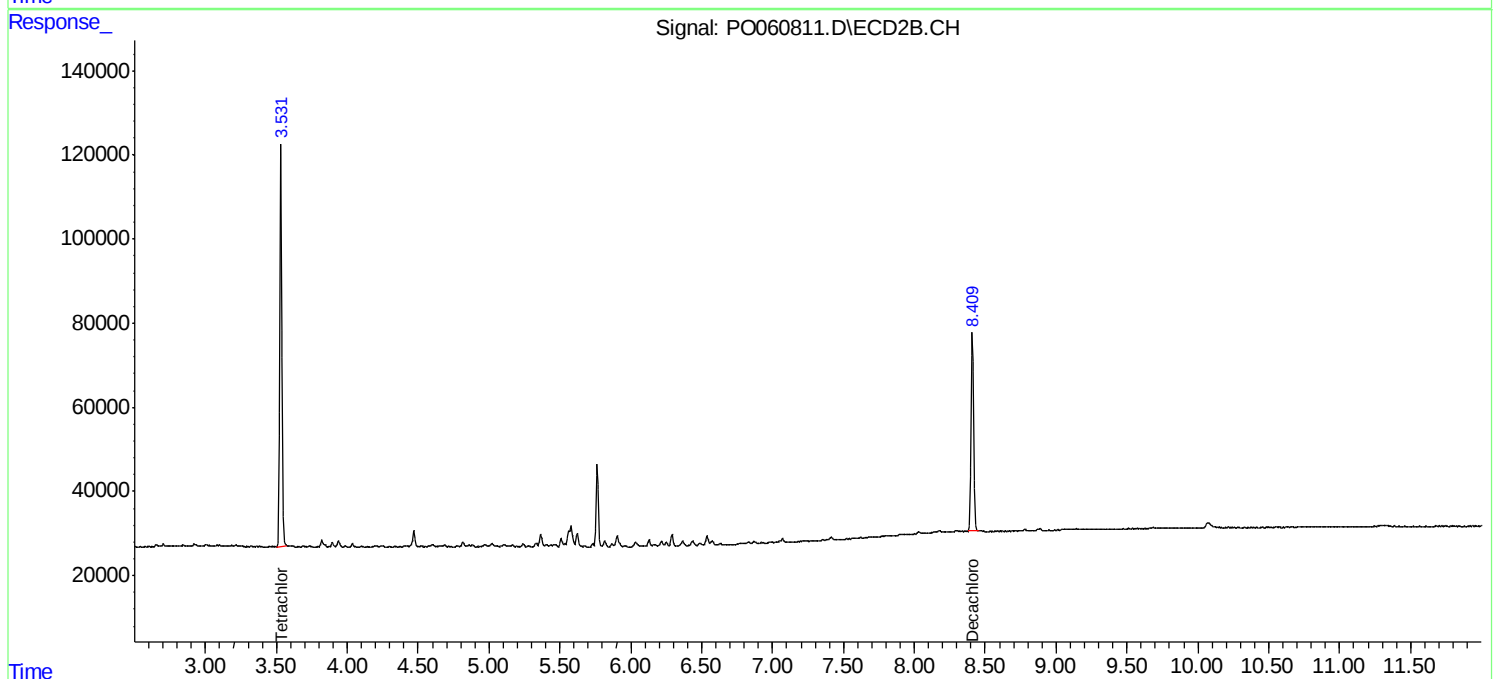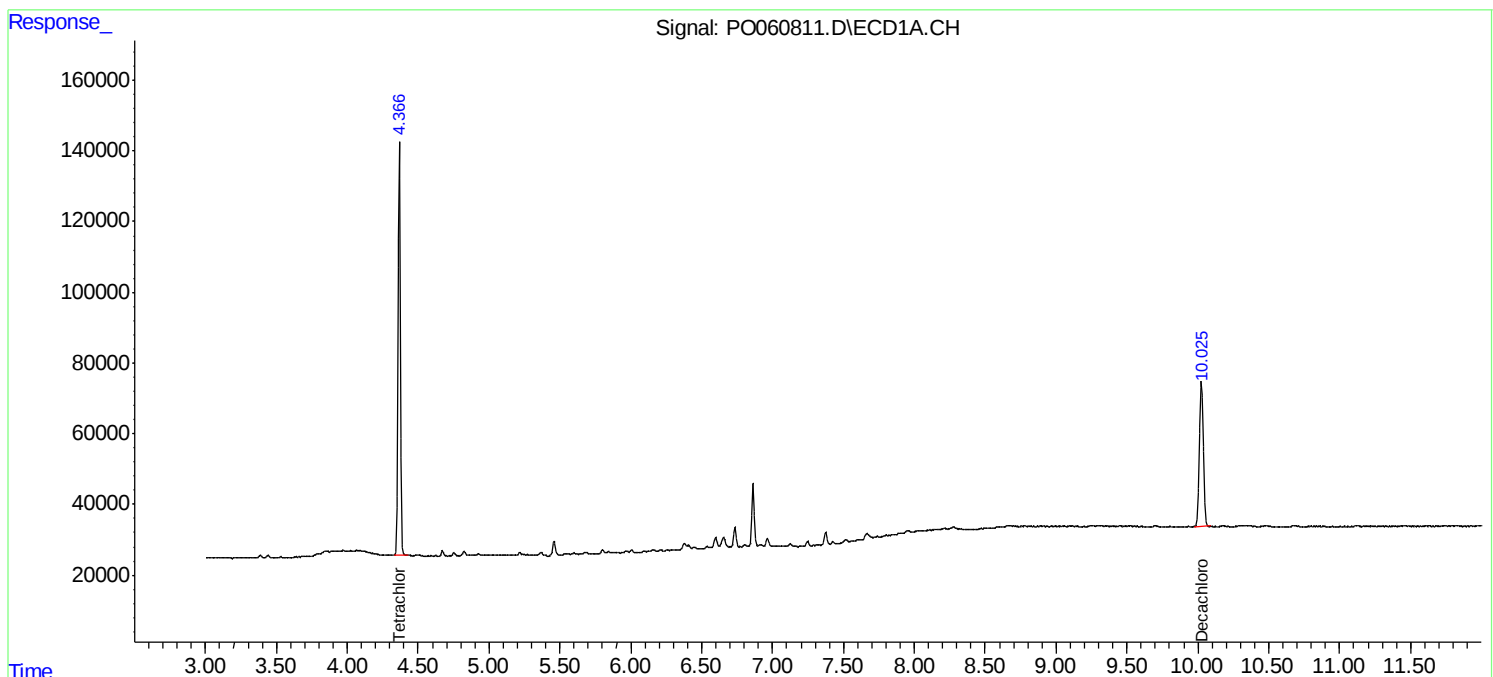


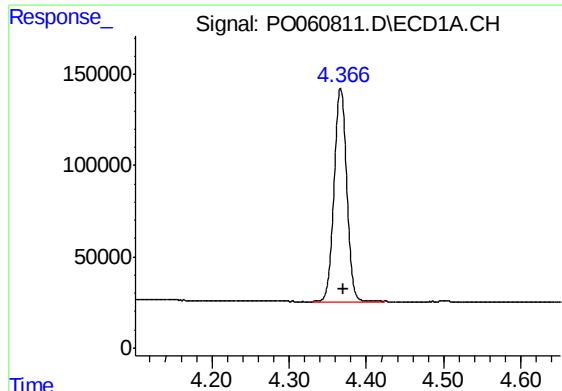

#1 Tetrachloro-m-xylene


R.T.: 4.367 min
Delta R.T.: -0.003 min
Response: 1281854
Conc: 34.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
RI14-07-(6-12)

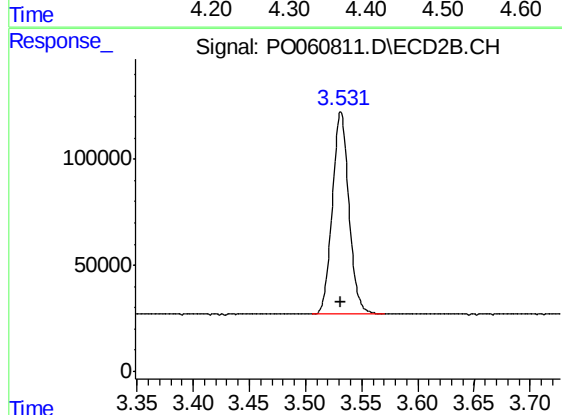


#1 Tetrachloro-m-xylene

R.T.: 3.531 min
Delta R.T.: 0.000 min
Response: 982758
Conc: 35.20 ng/ml

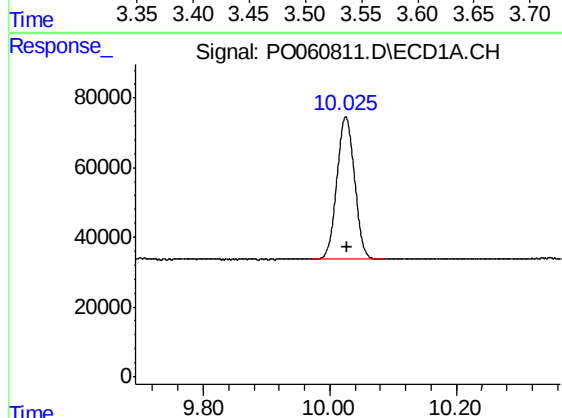

#2 Decachlorobiphenyl

R.T.: 10.025 min
Delta R.T.: -0.002 min
Response: 790000
Conc: 17.19 ng/ml

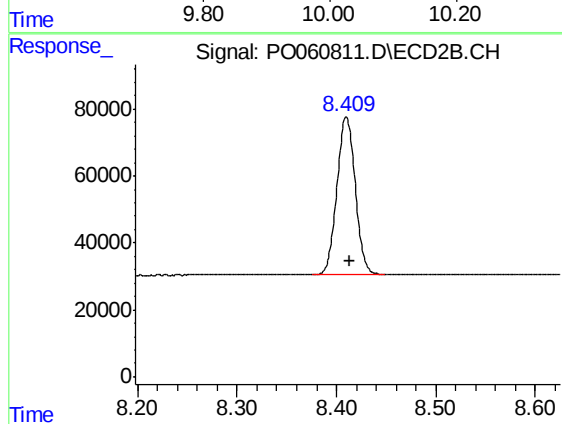

#2 Decachlorobiphenyl

R.T.: 8.410 min
Delta R.T.: -0.003 min
Response: 603327
Conc: 17.21 ng/ml