

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091321\
 Data File : P0081175.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Sep 2021 23:10
 Operator : AJ\MA
 Sample : M3687-23
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 A010015

Manual Integrations
 APPROVED

mohammad
 9/15/2021 2:00:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 05:52:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.053	1814684	560274	22.987	22.672
2) SA Decachlor...	10.991	9.414	1325567	469084	22.325	20.094
Target Compounds						
26) L6 AR-1254-1	7.172	6.204	266420	130461	82.437m	82.472m
27) L6 AR-1254-2	7.406	6.364	394817	88211	79.329m	61.013m
28) L6 AR-1254-3	7.789	6.789	197686	118668	39.097m	53.041m#
29) L6 AR-1254-4	8.085	7.028	237468	69292	63.544m	48.950m
30) L6 AR-1254-5	8.515	7.462	192519	105967	46.541	50.223

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091321\
Data File : PO081175.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Sep 2021 23:10
Operator : AJ\MA
Sample : M3687-23
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
A010015


Manual Integrations
APPROVED

mohammad
9/15/2021 2:00:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 05:52:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

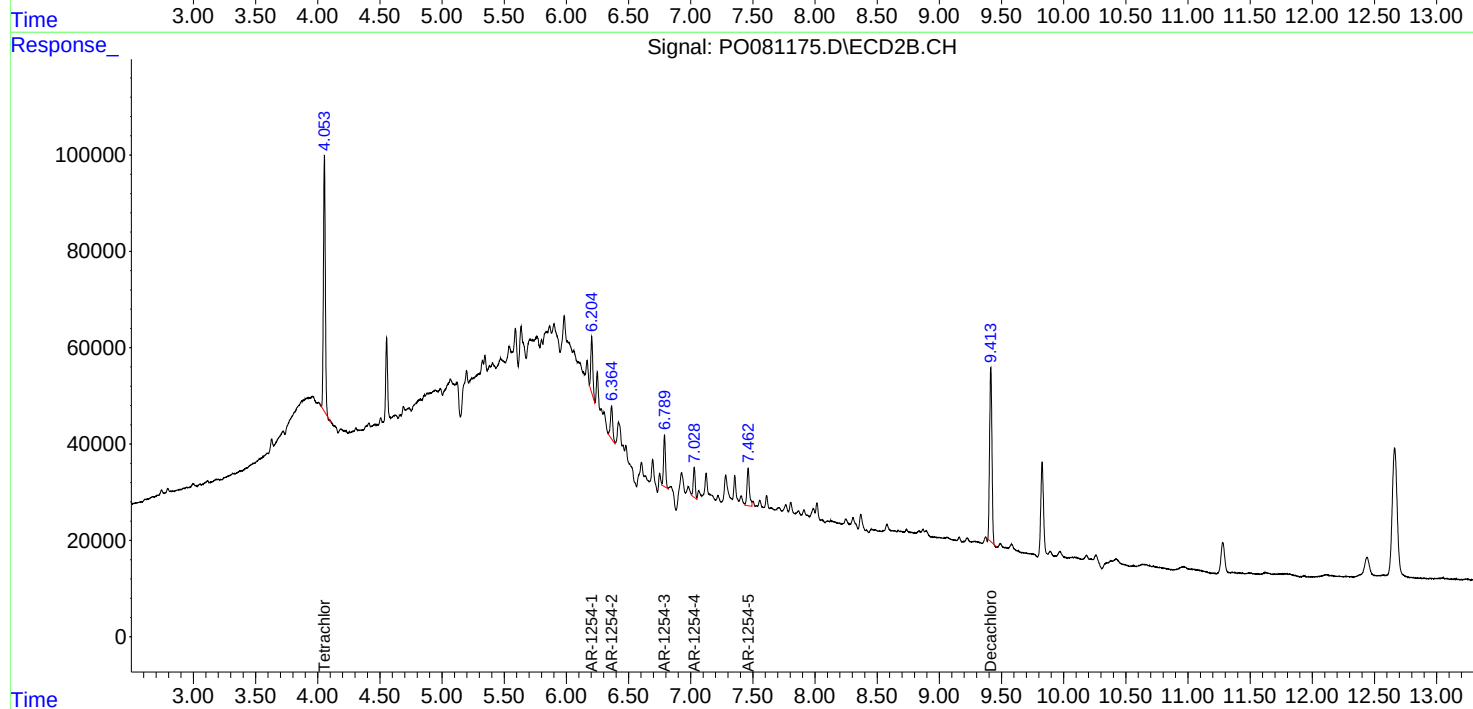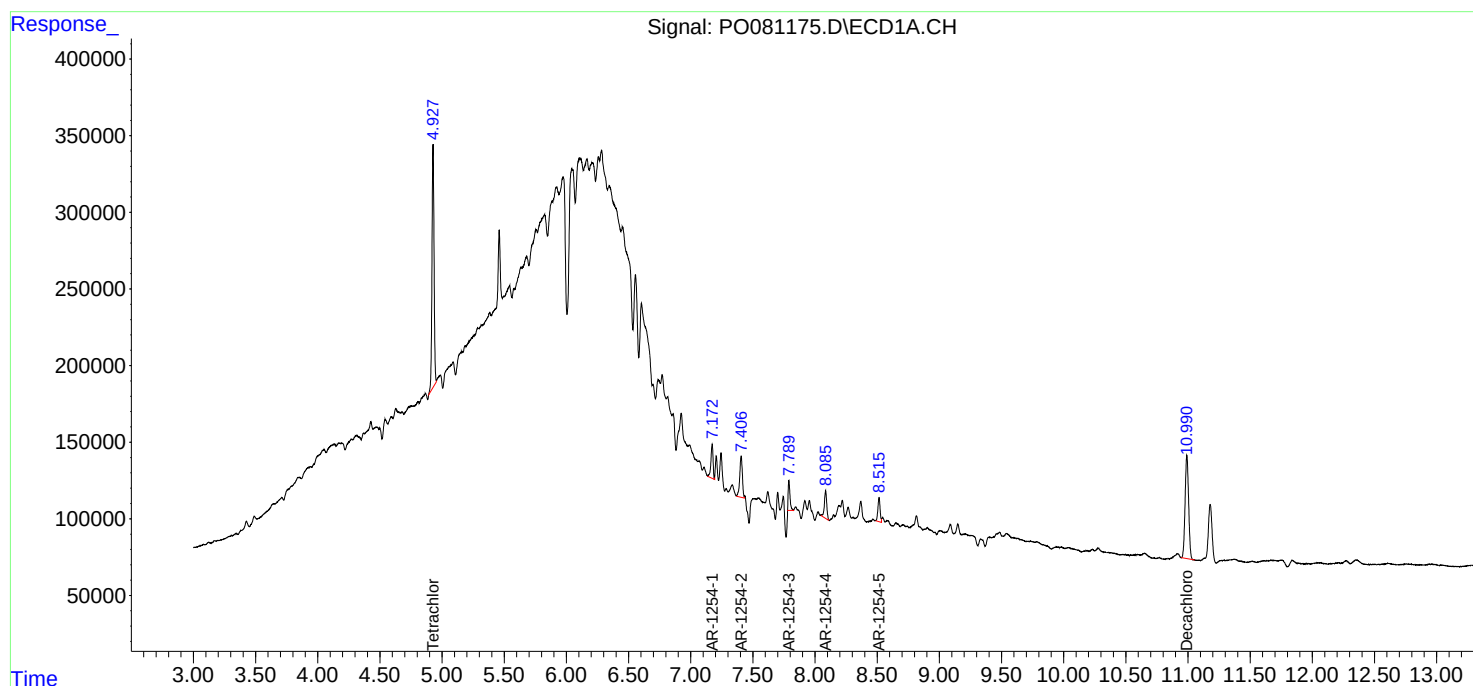

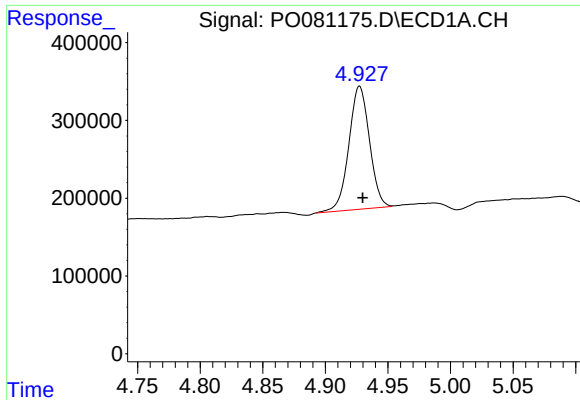


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
Delta R.T.: -0.003 min
Response: 1814684
Conc: 22.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
A010015


Manual Integrations
APPROVED

mohammad
9/15/2021 2:00:20 PM

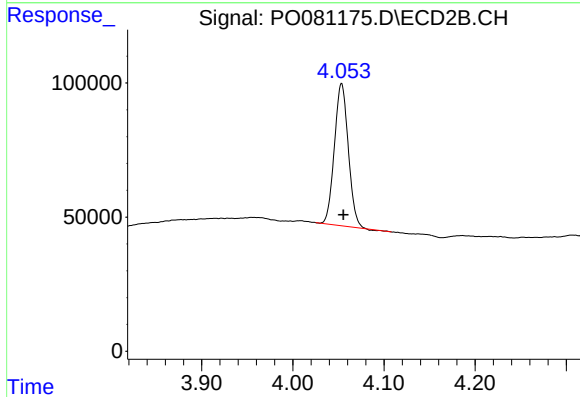


#1 Tetrachloro-m-xylene

R.T.: 4.053 min
Delta R.T.: -0.002 min
Response: 560274
Conc: 22.67 ng/ml

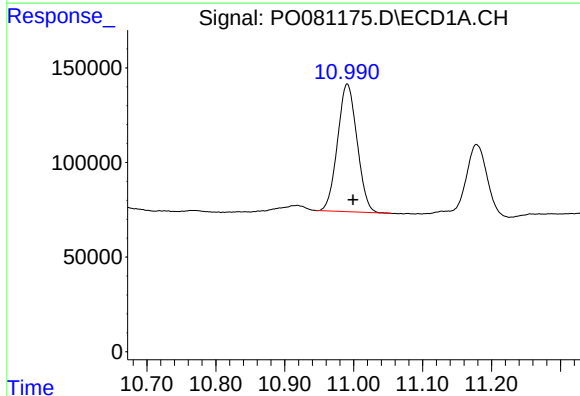


#2 Decachlorobiphenyl

R.T.: 10.991 min
Delta R.T.: -0.008 min
Response: 1325567
Conc: 22.33 ng/ml

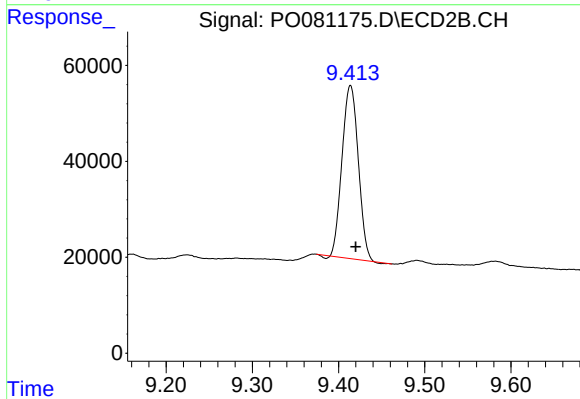

#2 Decachlorobiphenyl

R.T.: 9.414 min
Delta R.T.: -0.006 min
Response: 469084
Conc: 20.09 ng/ml

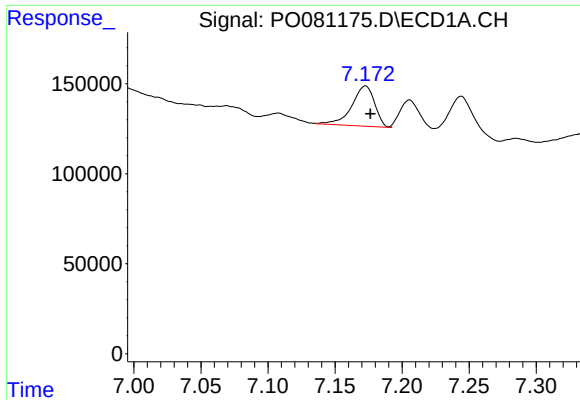


#26 AR-1254-1

R.T.: 7.172 min
Delta R.T.: -0.004 min
Response: 266420
Conc: 82.44 ng/ml m

Instrument :
ECD_O
ClientSampleId :
A010015


Manual Integrations
APPROVED

mohammad
9/15/2021 2:00:20 PM

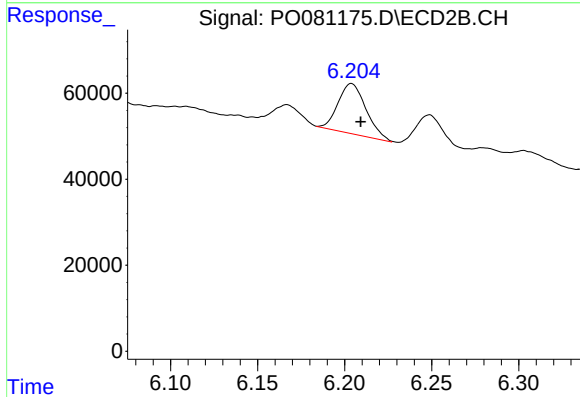


#26 AR-1254-1

R.T.: 6.204 min
Delta R.T.: -0.006 min
Response: 130461
Conc: 82.47 ng/ml m

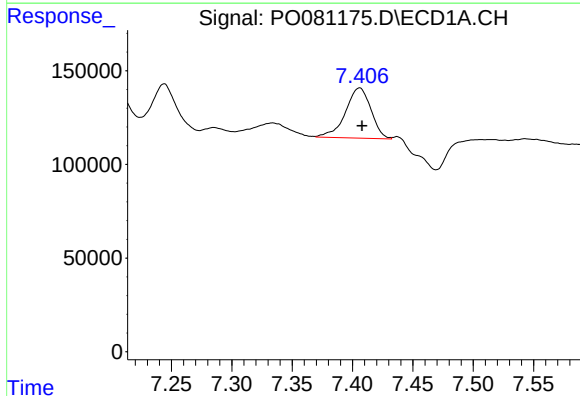


#27 AR-1254-2

R.T.: 7.406 min
Delta R.T.: -0.002 min
Response: 394817
Conc: 79.33 ng/ml m

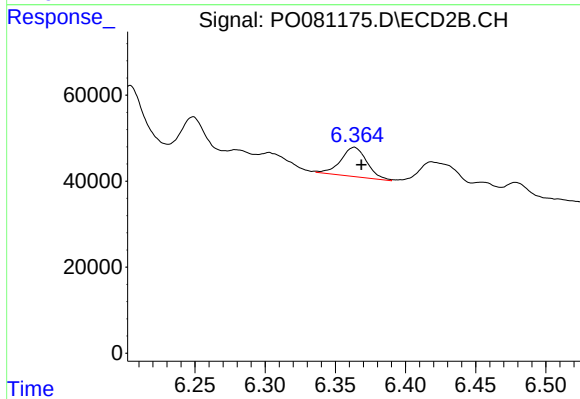

#27 AR-1254-2

R.T.: 6.364 min
Delta R.T.: -0.005 min
Response: 88211
Conc: 61.01 ng/ml m

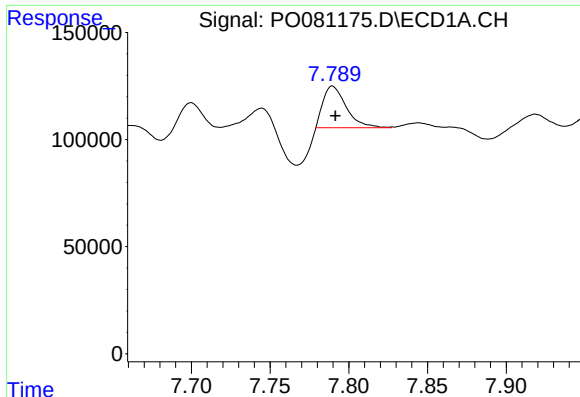


#28 AR-1254-3

R.T.: 7.789 min
Delta R.T.: -0.002 min
Response: 197686
Conc: 39.10 ng/ml m

Instrument :
ECD_O
ClientSampleId :
A010015


Manual Integrations
APPROVED

mohammad
9/15/2021 2:00:20 PM

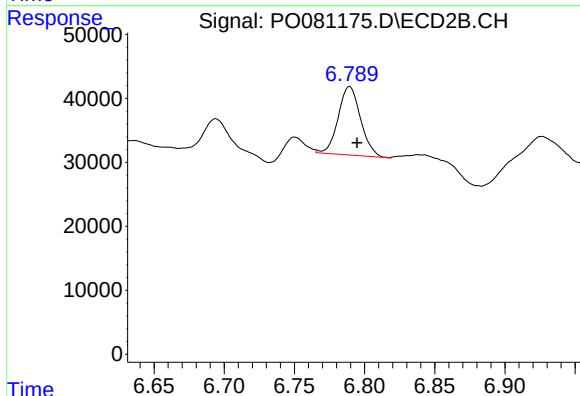


#28 AR-1254-3

R.T.: 6.789 min
Delta R.T.: -0.006 min
Response: 118668
Conc: 53.04 ng/ml m

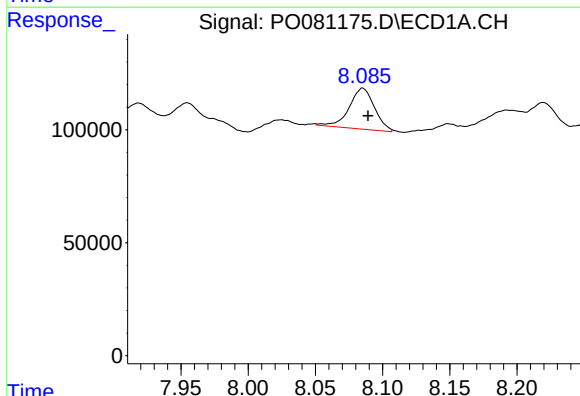


#29 AR-1254-4

R.T.: 8.085 min
Delta R.T.: -0.005 min
Response: 237468
Conc: 63.54 ng/ml m

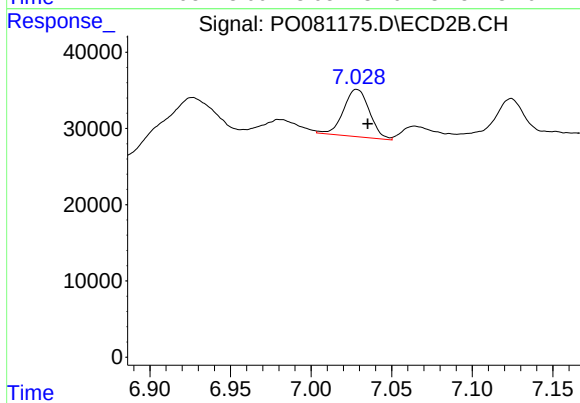

#29 AR-1254-4

R.T.: 7.028 min
Delta R.T.: -0.007 min
Response: 69292
Conc: 48.95 ng/ml m

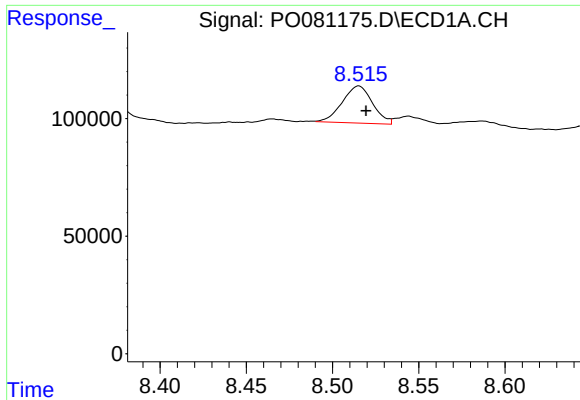


#30 AR-1254-5

R.T.: 8.515 min
Delta R.T.: -0.004 min
Response: 192519
Conc: 46.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
A010015

Manual Integrations
APPROVED

mohammad
9/15/2021 2:00:20 PM

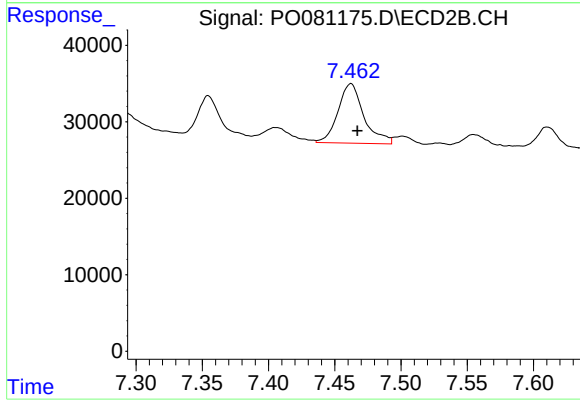

#30 AR-1254-5

R.T.: 7.462 min
Delta R.T.: -0.005 min
Response: 105967
Conc: 50.22 ng/ml