

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091321\
 Data File : P0081183.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Sep 2021 1:58
 Operator : AJ\MA
 Sample : M3687-31
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 A003145

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 05:54:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.053	2056144	636423	26.046	25.754
2) SA Decachlor...	10.990	9.412	1519920	587521	25.598	25.168

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091321\
Data File : P0081183.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Sep 2021 1:58
Operator : AJ\MA
Sample : M3687-31
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
A003145

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 05:54:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

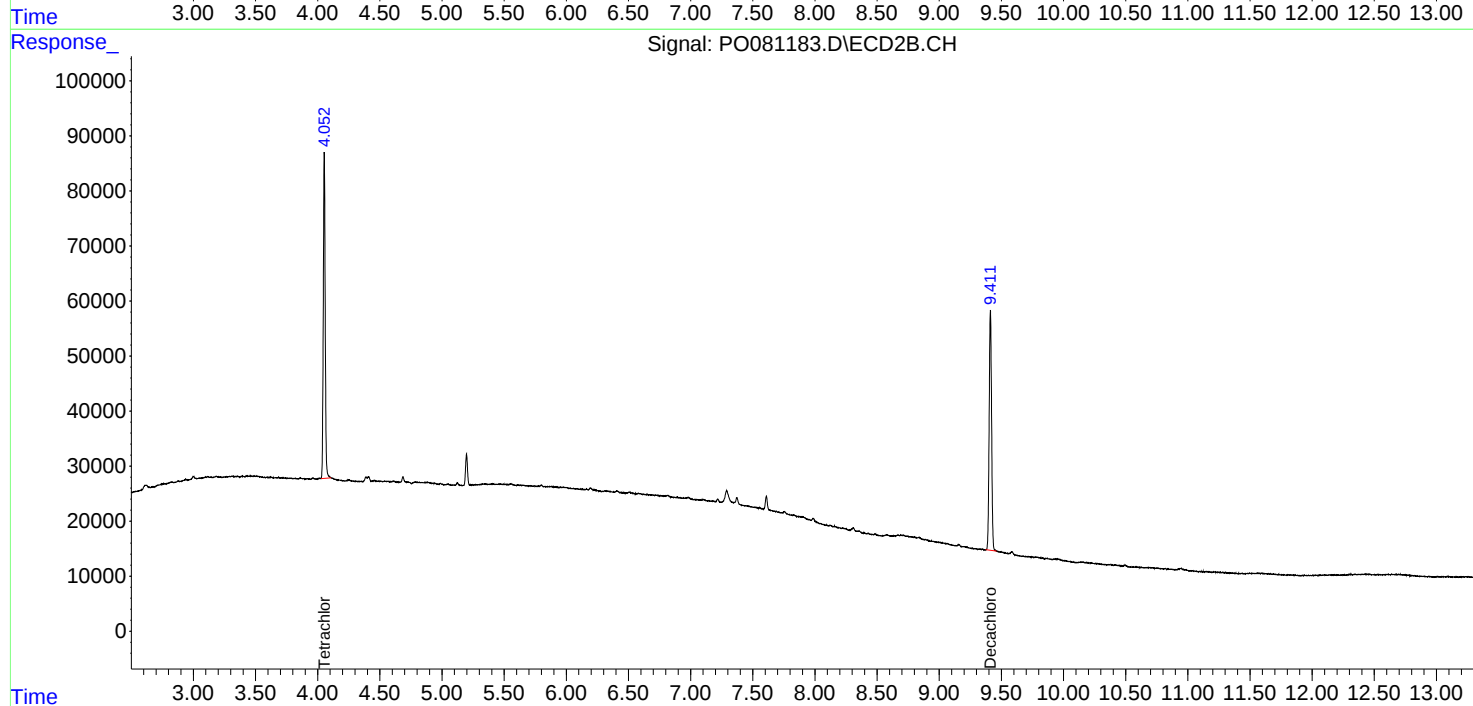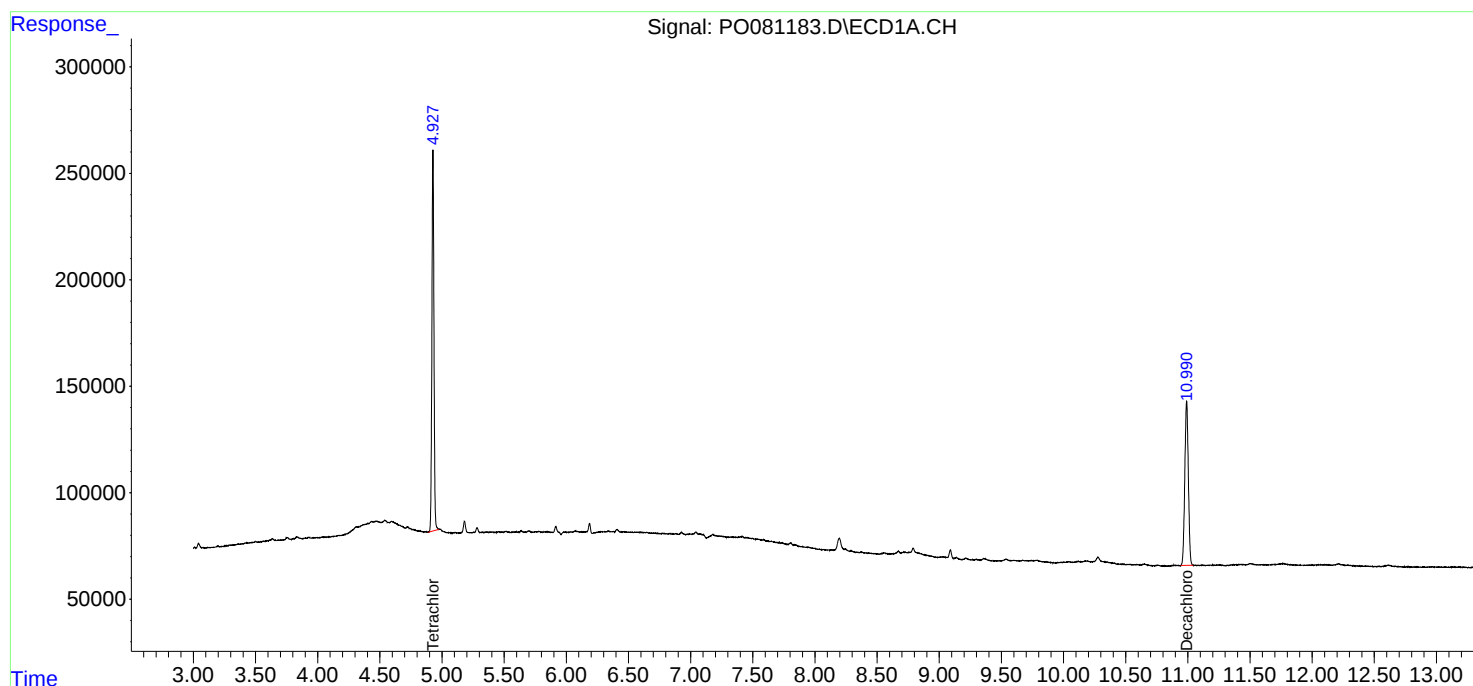


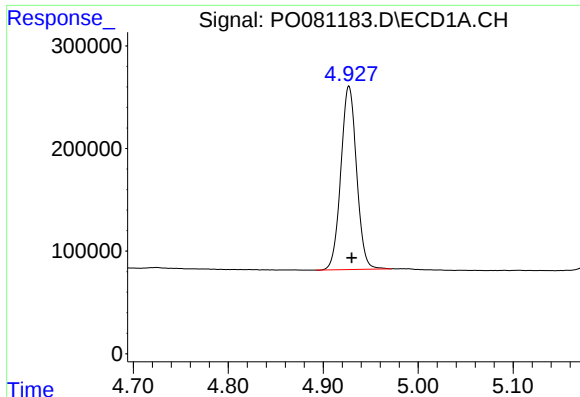

#1 Tetrachloro-m-xylene


R.T.: 4.927 min
Delta R.T.: -0.003 min
Response: 2056144
Conc: 26.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
A003145

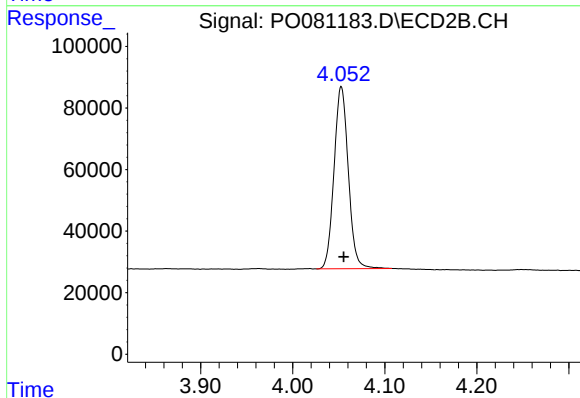


#1 Tetrachloro-m-xylene

R.T.: 4.053 min
Delta R.T.: -0.003 min
Response: 636423
Conc: 25.75 ng/ml

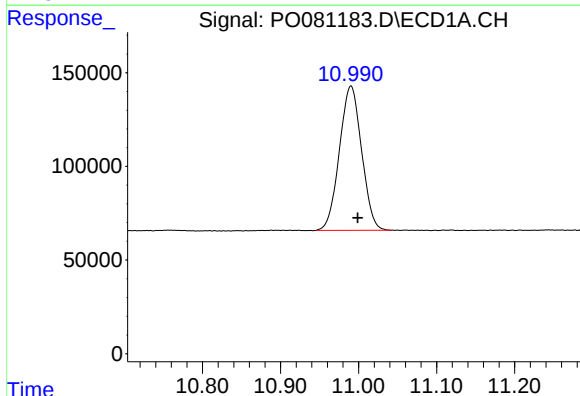

#2 Decachlorobiphenyl

R.T.: 10.990 min
Delta R.T.: -0.009 min
Response: 1519920
Conc: 25.60 ng/ml

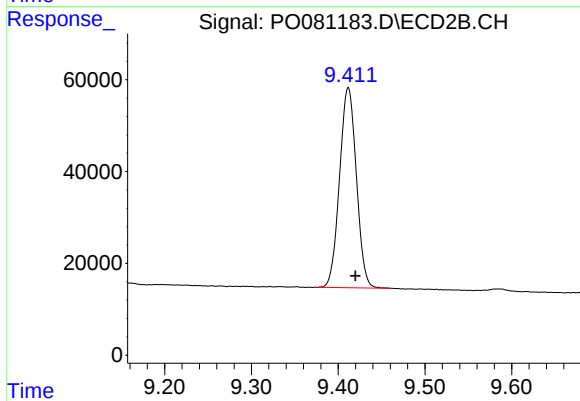

#2 Decachlorobiphenyl

R.T.: 9.412 min
Delta R.T.: -0.008 min
Response: 587521
Conc: 25.17 ng/ml