

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091321\
 Data File : P0081218.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Sep 2021 12:38
 Operator : AJ\MA
 Sample : M3696-11 20X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 333000-END-1-2

Manual Integrations
 APPROVED

mohammad
 9/15/2021 2:00:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 14:19:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.052	60532	19531	0.767	0.790
2) SA Decachlor...	10.985	9.412	50580	20964	0.852m	0.898

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091321\
Data File : P0081218.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Sep 2021 12:38
Operator : AJ\MA
Sample : M3696-11 20X
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
333000-END-1-2


Manual Integrations
APPROVED

mohammad
9/15/2021 2:00:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 14:19:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

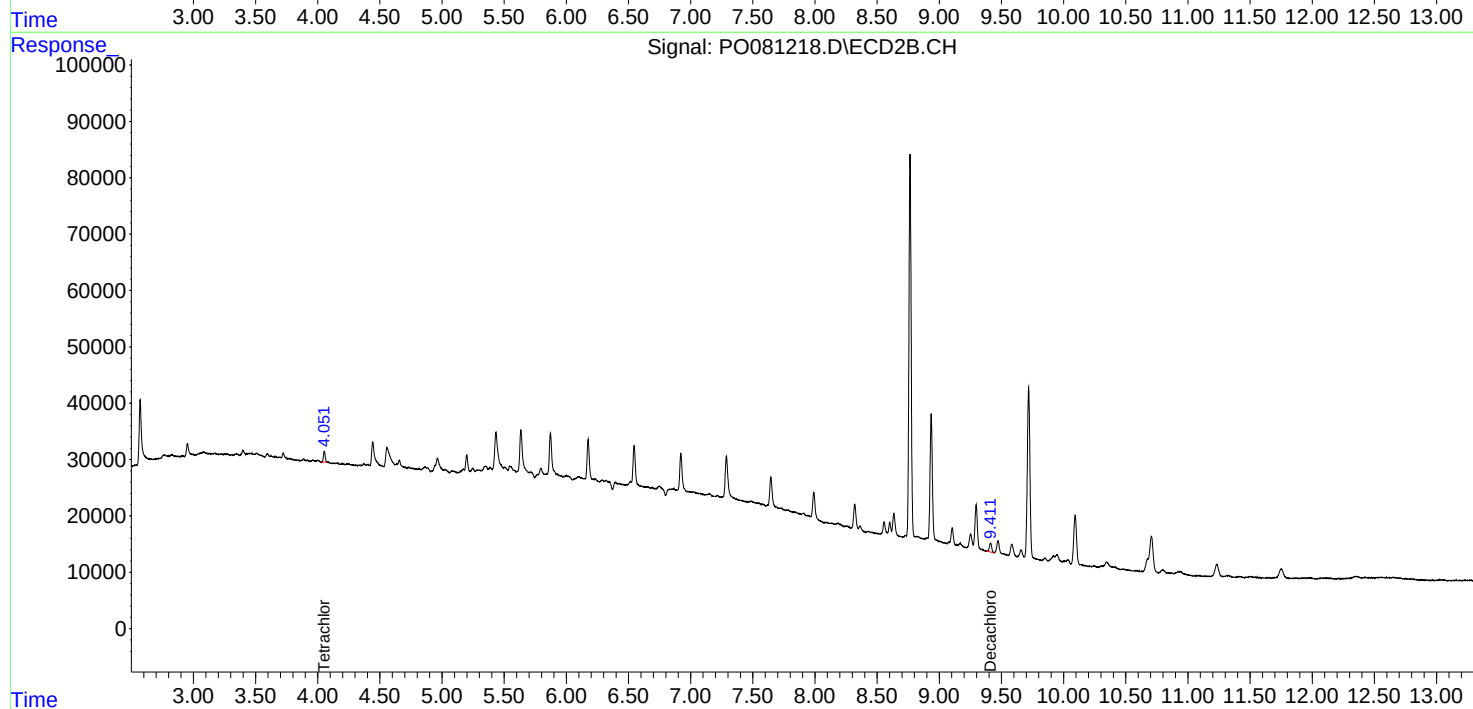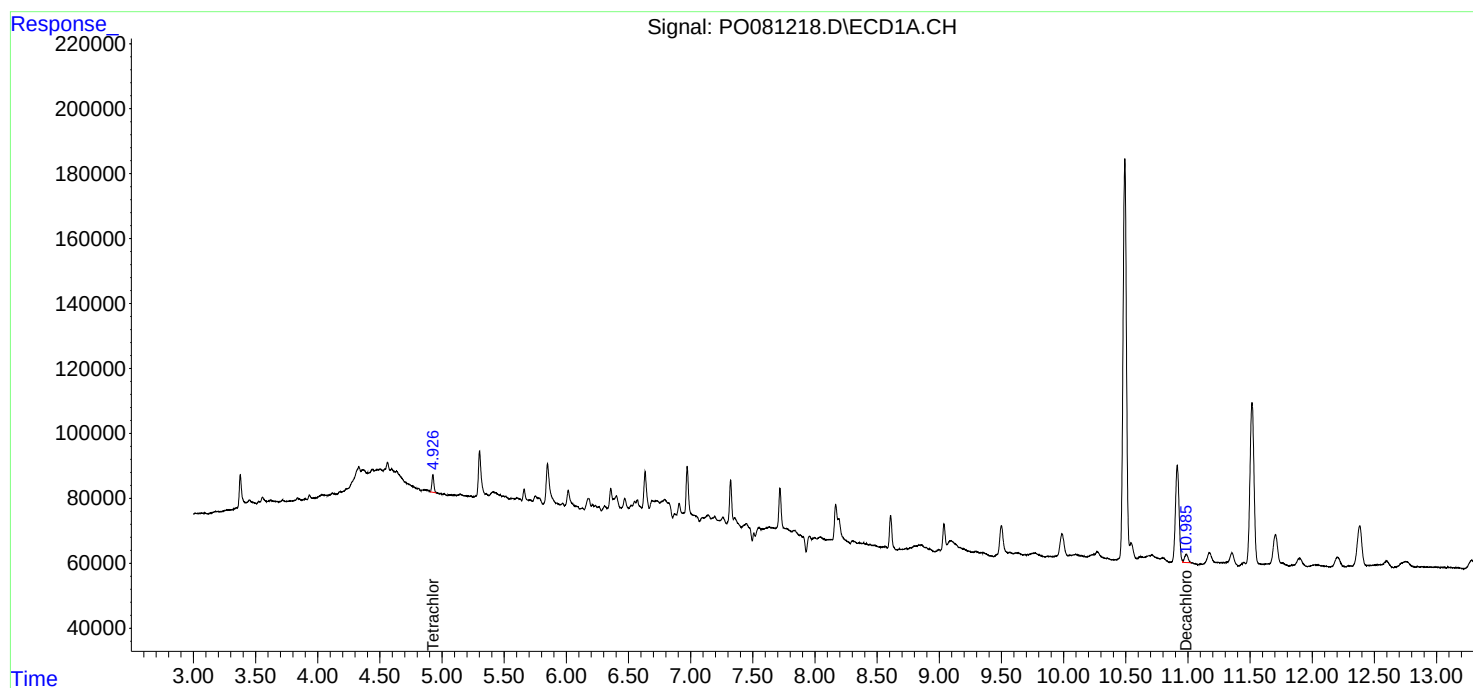

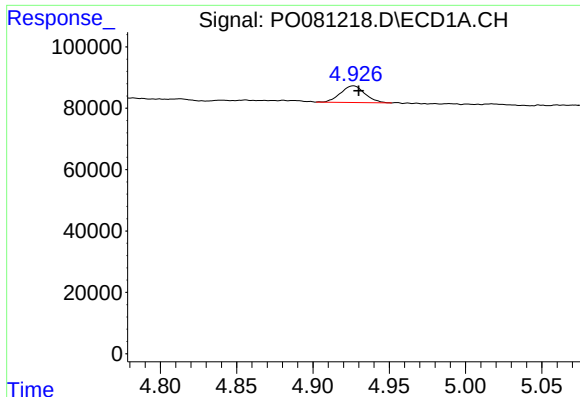


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
Delta R.T.: -0.003 min
Response: 60532
Conc: 0.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
333000-END-1-2


Manual Integrations
APPROVED

mohammad
9/15/2021 2:00:44 PM

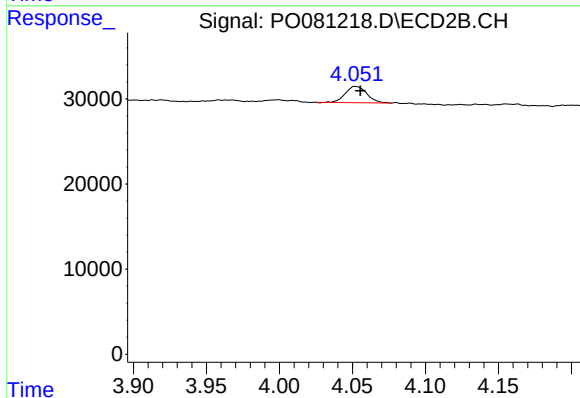


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: -0.003 min
Response: 19531
Conc: 0.79 ng/ml

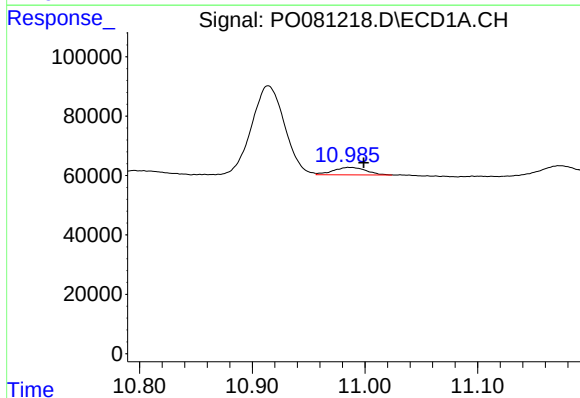

#2 Decachlorobiphenyl

R.T.: 10.985 min
Delta R.T.: -0.014 min
Response: 50580
Conc: 0.85 ng/ml m

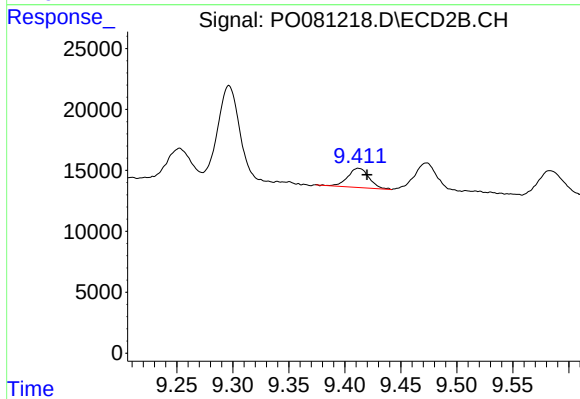

#2 Decachlorobiphenyl

R.T.: 9.412 min
Delta R.T.: -0.008 min
Response: 20964
Conc: 0.90 ng/ml