

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091323\
 Data File : P0097983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2023 14:58
 Operator : YP/AJ
 Sample : 04396-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CHRT-24313

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/14/2023
 Supervised By :Ankita Jodhani 09/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 16:33:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 07 02:56:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.440	3.621	44624599	11502712	11.201	12.011
2) SA Decachlor...	10.285	8.651	32550481	18218072	17.421	21.323
Target Compounds						
31) L7 AR-1260-1	7.236	6.200	10924757	3337043	77.305	62.721
32) L7 AR-1260-2	7.493	6.389	32320376	5192226	213.821	82.918 #
33) L7 AR-1260-3	7.858	6.543	8733472	3839576	77.097	66.585
34) L7 AR-1260-4	8.084	7.022	22021124	6861820	185.246m	146.273
35) L7 AR-1260-5	8.414	7.259	15944205	8980674	77.884	90.599

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091323\
Data File : PO097983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2023 14:58
Operator : YP/AJ
Sample : 04396-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CHRT-24313


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 16:33:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 07 02:56:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

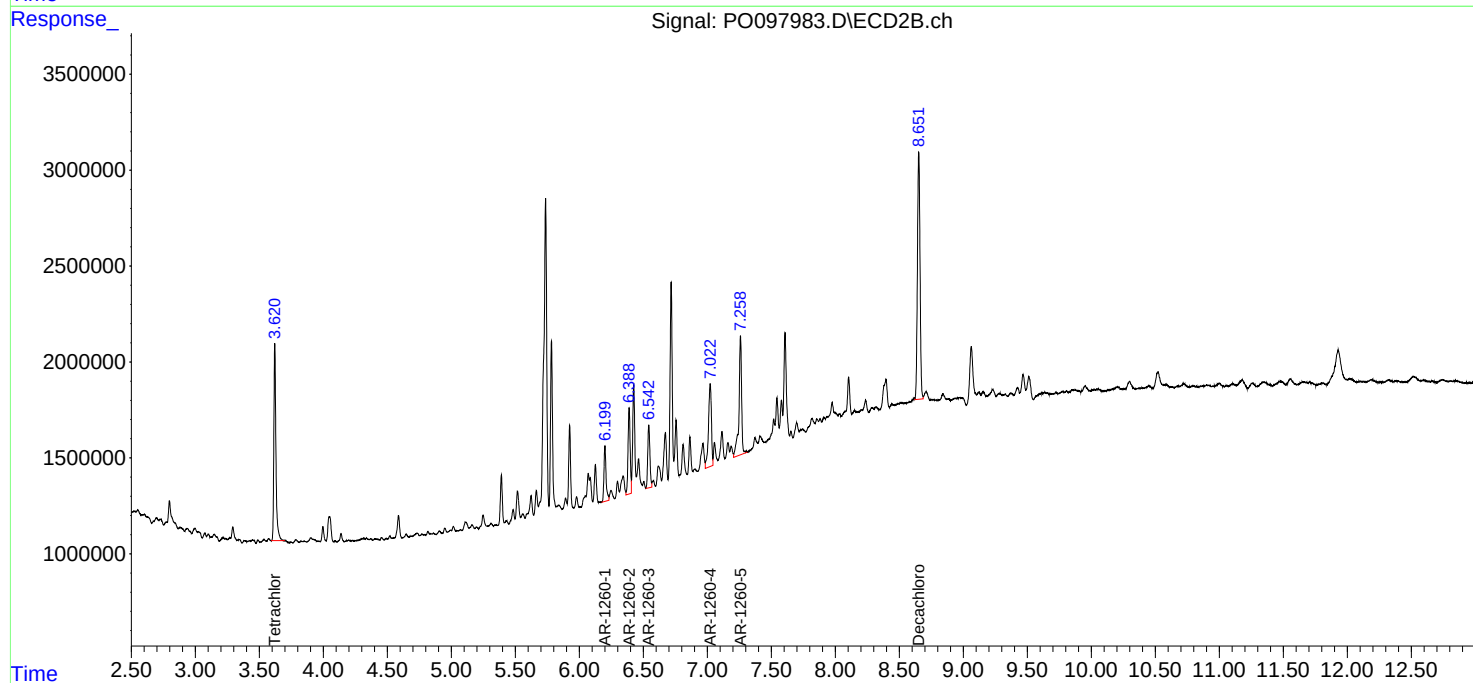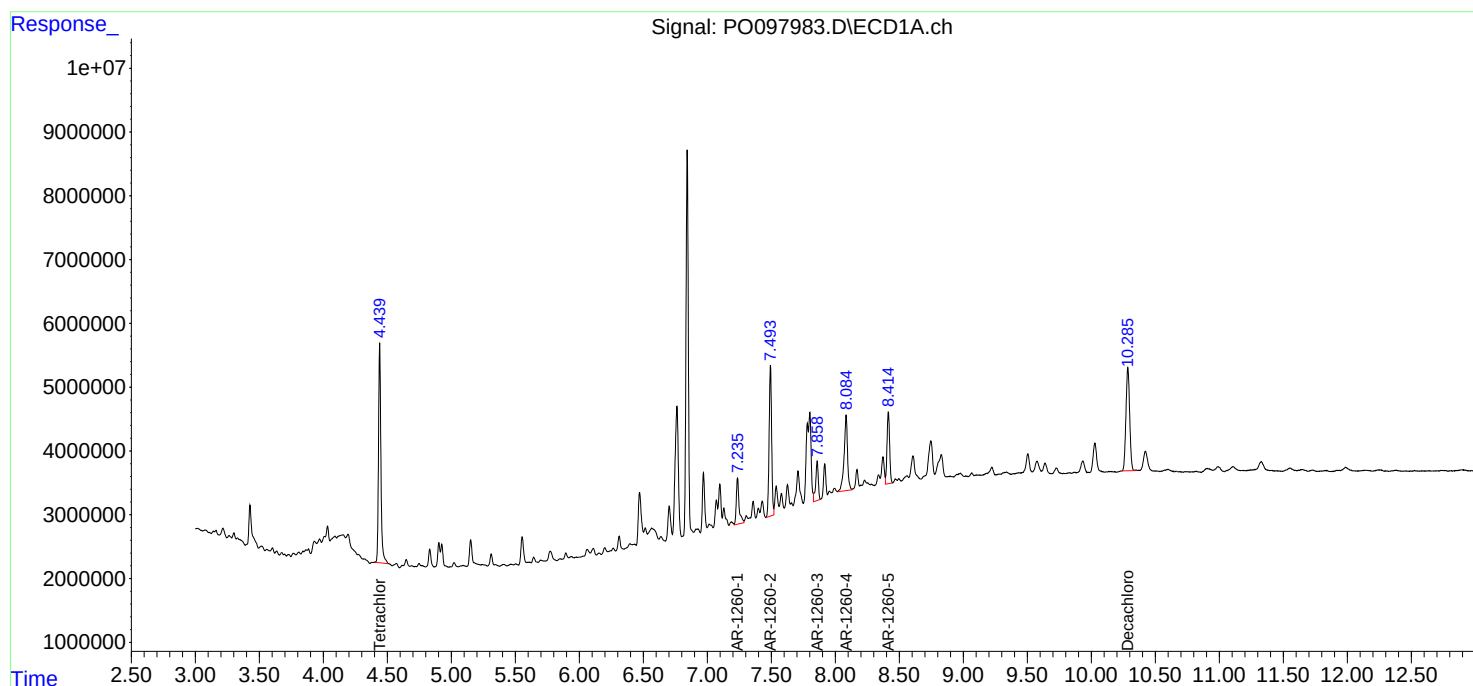

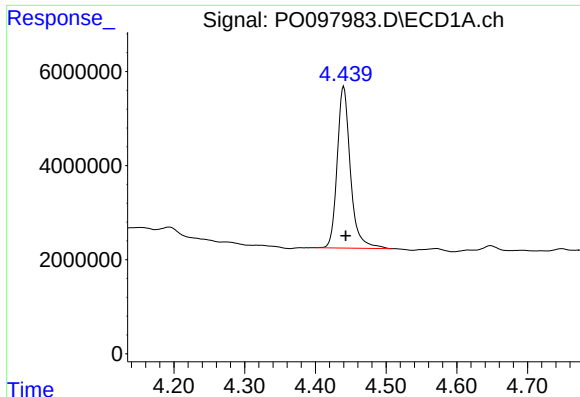


#1 Tetrachloro-m-xylene

R.T.: 4.440 min
Delta R.T.: -0.003 min
Response: 44624599
Conc: 11.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-24313


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

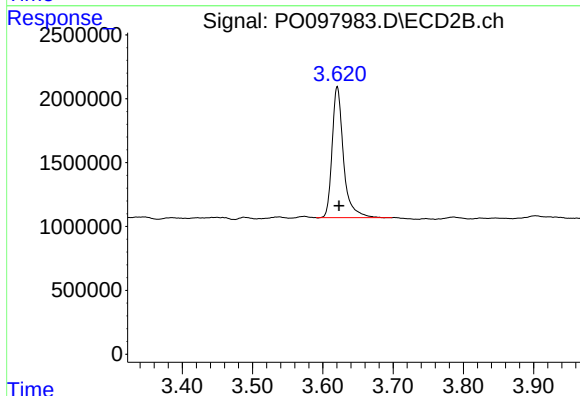


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.002 min
Response: 11502712
Conc: 12.01 ng/ml

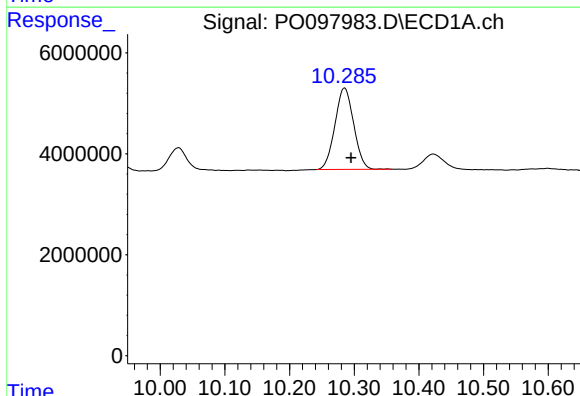


#2 Decachlorobiphenyl

R.T.: 10.285 min
Delta R.T.: -0.010 min
Response: 32550481
Conc: 17.42 ng/ml

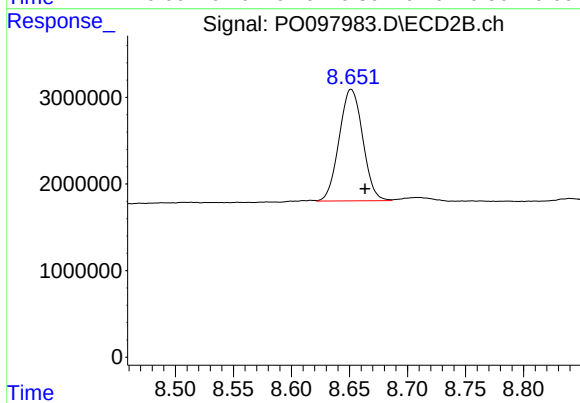

#2 Decachlorobiphenyl

R.T.: 8.651 min
Delta R.T.: -0.012 min
Response: 18218072
Conc: 21.32 ng/ml

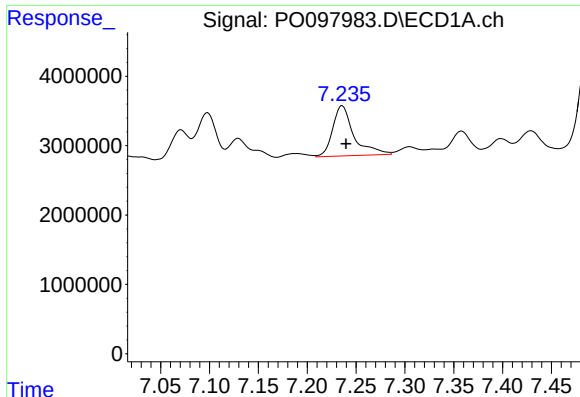


#31 AR-1260-1

R.T.: 7.236 min
Delta R.T.: -0.004 min
Response: 10924757
Conc: 77.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-24313


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

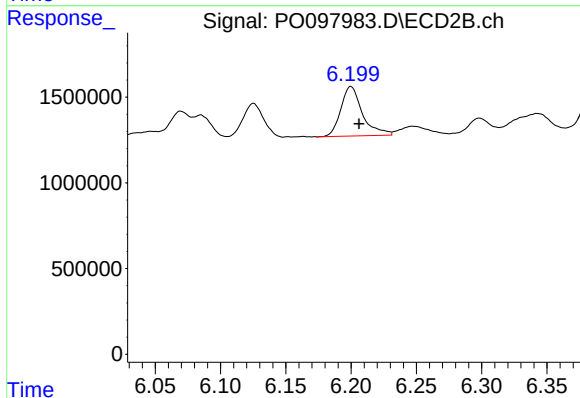


#31 AR-1260-1

R.T.: 6.200 min
Delta R.T.: -0.006 min
Response: 3337043
Conc: 62.72 ng/ml

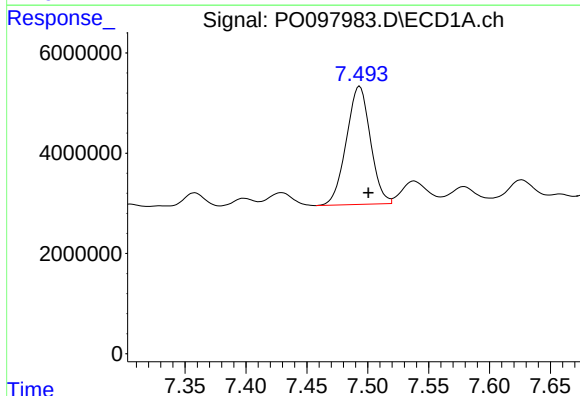


#32 AR-1260-2

R.T.: 7.493 min
Delta R.T.: -0.007 min
Response: 32320376
Conc: 213.82 ng/ml

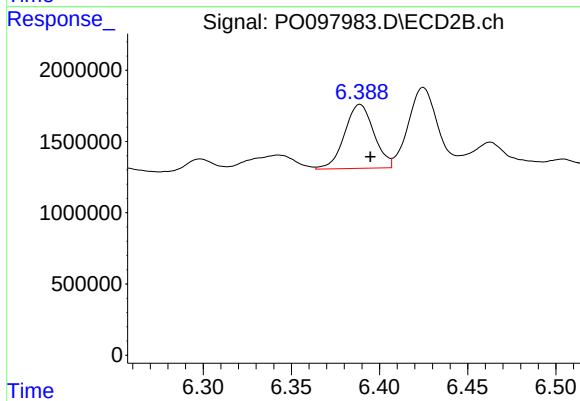

#32 AR-1260-2

R.T.: 6.389 min
Delta R.T.: -0.006 min
Response: 5192226
Conc: 82.92 ng/ml

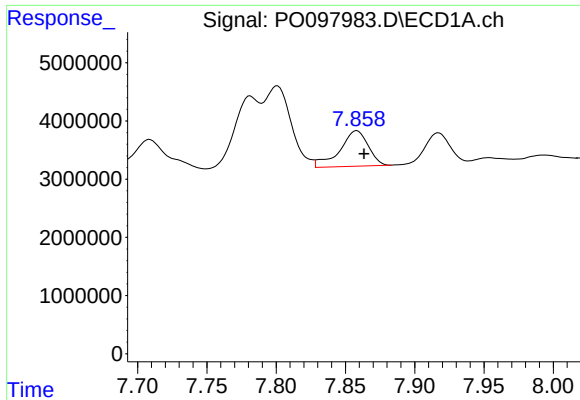


#33 AR-1260-3

R.T.: 7.858 min
Delta R.T.: -0.005 min
Response: 8733472
Conc: 77.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-24313


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

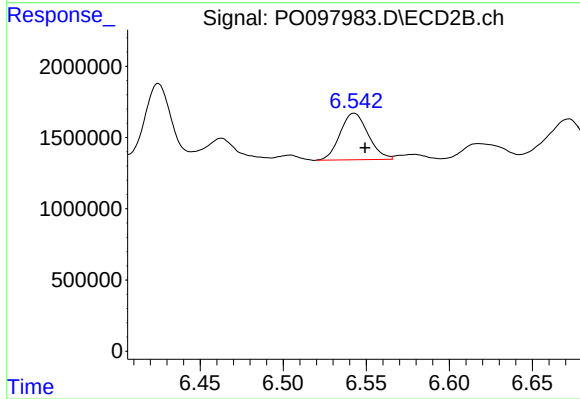


#33 AR-1260-3

R.T.: 6.543 min
Delta R.T.: -0.007 min
Response: 3839576
Conc: 66.58 ng/ml

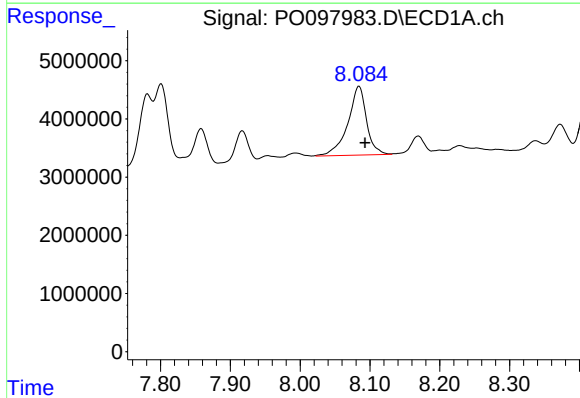


#34 AR-1260-4

R.T.: 8.084 min
Delta R.T.: -0.009 min
Response: 22021124
Conc: 185.25 ng/ml m

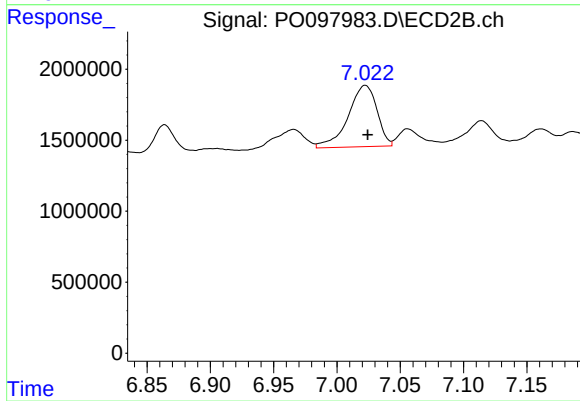

#34 AR-1260-4

R.T.: 7.022 min
Delta R.T.: -0.002 min
Response: 6861820
Conc: 146.27 ng/ml

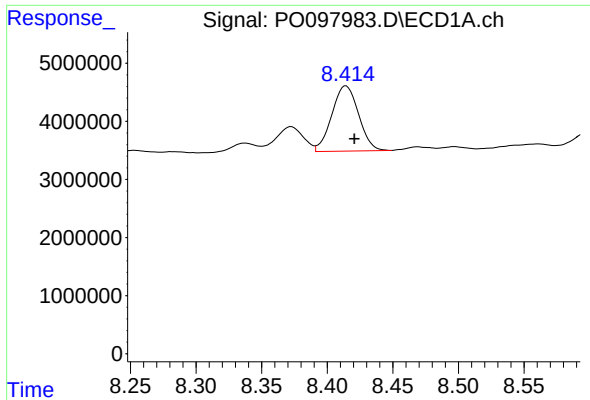


#35 AR-1260-5

R.T.: 8.414 min
Delta R.T.: -0.006 min
Response: 15944205
Conc: 77.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-24313

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

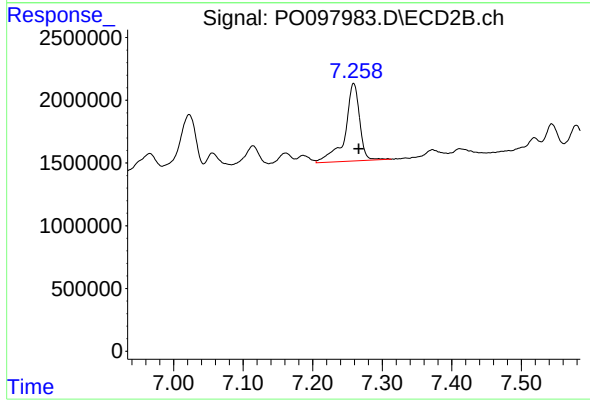

#35 AR-1260-5

R.T.: 7.259 min
Delta R.T.: -0.007 min
Response: 8980674
Conc: 90.60 ng/ml