

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091323\
 Data File : P0098000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2023 20:00
 Operator : YP/AJ
 Sample : 04405-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-02-091223

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/14/2023
 Supervised By :Ankita Jodhani 09/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 01:17:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 07 02:56:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.439	3.620	60347965	15967157	15.147m	16.673m
2) SA Decachlor...	10.283	8.651	29204715	12846657	15.630	15.036

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091323\
Data File : PO098000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2023 20:00
Operator : YP/AJ
Sample : 04405-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-02-091223


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 01:17:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 07 02:56:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

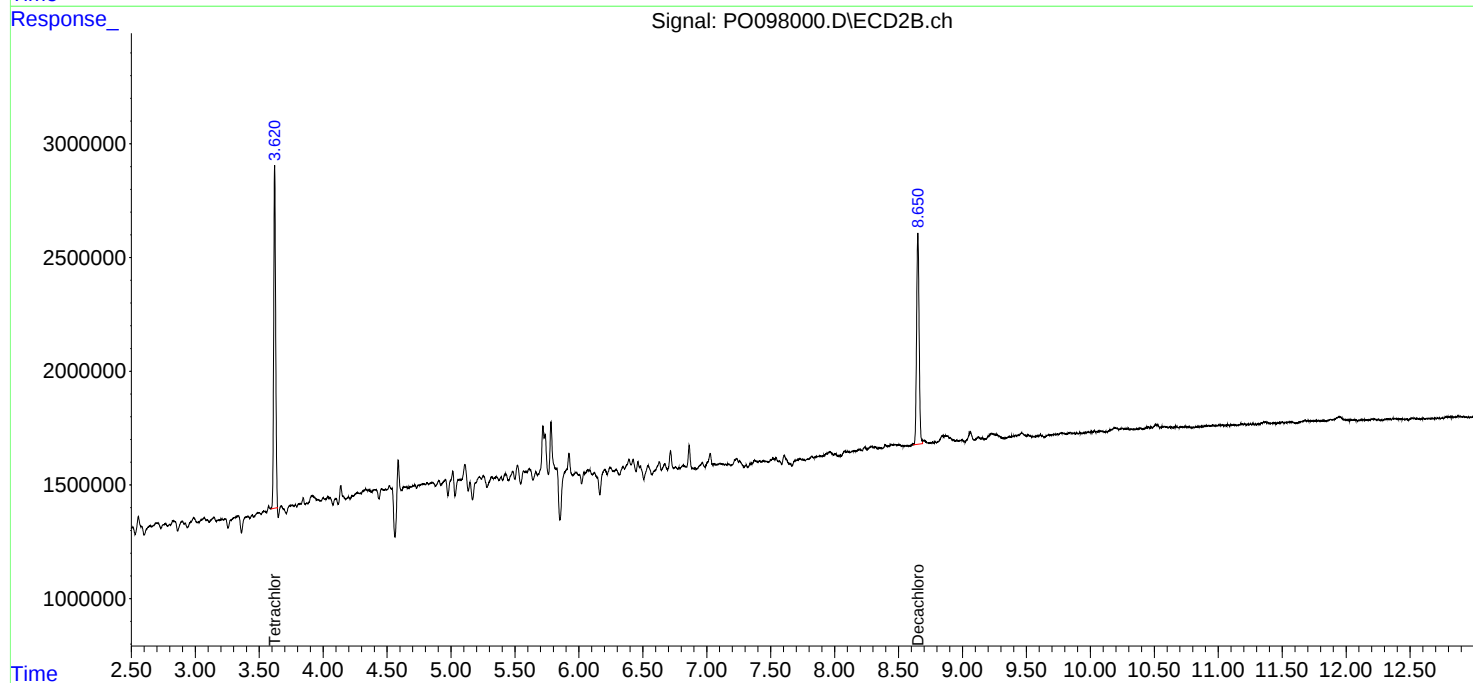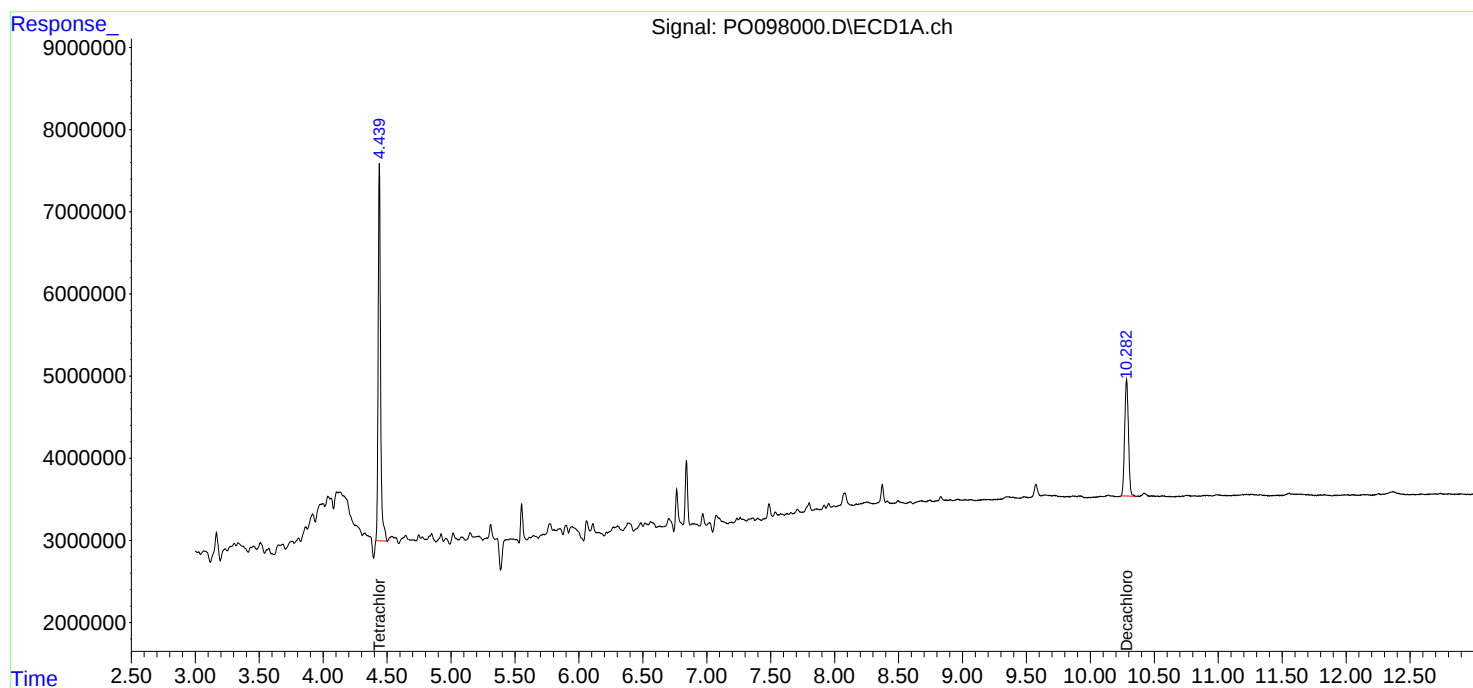

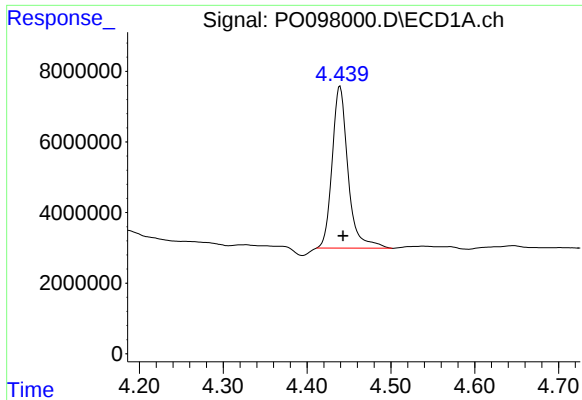


#1 Tetrachloro-m-xylene

R.T.: 4.439 min
Delta R.T.: -0.004 min
Response: 60347965
Conc: 15.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
OR-02-091223


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

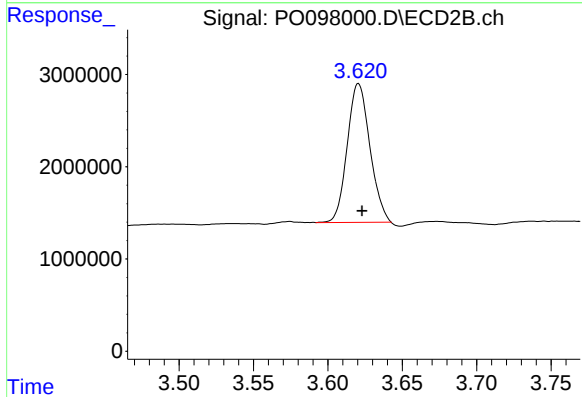


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.003 min
Response: 15967157
Conc: 16.67 ng/ml m

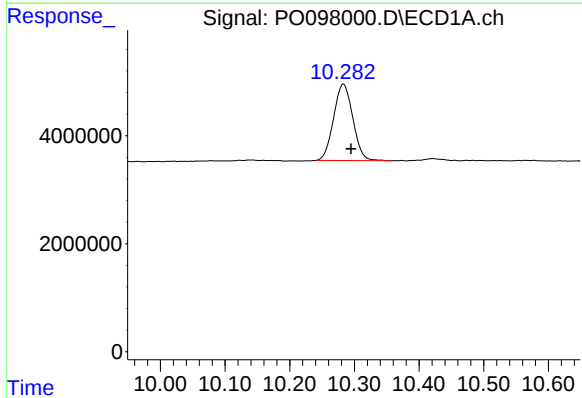

#2 Decachlorobiphenyl

R.T.: 10.283 min
Delta R.T.: -0.012 min
Response: 29204715
Conc: 15.63 ng/ml

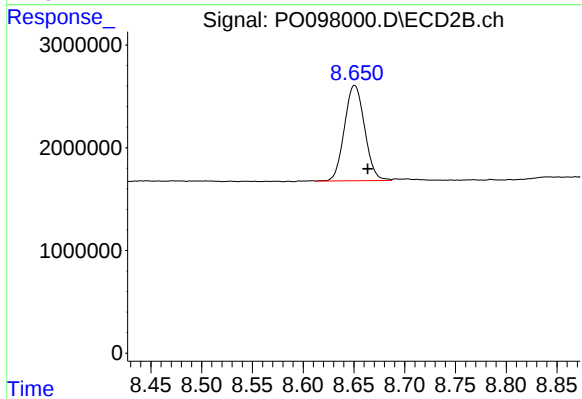

#2 Decachlorobiphenyl

R.T.: 8.651 min
Delta R.T.: -0.013 min
Response: 12846657
Conc: 15.04 ng/ml