

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091323\
 Data File : P0098001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2023 20:17
 Operator : YP/AJ
 Sample : 04407-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 306-TP-1-2-CS-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/14/2023
 Supervised By :Ankita Jodhani 09/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 01:18:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 07 02:56:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.439	3.620	71804204	21151614	18.023	22.086
2) SA Decachlor...	10.285	8.652	35755263	16490272	19.136	19.301

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091323\
Data File : PO098001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2023 20:17
Operator : YP/AJ
Sample : 04407-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
306-TP-1-2-CS-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 01:18:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 07 02:56:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

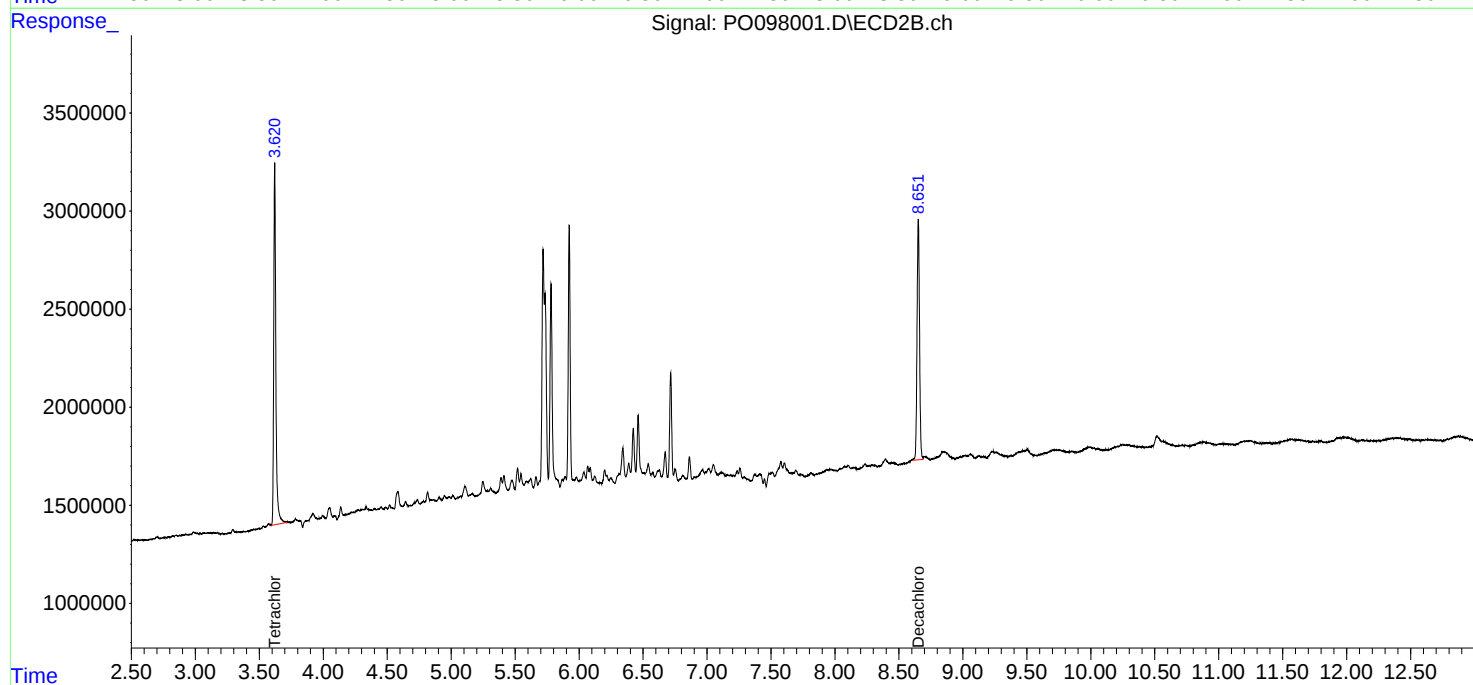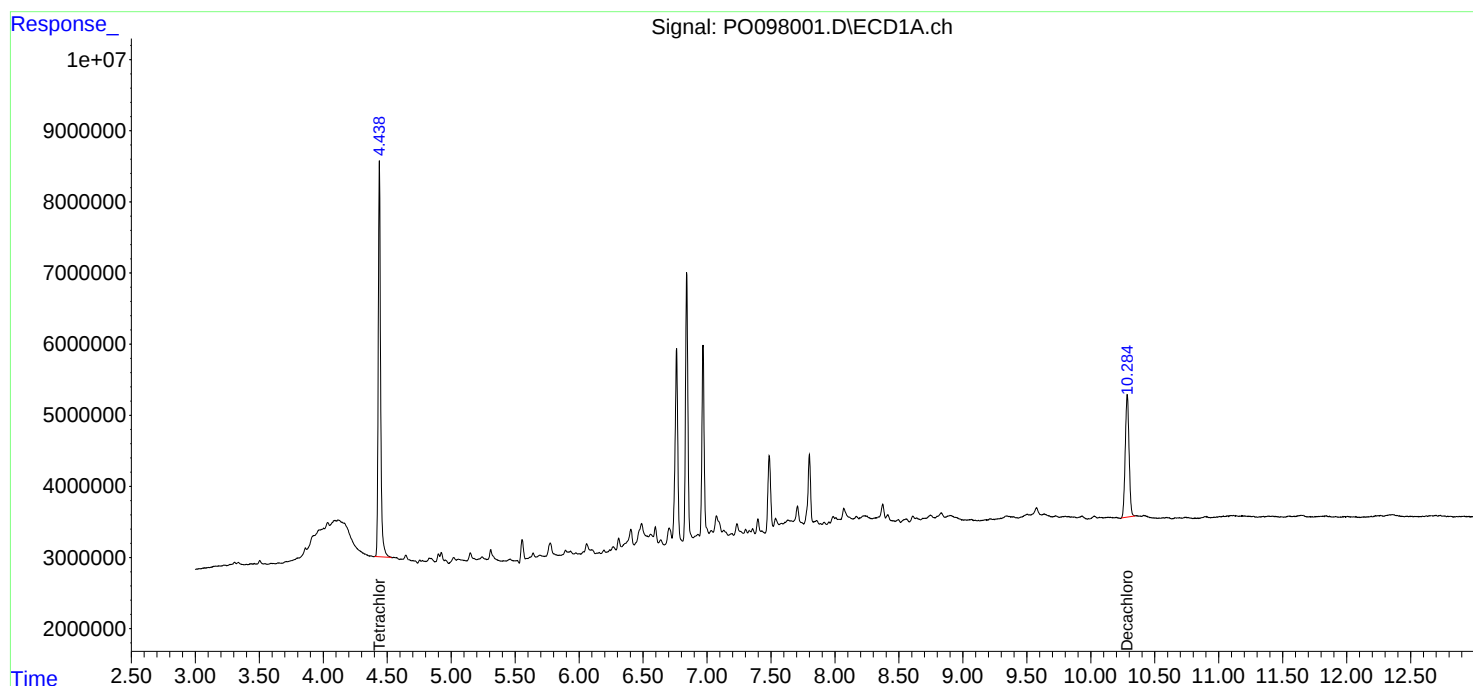

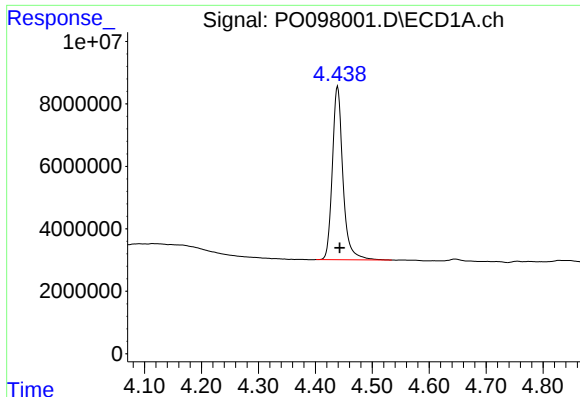


#1 Tetrachloro-m-xylene

R.T.: 4.439 min
Delta R.T.: -0.004 min
Response: 71804204
Conc: 18.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
306-TP-1-2-CS-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

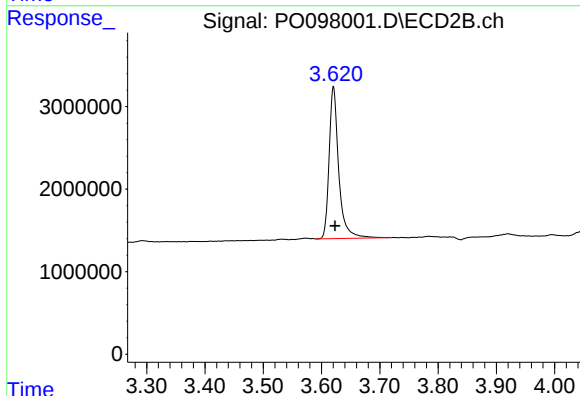


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.003 min
Response: 21151614
Conc: 22.09 ng/ml

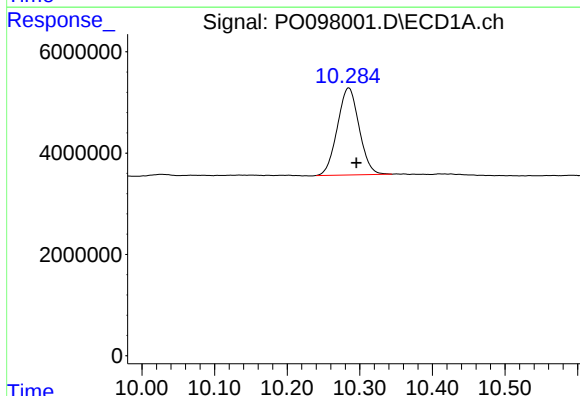

#2 Decachlorobiphenyl

R.T.: 10.285 min
Delta R.T.: -0.010 min
Response: 35755263
Conc: 19.14 ng/ml

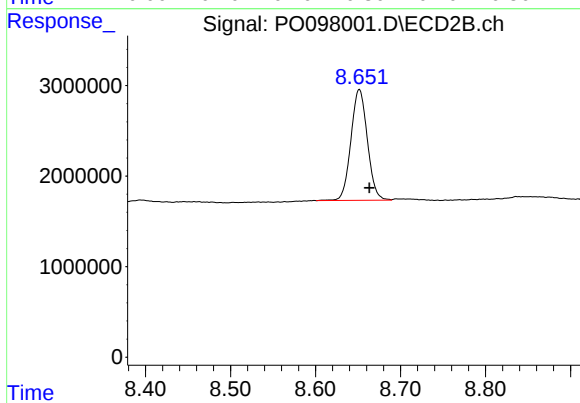

#2 Decachlorobiphenyl

R.T.: 8.652 min
Delta R.T.: -0.012 min
Response: 16490272
Conc: 19.30 ng/ml