

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091325\
 Data File : P0113705.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2025 13:42
 Operator : YP/AJ
 Sample : Q3080-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-03-091125

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/15/2025
 Supervised By :mohammad ahmed 09/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 14:16:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 09 15:11:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.656	3.648	122.3E6	82026025	14.935m	16.209
2) SA Decachlor...	8.668	8.613	96618972	30006392	13.939	15.836

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091325\
Data File : PO113705.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2025 13:42
Operator : YP/AJ
Sample : Q3080-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-03-091125


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/15/2025
Supervised By :mohammad ahmed 09/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 14:16:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 09 15:11:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

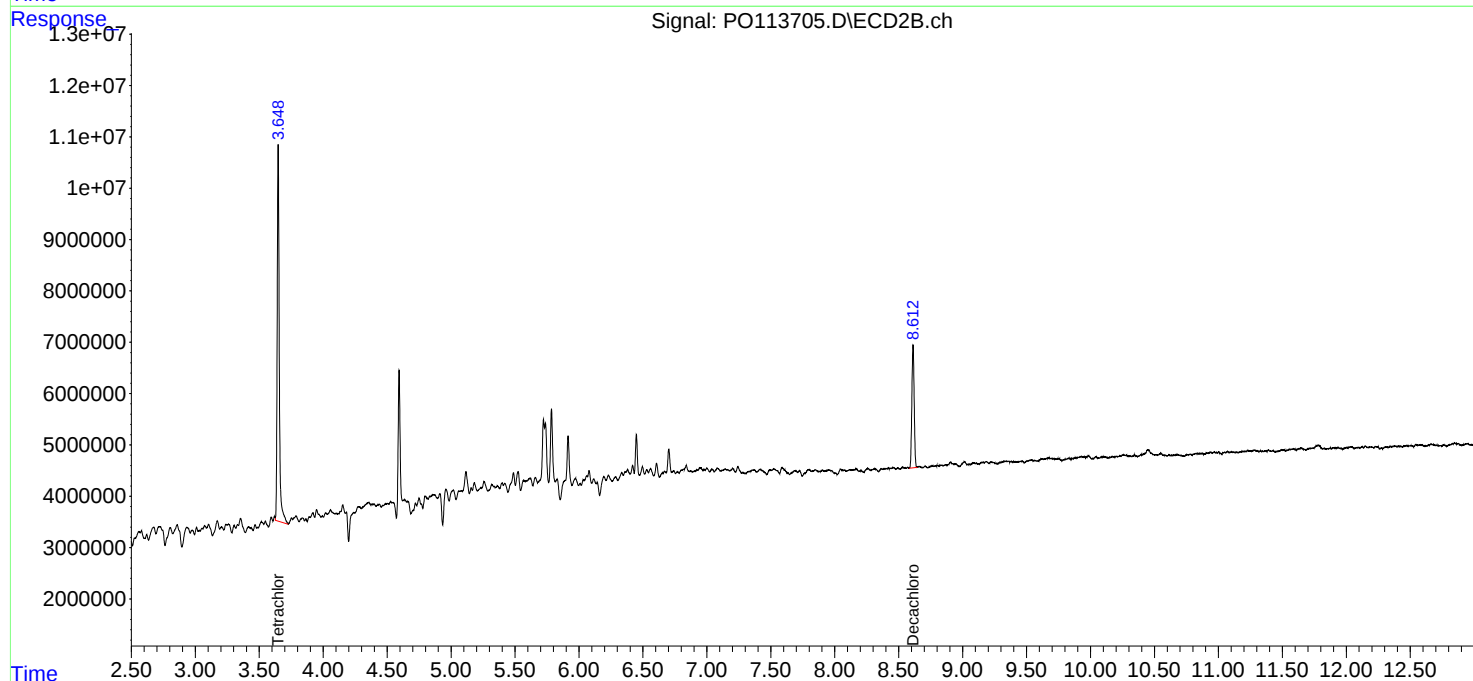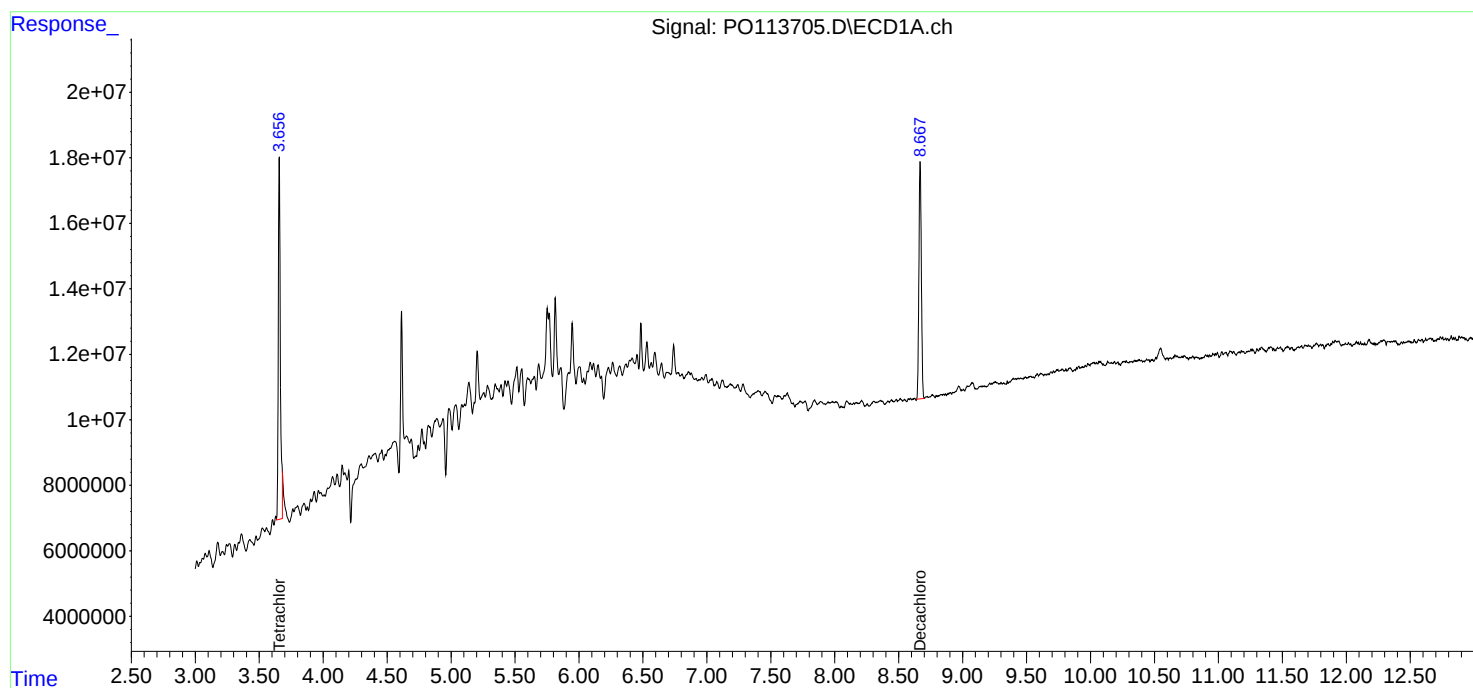

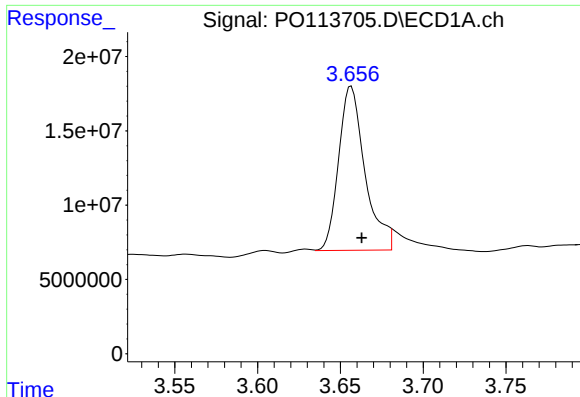


#1 Tetrachloro-m-xylene

R.T.: 3.656 min
Delta R.T.: -0.007 min
Response: 122267276
Conc: 14.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-03-091125


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/15/2025
Supervised By :mohammad ahmed 09/16/2025

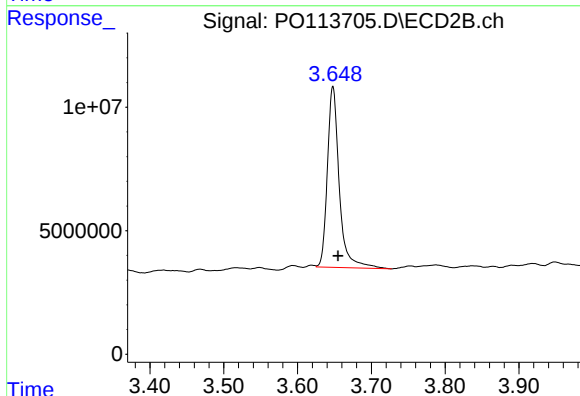


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: -0.007 min
Response: 82026025
Conc: 16.21 ng/ml

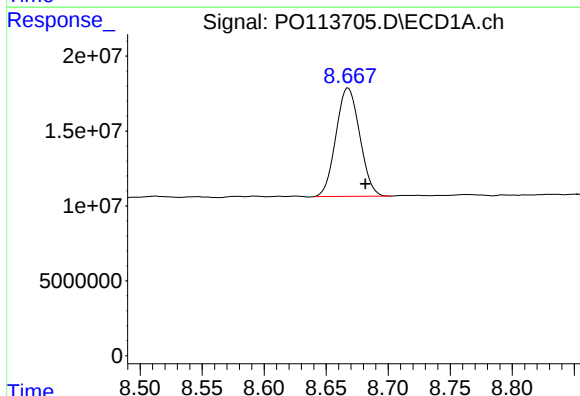

#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: -0.014 min
Response: 96618972
Conc: 13.94 ng/ml

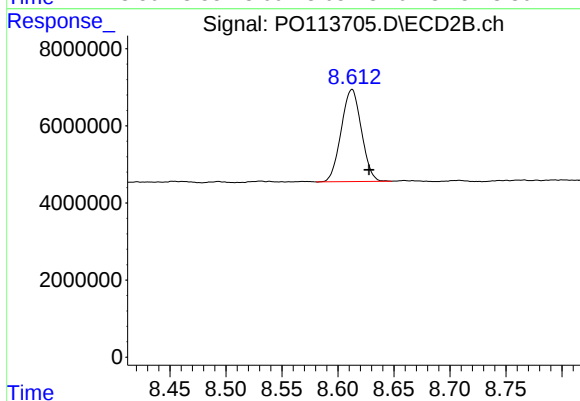

#2 Decachlorobiphenyl

R.T.: 8.613 min
Delta R.T.: -0.015 min
Response: 30006392
Conc: 15.84 ng/ml