

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091418\
 Data File : P0048998.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Sep 2018 17:01
 Operator : SM/SJ
 Sample : J4898-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ROLLOFF02-COMP-FILL

Manual Integrations
 APPROVED

Sohil
 9/17/2018 11:37:26 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 04:06:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 12 08:13:07 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.395	3.524	3672702	4739624	22.418m	25.980m
2) SA Decachlor...	10.107	8.459	4309837	5180121	19.345	27.915 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091418\
Data File : PO048998.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Sep 2018 17:01
Operator : SM/SJ
Sample : J4898-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ROLLOFF02-COMP-FILL


Manual Integrations
APPROVED

Sohil
9/17/2018 11:37:26 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 04:06:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091118.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 12 08:13:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

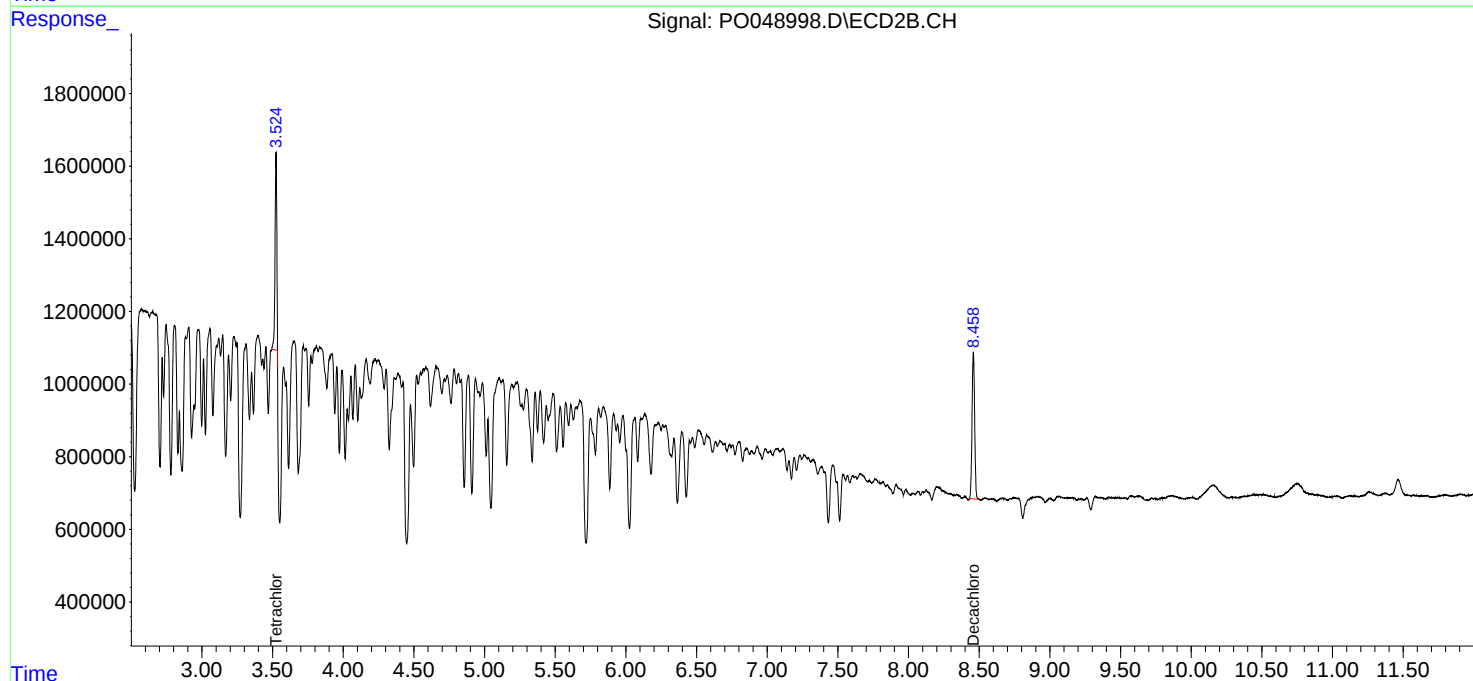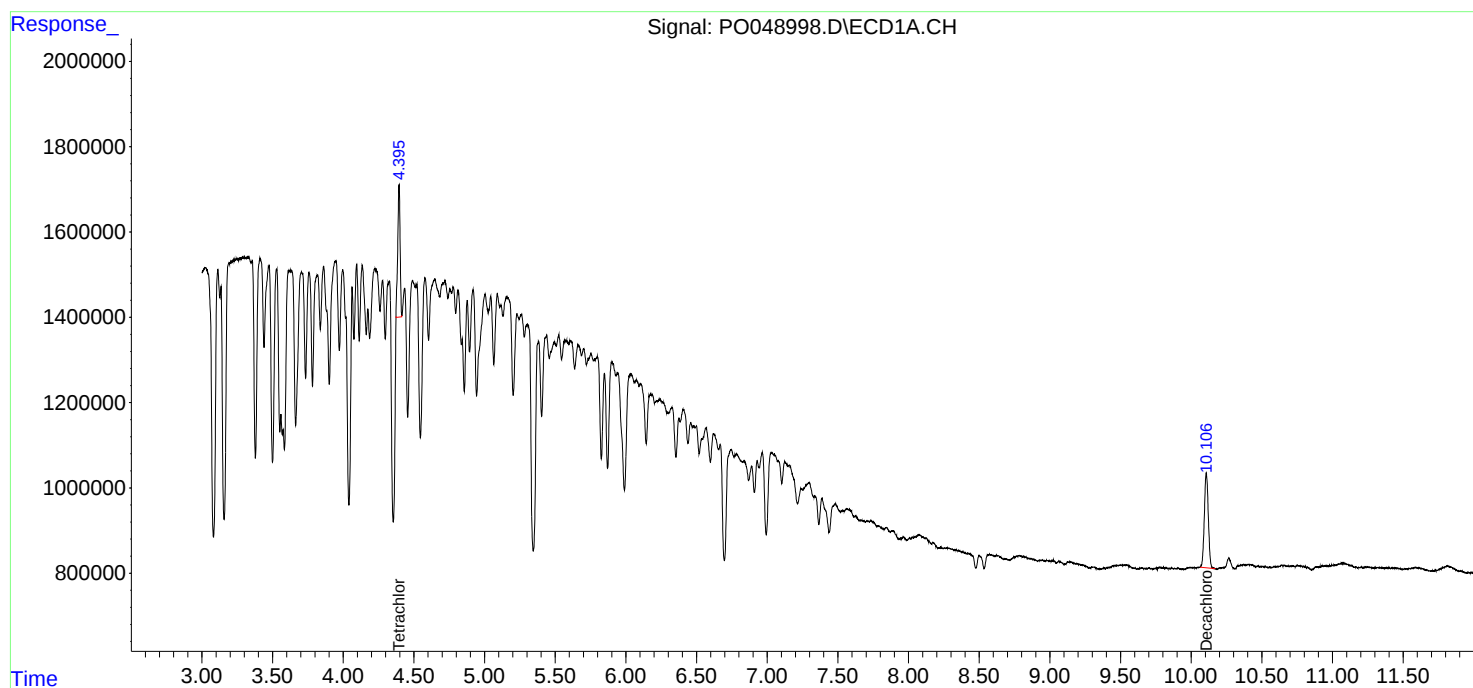

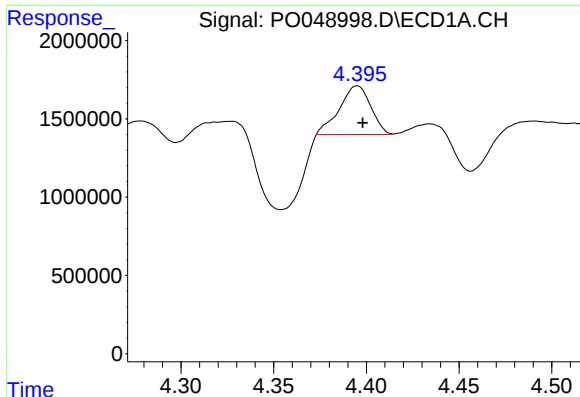


#1 Tetrachloro-m-xylene

R.T.: 4.395 min
Delta R.T.: -0.003 min
Response: 3672702
Conc: 22.42 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ROLLOFF02-COMP-FILL


Manual Integrations
APPROVED

Sohil
9/17/2018 11:37:26 AM

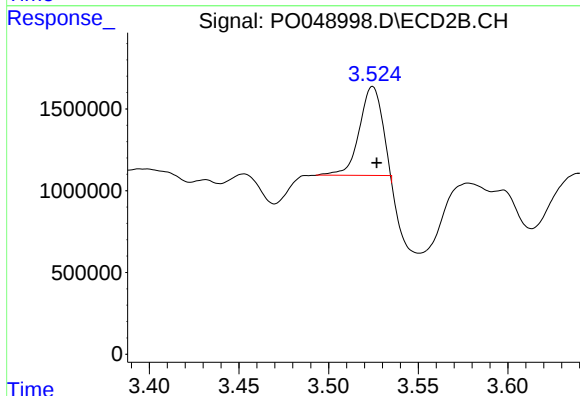


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: -0.003 min
Response: 4739624
Conc: 25.98 ng/ml m

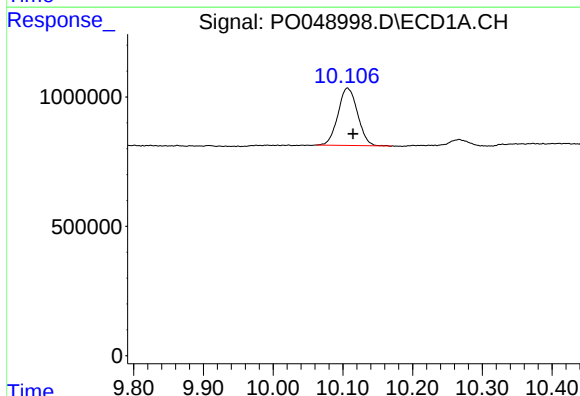

#2 Decachlorobiphenyl

R.T.: 10.107 min
Delta R.T.: -0.007 min
Response: 4309837
Conc: 19.34 ng/ml

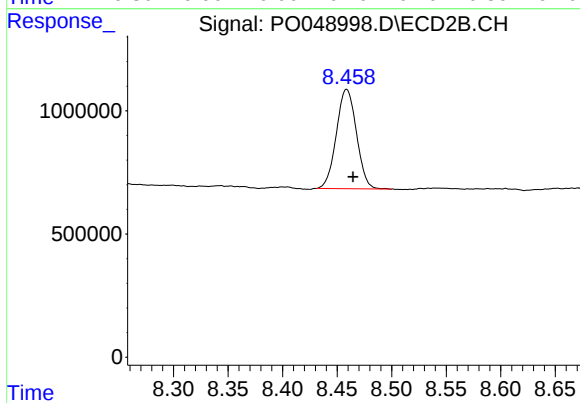

#2 Decachlorobiphenyl

R.T.: 8.459 min
Delta R.T.: -0.006 min
Response: 5180121
Conc: 27.92 ng/ml