

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091418\
 Data File : P0049024.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Sep 2018 00:13
 Operator : SM/SJ
 Sample : J4901-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 091218-SIDI-F-D-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 01:42:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 12 08:13:07 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.395	3.525	2837466	3623349	17.320	19.862
2) SA Decachlor...	10.108	8.459	3610246	4185130	16.205	22.553 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091418\
Data File : PO049024.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Sep 2018 00:13
Operator : SM/SJ
Sample : J4901-11
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
091218-SIDI-F-D-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 01:42:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091118.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 12 08:13:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

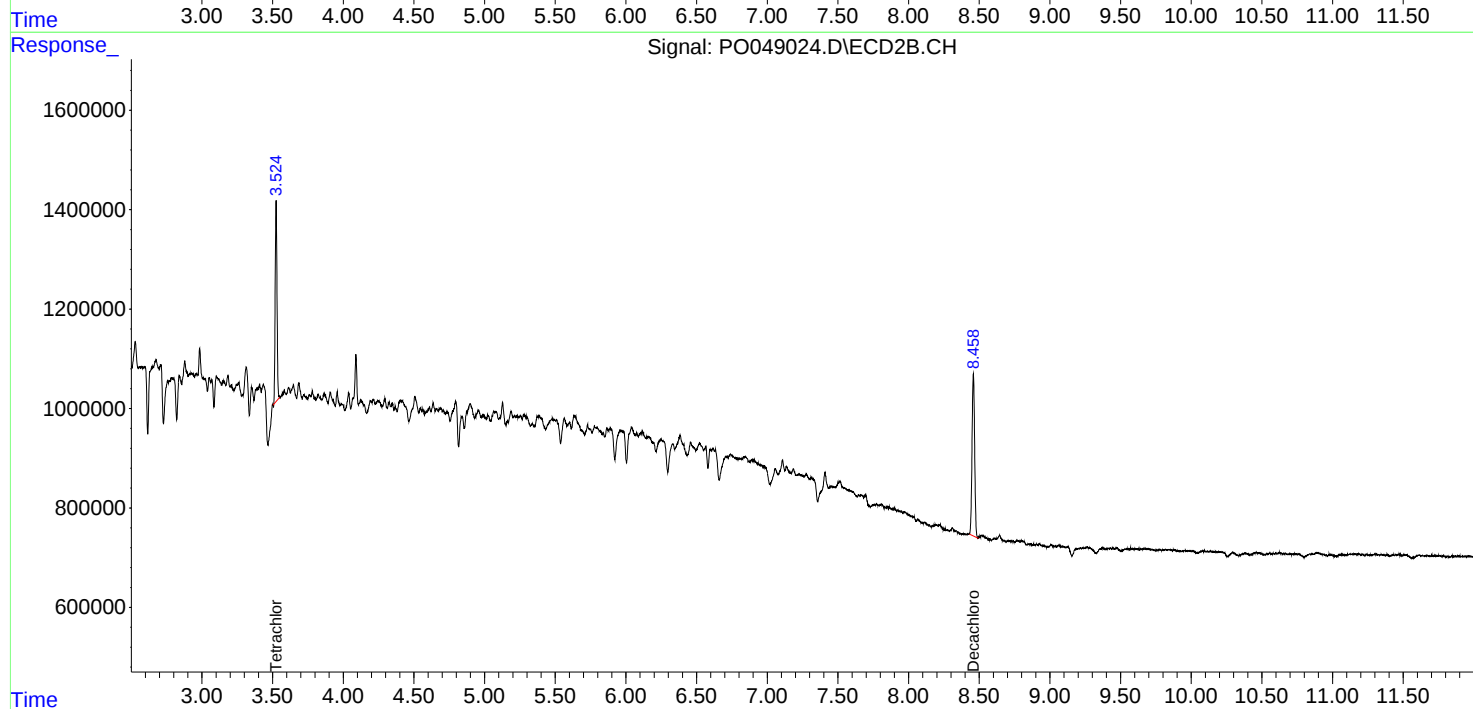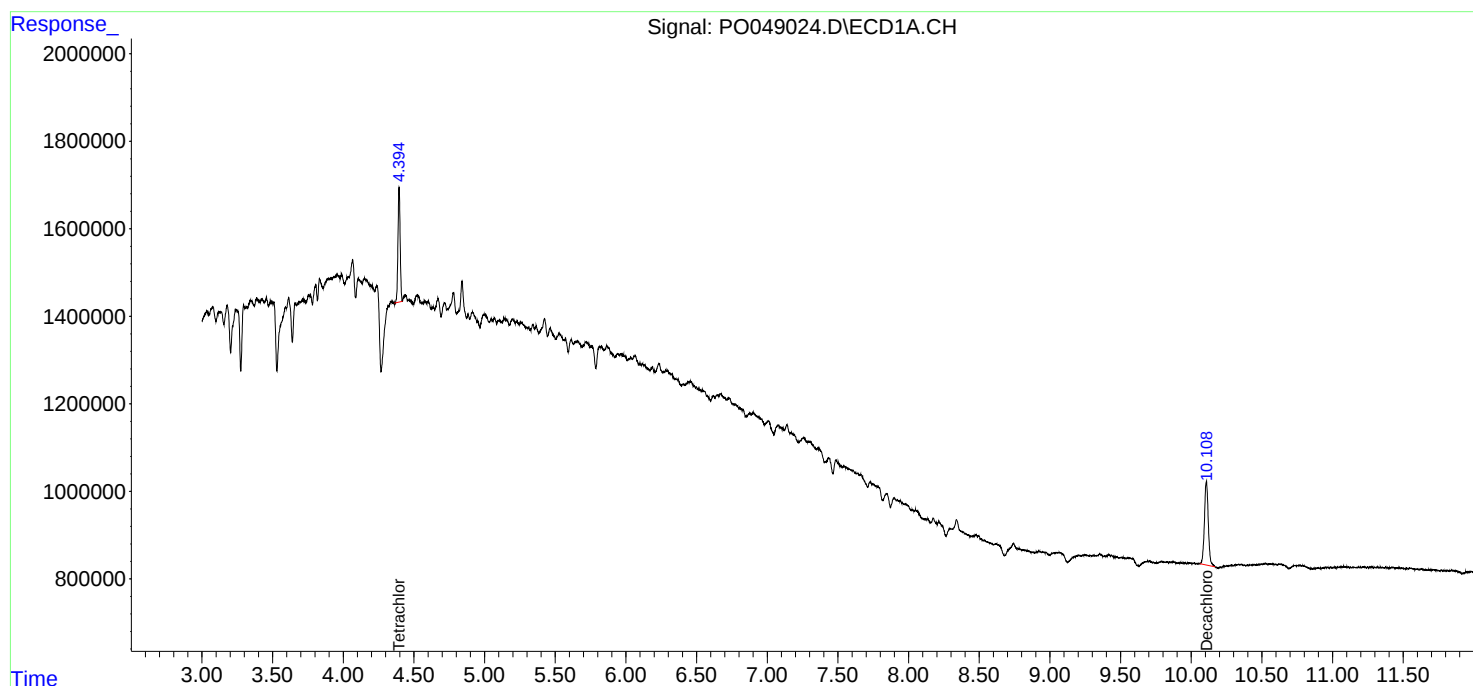


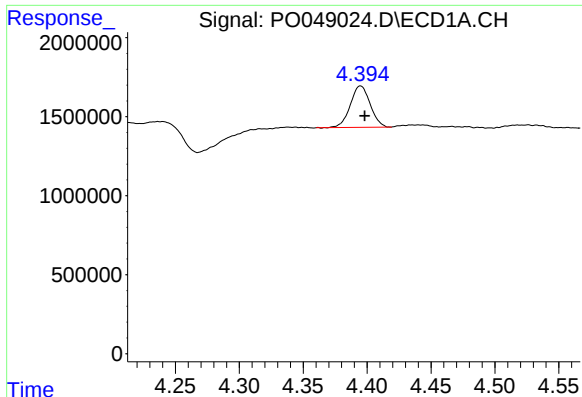

#1 Tetrachloro-m-xylene


R.T.: 4.395 min
Delta R.T.: -0.003 min
Response: 2837466
Conc: 17.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
091218-SIDI-F-D-B

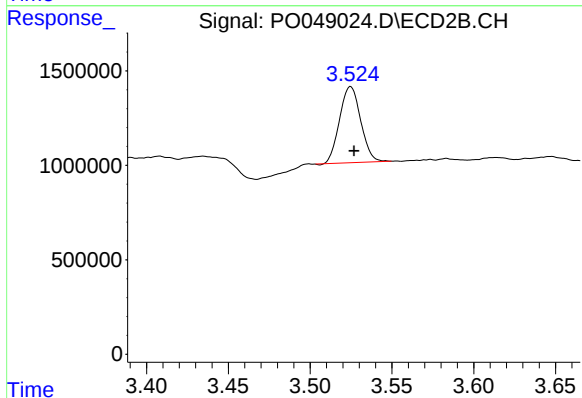


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: -0.002 min
Response: 3623349
Conc: 19.86 ng/ml

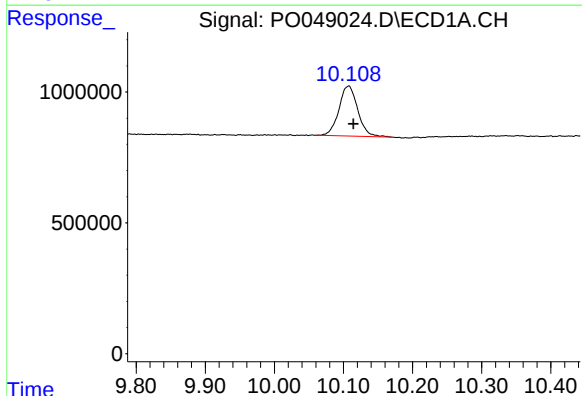

#2 Decachlorobiphenyl

R.T.: 10.108 min
Delta R.T.: -0.007 min
Response: 3610246
Conc: 16.20 ng/ml

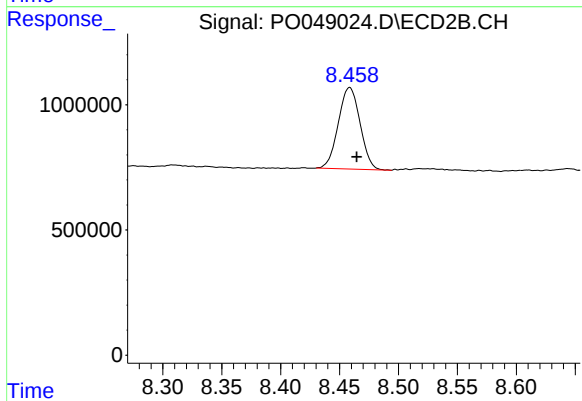

#2 Decachlorobiphenyl

R.T.: 8.459 min
Delta R.T.: -0.006 min
Response: 4185130
Conc: 22.55 ng/ml