

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091420\
 Data File : P0071309.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Sep 2020 11:08
 Operator : DD\AJ
 Sample : L3952-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 16744RE

Manual Integrations
 APPROVED

Ankita
 9/15/2020 10:18:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 16:29:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.354	3.549f	2339179	788307	33.008m	20.192 #
2) SA Decachlor...	10.006f	8.747f	6945198	3477145	74.476m	63.124m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091420\
Data File : PO071309.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Sep 2020 11:08
Operator : DD\AJ
Sample : L3952-05
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
16744RE


Manual Integrations
APPROVED

Ankita
9/15/2020 10:18:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 16:29:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

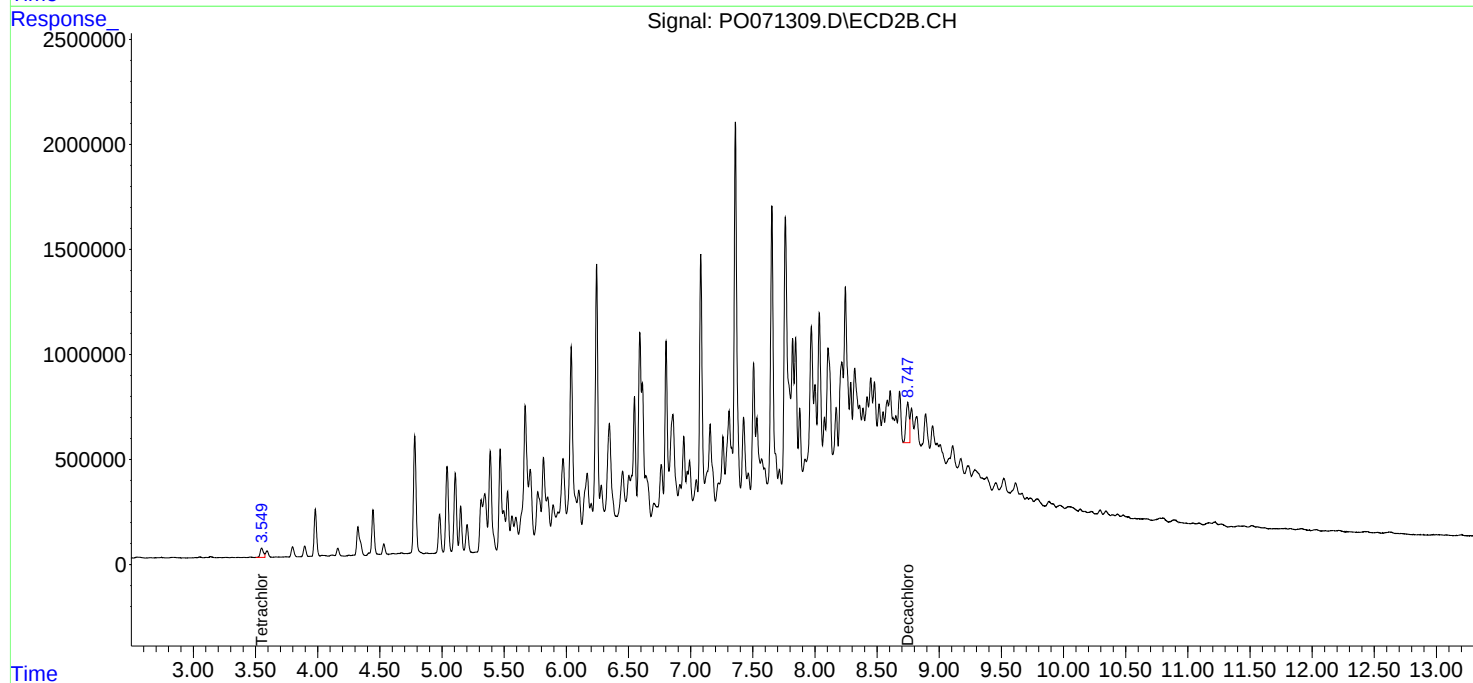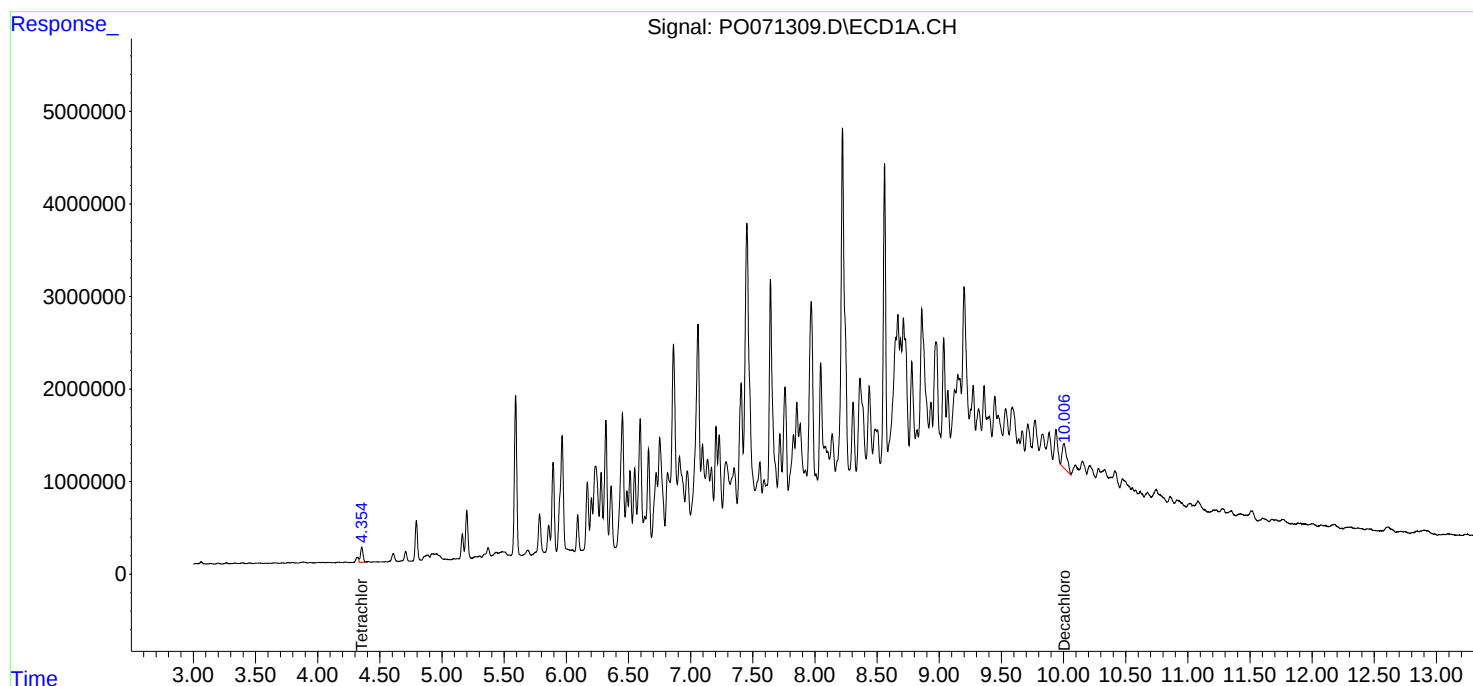

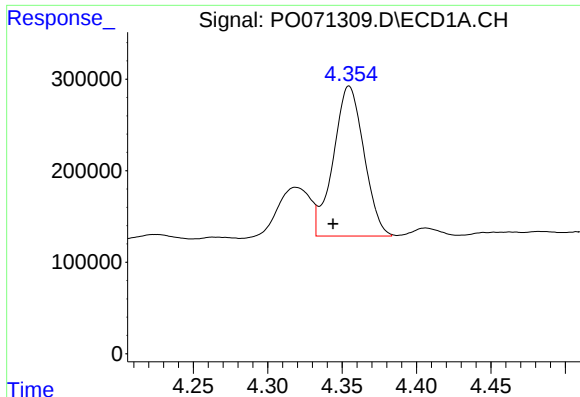

#1 Tetrachloro-m-xylene

R.T.: 4.354 min

Delta R.T.: 0.010 min


Response: 2339179

Conc: 33.01 ng/ml m

Instrument :
ECD_O
ClientSampleId :
16744RE

Manual Integrations
APPROVED

Ankita
9/15/2020 10:18:27 AM

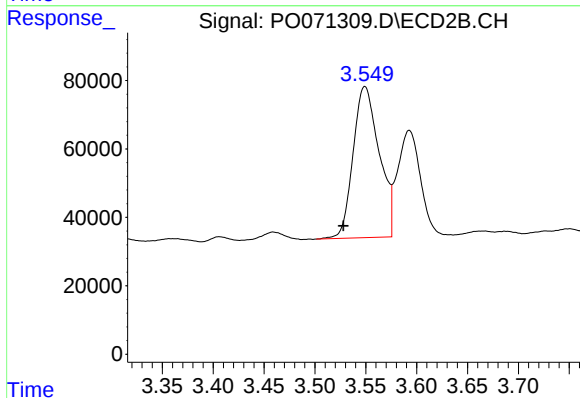


#1 Tetrachloro-m-xylene

R.T.: 3.549 min

Delta R.T.: 0.021 min

Response: 788307

Conc: 20.19 ng/ml

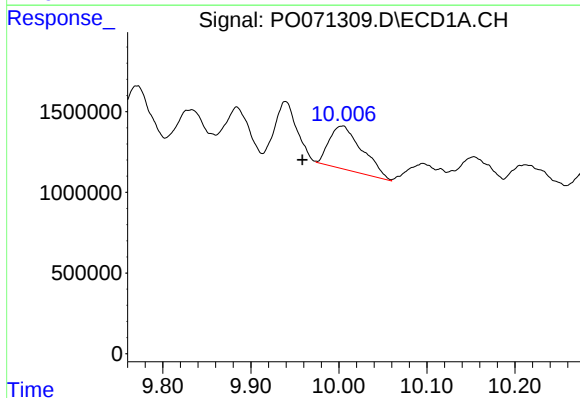


#2 Decachlorobiphenyl

R.T.: 10.006 min

Delta R.T.: 0.047 min

Response: 6945198

Conc: 74.48 ng/ml m

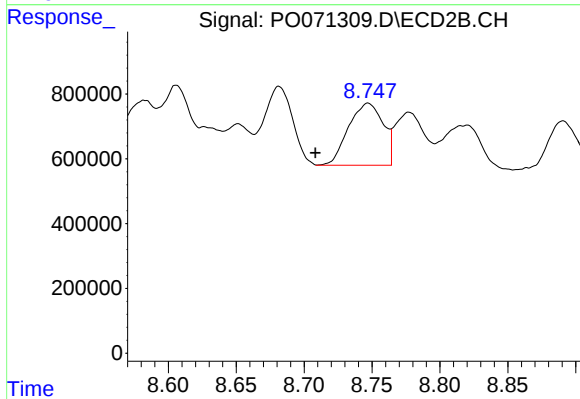

#2 Decachlorobiphenyl

R.T.: 8.747 min

Delta R.T.: 0.038 min

Response: 3477145

Conc: 63.12 ng/ml m