

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091420\
 Data File : P0071332.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Sep 2020 18:30
 Operator : DD\AJ
 Sample : L3993-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PAV-B38-091120-10-17

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 01:52:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.529	1940149	1028752	27.377	26.350
2) SA Decachlor...	9.958	8.708	1902062	1010623	20.396	18.347

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091420\
Data File : P0071332.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Sep 2020 18:30
Operator : DD\AJ
Sample : L3993-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PAV-B38-091120-10-17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 01:52:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

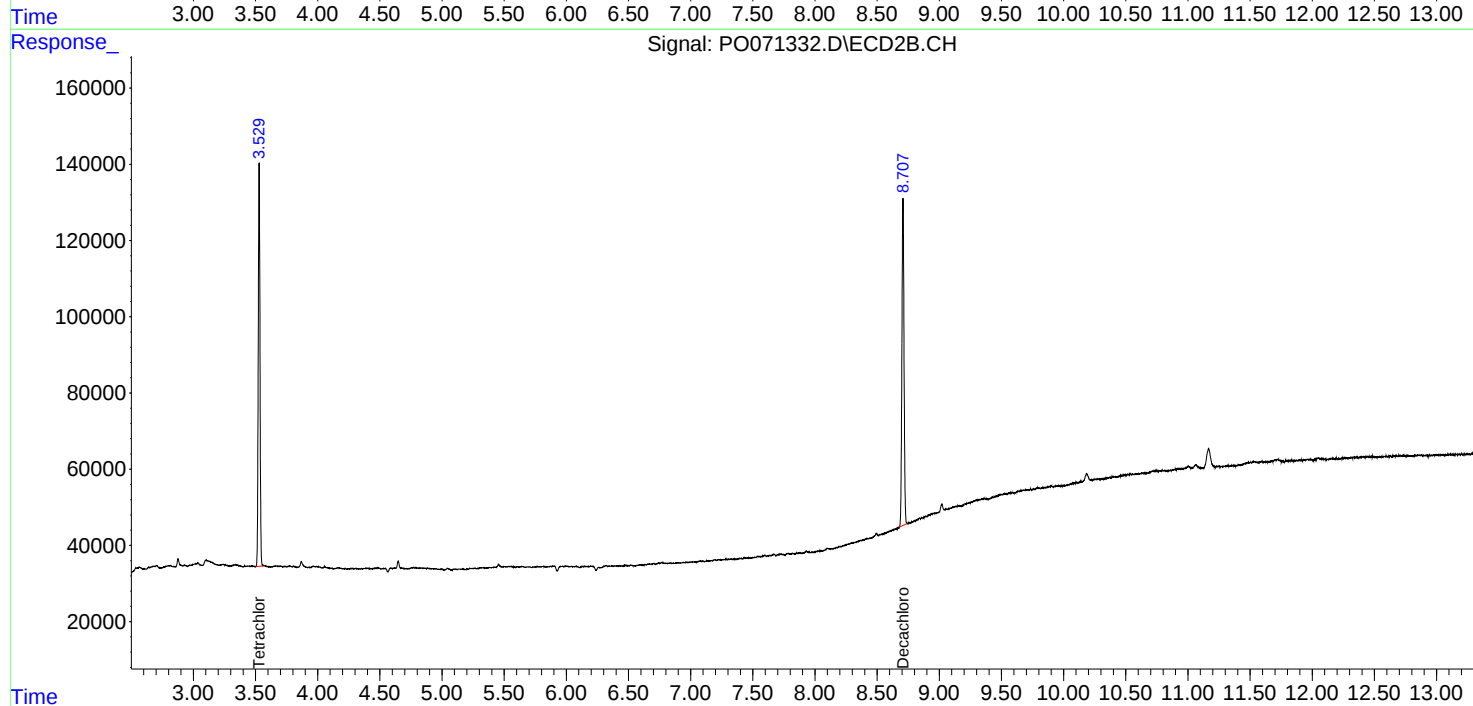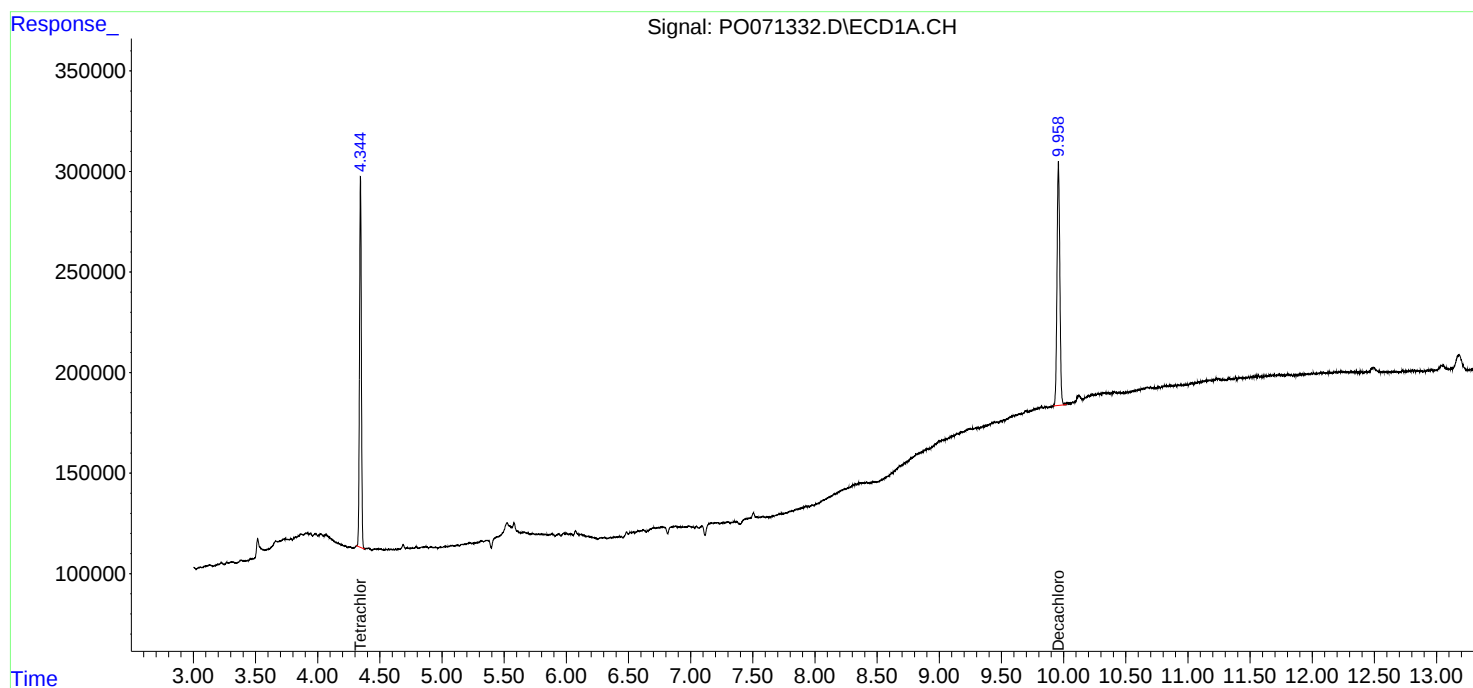


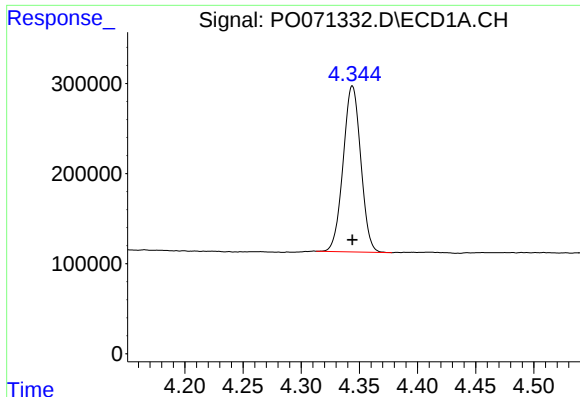

#1 Tetrachloro-m-xylene


R.T.: 4.344 min
Delta R.T.: 0.000 min
Response: 1940149
Conc: 27.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAV-B38-091120-10-17

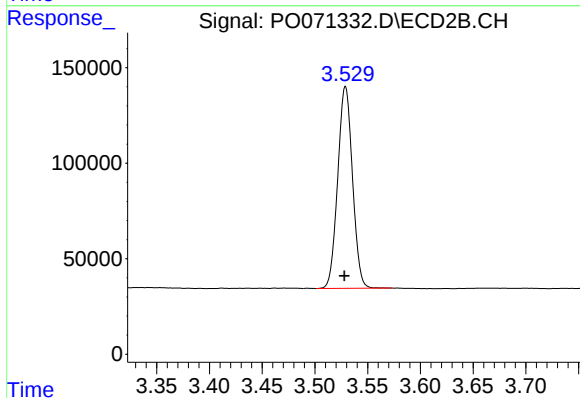


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: 0.001 min
Response: 1028752
Conc: 26.35 ng/ml

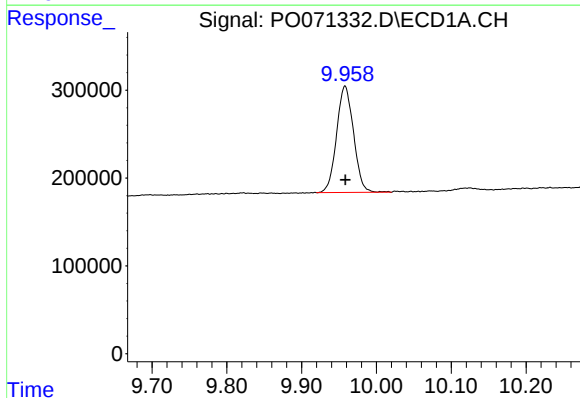

#2 Decachlorobiphenyl

R.T.: 9.958 min
Delta R.T.: 0.000 min
Response: 1902062
Conc: 20.40 ng/ml

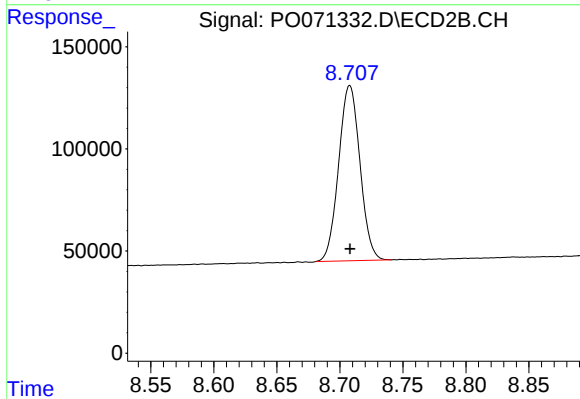

#2 Decachlorobiphenyl

R.T.: 8.708 min
Delta R.T.: 0.000 min
Response: 1010623
Conc: 18.35 ng/ml