

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091423\
 Data File : P0098039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2023 22:58
 Operator : YP/AJ
 Sample : 04436-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CPT102-16

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :Ankita Jodhani 09/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 07:22:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 07 02:56:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.437	3.618	69371274	19704416	17.412	20.575
2) SA Decachlor...	10.276	8.646	27814836	13466336	14.887m	15.761

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091423\
Data File : PO098039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2023 22:58
Operator : YP/AJ
Sample : 04436-16
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CPT102-16


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/15/2023
Supervised By :Ankita Jodhani 09/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 07:22:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 07 02:56:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

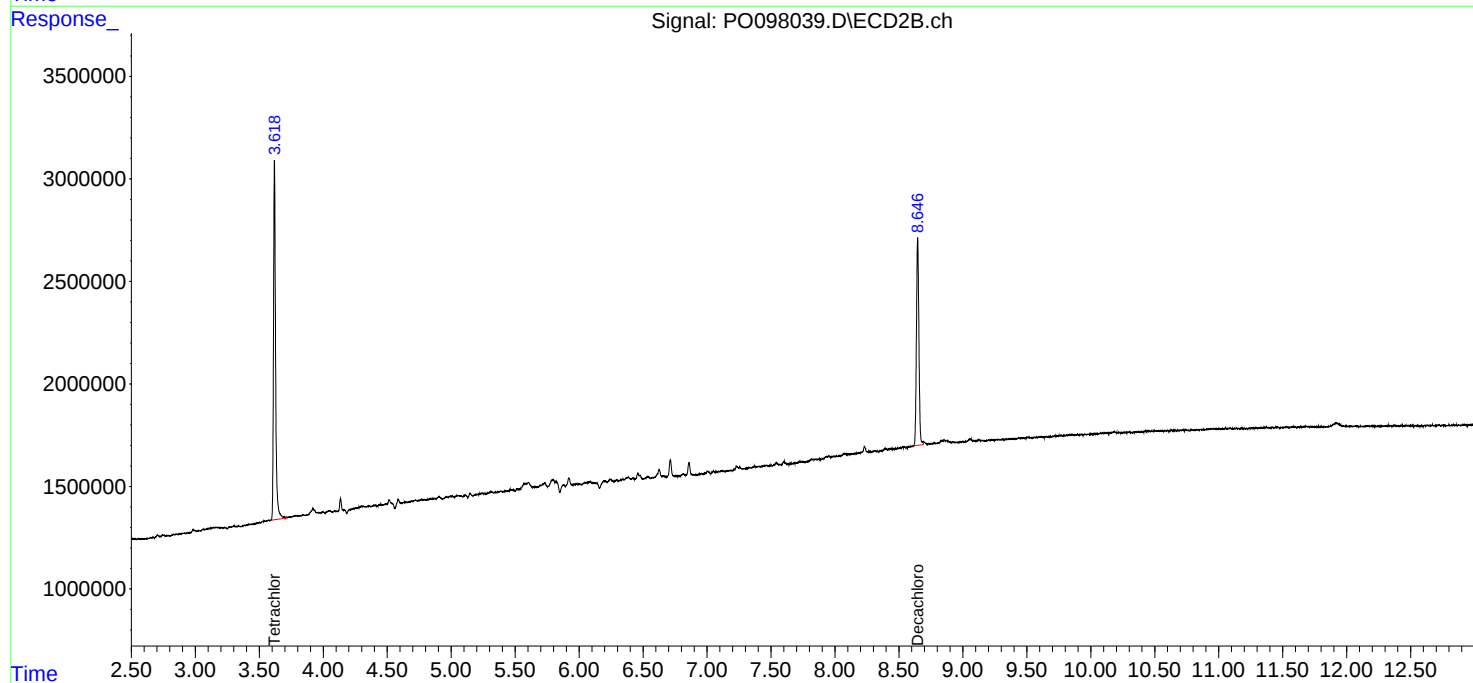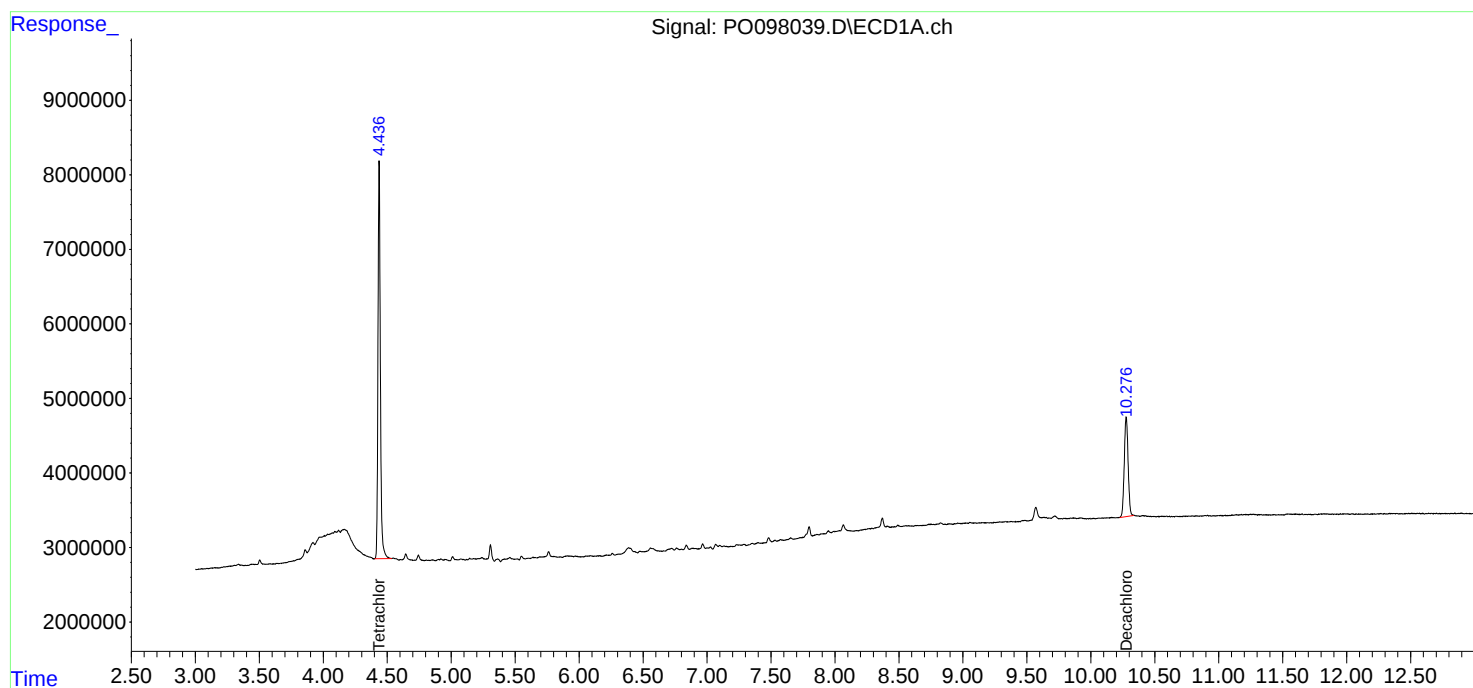

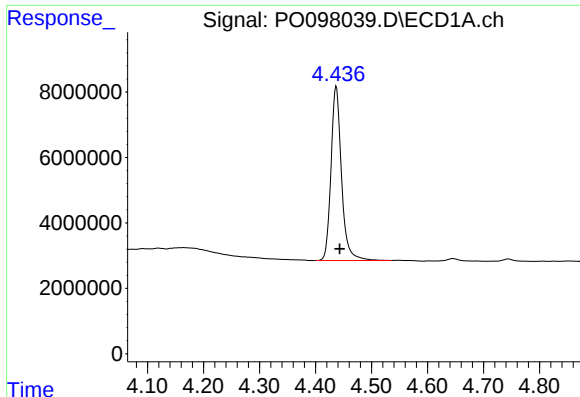


#1 Tetrachloro-m-xylene

R.T.: 4.437 min
Delta R.T.: -0.006 min
Response: 69371274
Conc: 17.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
CPT102-16


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/15/2023
Supervised By :Ankita Jodhani 09/15/2023

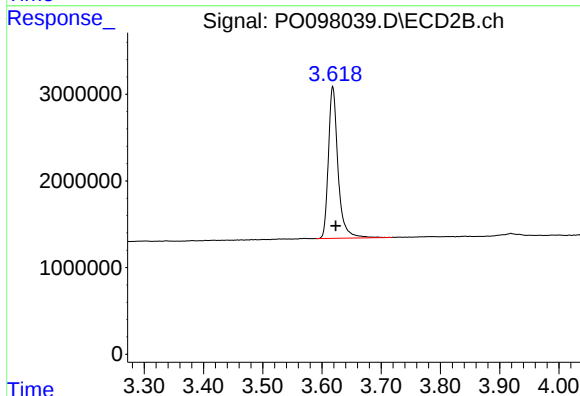


#1 Tetrachloro-m-xylene

R.T.: 3.618 min
Delta R.T.: -0.005 min
Response: 19704416
Conc: 20.58 ng/ml

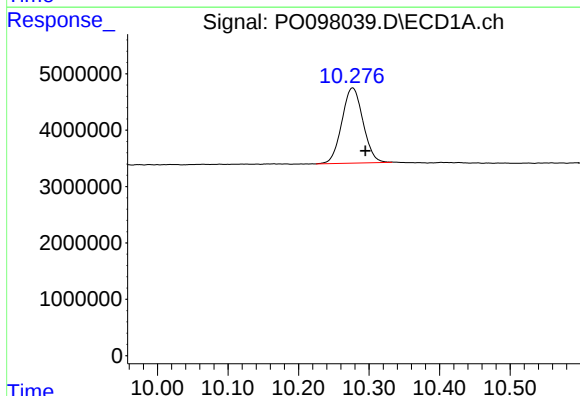

#2 Decachlorobiphenyl

R.T.: 10.276 min
Delta R.T.: -0.019 min
Response: 27814836
Conc: 14.89 ng/ml m

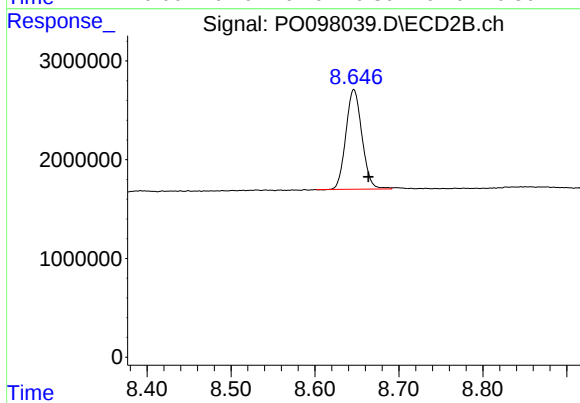

#2 Decachlorobiphenyl

R.T.: 8.646 min
Delta R.T.: -0.017 min
Response: 13466336
Conc: 15.76 ng/ml